

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030809.D
 Acq On : 03 Jul 2021 12:49
 Operator : CG/JU
 Sample : M2905-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030809.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	19	23	27	rBV	22624	31485	0.75%	0.118%
2	3.258	27	29	39	rVB	24157	32650	0.78%	0.122%
3	3.687	98	102	120	rBV	83701	201946	4.80%	0.757%
4	3.987	149	153	159	rVB2	5934	10549	0.25%	0.040%
5	4.511	236	242	253	rBV	434707	654797	15.55%	2.456%
6	5.105	336	343	348	rBV	40664	62528	1.49%	0.235%
7	5.793	456	460	466	rVB5	4211	6203	0.15%	0.023%
8	6.264	536	540	545	rBV2	4340	6573	0.16%	0.025%
9	6.934	648	654	665	rBV	91713	152750	3.63%	0.573%
10	7.105	675	683	694	rBV	316376	514473	12.22%	1.930%
11	7.299	708	716	727	rBV	344856	558620	13.27%	2.095%
12	7.763	789	795	806	rBV	277126	460621	10.94%	1.728%
13	8.005	830	836	839	rBV5	4764	6976	0.17%	0.026%
14	8.116	849	855	864	rVB2	39073	72280	1.72%	0.271%
15	8.199	864	869	877	rBV2	8410	15855	0.38%	0.059%
16	8.469	909	915	926	rBV	242060	408045	9.69%	1.530%
17	8.575	928	933	938	rVB3	5239	9418	0.22%	0.035%
18	8.922	985	992	1002	rVV	381018	634002	15.06%	2.378%
19	9.175	1029	1035	1039	rBV7	3122	6251	0.15%	0.023%
20	9.522	1090	1094	1097	rVB4	4769	6589	0.16%	0.025%
21	9.640	1106	1114	1124	rBV	298773	508899	12.09%	1.909%
22	9.804	1138	1142	1148	rVB6	3033	4674	0.11%	0.018%
23	10.093	1183	1191	1198	rBV6	3954	9437	0.22%	0.035%
24	10.175	1198	1205	1230	rVV	400463	732004	17.39%	2.745%
25	10.552	1261	1269	1277	rBV	345308	600801	14.27%	2.253%
26	10.693	1286	1293	1308	rBV	342200	665783	15.82%	2.497%
27	10.816	1308	1314	1317	rVV7	5100	10330	0.25%	0.039%
28	10.904	1325	1329	1334	rVB4	3654	4868	0.12%	0.018%
29	11.199	1373	1379	1384	rBV6	3069	4889	0.12%	0.018%
30	11.469	1420	1425	1429	rBV5	4654	8020	0.19%	0.030%
31	11.969	1504	1510	1515	rVB5	2002	4475	0.11%	0.017%
32	12.146	1536	1540	1546	rVB4	5855	10952	0.26%	0.041%
33	13.804	1816	1822	1836	rBV	718884	1071593	25.46%	4.019%
34	14.087	1863	1870	1883	rBV	913523	1320427	31.37%	4.952%
35	14.392	1916	1922	1932	rBV	491150	736910	17.51%	2.764%
36	14.616	1952	1960	1976	rBV2	24599	86177	2.05%	0.323%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
 Data File : BM030809.D
 Acq On : 03 Jul 2021 12:49
 Operator : CG/JU
 Sample : M2905-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBK38

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
 Title : SVOA CALIBRATION

37	14.945	2009	2016	2020	rBV2	37082	63644	1.51%	0.239%
38	14.992	2020	2024	2025	rVV4	4783	5438	0.13%	0.020%
39	15.028	2025	2030	2035	rVB	40281	57565	1.37%	0.216%
40	15.386	2081	2091	2107	rBV	1134623	1660264	39.44%	6.227%
41	15.510	2107	2112	2120	rVV	272441	435713	10.35%	1.634%
42	15.569	2120	2122	2127	rVV4	15441	24420	0.58%	0.092%
43	15.634	2127	2133	2142	rVV3	17792	37385	0.89%	0.140%
44	15.716	2142	2147	2151	rVB7	5178	7765	0.18%	0.029%
45	16.169	2218	2224	2227	rBV5	3541	5014	0.12%	0.019%
46	16.210	2227	2231	2236	rVB2	11509	15236	0.36%	0.057%
47	16.786	2323	2329	2350	rBV	2761263	4209575	100.00%	15.789%
48	17.133	2382	2388	2399	rBV	577695	835546	19.85%	3.134%
49	17.233	2399	2405	2418	rBV	1391888	1939334	46.07%	7.274%
50	17.492	2440	2449	2455	rBV5	7571	14626	0.35%	0.055%
51	17.751	2490	2493	2497	rVB5	3285	4760	0.11%	0.018%
52	18.027	2536	2540	2545	rBV6	3938	6772	0.16%	0.025%
53	18.098	2549	2552	2555	rBV3	4724	6459	0.15%	0.024%
54	19.157	2729	2732	2736	rBV2	14510	18998	0.45%	0.071%
55	19.410	2771	2775	2779	rBV	13779	19063	0.45%	0.071%
56	19.522	2788	2794	2806	rBV	1821845	2460024	58.44%	9.227%
57	21.304	3092	3097	3105	rBV	797903	1044111	24.80%	3.916%
58	23.409	3448	3455	3467	rVB	1544650	2984703	70.90%	11.195%
59	23.551	3473	3479	3492	rVB2	602324	1172884	27.86%	4.399%




Sum of corrected areas: 26662149

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030809.D
Acq On : 03 Jul 2021 12:49
Operator : CG/JU
Sample : M2905-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

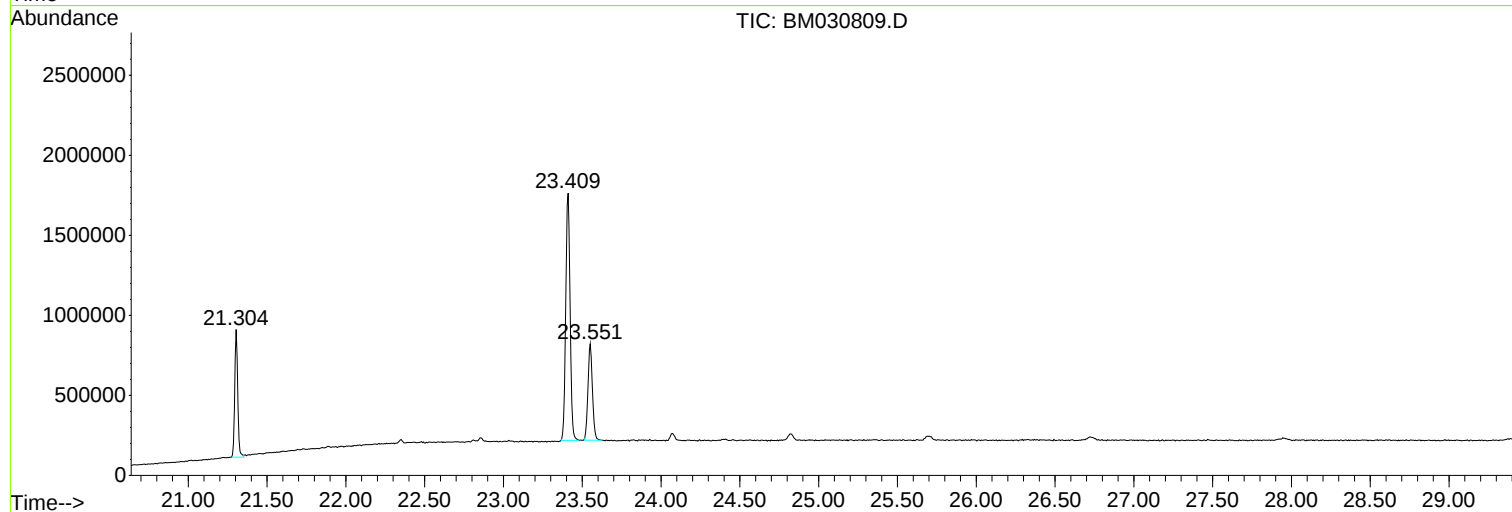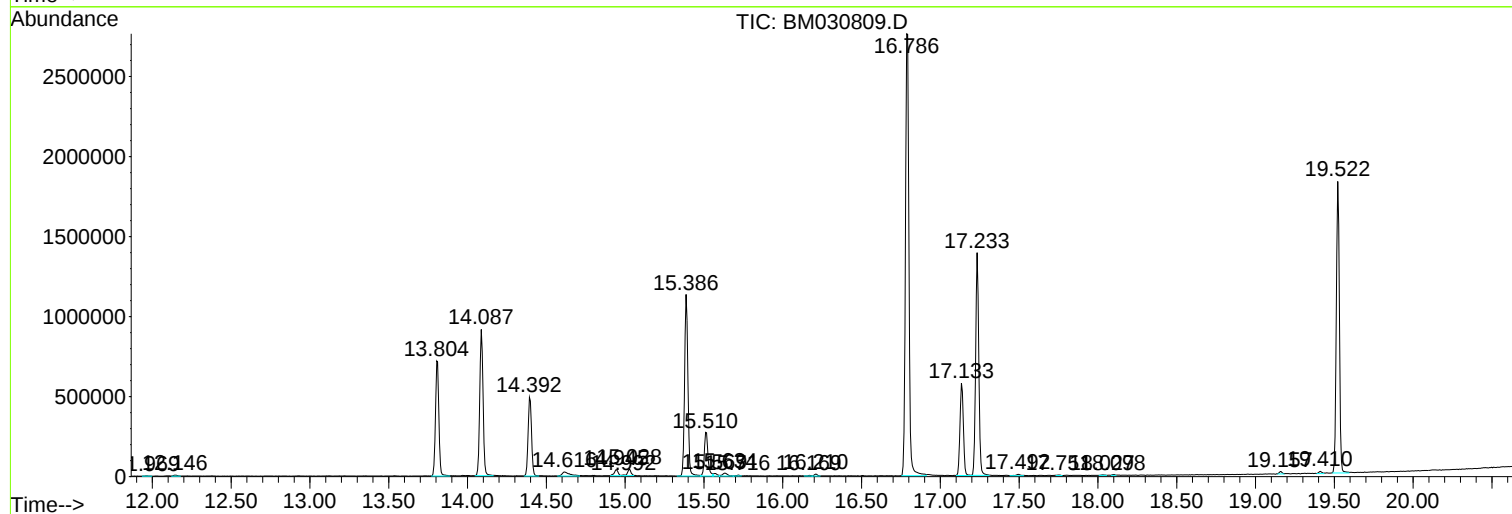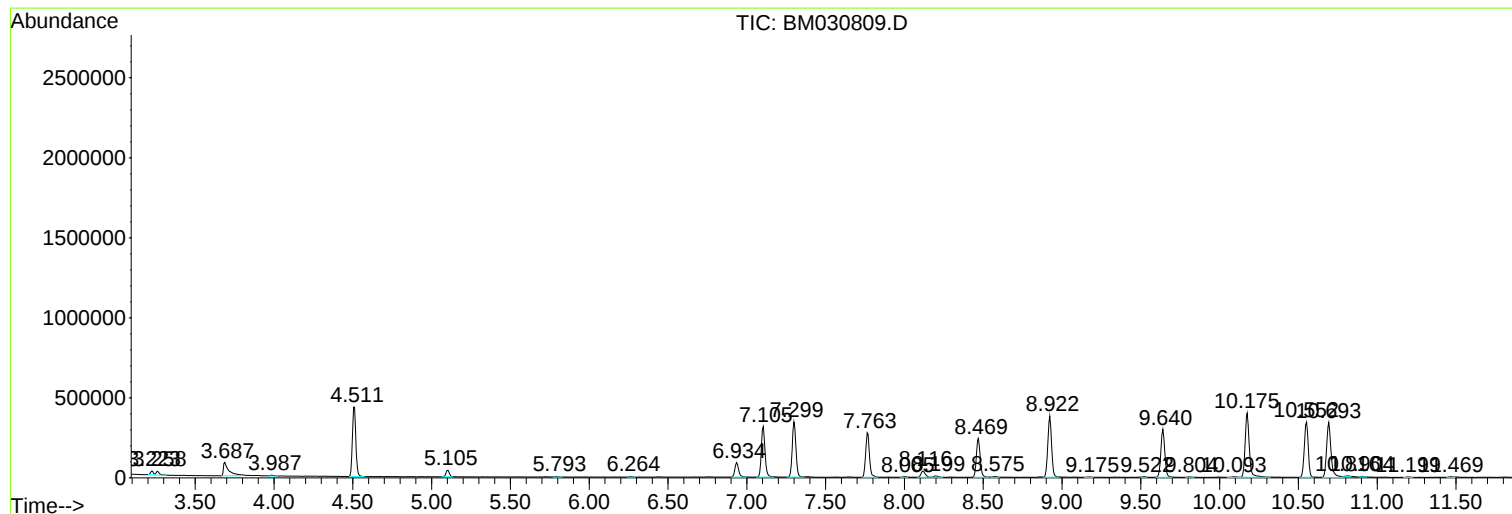

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030809.D
Acq On : 03 Jul 2021 12:49
Operator : CG/JU
Sample : M2905-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063021\
Data File : BM030809.D
Acq On : 03 Jul 2021 12:49
Operator : CG/JU
Sample : M2905-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBK38

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM062221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
