

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035781.D
 Acq On : 30 Jun 2022 14:57
 Operator : CG/JU
 Sample : N3374-06RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 01 01:16:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng/ul	-7.87
4) Naphthalene-d8	10.567	136	10554	0.400	ng/ul	#-0.05
9) Acenaphthene-d10	14.414	164	4983	0.400	ng/ul	-0.02
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.20
17) Chrysene-d12	21.359	240	13025	0.400	ng/ul	#-0.01
23) Perylene-d12	23.674	264	14272	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	18923	0.000	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.167	152	5671	0.343	ng/ul	-0.06
18) Fluoranthene-d10	19.197	212	11988	0.273	ng/ul	-0.02
Target Compounds						
					Qvalue	
10) Acenaphthylene	14.136	152	538	0.021	ng/ul#	1
11) Acenaphthene	14.474	153	1269	0.063	ng/ul	85
26) Benzo(a)pyrene	23.522	252	4019	0.064	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
Data File : BM035781.D
Acq On : 30 Jun 2022 14:57
Operator : CG/JU
Sample : N3374-06RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 01 01:16:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration




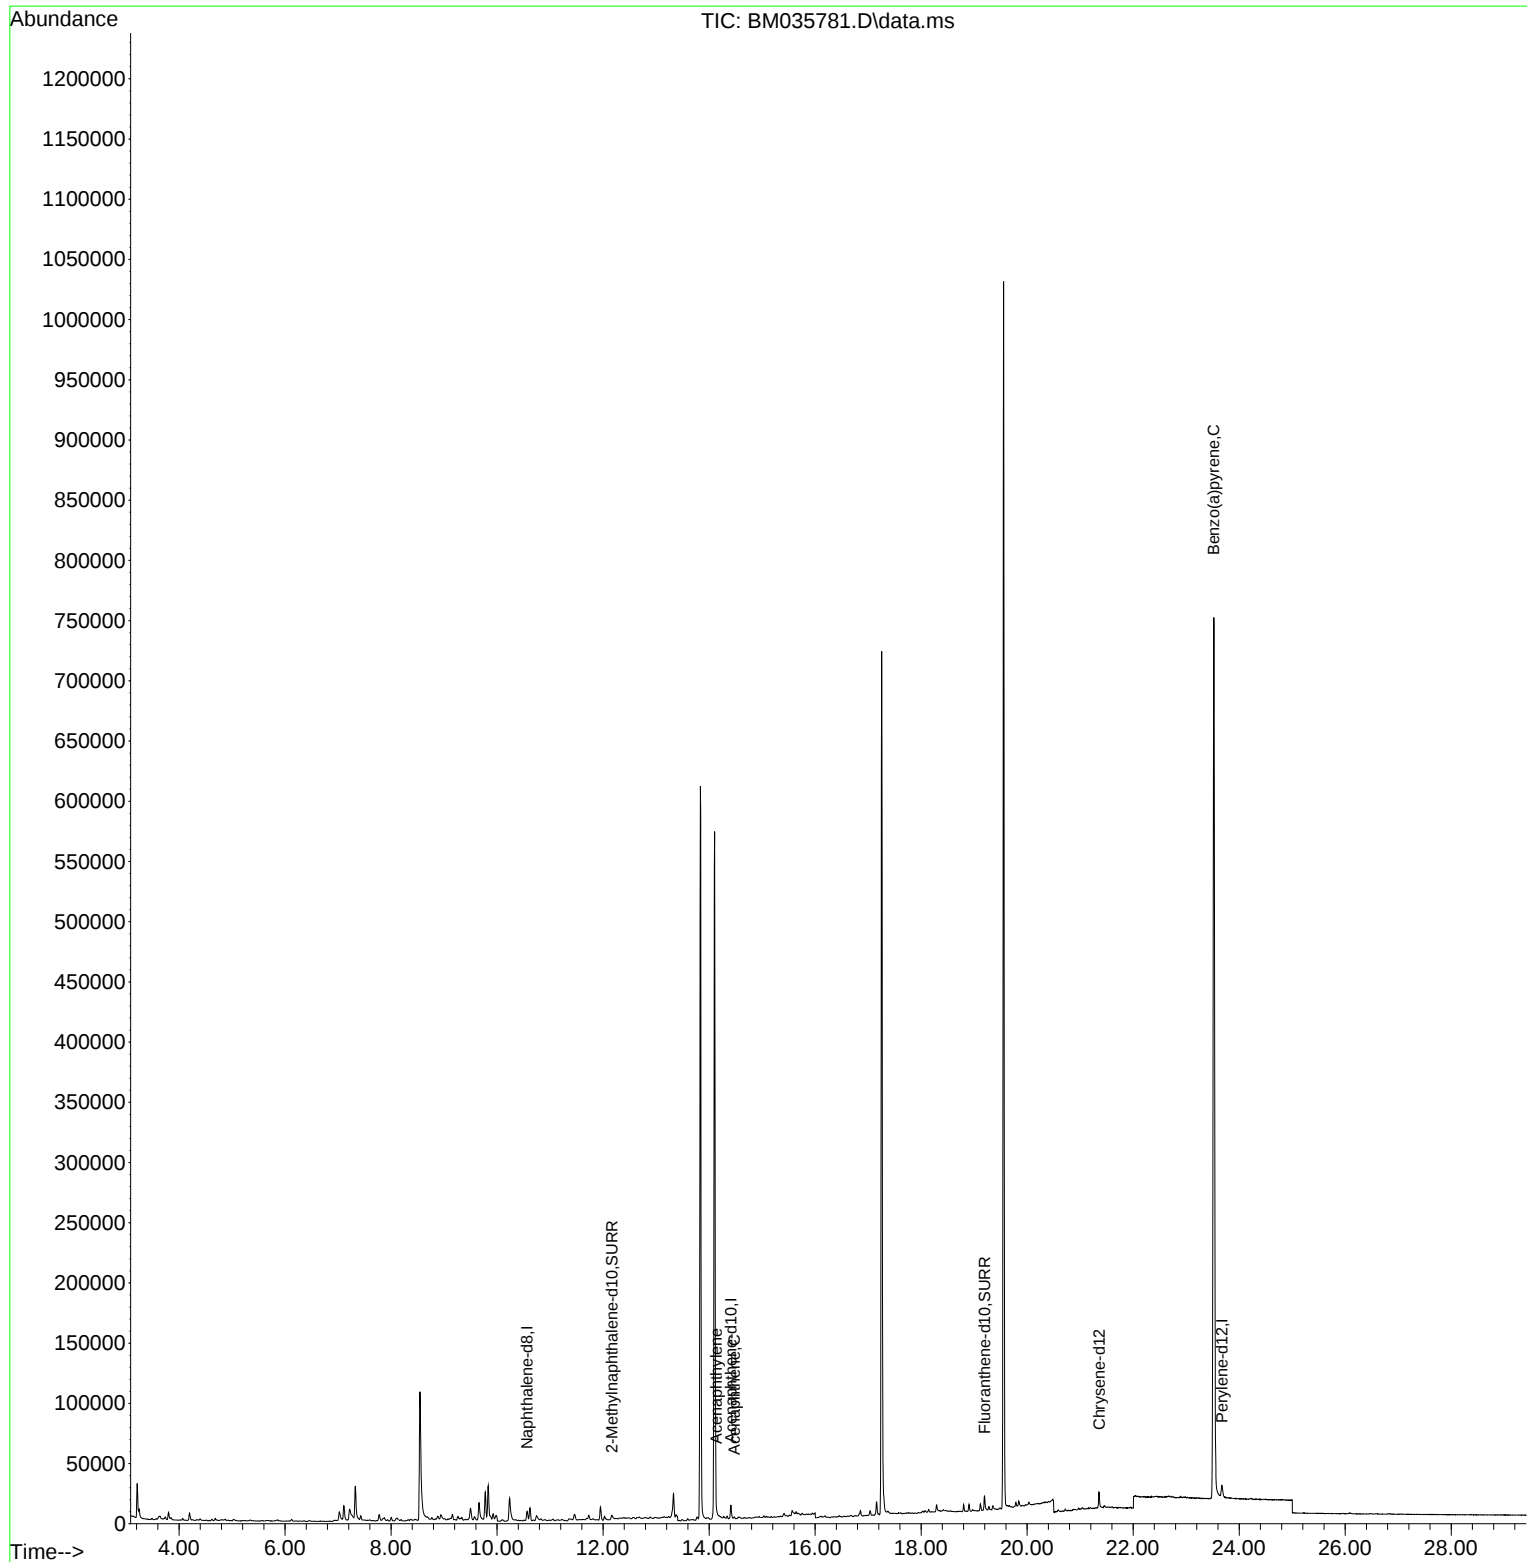


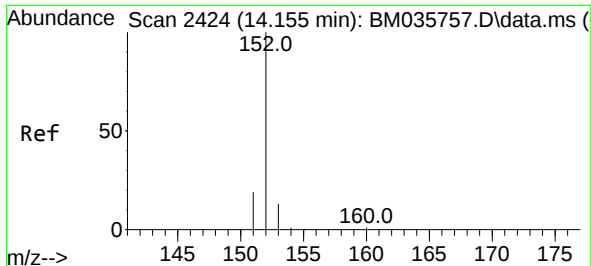

#10
Acenaphthylene
Concen: 0.021 ng/ul
RT: 14.136 min Scan# 2420
Delta R.T. -0.028 min
Lab File: BM035781.D
Acq: 30 Jun 2022 14:57




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:152 Resp: 538
Ion Ratio Lower Upper
152 100
151 99.4 16.6 24.8#
153 113.3 11.4 17.0#

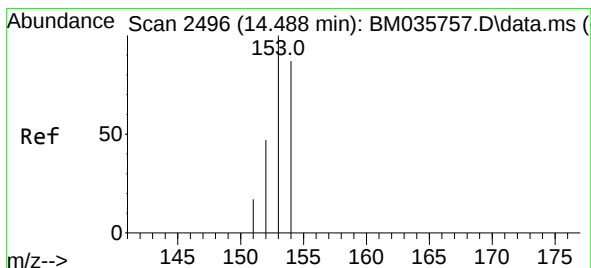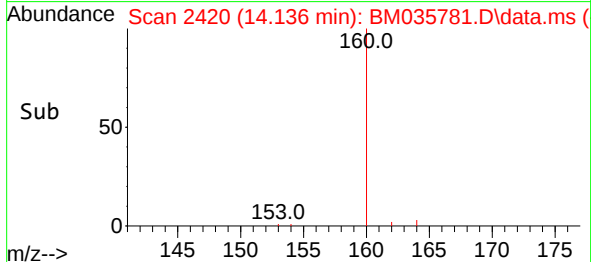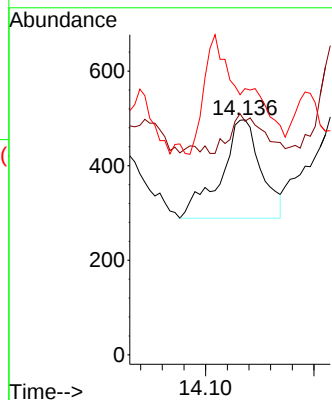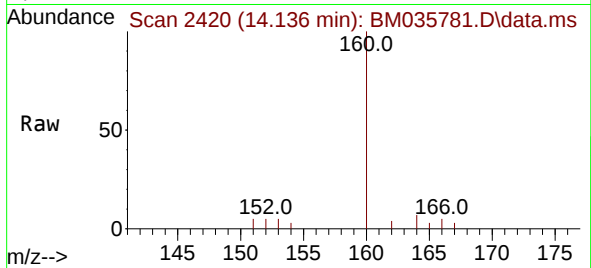

#11
Acenaphthene
Concen: 0.063 ng/ul
RT: 14.474 min Scan# 2493
Delta R.T. -0.023 min
Lab File: BM035781.D
Acq: 30 Jun 2022 14:57


Tgt Ion:153 Resp: 1269
Ion Ratio Lower Upper
153 100
152 58.6 40.2 60.4
154 71.3 69.7 104.5

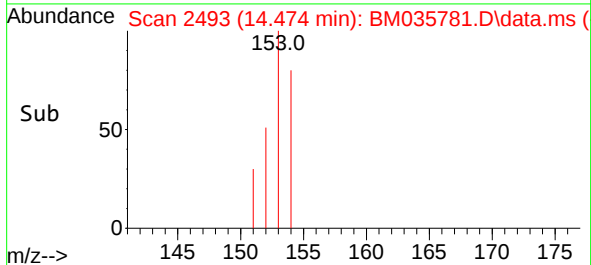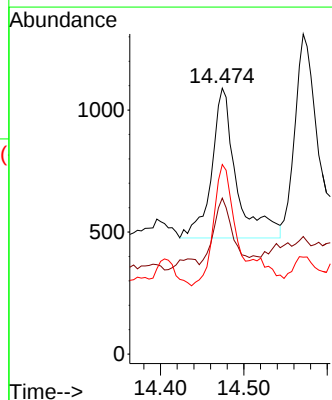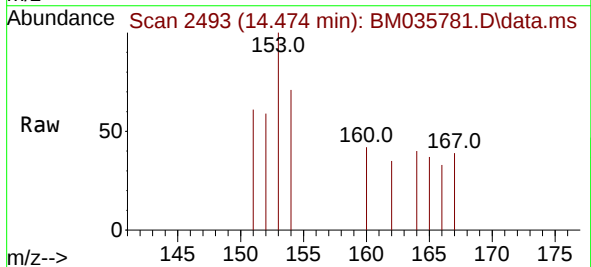

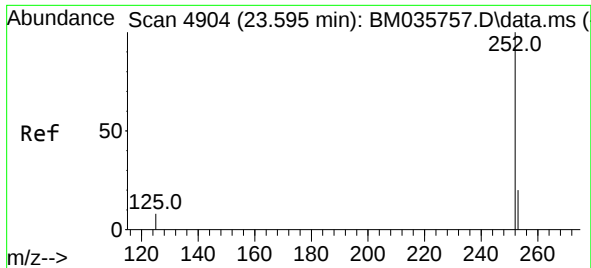

#26
Benzo(a)pyrene
Concen: 0.064 ng/ul
RT: 23.522 min Scan# 4879
Delta R.T. -0.079 min
Lab File: BM035781.D
Acq: 30 Jun 2022 14:57

Instrument :
BNA_M
ClientSampleId :

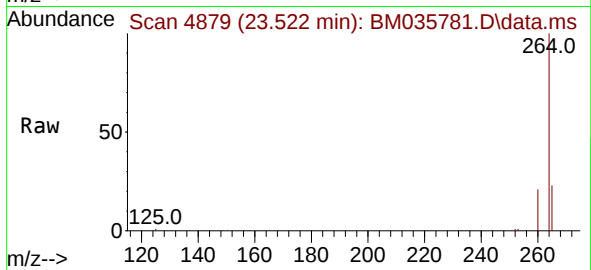

Tgt Ion:252 Resp: 4019
Ion Ratio Lower Upper
252 100
253 117.0 29.7 44.5#
125 104.3 23.6 35.4#

