




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035761.D
Acq On : 29 Jun 2022 15:07
Operator : CG/JU
Sample : N3374-07RE
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

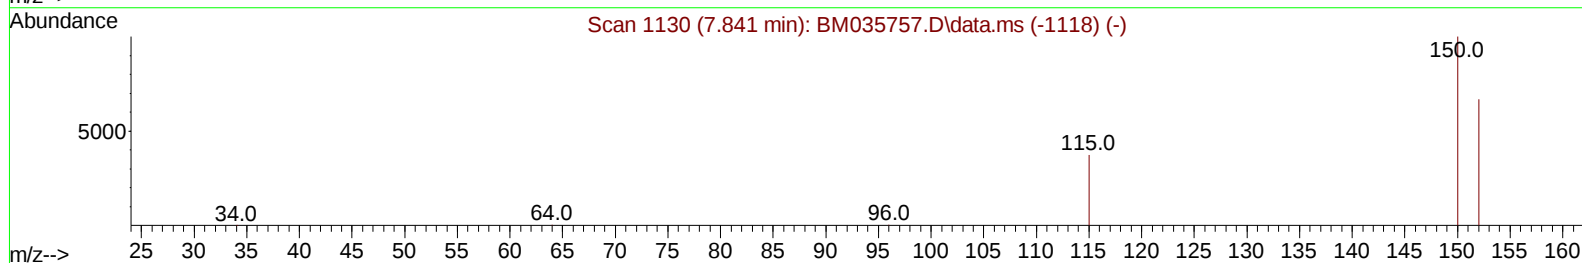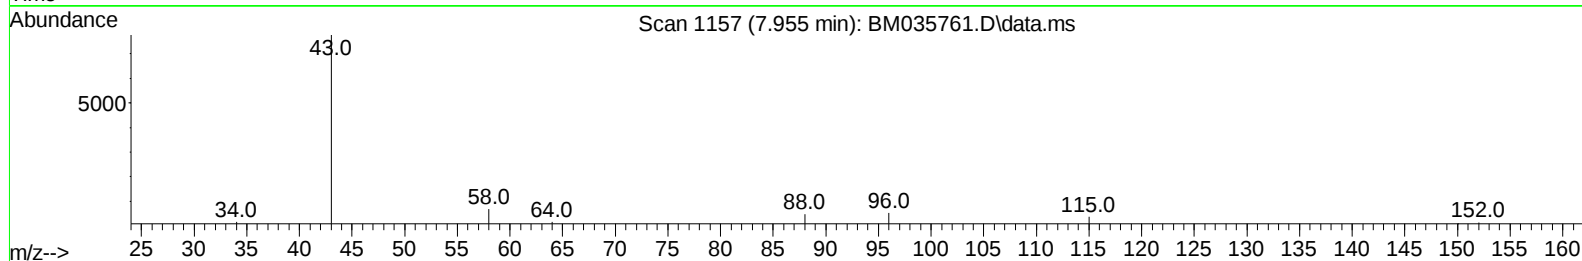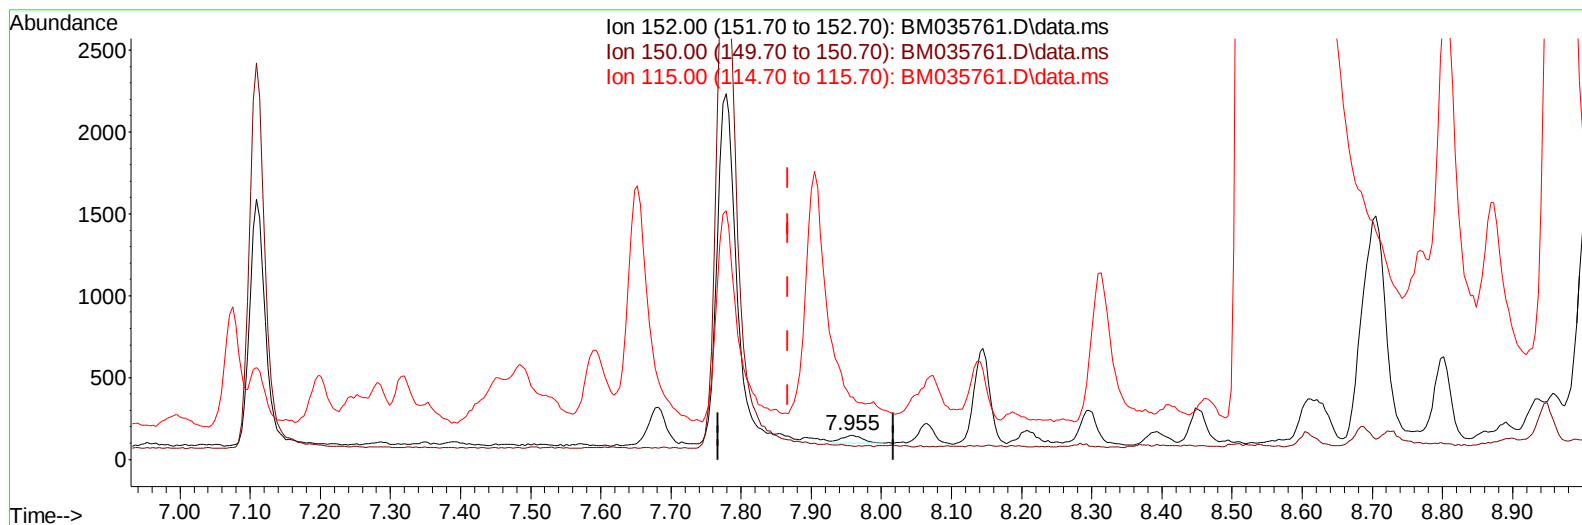

TIC: BM035761.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.955min (+ 0.088) 0.40 ng/u1

response 99

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	147.40	57.82#
115.00	74.40	259.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035761.D
Acq On : 29 Jun 2022 15:07
Operator : CG/JU
Sample : N3374-07RE
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

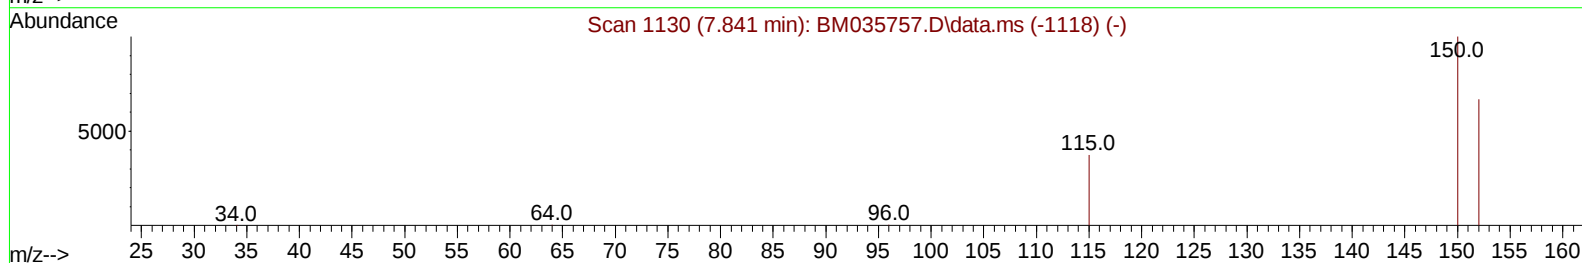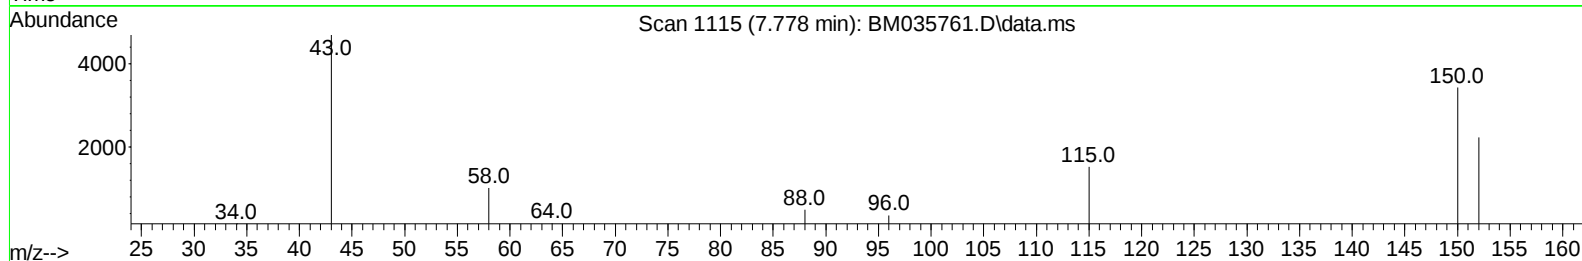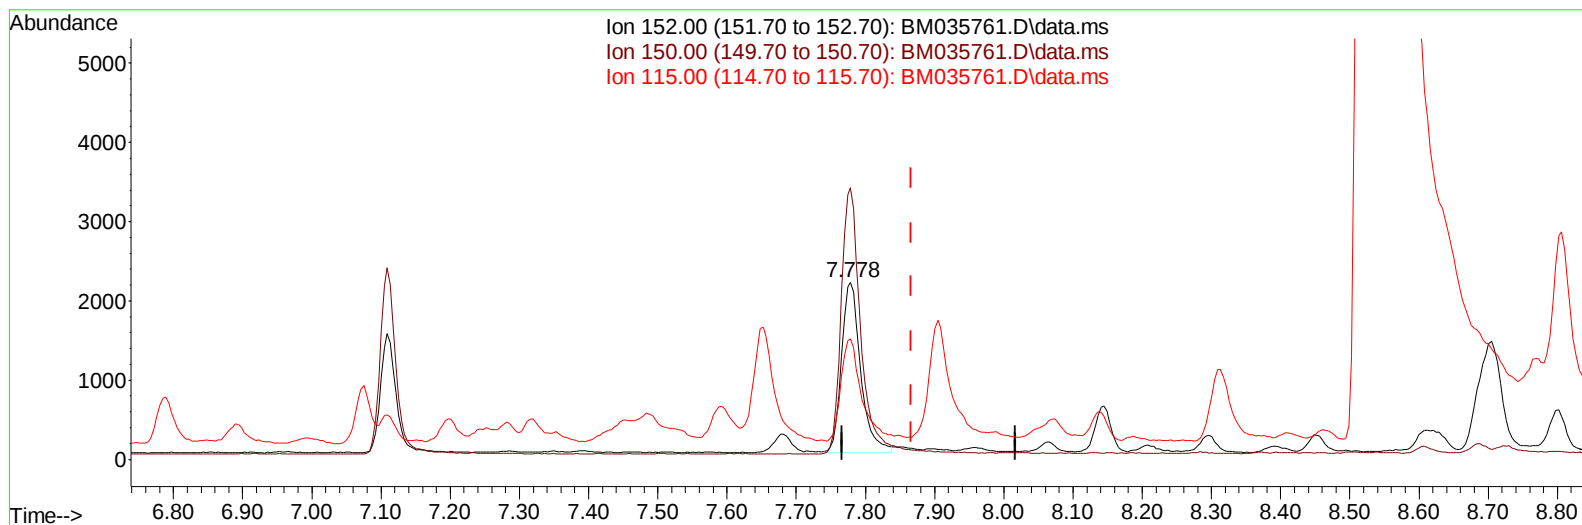

TIC: BM035761.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.778min (-0.089) 0.40 ng/ul m

response 4125

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	147.40	153.36
115.00	74.40	68.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035761.D
Acq On : 29 Jun 2022 15:07
Operator : CG/JU
Sample : N3374-07RE
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

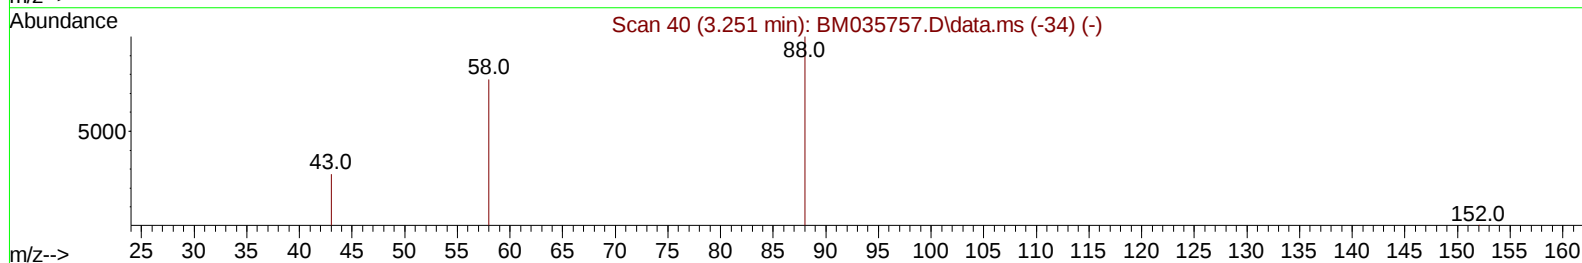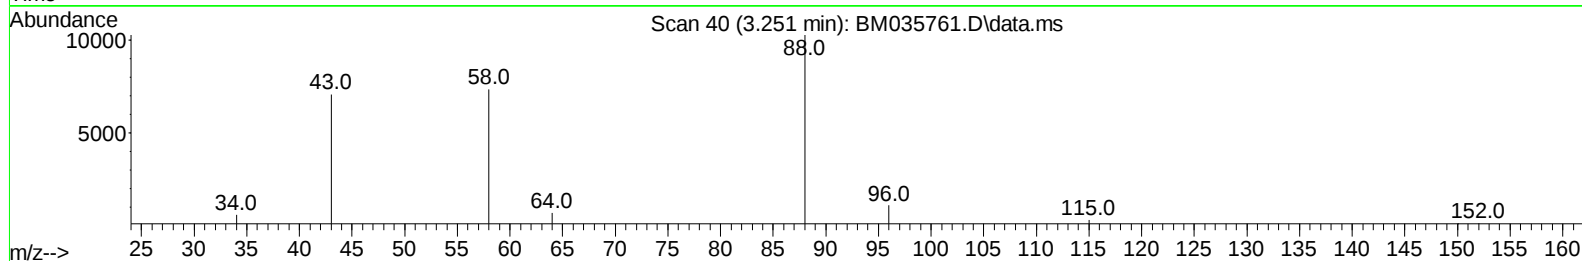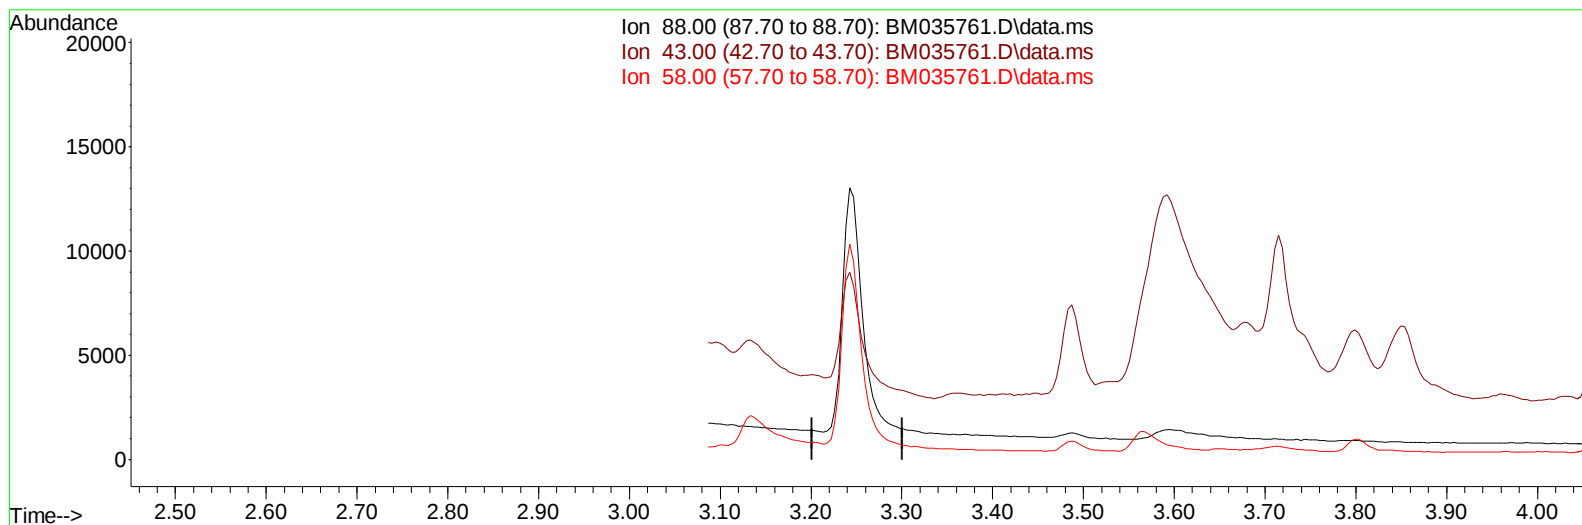

TIC: BM035761.D\data.ms

(2) 1,4-Dioxane

3.251min (-3.251) 0.00 ng/u1

response 0

Ion	Exp%	Act%
88.00	100.00	0.00
43.00	47.20	0.00#
58.00	53.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035761.D
 Acq On : 29 Jun 2022 15:07
 Operator : CG/JU
 Sample : N3374-07RE
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

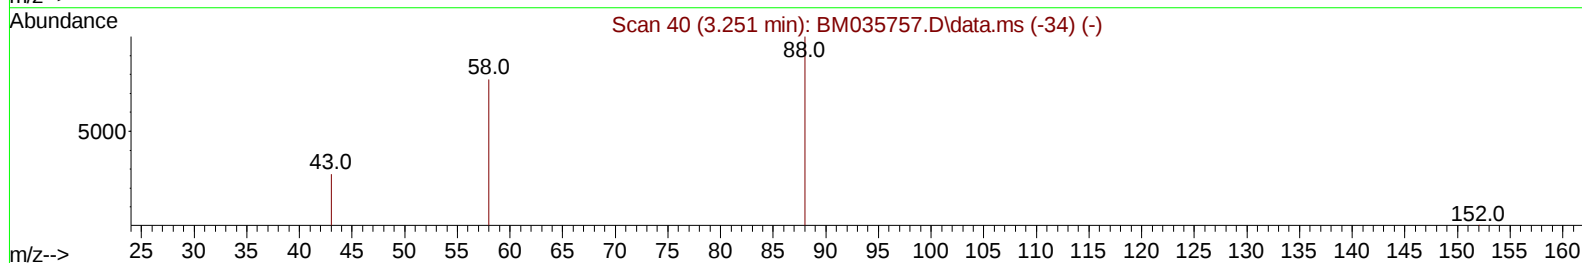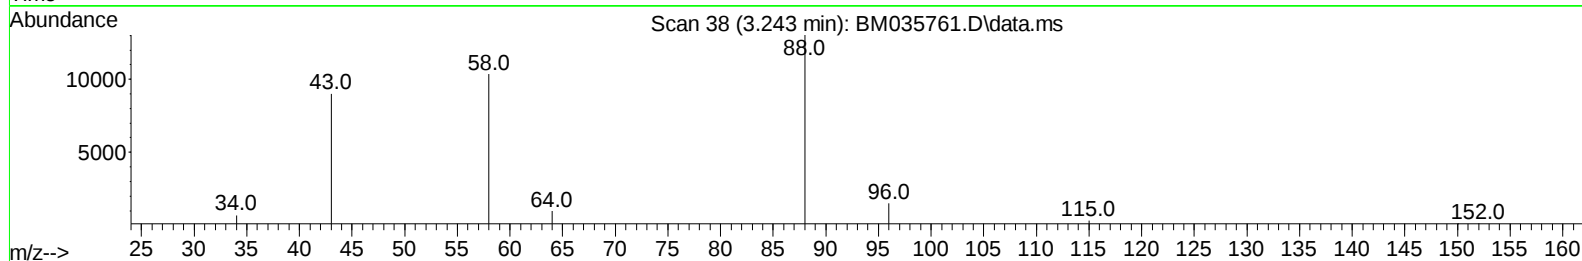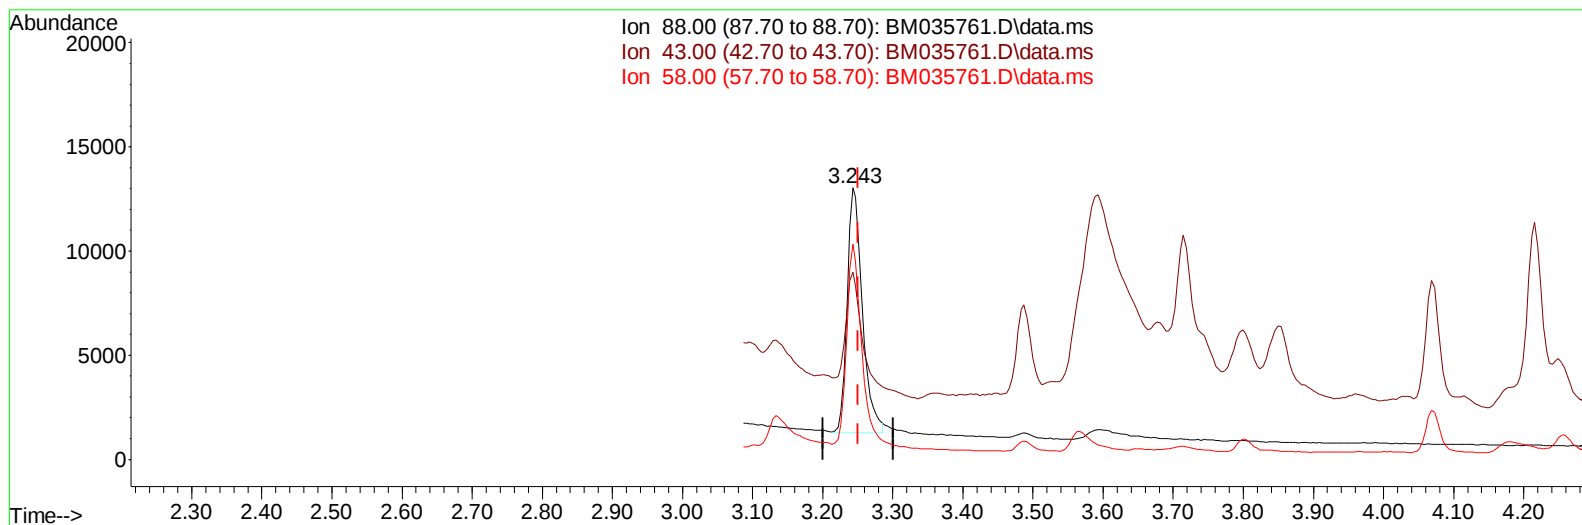

TIC: BM035761.D\data.ms

(2) 1,4-Dioxane

3.243min (-0.008) 3.21 ng/ul m

response 17773

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	47.20	68.91#
58.00	53.20	79.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
Data File : BM035761.D
Acq On : 29 Jun 2022 15:07
Operator : CG/JU
Sample : N3374-07RE
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

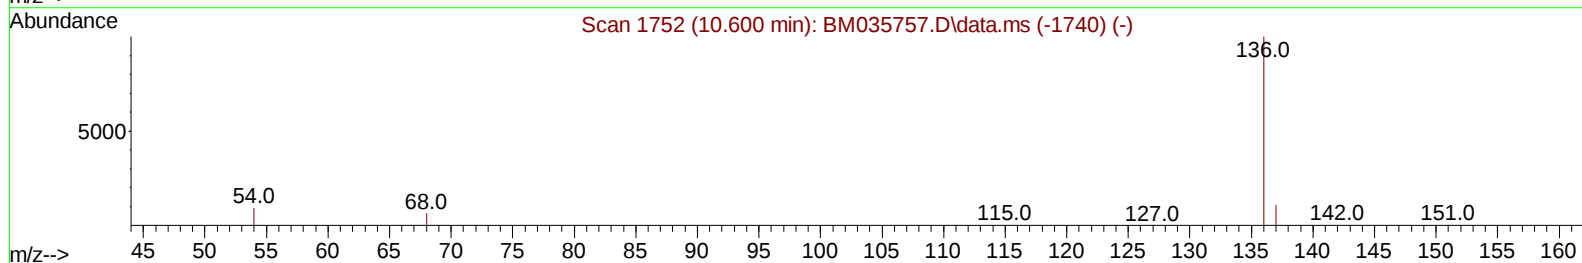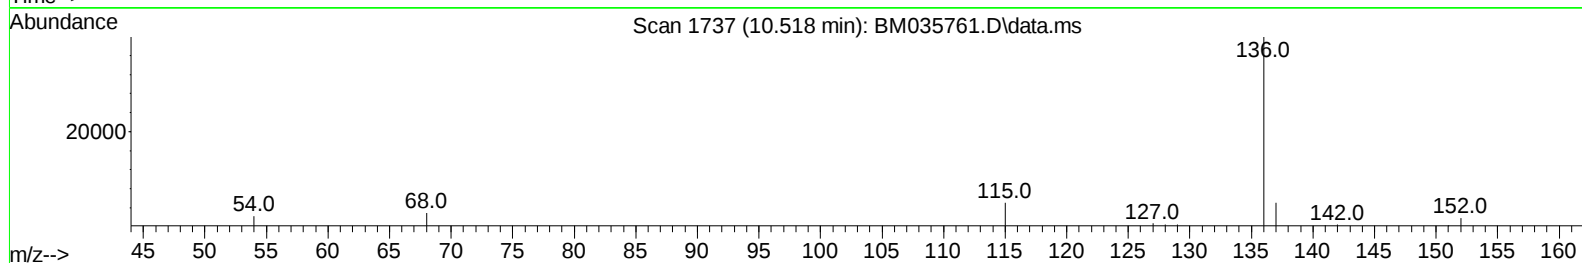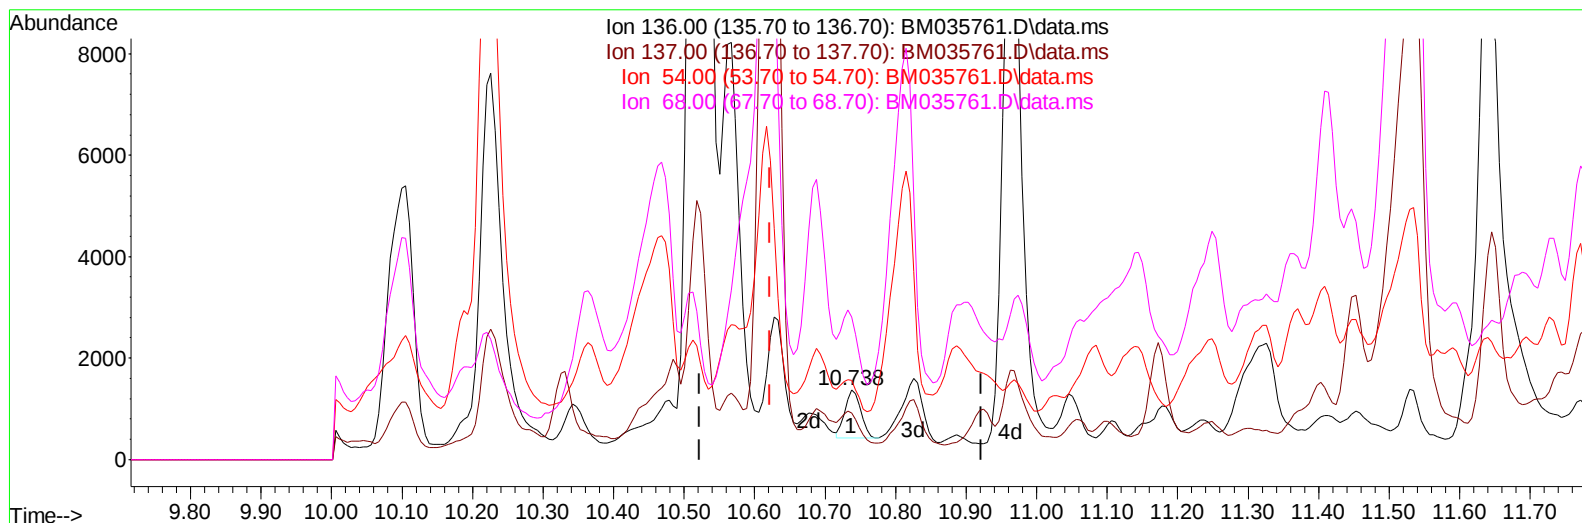

TIC: BM035761.D\data.ms

(4) Naphthalene-d8 (I)

10.738min (+ 0.116) 0.40 ng/u1

response 1487

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	67.11#
54.00	12.20	113.99#
68.00	8.00	206.08#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035761.D
 Acq On : 29 Jun 2022 15:07
 Operator : CG/JU
 Sample : N3374-07RE
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

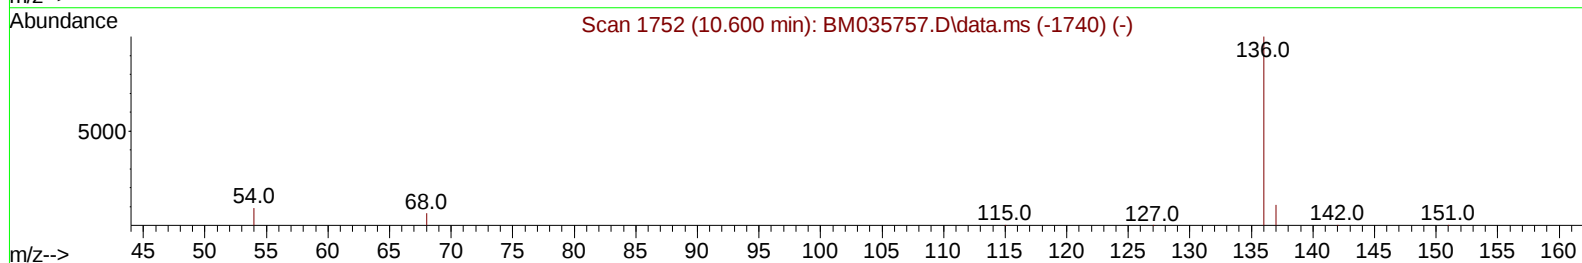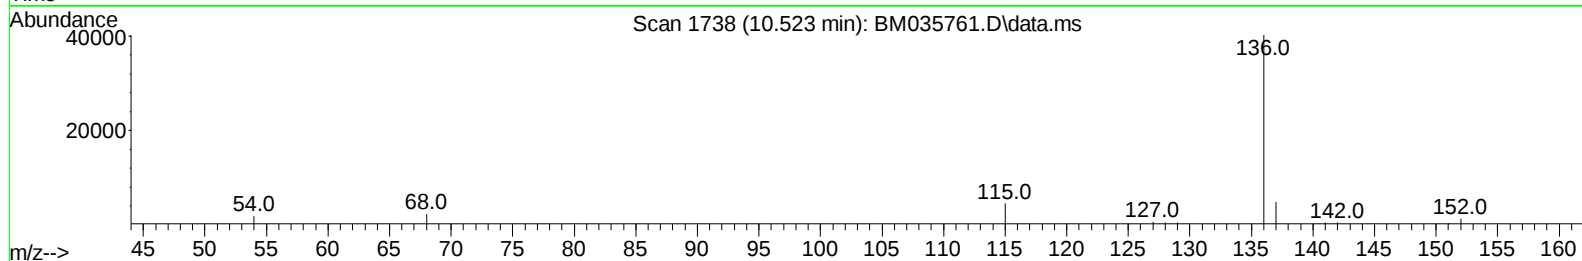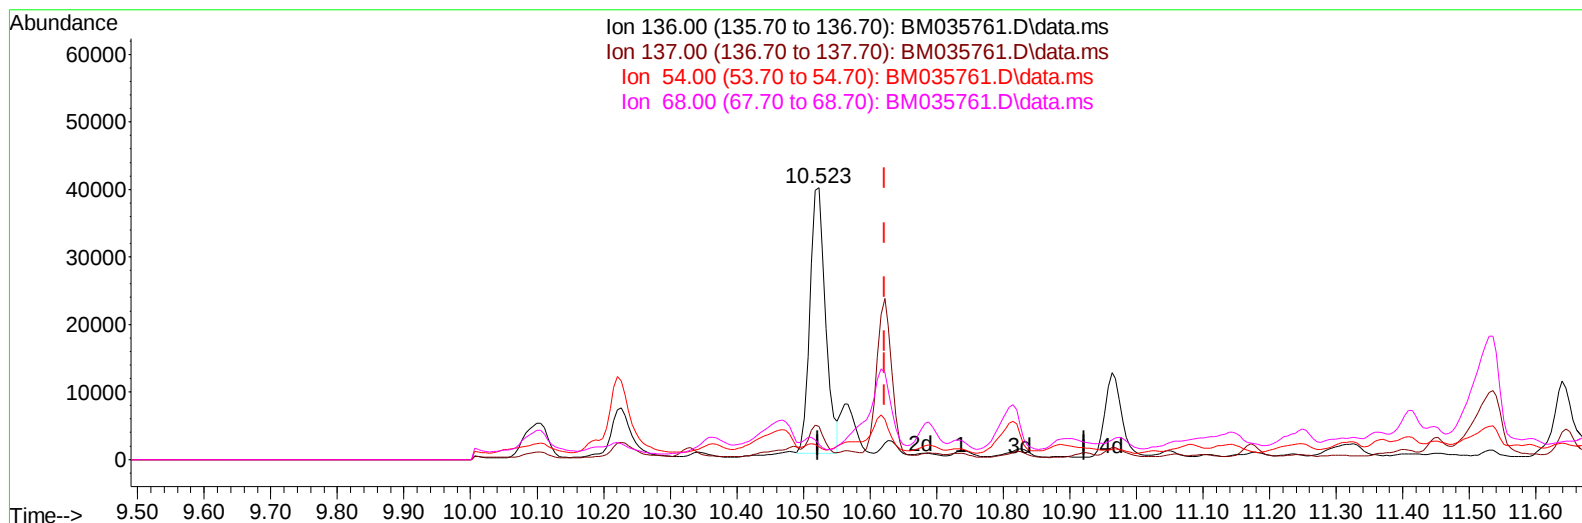

TIC: BM035761.D\data.ms

(4) Naphthalene-d8 (I)

10.523min (-0.099) 0.40 ng/ul m

response 64416

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	12.07
54.00	12.20	4.65#
68.00	8.00	5.59#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035761.D
 Acq On : 29 Jun 2022 15:07
 Operator : CG/JU
 Sample : N3374-07RE
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 STDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

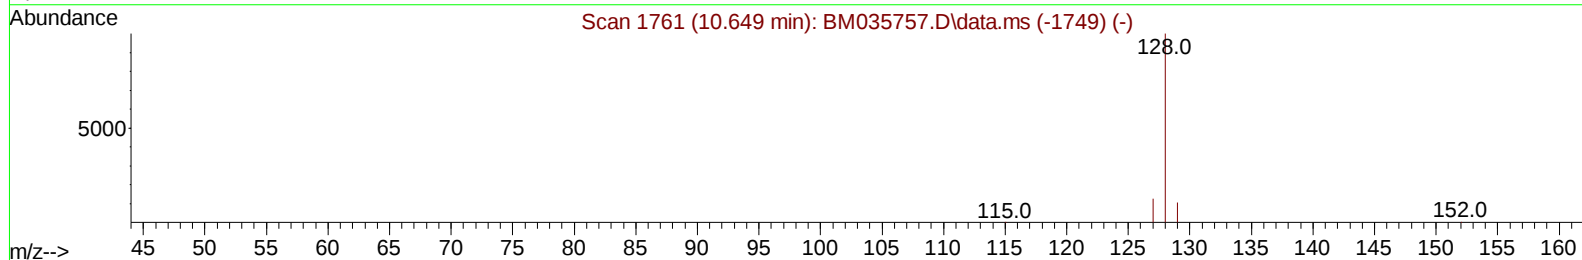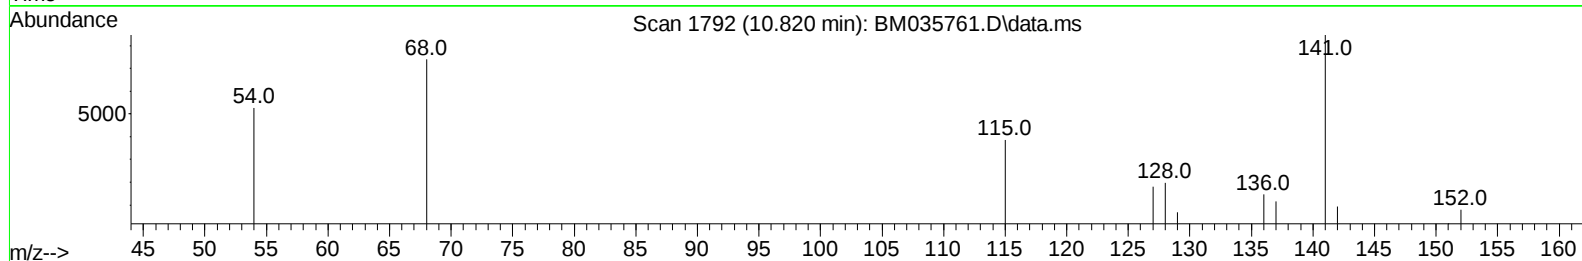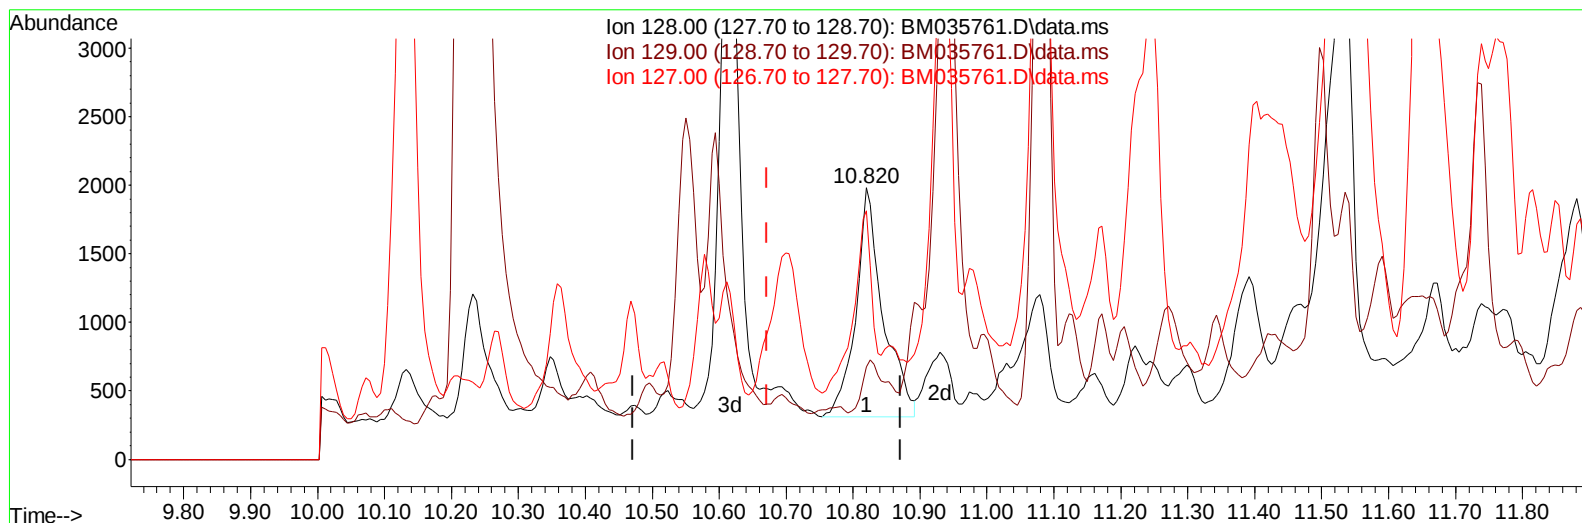

TIC: BM035761.D\data.ms

(5) Naphthalene

10.820min (+ 0.149) 0.02 ng/u1

response 4667

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.70	34.09#
127.00	14.60	91.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035761.D
 Acq On : 29 Jun 2022 15:07
 Operator : CG/JU
 Sample : N3374-07RE
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

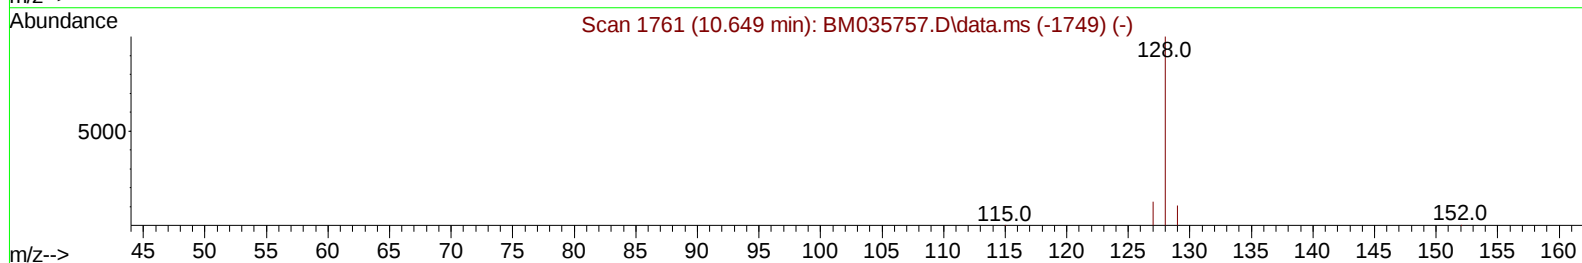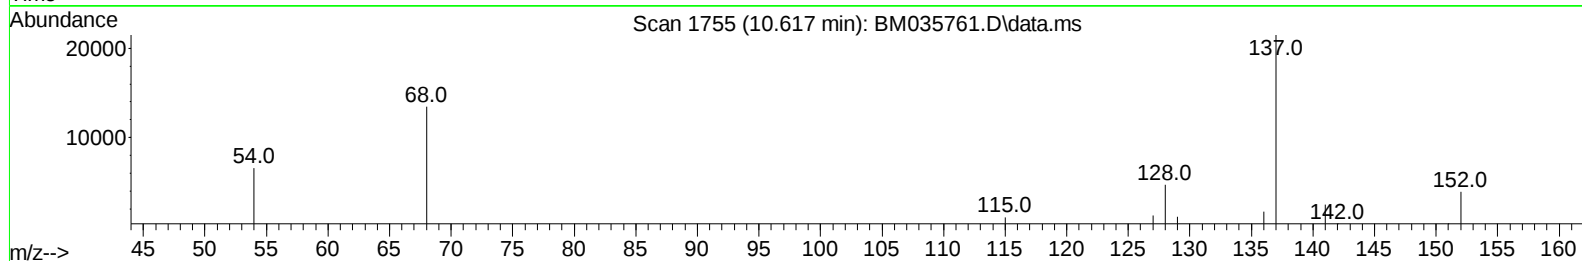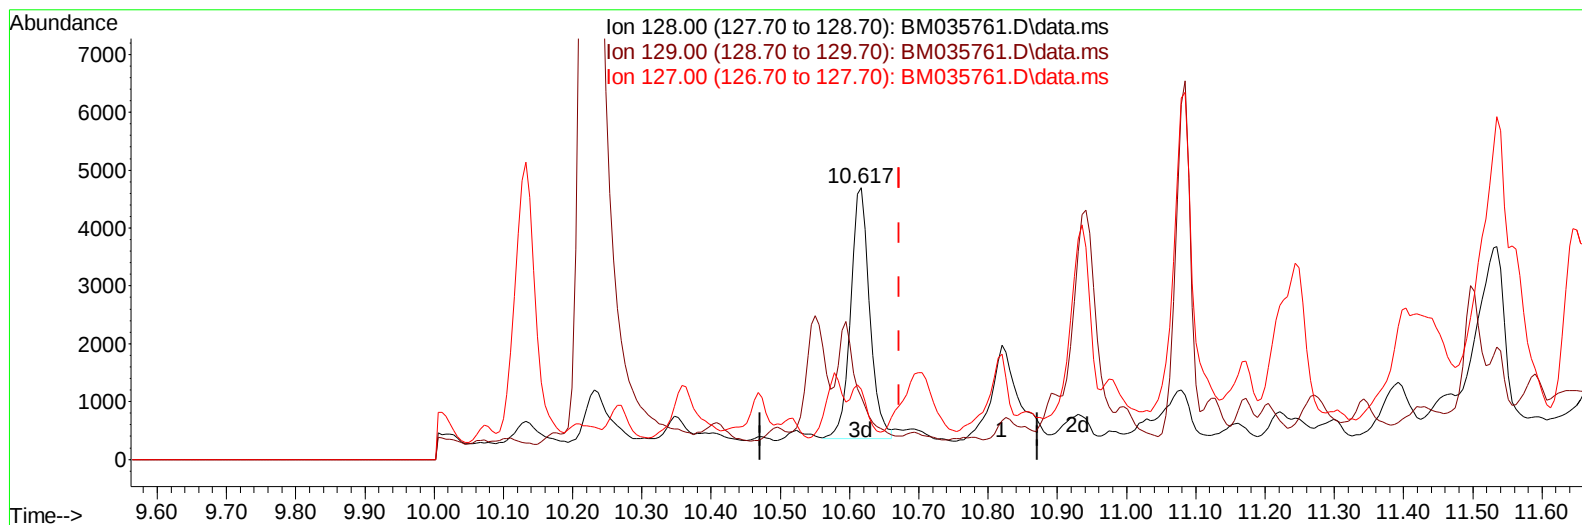

TIC: BM035761.D\data.ms

(5) Naphthalene

10.617min (-0.055) 0.04 ng/ul m

response 8232

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.70	22.97#
127.00	14.60	25.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035761.D
 Acq On : 29 Jun 2022 15:07
 Operator : CG/JU
 Sample : N3374-07RE
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

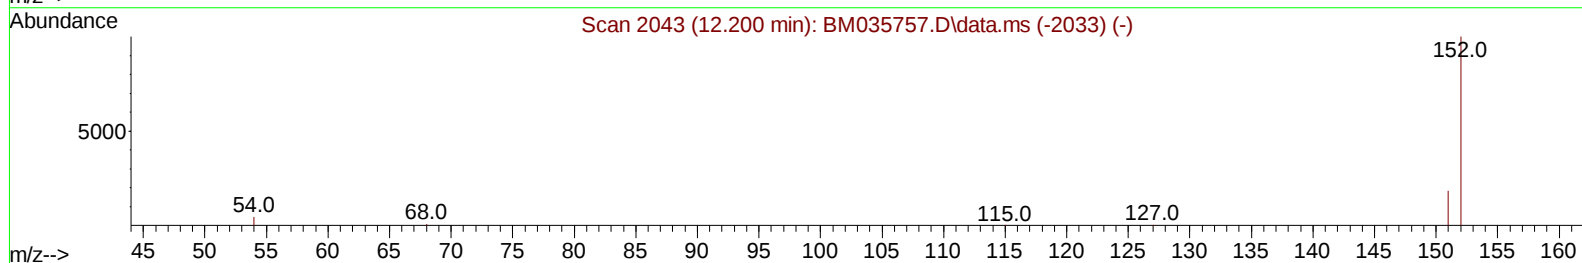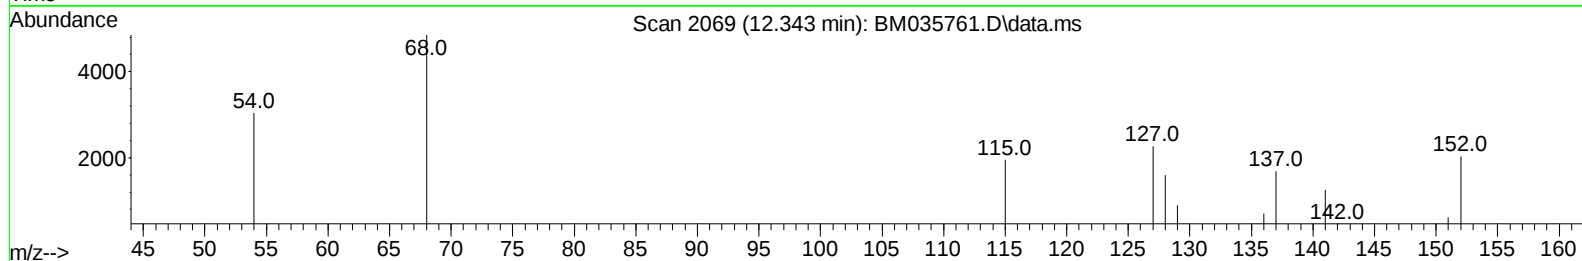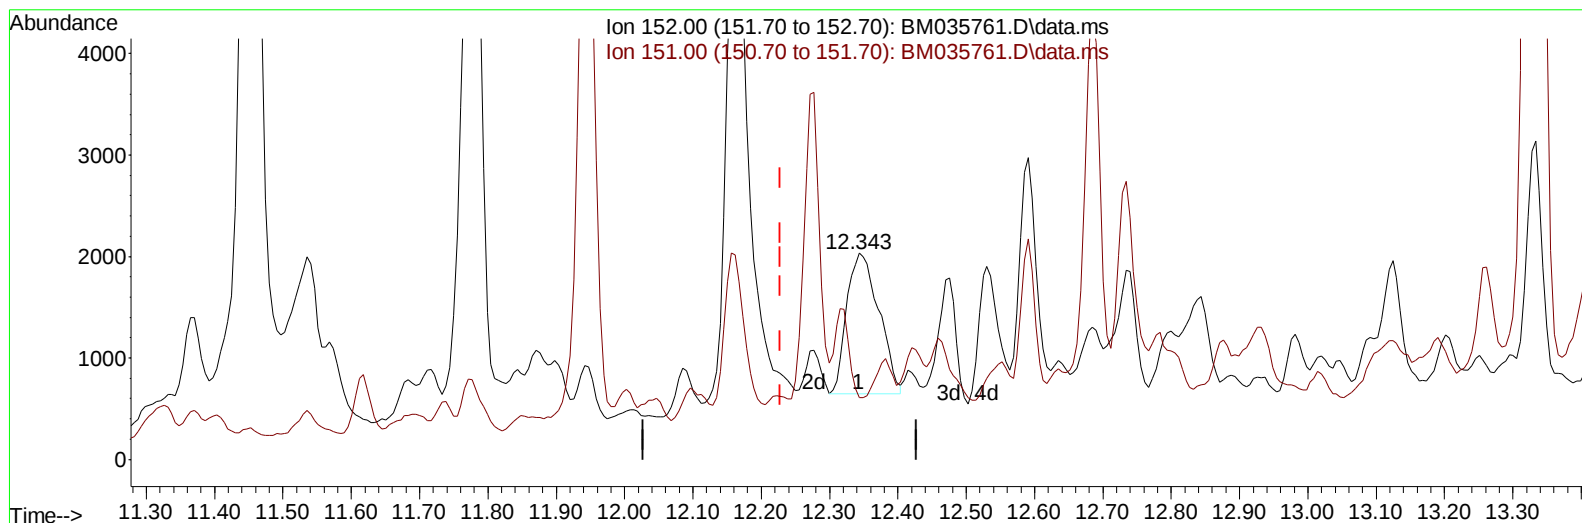

TIC: BM035761.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.343min (+ 0.116) 0.04 ng/u1

response 4510

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.80	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062822\
 Data File : BM035761.D
 Acq On : 29 Jun 2022 15:07
 Operator : CG/JU
 Sample : N3374-07RE
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jun 30 02:42:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

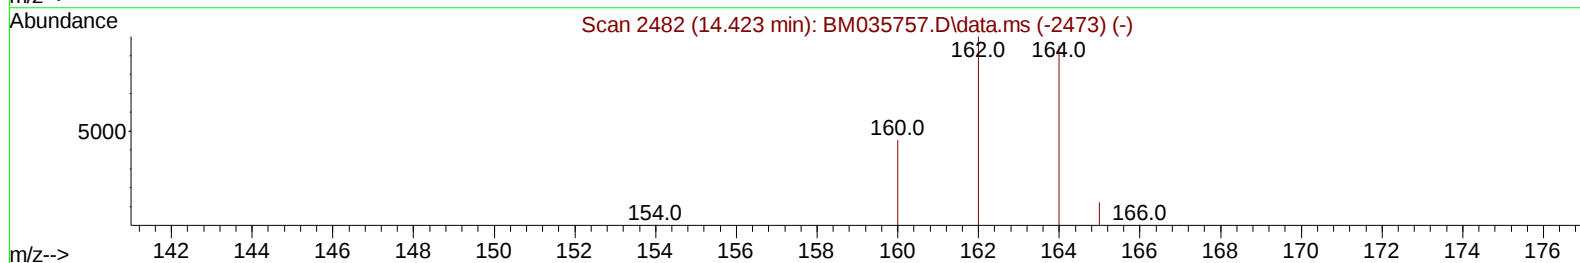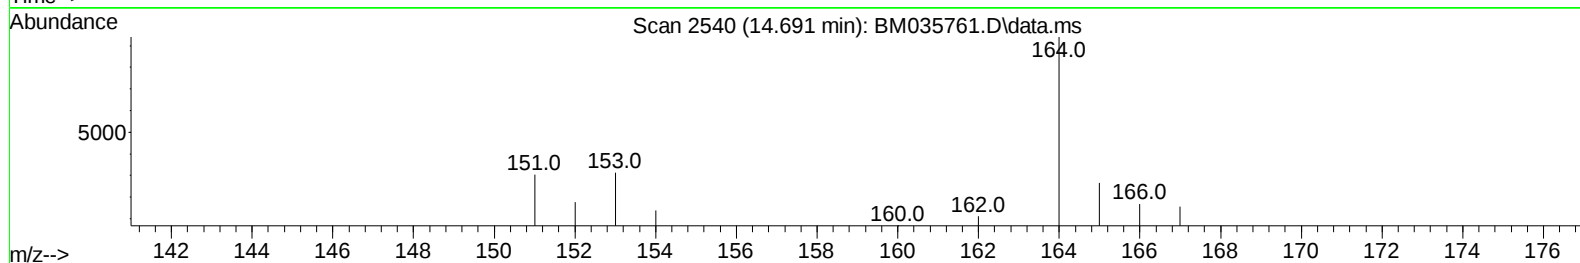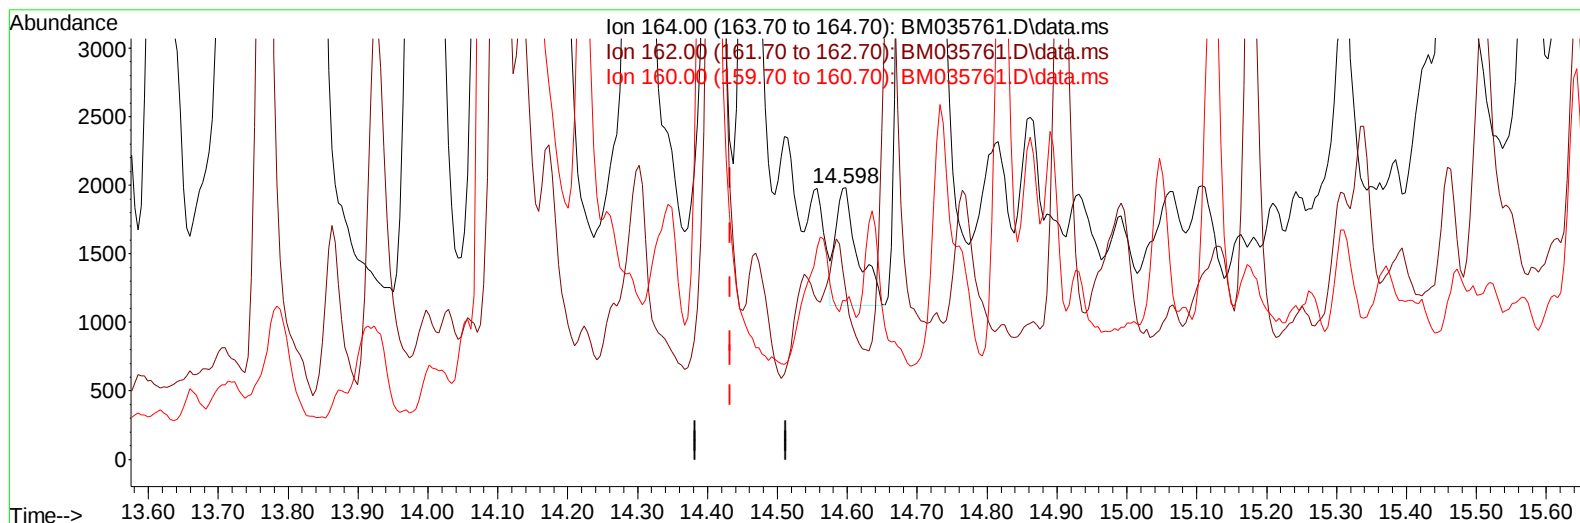

TIC: BM035761.D\data.ms

(9) Acenaphthene-d10 (I)

14.598min (+ 0.166) 0.40 ng/u1

response 1860

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.10	61.87#
160.00	48.90	58.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
Data File : BM035776.D
Acq On : 30 Jun 2022 11:49
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

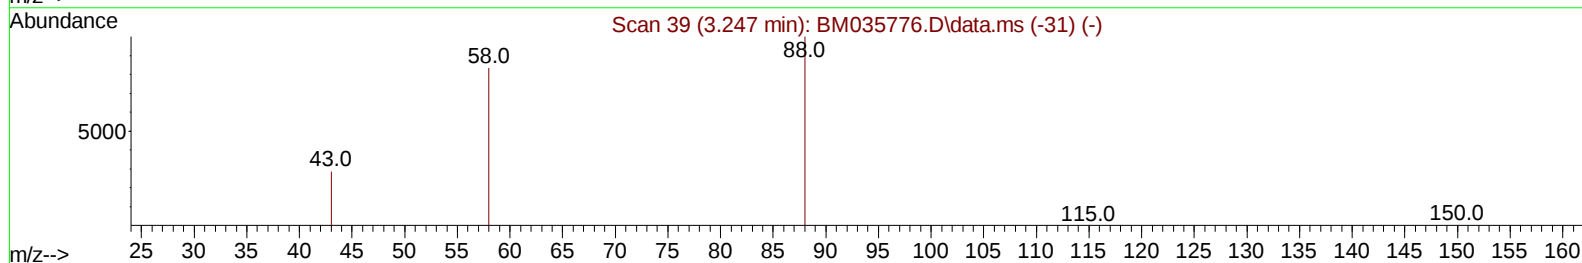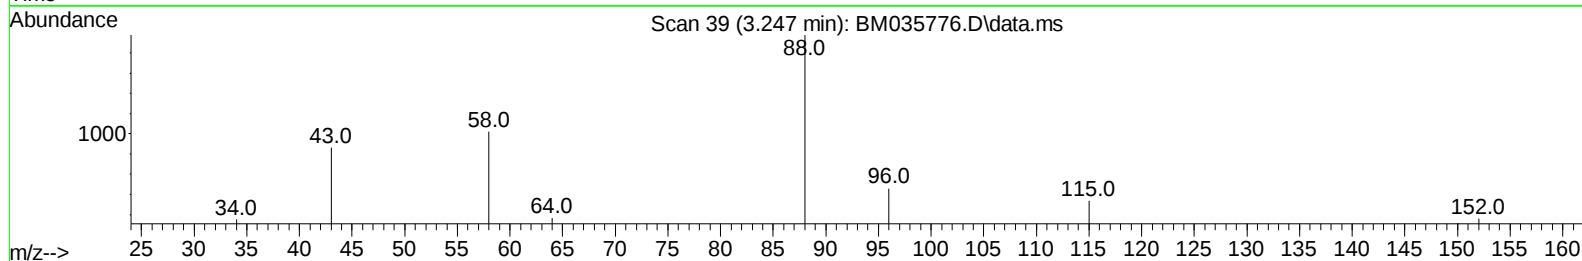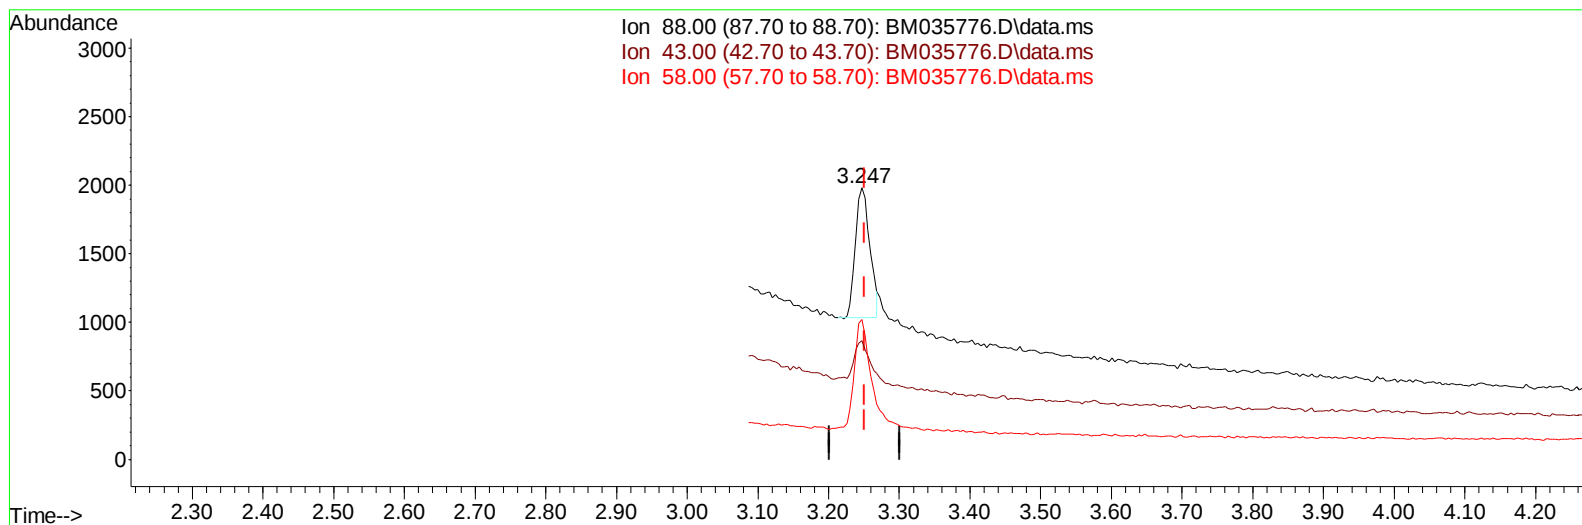

TIC: BM035776.D\data.ms

(2) 1,4-Dioxane

3.247min (-0.004) 0.43 ng/u1

response 1349

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	47.20	43.74
58.00	53.20	51.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035776.D
 Acq On : 30 Jun 2022 11:49
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

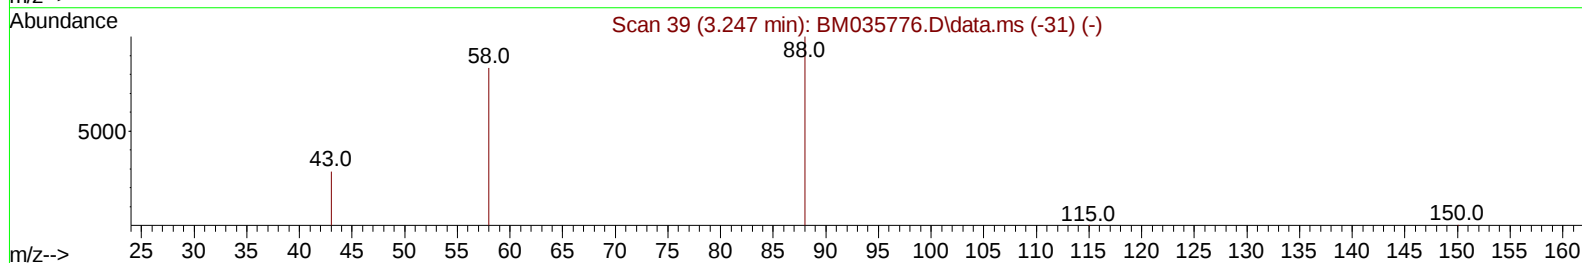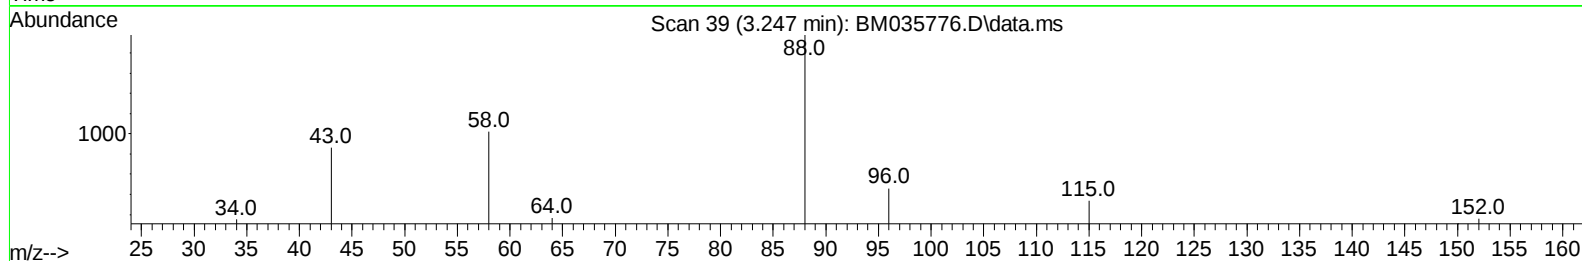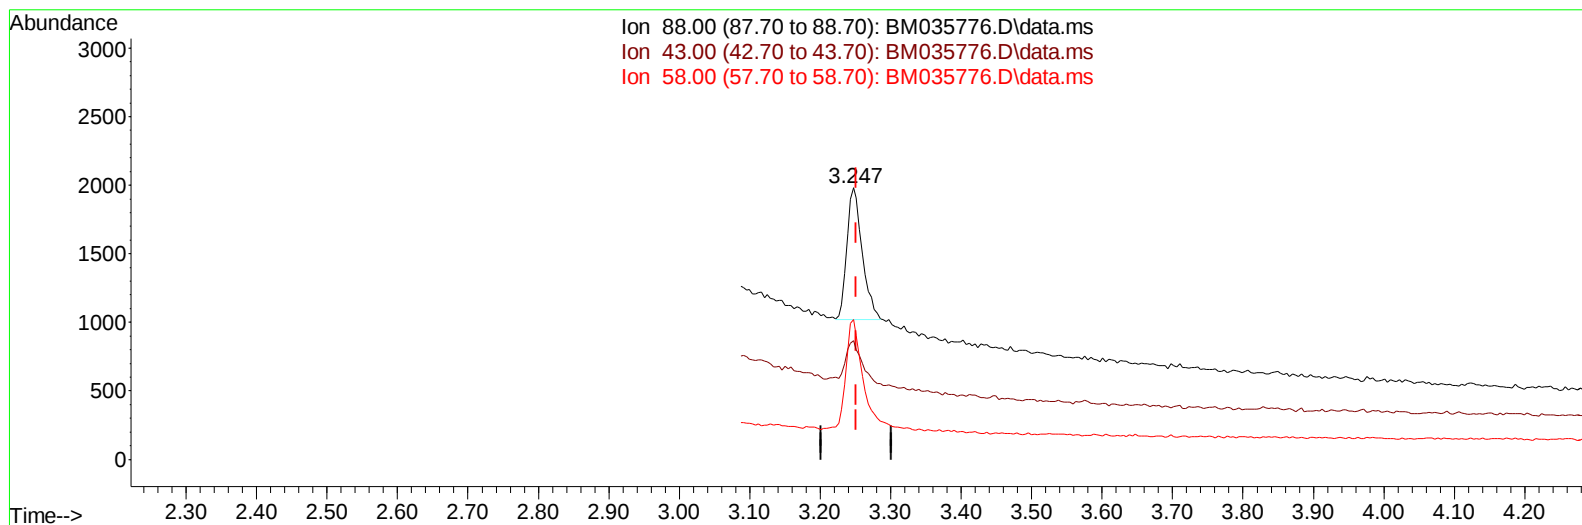

TIC: BM035776.D\data.ms

(2) 1,4-Dioxane

3.247min (-0.004) 0.46 ng/ul m

response 1459

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	47.20	43.74
58.00	53.20	51.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035776.D
 Acq On : 30 Jun 2022 11:49
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

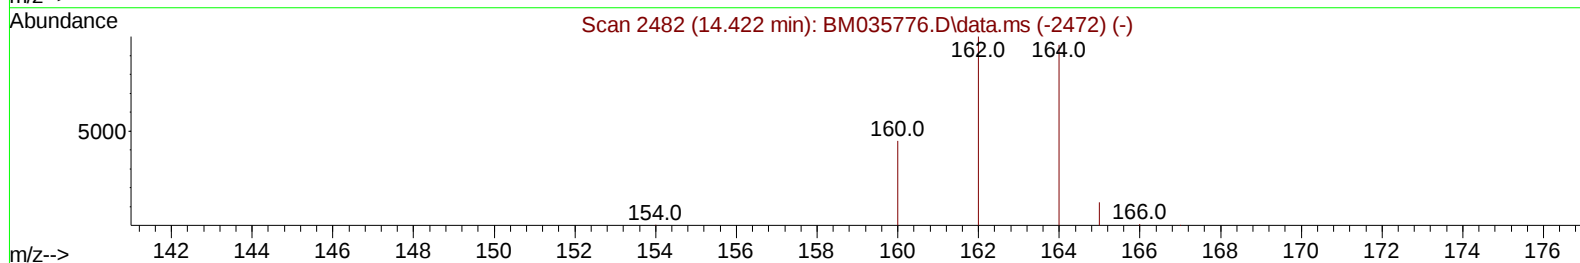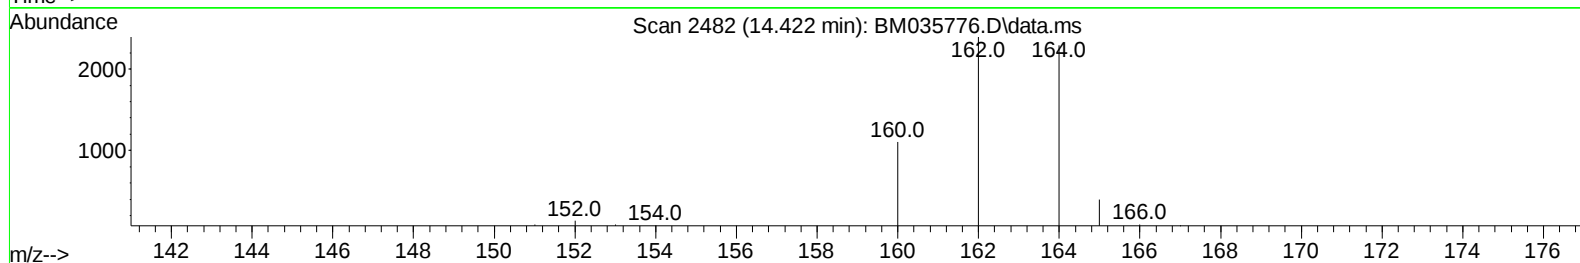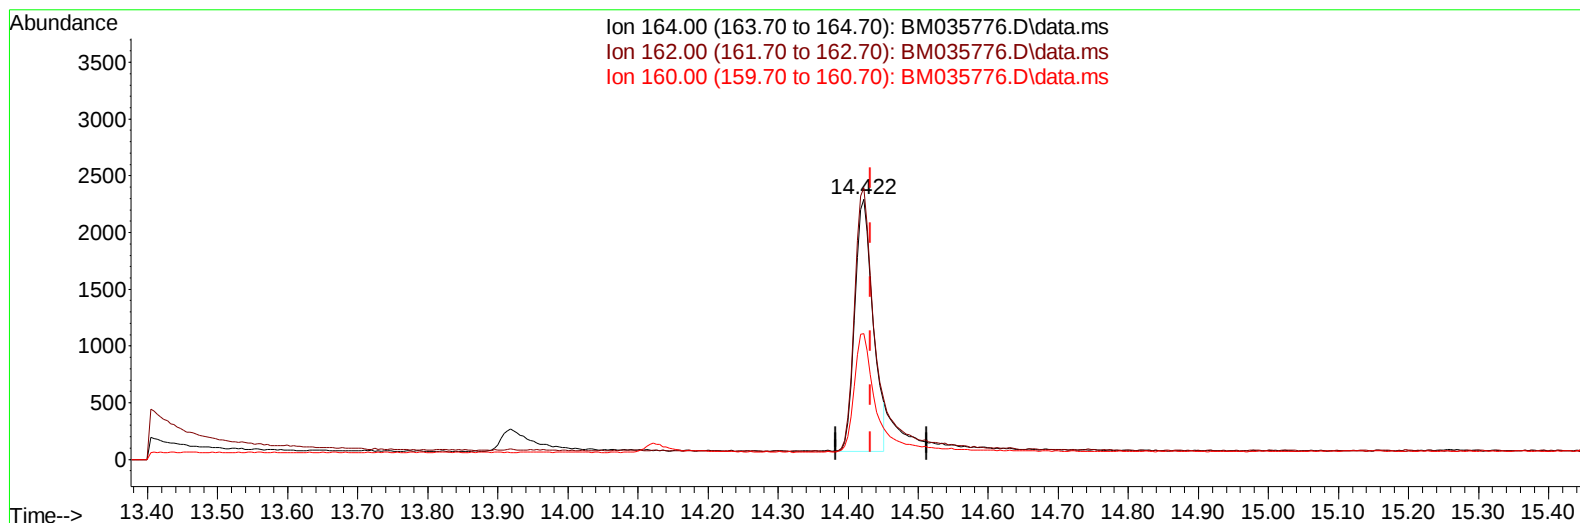

TIC: BM035776.D\data.ms

(9) Acenaphthene-d10 (I)

14.422min (-0.010) 0.40 ng/u1

response 4020

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.10	104.32
160.00	48.90	48.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035776.D
 Acq On : 30 Jun 2022 11:49
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

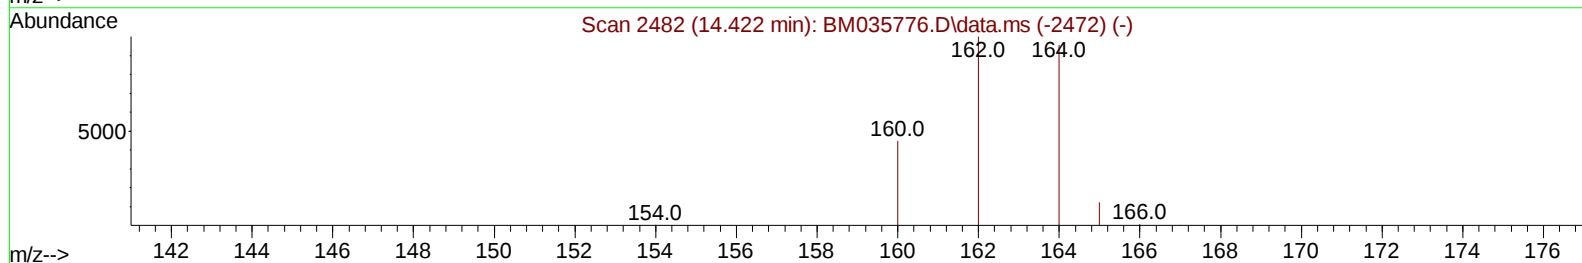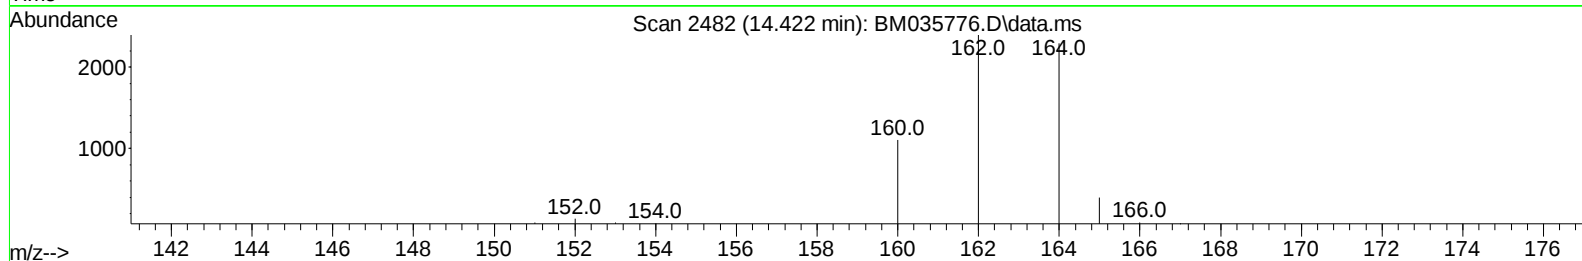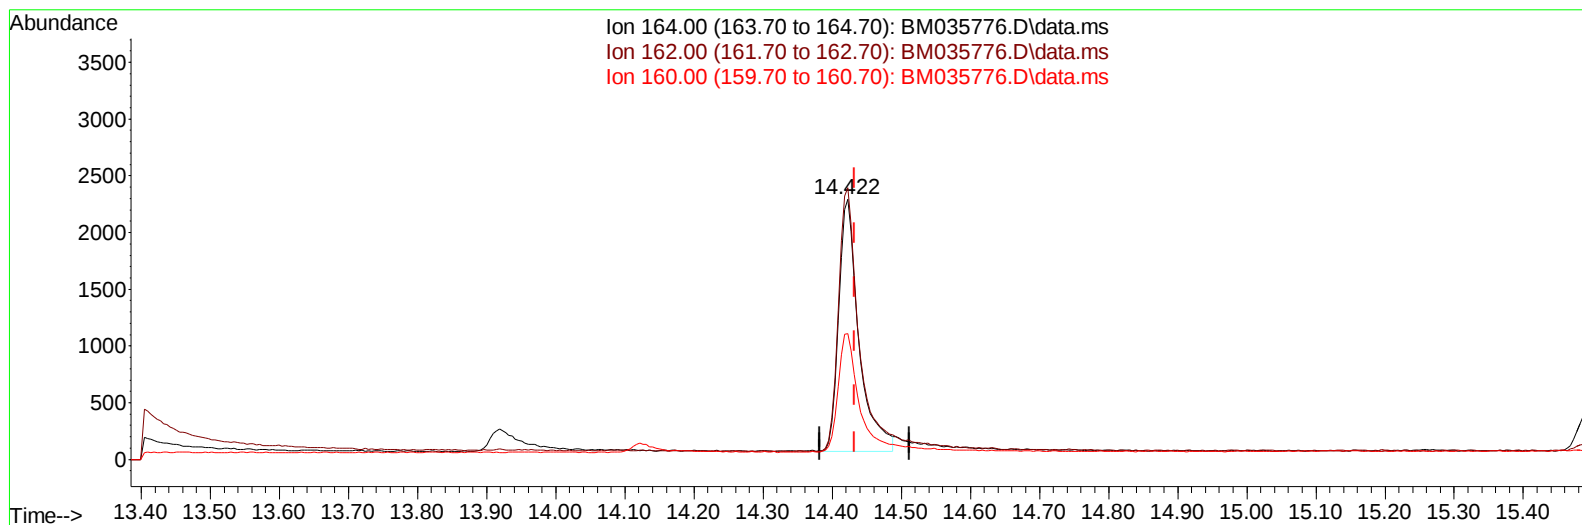

TIC: BM035776.D\data.ms

(9) Acenaphthene-d10 (I)

14.422min (-0.010) 0.40 ng/ul m

response 4514

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.10	104.32
160.00	48.90	48.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
Data File : BM035776.D
Acq On : 30 Jun 2022 11:49
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

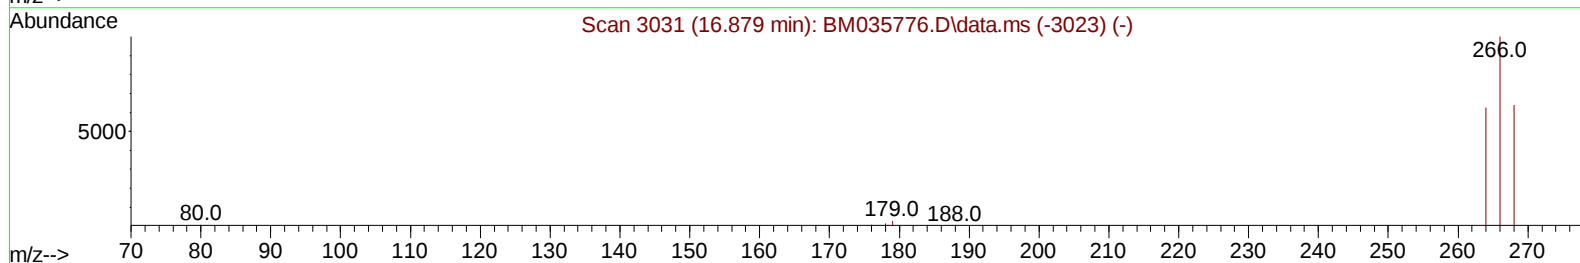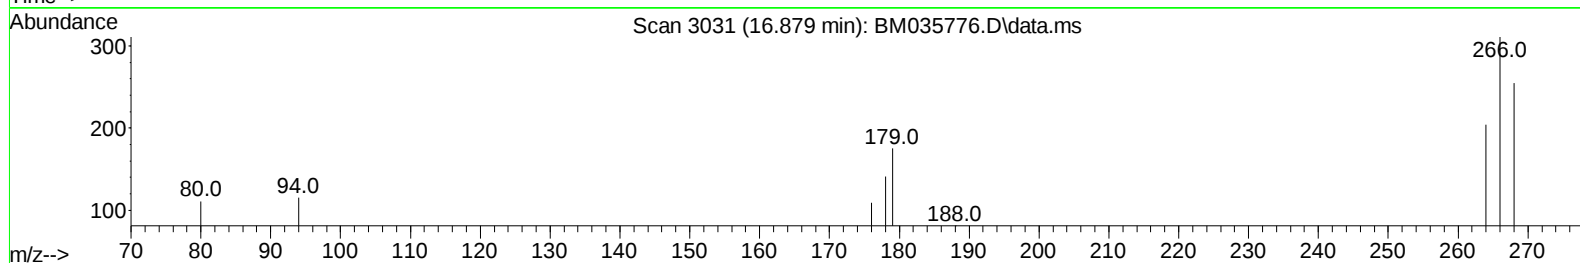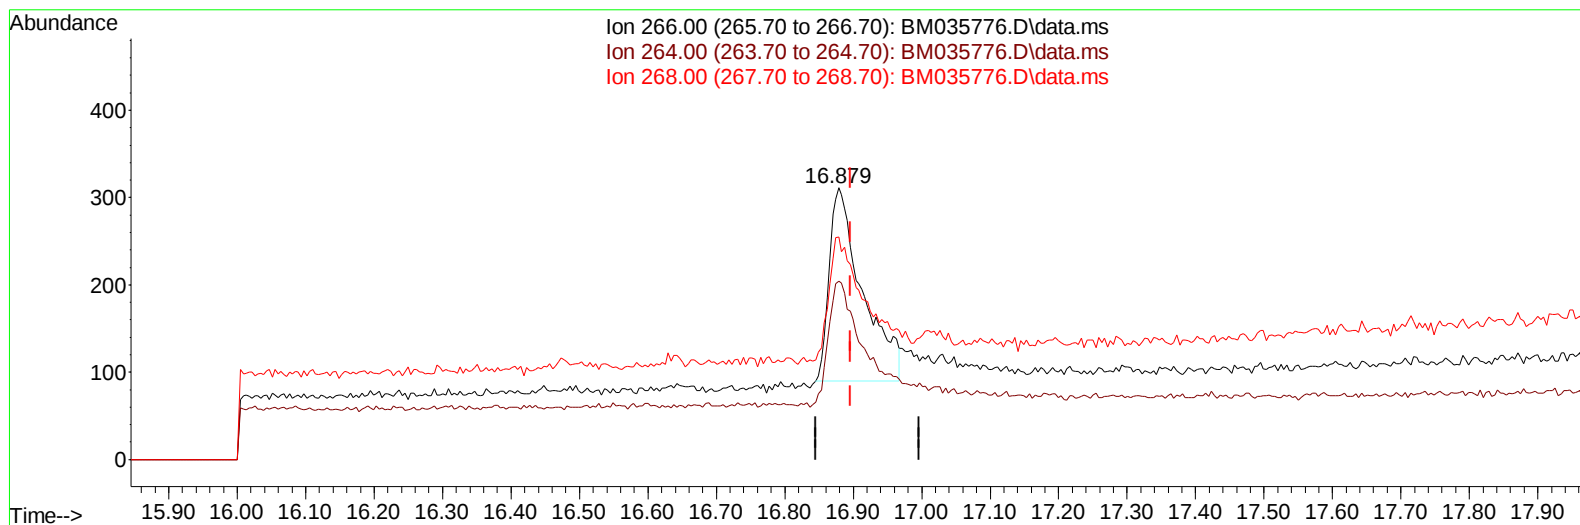

TIC: BM035776.D\data.ms

(14) Pentachloropheno1

16.879min (-0.017) 0.53 ng/u1

response 747

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.90	64.93
268.00	66.90	69.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
Data File : BM035776.D
Acq On : 30 Jun 2022 11:49
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

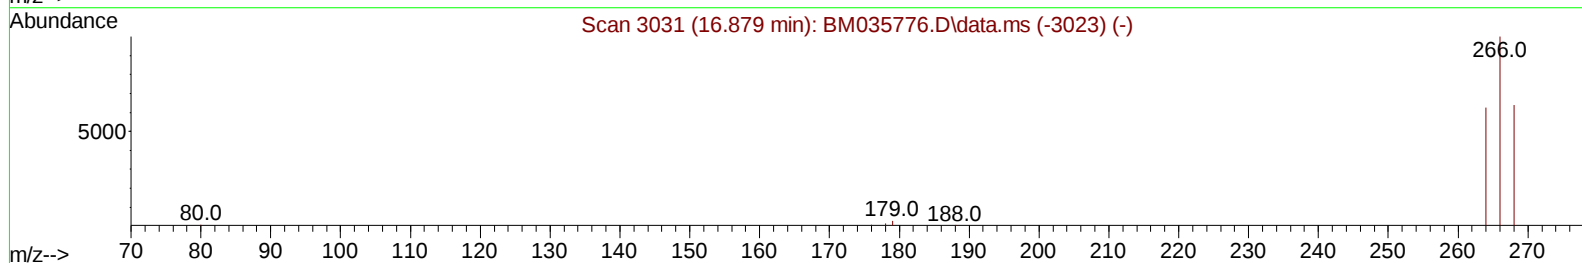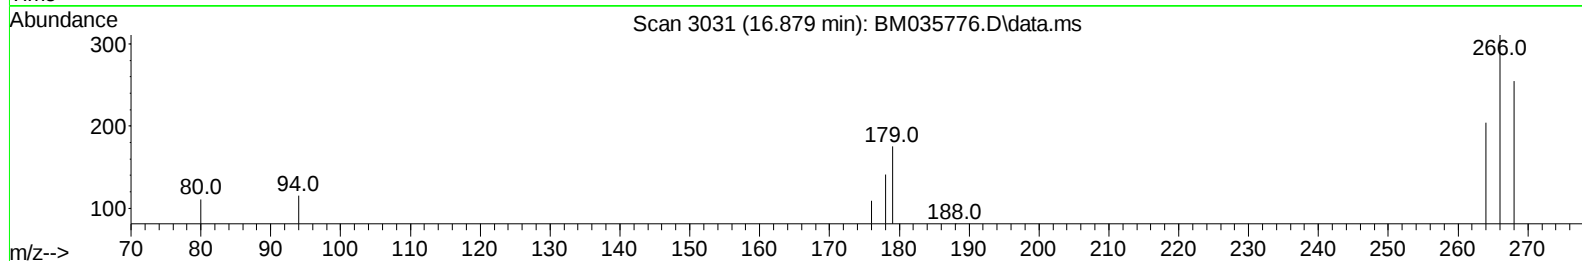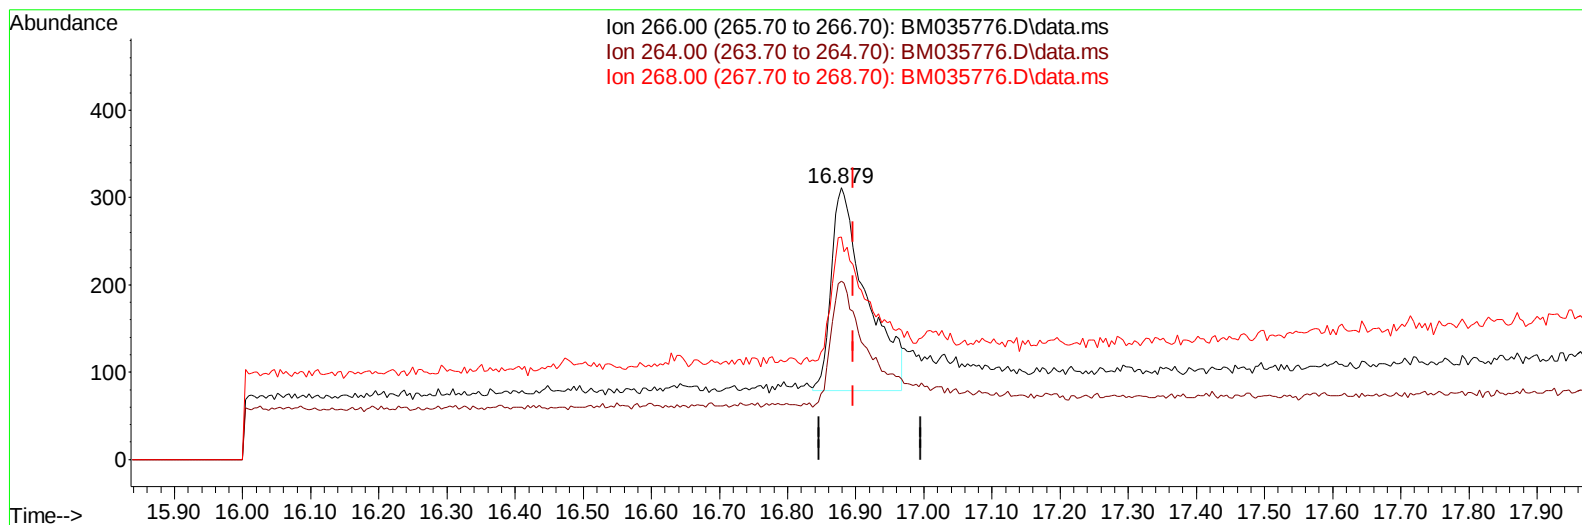

TIC: BM035776.D\data.ms

(14) Pentachloropheno1

16.879min (-0.017) 0.59 ng/u1 m

response 832

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.90	58.29
268.00	66.90	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035776.D
 Acq On : 30 Jun 2022 11:49
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
 Supervised By :mohammad ahmed 07/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	2347	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.589	136	8606	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.422	164	4514m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.187	188	8969	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.365	240	10757	0.400	ng/ul	# 0.00
23) Perylene-d12	23.686	264	11490	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	1499	0.471	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.195	152	4878	0.362	ng/ul	-0.03
18) Fluoranthene-d10	19.205	212	11657	0.322	ng/ul	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.247	88	1459m	0.463	ng/ul	
5) Naphthalene	10.644	128	9064	0.345	ng/ul	98
7) 2-Methylnaphthalene	12.266	142	5100	0.309	ng/ul	99
8) 1-Methylnaphthalene	12.470	142	5409	0.347	ng/ul	99
10) Acenaphthylene	14.150	152	8803	0.372	ng/ul	98
11) Acenaphthene	14.483	153	6299	0.346	ng/ul	99
12) Fluorene	15.491	166	7165	0.341	ng/ul	97
14) Pentachlorophenol	16.879	266	832m	0.587	ng/ul	
15) Phenanthrene	17.225	178	10923	0.336	ng/ul	95
16) Anthracene	17.326	178	10379	0.384	ng/ul	95
19) Fluoranthene	19.238	202	14608	0.271	ng/ul	97
20) Pyrene	19.600	202	16403	0.272	ng/ul	98
21) Benzo(a)anthracene	21.353	228	12802	0.344	ng/ul#	93
22) Chrysene	21.403	228	14791	0.309	ng/ul#	94
24) Benzo(b)fluoranthene	22.984	252	15552	0.316	ng/ul	77
25) Benzo(k)fluoranthene	23.028	252	15997	0.318	ng/ul#	78
26) Benzo(a)pyrene	23.586	252	17113	0.340	ng/ul#	79
27) Indeno(1,2,3-cd)pyrene	26.094	276	20558	0.375	ng/ul#	100
28) Dibenzo(a,h)anthracene	26.101	278	16597	0.382	ng/ul#	74
29) Benzo(g,h,i)perylene	26.829	276	18603	0.368	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
Data File : BM035776.D
Acq On : 30 Jun 2022 11:49
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/01/2022
Supervised By :mohammad ahmed 07/01/2022

