

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 152.00 (151.70 to 152.70): BM035780.D\data.ms
 Ion 150.00 (149.70 to 150.70): BM035780.D\data.ms
 Ion 115.00 (114.70 to 115.70): BM035780.D\data.ms

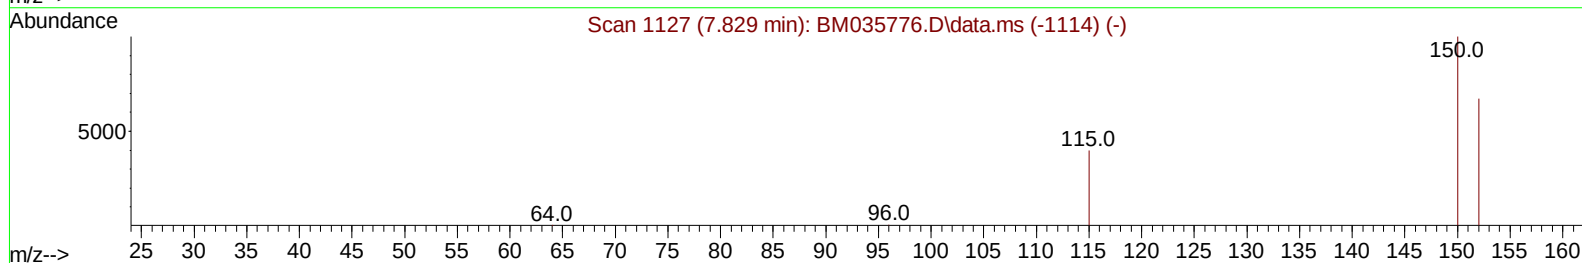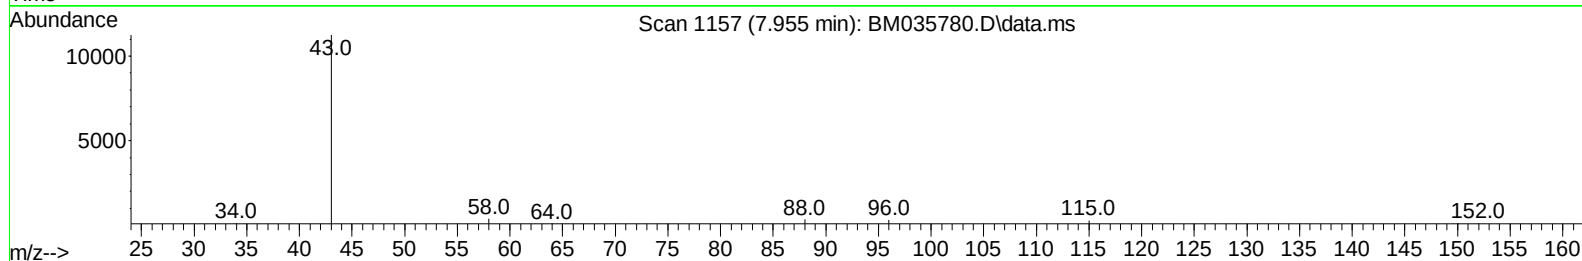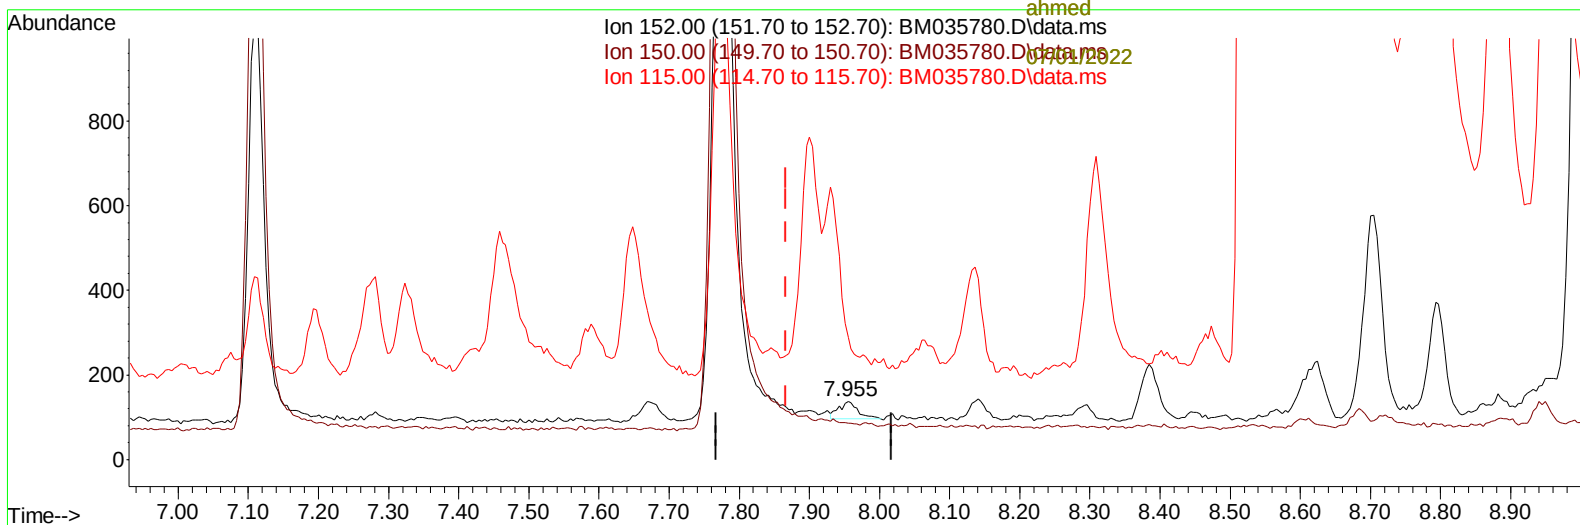

TIC: BM035780.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.955min (+ 0.088) 0.40 ng/ul

response 75

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	147.40	62.32#
115.00	74.40	208.70#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 152.00 (151.70 to 152.70): BM035780.D\data.ms
 Ion 150.00 (149.70 to 150.70): BM035780.D\data.ms
 Ion 115.00 (114.70 to 115.70): BM035780.D\data.ms

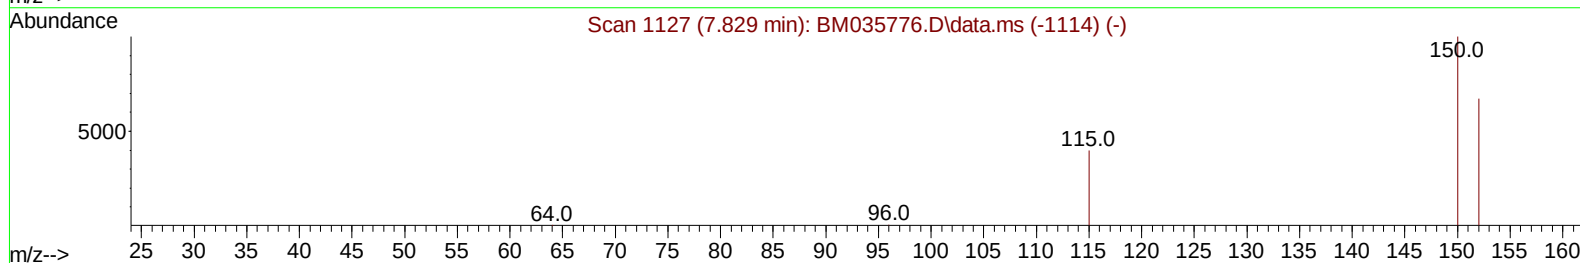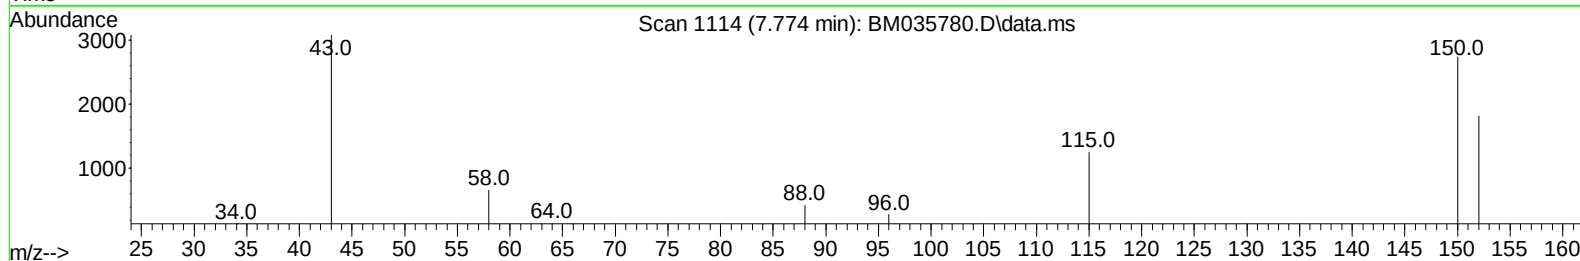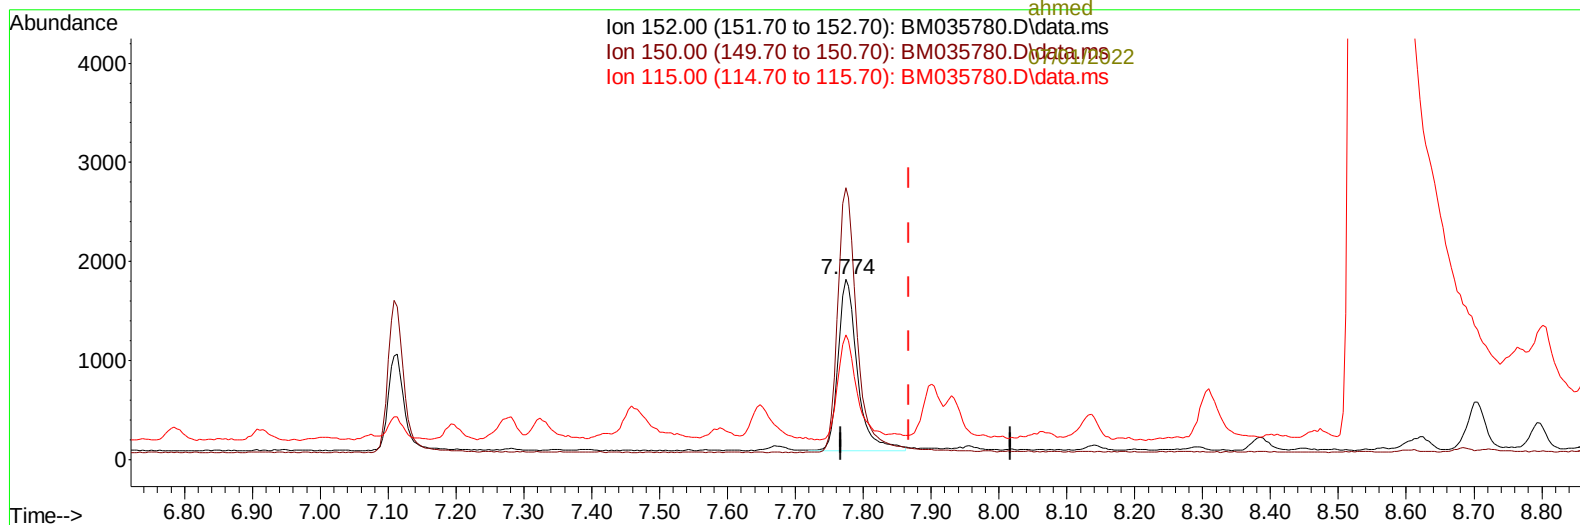

TIC: BM035780.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.774min (-0.093) 0.40 ng/ul m

response 3422

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	147.40	150.52
115.00	74.40	68.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 88.00 (87.70 to 88.70): BM035780.D\data.ms
 Ion 43.00 (42.70 to 43.70): BM035780.D\data.ms
 Ion 58.00 (57.70 to 58.70): BM035780.D\data.ms

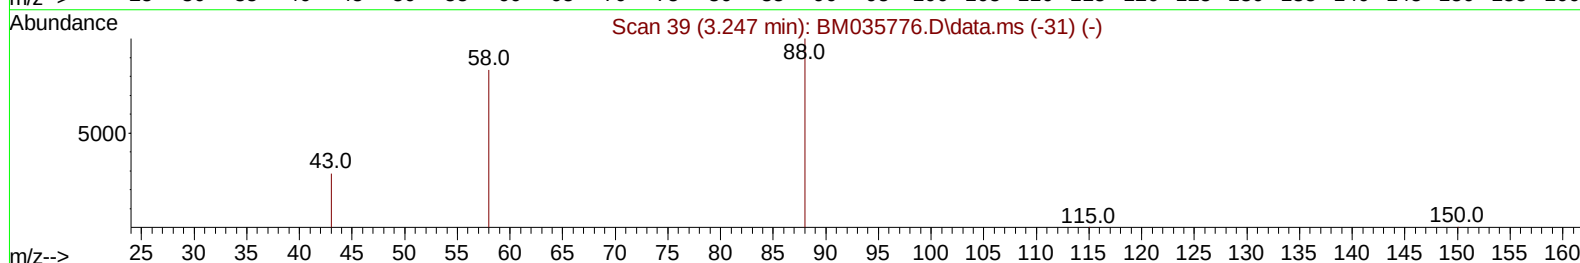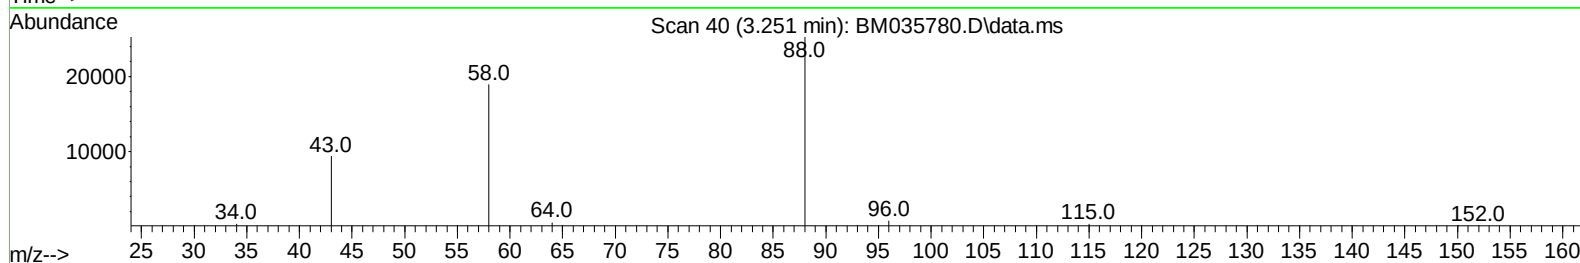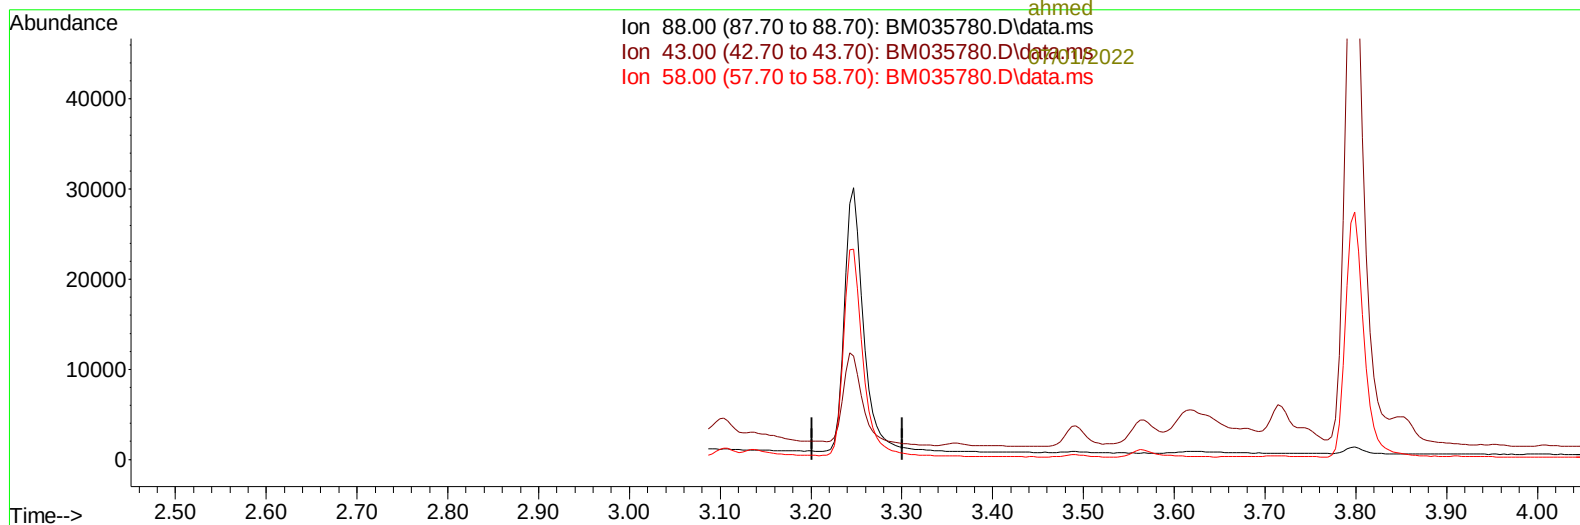

TIC: BM035780.D\data.ms

(2) 1,4-Dioxane

3.251min (-3.251) 0.00 ng/ul

response 0

Ion	Exp%	Act%
88.00	100.00	0.00
43.00	47.20	0.00#
58.00	53.20	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 88.00 (87.70 to 88.70): BM035780.D\data.ms
 Ion 43.00 (42.70 to 43.70): BM035780.D\data.ms
 Ion 58.00 (57.70 to 58.70): BM035780.D\data.ms

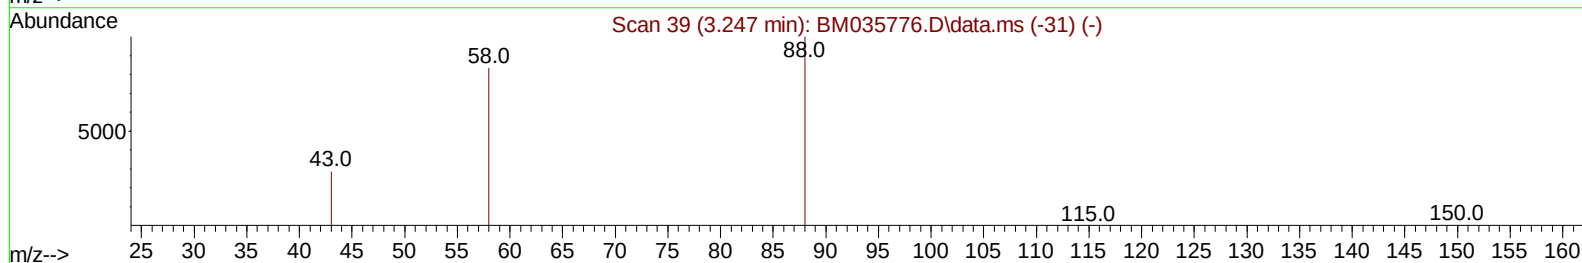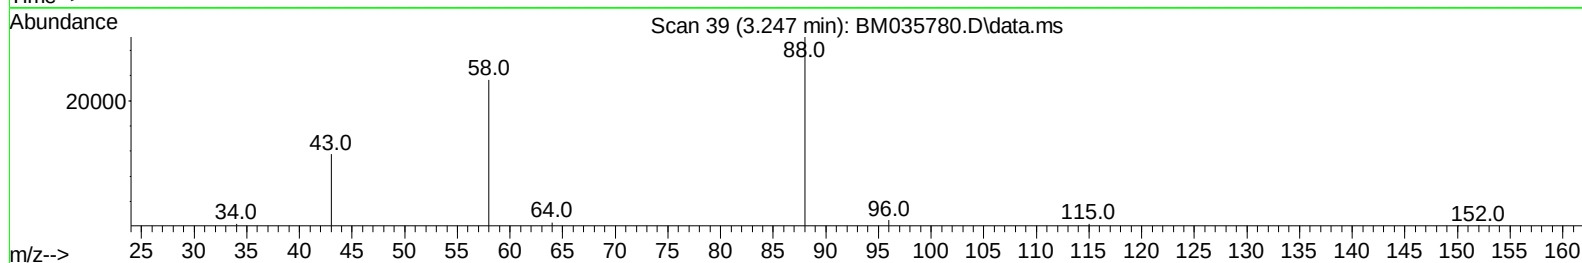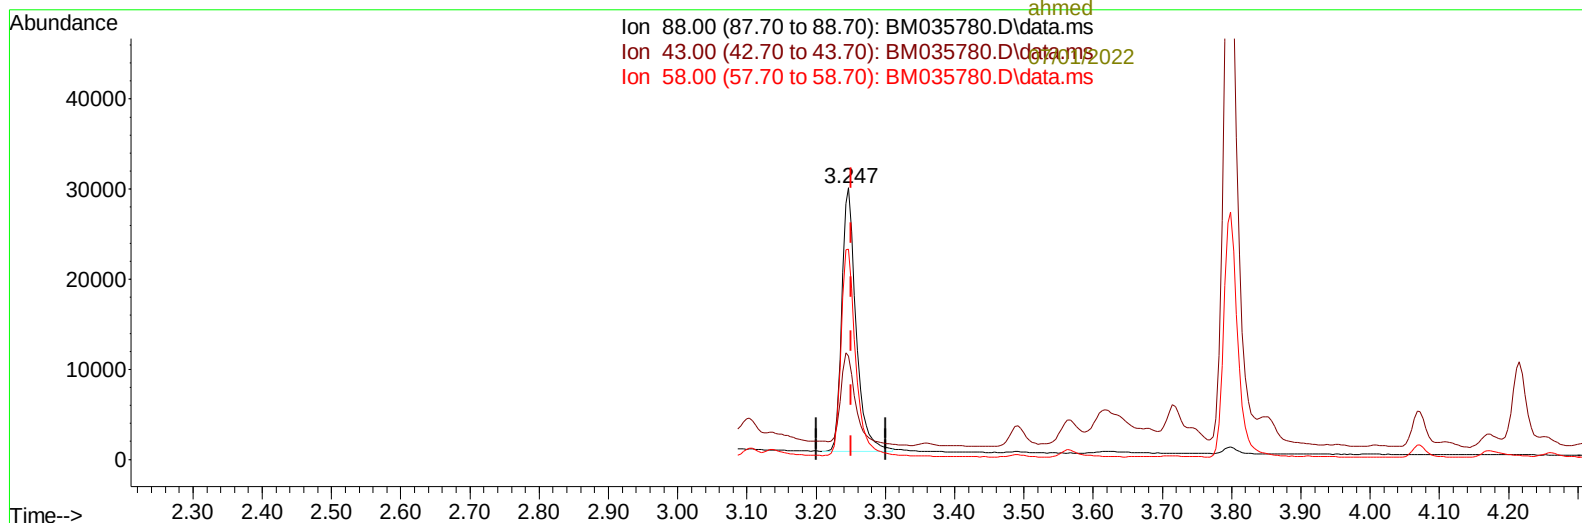

TIC: BM035780.D\data.ms

(2) 1,4-Dioxane

3.247min (-0.004) 9.19 ng/ul m

response 42202

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	47.20	38.09
58.00	53.20	77.46#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

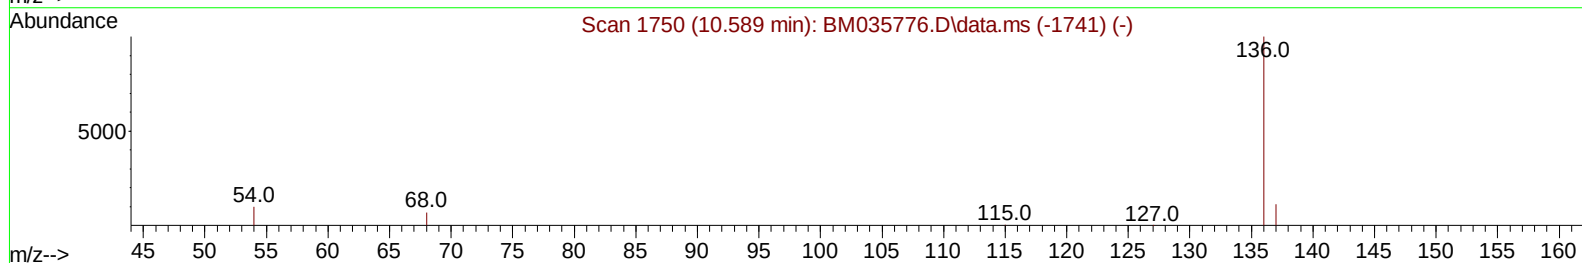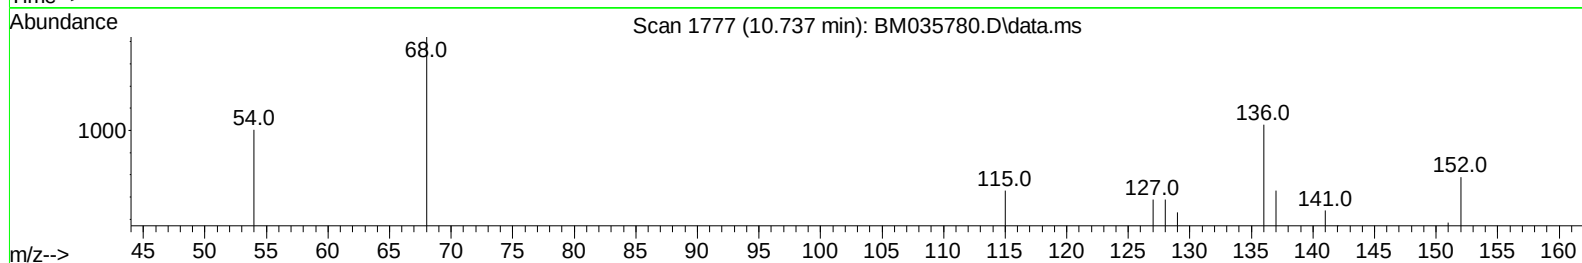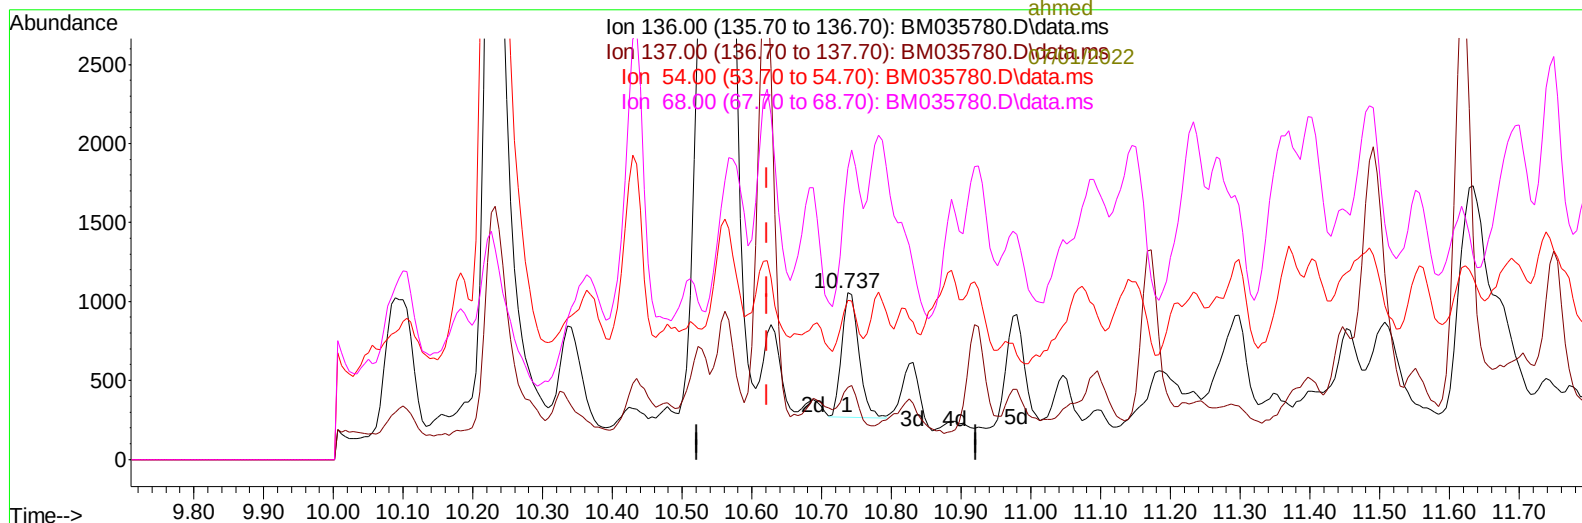

TIC: BM035780.D\data.ms

(4) Naphthalene-d8 (I)

10.737min (+ 0.116) 0.40 ng/ul

response 1343

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	43.41#
54.00	12.20	95.45#
68.00	8.00	174.69#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

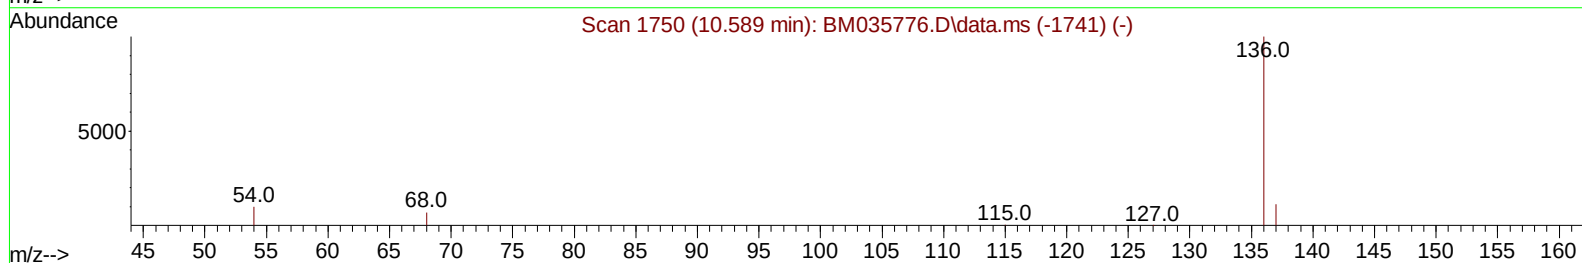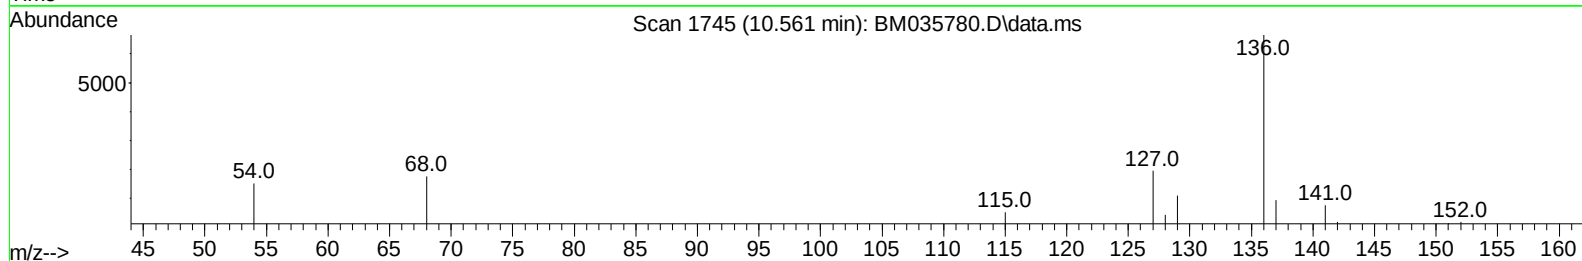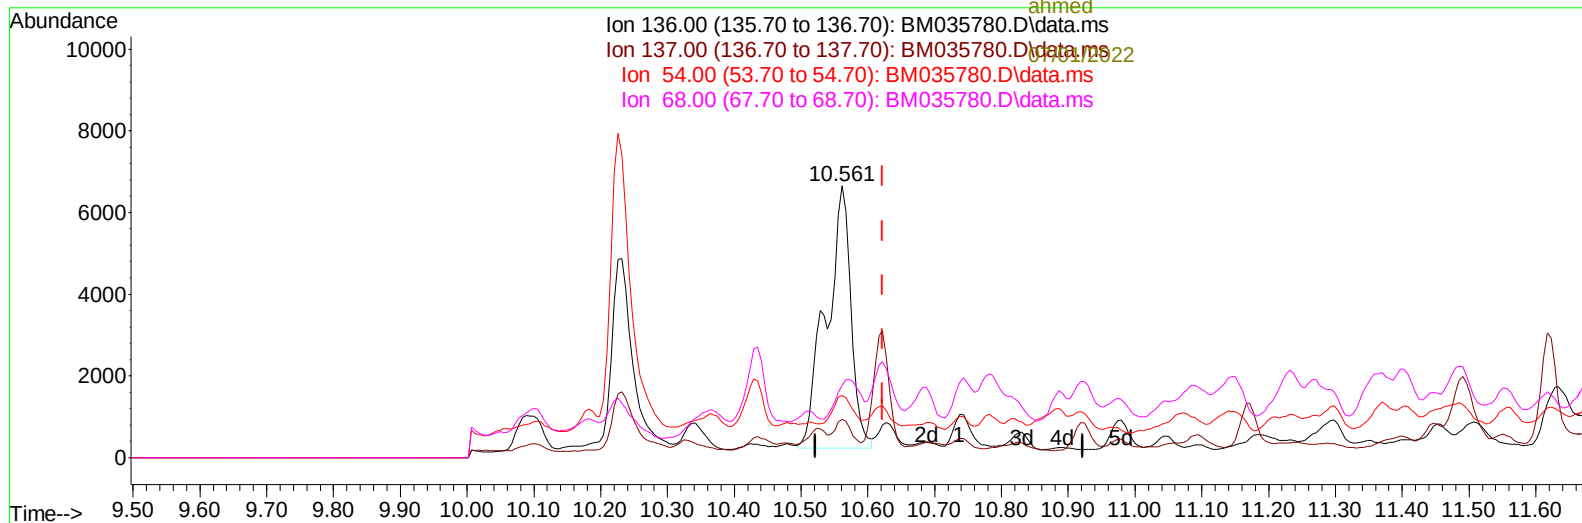

TIC: BM035780.D\data.ms

(4) Naphthalene-d8 (I)

10.561min (-0.060) 0.40 ng/ul m

response 16487

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	12.20	14.13
54.00	12.20	22.88#
68.00	8.00	26.53#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 128.00 (127.70 to 128.70): BM035780.D\data.ms
 Ion 129.00 (128.70 to 129.70): BM035780.D\data.ms
 Ion 127.00 (126.70 to 127.70): BM035780.D\data.ms

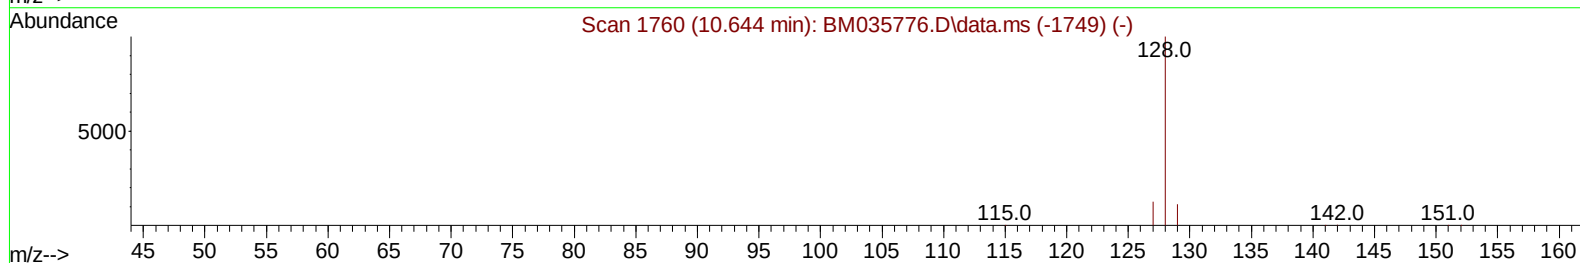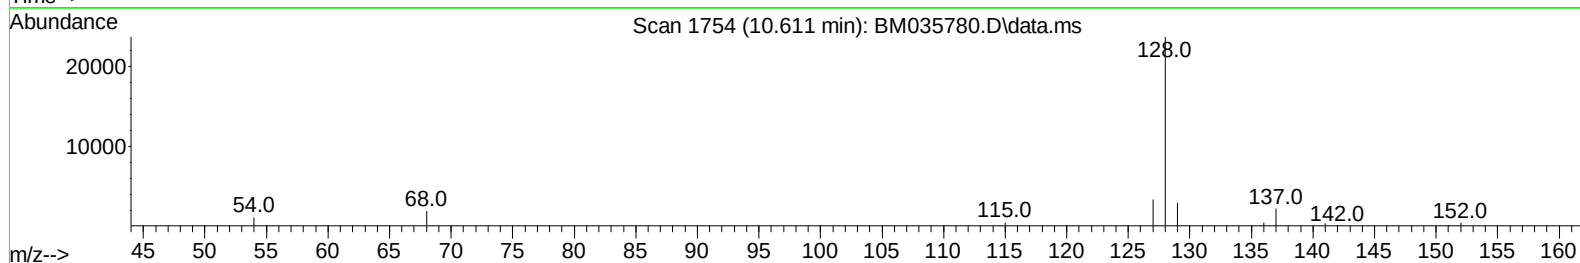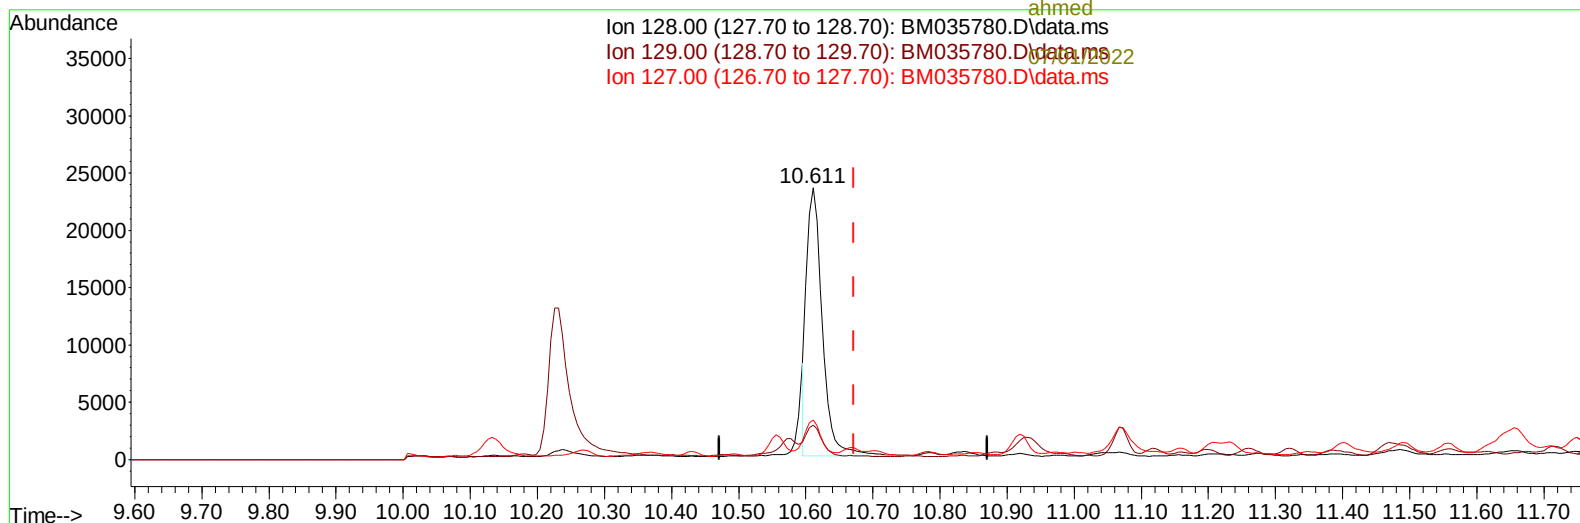

TIC: BM035780.D\data.ms

(5) Naphthalene

10.611min (-0.060) 0.76 ng/u1

response 38308

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.70	12.71
127.00	14.60	14.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 128.00 (127.70 to 128.70): BM035780.D\data.ms
 Ion 129.00 (128.70 to 129.70): BM035780.D\data.ms
 Ion 127.00 (126.70 to 127.70): BM035780.D\data.ms

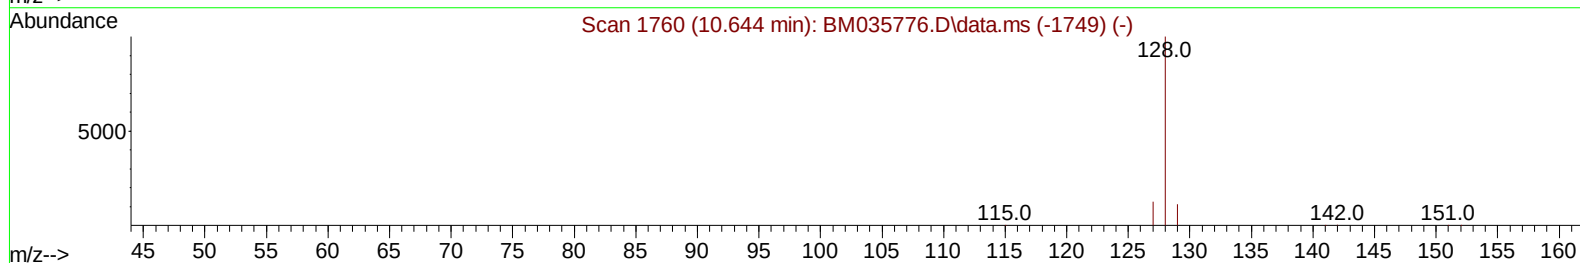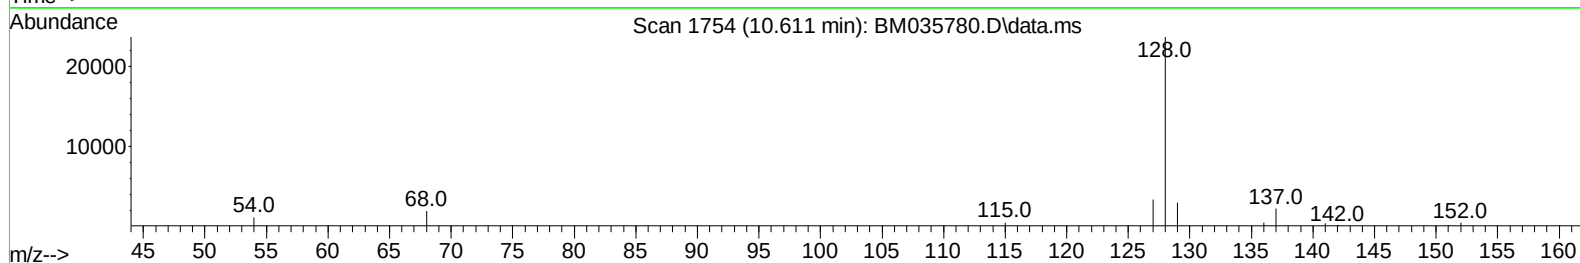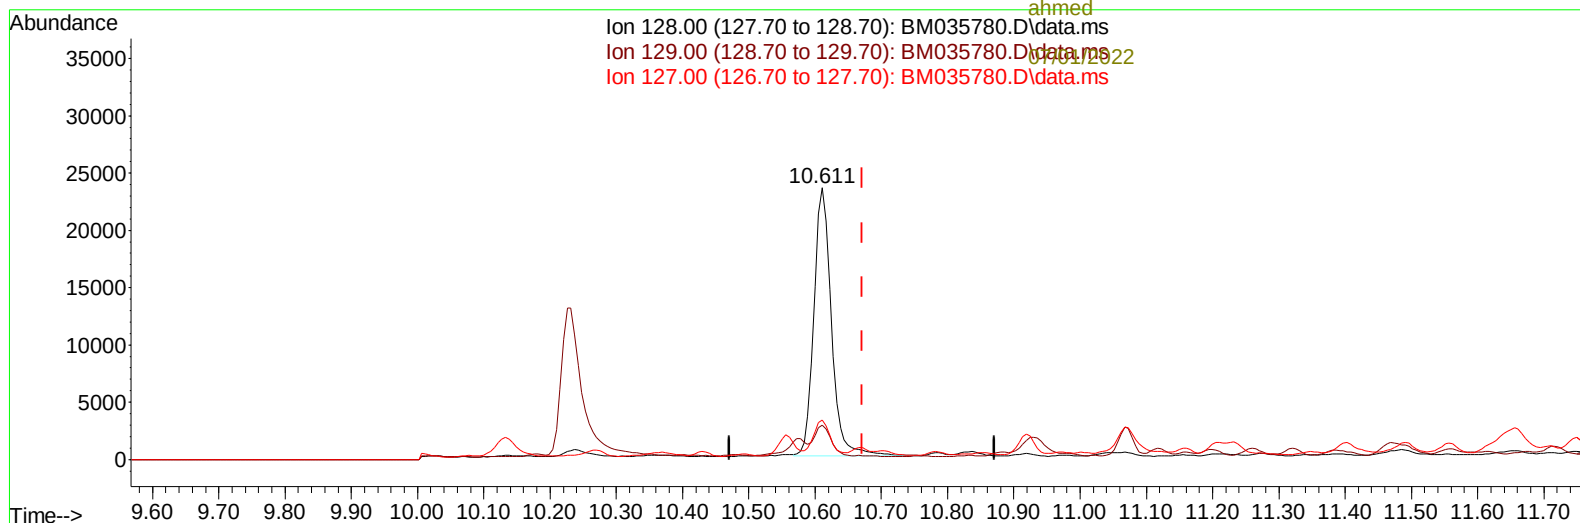

TIC: BM035780.D\data.ms

(5) Naphthalene

10.611min (-0.060) 0.85 ng/ul m

response 42909

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.70	12.71
127.00	14.60	14.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

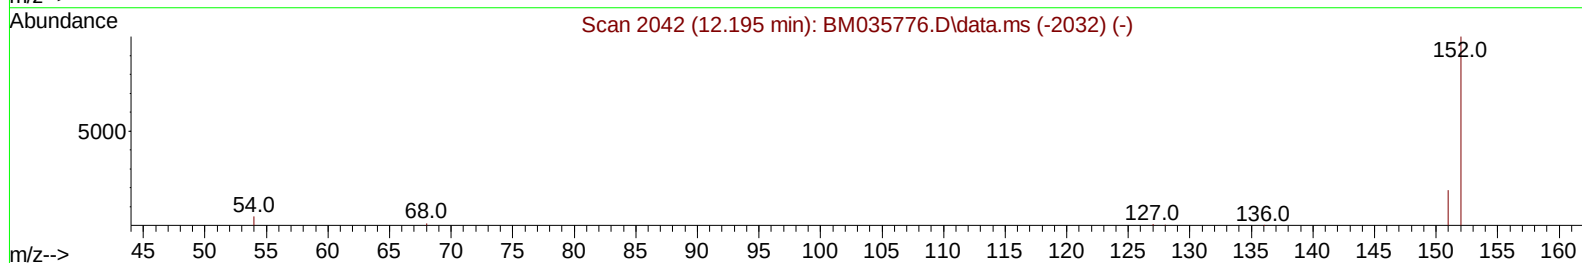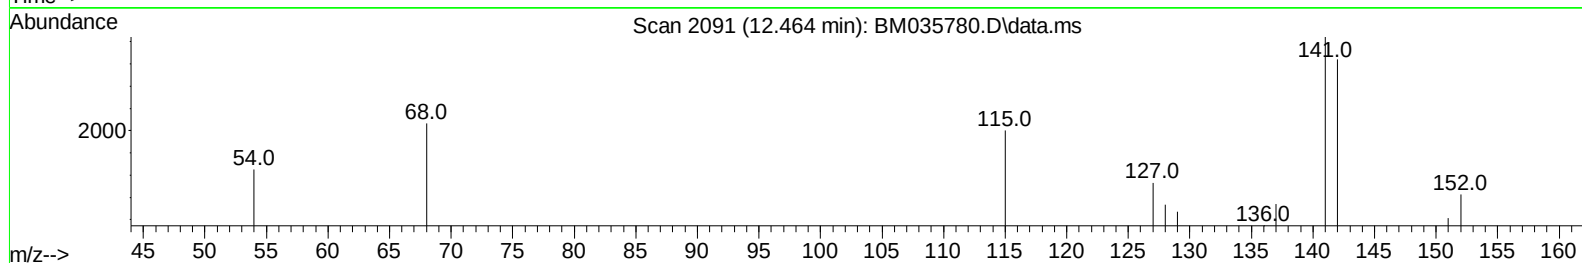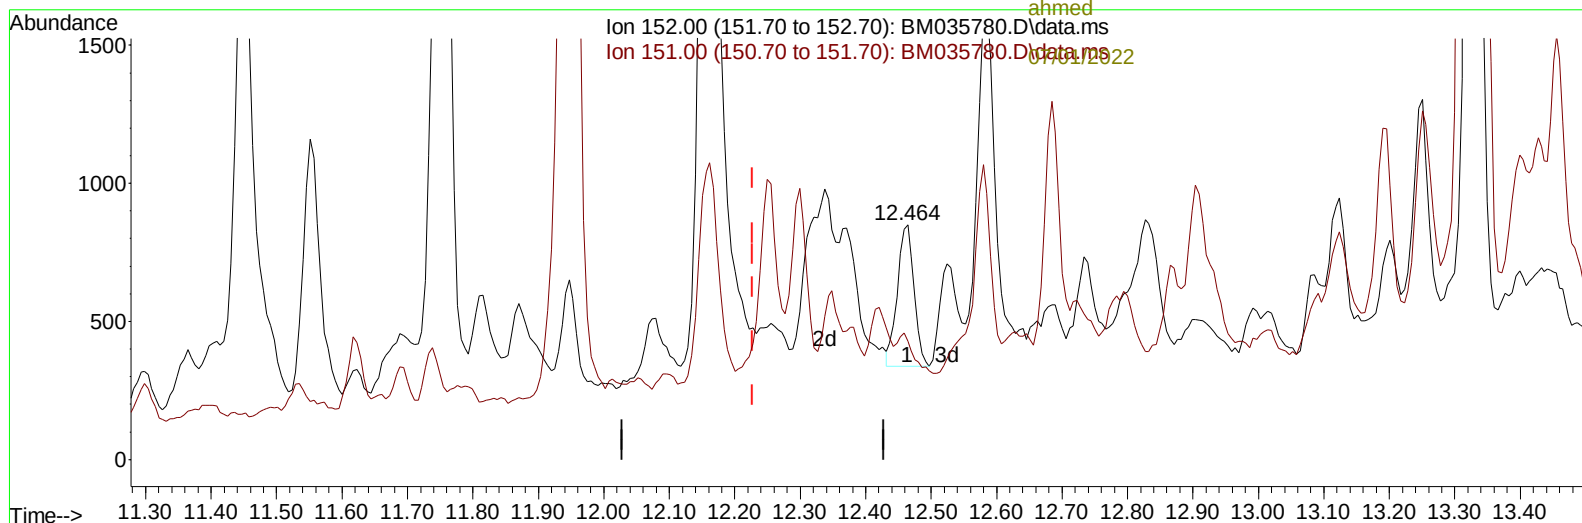

TIC: BM035780.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.464min (+ 0.237) 0.04 ng/ul

response 904

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.80	22.68
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

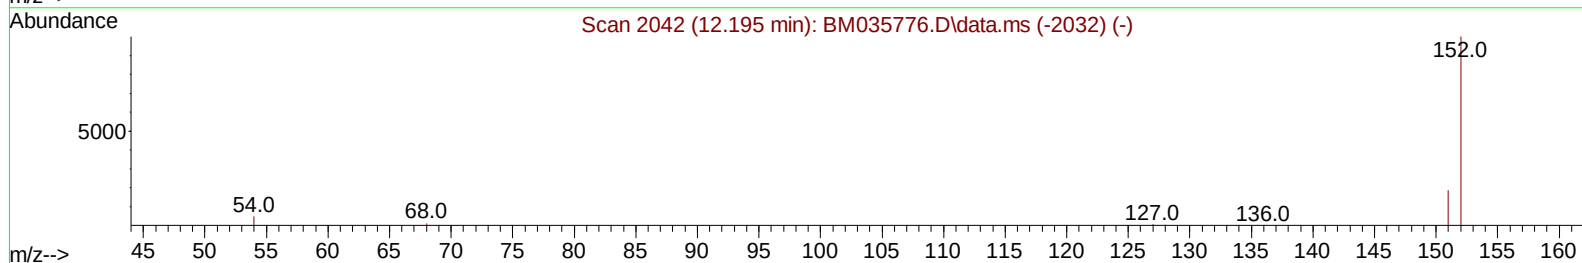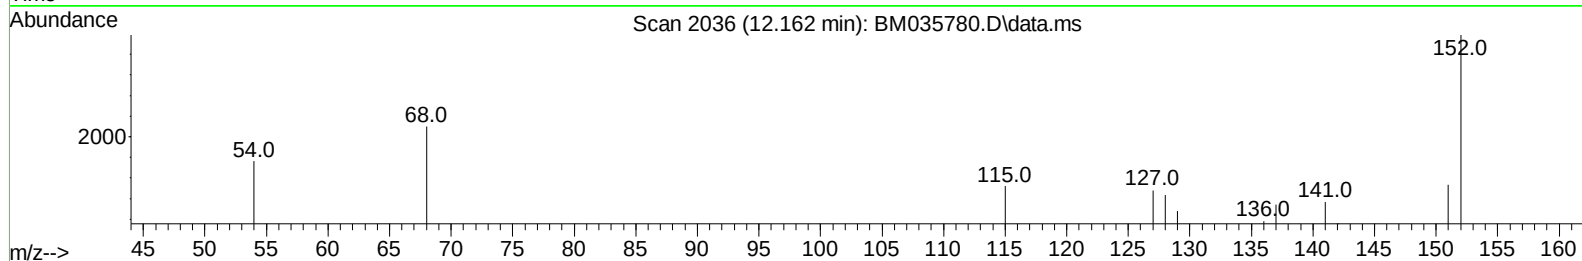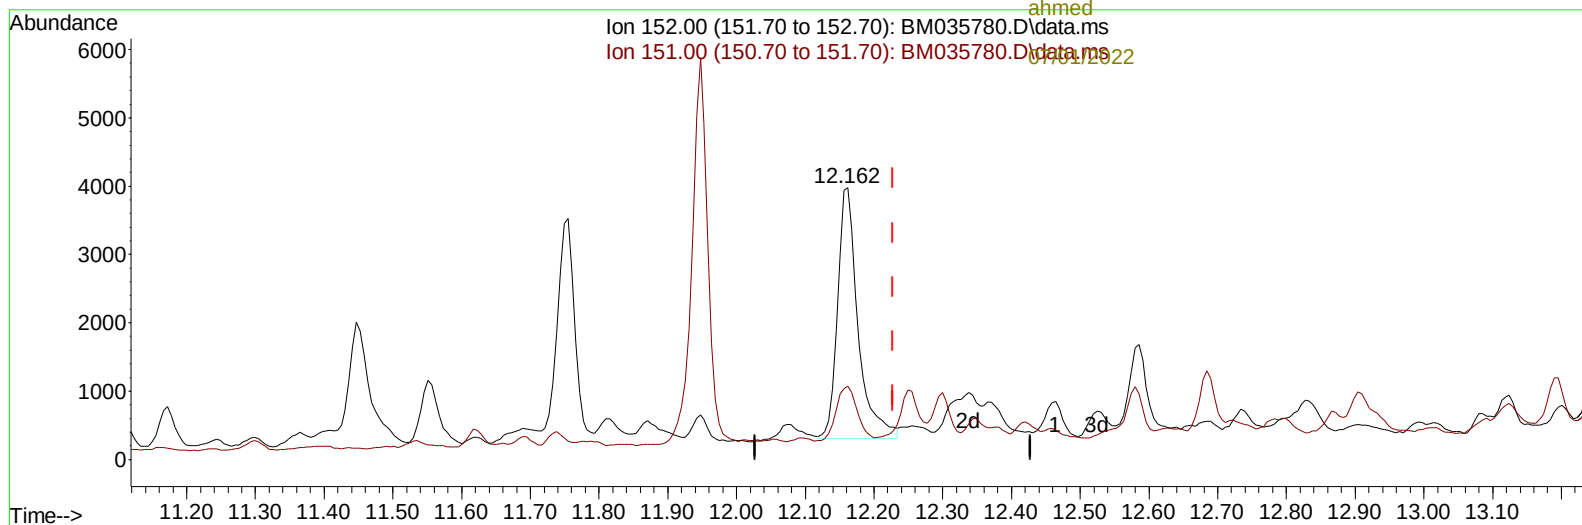

TIC: BM035780.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.162min (-0.066) 0.29 ng/ul m

response 7526

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.80	2.72#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

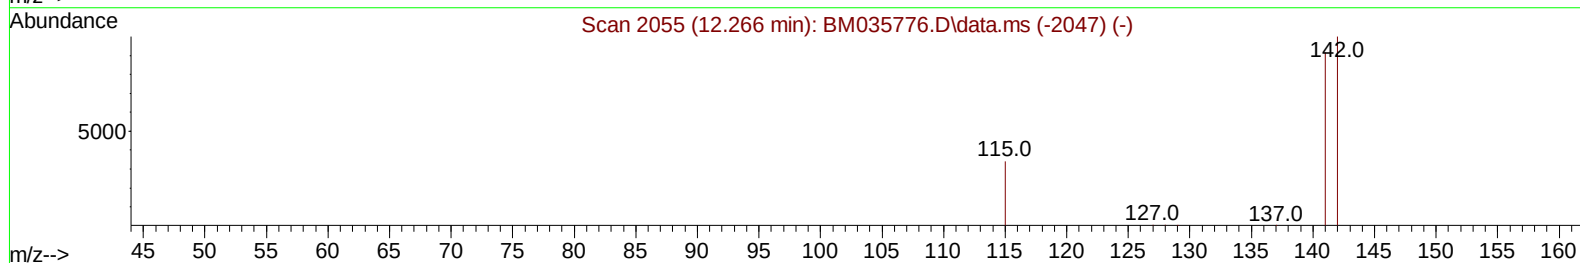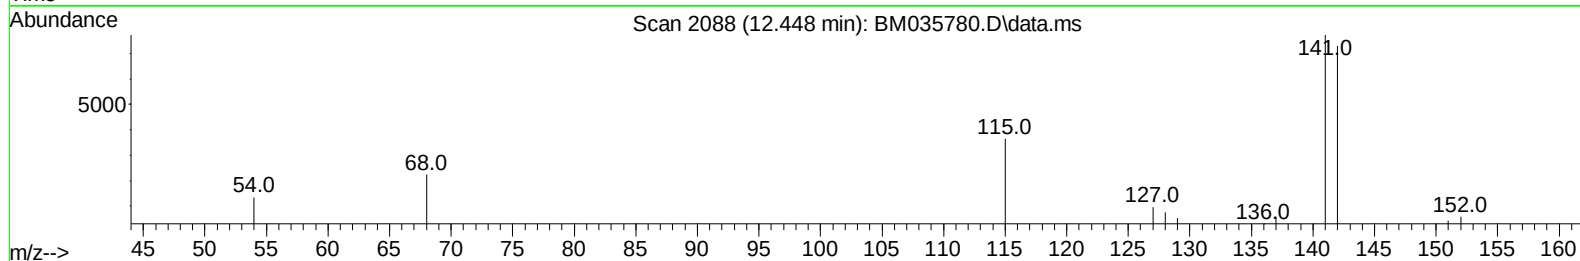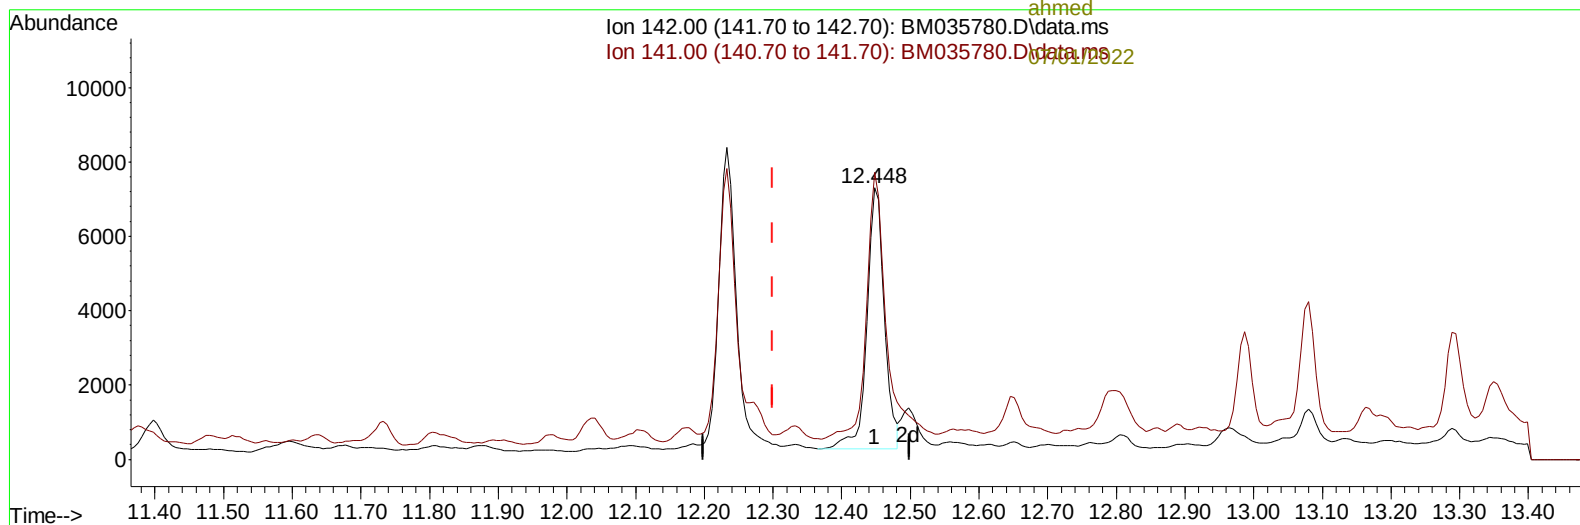

TIC: BM035780.D\data.ms

(7) 2-Methylnaphthalene

12.448min (+ 0.149) 0.39 ng/ul

response 12464

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	96.70	118.07#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

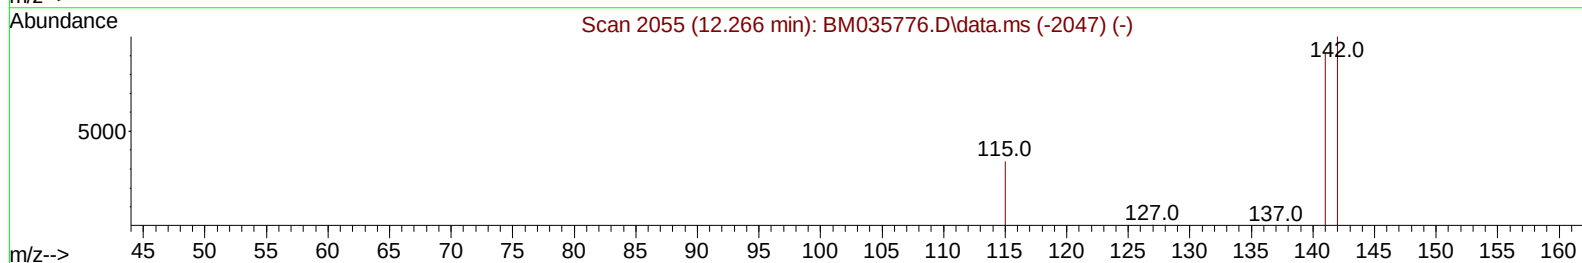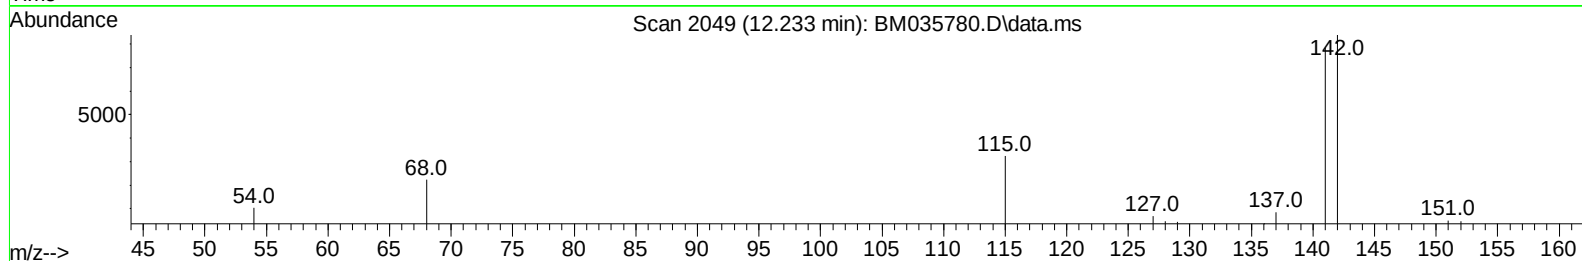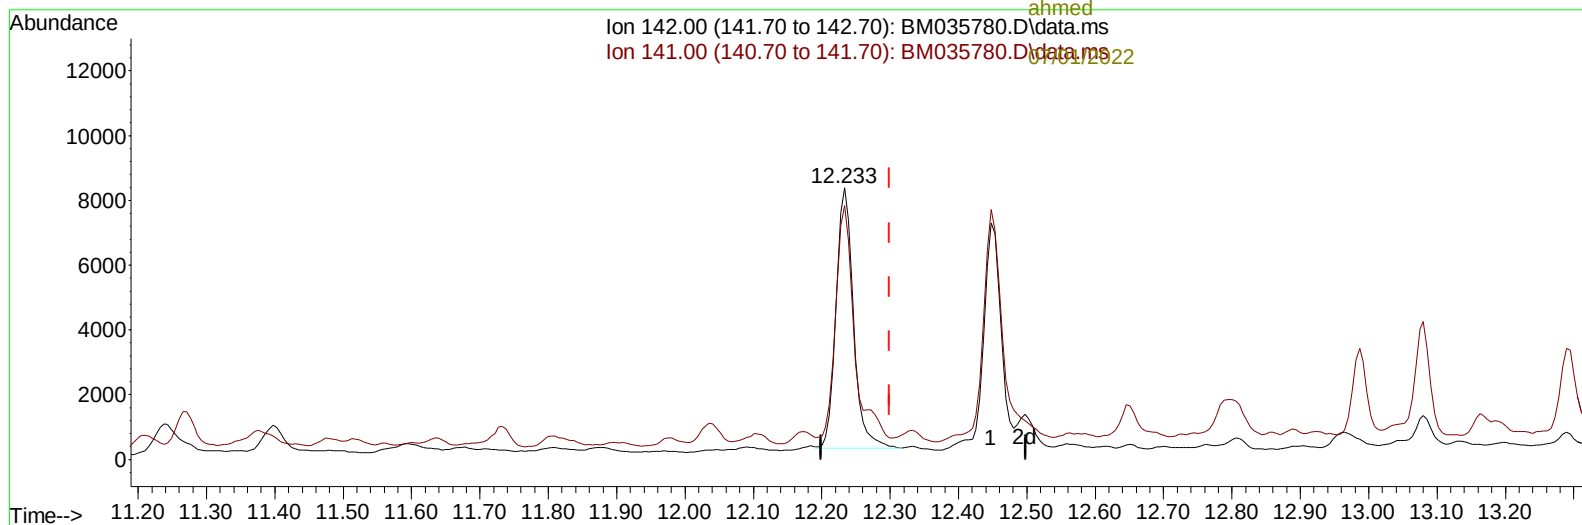

TIC: BM035780.D\data.ms

(7) 2-Methylnaphthalene

12.233min (-0.066) 0.45 ng/ul m

response 14257

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	96.70	103.22
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

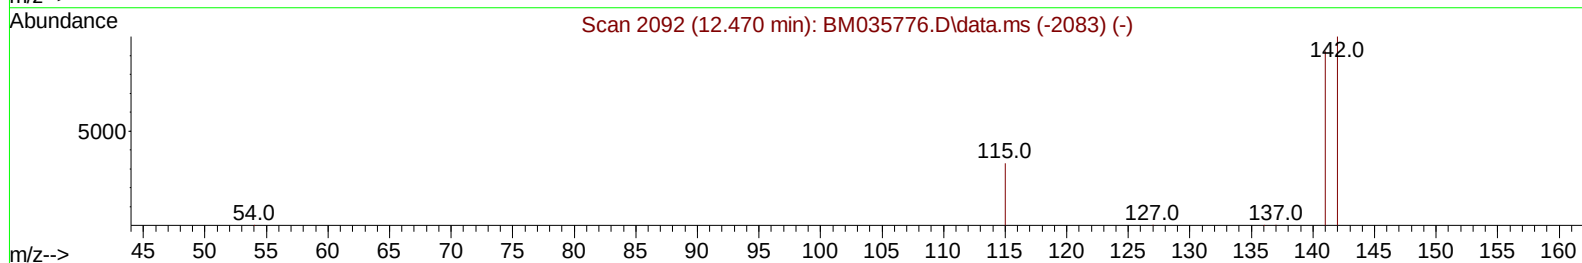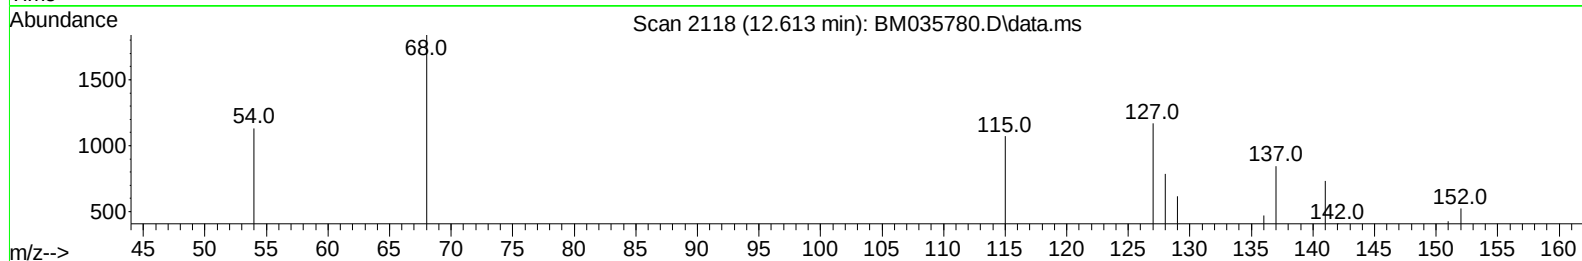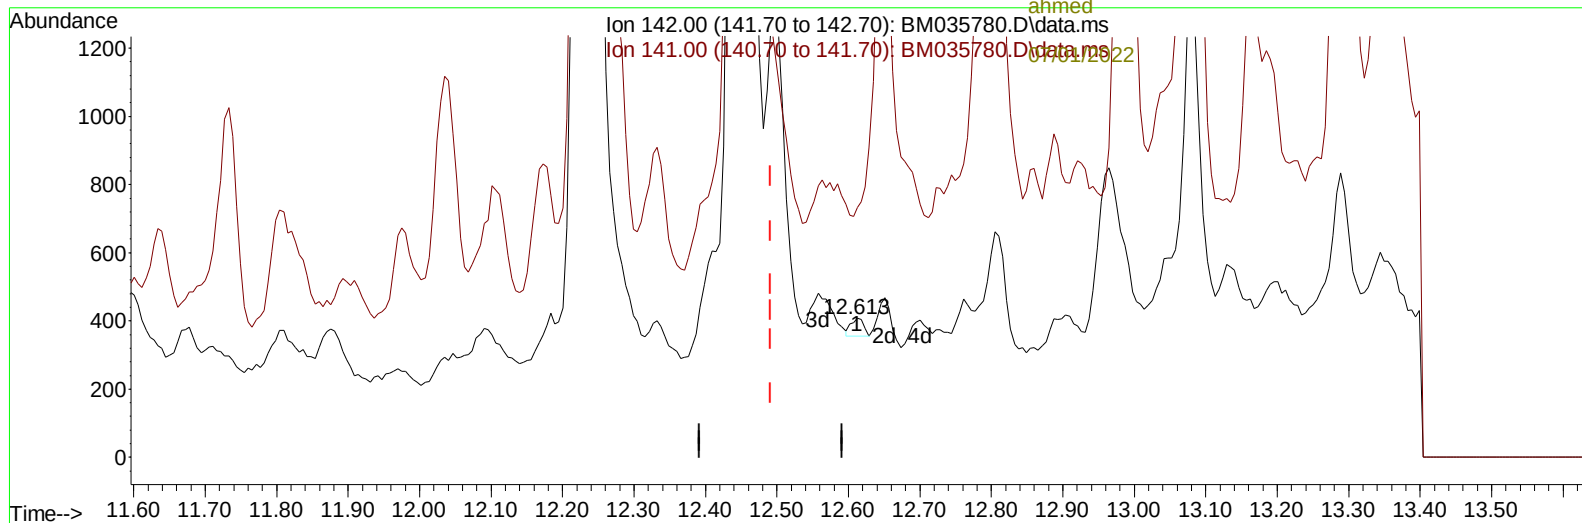

TIC: BM035780.D\data.ms

(8) 1-Methylnaphthalene

12.613min (+ 0.121) 0.00 ng/ul

response 65

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.60	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

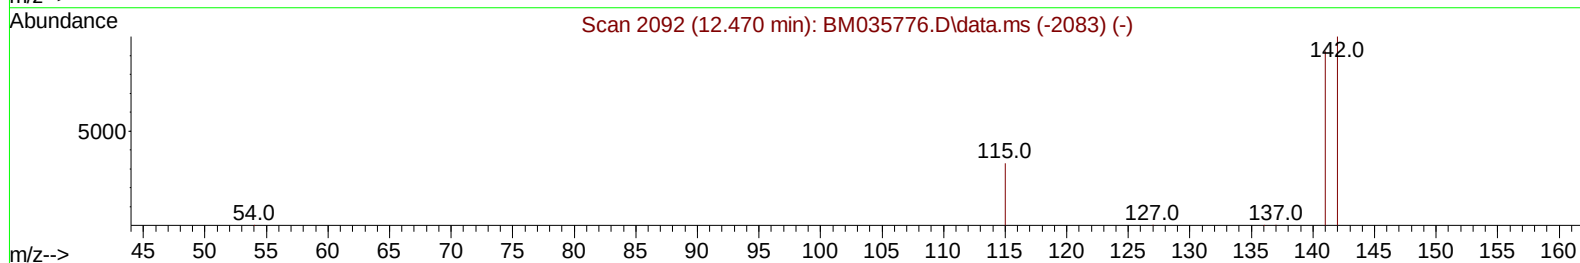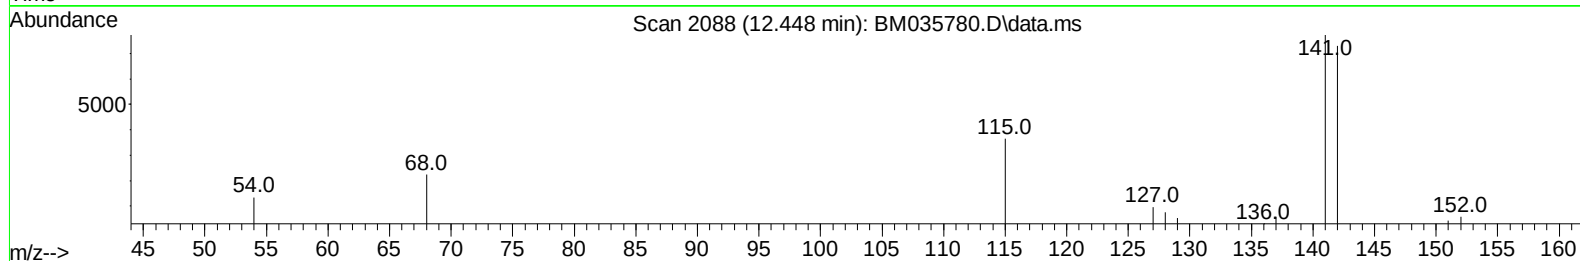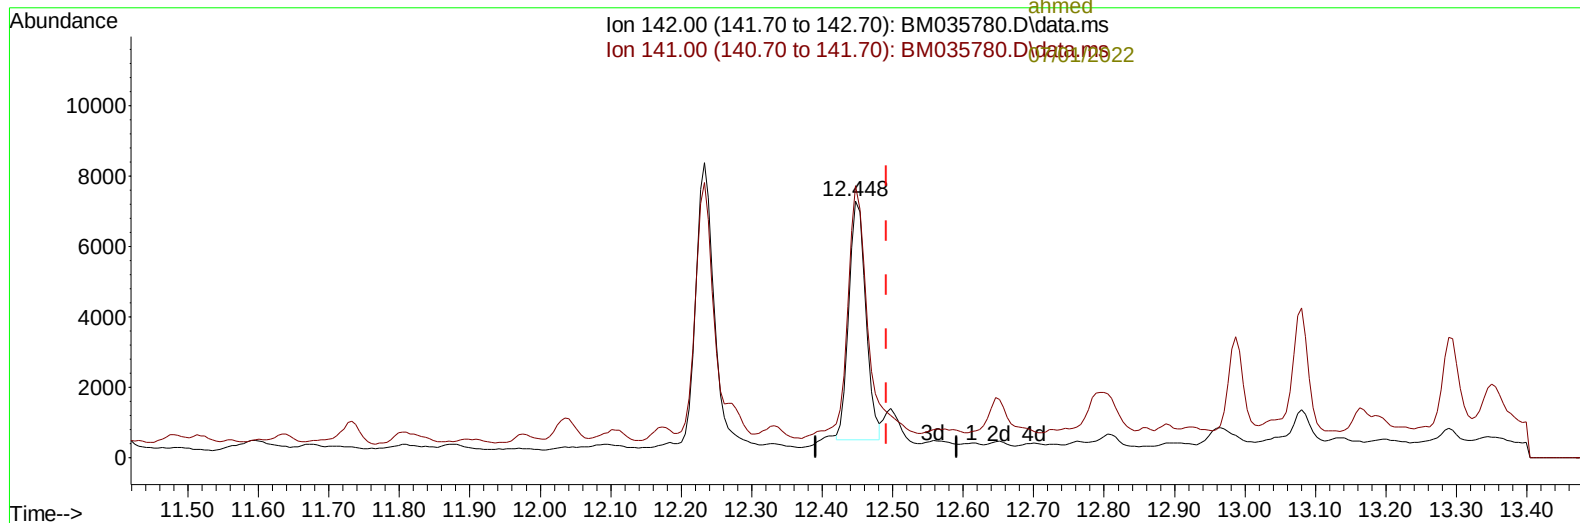

TIC: BM035780.D\data.ms

(8) 1-Methylnaphthalene

12.448min (-0.044) 0.37 ng/ul m

response 11141

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.60	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

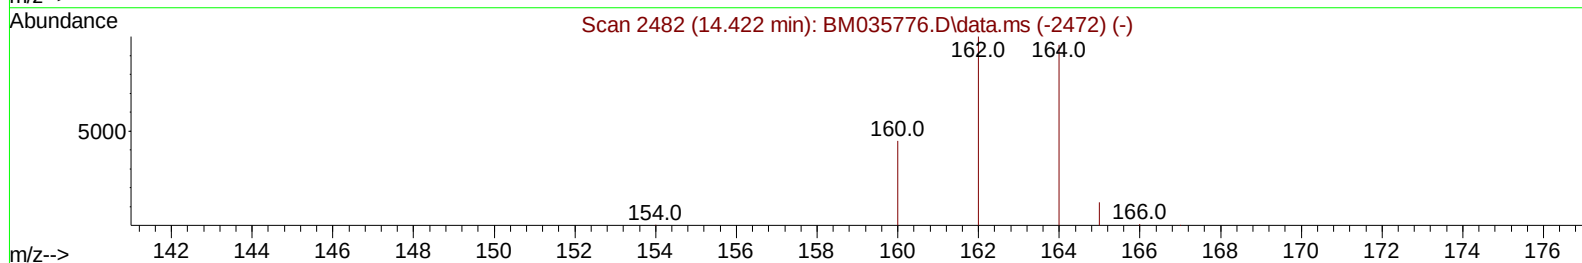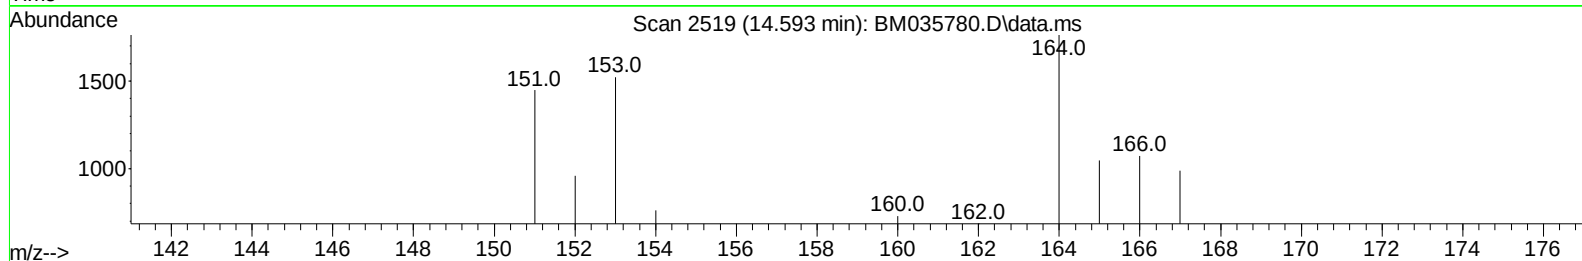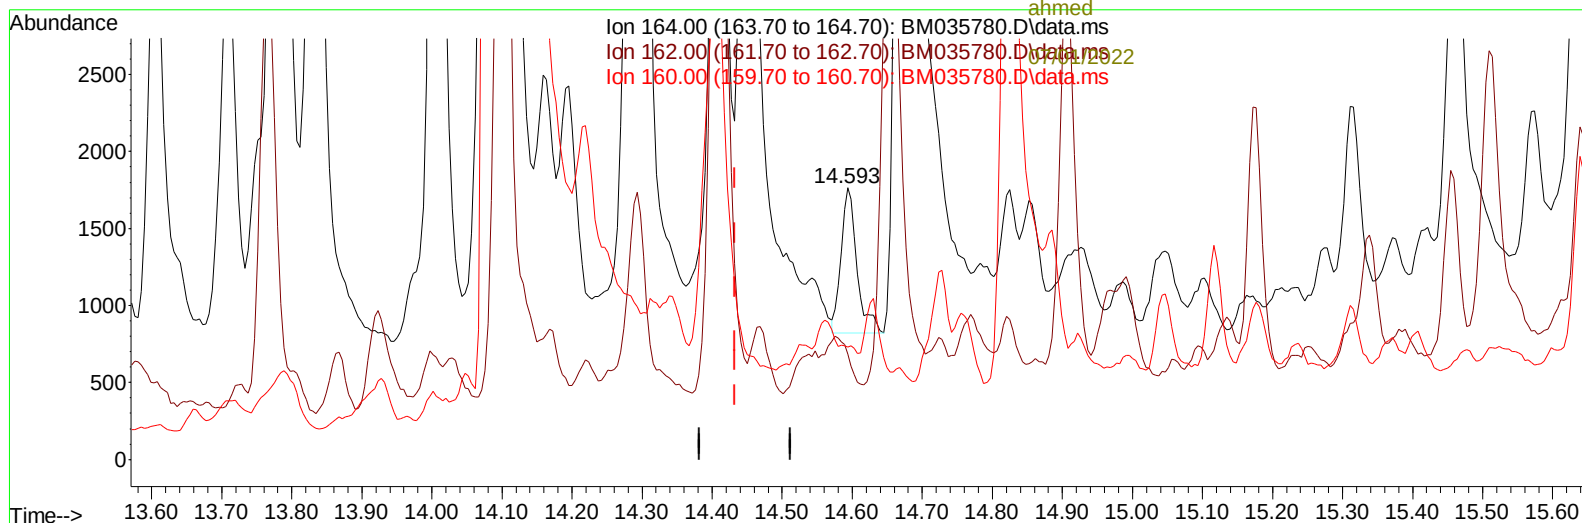

TIC: BM035780.D\data.ms

(9) Acenaphthene-d10 (I)

14.593min (+ 0.161) 0.40 ng/u1

response 1503

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.10	38.80#
160.00	48.90	41.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

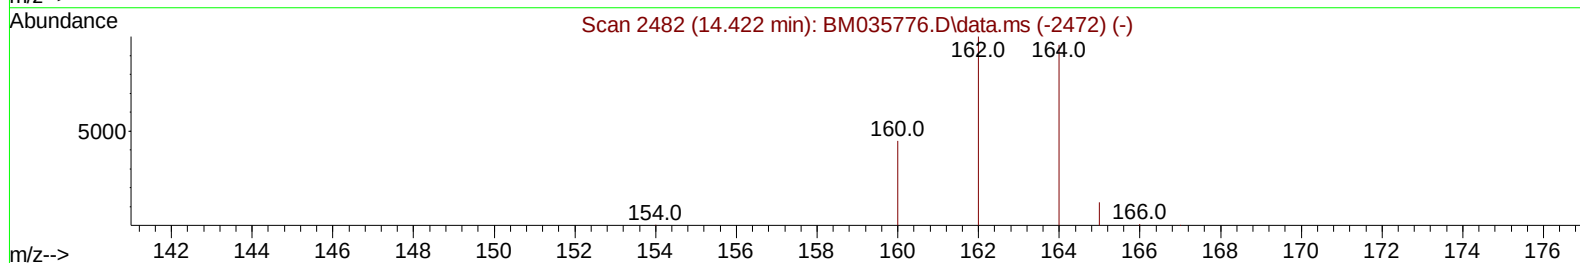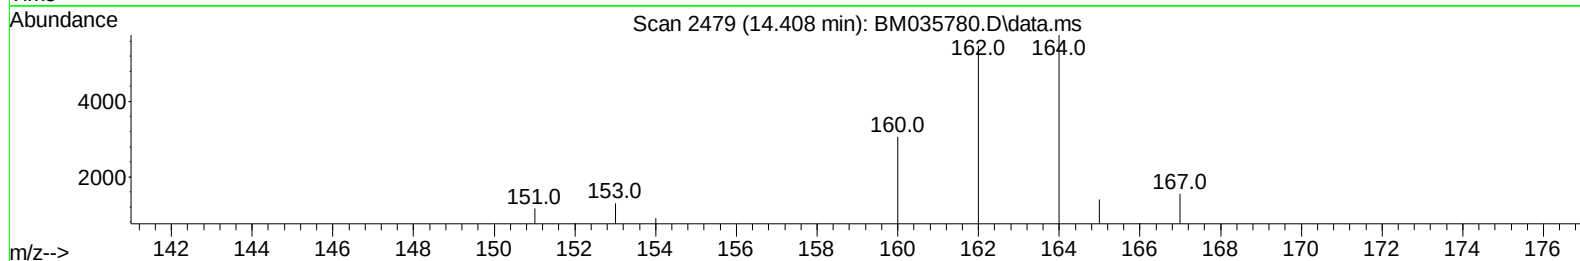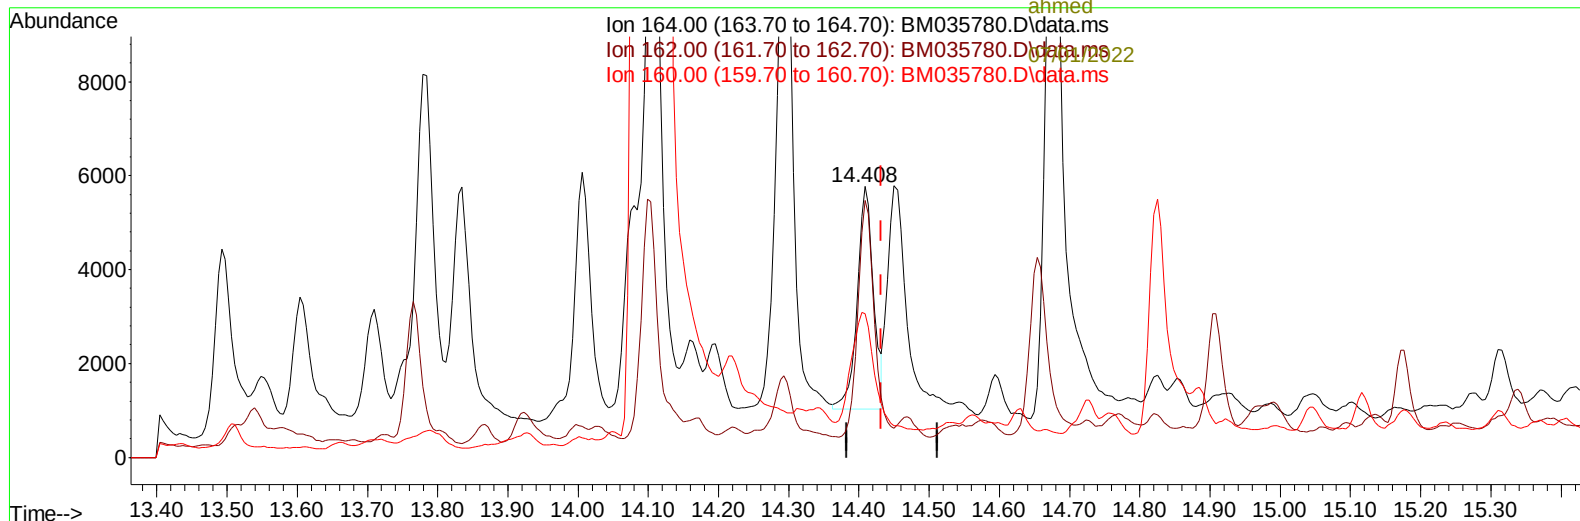

TIC: BM035780.D\data.ms

(9) Acenaphthene-d10 (I)

14.408min (-0.024) 0.40 ng/ul m

response 7623

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	104.10	94.88
160.00	48.90	53.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 153.00 (152.70 to 153.70): BM035780.D\data.ms
 Ion 152.00 (151.70 to 152.70): BM035780.D\data.ms
 Ion 154.00 (153.70 to 154.70): BM035780.D\data.ms

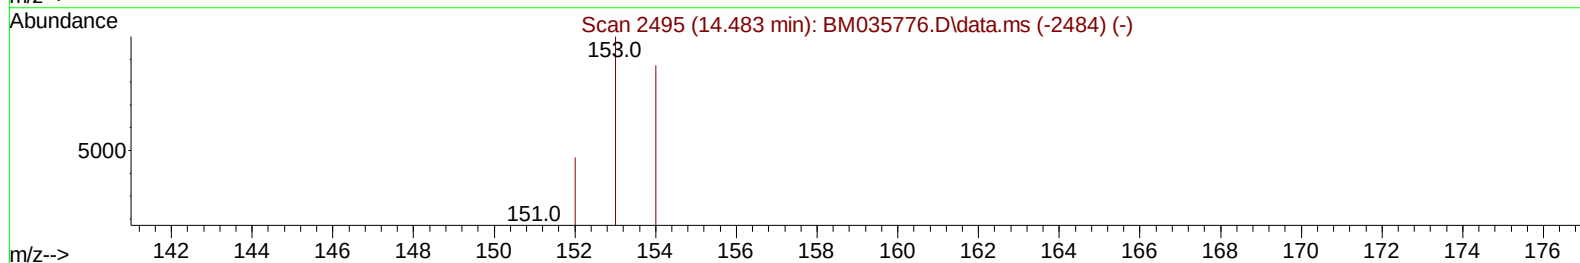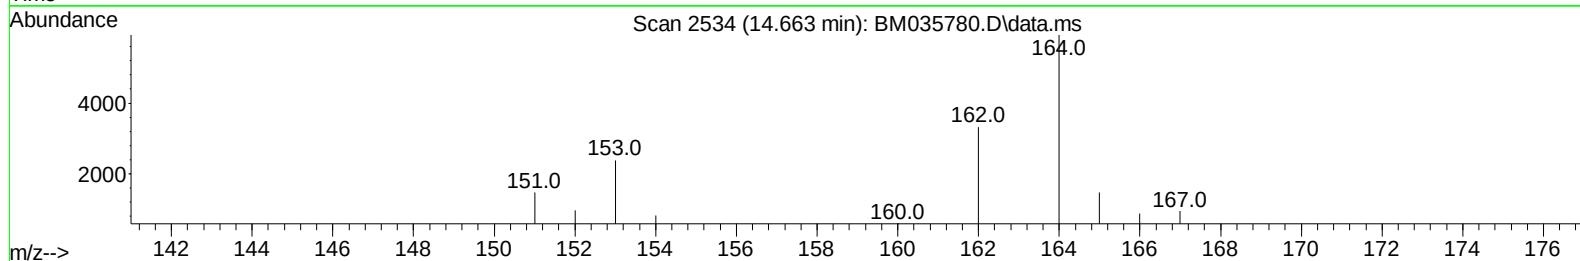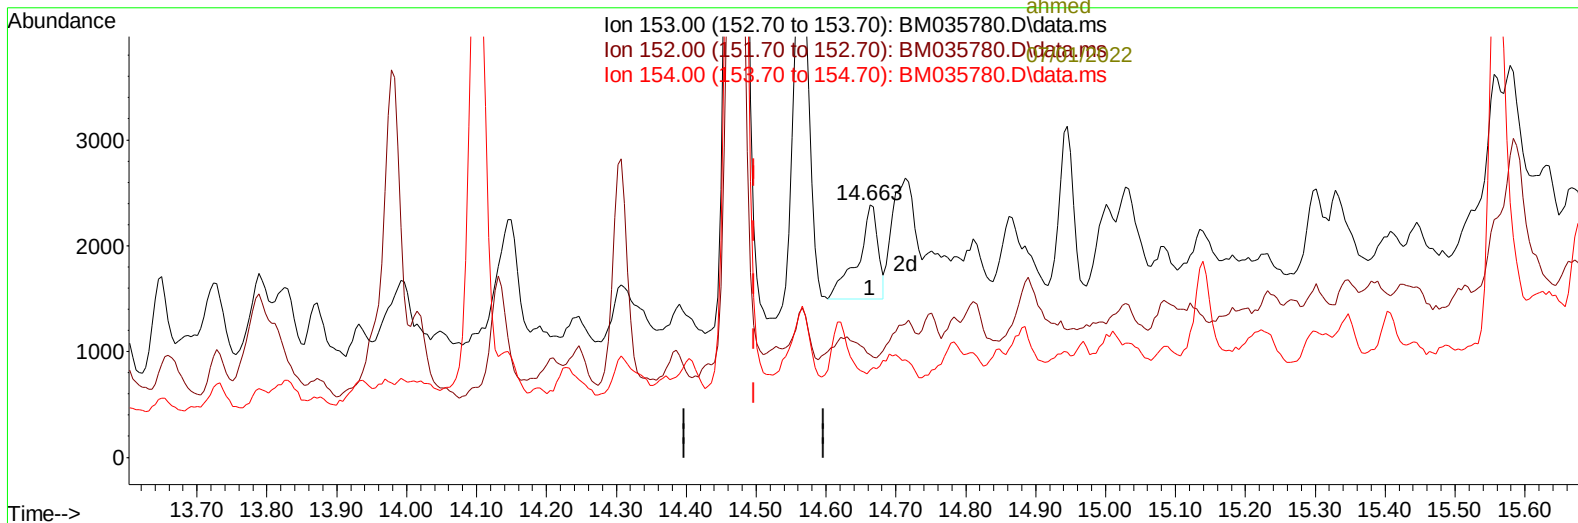

TIC: BM035780.D\data.ms

(11) Acenaphthene (C)

14.663min (+ 0.166) 0.06 ng/ul

response 1814

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	50.30	40.80
154.00	87.10	34.63#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

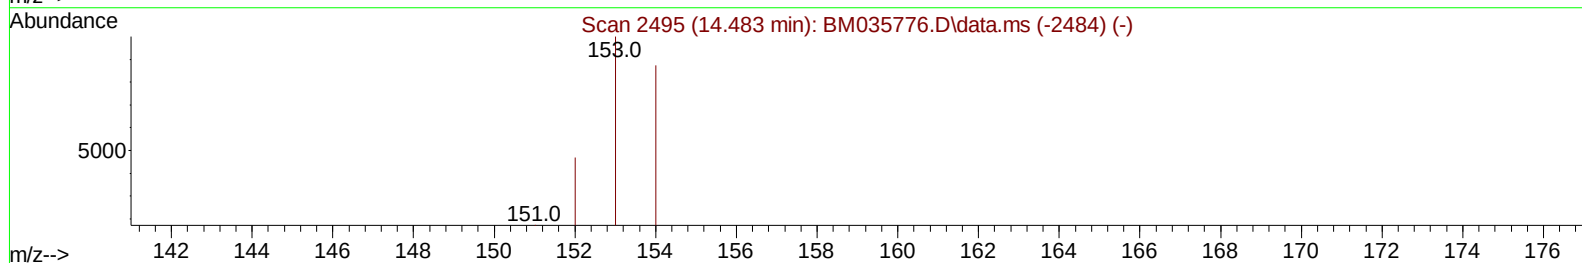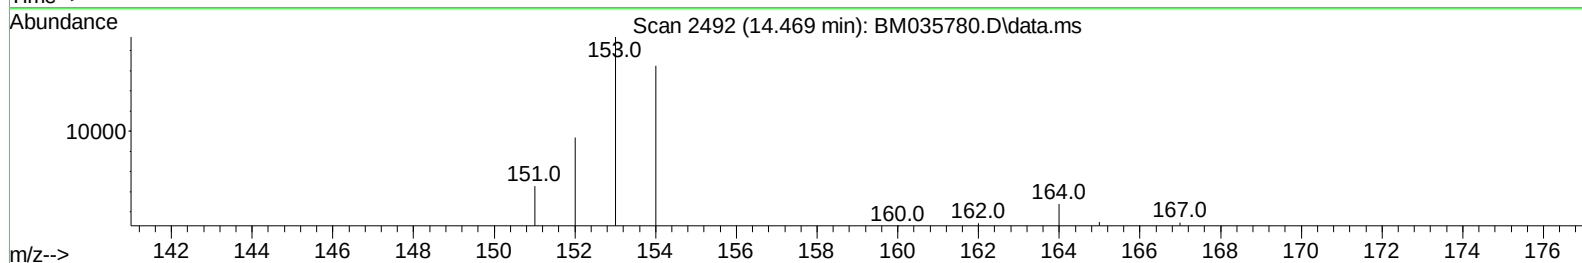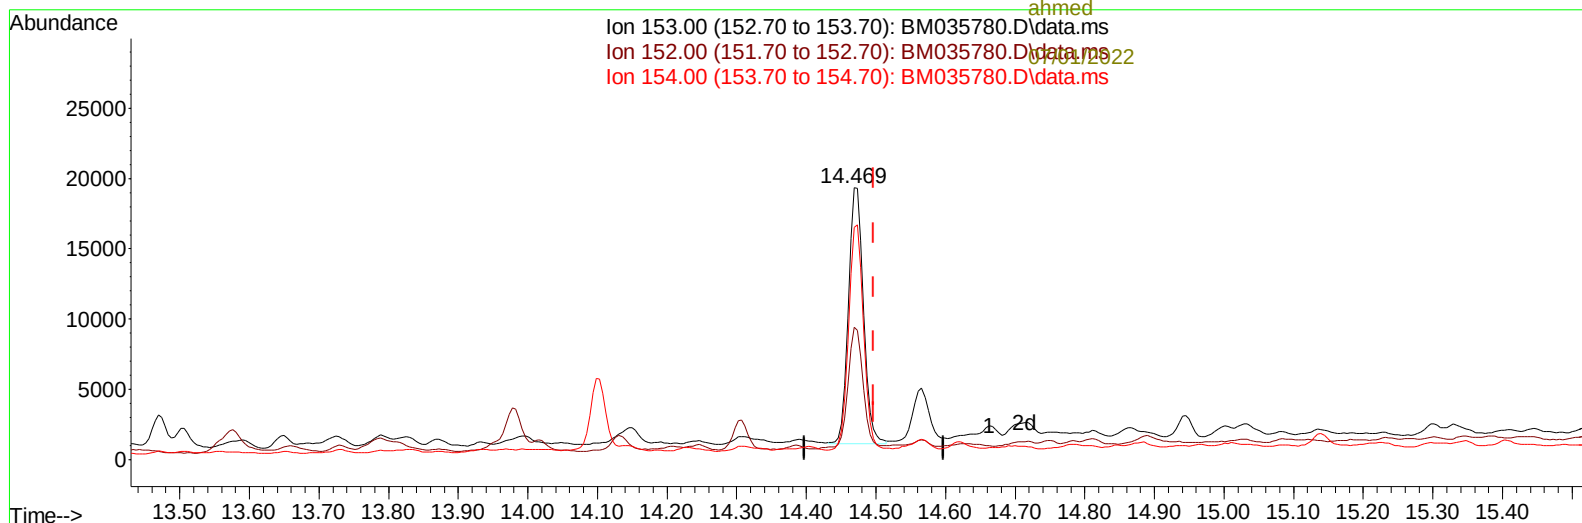

TIC: BM035780.D\data.ms

(11) Acenaphthene (C)

14.469min (-0.029) 0.89 ng/ul m

response 27459

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	50.30	48.60
154.00	87.10	85.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

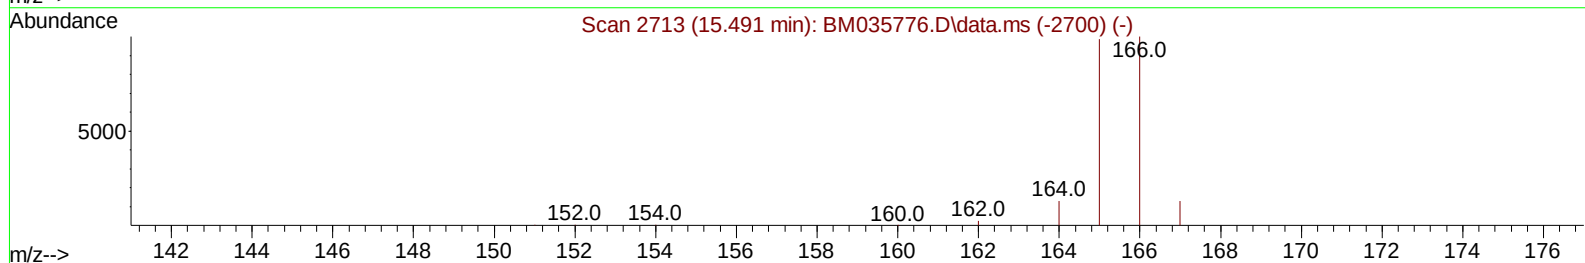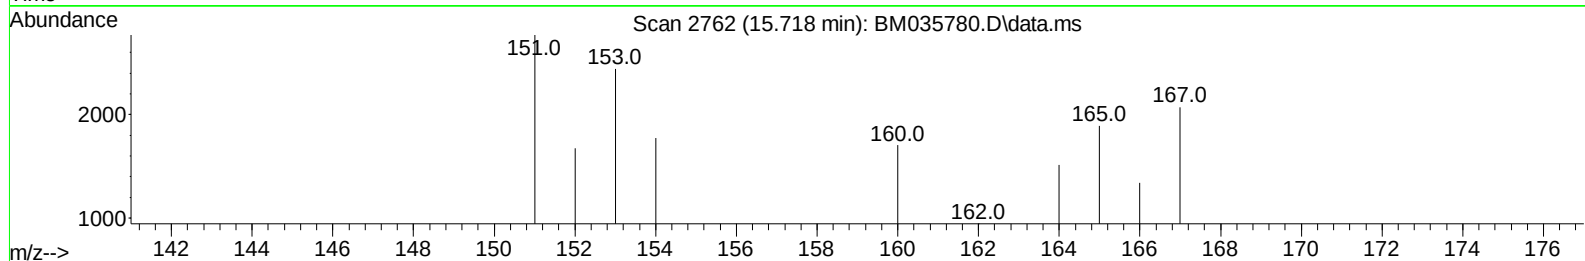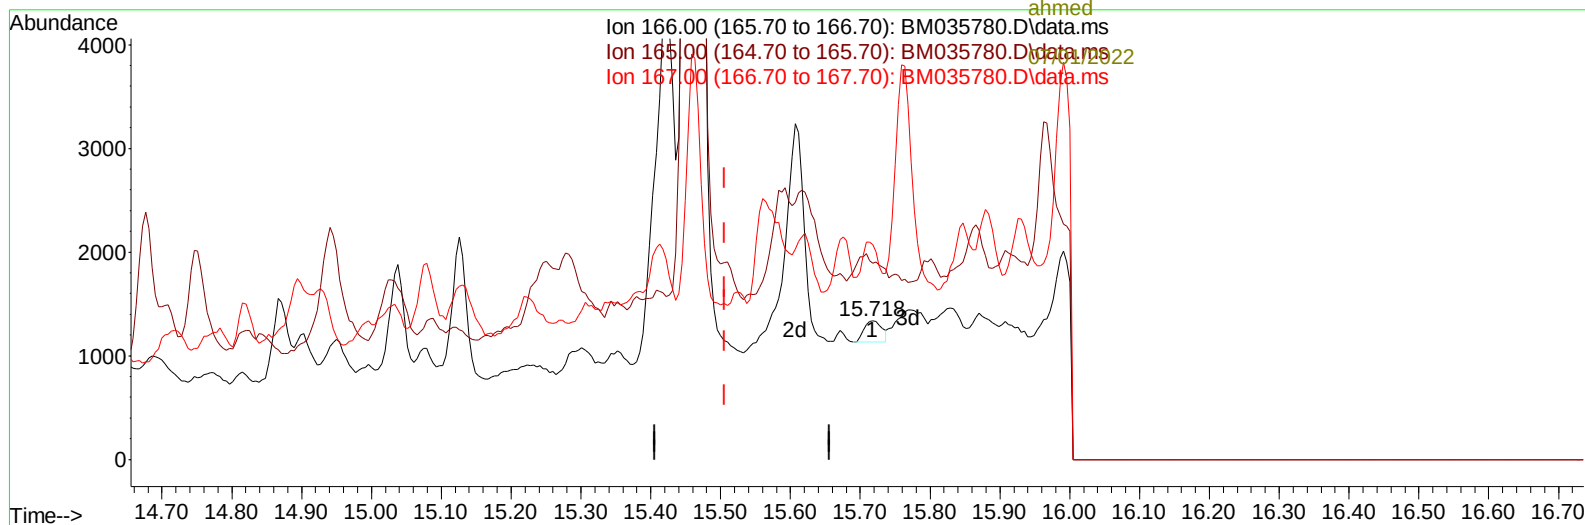

TIC: BM035780.D\data.ms

(12) Fluorene

15.718min (+ 0.212) 0.01 ng/u1

response 371

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	98.60	141.22#
167.00	14.10	154.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 166.00 (165.70 to 166.70): BM035780.D\data.ms
 Ion 165.00 (164.70 to 165.70): BM035780.D\data.ms
 Ion 167.00 (166.70 to 167.70): BM035780.D\data.ms

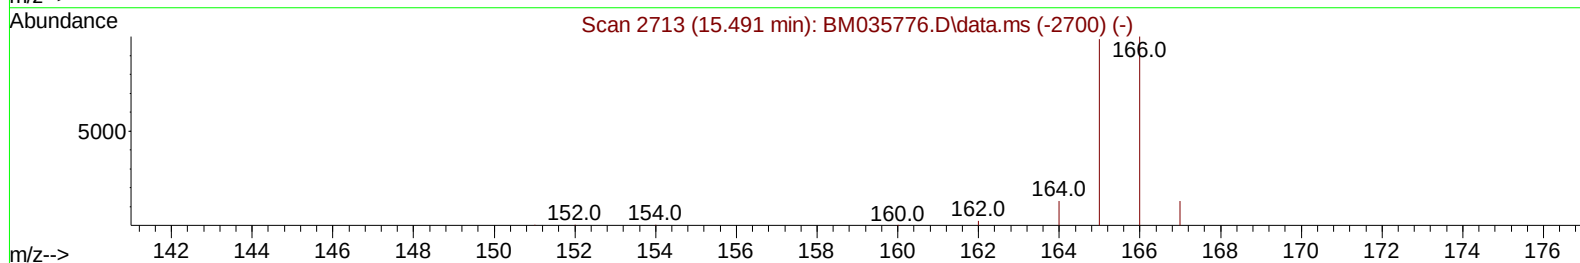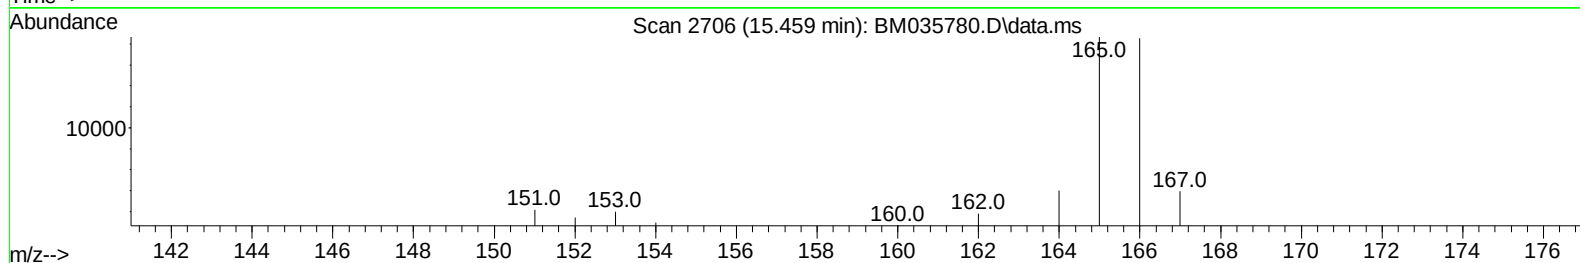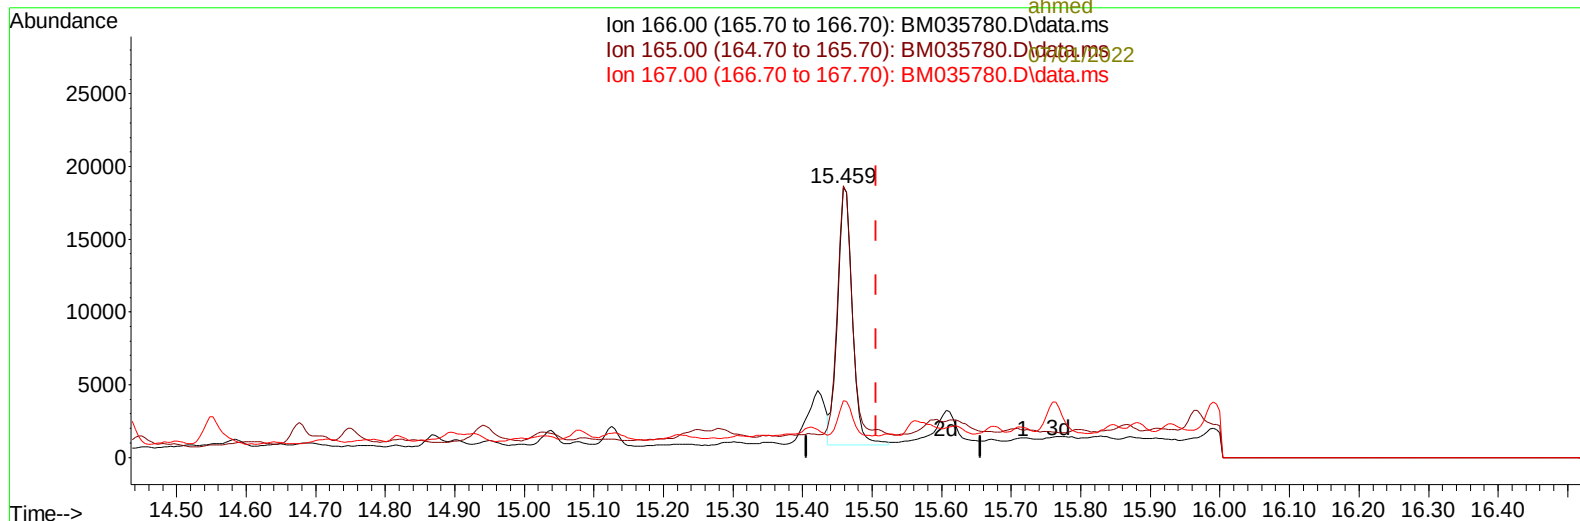

TIC: BM035780.D\data.ms

(12) Fluorene

15.459min (-0.047) 0.74 ng/ul m

response 26161

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	98.60	100.56
167.00	14.10	21.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

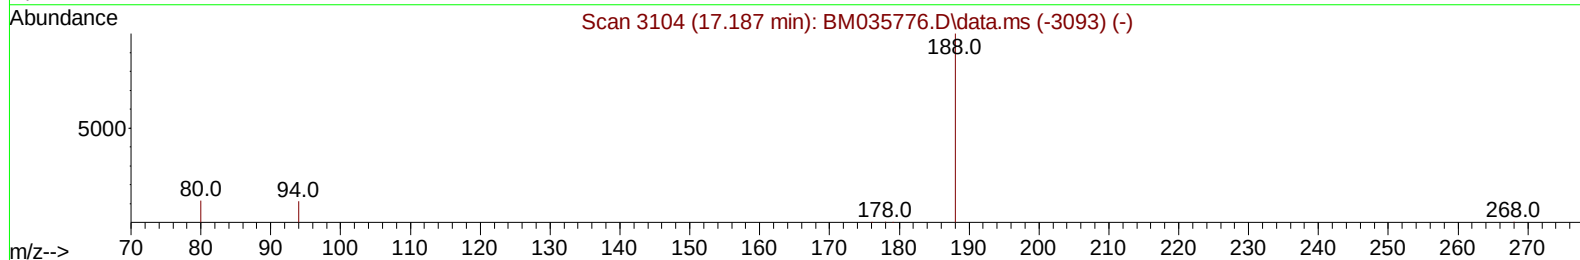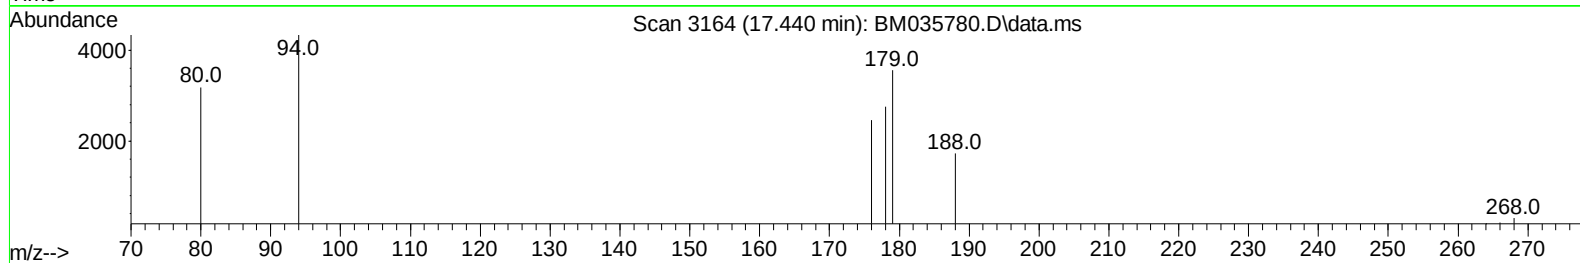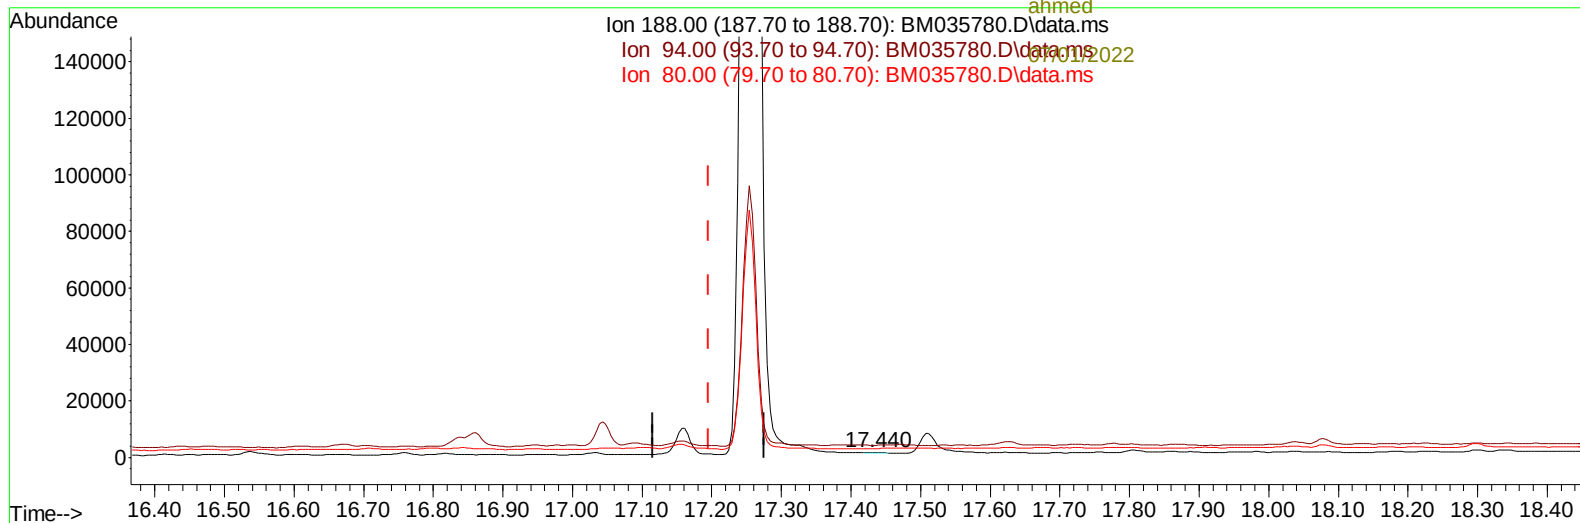

TIC: BM035780.D\data.ms

(13) Phenanthrene-d10 (I)

17.440min (+ 0.244) 0.40 ng/ul

response 193

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	251.92#
80.00	12.70	184.88#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

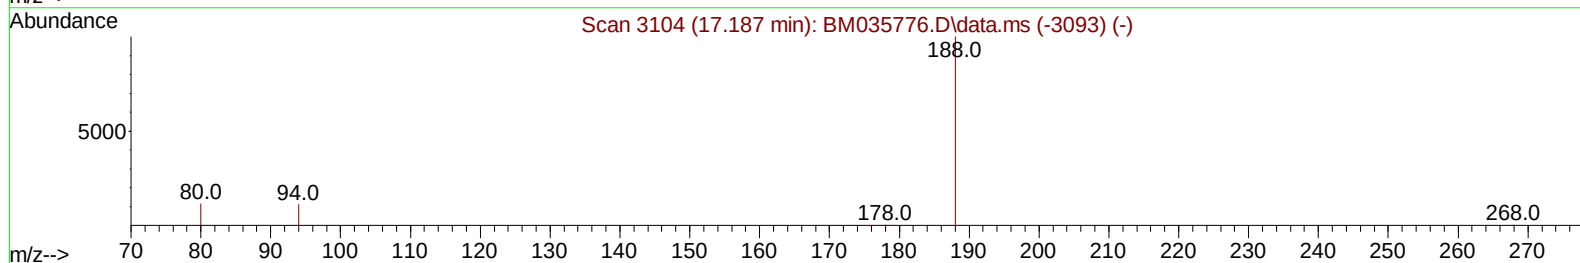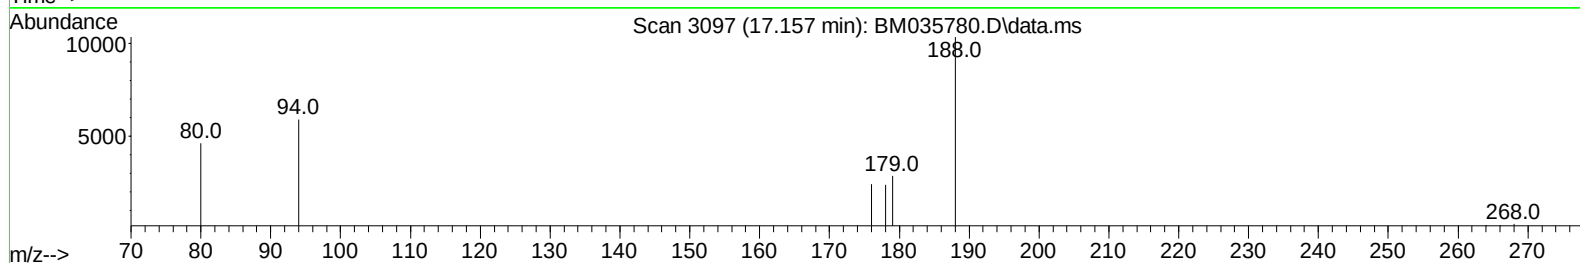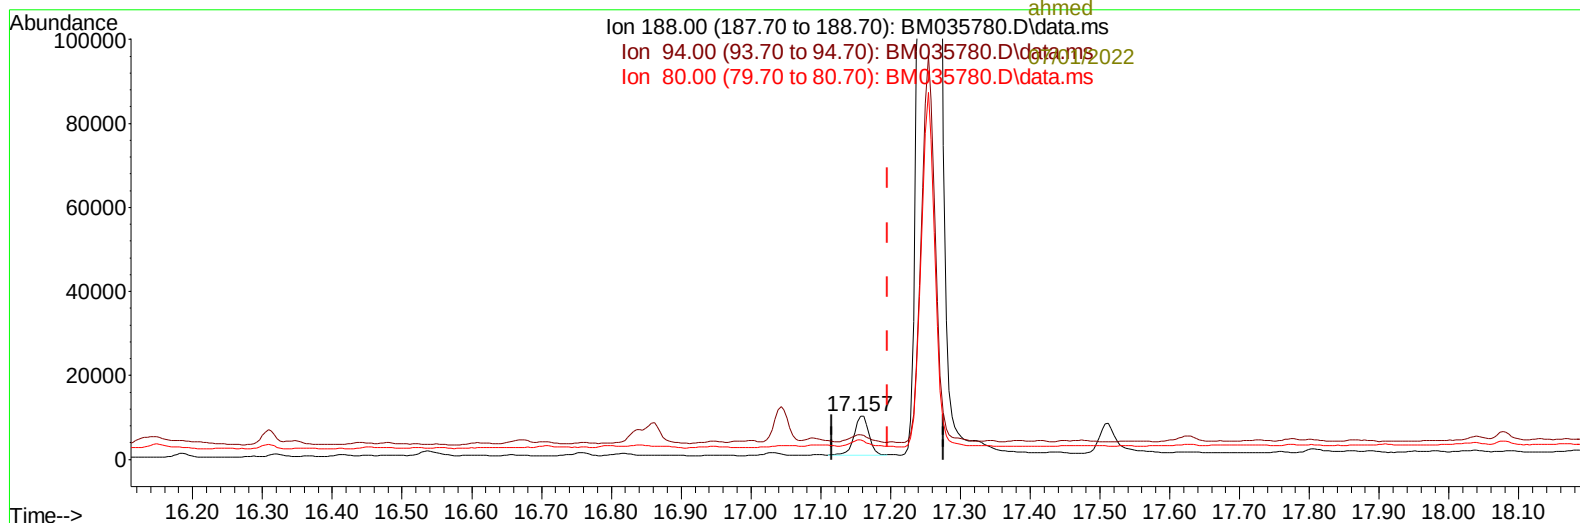

TIC: BM035780.D\data.ms

(13) Phenanthrene-d10 (I)

17.157min (-0.039) 0.40 ng/ul m

response 13699

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.40	57.03#
80.00	12.70	44.67#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

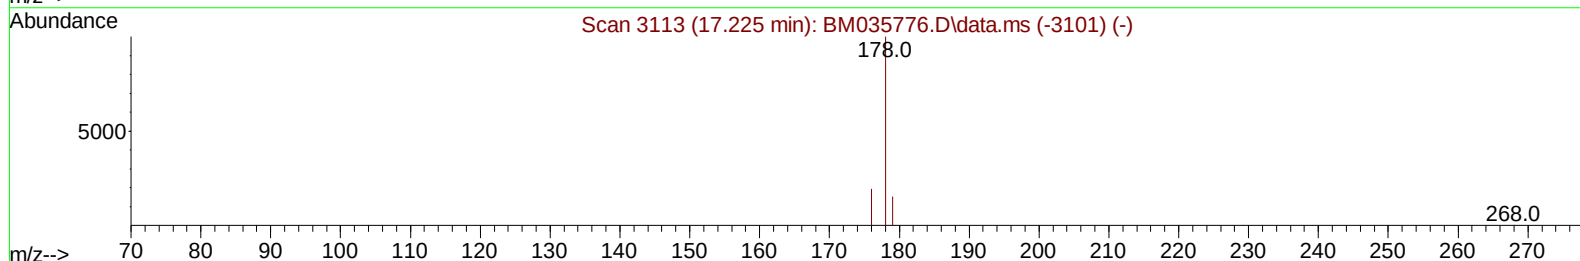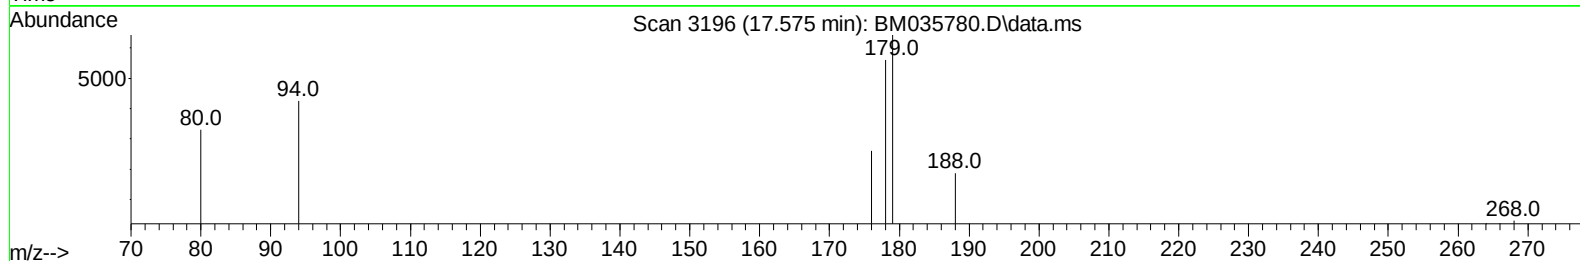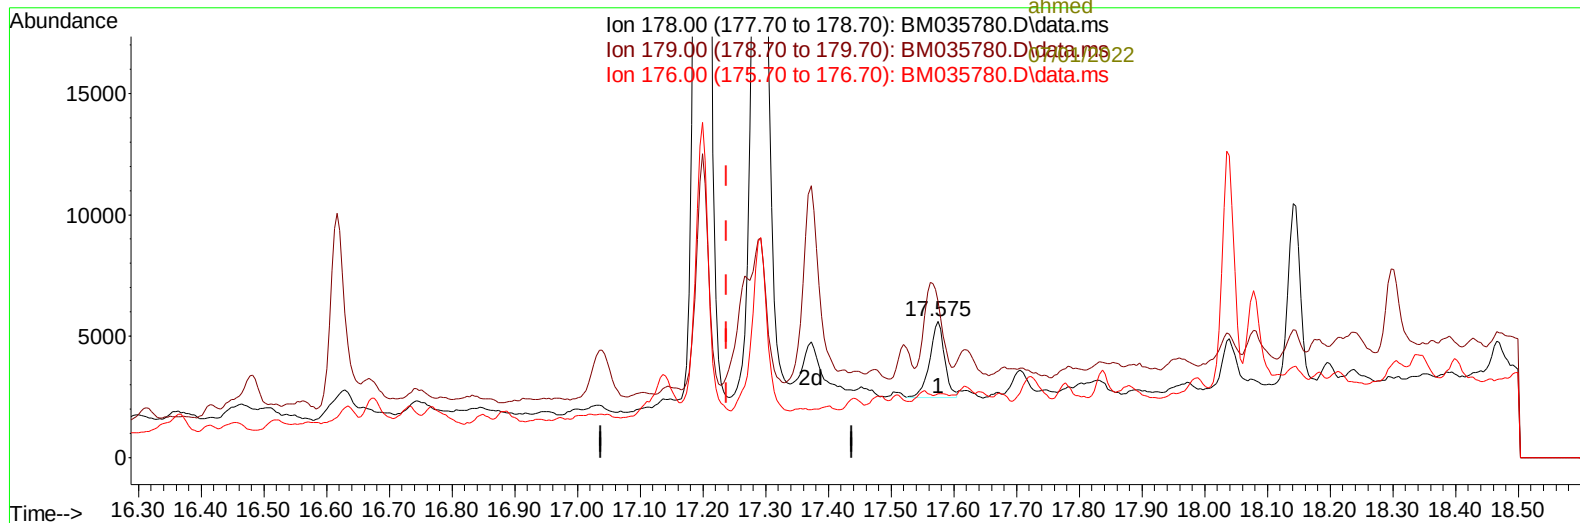

TIC: BM035780.D\data.ms

(15) Phenanthrene

17.575min (+ 0.337) 0.10 ng/u1

response 5186

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.30	114.51#
176.00	19.50	46.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 178.00 (177.70 to 178.70): BM035780.D\data.ms
 Ion 179.00 (178.70 to 179.70): BM035780.D\data.ms
 Ion 176.00 (175.70 to 176.70): BM035780.D\data.ms

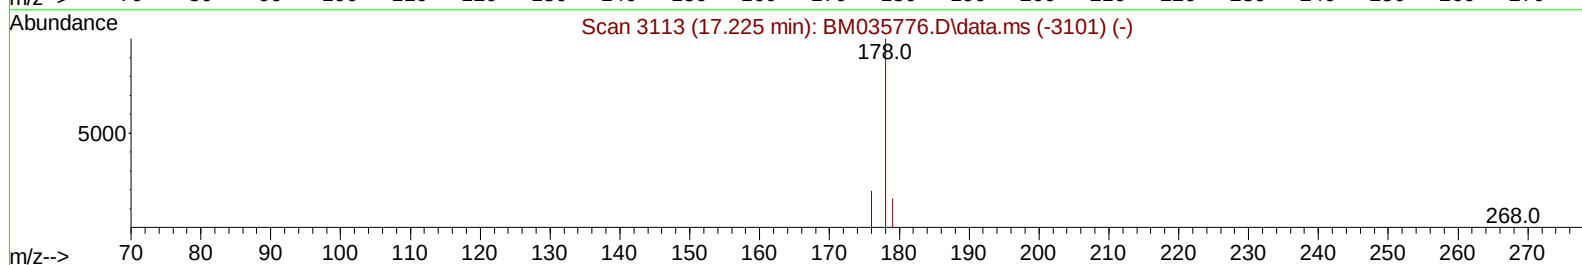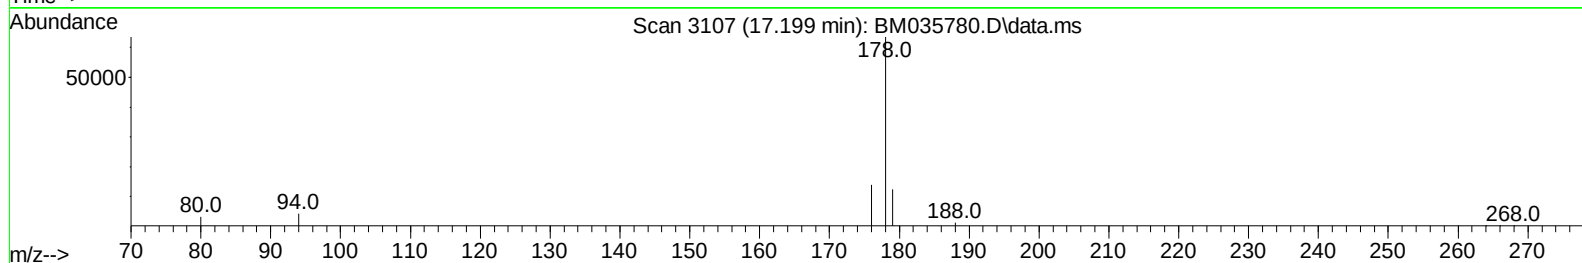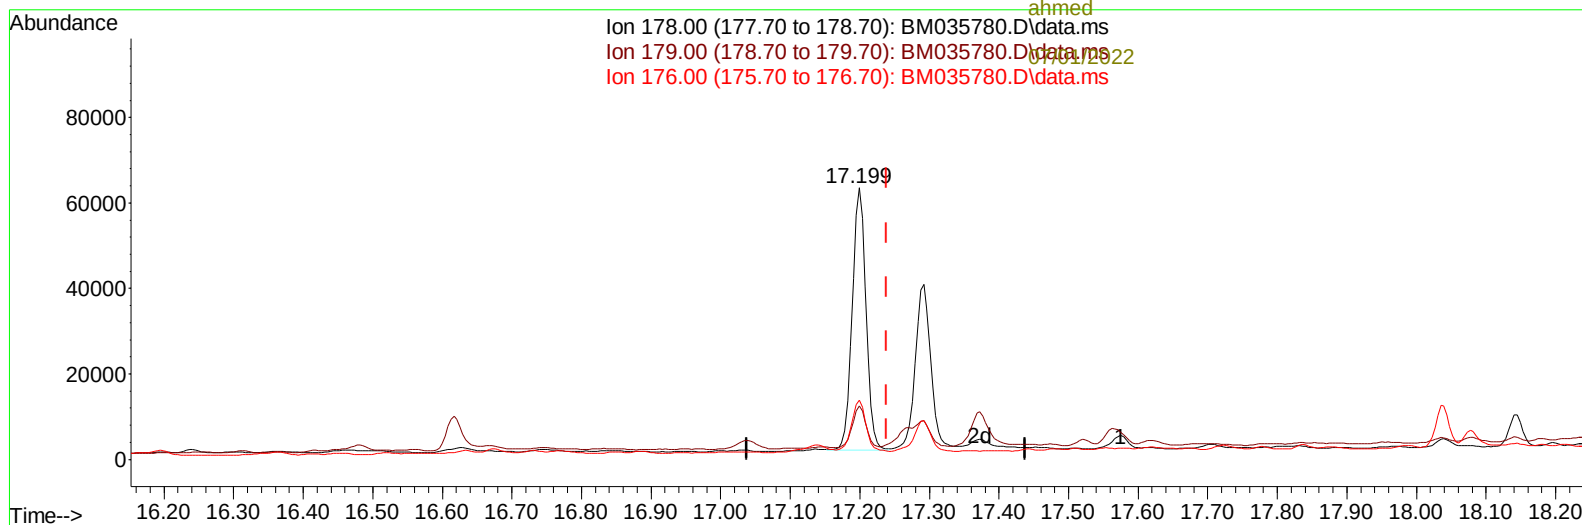

TIC: BM035780.D\data.ms

(15) Phenanthrene

17.199min (-0.039) 1.69 ng/ul m

response 83832

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.30	19.70#
176.00	19.50	21.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

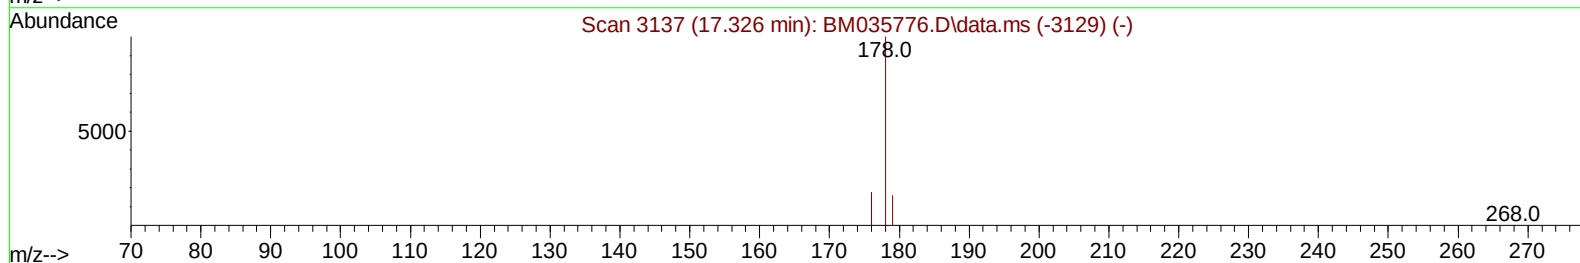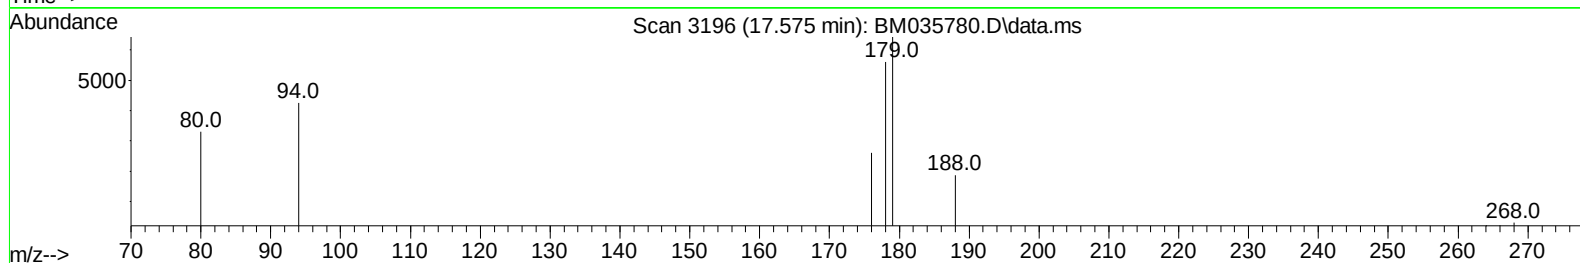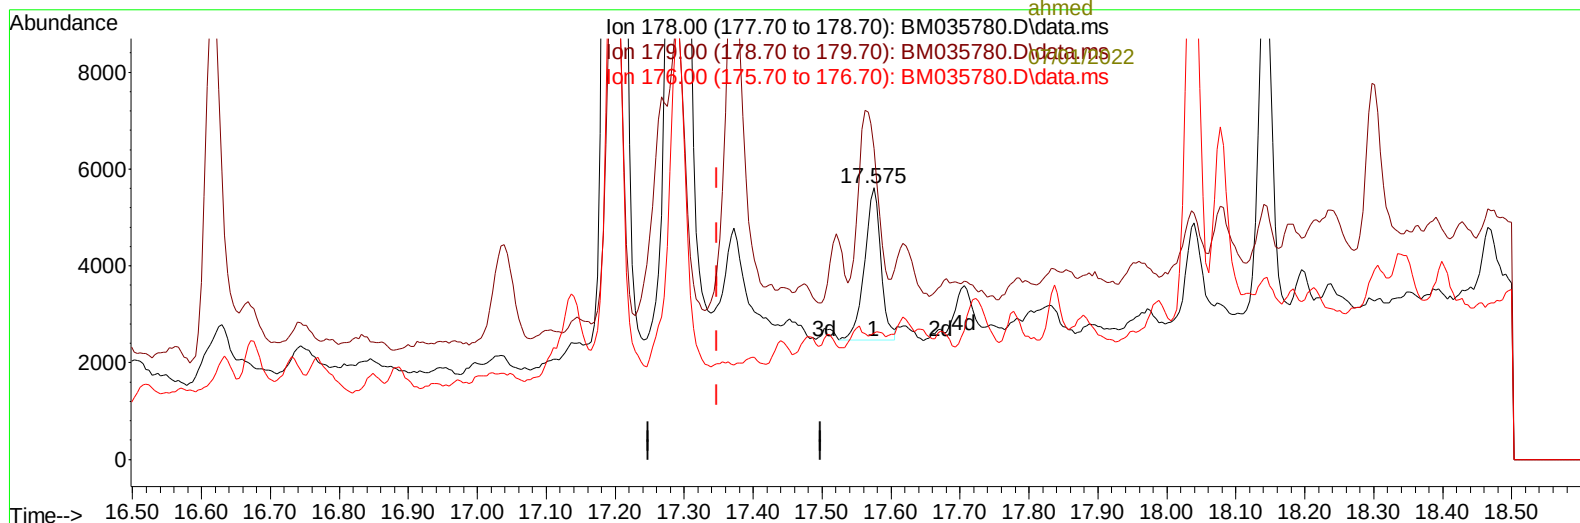

TIC: BM035780.D\data.ms

(16) Anthracene

17.575min (+ 0.227) 0.13 ng/u1

response 5186

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.00	114.51#
176.00	19.50	46.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 240.00 (239.70 to 240.70): BM035780.D\data.ms
 Ion 120.00 (119.70 to 120.70): BM035780.D\data.ms
 Ion 236.00 (235.70 to 236.70): BM035780.D\data.ms

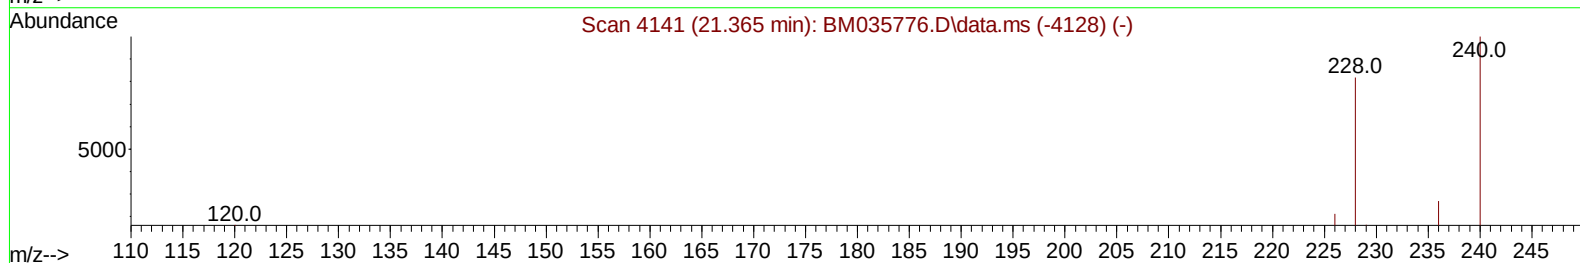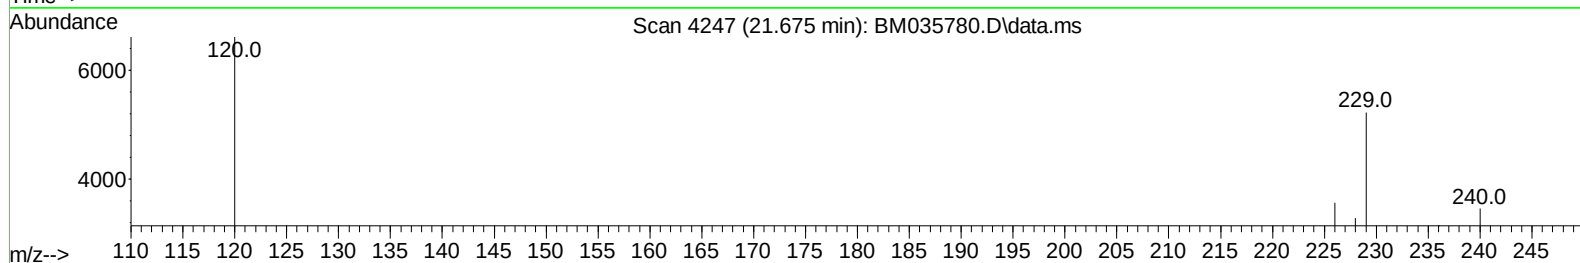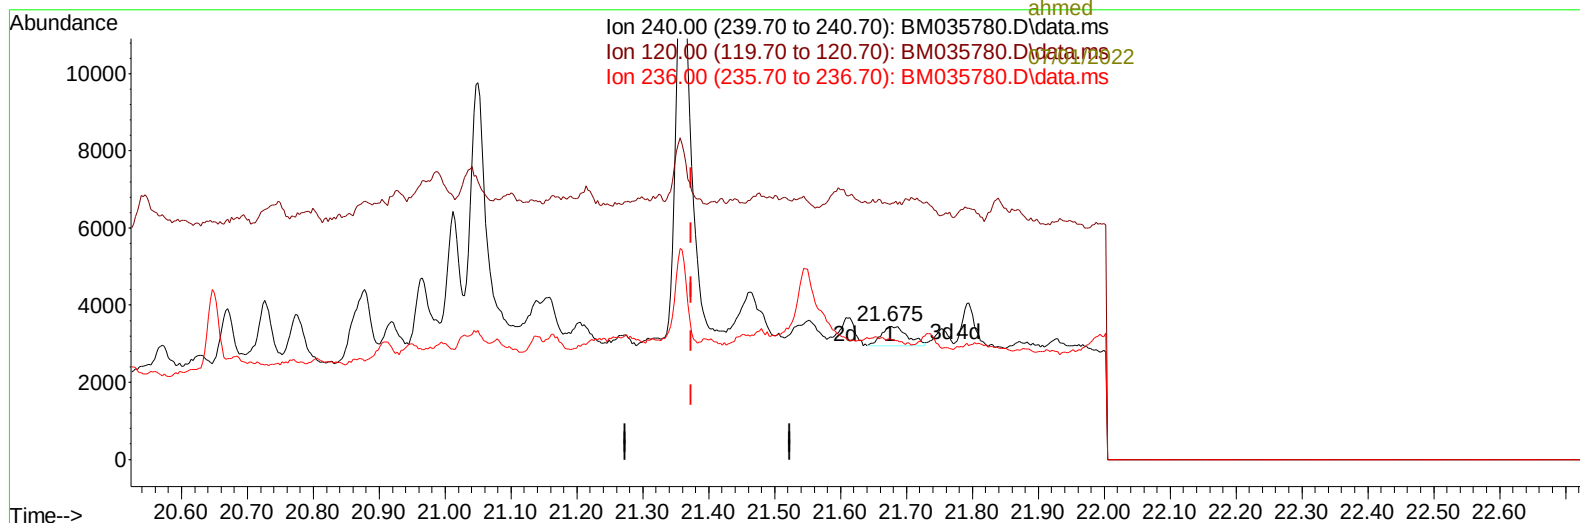

TIC: BM035780.D\data.ms

(17) Chrysene-d12

21.675min (+ 0.302) 0.40 ng/u1

response 1384

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.90	191.65#
236.00	29.40	90.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 240.00 (239.70 to 240.70): BM035780.D\data.ms
 Ion 120.00 (119.70 to 120.70): BM035780.D\data.ms
 Ion 236.00 (235.70 to 236.70): BM035780.D\data.ms

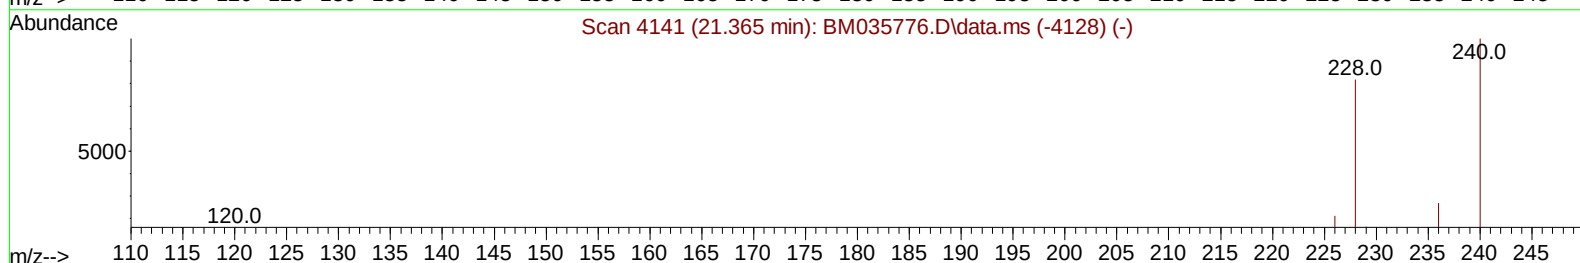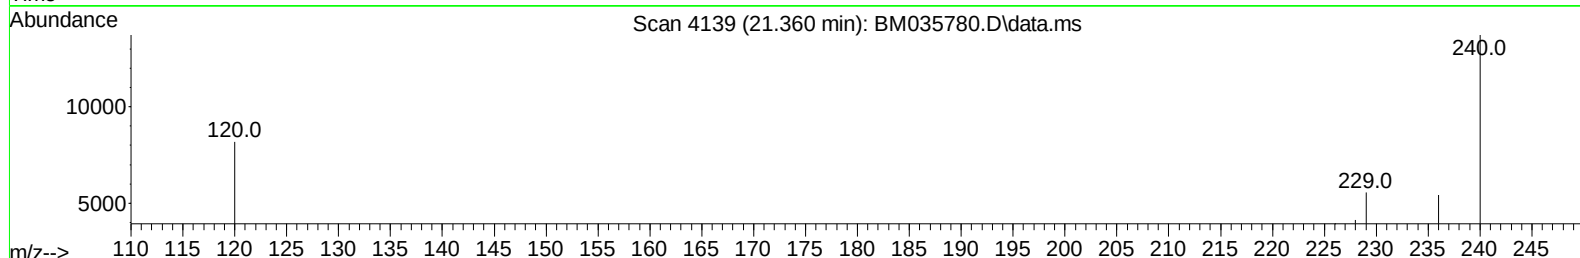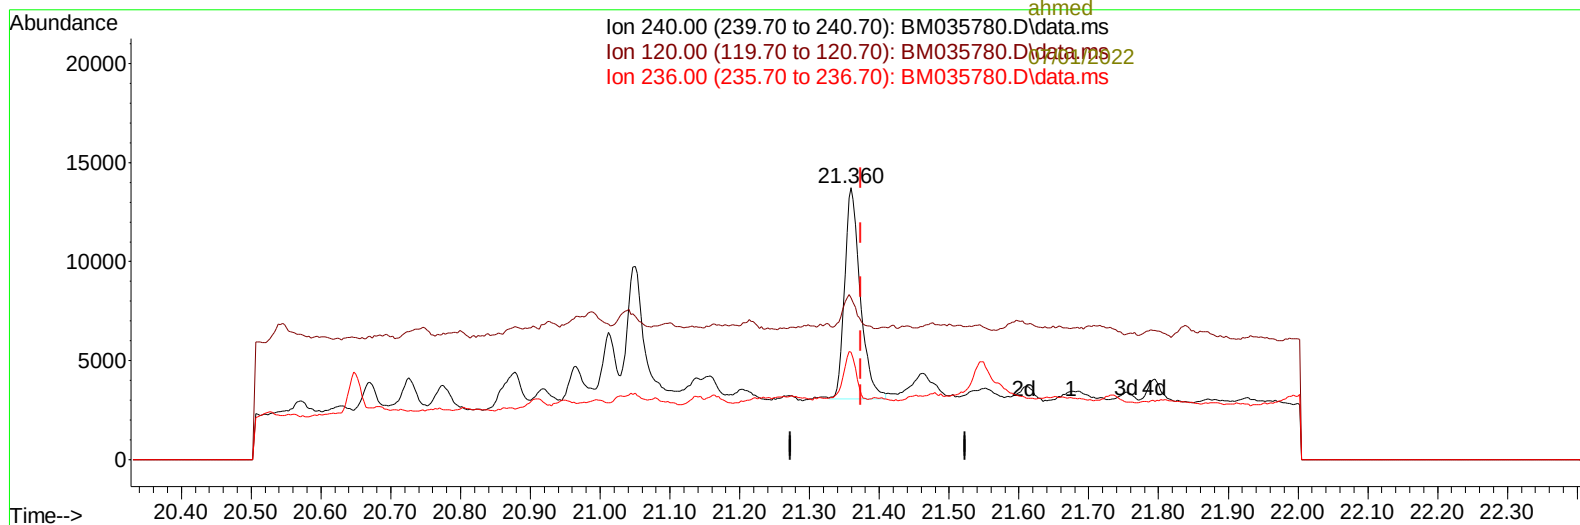

TIC: BM035780.D\data.ms

(17) Chrysene-d12

21.360min (-0.014) 0.40 ng/ul m

response 16570

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.90	59.59#
236.00	29.40	39.58#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9




Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Ion 212.00 (211.70 to 212.70): BM035780.D\data.ms
 Ion 106.00 (105.70 to 106.70): BM035780.D\data.ms
 Ion 104.00 (103.70 to 104.70): BM035780.D\data.ms

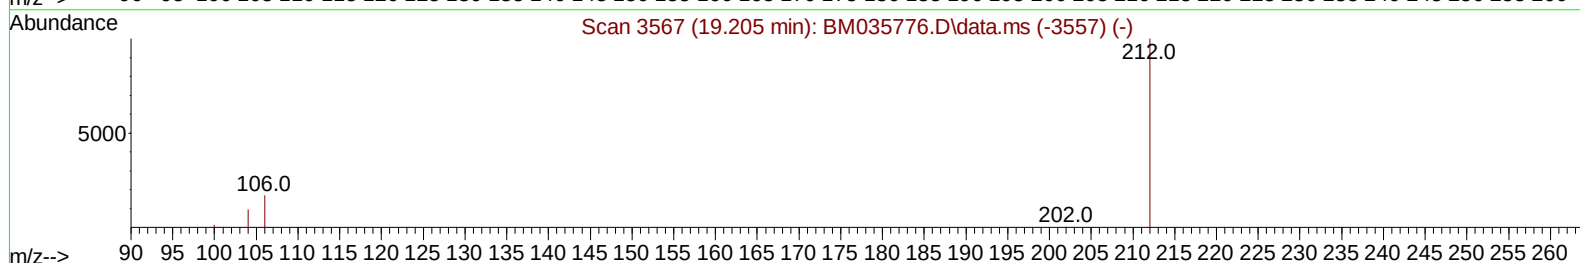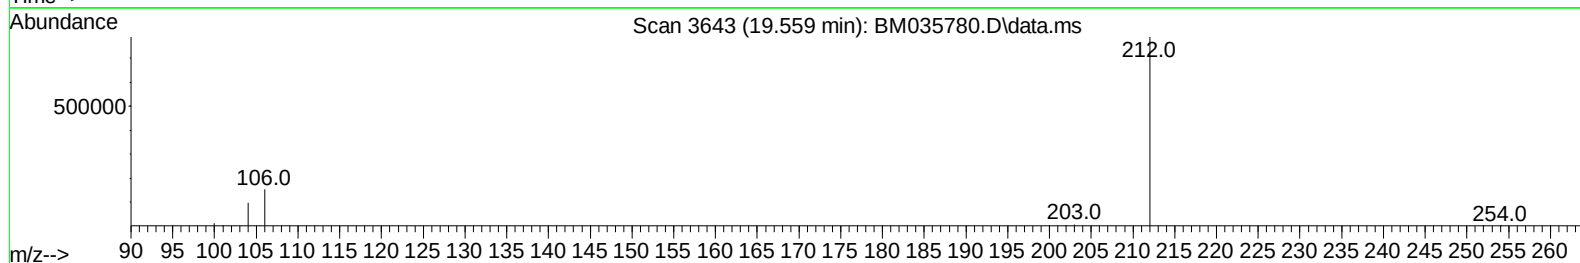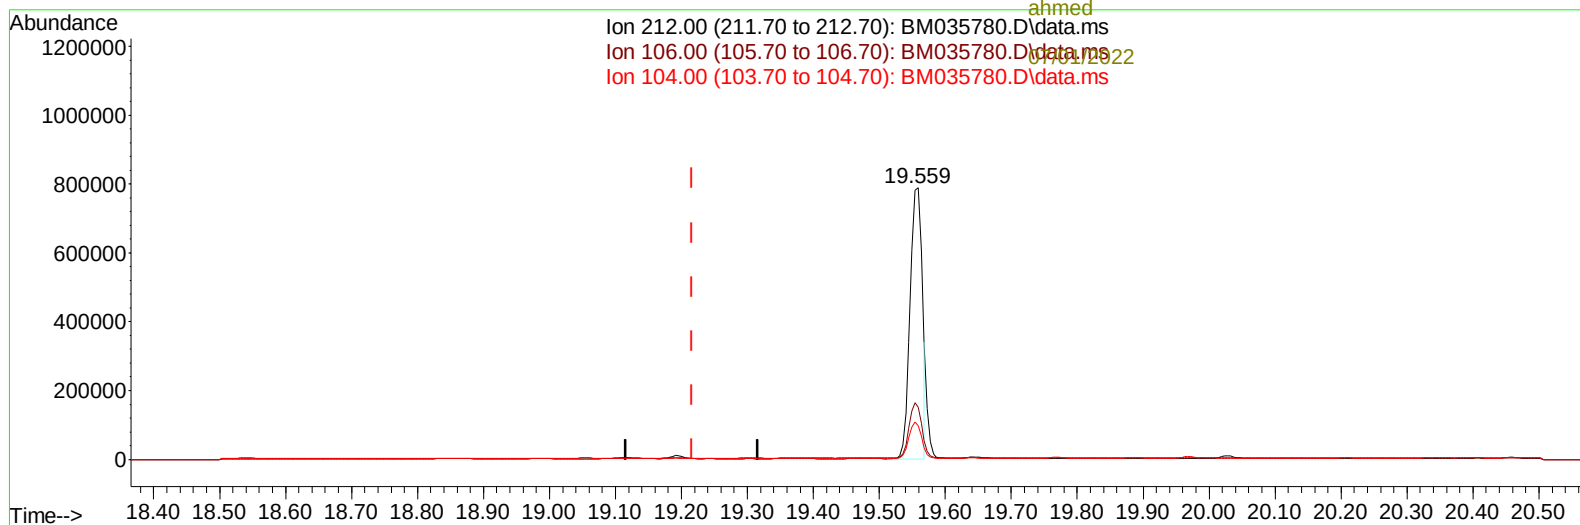

TIC: BM035780.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.559min (+ 0.343) 18.14 ng/u1

response 1013274

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	16.20	20.35#
104.00	9.70	13.45#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9


Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration


Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed


Ion 212.00 (211.70 to 212.70): BM035780.D\data.ms
 Ion 106.00 (105.70 to 106.70): BM035780.D\data.ms
 Ion 104.00 (103.70 to 104.70): BM035780.D\data.ms

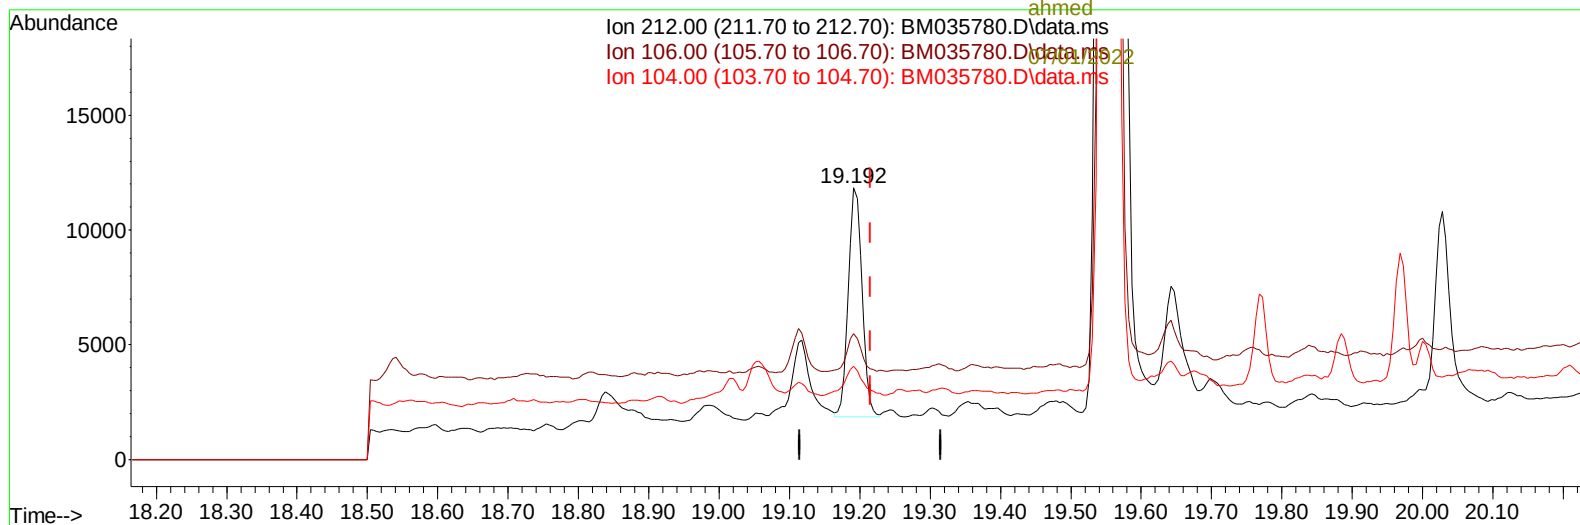

Scan 3564 (19.192 min): BM035780.D\data.ms

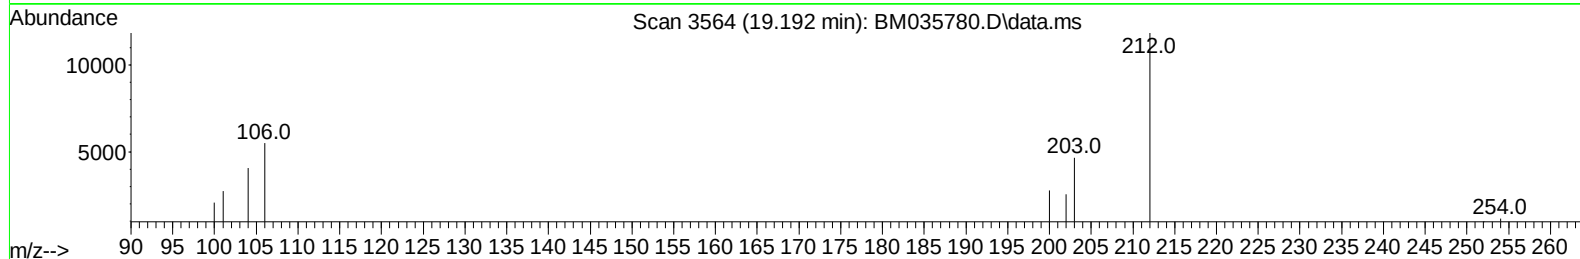

Scan 3567 (19.205 min): BM035776.D\data.ms (-3557) (-)

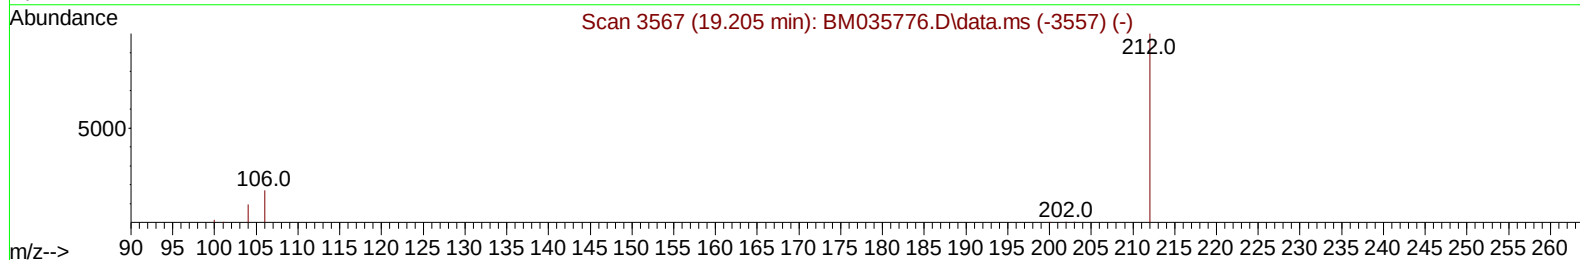

TIC: BM035780.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.192min (-0.024) 0.24 ng/ul m

response 13356

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	16.20	1543.99#
104.00	9.70	1020.50#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

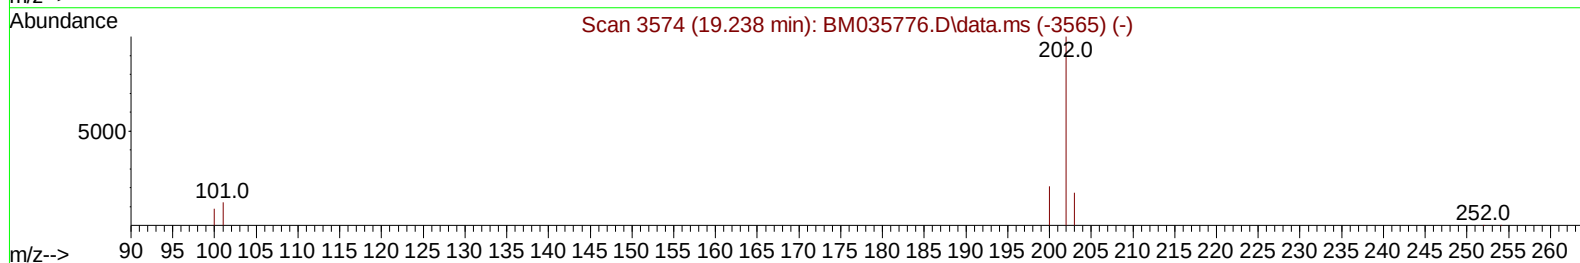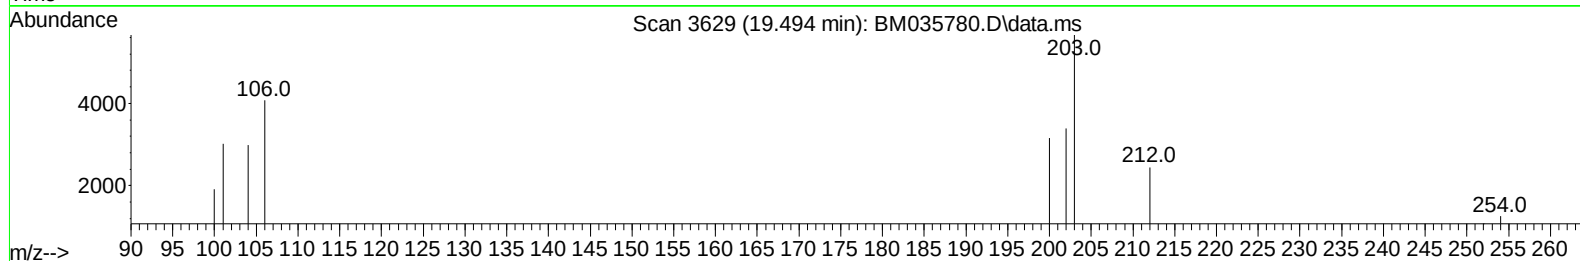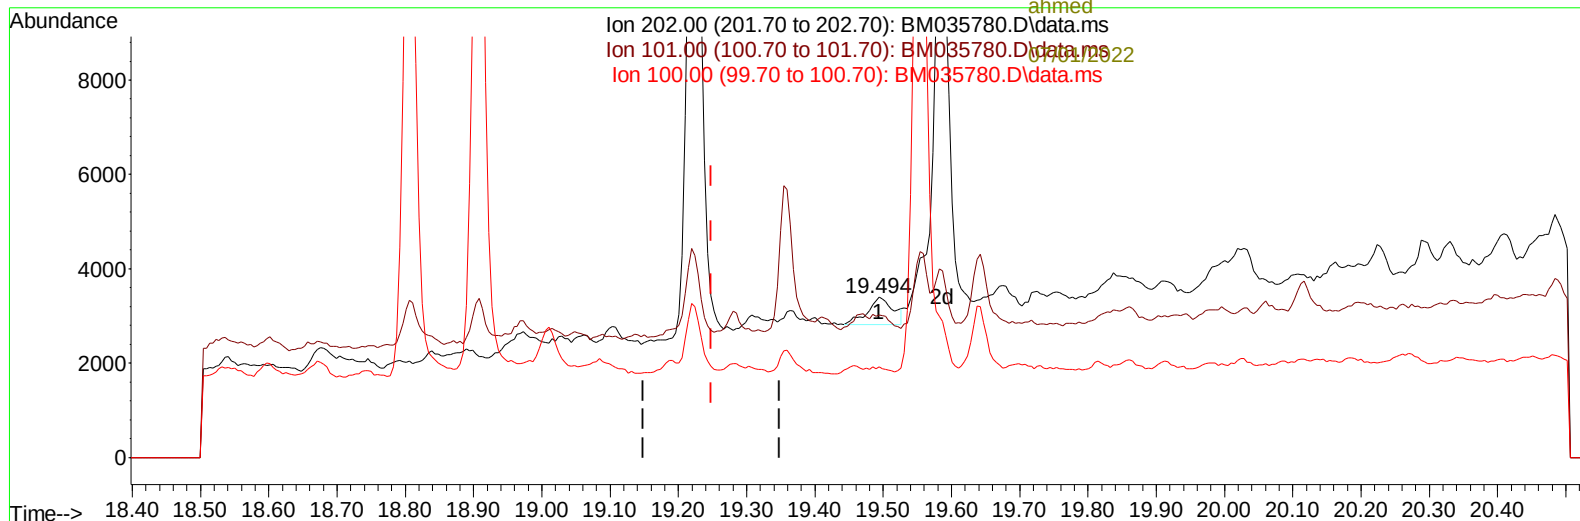

TIC: BM035780.D\data.ms

(19) Fluoranthene (C)

19.494min (+ 0.246) 0.02 ng/u1

response 1502

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.60	88.93#
100.00	9.90	56.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

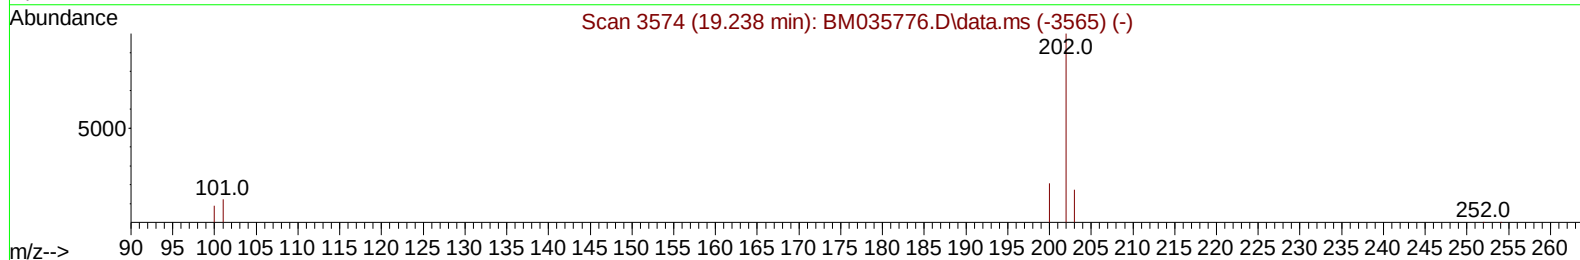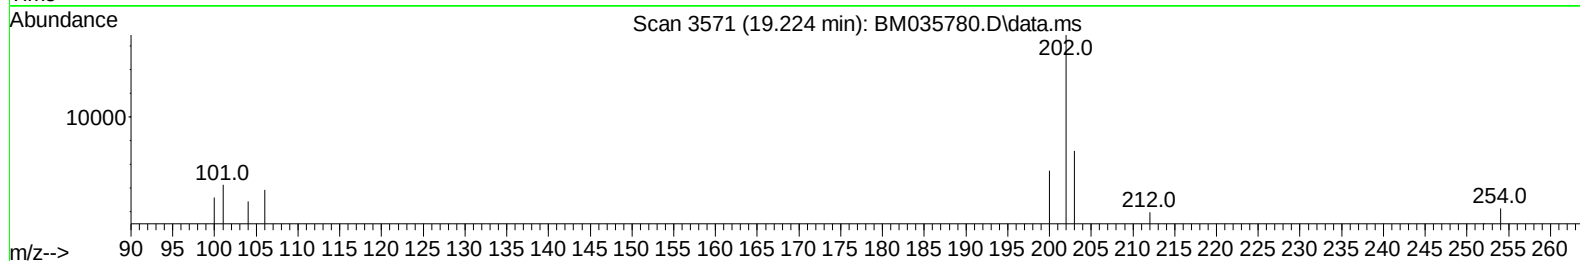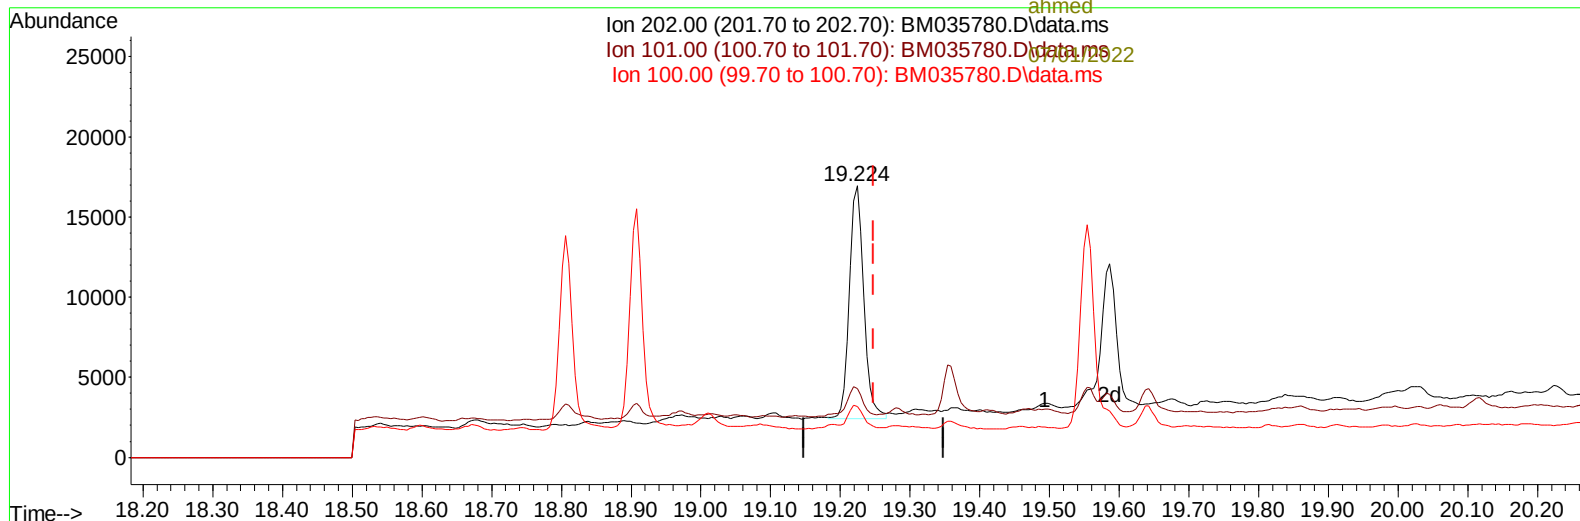

TIC: BM035780.D\data.ms

(19) Fluoranthene (C)

19.224min (-0.024) 0.25 ng/ul m

response 20528

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	12.60	25.31#
100.00	9.90	18.85#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

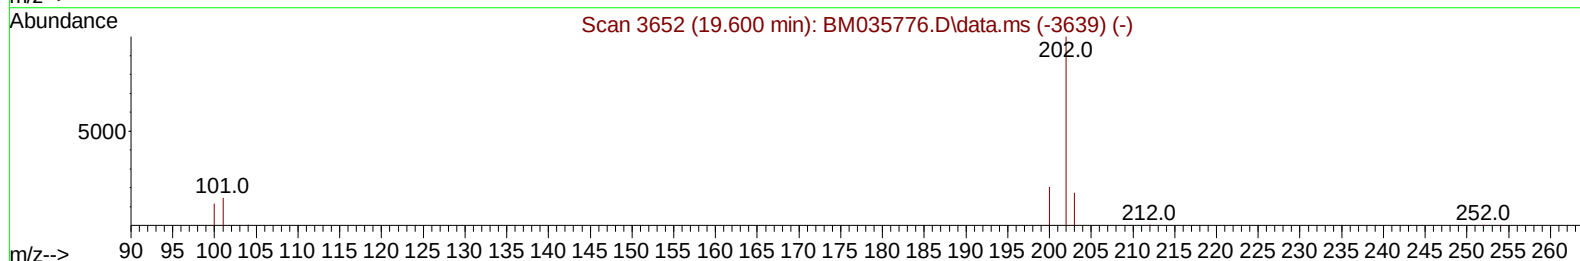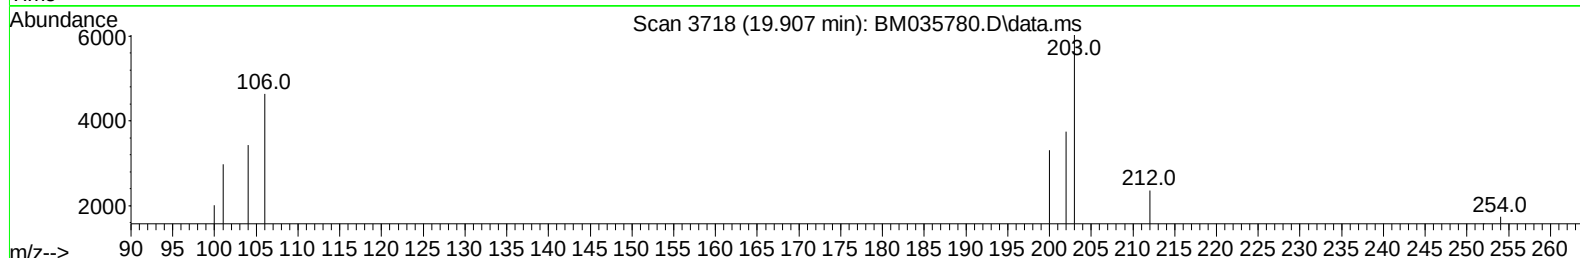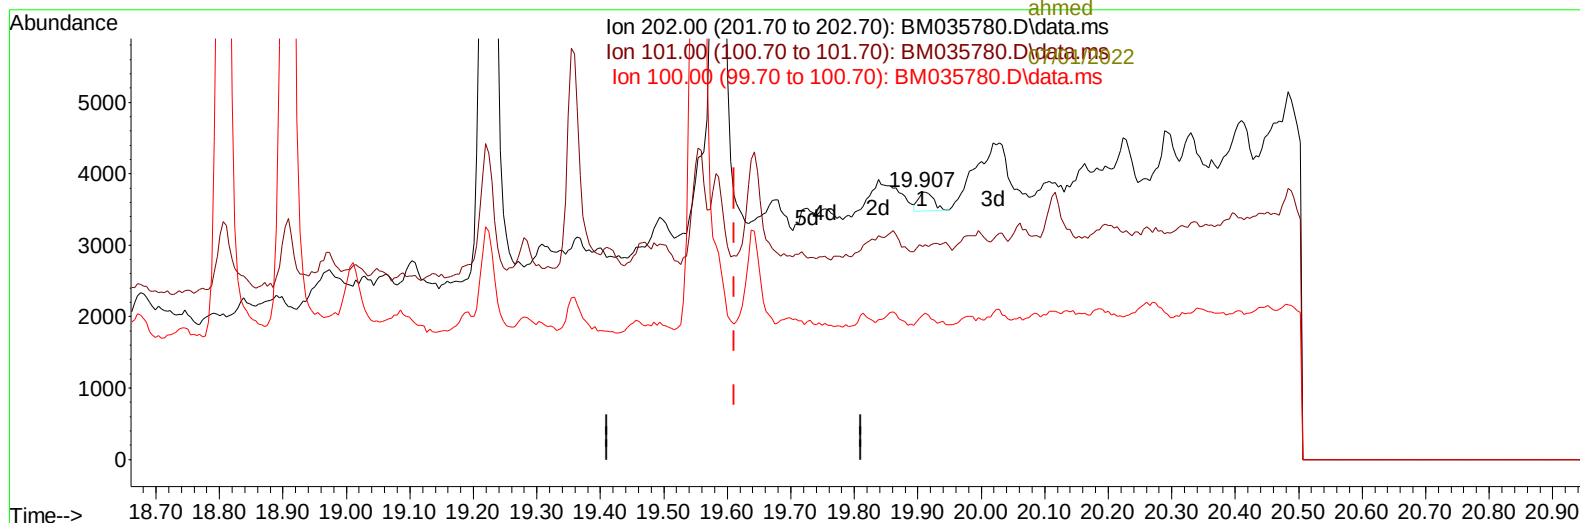

TIC: BM035780.D\data.ms

(20) Pyrene

19.907min (+ 0.297) 0.00 ng/u1

response 454

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.00	79.68#
100.00	12.20	53.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

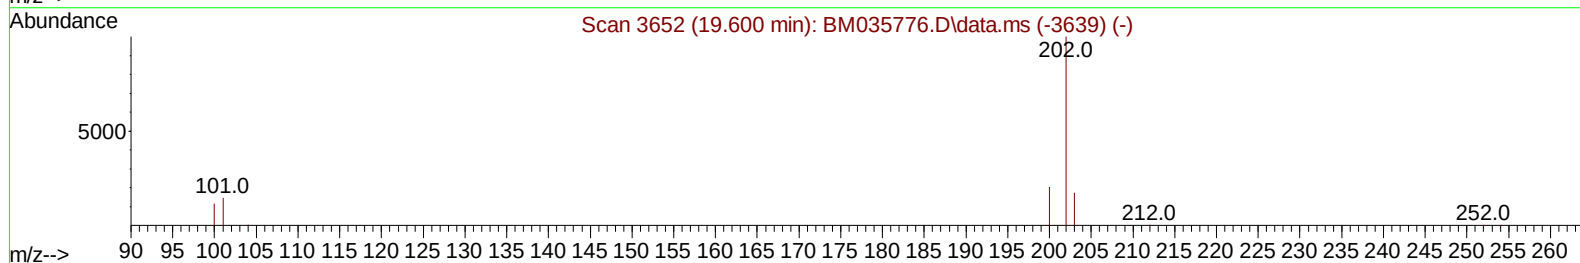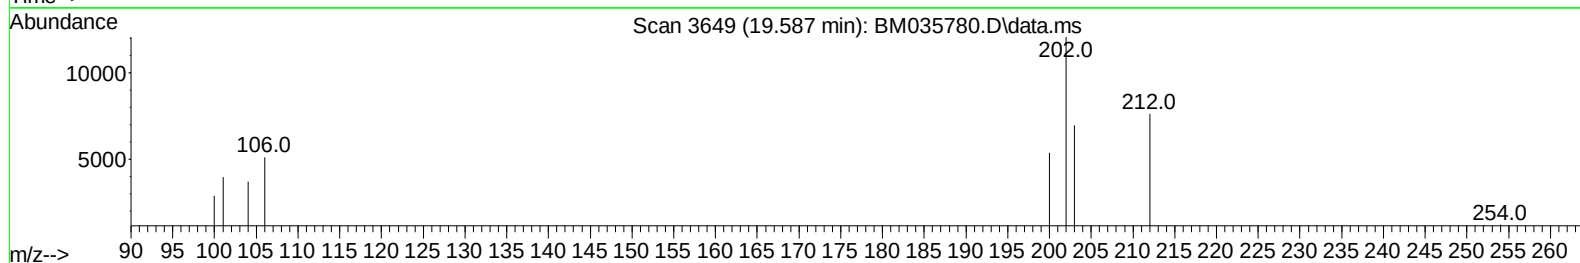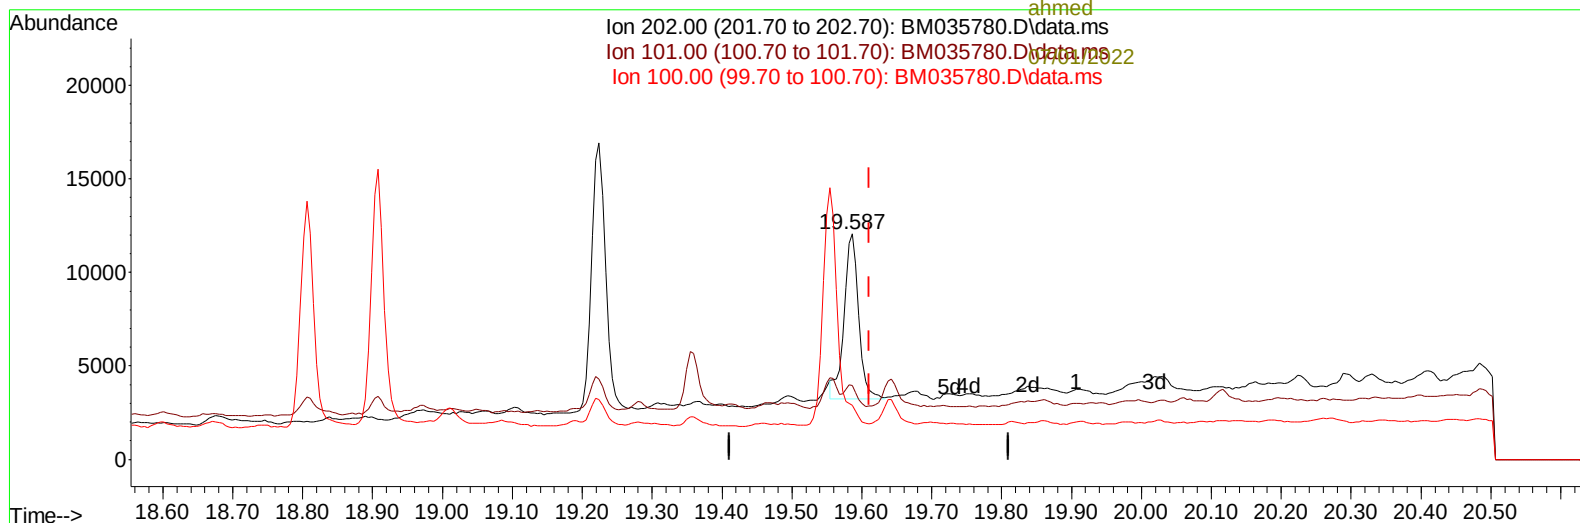

TIC: BM035780.D\data.ms

(20) Pyrene

19.587min (-0.024) 0.14 ng/ul m

response 12824

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.00	32.79#
100.00	12.20	23.97#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

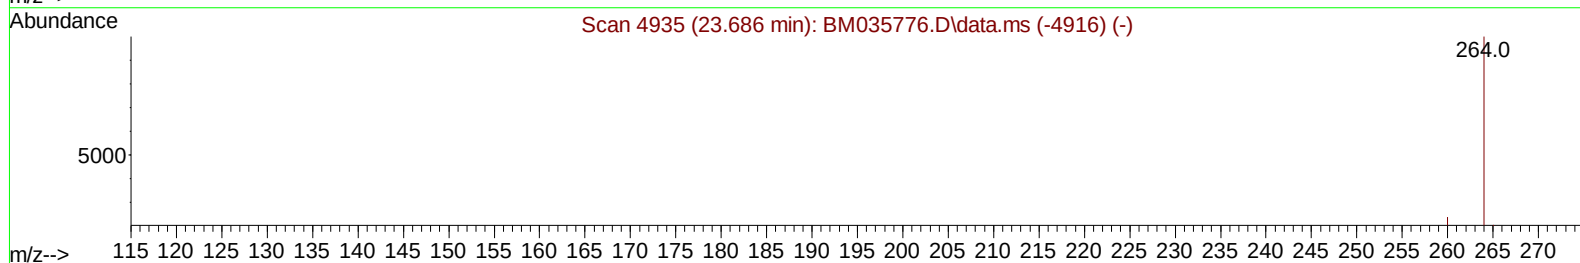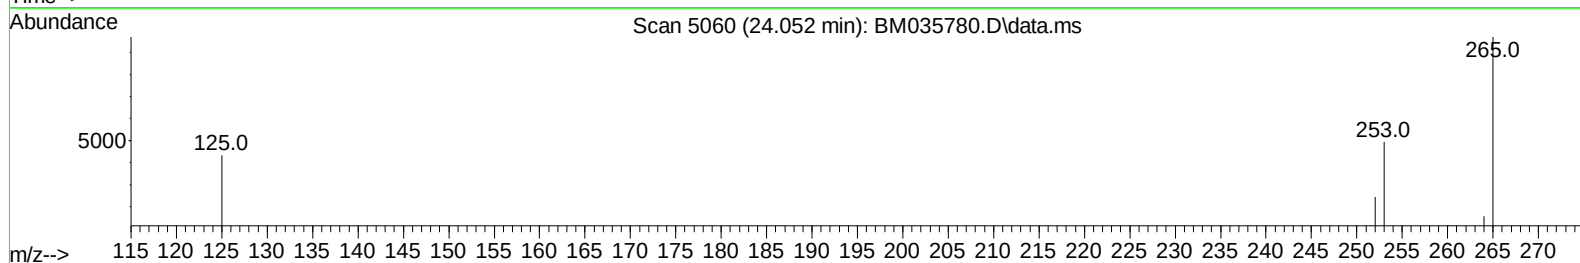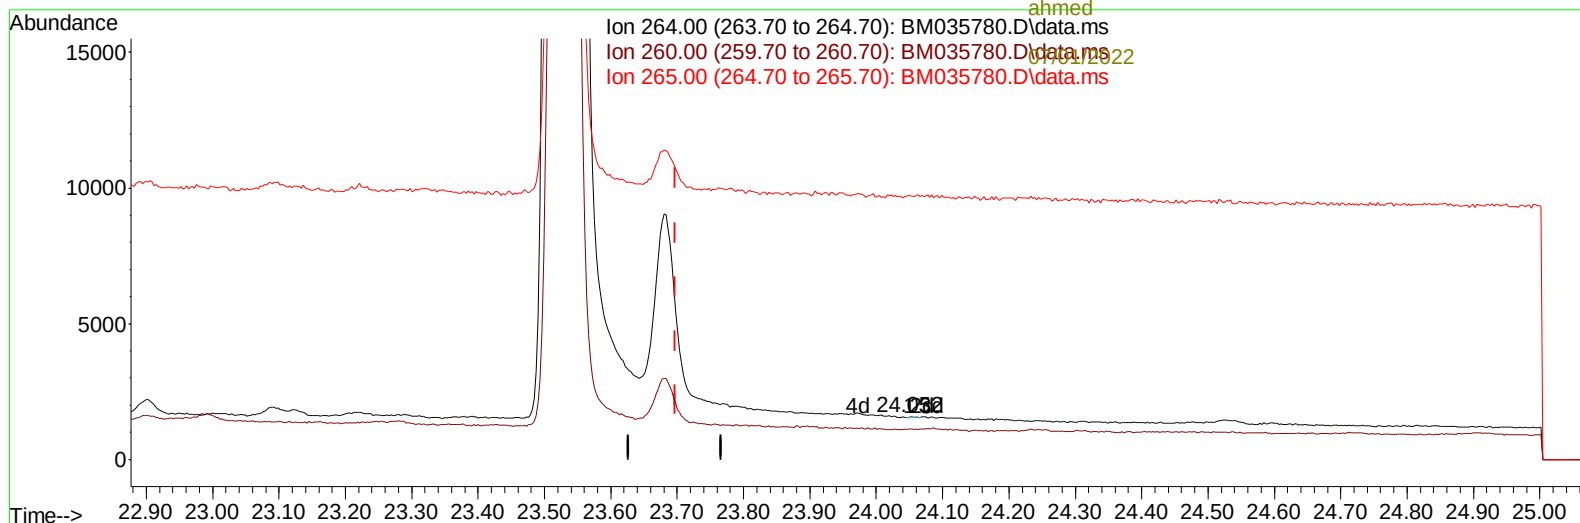

TIC: BM035780.D\data.ms

(23) Perylene-d12 (I)

24.052min (+ 0.355) 0.40 ng/ul

response 31

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	71.53#
265.00	119.70	618.15#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

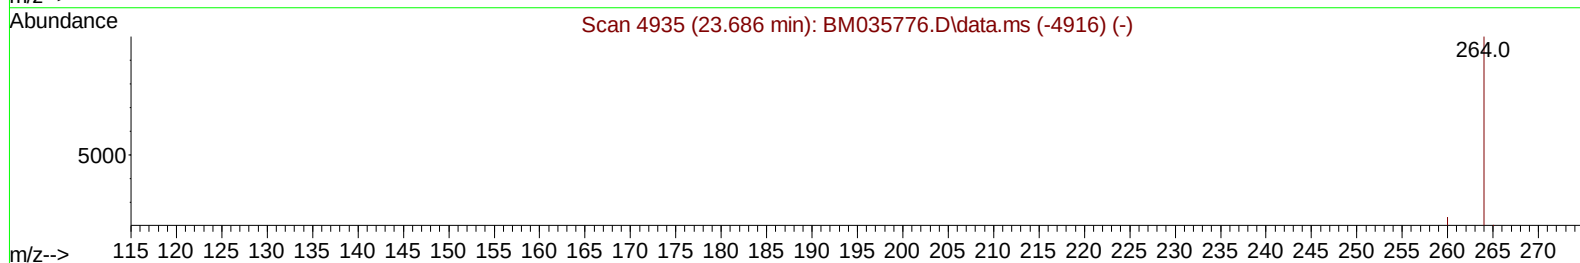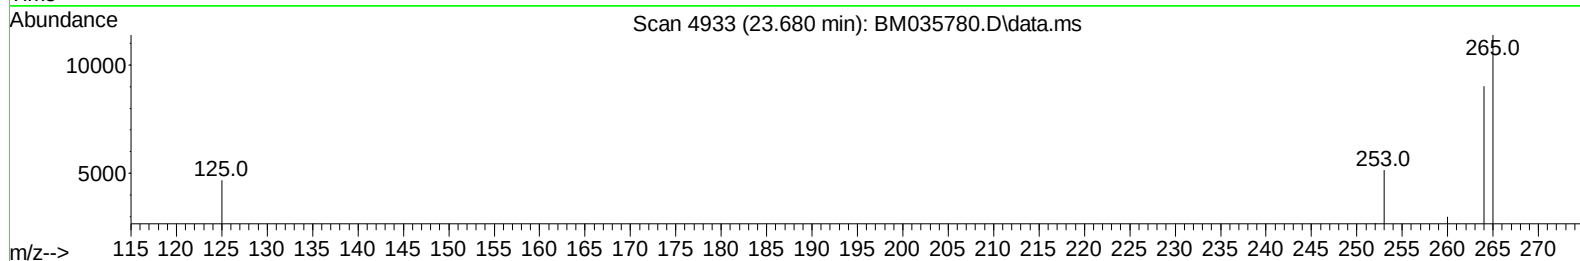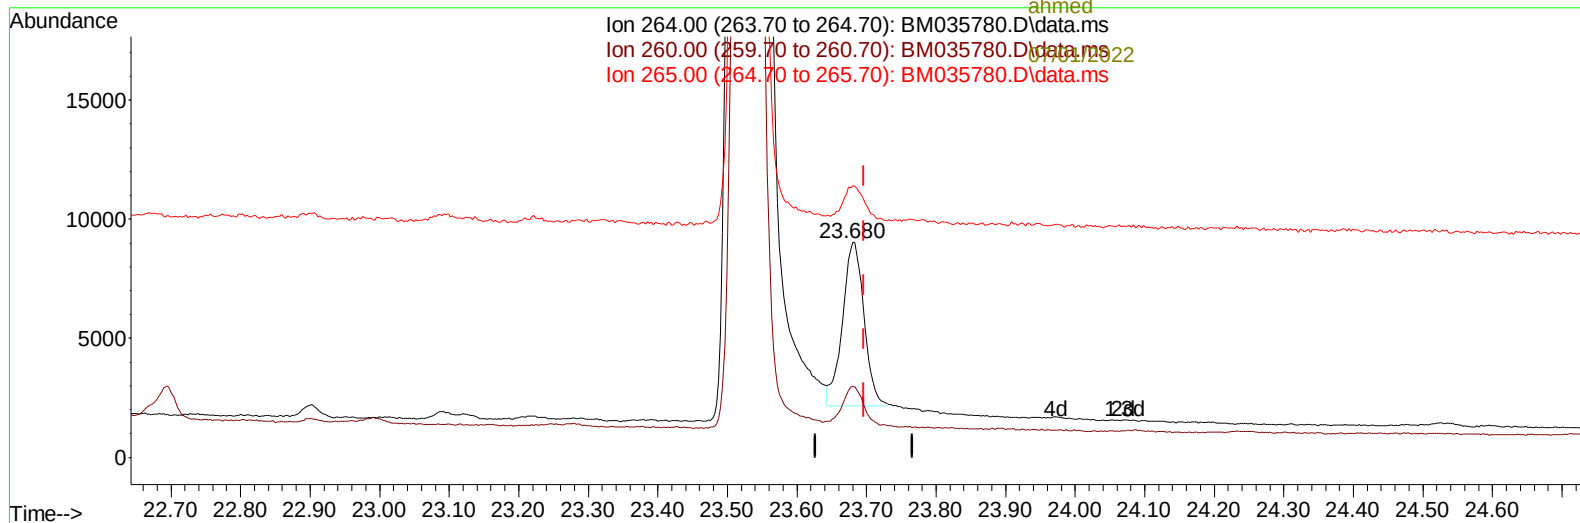

TIC: BM035780.D\data.ms

(23) Perylene-d12 (I)

23.680min (-0.017) 0.40 ng/ul m

response 14766

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	32.95#
265.00	119.70	126.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
 Data File : BM035780.D
 Acq On : 30 Jun 2022 14:19
 Operator : CG/JU
 Sample : N3375-08RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4T9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
 Upadhyay

07/01/2022
 Supervised By :mohammad
 ahmed

Quant Time: Jul 01 01:16:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----07/01/2022							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.774	152		3422m	0.400	ng/ul	-0.09
4) Naphthalene-d8	10.561	136		16487m	0.400	ng/ul	-0.06
9) Acenaphthene-d10	14.408	164		7623m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.157	188		13699m	0.400	ng/ul	-0.04
17) Chrysene-d12	21.360	240		16570m	0.400	ng/ul	-0.01
23) Perylene-d12	23.680	264		14766m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.213	96		22336	4.810	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.162	152		7526m	0.292	ng/ul	-0.07
18) Fluoranthene-d10	19.192	212		13356m	0.239	ng/ul	-0.02
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.247	88		42202m	9.188	ng/ul	
5) Naphthalene	10.611	128		42909m	0.851	ng/ul	
7) 2-Methylnaphthalene	12.233	142		14257m	0.452	ng/ul	
8) 1-Methylnaphthalene	12.448	142		11141m	0.373	ng/ul	
11) Acenaphthene	14.469	153		27459m	0.892	ng/ul	
12) Fluorene	15.459	166		26161m	0.738	ng/ul	
15) Phenanthrene	17.199	178		83832m	1.689	ng/ul	
16) Anthracene	17.292	178		60378m	1.464	ng/ul	
19) Fluoranthene	19.224	202		20528m	0.247	ng/ul	
20) Pyrene	19.587	202		12824m	0.138	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM063022\
Data File : BM035780.D
Acq On : 30 Jun 2022 14:19
Operator : CG/JU
Sample : N3375-08RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4T9

Manual IntegrationsAPPROVED

Quant Time: Jul 01 01:16:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:48:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

07/01/2022
Supervised By :mohammad
ahmed

