

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070115\
 Data File : BM001809.D
 Acq On : 01 Jul 2015 16:00
 Operator : TP/UM
 Sample : G2854-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FB7

Quant Time: Jul 02 07:09:59 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 02 07:09:03 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	60043	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	242692	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	146945	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	333962	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	414003	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	431515	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	861	0.68	ng/uL	0.00
5) Phenol-d5	6.83	99	16256	3.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	31922	12.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	38469	10.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	26675	7.21	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	19612	11.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	21918	11.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	43173	10.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	9396	2.35	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	127292	11.68	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	164629	11.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	4447	2.21	ng/ul	0.00
57) Fluorene-d10	15.31	176	124109	12.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	17337	8.50	ng/ul	0.00
70) Anthracene-d10	17.16	188	184059	11.83	ng/ul	0.00
78) Pyrene-d10	19.46	212	206669	11.79	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	195574	10.28	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.77	163	77445	6.50	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070115\
Data File : BM001809.D
Acq On : 01 Jul 2015 16:00
Operator : TP/UM
Sample : G2854-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FB7

Quant Time: Jul 02 07:09:59 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 02 07:09:03 2015
Response via : Initial Calibration

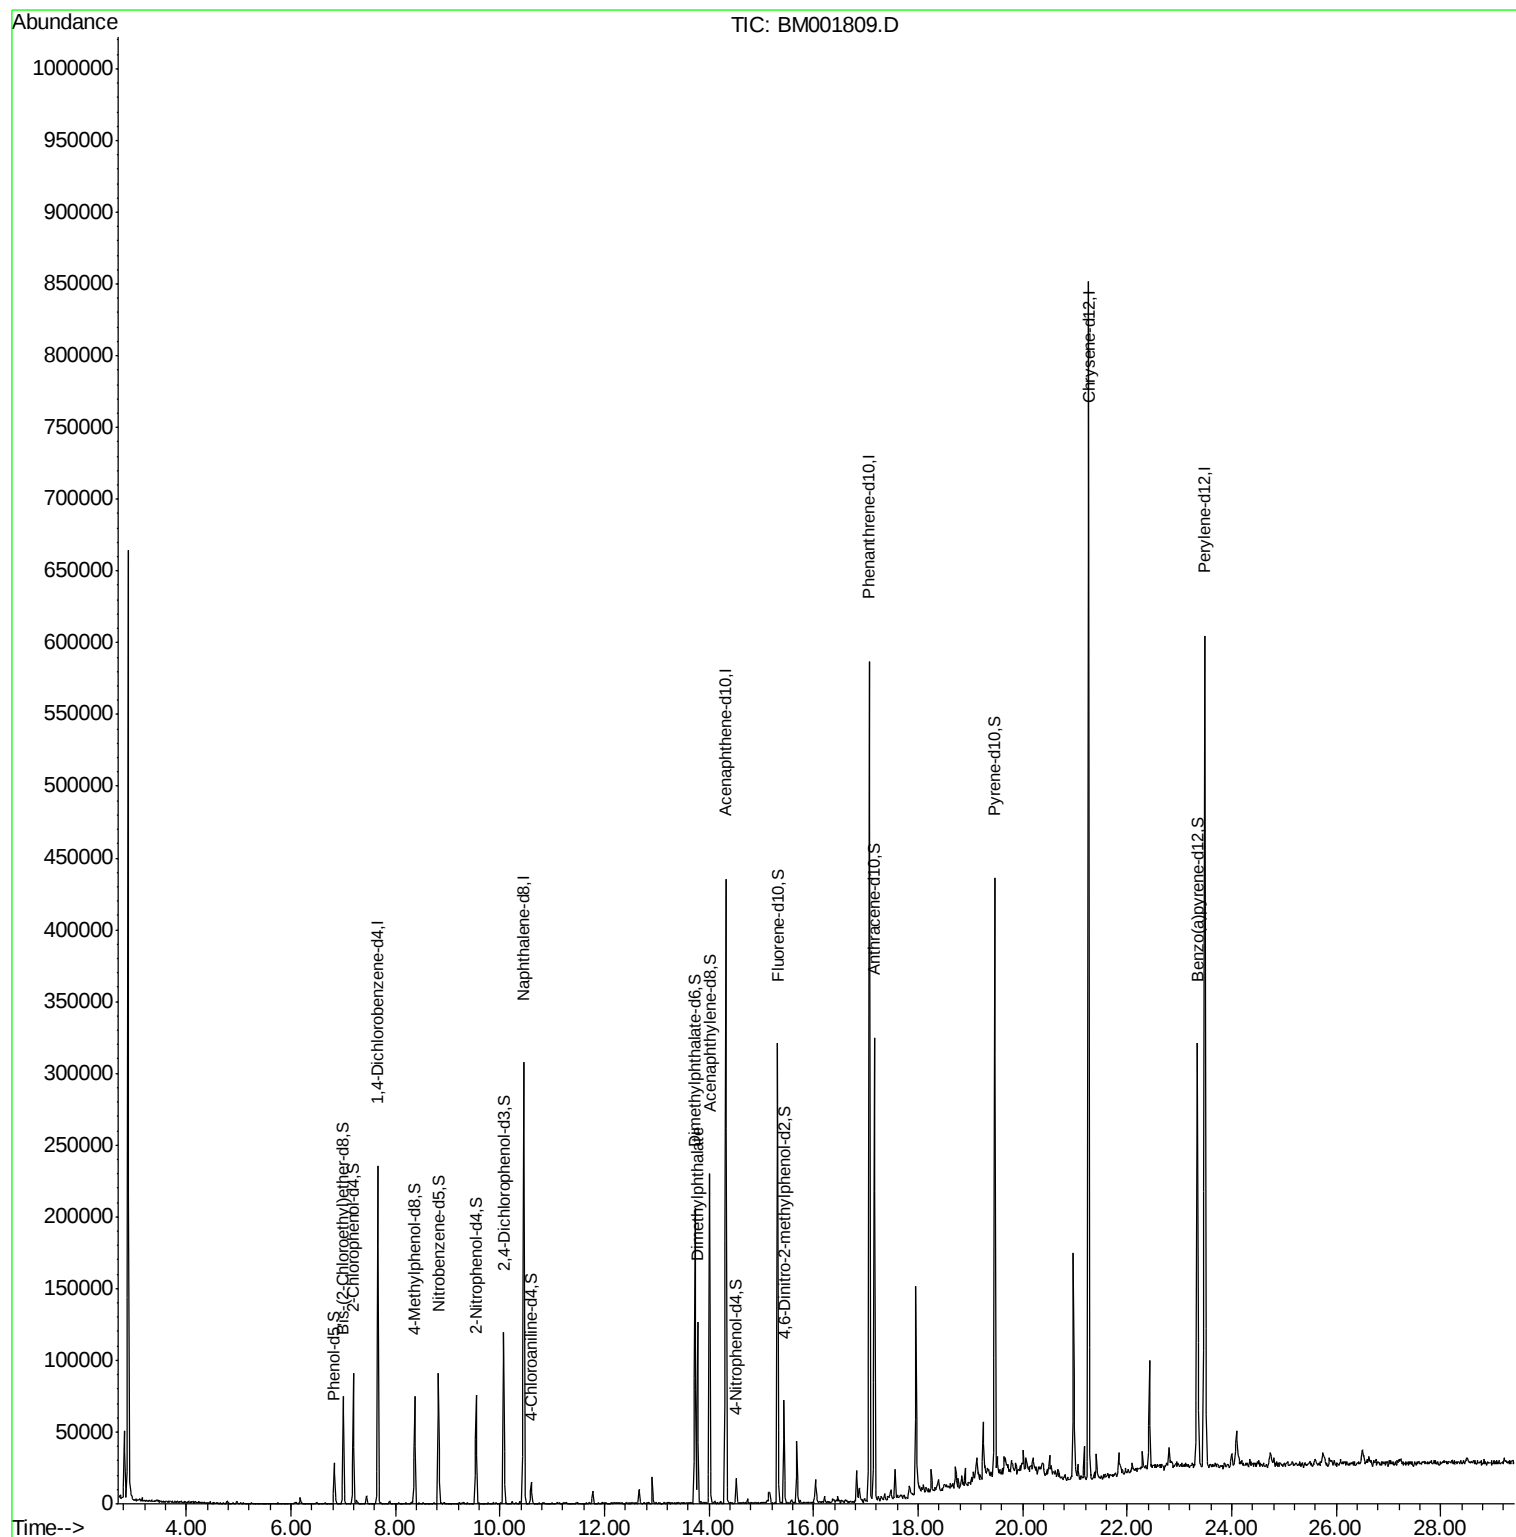

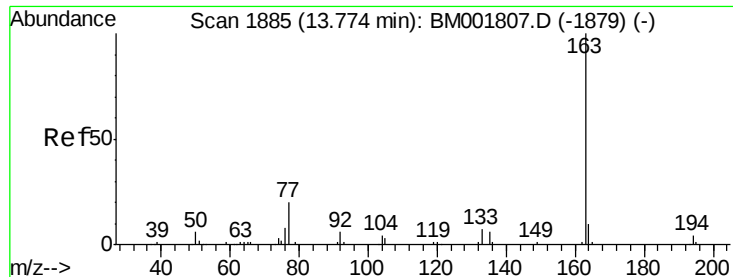

#44

Dimethylphthalate

Concen: 6.50 ng/ul

RT: 13.77 min Scan# 1885

Delta R.T. 0.00 min

Lab File: BM001809.D


Acq: 01 Jul 2015 16:00

Instrument :

BNA_M

ClientSampleId :

H0FB7

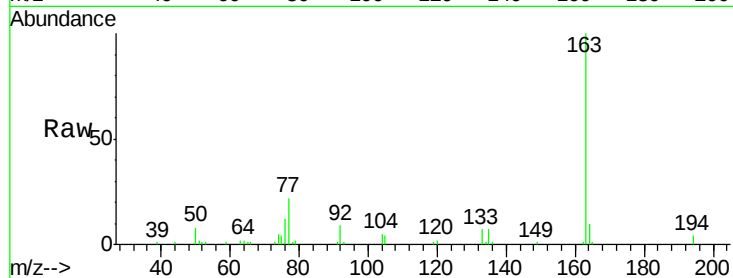

Tgt Ion:163 Resp: 77445

Ion Ratio Lower Upper

163 100

194 4.2 3.6 5.4

164 10.5 8.0 12.0

