

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070115\
 Data File : BM001812.D
 Acq On : 01 Jul 2015 17:49
 Operator : TP/UM
 Sample : G2854-04MSD
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FC2MSD

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.734	6	8	10	rVB2	1855	1454	0.12%	0.008%
2	2.810	17	21	29	rBV	48973	70314	5.66%	0.390%
3	2.881	29	33	50	rVB	544161	628914	50.63%	3.490%
4	3.140	75	77	82	rBV2	3019	3248	0.26%	0.018%
5	3.875	198	202	206	rVB3	1740	2322	0.19%	0.013%
6	4.210	258	259	263	rBV	1172	1281	0.10%	0.007%
7	6.828	699	704	706	rBV	44386	69227	5.57%	0.384%
8	6.851	706	708	715	rVB	51351	67660	5.45%	0.375%
9	6.998	726	733	740	rBB	144058	218489	17.59%	1.212%
10	7.192	759	766	768	rBV	168064	256840	20.68%	1.425%
11	7.222	768	771	779	rVB	175882	267972	21.57%	1.487%
12	7.663	839	846	849	rBV	235554	393263	31.66%	2.182%
13	7.698	849	852	859	rVB	269747	390034	31.40%	2.164%
14	8.369	960	966	972	rVB	126601	193637	15.59%	1.074%
15	8.463	976	982	993	rBV	200416	307481	24.76%	1.706%
16	8.822	1035	1043	1051	rBV	186573	300788	24.22%	1.669%
17	9.539	1159	1165	1171	rBB	159195	249516	20.09%	1.385%
18	10.069	1249	1255	1262	rBV	247796	387196	31.17%	2.149%
19	10.316	1290	1297	1305	rBB	315256	500511	40.30%	2.777%
20	10.451	1313	1320	1328	rBB	319082	505155	40.67%	2.803%
21	10.592	1341	1344	1348	rVB2	1541	2078	0.17%	0.012%
22	10.827	1383	1384	1389	rVB2	1231	1338	0.11%	0.007%
23	11.739	1532	1539	1548	rBV	239973	373345	30.06%	2.072%
24	12.657	1691	1695	1700	rVB3	4459	6260	0.50%	0.035%
25	12.916	1734	1739	1743	rBV2	7833	10725	0.86%	0.060%
26	13.727	1871	1877	1882	rBV	416479	567991	45.73%	3.152%
27	13.774	1882	1885	1892	rVB	22553	27948	2.25%	0.155%
28	14.010	1918	1925	1932	rBV	498011	716230	57.66%	3.974%
29	14.316	1971	1977	1983	rBV2	435910	667947	53.78%	3.706%
30	14.380	1983	1988	1995	rVB	595973	834435	67.18%	4.630%
31	14.521	2006	2012	2019	rVB3	55051	102180	8.23%	0.567%
32	14.686	2034	2040	2046	rVB	303765	396695	31.94%	2.201%
33	15.145	2115	2118	2120	rBV	2370	2795	0.23%	0.016%
34	15.168	2120	2122	2125	rVB2	2351	1685	0.14%	0.009%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070115\
 Data File : BM001812.D
 Acq On : 01 Jul 2015 17:49
 Operator : TP/UM
 Sample : G2854-04MSD
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0FC2MSD

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Title : SVOA CALIBRATION

35	15.310	2140	2146	2154	rVB	645899	907357	73.05%	5.035%
36	15.433	2161	2167	2174	rVB	191863	253121	20.38%	1.405%
37	16.033	2265	2269	2276	rVB2	4775	8032	0.65%	0.045%
38	16.209	2297	2299	2302	rBV2	1733	1606	0.13%	0.009%
39	16.709	2379	2384	2394	rBV	349520	466361	37.55%	2.588%
40	16.821	2399	2403	2406	rVV	6947	8161	0.66%	0.045%
41	16.874	2406	2412	2416	rVB3	4107	6724	0.54%	0.037%
42	17.062	2438	2444	2450	rBV2	606759	809044	65.14%	4.489%
43	17.162	2455	2461	2468	rVB	714098	994886	80.10%	5.521%
44	17.351	2489	2493	2495	rBV3	2284	2817	0.23%	0.016%
45	17.439	2506	2508	2511	rBV2	1070	1427	0.11%	0.008%
46	17.474	2511	2514	2519	rVB4	3229	5296	0.43%	0.029%
47	17.556	2524	2528	2533	rVB	9754	12434	1.00%	0.069%
48	17.627	2536	2540	2542	rBV2	1233	1869	0.15%	0.010%
49	17.651	2542	2544	2546	rBV2	1718	1259	0.10%	0.007%
50	17.733	2555	2558	2559	rVB	2087	1734	0.14%	0.010%
51	17.827	2568	2574	2575	rBV2	2699	3368	0.27%	0.019%
52	17.874	2580	2582	2585	rVB	1288	1434	0.12%	0.008%
53	17.956	2591	2596	2600	rBV	61069	80921	6.51%	0.449%
54	18.033	2605	2609	2612	rVV	4229	7496	0.60%	0.042%
55	18.103	2616	2621	2624	rVV4	3365	6829	0.55%	0.038%
56	18.151	2627	2629	2631	rVV2	3109	3042	0.24%	0.017%
57	18.209	2634	2639	2642	rBV4	2752	4983	0.40%	0.028%
58	18.251	2642	2646	2650	rVB2	8955	10612	0.85%	0.059%
59	18.362	2661	2665	2666	rBV4	1795	2033	0.16%	0.011%
60	18.433	2676	2677	2680	rVB3	1863	1355	0.11%	0.008%
61	18.503	2686	2689	2694	rBV5	1663	2898	0.23%	0.016%
62	18.715	2721	2725	2730	rVB5	8697	12656	1.02%	0.070%
63	18.768	2732	2734	2739	rVB6	3027	3415	0.27%	0.019%
64	18.833	2742	2745	2752	rVB4	3982	5556	0.45%	0.031%
65	18.892	2752	2755	2759	rBV6	5326	6265	0.50%	0.035%
66	18.927	2759	2761	2764	rBV4	1535	1941	0.16%	0.011%
67	19.015	2774	2776	2779	rBV4	2260	2131	0.17%	0.012%
68	19.050	2780	2782	2784	rBV2	3701	3674	0.30%	0.020%
69	19.109	2789	2792	2797	rBV5	3934	6890	0.55%	0.038%
70	19.150	2797	2799	2801	rVB3	3194	2370	0.19%	0.013%
71	19.186	2803	2805	2808	rVB3	3596	2566	0.21%	0.014%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070115\
Data File : BM001812.D
Acq On : 01 Jul 2015 17:49
Operator : TP/UM
Sample : G2854-04MSD
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0FC2MSD

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Title : SVOA CALIBRATION

72	19.239	2809	2814	2822	rBV3	36843	58939	4.75%	0.327%
73	19.345	2830	2832	2833	rBV2	3577	2655	0.21%	0.015%
74	19.462	2846	2852	2854	rBV	879182	1242082	100.00%	6.892%
75	19.492	2854	2857	2863	rVB	955644	1175762	94.66%	6.524%
76	19.603	2874	2876	2878	rVB2	3599	2663	0.21%	0.015%
77	19.645	2879	2883	2886	rBV6	7194	11656	0.94%	0.065%
78	19.868	2918	2921	2926	rVB6	4975	5706	0.46%	0.032%
79	20.009	2943	2945	2949	rVB4	6293	4586	0.37%	0.025%
80	20.062	2952	2954	2959	rVB5	5329	8134	0.65%	0.045%
81	20.103	2959	2961	2965	rBV5	3152	3543	0.29%	0.020%
82	20.297	2992	2994	2995	rBV2	2998	1683	0.14%	0.009%
83	20.621	3047	3049	3052	rBV4	2575	2487	0.20%	0.014%
84	20.803	3076	3080	3083	rBV6	3623	5171	0.42%	0.029%
85	20.909	3097	3098	3100	rBV	3460	2681	0.22%	0.015%
86	20.933	3100	3102	3104	rBV4	4127	3690	0.30%	0.020%
87	20.962	3104	3107	3118	rVV6	17992	32531	2.62%	0.181%
88	21.044	3118	3121	3126	rVB2	7007	9032	0.73%	0.050%
89	21.115	3131	3133	3134	rVB2	2928	1291	0.10%	0.007%
90	21.168	3139	3142	3145	rVB3	3066	4233	0.34%	0.023%
91	21.250	3151	3156	3163	rBV	840797	1019435	82.07%	5.657%
92	21.797	3247	3249	3252	rBV3	2978	3868	0.31%	0.021%
93	21.939	3272	3273	3275	rVB2	3378	1454	0.12%	0.008%
94	22.738	3406	3409	3410	rBV3	4542	4603	0.37%	0.026%
95	23.333	3503	3510	3523	rVB2	678415	1202066	96.78%	6.670%
96	23.474	3527	3534	3543	rVB2	562635	1029928	82.92%	5.715%


Sum of corrected areas: 18021396

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070115\
Data File : BM001812.D
Acq On : 01 Jul 2015 17:49
Operator : TP/UM
Sample : G2854-04MSD
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
H0FC2MSD

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

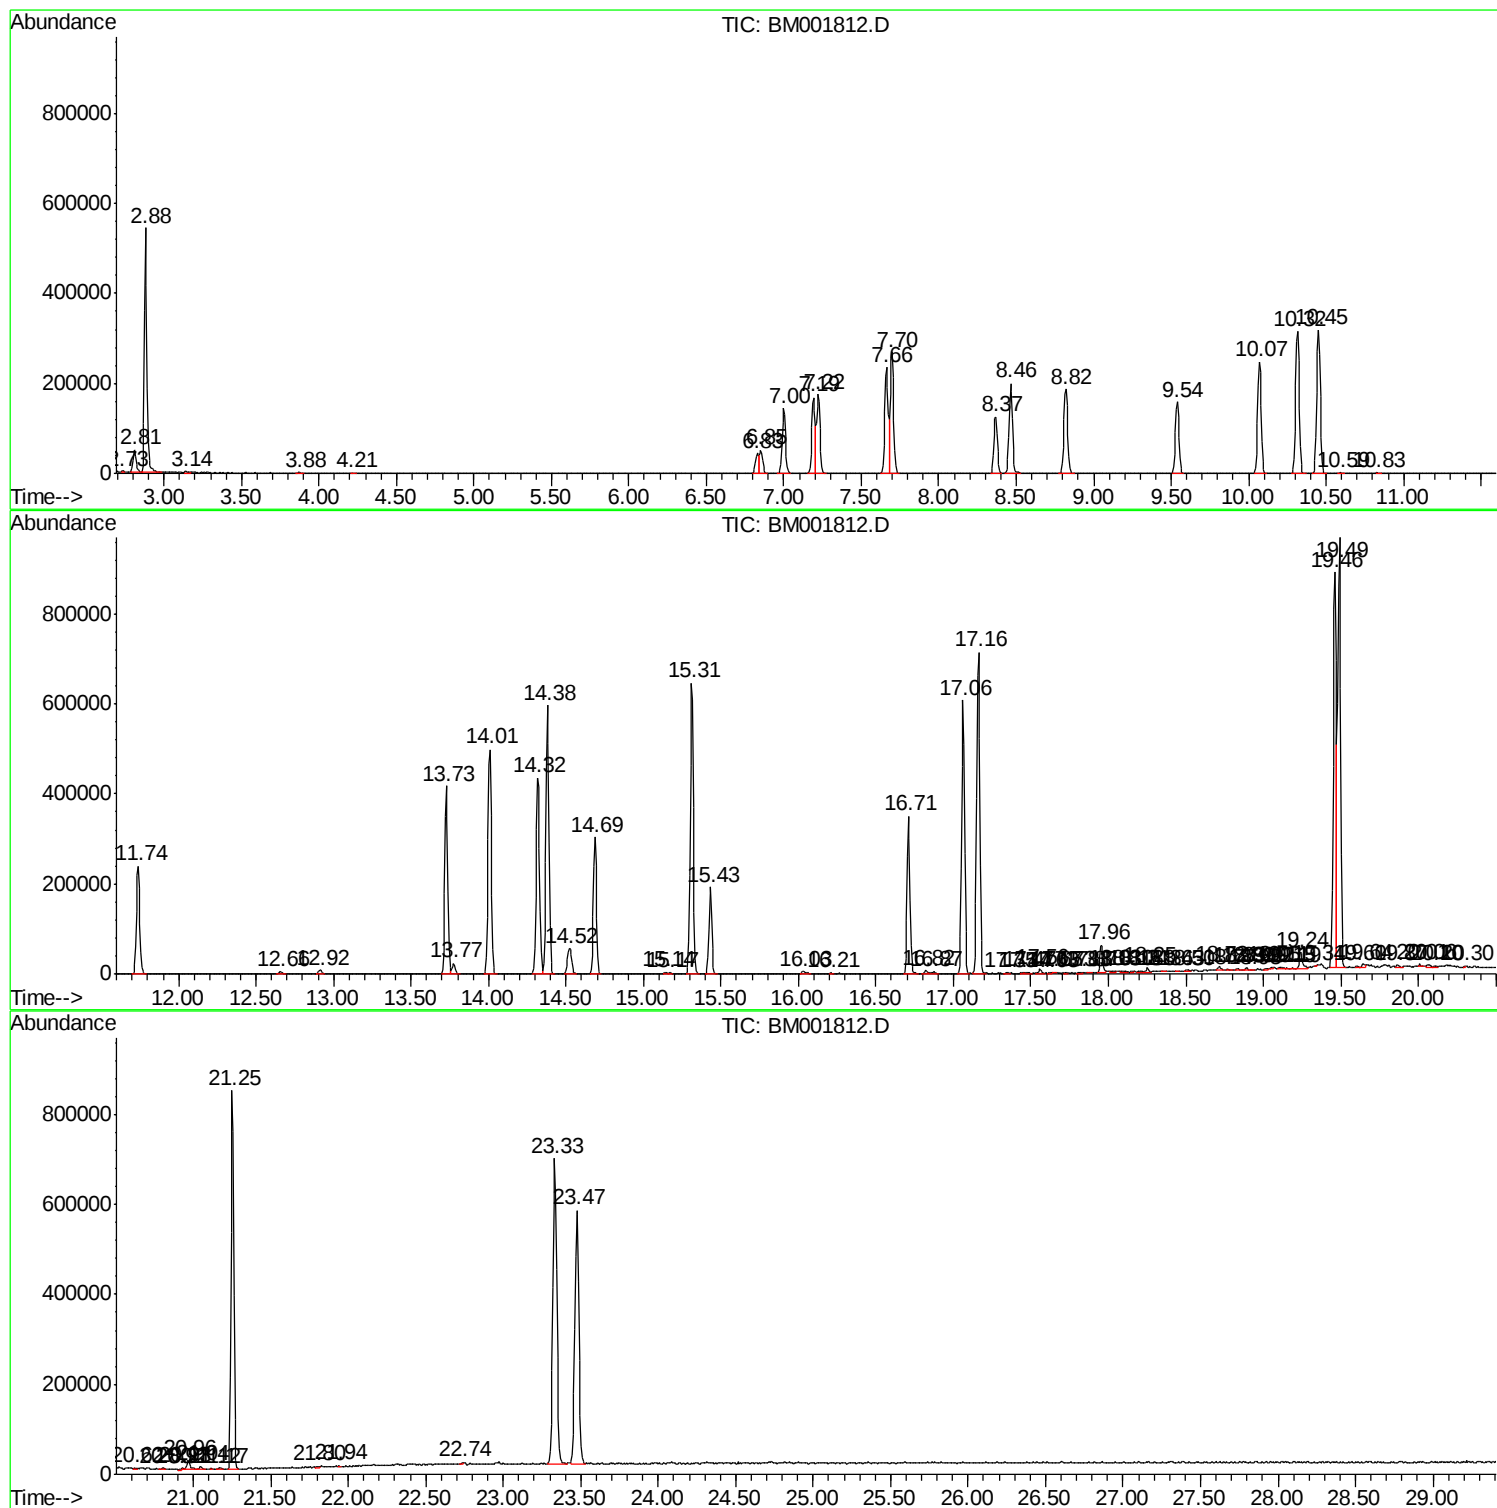

DaaaPathh::ZZ\NRPBMM1BNAAMMDAAAB0000155\
DaaaFile::B0008822DD
AeqqOn ::001JUW120055 177409
Opeaor ::TPPMM
Sample ::G0285400MDD
Misc ::
ASSVal ::77 SampleMultiplier:11

Instrument :
BNA_M
ClientSampleId :
H0FC2MSD

QqantMebdd::ZZ\NRPBMM1BNAAMMEEH00SS0000222EPAB0006555MM
QqantTitle ::SUACALIBRATION

TICLibrary :CC\DATA\BASSENDS002LL
TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc

No Library Search Compounds Detected
