


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070115\
Data File : BM001806.D
Acq On : 01 Jul 2015 10:18
Operator : TP/UM
Sample : DFTPP66
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP66

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM013015.M
Title : SVOA CALIBRATION
Last Update : Fri Jan 30 14:05:47 2015

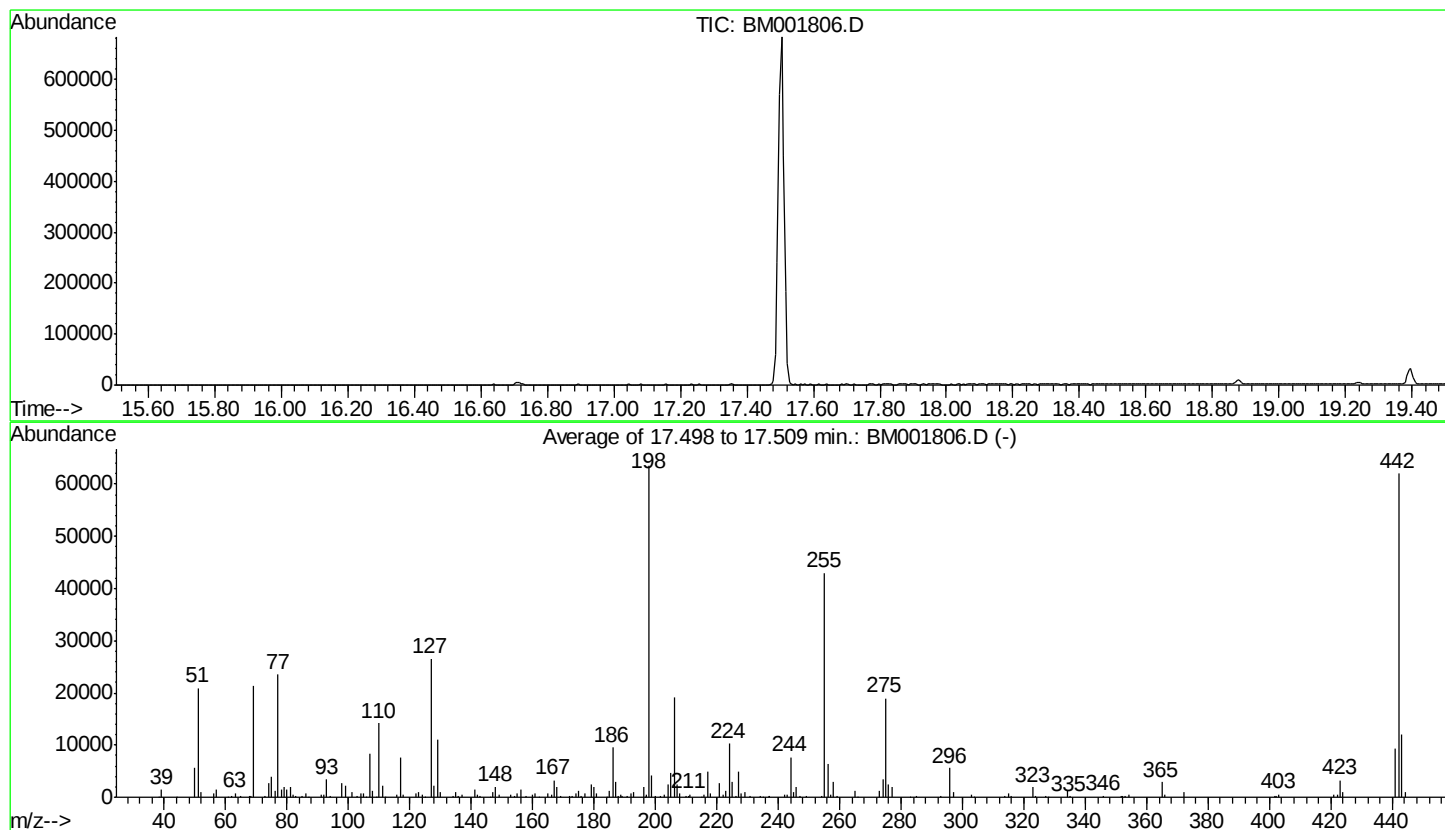

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	20917	PASS
68	69	0.00	2	1.5	312	PASS
69	198	0.00	100	33.7	21389	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	26557	PASS
197	198	0.00	2	0.8	503	PASS
198	198	100	100	100.0	63557	PASS
199	198	5	9	6.7	4243	PASS
275	198	10	60	29.9	18984	PASS
365	198	1	100	4.6	2919	PASS
441	443	0.01	100	76.6	9283	PASS
442	198	50	100	97.6	62053	PASS
443	442	15	24	19.5	12116	PASS

m/z	Abundance
38.00	308.0
39.10	1665.0
44.00	1114.0
50.00	6860.0
51.00	24544.0
52.00	1114.0
56.00	892.0
57.00	1460.0
60.90	312.0
61.90	400.0
63.10	856.0
65.10	376.0
67.90	520.0
69.00	25432.0
73.10	332.0
74.00	3010.0
75.00	4878.0
76.00	1251.0
77.10	26400.0
78.00	1808.0
79.00	2241.0
79.90	1637.0
81.00	2376.0
82.00	739.0
83.00	521.0
85.00	348.0
85.90	825.0
91.00	489.0
91.90	641.0
93.00	3706.0
94.00	312.0
98.00	3105.0
99.00	2607.0
100.90	1036.0
103.00	453.0
104.00	967.0
105.10	797.0
107.00	9729.0
108.00	1479.0
110.00	15316.0
111.00	2330.0
111.90	326.0
115.90	733.0
117.00	8656.0
118.00	693.0
121.90	635.0
122.90	903.0
124.00	530.0
127.00	29232.0
128.00	2363.0
129.00	12412.0
130.00	973.0
133.90	488.0
135.00	901.0
137.10	658.0
141.00	1847.0
141.90	558.0
142.90	436.0
147.00	942.0
148.00	2363.0
149.00	590.0
153.00	547.0
154.00	331.0
154.90	842.0
156.00	1496.0
158.00	344.0
159.90	540.0
161.00	784.0
162.00	307.0
165.00	836.0
166.10	593.0
167.00	3707.0
168.00	2025.0
168.90	414.0
171.90	435.0
173.00	449.0
173.90	758.0
175.00	1396.0
176.00	314.0
176.90	818.0
179.00	2666.0
180.00	1939.0
180.90	830.0
184.90	1365.0
186.00	9891.0
187.00	2949.0
188.10	350.0
188.90	835.0
190.90	504.0
191.90	747.0
193.10	761.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

196.10	1912.0
196.70	308.0
197.10	410.0
198.00	65712.0
198.90	4628.0
200.10	421.0
201.50	389.0
203.00	517.0
204.00	2552.0
205.00	4766.0
206.00	19744.0
207.00	2964.0
207.90	876.0
210.80	628.0
216.10	367.0
217.00	5030.0
218.00	598.0
221.00	2756.0
222.00	598.0
222.90	1194.0
224.00	10611.0
225.00	2831.0
226.10	309.0
227.00	4627.0
228.00	642.0
228.90	778.0
231.00	417.0
234.00	448.0
234.90	381.0
236.90	463.0
242.00	412.0
243.00	470.0
244.10	6919.0
245.10	1026.0
246.00	1723.0
247.00	306.0
249.00	343.0
254.10	417.0
255.00	39440.0
256.10	5827.0
257.00	457.0
258.00	2401.0
264.90	931.0
265.80	308.0
273.00	974.0
274.00	3240.0
275.00	17400.0
276.00	2068.0
277.00	1977.0
293.00	393.0
296.00	5545.0
297.10	922.0
303.00	477.0
313.90	308.0
314.90	621.0
323.00	1442.0
324.00	341.0
333.90	916.0
346.00	374.0
351.90	434.0
353.00	432.0
354.10	539.0
365.00	2212.0
366.10	402.0
372.10	696.0
403.00	537.0
421.00	330.0
422.00	436.0
423.10	2228.0
424.00	943.0
441.00	6972.0
442.10	47720.0
443.00	9470.0
444.10	778.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

m/z	Abundance
39.10	1807.0
44.00	952.0
50.00	6521.0
51.10	24448.0
52.00	1200.0
56.00	578.0
57.00	1644.0
62.00	445.0
63.00	1103.0
64.90	460.0
68.10	572.0
69.00	24176.0
72.90	336.0
74.00	3340.0
75.10	4377.0
76.10	1452.0
77.10	27440.0
78.10	1701.0
79.00	2067.0
80.00	2017.0
81.00	2112.0
82.00	621.0
83.00	489.0
85.00	437.0
86.00	814.0
87.00	309.0
90.90	551.0
92.00	782.0
93.00	3950.0
94.00	327.0
98.00	3314.0
98.90	2570.0
101.00	1289.0
103.00	386.0
103.90	752.0
105.00	809.0
105.90	302.0
107.00	10038.0
108.00	1557.0
109.00	339.0
110.00	17304.0
111.00	2522.0
115.90	569.0
117.00	9037.0
118.00	764.0
122.00	747.0
122.90	1088.0
124.00	665.0
125.00	387.0
127.00	31088.0
128.00	2624.0
129.00	13029.0
130.00	1157.0
133.90	401.0
135.00	1231.0
135.90	426.0
137.10	719.0
141.00	1908.0
142.00	471.0
142.90	567.0
146.10	353.0
147.00	1026.0
148.00	2104.0
149.10	486.0
153.00	721.0
153.90	558.0
155.00	1066.0
156.00	1449.0
157.90	452.0
159.90	719.0
160.90	807.0
165.00	744.0
166.00	609.0
167.00	3688.0
168.00	2267.0
171.90	323.0
173.00	397.0
174.00	881.0
175.00	1571.0
175.90	410.0
177.00	710.0
179.00	3043.0
180.00	2324.0
180.90	674.0
183.90	309.0
184.90	1289.0
186.00	10980.0
187.00	3726.0
189.10	982.0
192.00	932.0
193.00	1181.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

196.00	2090.0
197.10	622.0
198.00	75072.0
198.90	4882.0
199.90	517.0
201.60	328.0
203.00	656.0
204.00	3038.0
205.00	5676.0
206.00	22128.0
207.00	3186.0
207.90	956.0
210.00	401.0
211.00	1005.0
215.00	309.0
215.90	491.0
216.90	6092.0
218.10	901.0
221.00	3143.0
221.90	917.0
223.00	1409.0
224.00	12042.0
225.00	3319.0
226.00	478.0
227.00	5905.0
228.00	845.0
229.00	1199.0
230.90	359.0
233.90	390.0
237.10	537.0
242.00	592.0
242.90	492.0
244.00	9666.0
245.00	1232.0
246.00	2406.0
246.90	389.0
248.90	406.0
254.10	371.0
255.00	53080.0
256.00	7621.0
257.00	556.0
258.00	3658.0
259.00	363.0
265.00	1537.0
273.00	1437.0
274.00	4390.0
275.00	22824.0
276.00	3091.0
277.00	2361.0
282.90	340.0
285.00	565.0
293.00	392.0
296.00	6295.0
297.00	1161.0
303.00	703.0
303.90	371.0
313.90	345.0
315.00	741.0
315.90	469.0
323.00	2495.0
323.90	420.0
327.00	471.0
328.00	300.0
334.00	1401.0
334.90	306.0
346.00	619.0
352.10	560.0
353.00	562.0
354.00	750.0
365.00	3678.0
366.00	378.0
372.00	1061.0
401.90	484.0
403.10	624.0
421.00	479.0
422.10	574.0
423.10	4047.0
423.90	926.0
441.10	11323.0
442.10	76704.0
443.10	15004.0
444.10	1235.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

m/z	Abundance
39.10	855.0
44.00	858.0
50.10	3599.0
51.10	13760.0
51.90	591.0
56.00	560.0
57.00	1183.0
63.00	548.0
68.20	365.0
69.00	14559.0
74.00	1601.0
75.00	2458.0
76.00	918.0
77.10	16696.0
78.00	1129.0
79.00	1272.0
80.00	1013.0
81.00	1457.0
81.90	357.0
85.90	397.0
90.90	396.0
92.00	441.0
93.00	2416.0
98.00	1927.0
99.00	1362.0
101.00	724.0
104.00	498.0
105.00	448.0
107.00	5498.0
108.00	1036.0
110.00	10068.0
111.00	1480.0
115.90	337.0
117.00	5189.0
118.00	385.0
122.00	560.0
123.00	738.0
124.00	343.0
127.00	19352.0
128.10	1537.0
129.00	7753.0
129.90	644.0
135.00	710.0
137.10	448.0
140.90	1033.0
142.00	469.0
147.00	779.0
147.90	1546.0
149.00	302.0
153.00	413.0
155.00	654.0
156.00	1191.0
159.90	371.0
160.90	579.0
164.90	684.0
166.00	310.0
167.00	2264.0
168.00	1397.0
174.00	385.0
175.00	996.0
177.00	555.0
179.00	1954.0
180.10	1558.0
181.00	586.0
185.00	1017.0
186.00	7813.0
187.00	2132.0
188.00	403.0
188.90	631.0
192.00	674.0
193.00	855.0
196.00	1644.0
197.10	477.0
197.90	49888.0
198.90	3219.0
203.00	390.0
204.00	1809.0
205.00	3630.0
206.00	15548.0
207.10	2096.0
208.00	721.0
211.00	572.0
215.90	408.0
216.90	3483.0
217.90	530.0
220.90	2193.0
223.00	1036.0
224.10	8265.0
225.10	2497.0
227.00	3965.0
228.00	494.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

229.00	758.0
237.00	336.0
242.00	419.0
243.00	596.0
244.00	6312.0
245.00	812.0
246.00	1566.0
255.00	36320.0
256.00	5370.0
257.00	428.0
257.90	2497.0
258.90	368.0
264.90	934.0
272.90	1250.0
274.00	2769.0
275.00	16728.0
276.00	2235.0
277.00	1626.0
292.90	310.0
296.00	4925.0
297.00	692.0
303.10	641.0
315.00	524.0
323.10	1613.0
327.00	322.0
334.10	1069.0
334.90	326.0
352.10	397.0
354.20	410.0
365.00	2867.0
366.10	416.0
372.00	1100.0
402.10	401.0
403.00	606.0
421.00	400.0
422.00	428.0
423.00	3308.0
424.00	882.0
441.10	9556.0
442.10	61736.0
443.10	11875.0
444.10	1277.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66

m/z	Abundance
44.00	893.0
207.00	301.0

Instrument :
BNA_M
ClientSampleId :
DFTPP66