

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070116\
 Data File : BM006179.D
 Acq On : 01 Jul 2016 13:02
 Operator : UM/SJ
 Sample : H3780-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YF9

Quant Time: Jul 01 17:32:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 29 00:57:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	349072	20.00	ng/ul	0.01
7) Naphthalene-d8	10.45	136	1572371	20.00	ng/ul	0.01
15) Acenaphthene-d10	14.32	164	884897	20.00	ng/ul	0.01
23) Phenanthrene-d10	17.07	188	1931125	20.00	ng/ul	0.02
29) Chrysene-d12	21.27	240	1435264	20.00	ng/ul	0.02
34) Perylene-d12	23.50	264	1471482	20.00	ng/ul	0.04

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	5645	0.75	ng/uL	0.00
3) Phenol-d5	6.85	99	524746	18.40	ng/ul	0.02
4) Bis-(2-Chloroethyl)ether-d	7.00	67	298252	17.74	ng/ul	0.00
5) 2-Chlorophenol-d4	7.20	132	388539	17.75	ng/ul	0.01
6) 4-Methylphenol-d8	8.37	113	436726	19.03	ng/ul	0.01
8) Nitrobenzene-d5	8.82	128	206652	19.51	ng/ul	0.01
9) 2-Nitrophenol-d4	9.53	143	240895	19.87	ng/ul	0.01
10) 2,4-Dichlorophenol-d3	10.07	165	426867	19.30	ng/ul	0.02
12) 4-Chloroaniline-d4	10.59	131	304909	17.44	ng/ul	0.01
16) Dimethylphthalate-d6	13.73	166	1278999	20.16	ng/ul	0.01
17) Acenaphthylene-d8	14.00	160	1631450	21.19	ng/ul	0.01
20) 4-Nitrophenol-d4	14.54	143	236049	19.61	ng/ul	0.03
21) Fluorene-d10	15.31	176	1118332	20.66	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.45	200	165557	24.20	ng/ul	0.02
26) Anthracene-d10	17.16	188	1684261	21.74	ng/ul	0.01
30) Pyrene-d10	19.47	212	1582518	27.38	ng/ul	0.02
37) Benzo(a)pyrene-d12	23.36	264	1251420	21.37	ng/ul	0.04

Target Compounds


						Qvalue
18) Acenaphthylene	14.03	152	93734	1.16	ng/ul#	94
25) Phenanthrene	17.11	178	792933	8.68	ng/ul	100
27) Anthracene	17.20	178	255250	2.72	ng/ul	100
28) Fluoranthene	19.13	202	1694744	15.14	ng/ul	99
31) Pyrene	19.50	202	1530608	20.22	ng/ul	96
32) Benzo(a)anthracene	21.25	228	799605	10.71	ng/ul	97
33) Chrysene	21.30	228	887484	12.92	ng/ul	97
35) Benzo(b)fluoranthene	22.83	252	1317166	17.25	ng/ul	97
36) Benzo(k)fluoranthene	22.83	252	1317166	18.39	ng/ul	98
38) Benzo(a)pyrene	23.40	252	829222	11.49	ng/ul	97
39) Indeno(1,2,3-cd)pyrene	25.74	276	643689	8.58	ng/ul#	94
40) Dibenzo(a,h)anthracene	25.74	278	202070	3.26	ng/ul#	68
41) Benzo(g,h,i)perylene	26.43	276	637203	10.15	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070116\
Data File : BM006179.D
Acq On : 01 Jul 2016 13:02
Operator : UM/SJ
Sample : H3780-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9YF9

Quant Time: Jul 01 17:32:17 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 29 00:57:09 2016
Response via : Initial Calibration

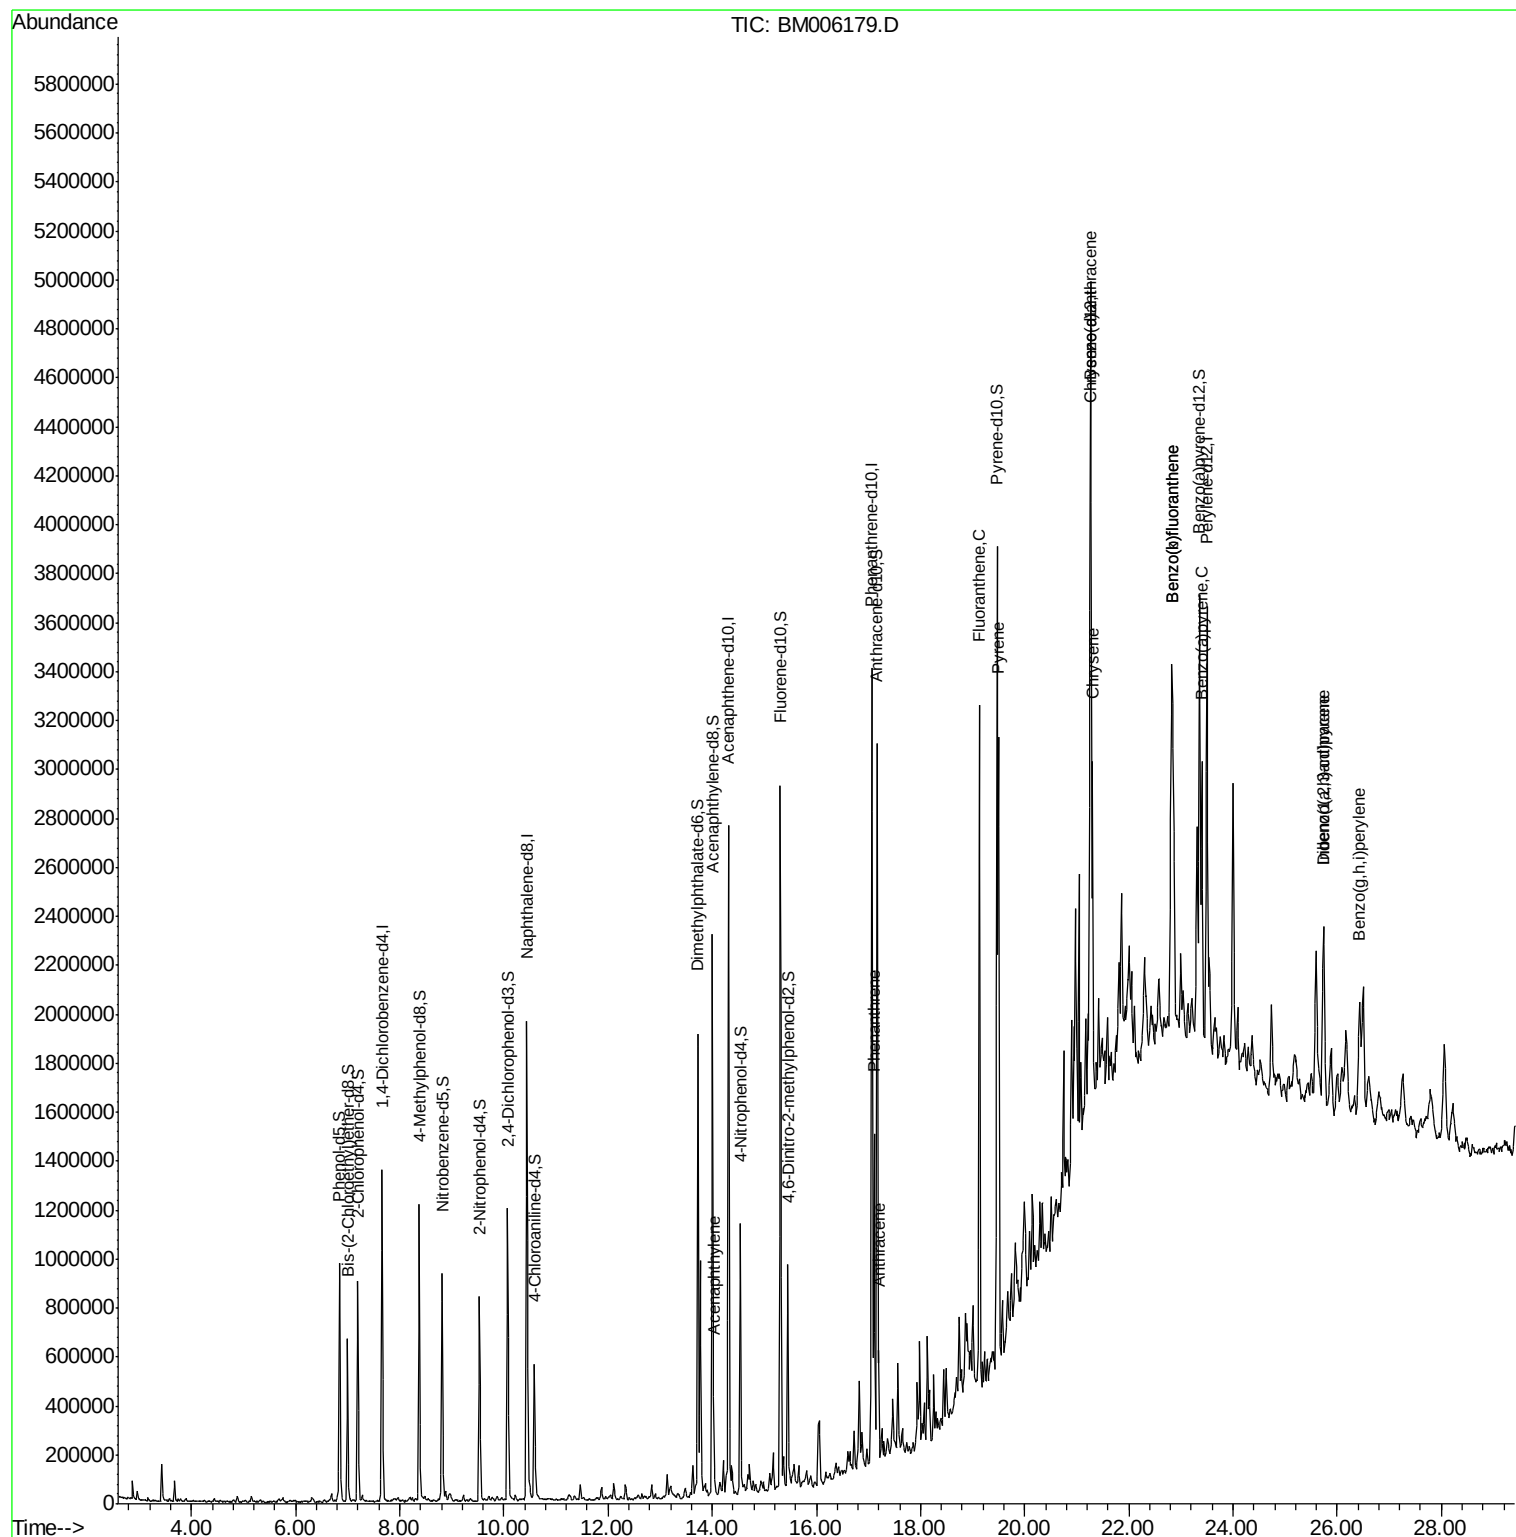

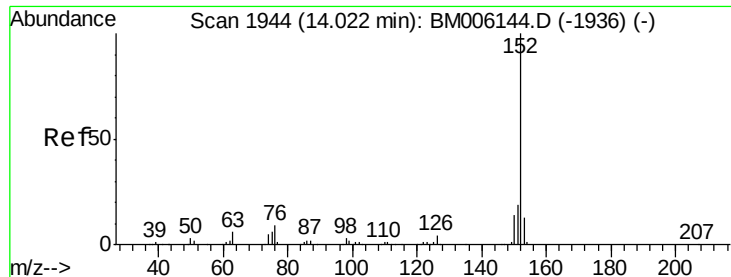

#18

Acenaphthylene

Concen: 1.16 ng/ul

RT: 14.03 min Scan# 1946

Delta R.T. 0.01 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02

Instrument :

BNA_M

ClientSampleId :

D9YF9


Tgt Ion:152 Resp: 93734

Ion Ratio Lower Upper

152 100

151 21.5 15.8 23.6




153 16.4 10.3 15.5#

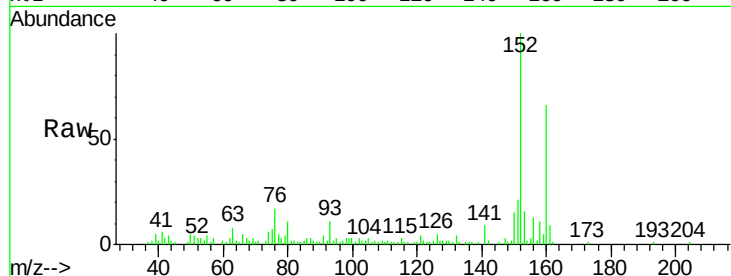

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

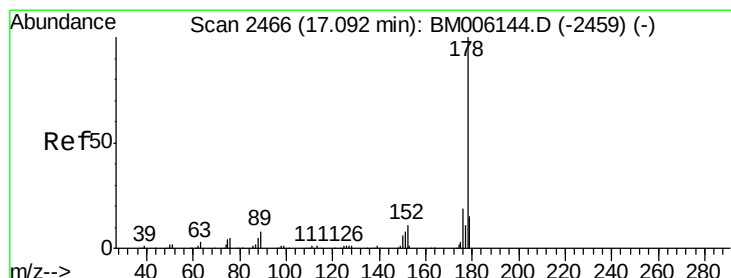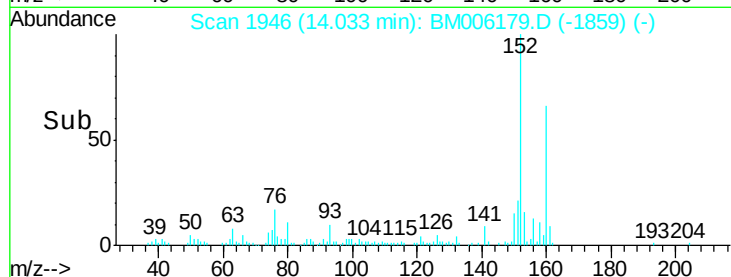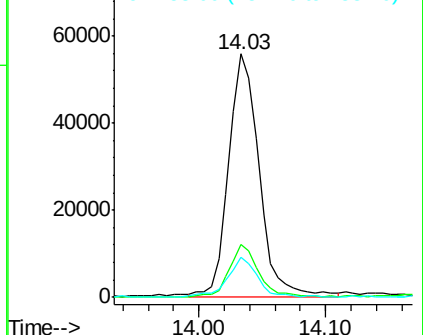

#25

Phenanthrene

Concen: 8.68 ng/ul

RT: 17.11 min Scan# 2469

Delta R.T. 0.02 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02


Tgt Ion:178 Resp: 792933

Ion Ratio Lower Upper

178 100

179 15.2 12.2 18.2



176 19.0 15.3 22.9

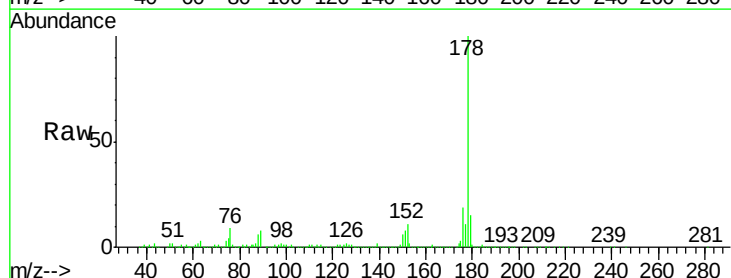


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

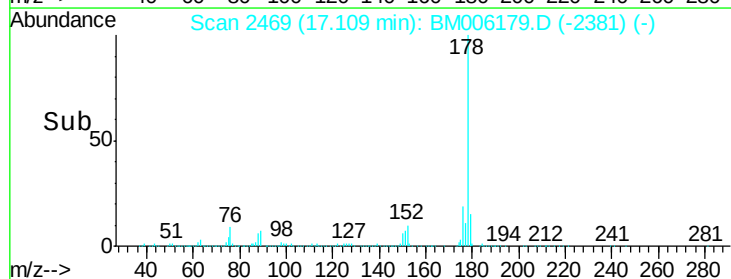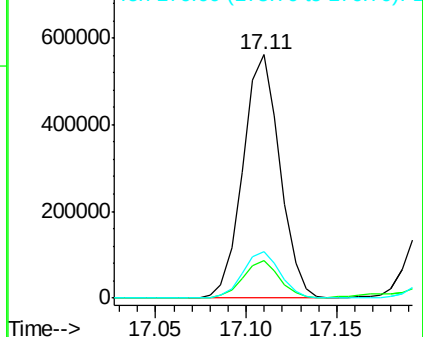

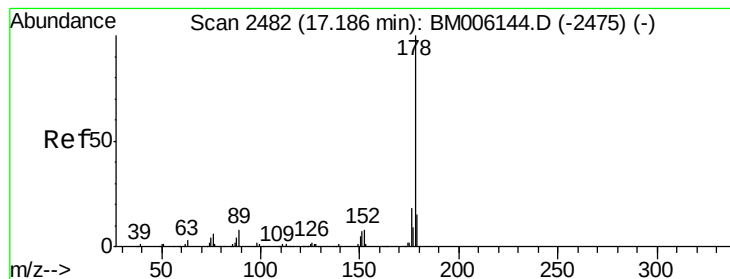

#27

Anthracene

Concen: 2.72 ng/ul

RT: 17.20 min Scan# 2484

Delta R.T. 0.01 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02

Instrument :

BNA_M

ClientSampleId :

D9YF9


Tgt Ion:178 Resp: 255250

Ion Ratio Lower Upper

178 100

179 15.6 12.3 18.5




176 18.3 14.6 22.0

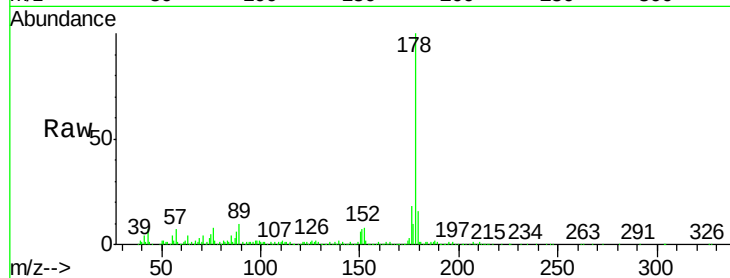

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

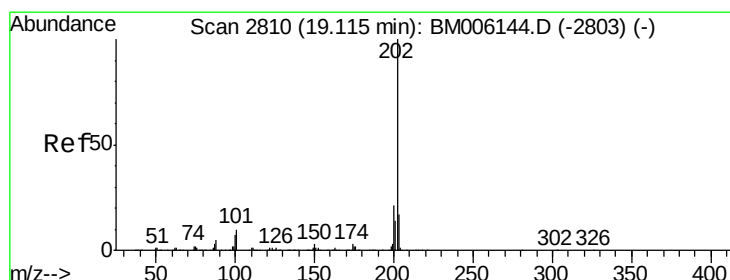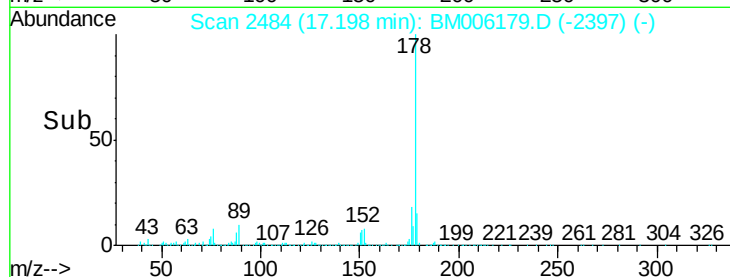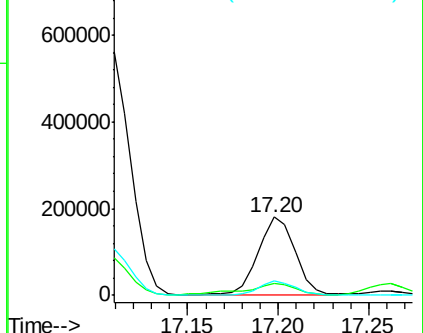

#28

Fluoranthene

Concen: 15.14 ng/ul

RT: 19.13 min Scan# 2813

Delta R.T. 0.02 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02


Tgt Ion:202 Resp: 1694744

Ion Ratio Lower Upper

202 100

101 10.4 8.5 12.7



100 7.4 6.5 9.7

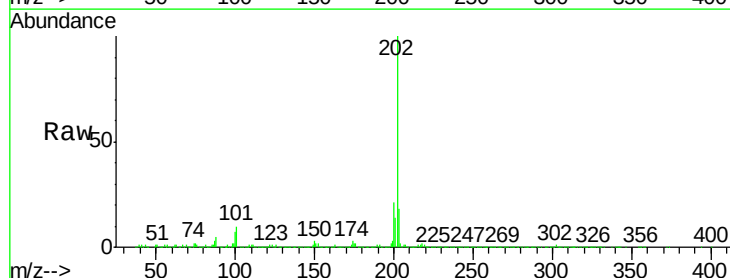


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



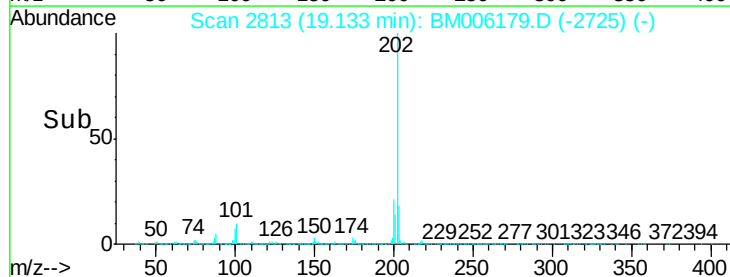
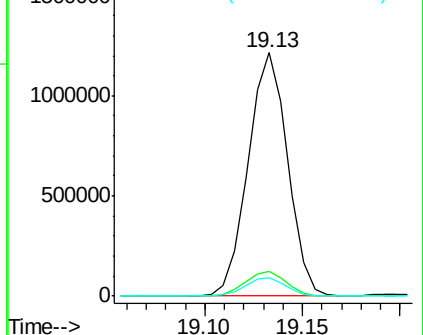


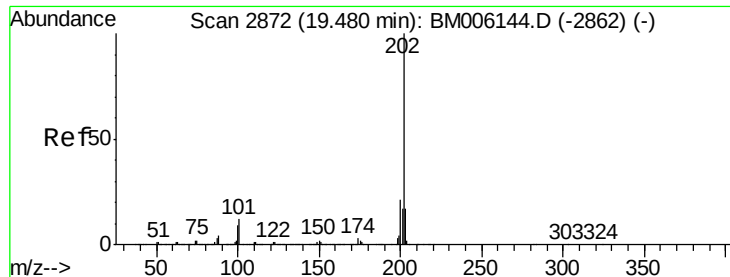

#31
 Pyrene
 Concen: 20.22 ng/ul
 RT: 19.50 min Scan# 2875
 Delta R.T. 0.02 min
 Lab File: BM006179.D
 Acq: 01 Jul 2016 13:02




Instrument :
 BNA_M
 ClientSampleId :
 D9YF9


Tgt Ion:202 Resp: 1530608
 Ion Ratio Lower Upper
 202 100
 101 11.8 11.0 16.4
 100 9.7 8.9 13.3

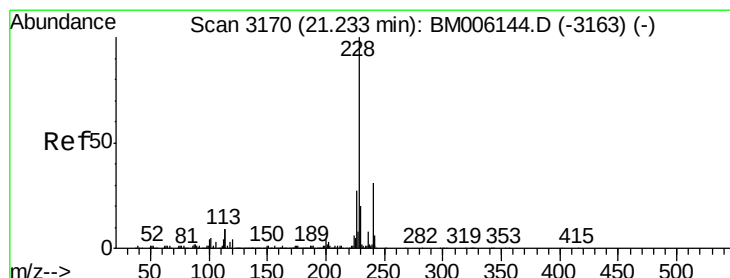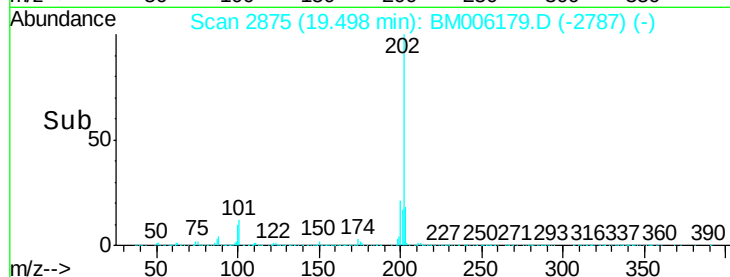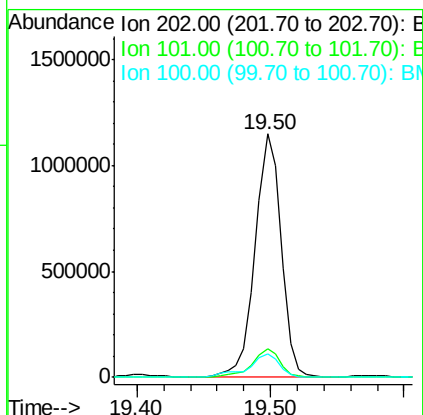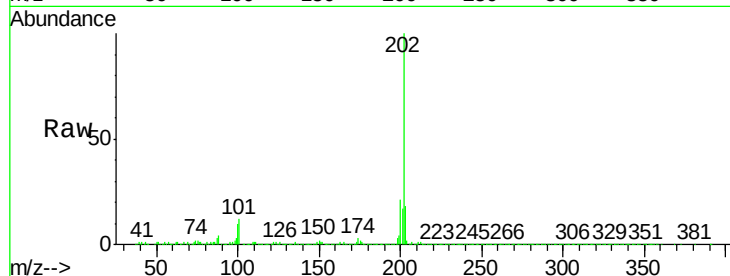

#32
 Benzo(a)anthracene
 Concen: 10.71 ng/ul
 RT: 21.25 min Scan# 3173
 Delta R.T. 0.02 min
 Lab File: BM006179.D
 Acq: 01 Jul 2016 13:02

Tgt Ion:228 Resp: 799605
 Ion Ratio Lower Upper
 228 100
 229 21.1 15.6 23.4
 226 28.6 21.6 32.4

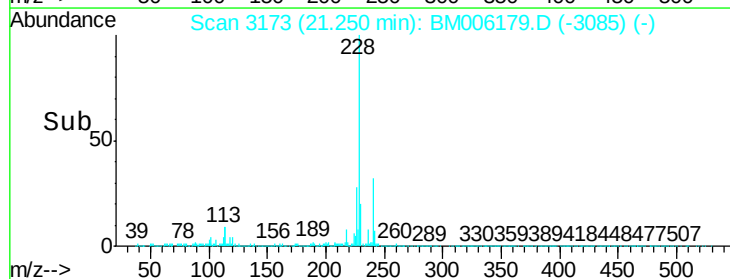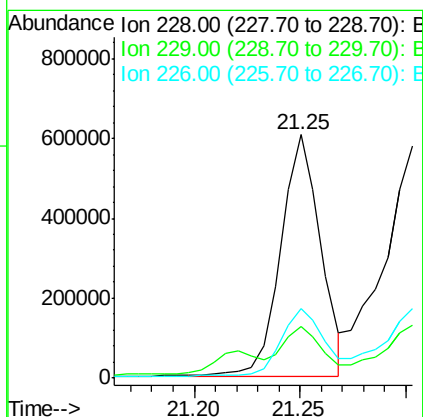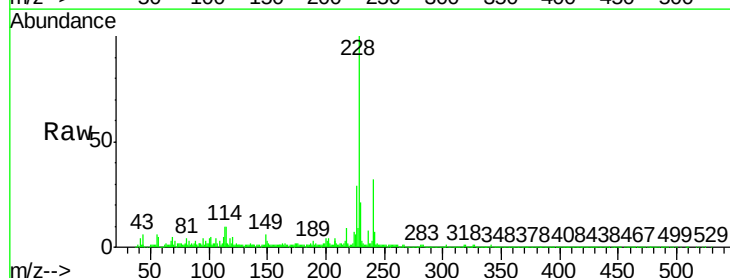

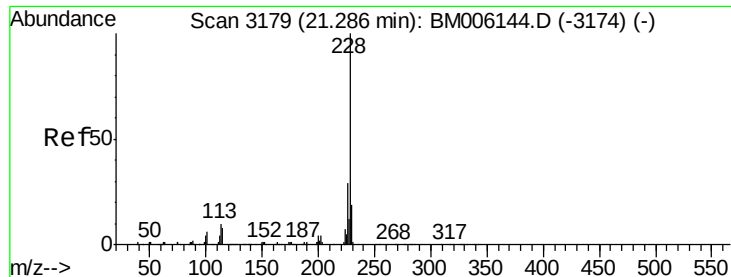

#33

Chrysene

Concen: 12.92 ng/ul

RT: 21.30 min Scan# 3182

Delta R.T. 0.02 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02

Instrument :

BNA_M

ClientSampleId :

D9YF9


Tgt Ion:228 Resp: 887484

Ion Ratio Lower Upper

228 100

226 30.2 23.8 35.6




229 22.8 15.8 23.6

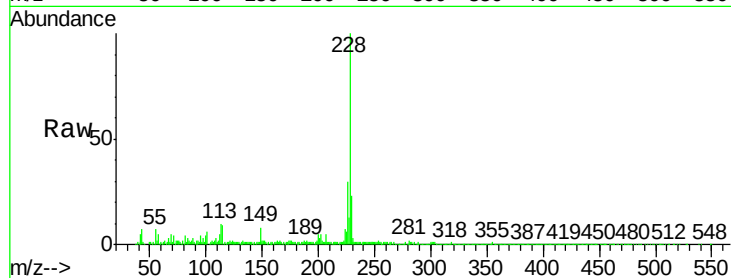

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

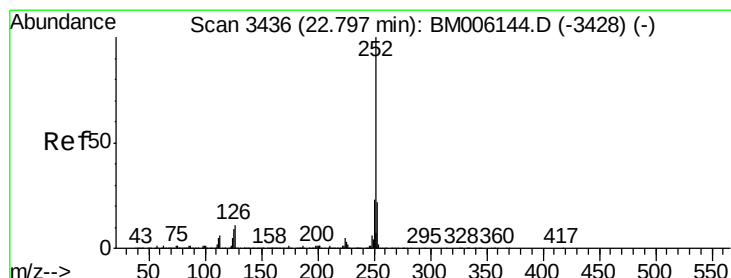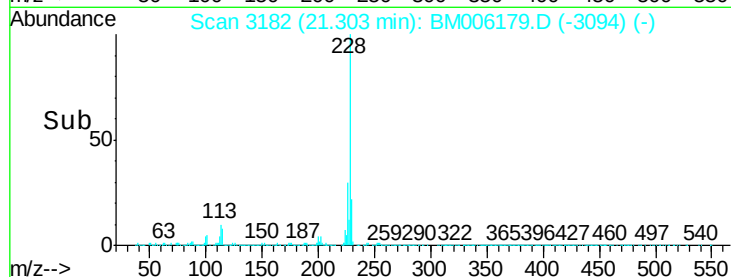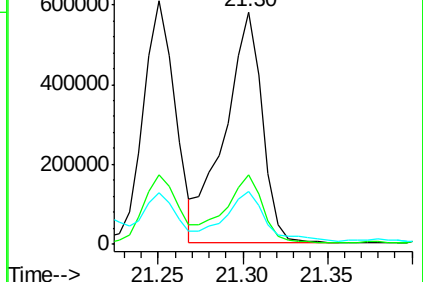

#35

Benzo(b)fluoranthene

Concen: 17.25 ng/ul

RT: 22.83 min Scan# 3442

Delta R.T. 0.04 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02


Tgt Ion:252 Resp: 1317166

Ion Ratio Lower Upper

252 100

253 23.0 17.2 25.8



125 10.5 7.8 11.6

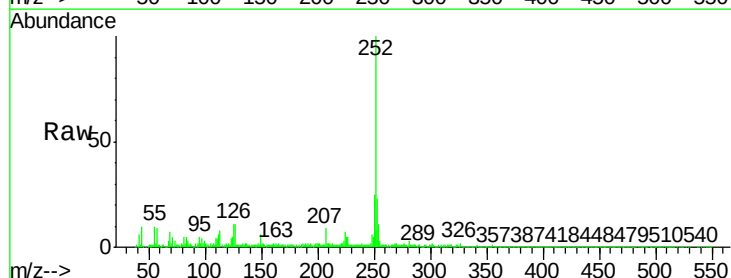


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



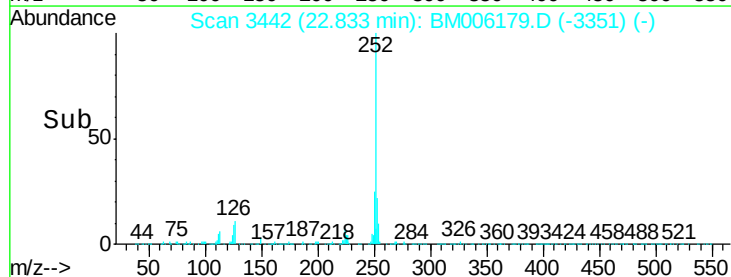
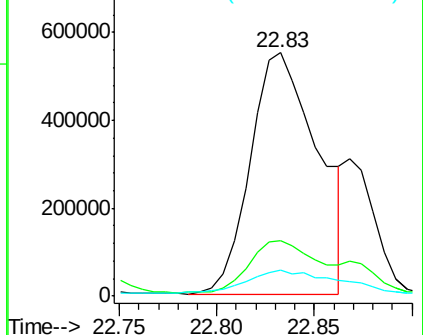


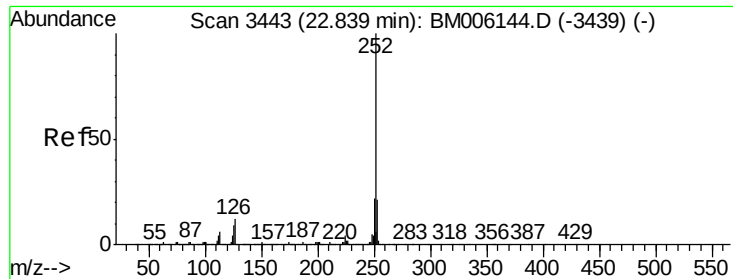

#36
Benzo(k)fluoranthene
Concen: 18.39 ng/ul
RT: 22.83 min Scan# 3442
Delta R.T. -0.01 min
Lab File: BM006179.D
Acq: 01 Jul 2016 13:02




Instrument :
BNA_M
ClientSampleId :
D9YF9


Tgt Ion:252 Resp: 1317166
Ion Ratio Lower Upper
252 100
253 23.0 17.6 26.4
125 10.5 8.1 12.1

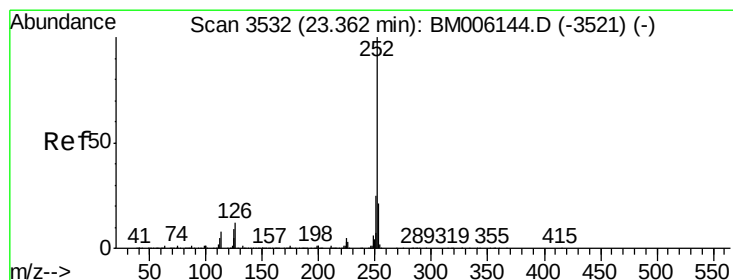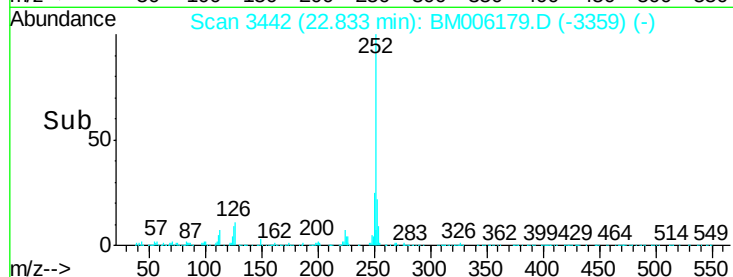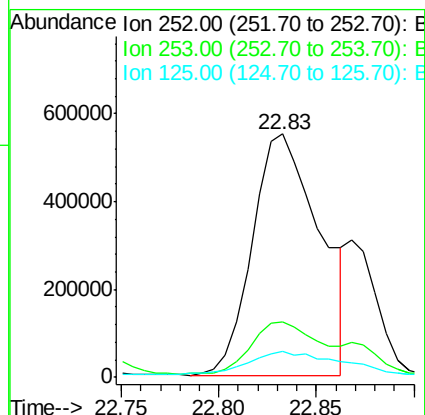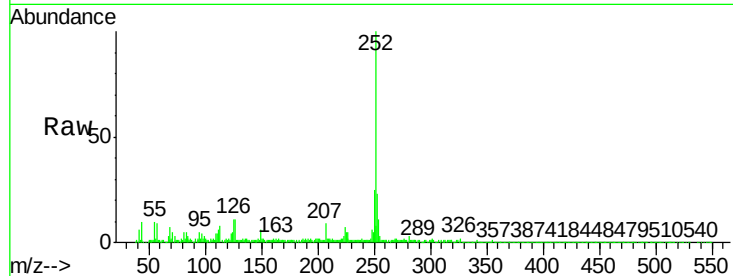

#38
Benzo(a)pyrene
Concen: 11.49 ng/ul
RT: 23.40 min Scan# 3539
Delta R.T. 0.04 min
Lab File: BM006179.D
Acq: 01 Jul 2016 13:02

Tgt Ion:252 Resp: 829222
Ion Ratio Lower Upper
252 100
253 24.2 17.8 26.6
125 10.5 8.7 13.1

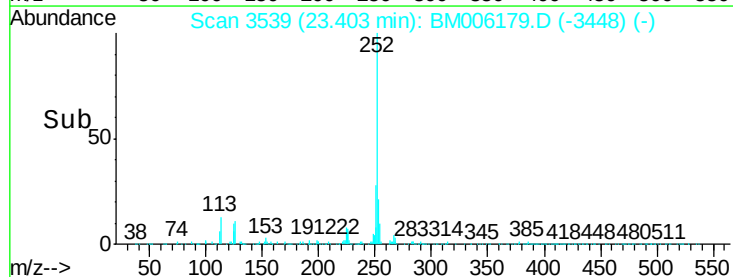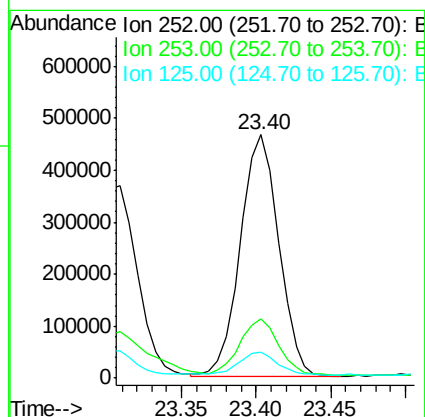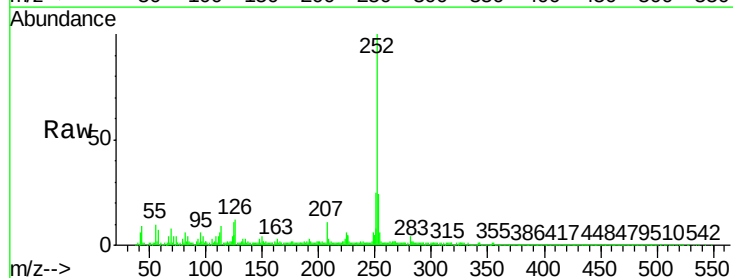

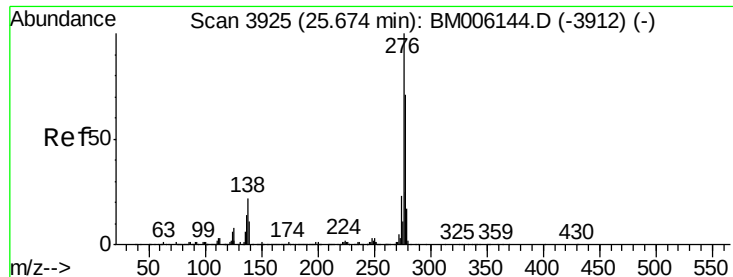

#39

Indeno(1,2,3-cd)pyrene

Concen: 8.58 ng/ul

RT: 25.74 min Scan# 3936

Delta R.T. 0.05 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02

Instrument :

BNA_M

ClientSampleId :

D9YF9


Tgt Ion:276 Resp: 643689

Ion Ratio Lower Upper

276 100

138 19.8 20.4 30.6#




277 25.6 20.6 30.8

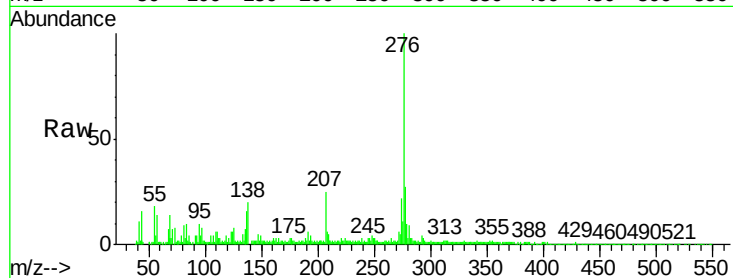

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

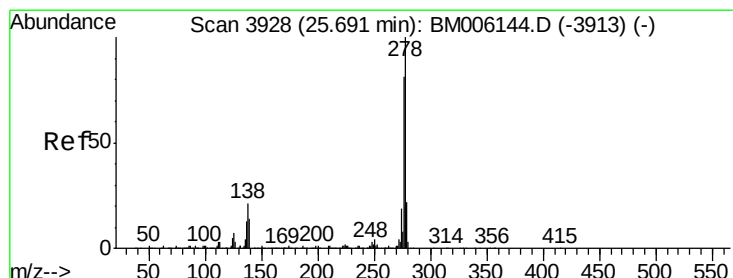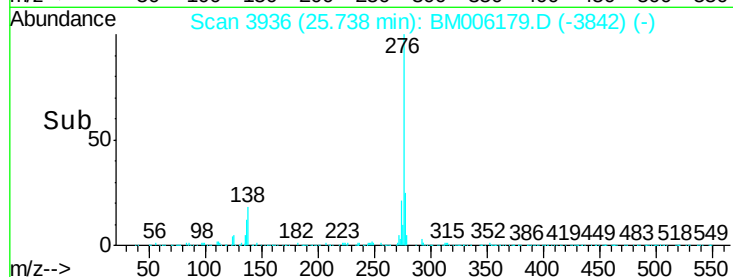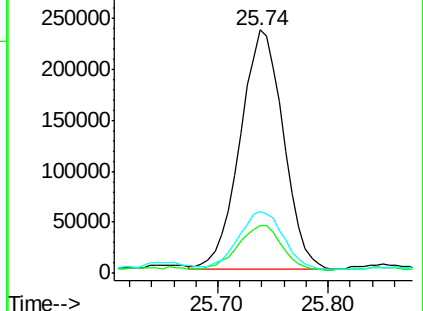

#40

Dibenzo(a,h)anthracene

Concen: 3.26 ng/ul

RT: 25.74 min Scan# 3936

Delta R.T. 0.05 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02


Tgt Ion:278 Resp: 202070

Ion Ratio Lower Upper

278 100

139 0.0 13.0 19.4#



279 36.7 18.8 28.2#

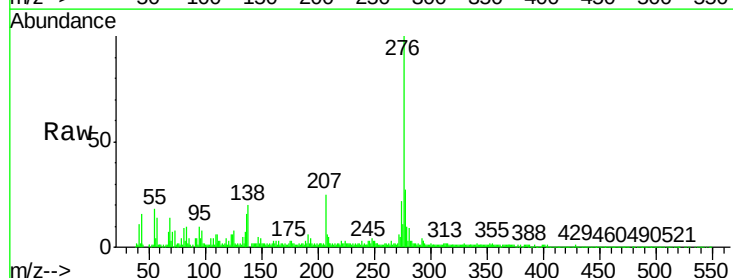


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

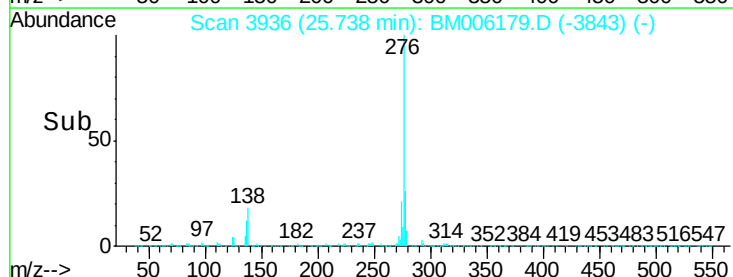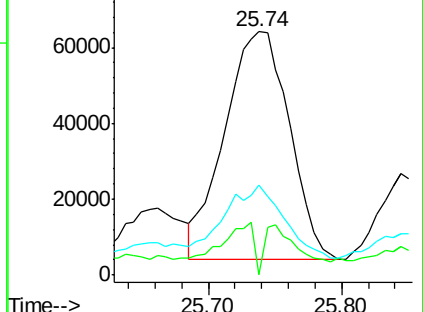

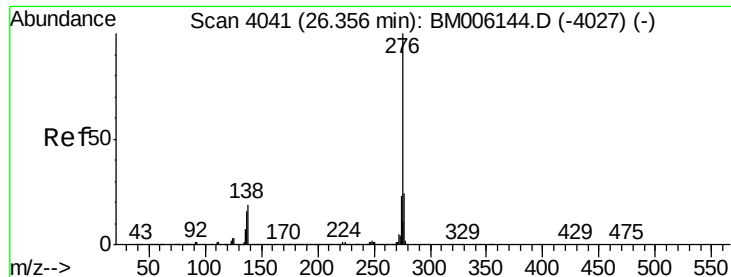

#41

Benzo(g,h,i)perylene

Concen: 10.15 ng/ul

RT: 26.43 min Scan# 4054

Delta R.T. 0.08 min

Lab File: BM006179.D

Acq: 01 Jul 2016 13:02

Instrument :

BNA_M

ClientSampleId :

D9YF9


Tgt Ion:276 Resp: 637203

Ion Ratio Lower Upper

276 100

138 18.6 16.6 25.0

277 25.4 18.9 28.3

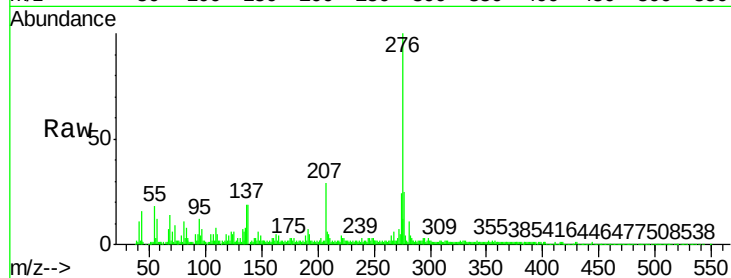

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

