

Data Path : Z:\HPCHEM1\BNA_M\Data\BM070116\
 Data File : BM006175.D
 Acq On : 01 Jul 2016 10:38
 Operator : UM/SJ
 Sample : H3779-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5

Manual Integrations
 APPROVED

sohil
 7/1/2016 7:16:39 PM

Quant Time: Jul 01 17:40:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 29 00:57:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	347980	20.00	ng/ul	0.00
7) Naphthalene-d8	10.44	136	1572388	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.31	164	894189	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.06	188	1920938	20.00	ng/ul	0.01
29) Chrysene-d12	21.26	240	1466670	20.00	ng/ul	0.01
34) Perylene-d12	23.49	264	1458694	20.00	ng/ul	0.03

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	6007	0.80	ng/uL	0.00
3) Phenol-d5	6.84	99	387225	13.62	ng/ul	0.01
4) Bis-(2-Chloroethyl)ether-d	6.99	67	225244	13.44	ng/ul	0.00
5) 2-Chlorophenol-d4	7.19	132	291342	13.35	ng/ul	0.00
6) 4-Methylphenol-d8	8.37	113	312184	13.64	ng/ul	0.00
8) Nitrobenzene-d5	8.81	128	148247	14.00	ng/ul	0.00
9) 2-Nitrophenol-d4	9.53	143	169433	13.98	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.07	165	310586	14.04	ng/ul	0.01
12) 4-Chloroaniline-d4	10.58	131	85828	4.91	ng/ul	0.00
16) Dimethylphthalate-d6	13.72	166	904924	14.12	ng/ul	0.00
17) Acenaphthylene-d8	14.00	160	1162639	14.95	ng/ul	0.00
20) 4-Nitrophenol-d4	14.53	143	157527	12.95	ng/ul	0.02
21) Fluorene-d10	15.30	176	815055	14.90	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.44	200	124609	18.31	ng/ul	0.01
26) Anthracene-d10	17.16	188	1211403	15.72	ng/ul	0.00
30) Pyrene-d10	19.46	212	1144315	19.38	ng/ul	0.01
37) Benzo(a)pyrene-d12	23.35	264	895887	15.43	ng/ul	0.03

Target Compounds

						Qvalue
18) Acenaphthylene	14.03	152	82210	1.01	ng/ul	99
25) Phenanthrene	17.10	178	888177	9.77	ng/ul	99
27) Anthracene	17.19	178	254149	2.72	ng/ul	100
28) Fluoranthene	19.13	202	2242368	20.14	ng/ul	99
31) Pyrene	19.49	202	1726723	22.32	ng/ul	96
32) Benzo(a)anthracene	21.24	228	1004688	13.17	ng/ul	97
33) Chrysene	21.30	228	940430	13.39	ng/ul	97
35) Benzo(b)fluoranthene	22.83	252	1437997	19.00	ng/ul	97
36) Benzo(k)fluoranthene	22.86	252	398777m	5.62	ng/ul	
38) Benzo(a)pyrene	23.40	252	889894	12.44	ng/ul	98
39) Indeno(1,2,3-cd)pyrene	25.74	276	705053	9.48	ng/ul#	93
40) Dibenzo(a,h)anthracene	25.73	278	195675	3.18	ng/ul#	81
41) Benzo(g,h,i)perylene	26.43	276	651873	10.48	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070116\
Data File : BM006175.D
Acq On : 01 Jul 2016 10:38
Operator : UM/SJ
Sample : H3779-06
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
D9YD5

Manual Integrations
APPROVED

sohil
7/1/2016 7:16:39 PM

Quant Time: Jul 01 17:40:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 29 00:57:09 2016
Response via : Initial Calibration

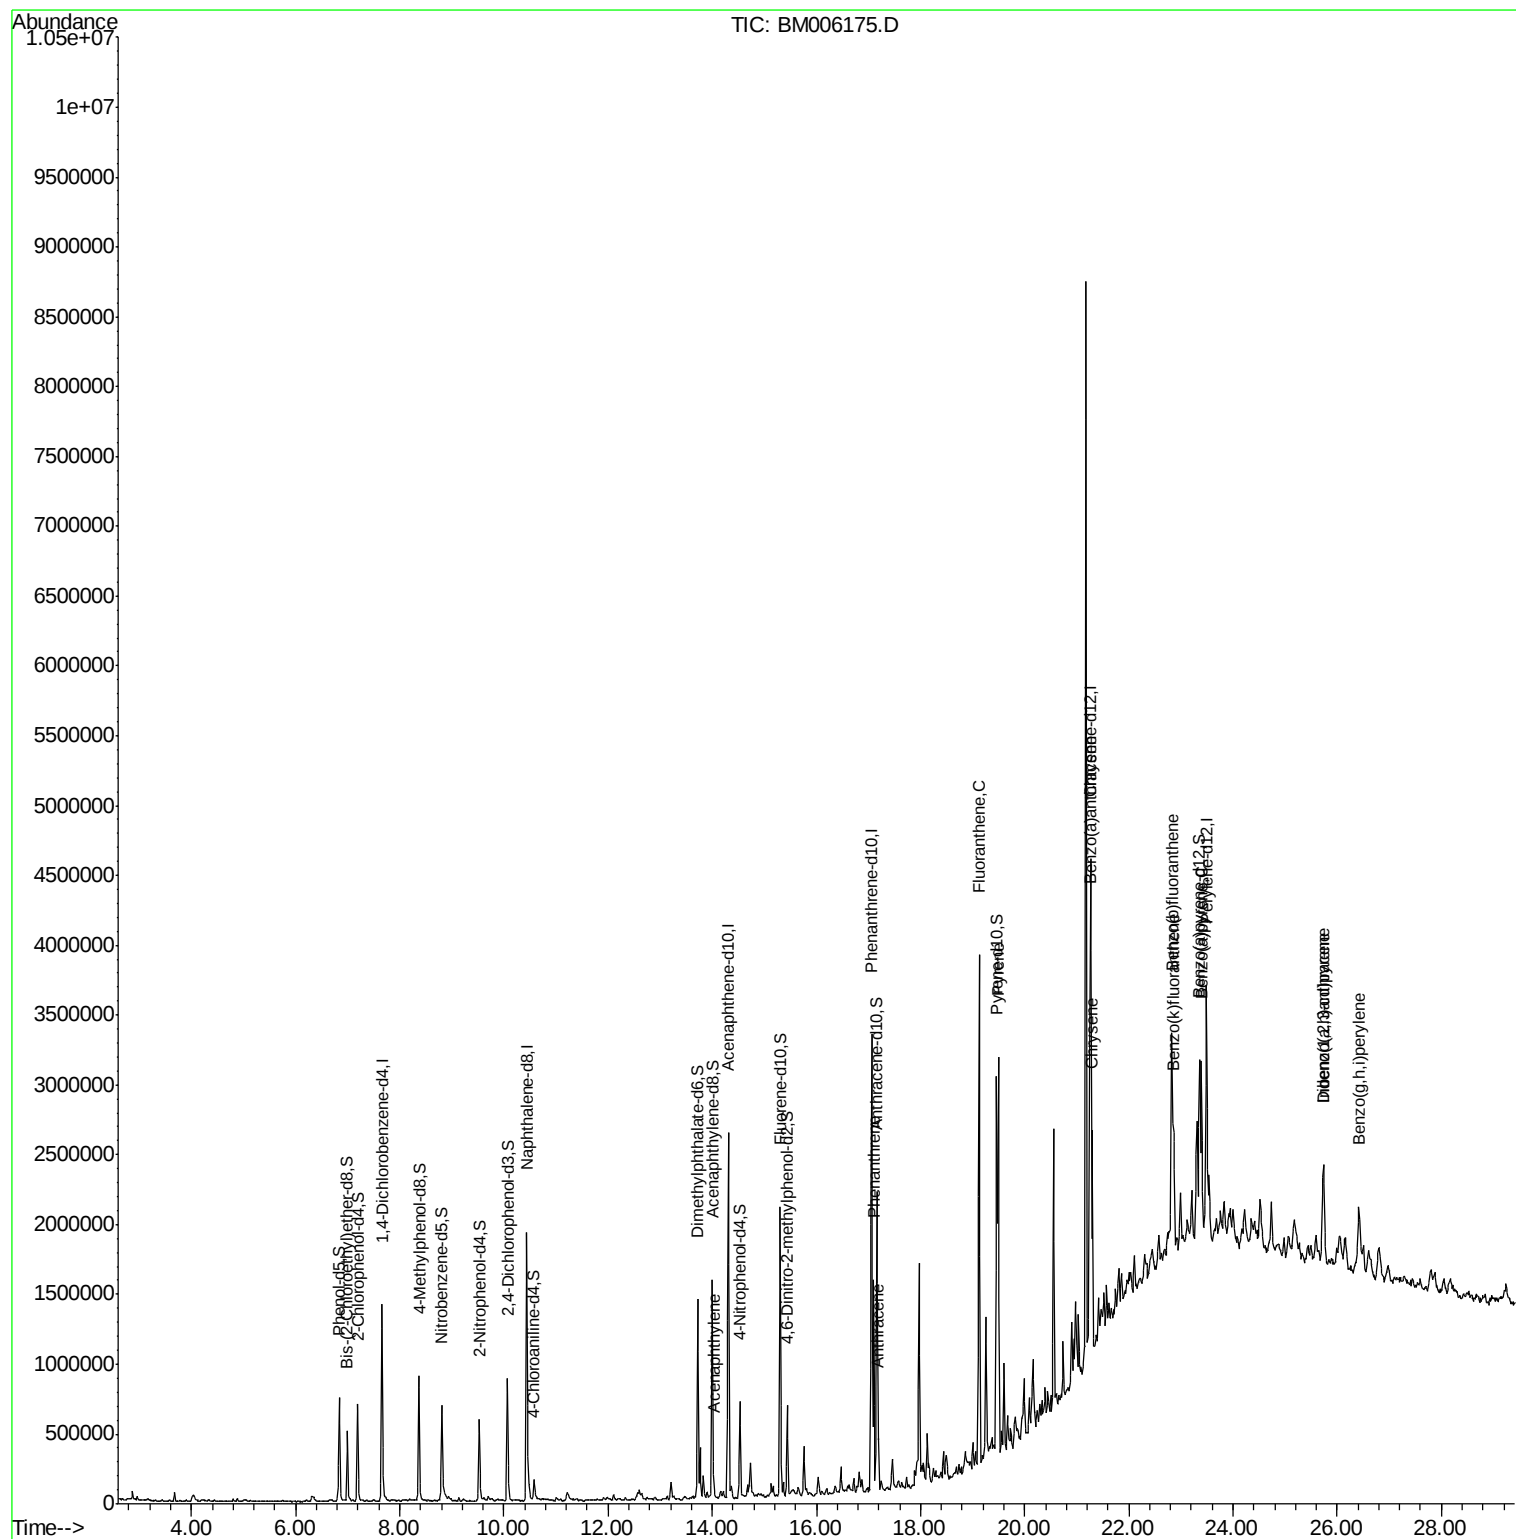

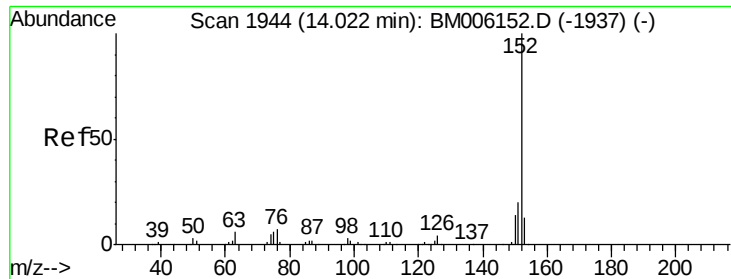





#18
Acenaphthylene
Concen: 1.01 ng/ul
RT: 14.03 min Scan# 1946
Delta R.T. 0.01 min
Lab File: BM006175.D
Acq: 01 Jul 2016 10:38

Instrument :
BNA_M
ClientSampleId :
D9YD5

Tgt Ion:	152	Resp:	82210
Ion Ratio	Lower	Upper	
152	100		
151	19.9	15.8	23.6
153	12.0	10.3	15.5




Manual Integrations
APPROVED


sohil
7/1/2016 7:16:39 PM

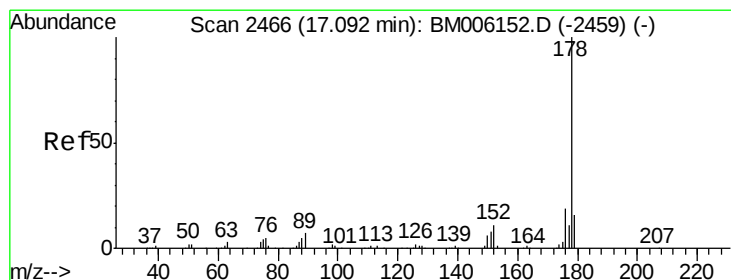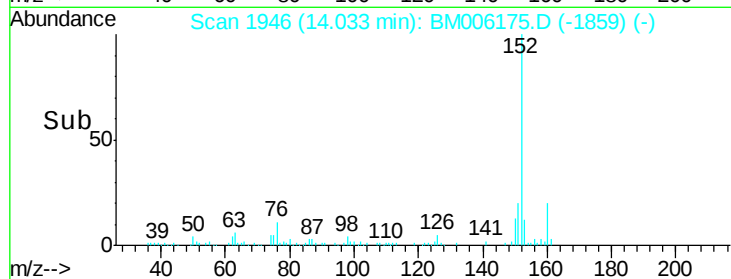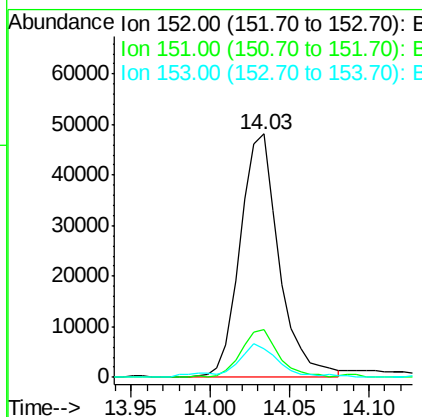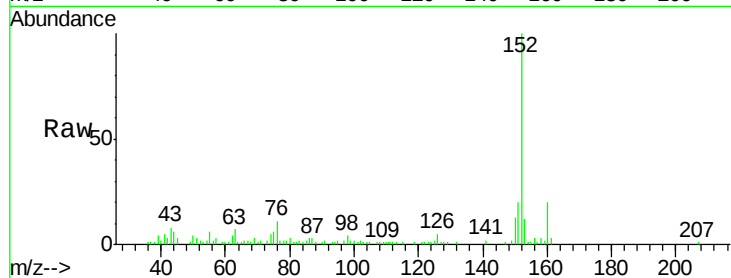

#25
Phenanthrene
Concen: 9.77 ng/ul
RT: 17.10 min Scan# 2468
Delta R.T. 0.01 min
Lab File: BM006175.D
Acq: 01 Jul 2016 10:38

Tgt Ion:	178	Resp:	888177
Ion Ratio	Lower	Upper	
178	100		
179	15.5	12.2	18.2
176	19.8	15.3	22.9

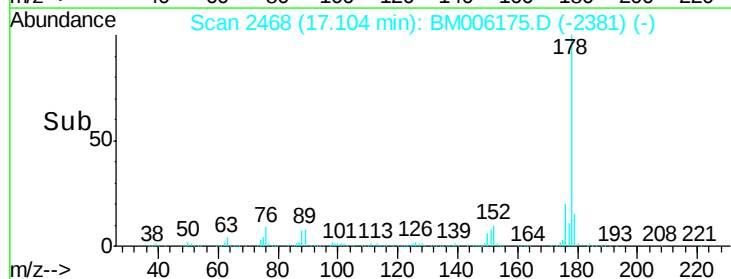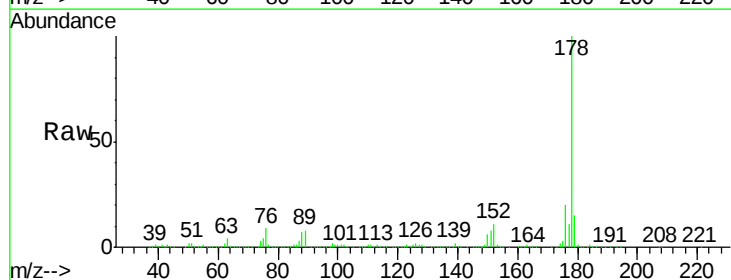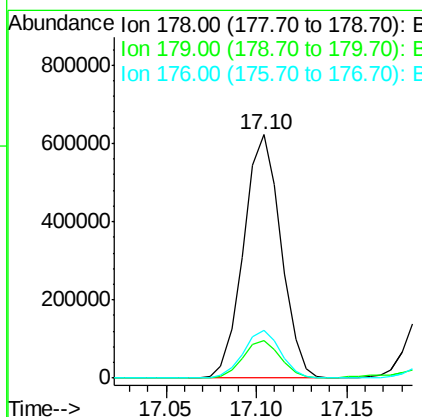

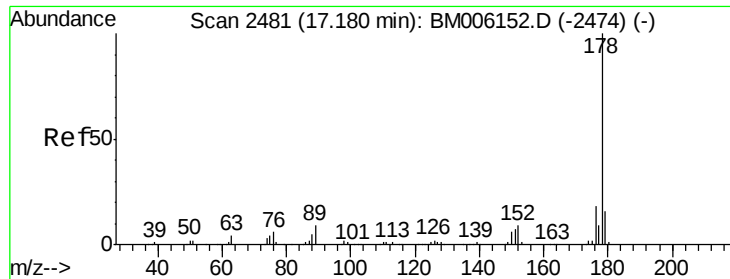





#27
 Anthracene
 Concen: 2.72 ng/ul
 RT: 17.19 min Scan# 2483
 Delta R.T. 0.01 min
 Lab File: BM006175.D
 Acq: 01 Jul 2016 10:38

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.3	18.5
176	18.2	14.6	22.0




Manual Integrations
 APPROVED


sohil
 7/1/2016 7:16:39 PM

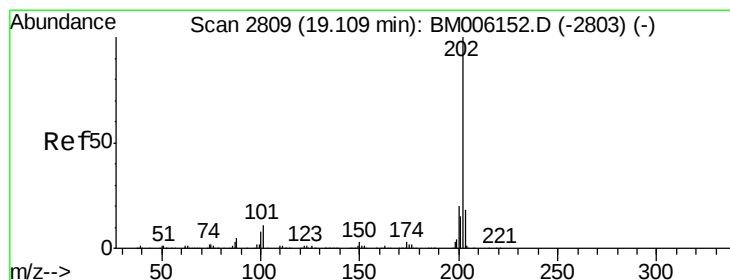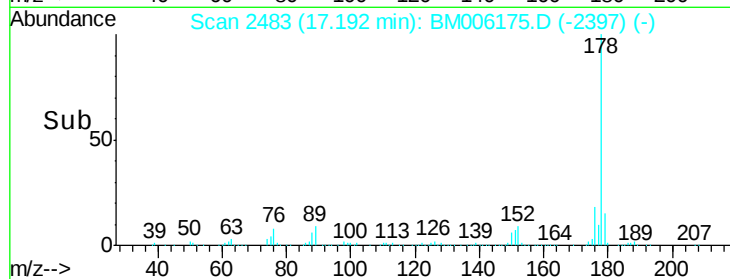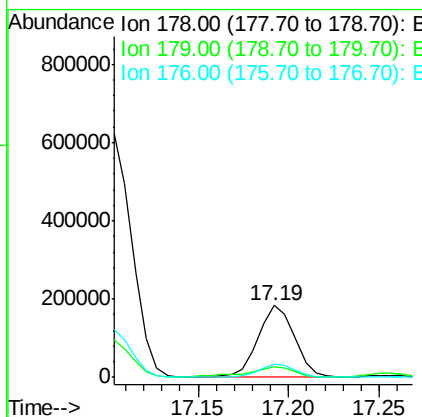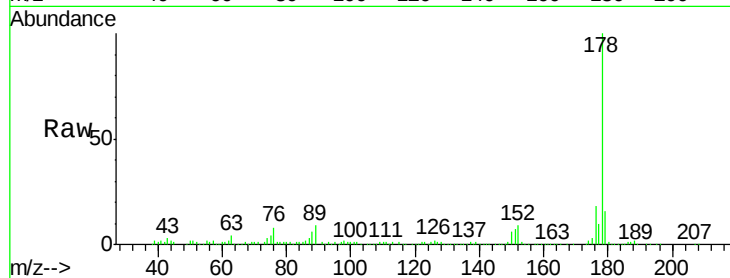

#28
 Fluoranthene
 Concen: 20.14 ng/ul
 RT: 19.13 min Scan# 2812
 Delta R.T. 0.01 min
 Lab File: BM006175.D
 Acq: 01 Jul 2016 10:38

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.2	8.5	12.7
100	7.7	6.5	9.7

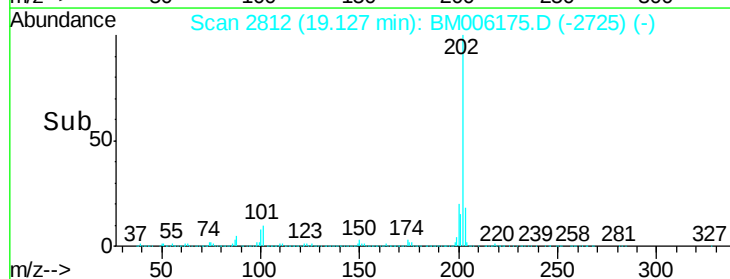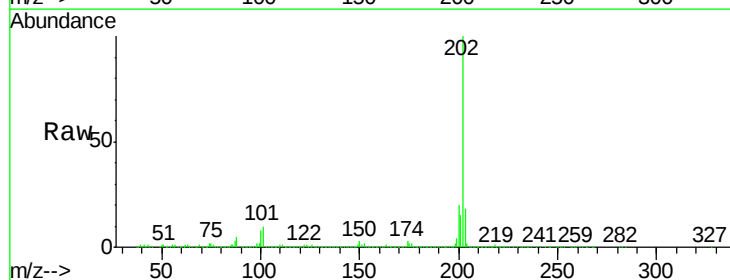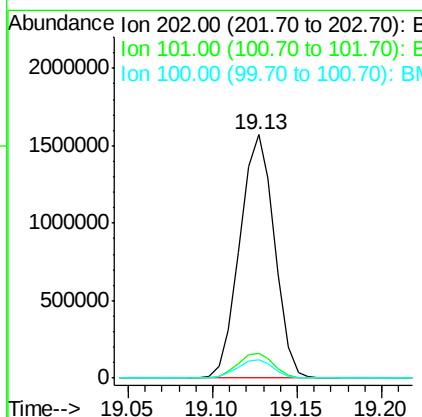

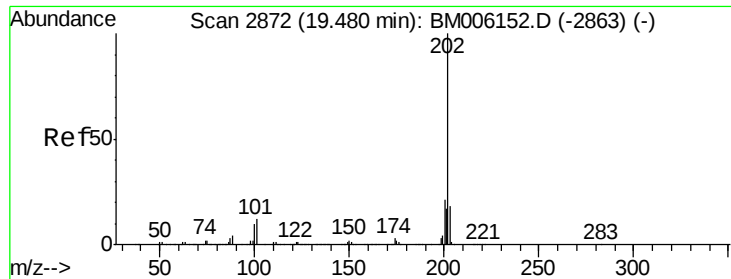





#31
 Pyrene
 Concen: 22.32 ng/ul
 RT: 19.49 min Scan# 2874
 Delta R.T. 0.01 min
 Lab File: BM006175.D
 Acq: 01 Jul 2016 10:38

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.1	11.0	16.4
100	9.6	8.9	13.3




Manual Integrations
 APPROVED


sohil
 7/1/2016 7:16:39 PM

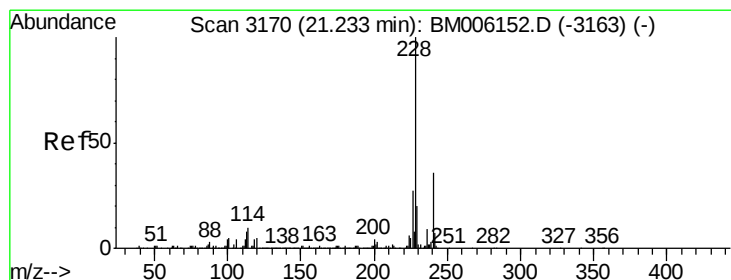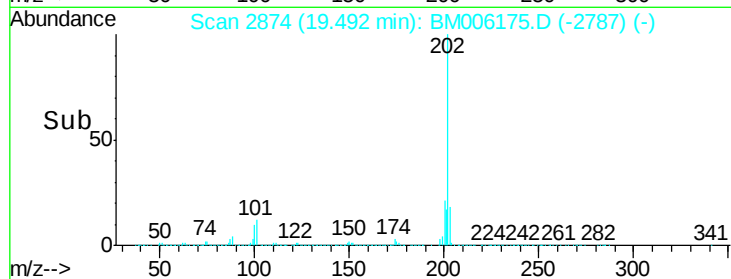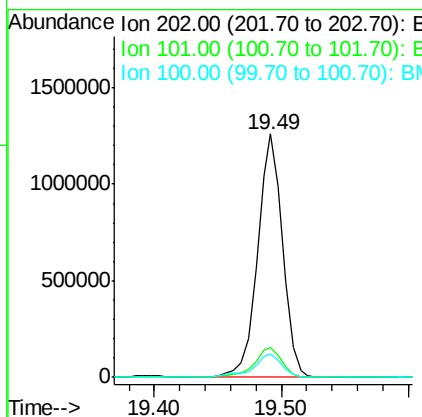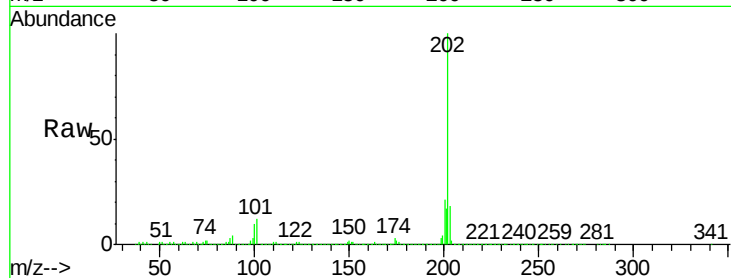

#32
 Benzo(a)anthracene
 Concen: 13.17 ng/ul
 RT: 21.24 min Scan# 3172
 Delta R.T. 0.01 min
 Lab File: BM006175.D
 Acq: 01 Jul 2016 10:38

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.0	15.6	23.4
226	28.5	21.6	32.4

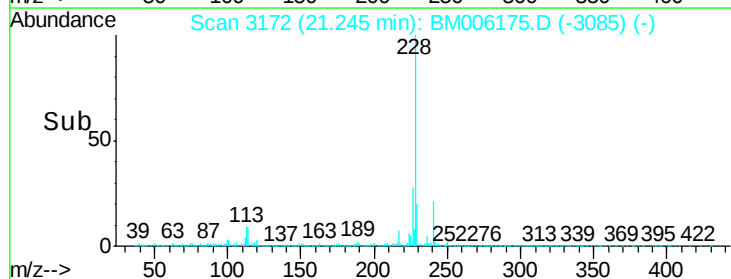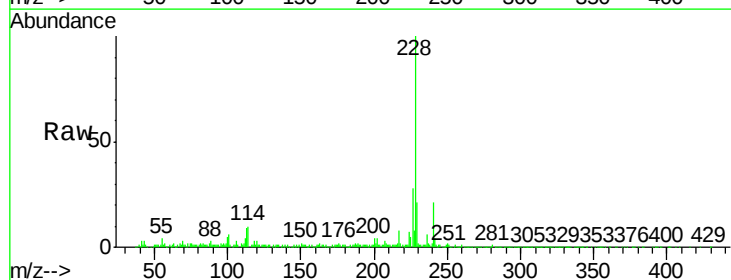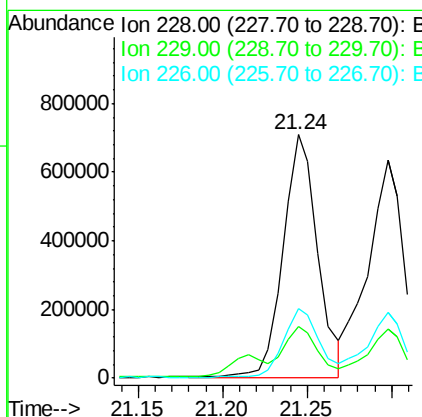

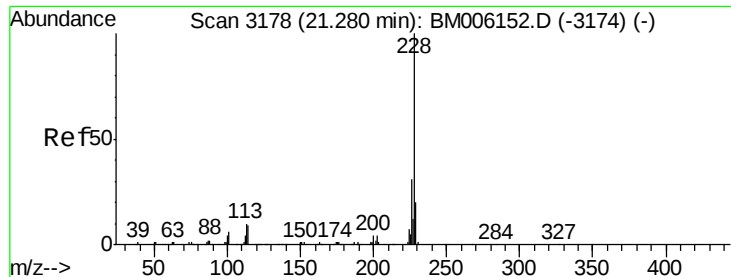

#33

Chrysene

Concen: 13.39 ng/ul

RT: 21.30 min Scan# 3181

Delta R.T. 0.01 min

Lab File: BM006175.D

Acq: 01 Jul 2016 10:38

Instrument :

BNA_M


ClientSampleId :

D9YD5




Tgt Ion:	228	Resp:	940430
Ion Ratio	Lower	Upper	
228	100		
226	30.1	23.8	35.6
229	22.7	15.8	23.6

Manual Integrations
APPROVED

sohil
7/1/2016 7:16:39 PM

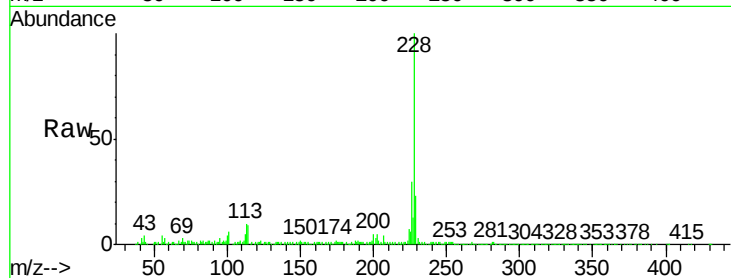

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

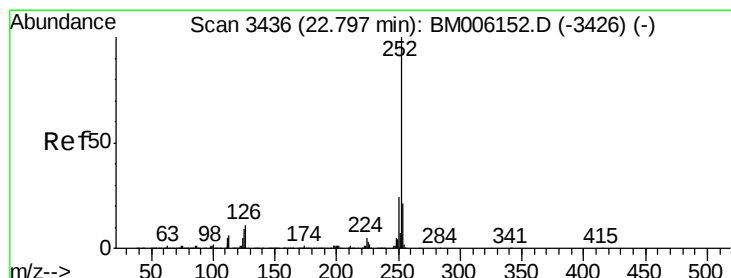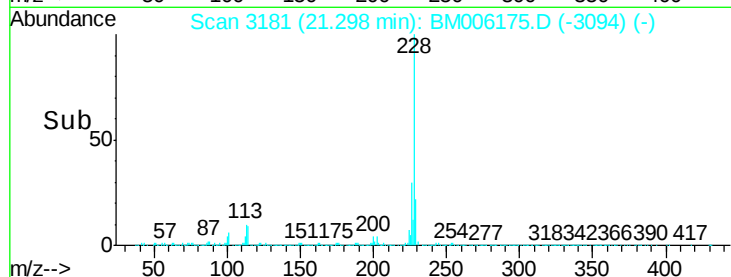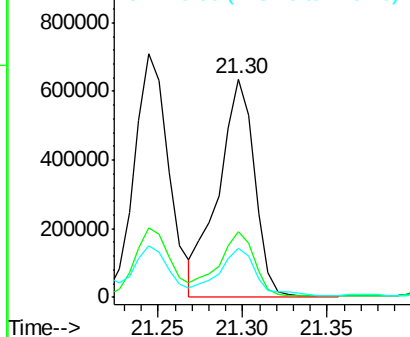

#35

Benzo(b)fluoranthene

Concen: 19.00 ng/ul

RT: 22.83 min Scan# 3441




Delta R.T. 0.03 min


Lab File: BM006175.D

Acq: 01 Jul 2016 10:38

Tgt Ion:	252	Resp:	1437997
Ion Ratio	Lower	Upper	
252	100		
253	23.3	17.2	25.8
125	9.6	7.8	11.6

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

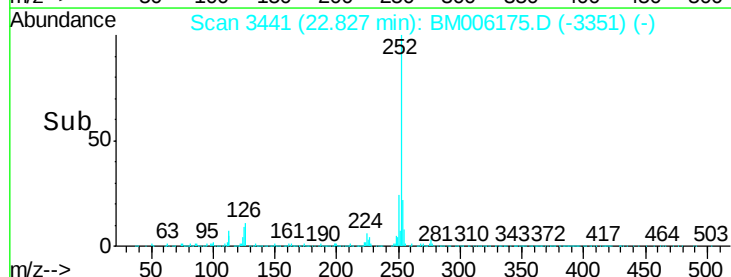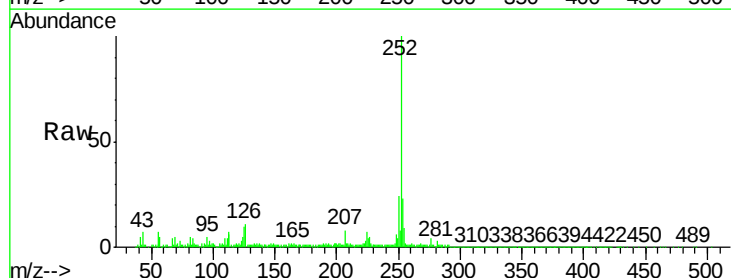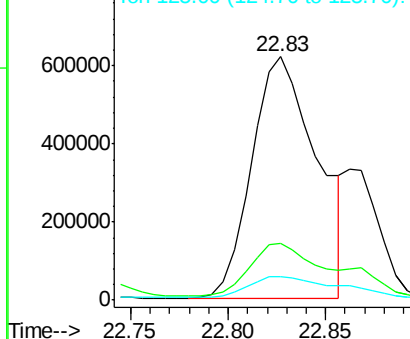

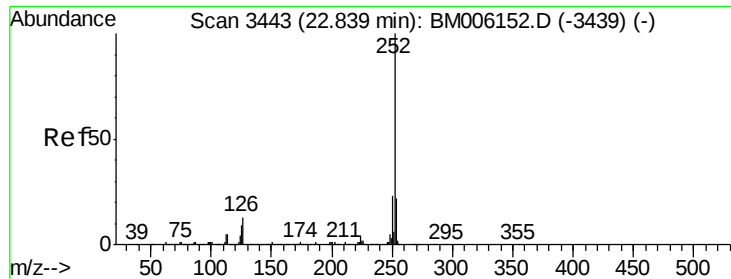

#36

Benzo(k)fluoranthene

Concen: 5.62 ng/ul m

RT: 22.86 min Scan# 3447

Delta R.T. 0.02 min

Lab File: BM006175.D


Acq: 01 Jul 2016 10:38

Instrument :

BNA_M

ClientSampleId :




D9YD5

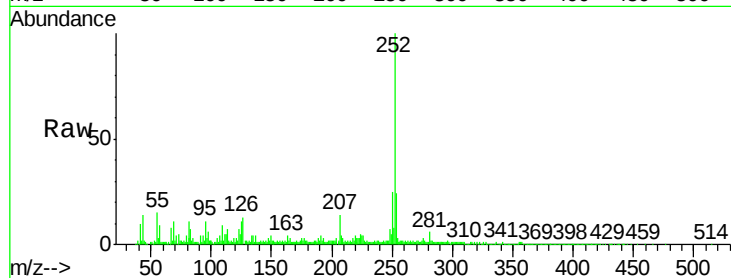

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.1	17.6	26.4
125	10.8	8.1	12.1

Manual Integrations
APPROVED

sohil
7/1/2016 7:16:39 PM

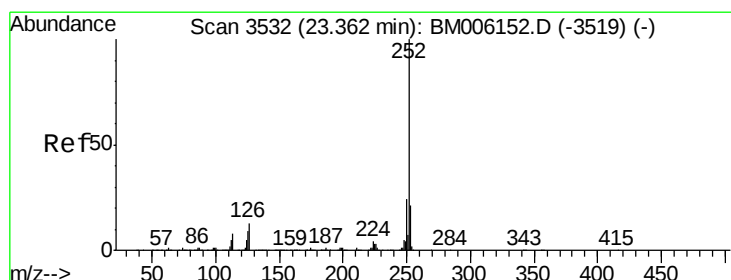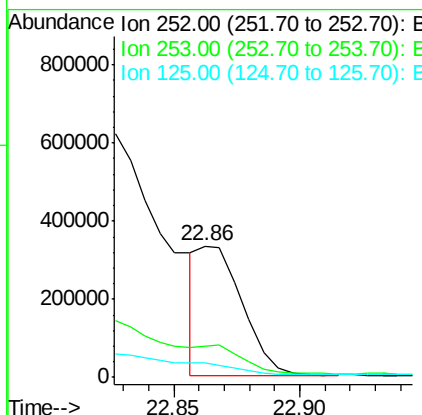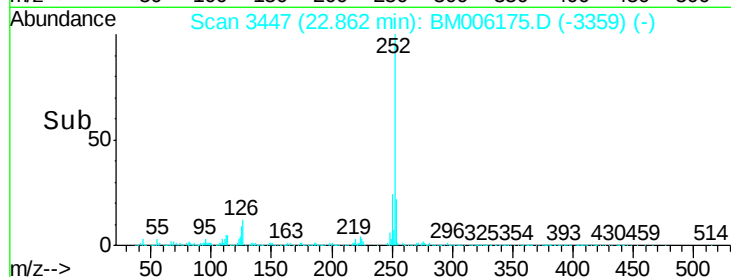

#38

Benzo(a)pyrene


Concen: 12.44 ng/ul

RT: 23.40 min Scan# 3538



Delta R.T. 0.03 min


Lab File: BM006175.D

Acq: 01 Jul 2016 10:38

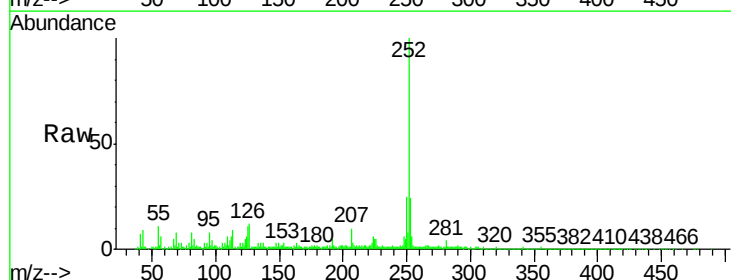

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	17.8	26.6
125	10.5	8.7	13.1

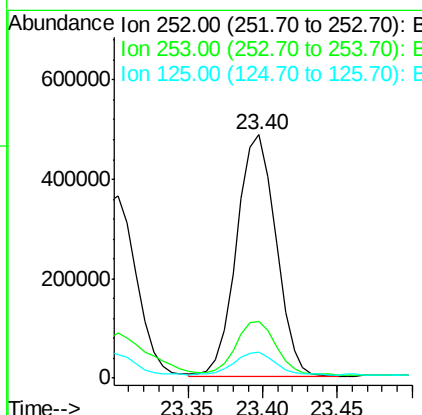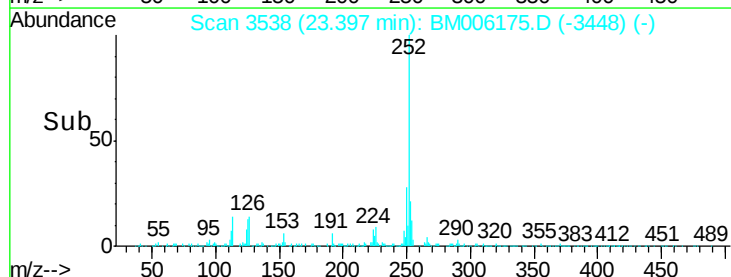

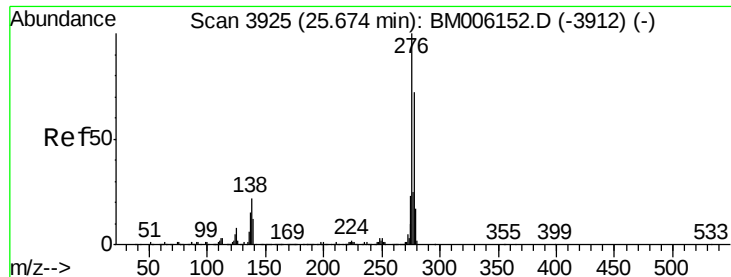

#39

Indeno(1,2,3-cd)pyrene

Concen: 9.48 ng/ul

RT: 25.74 min Scan# 3936

Delta R.T. 0.05 min

Lab File: BM006175.D

Acq: 01 Jul 2016 10:38

Instrument :

BNA_M





ClientSampleId :

D9YD5

Tgt Ion:	276	Resp:	705053
Ion Ratio	Lower	Upper	
276	100		
138	19.0	20.4	30.6#
277	25.3	20.6	30.8

Manual Integrations
APPROVED

sohil
7/1/2016 7:16:39 PM

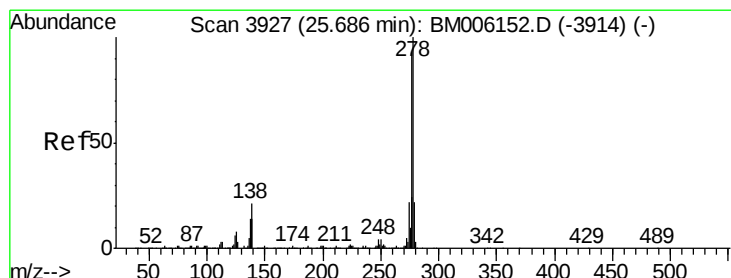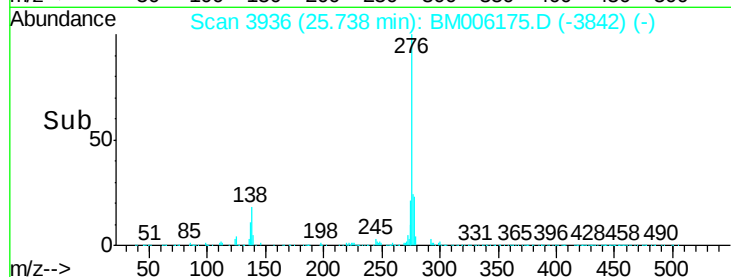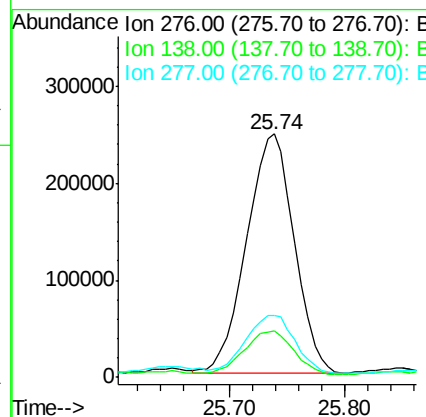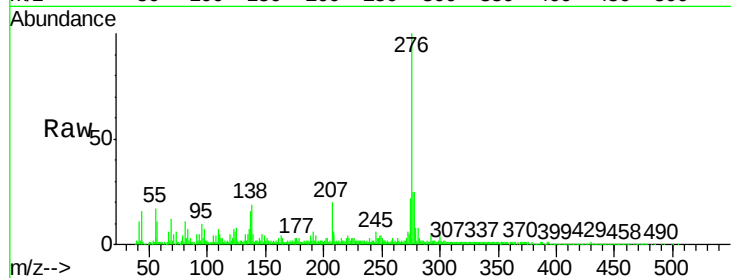

#40

Dibenzo(a,h)anthracene

Concen: 3.18 ng/ul




RT: 25.73 min Scan# 3935


Delta R.T. 0.04 min

Lab File: BM006175.D

Acq: 01 Jul 2016 10:38

Tgt Ion:	278	Resp:	195675
Ion Ratio	Lower	Upper	
278	100		
139	21.2	13.0	19.4#
279	35.0	18.8	28.2#

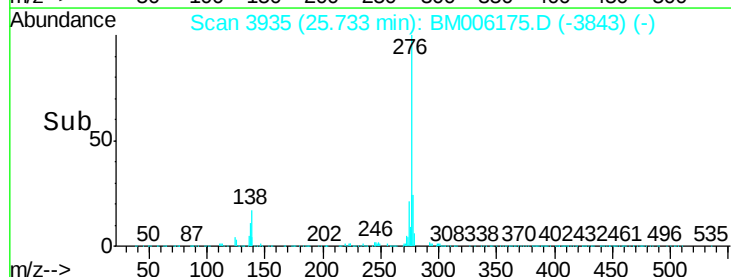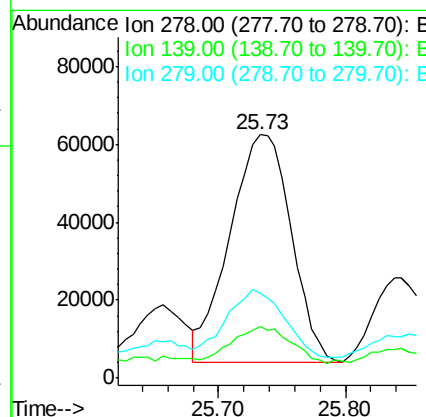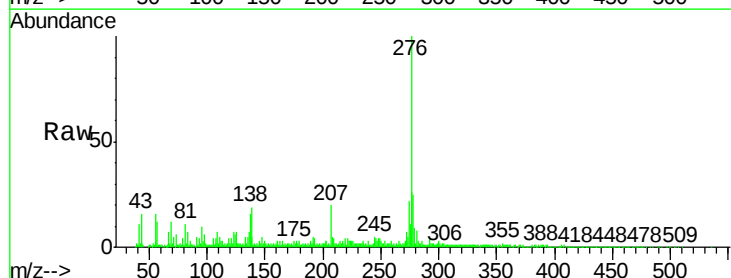

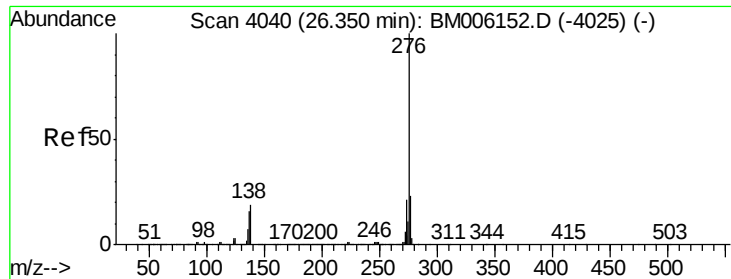

#41
 Benzo(g,h,i)perylene
 Concen: 10.48 ng/ul
 RT: 26.43 min Scan# 4053
 Delta R.T. 0.07 min
 Lab File: BM006175.D
 Acq: 01 Jul 2016 10:38

Instrument :
 BNA_M
 ClientSampleId :
 D9YD5

Tgt Ion:	276	Resp:	651873
Ion Ratio		Lower	Upper
276	100		
138	20.3	16.6	25.0
277	25.2	18.9	28.3

Manual Integrations
 APPROVED

sohil
 7/1/2016 7:16:39 PM

