
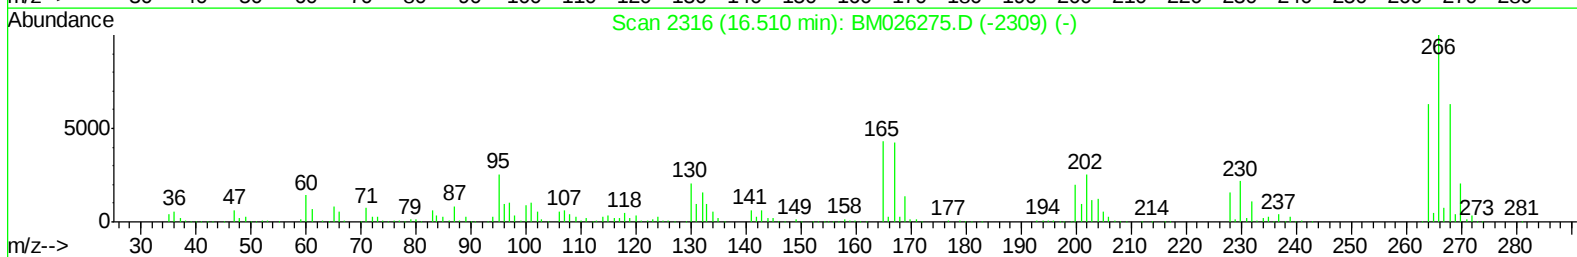
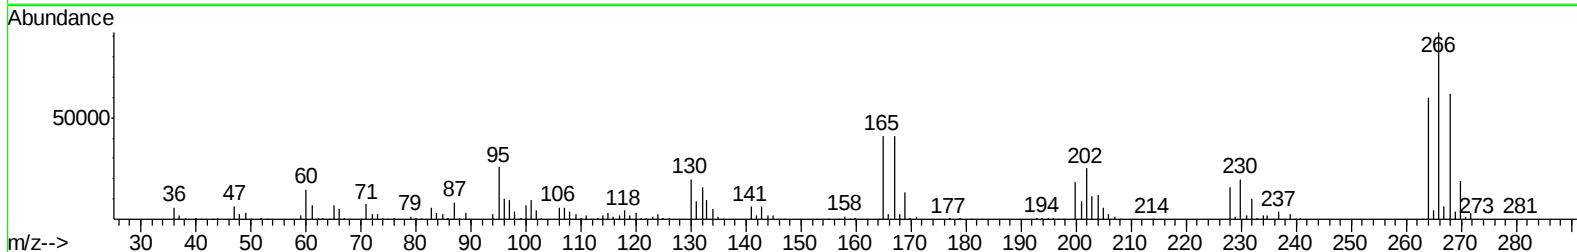


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070120\
Data File : BM026627.D
Acq On : 01 Jul 2020 08:45
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 01:17:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 01 13:20:43 2020
Response via : Initial Calibration

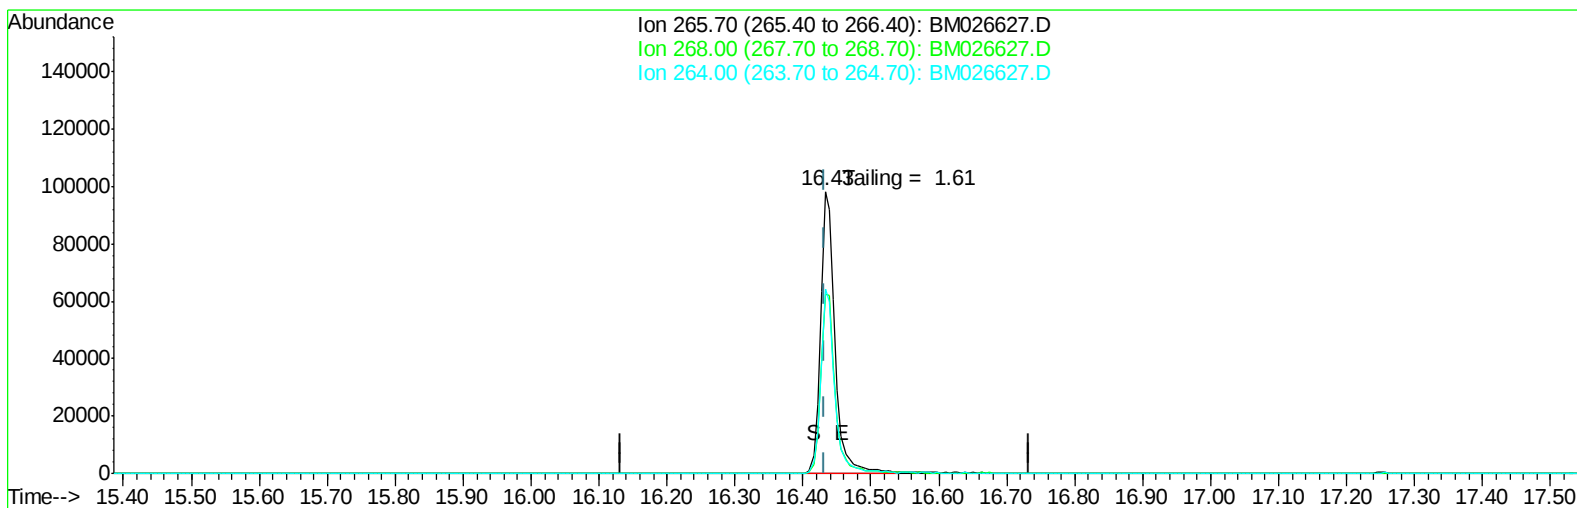

TIC: BM026627.D

(70) Pentachlorophenol (C)




16.433min (-0.000) 0.00ng

response 146781

Ion	Exp%	Act%
265.70	100	100
268.00	62.80	63.47
264.00	63.20	65.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070120\
 Data File : BM026627.D
 Acq On : 01 Jul 2020 08:45
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 01:17:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 01 13:20:43 2020
 Response via : Initial Calibration

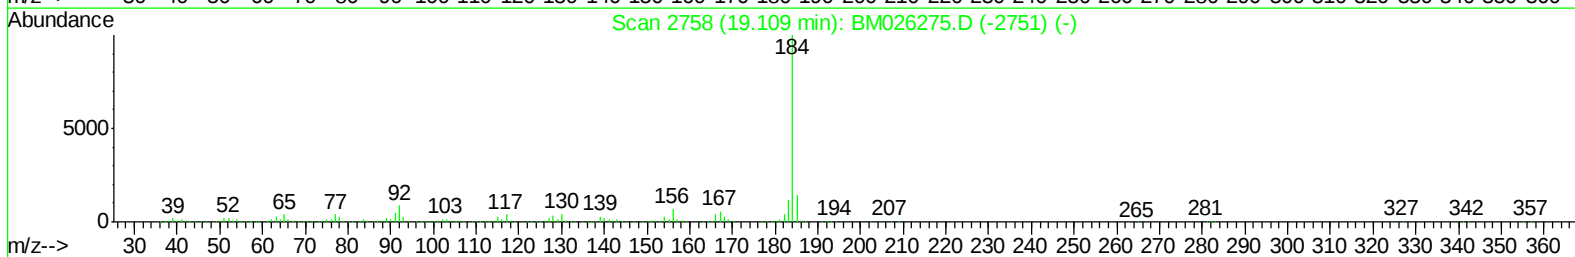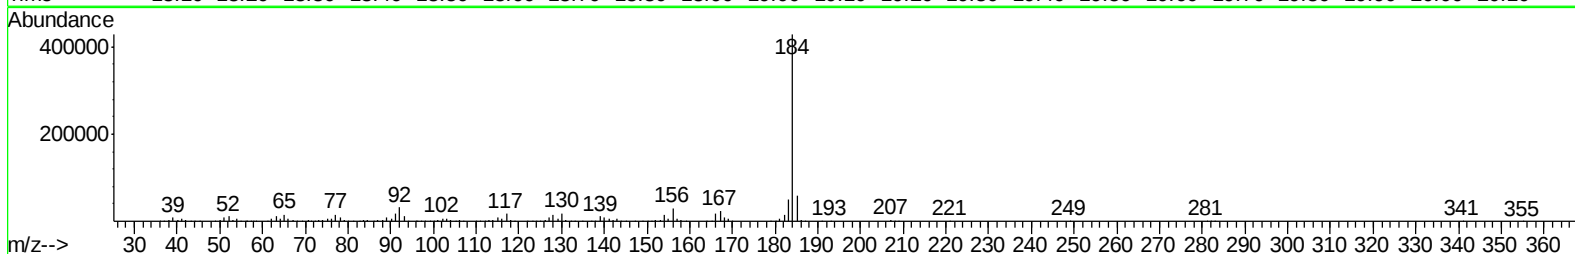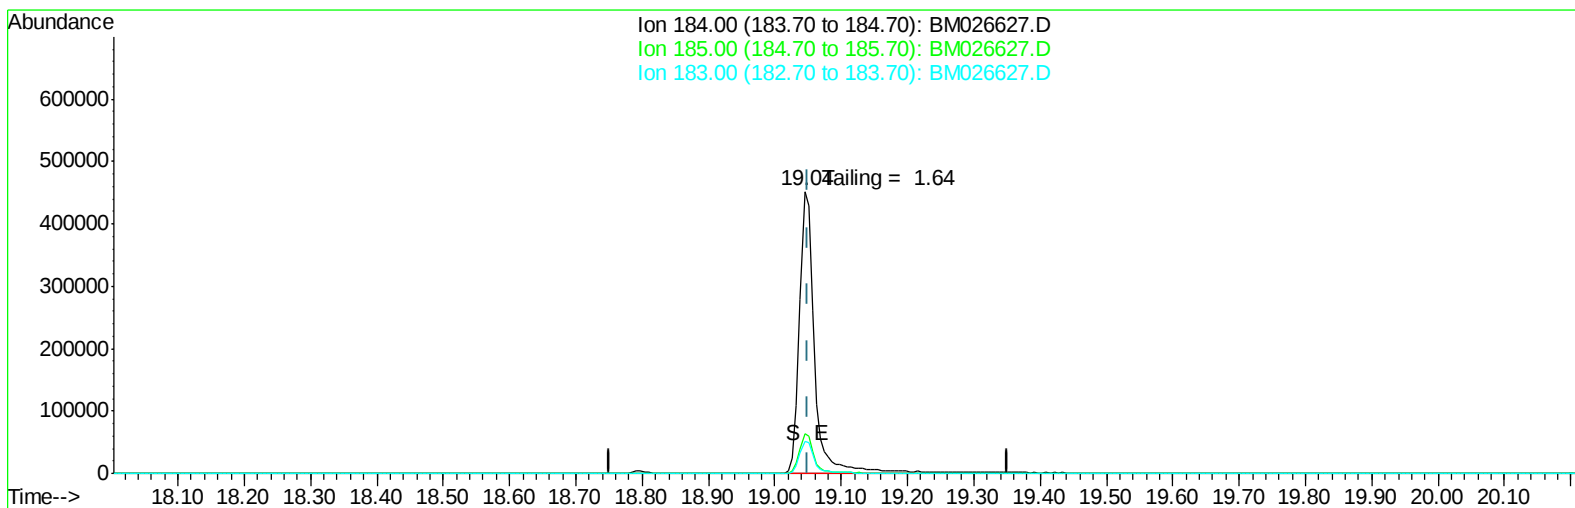

TIC: BM026627.D

(77) Benzidine

19.045min (-0.006) 0.00ng

response 688400

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.23
183.00	11.80	11.59
0.00	0.00	0.00