

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070120\
 Data File : BM026636.D
 Acq On : 01 Jul 2020 14:19
 Operator : JU/CG
 Sample : L2815-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OR-03-062920

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.987	14	17	27	rVB	312936	340249	4.63%	1.028%
2	3.905	169	173	182	rVB	62125	74869	1.02%	0.226%
3	4.081	199	203	213	rVB	75145	92072	1.25%	0.278%
4	4.516	273	277	288	rVB	88323	123475	1.68%	0.373%
5	4.993	352	358	375	rBV	2155543	2977017	40.49%	8.991%
6	6.563	618	625	640	rBV	1840373	2789466	37.94%	8.425%
7	7.351	753	759	766	rBV	352003	538793	7.33%	1.627%
8	7.669	806	813	824	rBV	1894291	2831525	38.51%	8.552%
9	8.504	948	955	975	rBV	1530257	2426254	33.00%	7.328%
10	10.110	1220	1228	1247	rBV	415927	704355	9.58%	2.127%
11	12.622	1648	1655	1671	rBV	3380728	4752520	64.64%	14.354%
12	14.016	1884	1892	1900	rBV	595898	879676	11.96%	2.657%
13	15.521	2141	2148	2169	rBV	2876284	3886755	52.86%	11.739%
14	16.774	2353	2361	2366	rBV	699235	1005461	13.67%	3.037%
15	19.433	2807	2813	2818	rBV	6075621	7352801	100.00%	22.207%
16	20.986	3072	3077	3086	rBV	921269	1176303	16.00%	3.553%
17	23.068	3426	3431	3441	rVB2	700541	1158616	15.76%	3.499%


Sum of corrected areas: 33110207

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070120\
Data File : BM026636.D
Acq On : 01 Jul 2020 14:19
Operator : JU/CG
Sample : L2815-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OR-03-062920

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

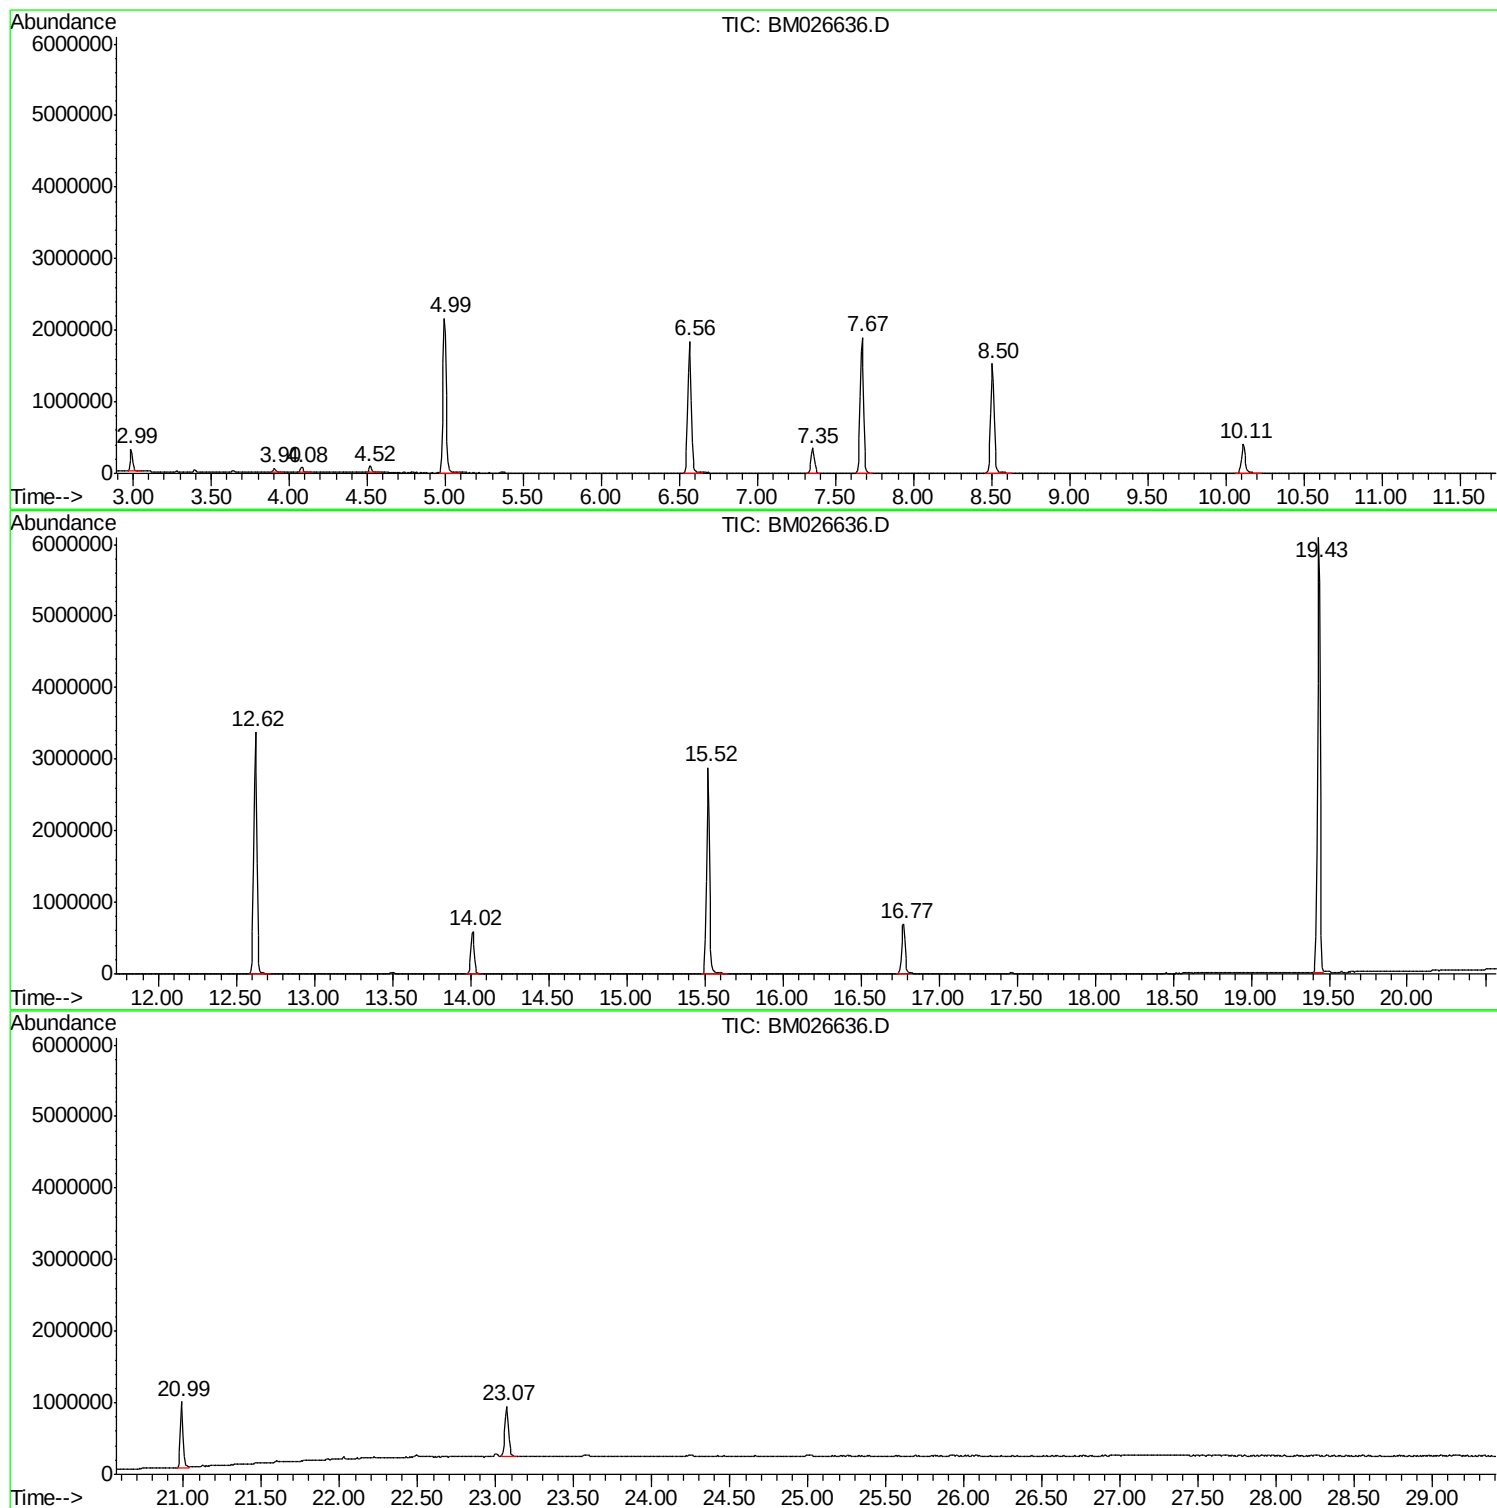

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070120\
Data File : BM026636.D
Acq On : 01 Jul 2020 14:19
Operator : JU/CG
Sample : L2815-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OR-03-062920

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM070120\
Data File : BM026636.D
Acq On : 01 Jul 2020 14:19
Operator : JU/CG
Sample : L2815-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OR-03-062920

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc