


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM070120\
 Data File : BM026627.D
 Acq On : 01 Jul 2020 08:45
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 01 13:20:43 2020

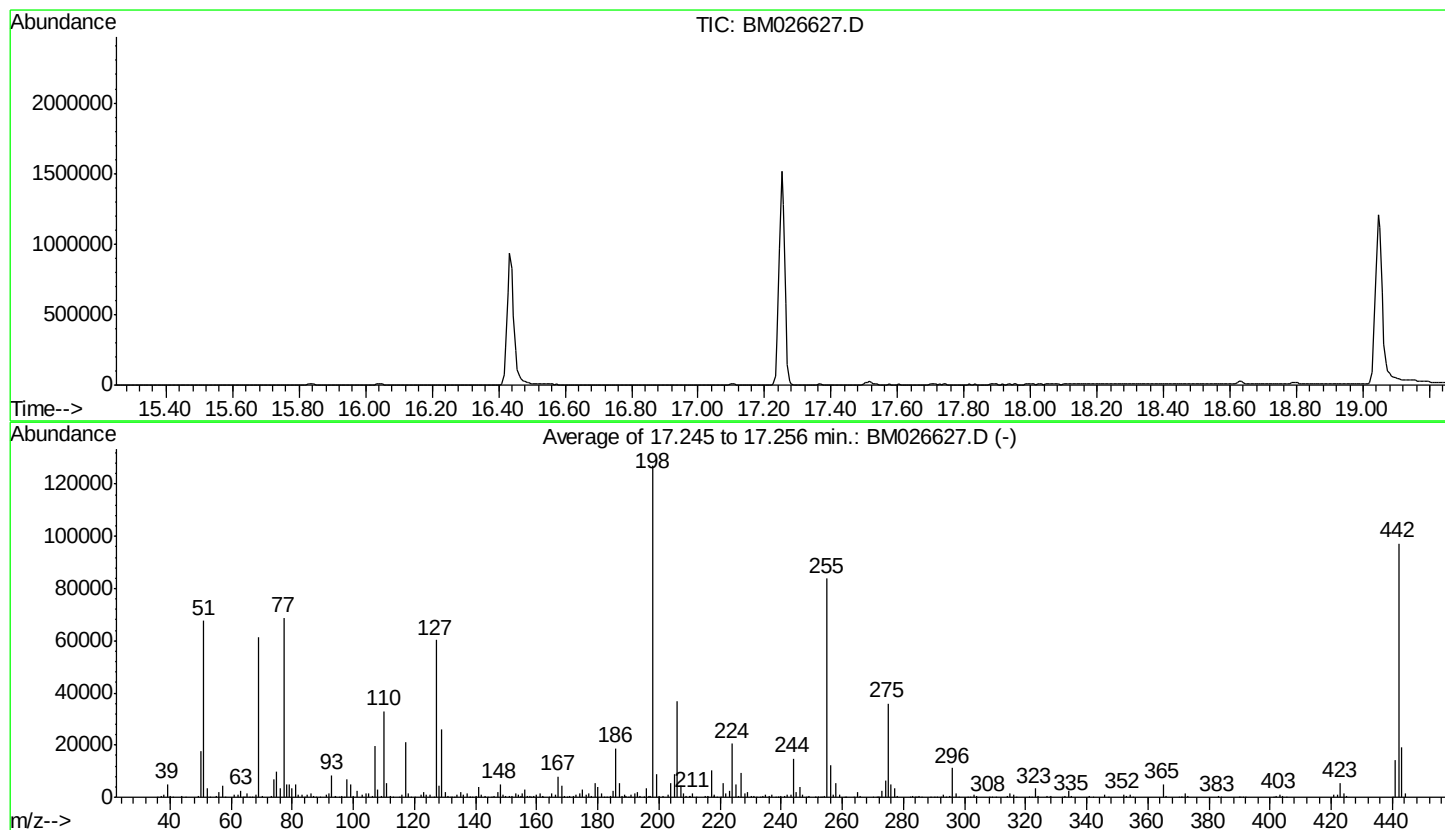

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	67650	PASS
68	69	0.00	2	1.9	1197	PASS
69	198	0.00	100	48.4	61560	PASS
70	69	0.00	2	0.5	314	PASS
127	198	10	80	47.4	60210	PASS
197	198	0.00	2	0.5	604	PASS
198	198	100	100	100.0	127101	PASS
199	198	5	9	6.8	8700	PASS
275	198	10	60	28.3	35954	PASS
365	198	1	100	4.0	5033	PASS
441	198	0.01	100	11.3	14388	PASS
442	198	50	100	76.5	97184	PASS
443	442	15	24	19.6	19092	PASS