
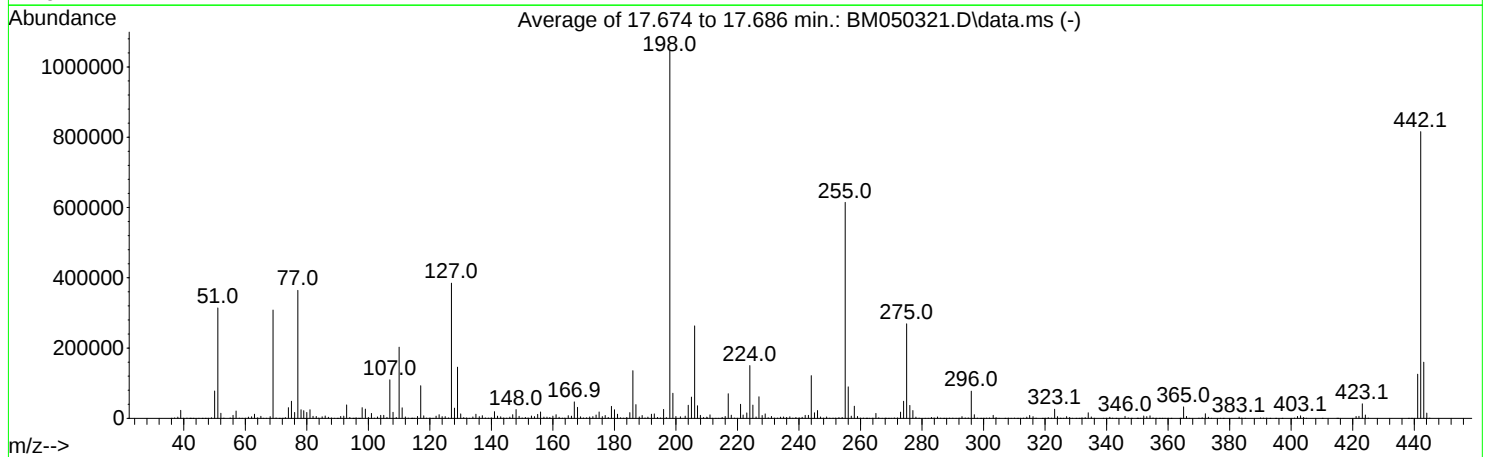


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070125\
Data File : BM050321.D
Acq On : 01 Jul 2025 09:05
Operator : RC/JU
Sample : DFTPP074
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP074

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM070125.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Jul 01 15:14:38 2025

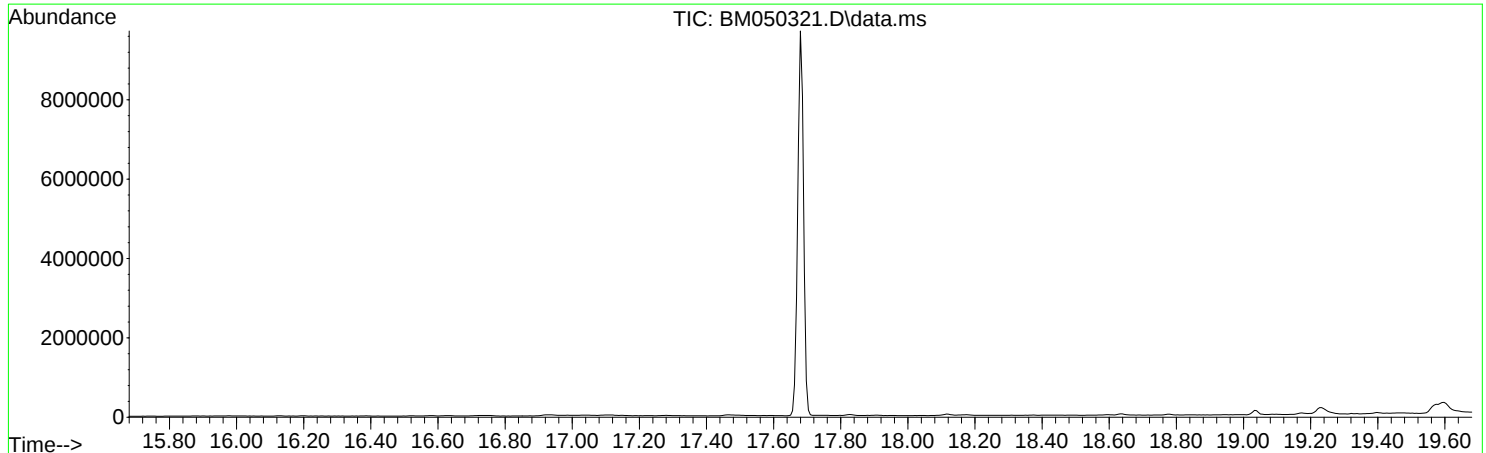

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	314105	PASS
68	69	0.00	2	1.6	4952	PASS
69	198	0.00	100	29.4	308170	PASS
70	69	0.00	2	0.5	1616	PASS
127	198	10	80	36.8	384811	PASS
197	198	0.00	2	0.2	2170	PASS
198	198	100	100	100.0	1046677	PASS
199	198	5	9	6.8	71400	PASS
275	198	10	60	25.7	269120	PASS
365	198	1	100	3.1	32845	PASS
441	198	0.01	100	12.0	125947	PASS
442	198	50	100	77.9	815723	PASS
443	442	15	24	19.6	159963	PASS