

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
 Data File : BM001821.D
 Acq On : 02 Jul 2015 16:20
 Operator : TP/UM
 Sample : G2868-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01M3

Quant Time: Jul 03 02:04:17 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 03 02:02:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	59753	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	243571	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	151608	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	349809	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	423383	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	420669	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	1552	1.24	ng/uL	0.00
5) Phenol-d5	6.83	99	30852	6.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	79125	30.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	89497	24.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	56305	15.28	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	52481	31.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	58099	31.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	109092	27.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	6837	1.70	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	331718	29.51	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	450194	30.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	9729	4.69	ng/ul	0.00
57) Fluorene-d10	15.31	176	324233	31.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	53939	25.24	ng/ul	0.00
70) Anthracene-d10	17.16	188	503206	30.88	ng/ul	0.00
78) Pyrene-d10	19.46	212	587642	32.77	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	560761	30.24	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	2.88	88	4525	3.16 ng/uL#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
Data File : BM001821.D
Acq On : 02 Jul 2015 16:20
Operator : TP/UM
Sample : G2868-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01M3

Quant Time: Jul 03 02:04:17 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 03 02:02:31 2015
Response via : Initial Calibration

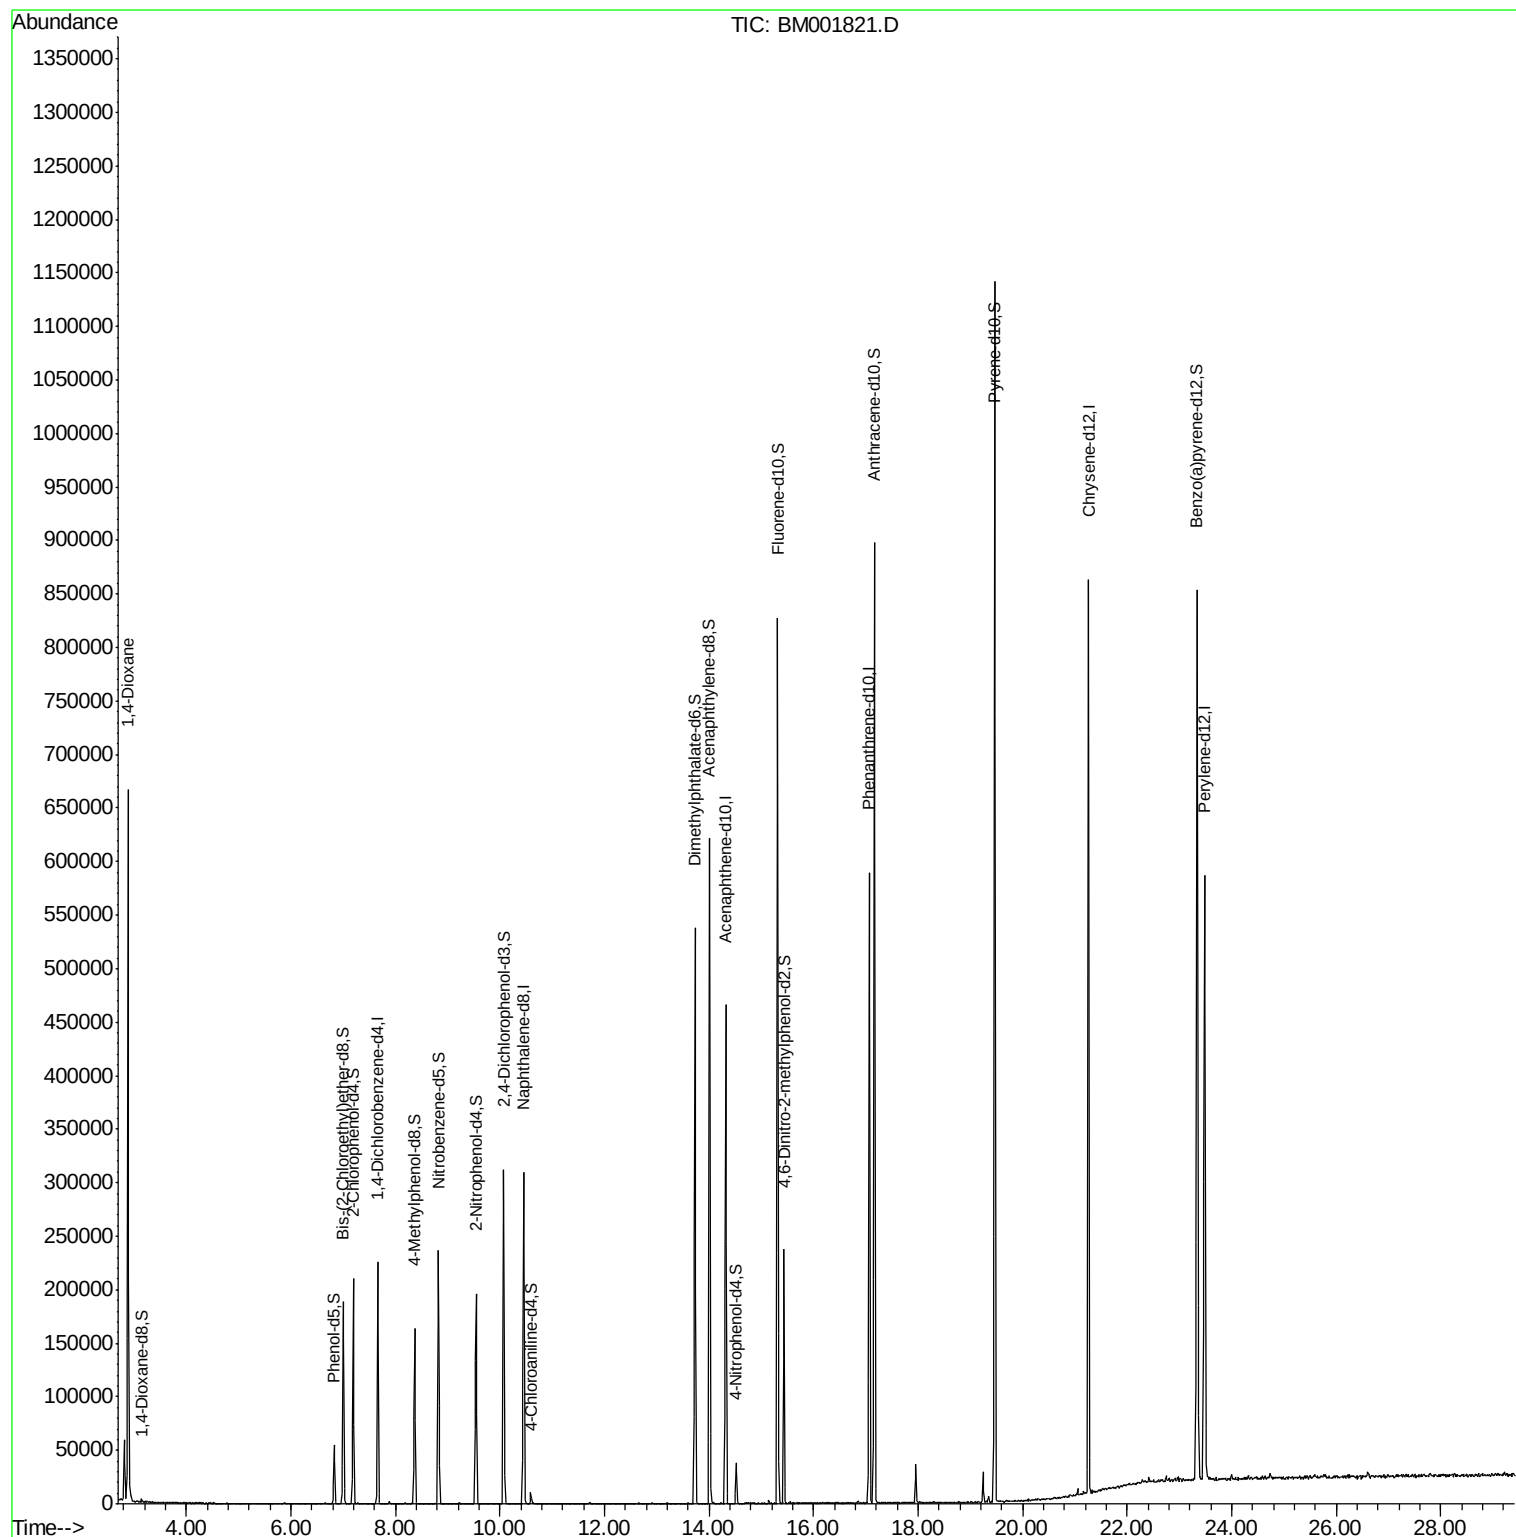

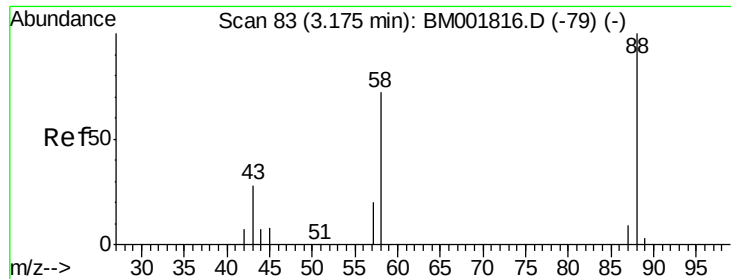

#2

1,4-Dioxane

Concen: 3.16 ng/uL

RT: 2.88 min Scan# 33

Delta R.T. -0.29 min

Lab File: BM001821.D

Acq: 02 Jul 2015 16:20

Instrument :

BNA_M

ClientSampleId :

C01M3



Tgt Ion: 88 Resp: 4525

Ion Ratio Lower Upper

88 100

43 2364.6 24.2 36.4#

58 26.1 56.2 84.2#

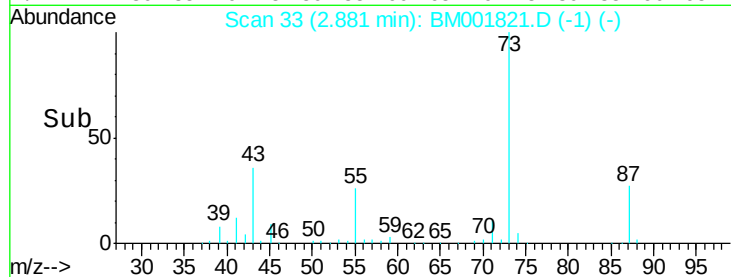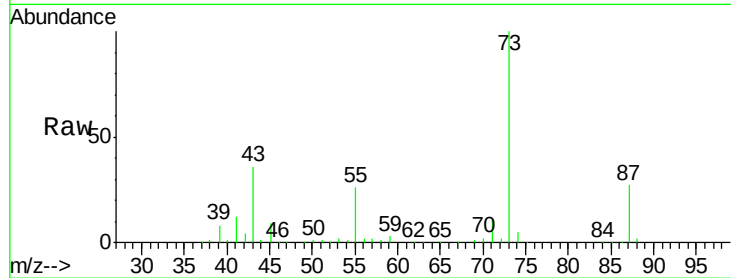

Abundance Ion 88.00 (87.70 to 88.70): BM001821.D (-1) (-)

Ion 43.00 (42.70 to 43.70): BM001821.D (-1) (-)

Ion 58.00 (57.70 to 58.70): BM001821.D (-1) (-)

