

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
 Data File : BM001824.D
 Acq On : 02 Jul 2015 18:09
 Operator : TP/UM
 Sample : G2868-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01M6

Quant Time: Jul 03 02:04:38 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 03 02:02:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	59450	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	241770	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	152033	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	358586	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	422244	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	420759	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	1113	0.89	ng/uL	0.00
5) Phenol-d5	6.82	99	21816	4.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	64925	25.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	74096	20.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	44892	12.25	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	45025	26.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	49545	27.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	94793	24.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	2906	0.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	295546	26.22	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	395106	26.73	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	7128	3.43	ng/ul	0.00
57) Fluorene-d10	15.31	176	294341	28.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	49528	22.61	ng/ul	0.00
70) Anthracene-d10	17.16	188	459780	27.53	ng/ul	0.00
78) Pyrene-d10	19.46	212	526435	29.44	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	488672	26.35	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	2.88	88	3703	2.60 ng/uL#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
Data File : BM001824.D
Acq On : 02 Jul 2015 18:09
Operator : TP/UM
Sample : G2868-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01M6

Quant Time: Jul 03 02:04:38 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 03 02:02:31 2015
Response via : Initial Calibration

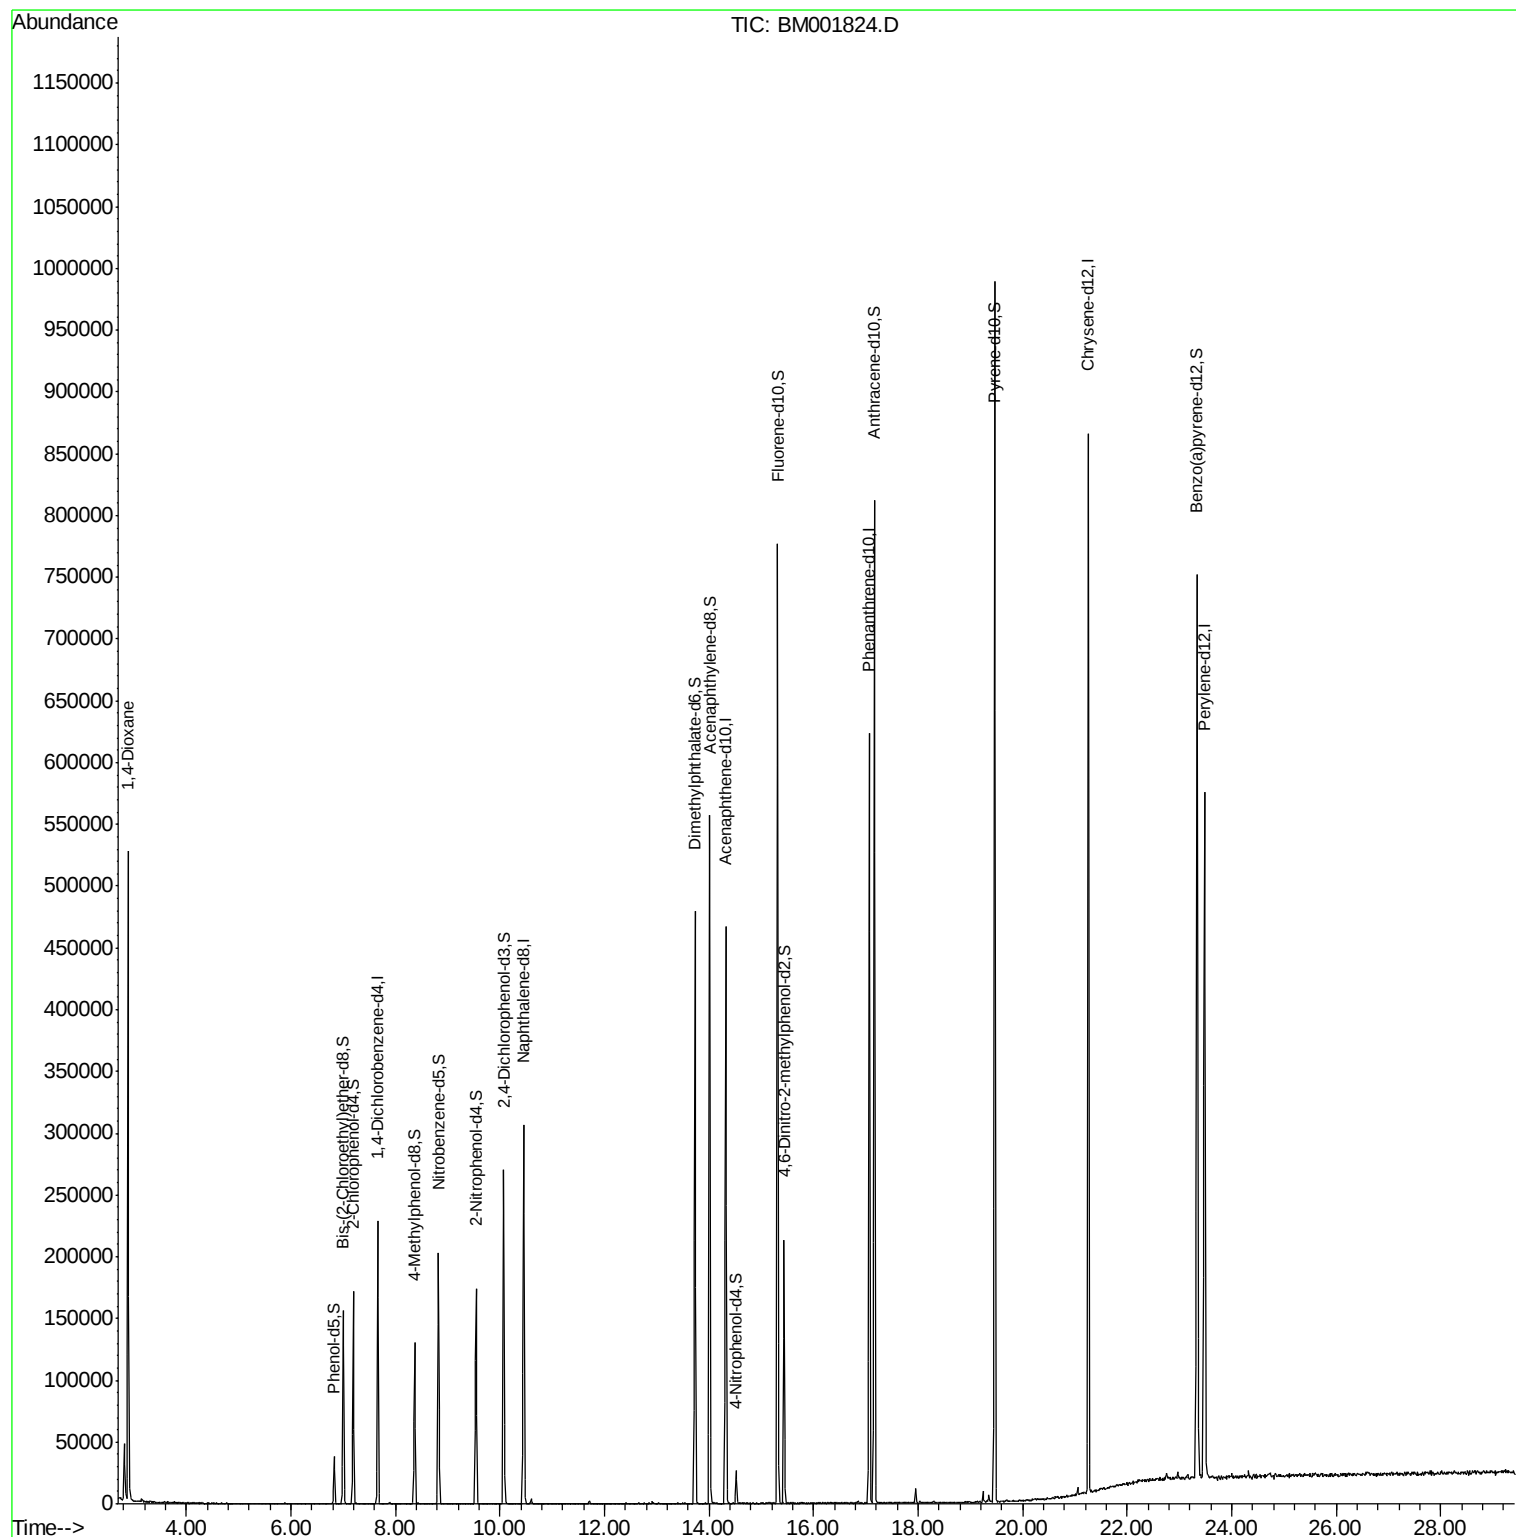

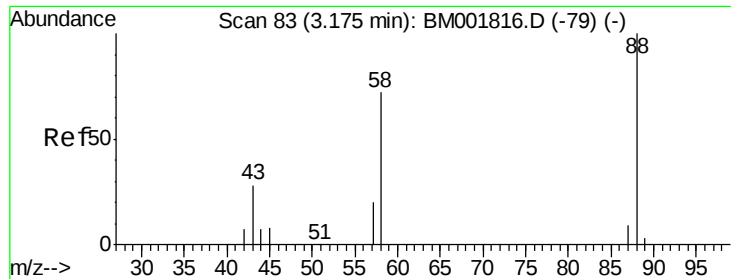

#2

1,4-Dioxane

Concen: 2.60 ng/uL

RT: 2.88 min Scan# 33

Delta R.T. -0.29 min

Lab File: BM001824.D

Acq: 02 Jul 2015 18:09

Instrument :

BNA_M

ClientSampleId :

C01M6



Tgt Ion: 88 Resp: 3703

Ion Ratio Lower Upper

88 100

43 2255.1 24.2 36.4#

58 30.7 56.2 84.2#

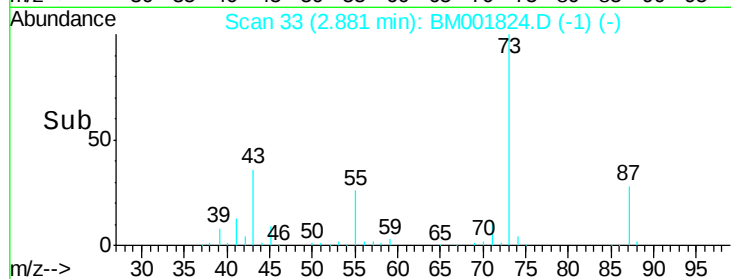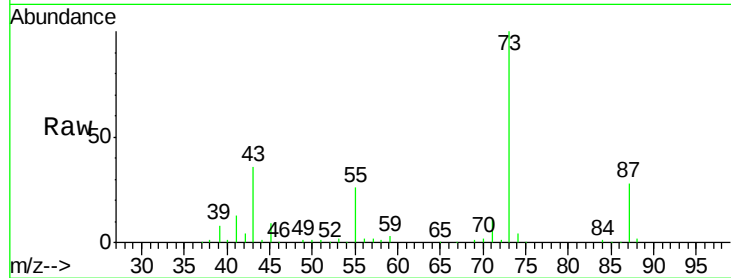

Abundance Ion 88.00 (87.70 to 88.70): BM001824.D (-1) (-)

Ion 43.00 (42.70 to 43.70): BM001824.D (-1) (-)

Ion 58.00 (57.70 to 58.70): BM001824.D (-1) (-)

