

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
 Data File : BM001825.D
 Acq On : 02 Jul 2015 18:45
 Operator : TP/UM
 Sample : G2868-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C01M7

Quant Time: Jul 03 02:04:45 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 03 02:02:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	60495	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	247118	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	155784	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	362651	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	426535	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	422350	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	1432	1.13	ng/uL	0.00
5) Phenol-d5	6.83	99	24078	5.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	64032	24.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	73760	20.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	45851	12.29	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	44090	25.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	49344	26.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	90487	22.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	7407	1.82	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	282546	24.46	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	374841	24.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	7894	3.70	ng/ul	0.00
57) Fluorene-d10	15.31	176	276665	25.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	46270	20.89	ng/ul	0.00
70) Anthracene-d10	17.16	188	426402	25.24	ng/ul	0.00
78) Pyrene-d10	19.46	212	483736	26.78	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	464735	24.96	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	2.88	88	4052	2.80 ng/uL#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
Data File : BM001825.D
Acq On : 02 Jul 2015 18:45
Operator : TP/UM
Sample : G2868-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C01M7

Quant Time: Jul 03 02:04:45 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 03 02:02:31 2015
Response via : Initial Calibration

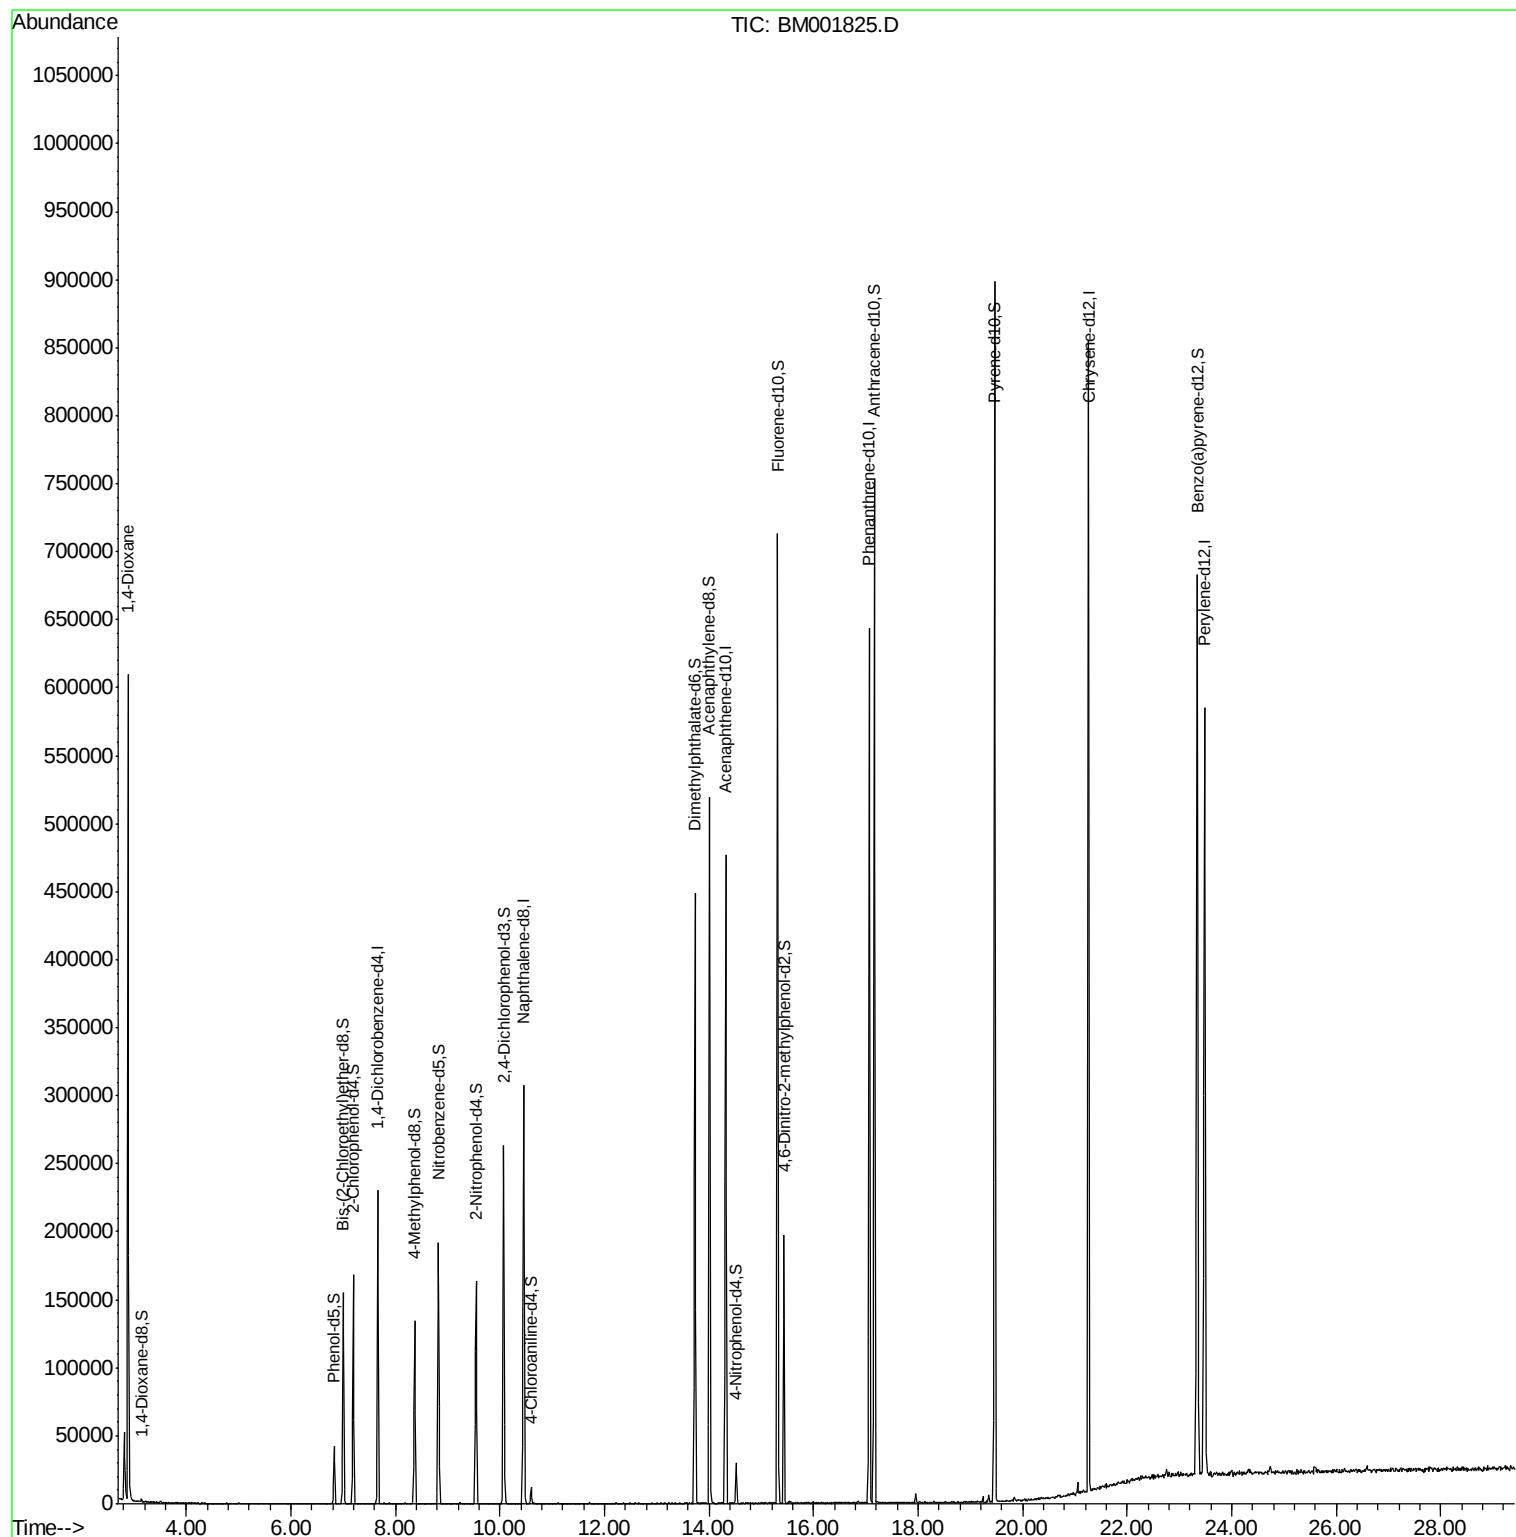

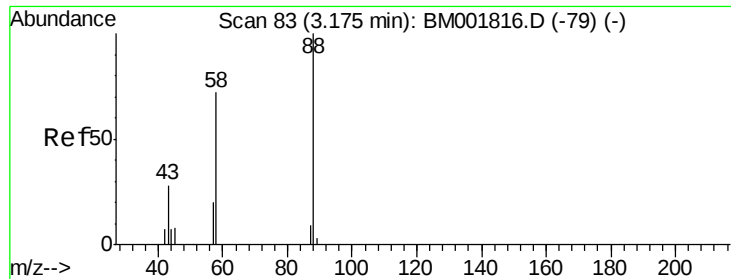

#2

1,4-Dioxane

Concen: 2.80 ng/uL

RT: 2.88 min Scan# 33

Delta R.T. -0.29 min

Lab File: BM001825.D

Acq: 02 Jul 2015 18:45

Instrument :

BNA_M

ClientSampleId :

C01M7

Tgt Ion: 88 Resp: 4052

Ion Ratio Lower Upper

88 100

43 2391.4 24.2 36.4#

58 31.8 56.2 84.2#

