

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
 Data File : BM001826.D
 Acq On : 02 Jul 2015 19:21
 Operator : TP/UM
 Sample : G2860-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G93H8

Quant Time: Jul 03 02:04:52 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 03 02:02:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	47562	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	198964	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	124014	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	279858	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	337076	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	370861	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	2879	2.89	ng/uL	0.00
5) Phenol-d5	6.83	99	55477	15.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	32601	15.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	45691	15.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	37018	12.62	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	20129	14.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	24212	16.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	46738	14.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	42285	12.89	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	130623	14.20	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	163671	13.58	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	17407	10.26	ng/ul	0.00
57) Fluorene-d10	15.31	176	121247	14.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	16446	9.62	ng/ul	0.00
70) Anthracene-d10	17.16	188	177333	13.60	ng/ul	0.00
78) Pyrene-d10	19.46	212	207968	14.57	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	213635	13.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
14) Acetophenone	8.48	105	12737	2.74	ng/ul	99
44) Dimethylphthalate	13.77	163	37444	3.73	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
Data File : BM001826.D
Acq On : 02 Jul 2015 19:21
Operator : TP/UM
Sample : G2860-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G93H8

Quant Time: Jul 03 02:04:52 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 03 02:02:31 2015
Response via : Initial Calibration

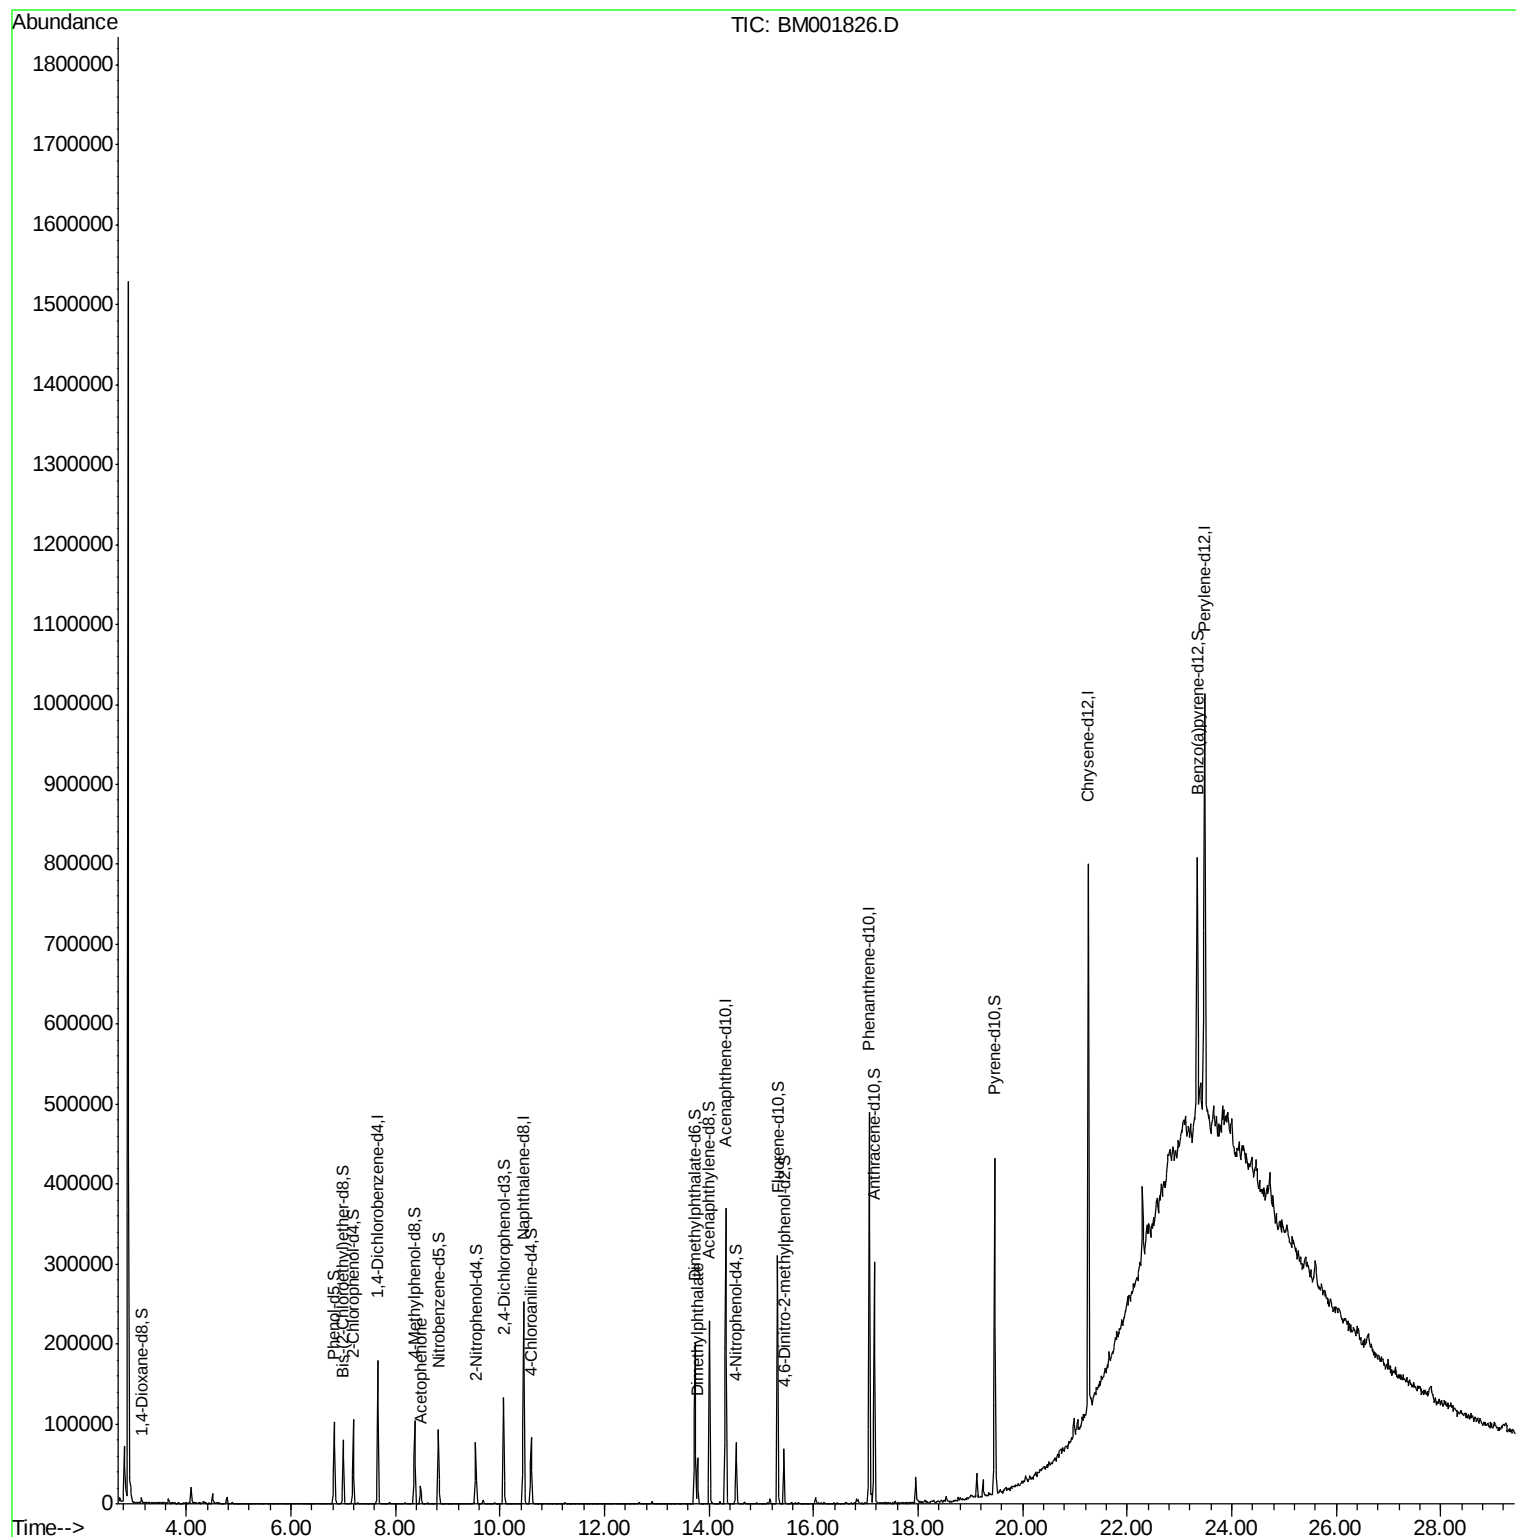

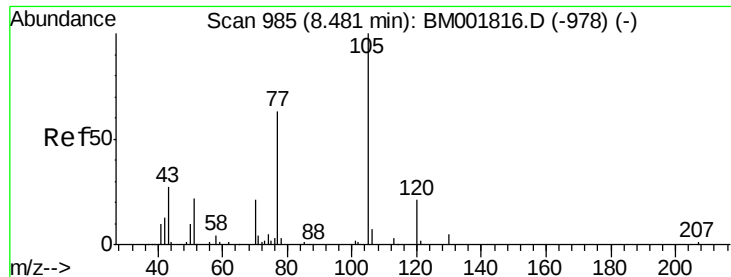

#14

Acetophenone

Concen: 2.74 ng/ul

RT: 8.48 min Scan# 985

Delta R.T. -0.00 min

Lab File: BM001826.D

Acq: 02 Jul 2015 19:21

Instrument :

BNA_M

ClientSampled :

G93H8


Tgt Ion:105 Resp: 12737

Ion Ratio Lower Upper

105 100

77 81.0 64.2 96.4




51 26.7 22.0 33.0

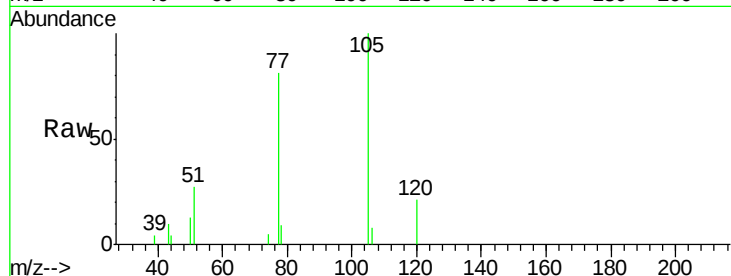

Abundance Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BM0

Ion 51.00 (50.70 to 51.70): BM0

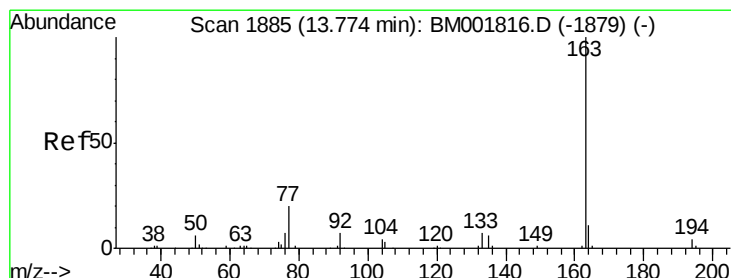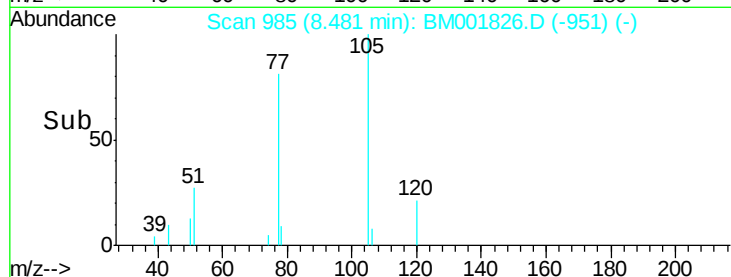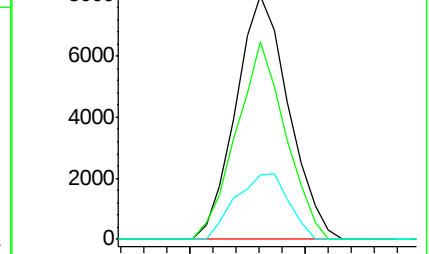

#44

Dimethylphthalate

Concen: 3.73 ng/ul

RT: 13.77 min Scan# 1885

Delta R.T. -0.00 min

Lab File: BM001826.D

Acq: 02 Jul 2015 19:21


Tgt Ion:163 Resp: 37444

Ion Ratio Lower Upper

163 100

194 4.6 3.6 5.4

164 9.5 8.0 12.0

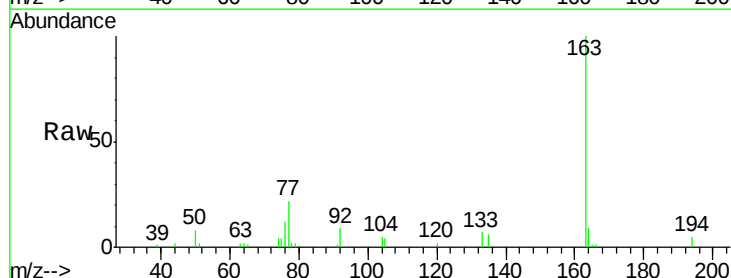

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

