

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
 Data File : BM001818.D
 Acq On : 02 Jul 2015 14:32
 Operator : TP/UM
 Sample : G2860-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 G93K4

Quant Time: Jul 03 02:03:56 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 03 02:02:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	58886	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	234387	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	144645	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	337416	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	414710	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	431576	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	3926	3.18	ng/uL	0.00
5) Phenol-d5	6.83	99	78713	17.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	44301	17.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	64139	17.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	63811	17.58	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	28703	17.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	31900	17.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	66626	17.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	83676	21.66	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	203341	18.96	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	244995	17.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	31305	15.82	ng/ul	0.00
57) Fluorene-d10	15.31	176	184373	18.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	21770	10.56	ng/ul	0.00
70) Anthracene-d10	17.16	188	293143	18.65	ng/ul	0.00
78) Pyrene-d10	19.46	212	334953	19.07	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	318313	16.73	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.77	163	66819	5.70	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
Data File : BM001818.D
Acq On : 02 Jul 2015 14:32
Operator : TP/UM
Sample : G2860-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
G93K4

Quant Time: Jul 03 02:03:56 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 03 02:02:31 2015
Response via : Initial Calibration

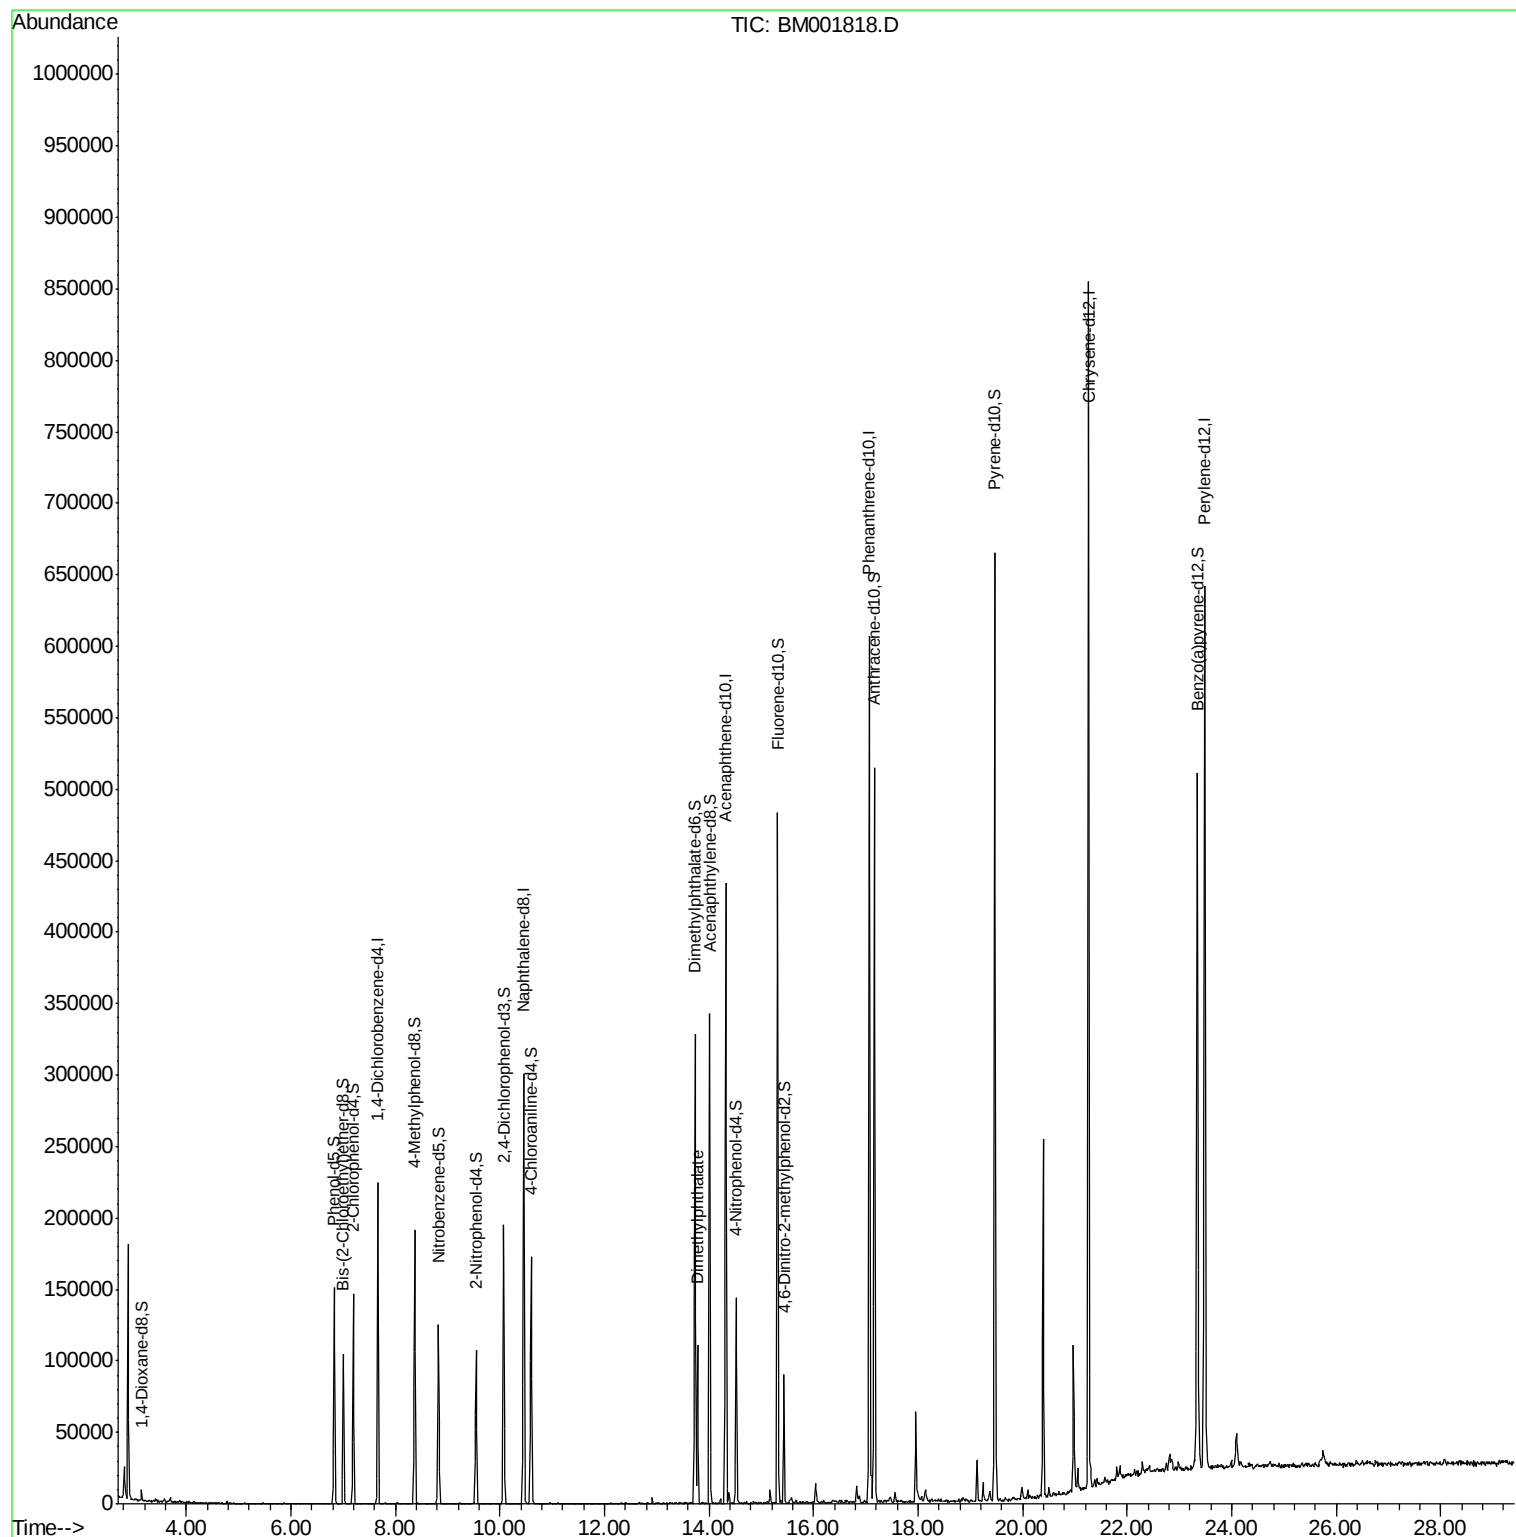

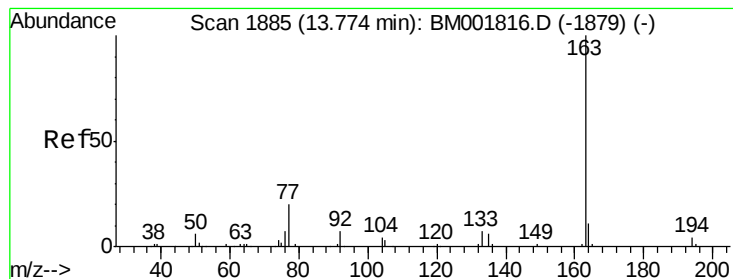

#44

Dimethylphthalate

Concen: 5.70 ng/ul

RT: 13.77 min Scan# 1885

Delta R.T. -0.00 min

Lab File: BM001818.D


Acq: 02 Jul 2015 14:32

Instrument :

BNA_M

ClientSampleId :

G93K4

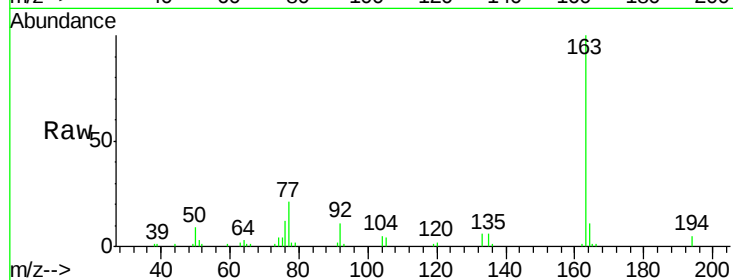


Tgt Ion:163 Resp: 66819

Ion Ratio Lower Upper

163 100

194 4.5 3.6 5.4

164 10.7 8.0 12.0

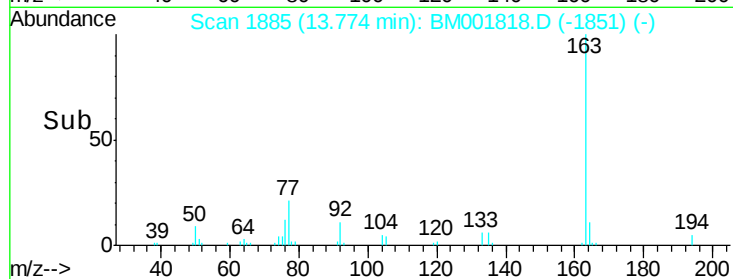

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

