


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070215\
Data File : BM001815.D
Acq On : 02 Jul 2015 11:55
Operator : TP/UM
Sample : DFTPP67
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP67

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
Title : SVOA CALIBRATION
Last Update : Tue Apr 28 06:36:34 2015

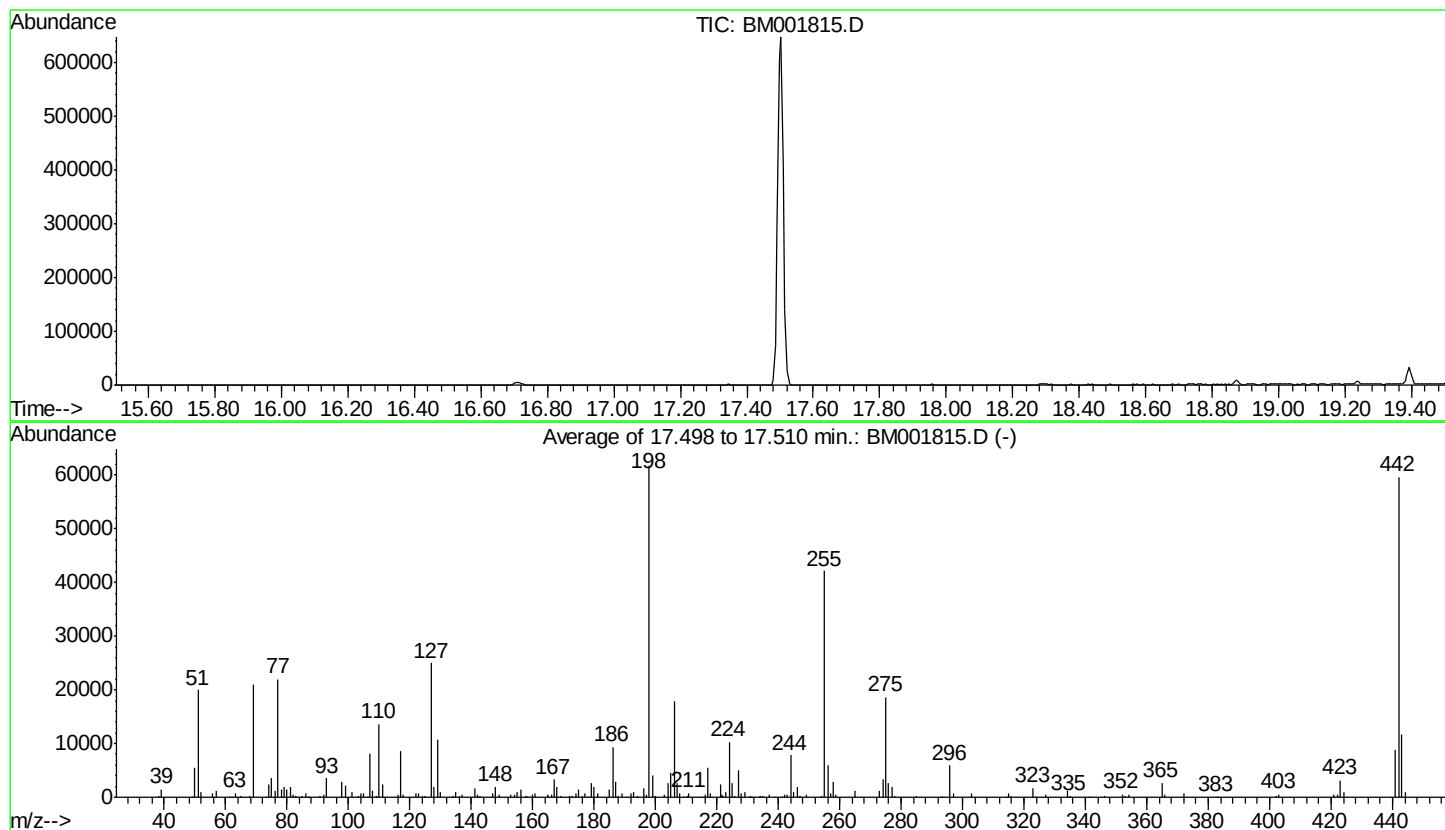

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	19976	PASS
68	69	0.00	2	0.7	141	PASS
69	198	0.00	100	34.0	20995	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.4	24962	PASS
197	198	0.00	2	0.7	440	PASS
198	198	100	100	100.0	61792	PASS
199	198	5	9	6.4	3984	PASS
275	198	10	60	30.1	18624	PASS
365	198	1	100	4.3	2671	PASS
441	443	0.01	100	74.8	8783	PASS
442	198	50	100	96.5	59640	PASS
443	442	15	24	19.7	11744	PASS

m/z	Abundance
38.00	460.0
39.10	1695.0
43.90	541.0
49.10	354.0
50.00	6432.0
51.10	24904.0
52.00	1174.0
55.90	653.0
57.00	1667.0
61.10	356.0
62.00	330.0
63.00	898.0
65.10	455.0
67.90	423.0
69.00	25072.0
74.10	2875.0
75.00	4433.0
76.10	1493.0
77.00	27464.0
78.00	1855.0
79.00	2249.0
80.00	1872.0
81.00	2201.0
82.00	585.0
82.80	399.0
85.00	327.0
86.00	862.0
86.90	356.0
90.90	446.0
92.00	800.0
93.00	4207.0
98.00	3404.0
99.00	2991.0
101.00	1167.0
103.10	495.0
104.00	978.0
104.90	696.0
107.00	9646.0
108.00	1626.0
108.90	388.0
110.00	16008.0
111.00	2604.0
116.00	580.0
117.00	9937.0
117.90	586.0
121.90	699.0
123.00	936.0
124.00	390.0
125.00	411.0
127.00	29024.0
128.00	2631.0
129.00	12556.0
129.90	1178.0
134.00	340.0
135.00	1271.0
136.10	489.0
137.00	669.0
141.00	2177.0
142.00	631.0
142.90	348.0
147.00	959.0
147.90	2455.0
149.00	605.0
153.00	631.0
154.00	432.0
155.00	1046.0
155.90	1504.0
157.90	410.0
159.90	509.0
161.00	885.0
164.90	711.0
166.00	500.0
167.00	3850.0
168.00	2314.0
169.00	425.0
171.90	330.0
172.90	535.0
173.90	640.0
175.00	1637.0
176.90	950.0
179.00	3175.0
179.90	1903.0
181.00	929.0
185.00	1643.0
186.00	10614.0
187.00	3224.0
187.90	406.0
188.90	702.0
190.90	332.0
192.00	935.0
193.00	851.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

194.00	365.0
196.00	1790.0
197.10	469.0
197.90	68304.0
199.00	4822.0
200.00	381.0
202.90	729.0
204.00	2815.0
205.00	4997.0
206.00	19048.0
207.00	2846.0
208.00	685.0
210.30	380.0
210.90	778.0
216.00	481.0
217.00	5581.0
218.00	603.0
221.00	2736.0
221.80	729.0
222.90	1167.0
224.00	11247.0
225.00	2821.0
225.90	348.0
227.00	5401.0
228.00	755.0
228.90	1246.0
233.80	307.0
237.00	764.0
242.00	498.0
242.90	506.0
244.00	8490.0
245.00	1042.0
246.00	1984.0
246.90	485.0
248.90	300.0
254.20	337.0
255.00	43944.0
256.00	7142.0
257.10	614.0
258.00	2789.0
258.90	487.0
265.00	1259.0
273.00	1423.0
274.00	3634.0
275.00	19472.0
276.00	2693.0
276.90	1907.0
277.90	544.0
285.10	324.0
292.90	356.0
296.00	5646.0
296.90	950.0
303.00	630.0
314.90	547.0
316.00	406.0
323.10	1531.0
326.90	338.0
334.00	974.0
334.90	320.0
346.10	332.0
352.00	553.0
354.10	461.0
365.00	2524.0
366.00	384.0
372.00	835.0
403.00	586.0
421.00	319.0
422.00	344.0
423.00	2815.0
424.10	890.0
441.00	7321.0
442.10	53296.0
443.00	10121.0
444.10	822.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

m/z	Abundance
39.10	1667.0
44.00	652.0
50.00	6308.0
51.00	22696.0
52.10	1271.0
55.90	665.0
57.00	1406.0
63.00	911.0
69.00	24248.0
73.10	374.0
74.10	2784.0
75.00	4349.0
76.20	1171.0
77.10	24680.0
78.10	1708.0
79.00	2151.0
80.00	1759.0
81.00	2344.0
81.90	493.0
83.00	544.0
86.00	700.0
87.10	324.0
90.90	540.0
92.00	590.0
93.00	4117.0
98.00	3293.0
99.00	2439.0
100.90	1127.0
103.00	365.0
104.00	834.0
105.00	835.0
106.00	333.0
107.00	9438.0
108.00	1443.0
109.20	326.0
110.00	15857.0
111.00	2826.0
112.00	378.0
115.90	571.0
117.00	9394.0
118.00	649.0
122.00	848.0
123.00	858.0
124.00	473.0
124.90	405.0
127.00	28624.0
128.00	1990.0
129.00	13280.0
130.00	1024.0
134.00	376.0
135.00	997.0
136.00	300.0
137.00	697.0
141.00	1783.0
141.90	658.0
143.00	412.0
147.00	1071.0
147.90	2250.0
149.00	581.0
153.00	513.0
154.00	333.0
155.10	930.0
156.00	1401.0
158.10	377.0
159.90	612.0
160.90	853.0
165.10	612.0
166.10	486.0
167.00	3588.0
168.00	2132.0
169.00	379.0
171.80	462.0
172.90	378.0
173.90	898.0
175.00	1603.0
176.20	405.0
177.00	809.0
177.80	311.0
179.00	2742.0
180.00	2177.0
181.00	755.0
185.00	1634.0
186.00	10943.0
187.00	3178.0
188.90	860.0
191.90	993.0
193.00	1116.0
194.10	310.0
196.00	1947.0
197.00	523.0
198.00	72040.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

198.90	4362.0
199.80	435.0
202.90	566.0
204.00	3028.0
205.00	4780.0
206.10	20984.0
207.00	3521.0
208.00	826.0
209.00	305.0
210.30	453.0
211.00	863.0
214.90	368.0
216.00	487.0
216.90	7053.0
218.10	1118.0
221.00	3371.0
221.80	589.0
223.00	1306.0
224.00	11832.0
225.00	2753.0
226.00	445.0
227.00	6040.0
227.90	935.0
229.00	1073.0
230.90	439.0
234.00	435.0
234.90	422.0
237.00	501.0
238.90	319.0
241.00	340.0
242.00	700.0
243.00	691.0
244.00	8841.0
244.90	1169.0
246.00	2038.0
248.90	464.0
254.10	486.0
255.00	50576.0
256.00	6696.0
257.00	841.0
258.00	3615.0
258.90	529.0
265.00	1168.0
273.00	1272.0
274.00	4164.0
275.00	20864.0
276.00	2998.0
276.90	2361.0
278.00	336.0
285.10	333.0
293.10	315.0
296.00	7335.0
297.00	857.0
303.00	657.0
314.10	334.0
315.00	786.0
316.00	580.0
323.00	1927.0
323.90	329.0
327.00	409.0
334.00	1320.0
334.90	456.0
341.10	341.0
346.00	325.0
351.90	593.0
352.90	411.0
354.10	673.0
365.00	3249.0
366.00	563.0
372.10	980.0
382.80	364.0
402.10	411.0
403.00	699.0
421.00	506.0
422.00	580.0
423.00	3702.0
424.10	1303.0
441.10	10634.0
442.10	69688.0
443.10	14280.0
444.00	1136.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

m/z	Abundance
39.00	950.0
44.00	510.0
50.10	3449.0
51.10	12329.0
52.00	625.0
55.90	548.0
57.00	794.0
63.00	402.0
65.00	304.0
69.00	13666.0
74.00	1561.0
75.00	2309.0
76.10	633.0
77.10	14032.0
78.00	828.0
79.00	1123.0
80.00	847.0
81.00	1217.0
82.00	404.0
85.10	375.0
86.00	491.0
93.10	2289.0
98.00	1741.0
99.00	1333.0
100.90	553.0
103.90	625.0
105.00	550.0
107.00	5442.0
107.90	813.0
110.00	9167.0
111.00	1410.0
117.00	6138.0
117.90	452.0
122.00	478.0
122.90	640.0
127.00	17240.0
128.00	1075.0
129.00	6738.0
130.00	839.0
134.90	715.0
136.80	334.0
141.00	1011.0
141.90	369.0
146.90	479.0
147.90	1391.0
152.80	425.0
153.80	351.0
155.00	818.0
156.10	1072.0
159.70	340.0
161.00	574.0
164.90	544.0
165.90	383.0
166.90	2377.0
168.00	989.0
174.00	598.0
174.90	817.0
176.90	494.0
179.00	2141.0
179.90	1359.0
181.00	604.0
184.90	1285.0
186.00	6508.0
187.10	2019.0
189.00	539.0
192.00	593.0
193.00	590.0
196.10	1452.0
197.10	330.0
197.90	45032.0
198.90	2768.0
203.90	1894.0
205.00	3517.0
206.00	13851.0
207.00	1665.0
208.00	586.0
210.90	683.0
216.00	388.0
217.00	3934.0
217.90	487.0
221.00	1259.0
222.00	535.0
223.10	562.0
224.00	7837.0
225.10	2019.0
227.00	3830.0
228.00	607.0
229.00	783.0
231.10	381.0
236.90	358.0
242.00	540.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

242.90	349.0
244.00	5960.0
245.00	711.0
246.00	1435.0
249.00	353.0
255.00	32136.0
256.00	4114.0
256.90	444.0
258.00	2341.0
259.00	304.0
264.90	957.0
273.00	1034.0
274.00	2569.0
275.00	15538.0
276.00	1963.0
277.00	1662.0
296.00	4699.0
297.00	717.0
303.10	558.0
314.90	482.0
323.00	1611.0
327.00	389.0
334.00	1123.0
352.10	378.0
354.00	418.0
365.00	2241.0
366.00	320.0
372.10	682.0
403.00	450.0
420.90	400.0
422.00	391.0
423.00	3025.0
424.00	850.0
441.10	8396.0
442.10	55936.0
443.10	10831.0
444.00	1019.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67

m/z	Abundance
44.00	633.0

Instrument :
BNA_M
ClientSampleId :
DFTPP67