

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
 Data File : BM006216.D
 Acq On : 03 Jul 2016 01:20
 Operator : UM/SJ
 Sample : H3797-22
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHS3

Quant Time: Jul 03 01:58:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:59:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	342336	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1589620	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	927284	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	2095096	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1960958	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1639346	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	10836	1.35	ng/uL	0.00
5) Phenol-d5	6.82	99	547797	17.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	359353	19.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	416646	16.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	453367	17.48	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	228528	18.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	258133	17.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	437720	16.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	624508	23.10	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1561795	20.18	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1855948	19.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	219102	14.94	ng/ul	0.00
57) Fluorene-d10	15.30	176	1288897	19.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	164919	13.43	ng/ul	0.00
70) Anthracene-d10	17.14	188	1947782	19.49	ng/ul	0.00
76) Pyrene-d10	19.45	212	2133276	22.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.32	264	1562675	20.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.76	163	489009	6.29	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006216.D
Acq On : 03 Jul 2016 01:20
Operator : UM/SJ
Sample : H3797-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHS3

Quant Time: Jul 03 01:58:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 03 00:59:09 2016
Response via : Initial Calibration

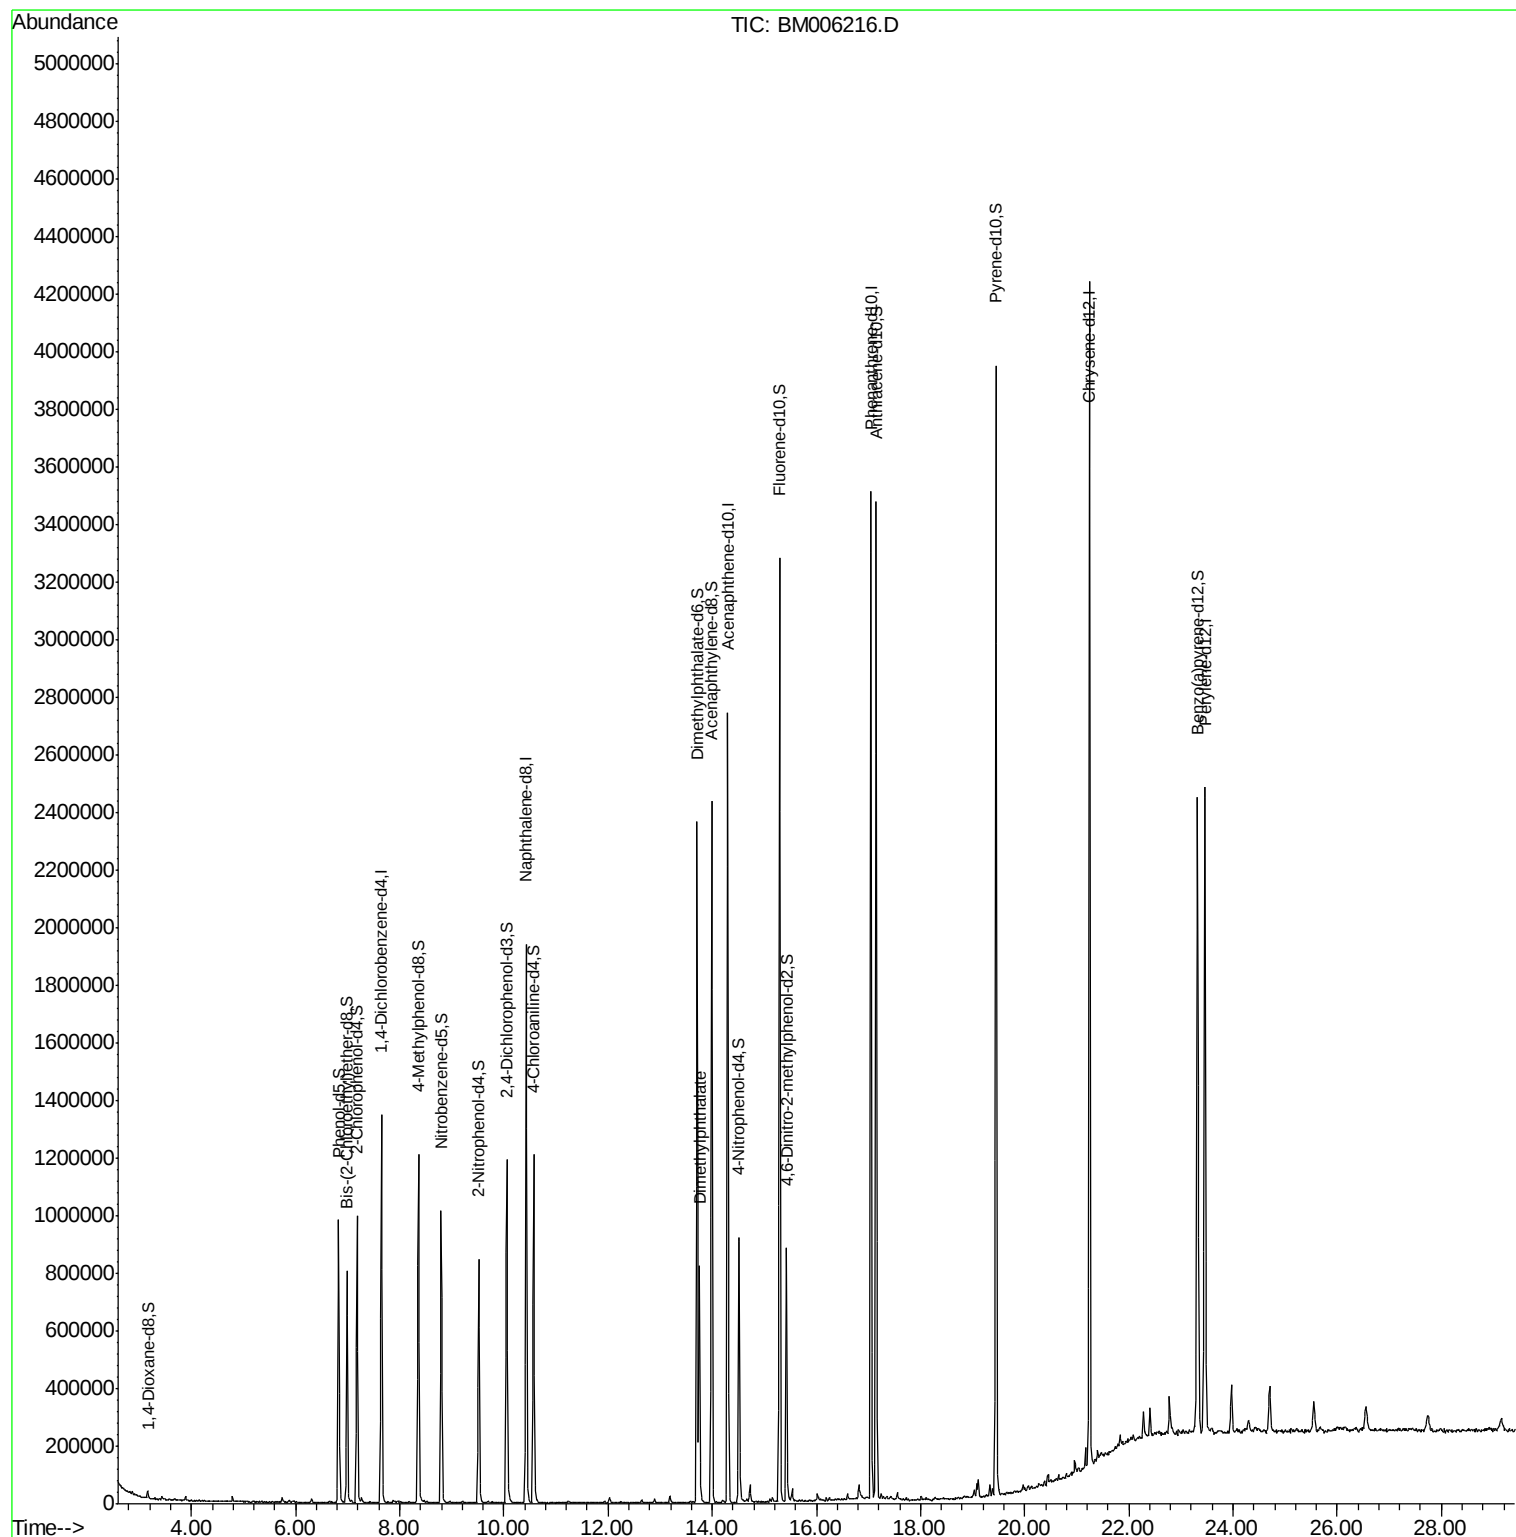

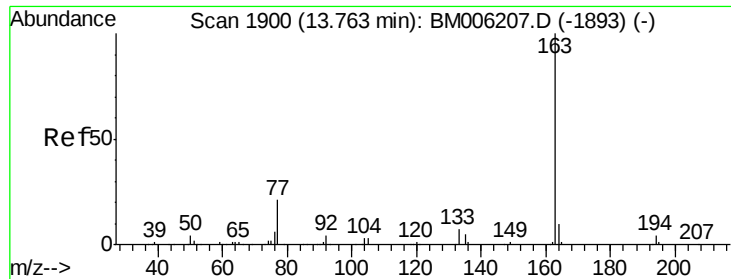

#44

Dimethylphthalate

Concen: 6.29 ng/ul

RT: 13.76 min Scan# 1899

Delta R.T. -0.01 min

Lab File: BM006216.D

Acq: 03 Jul 2016 01:20

Instrument :

BNA_M

ClientSampleId :

BDHS3

Tgt Ion:163 Resp: 489009

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.7 7.8 11.8

