

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
 Data File : BM006221.D
 Acq On : 03 Jul 2016 04:20
 Operator : UM/SJ
 Sample : H3819-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHW2

Quant Time: Jul 03 05:50:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:59:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	301733	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1469665	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	877756	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1866631	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1661799	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1585416	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	15867	2.25	ng/uL	0.00
5) Phenol-d5	6.82	99	714929	25.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	469558	28.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	547607	25.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	595071	26.03	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	294655	25.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	331534	24.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	549530	22.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	802609	32.11	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1794400	24.50	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	2183210	24.07	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	263669	18.99	ng/ul	-0.01
57) Fluorene-d10	15.30	176	1468184	23.25	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	215708	19.72	ng/ul	0.00
70) Anthracene-d10	17.14	188	2120398	23.81	ng/ul	0.00
76) Pyrene-d10	19.45	212	2142750	27.04	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.31	264	1829997	24.84	ng/ul	-0.01

Target Compounds


					Qvalue
44) Dimethylphthalate	13.76	163	289716	3.93	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
 Data File : BM006221.D
 Acq On : 03 Jul 2016 04:20
 Operator : UM/SJ
 Sample : H3819-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 BDHW2

Quant Time: Jul 03 05:50:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:59:09 2016
 Response via : Initial Calibration

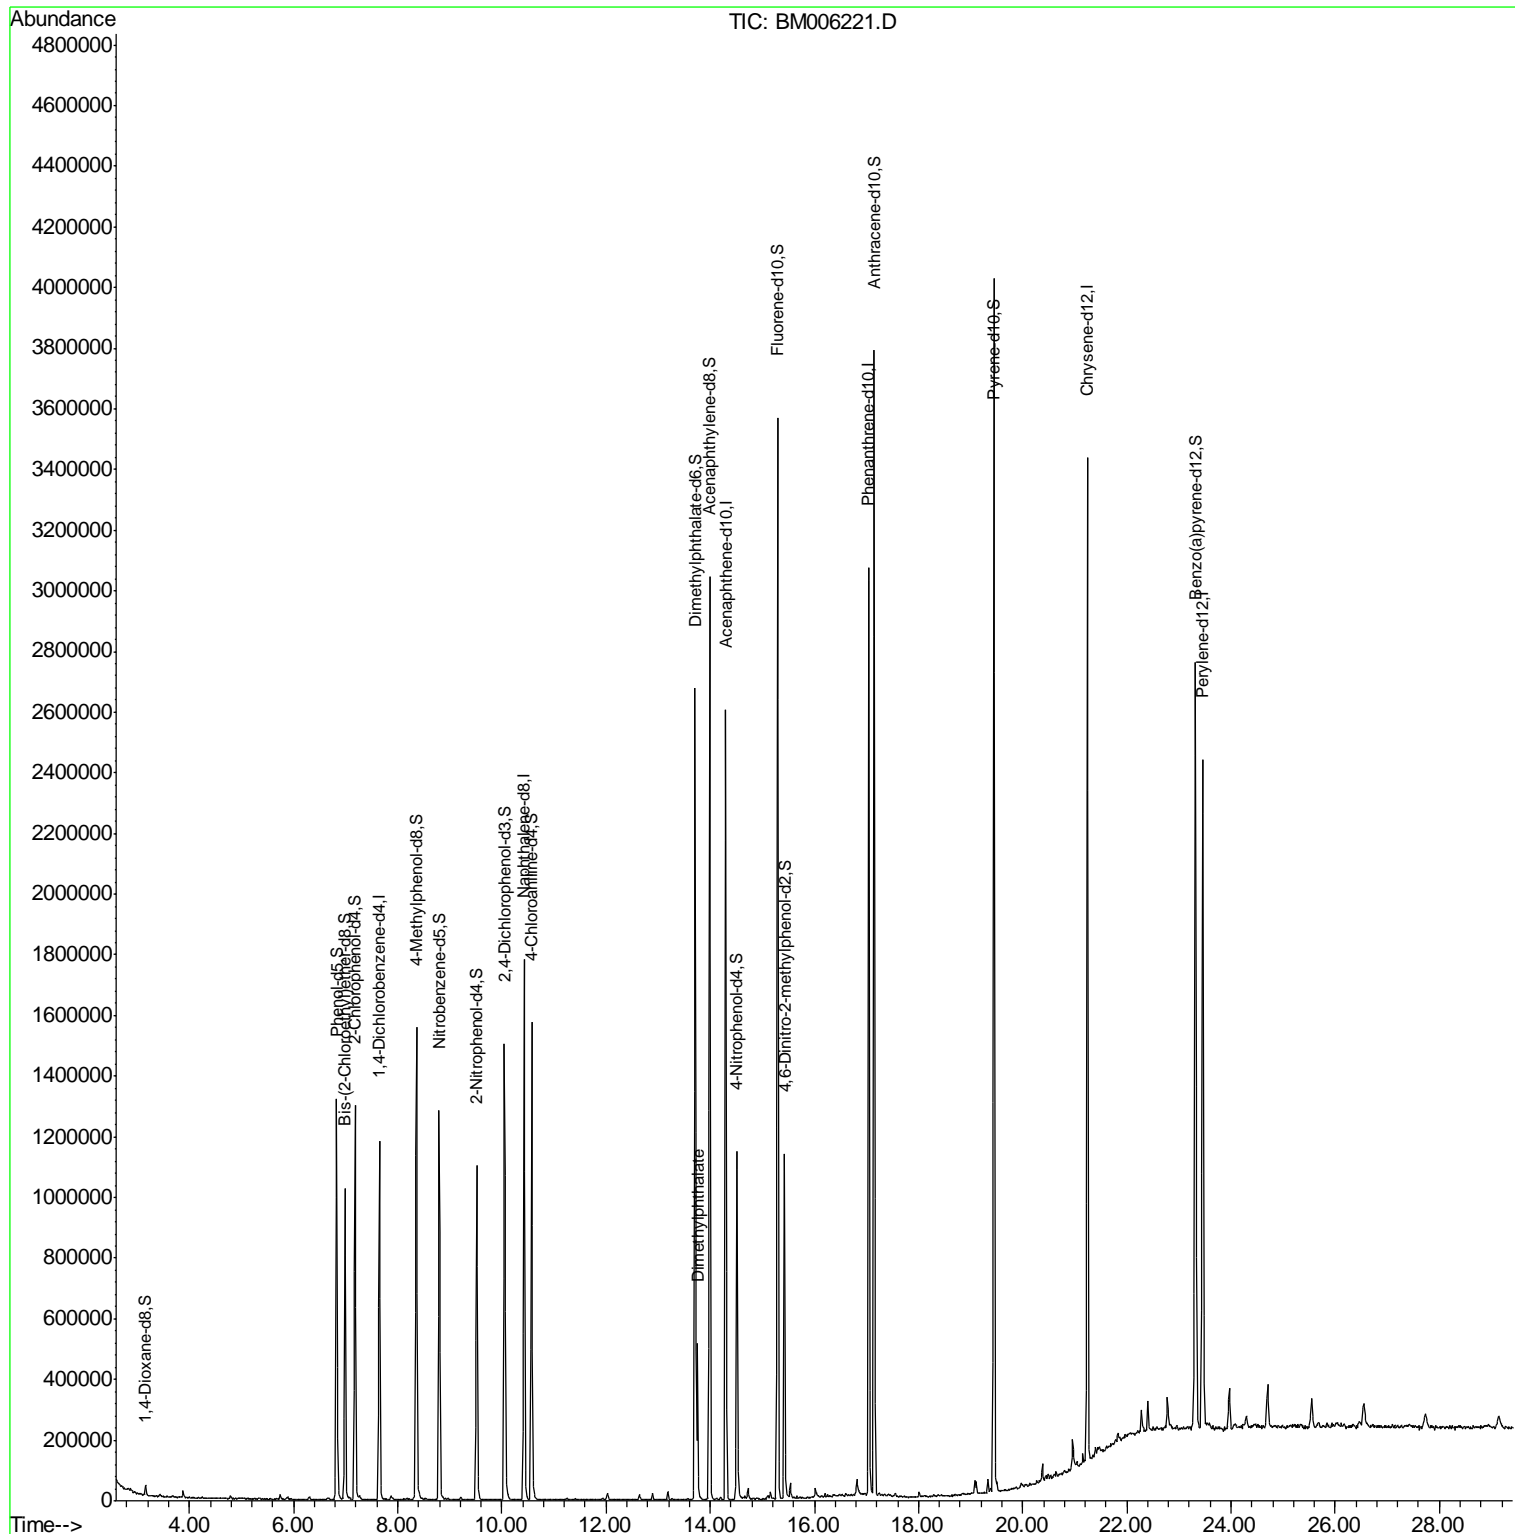

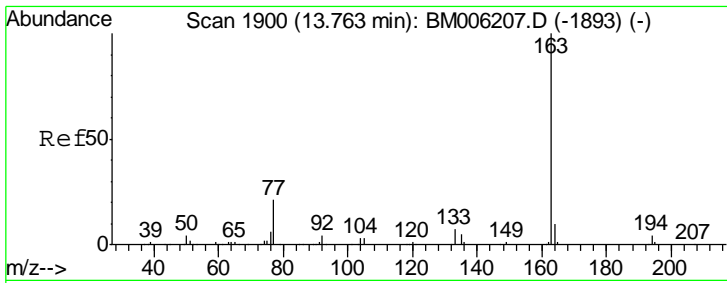

#44
 Dimethylphthalate
 Concen: 3.93 ng/ul
 RT: 13.76 min Scan# 1899
 Delta R.T. -0.01 min
 Lab File: BM006221.D
 Acq: 03 Jul 2016 04:20

Instrument :
 BNA_M
 ClientSampled :
 BDHW2

Tgt Ion:163 Resp: 289716

Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.4	5.0
164	9.9	7.8	11.8

