

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
 Data File : BM006217.D
 Acq On : 03 Jul 2016 01:56
 Operator : UM/SJ
 Sample : H3819-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 03 05:49:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:59:09 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	296310	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1399170	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	843402	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1837056	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1602285	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1473147	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	11110	1.60	ng/uL	0.00
5) Phenol-d5	6.82	99	536356	19.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	351982	21.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	415099	19.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	448298	19.97	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	221602	19.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	247189	19.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	420071	18.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	619900	26.05	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1406220	19.98	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1715264	19.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	190672	14.29	ng/ul	0.00
57) Fluorene-d10	15.30	176	1173933	19.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	144788	13.45	ng/ul	0.00
70) Anthracene-d10	17.14	188	1732106	19.76	ng/ul	0.00
76) Pyrene-d10	19.45	212	1769165	23.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.32	264	1388214	20.28	ng/ul	0.00


Target Compounds						Qvalue
16) 4-Methylphenol	8.41	108	27078	1.13	ng/ul	87
44) Dimethylphthalate	13.76	163	218509	3.09	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006217.D
Acq On : 03 Jul 2016 01:56
Operator : UM/SJ
Sample : H3819-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 03 05:49:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 03 00:59:09 2016
Response via : Initial Calibration




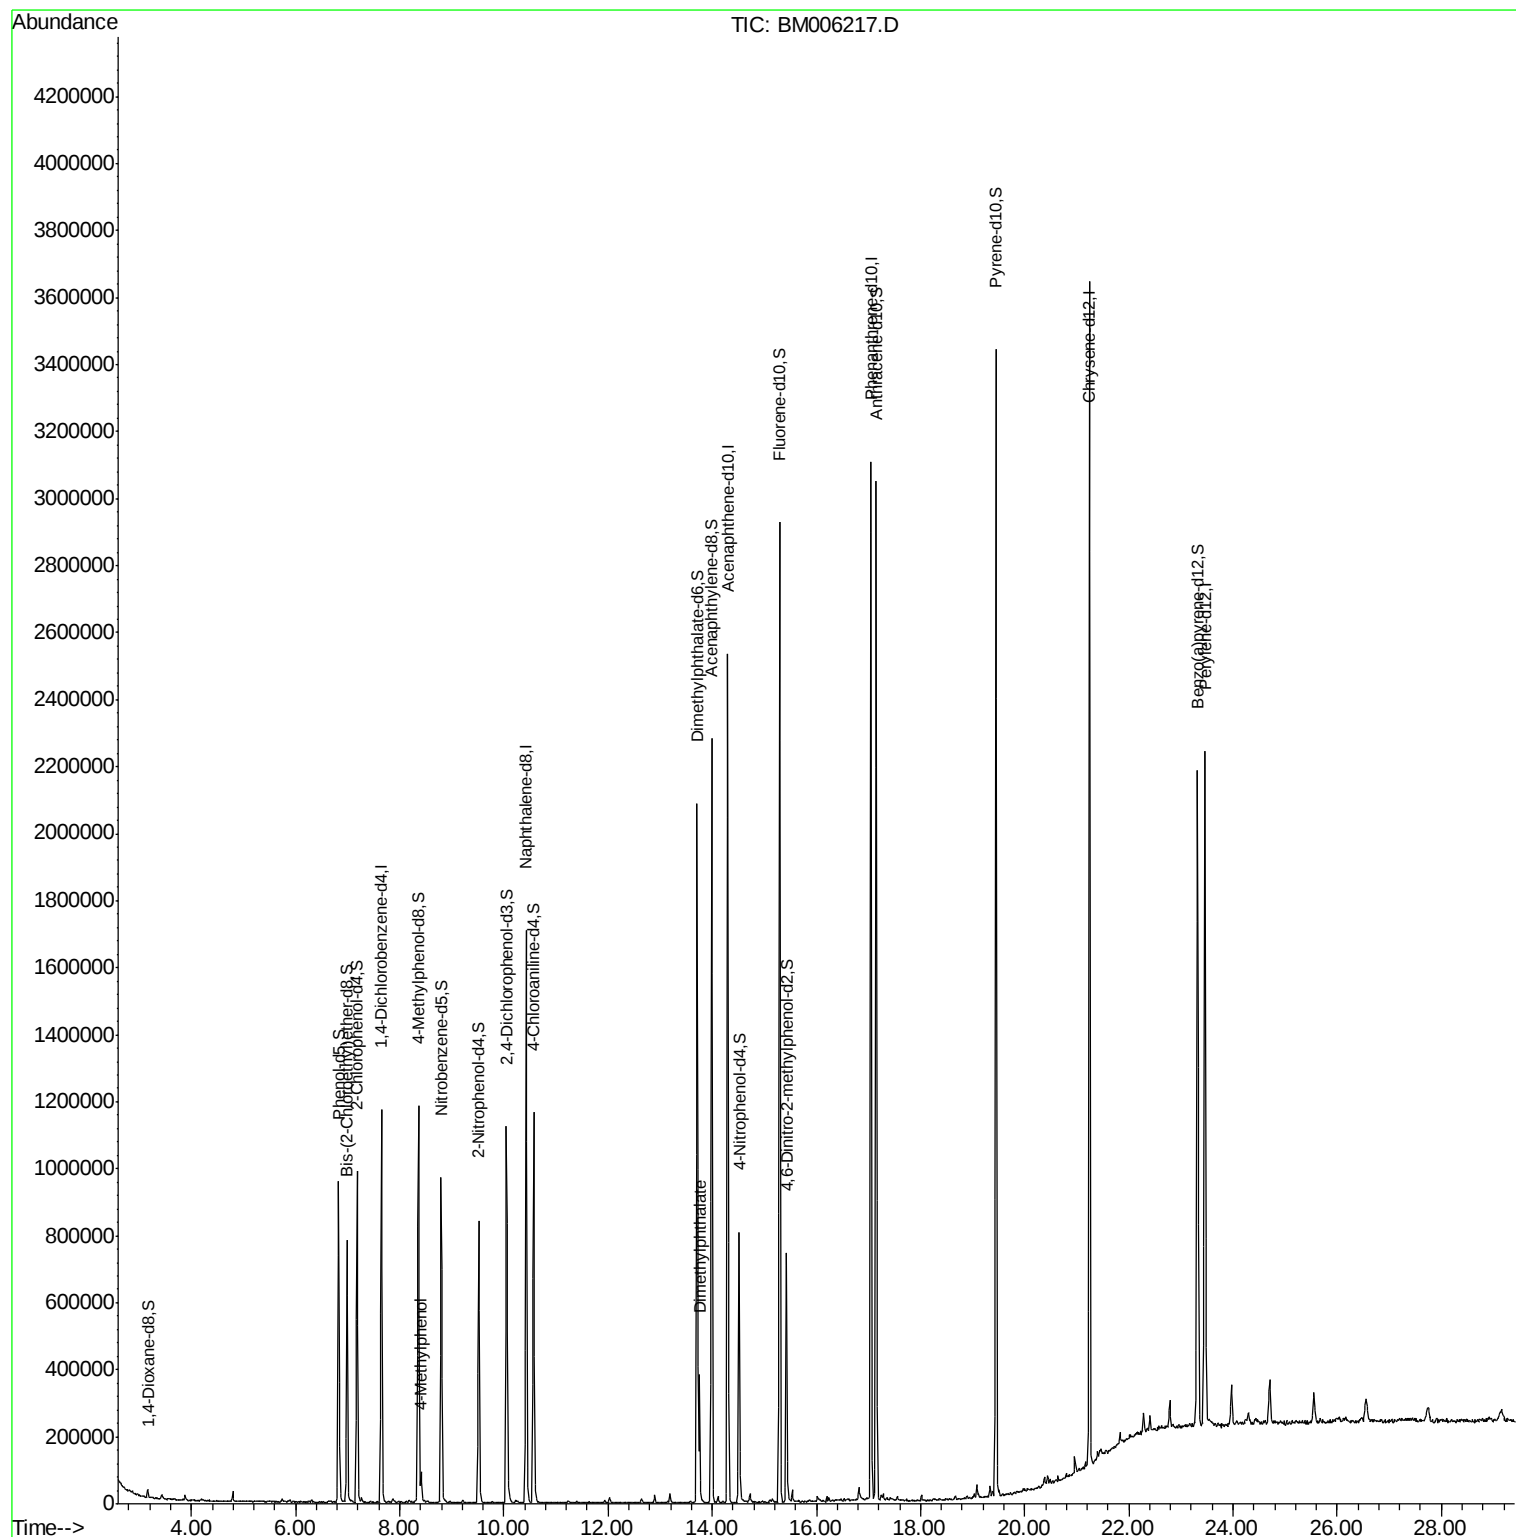


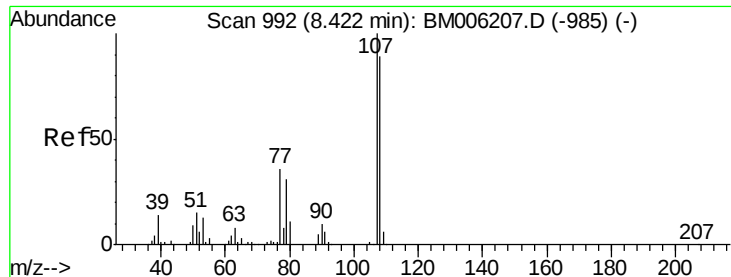

#16
4-Methylphenol
Concen: 1.13 ng/ul
RT: 8.41 min Scan# 990
Delta R.T. -0.01 min
Lab File: BM006217.D
Acq: 03 Jul 2016 01:56

Instrument :
BNA_M
ClientSampleId :
DFTPP

Tgt Ion:108 Resp: 27078
Ion Ratio Lower Upper
108 100
107 122.9 87.4 131.0

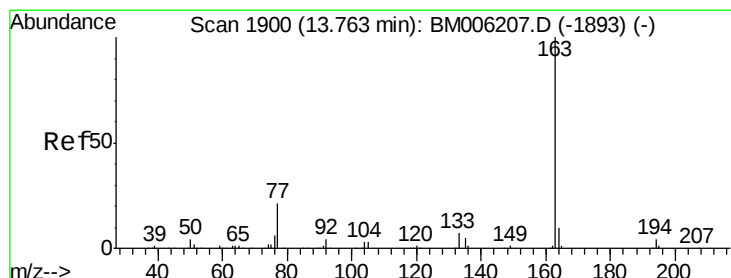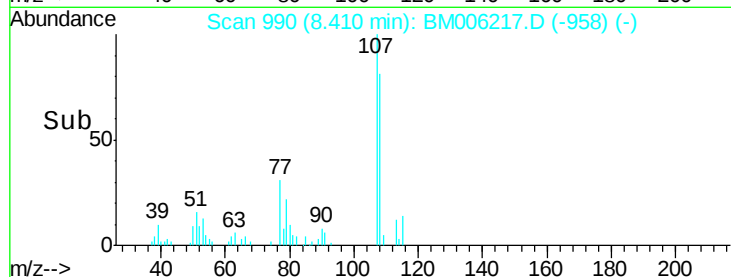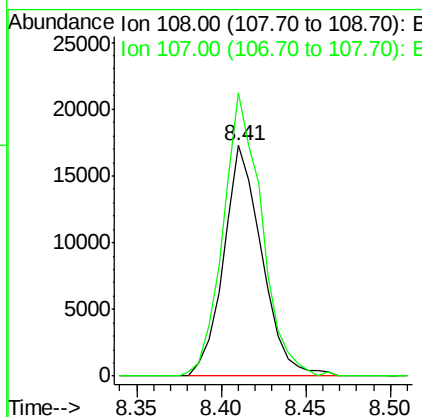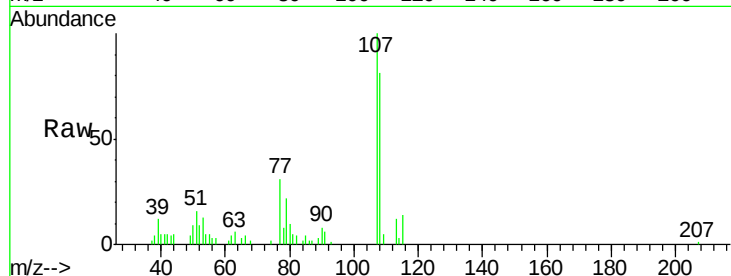

#44
Dimethylphthalate
Concen: 3.09 ng/ul
RT: 13.76 min Scan# 1899
Delta R.T. -0.01 min
Lab File: BM006217.D
Acq: 03 Jul 2016 01:56

Tgt Ion:163 Resp: 218509
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.0
164 9.8 7.8 11.8

