

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
 Data File : BM006200.D
 Acq On : 02 Jul 2016 15:43
 Operator : UM/SJ
 Sample : H3797-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHQ1

Quant Time: Jul 03 00:15:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Jul 03 00:14:45 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	310860	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1419754	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	868951	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1965883	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	2099278	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	1980253	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	12065	1.66	ng/uL	0.00
5) Phenol-d5	6.83	99	594779	20.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	399744	23.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	468039	21.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	496174	21.06	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	252693	22.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	284968	22.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	483096	20.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	708284	29.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1621713	22.36	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	2002008	22.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	200622	14.60	ng/ul	-0.01
57) Fluorene-d10	15.30	176	1390570	22.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	152520	13.24	ng/ul	0.00
70) Anthracene-d10	17.15	188	2124739	22.65	ng/ul	0.00
76) Pyrene-d10	19.45	212	2348678	23.46	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	2132041	23.17	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.76	163	708952	9.73	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006200.D
Acq On : 02 Jul 2016 15:43
Operator : UM/SJ
Sample : H3797-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHQ1

Quant Time: Jul 03 00:15:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Jul 03 00:14:45 2016
Response via : Initial Calibration

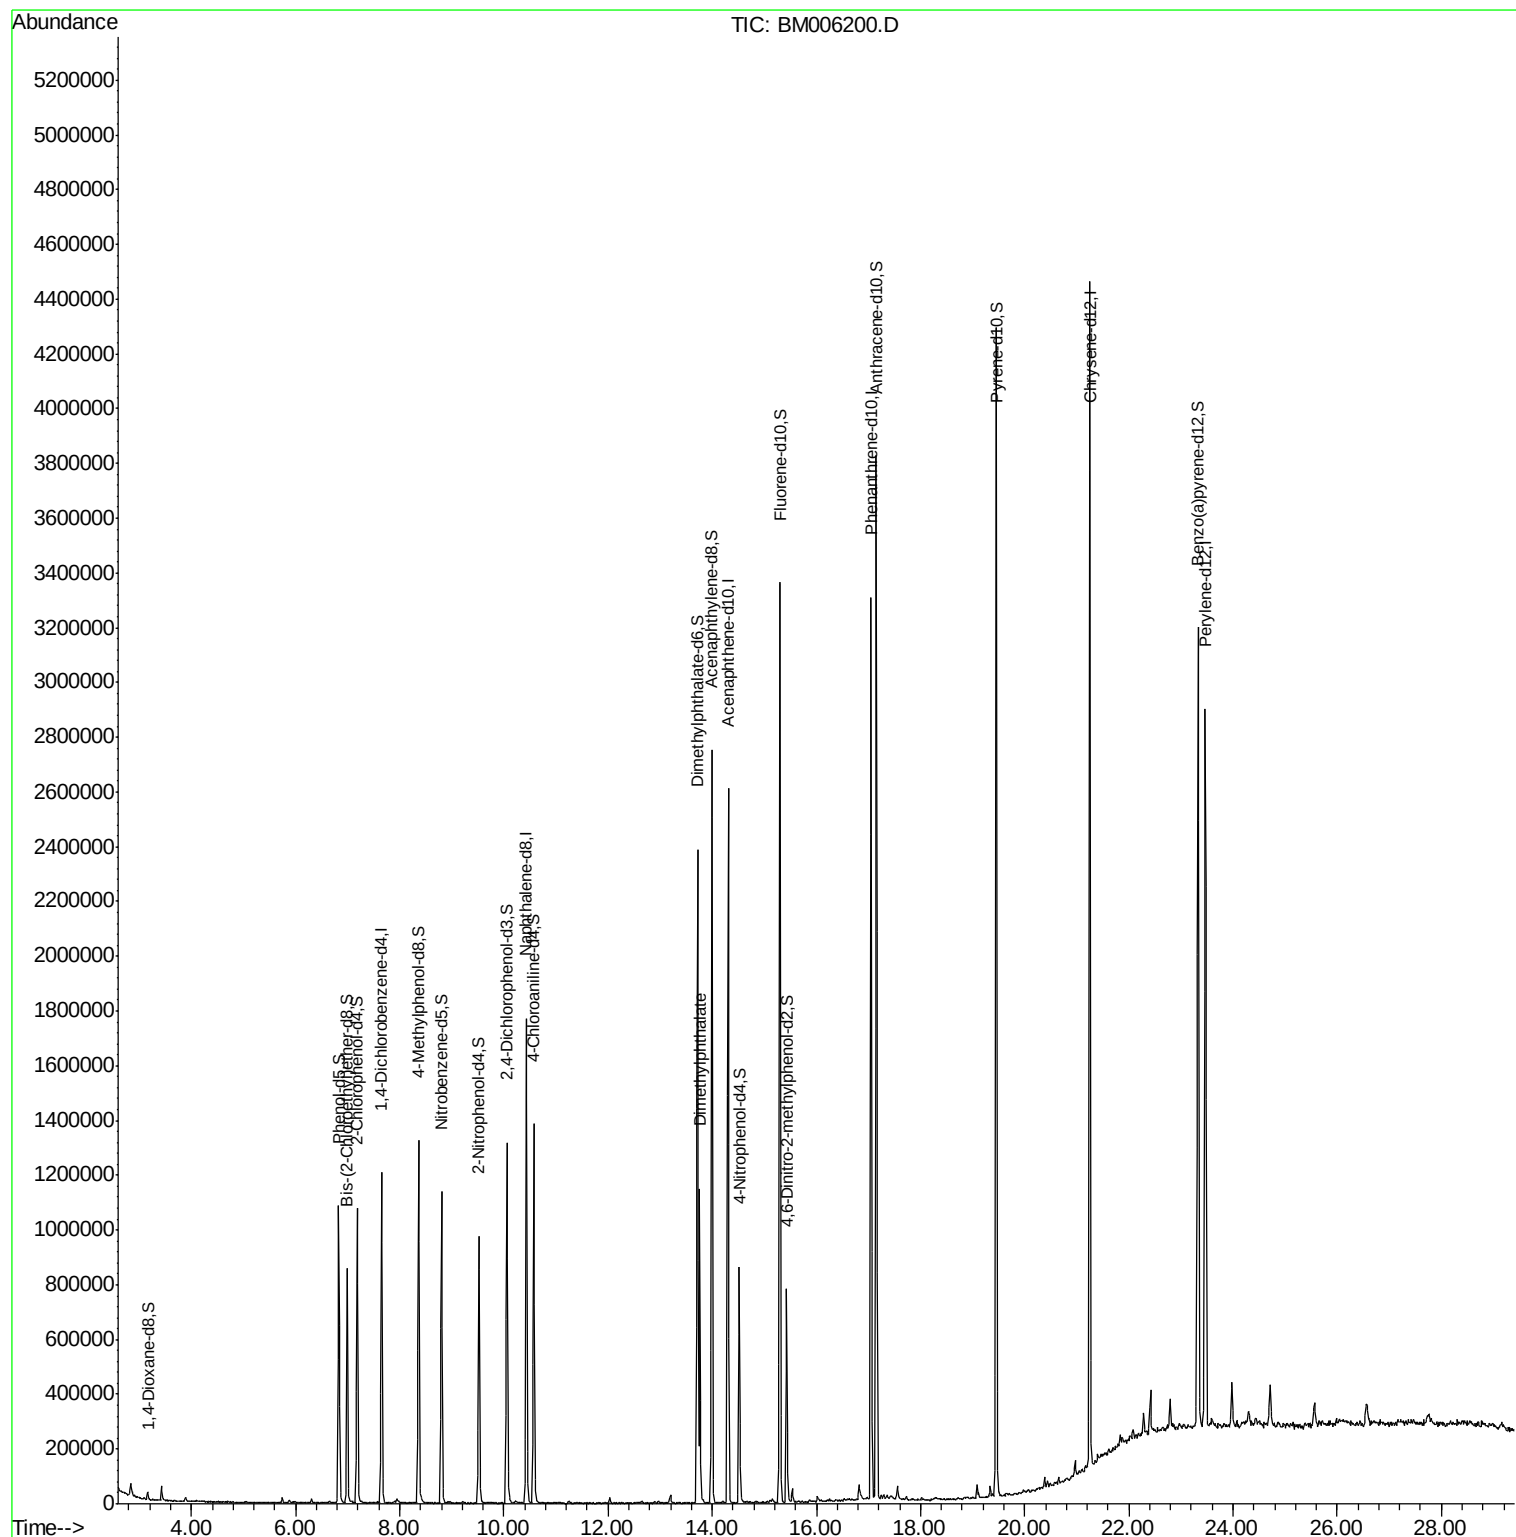

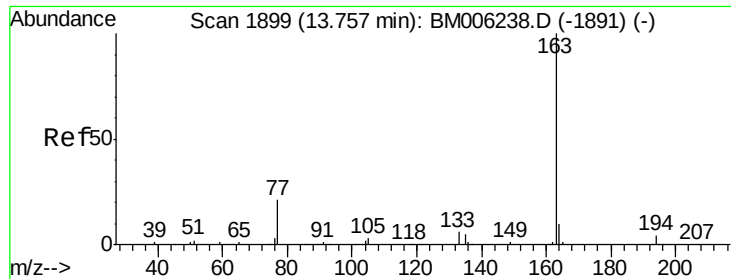

#44

Dimethylphthalate

Concen: 9.73 ng/ul

RT: 13.76 min Scan# 1900

Delta R.T. -0.00 min

Lab File: BM006200.D

Acq: 02 Jul 2016 15:43

Instrument :

BNA_M

ClientSampleId :

BDHQ1


Tgt Ion:163 Resp: 708952

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.0

164 9.9 7.8 11.8

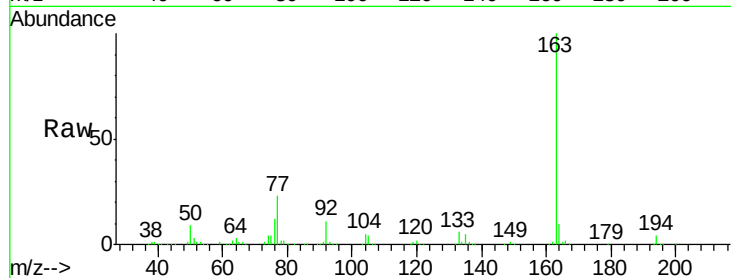

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

