

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
 Data File : BM006216.D
 Acq On : 03 Jul 2016 01:20
 Operator : UM/SJ
 Sample : H3797-22
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHS3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.822	711	720	736	rBV	983215	1720896	29.11%	2.347%
2	6.987	740	748	761	rBV	802859	1250271	21.15%	1.705%
3	7.181	774	781	792	rBV	995645	1605703	27.16%	2.190%
4	7.645	853	860	870	rBV	1348516	2196189	37.14%	2.995%
5	8.357	970	981	995	rBV	1211512	2091436	35.37%	2.853%
6	8.798	1048	1056	1071	rBV	1012660	1736670	29.37%	2.369%
7	9.516	1171	1178	1193	rBV	847761	1502207	25.41%	2.049%
8	10.057	1262	1270	1283	rBV	1191102	2144070	36.26%	2.924%
9	10.428	1325	1333	1349	rBV	1941028	3395269	57.42%	4.631%
10	10.569	1349	1357	1372	rBV	1208198	2211253	37.40%	3.016%
11	13.710	1884	1891	1895	rBV	2362322	3435619	58.11%	4.686%
12	13.757	1895	1899	1916	rVB	822203	1237846	20.94%	1.688%
13	13.992	1929	1939	1951	rBV	2435079	4011508	67.85%	5.471%
14	14.298	1984	1991	2005	rVB2	2745500	4524222	76.52%	6.171%
15	14.510	2021	2027	2044	rBV	921560	1553734	26.28%	2.119%
16	14.727	2057	2064	2069	rBV2	58111	85619	1.45%	0.117%
17	15.298	2154	2161	2171	rBV	3277775	4978867	84.21%	6.791%
18	15.427	2177	2183	2197	rBV	881138	1303116	22.04%	1.777%
19	15.533	2197	2201	2209	rVB2	44912	72482	1.23%	0.099%
20	16.815	2414	2419	2427	rBV4	48951	103041	1.74%	0.141%
21	17.051	2452	2459	2468	rBV2	3495794	5372825	90.87%	7.328%
22	17.145	2468	2475	2485	rVB2	3461697	5207249	88.07%	7.102%
23	19.109	2806	2809	2817	rVB	62532	84544	1.43%	0.115%
24	19.450	2860	2867	2875	rBV2	3922767	5912585	100.00%	8.064%
25	20.962	3121	3124	3132	rBV7	45264	77234	1.31%	0.105%
26	21.162	3155	3158	3162	rBV	65672	73513	1.24%	0.100%
27	21.244	3166	3172	3177	rBV2	4111495	5520020	93.36%	7.529%
28	22.286	3346	3349	3353	rVB2	74588	94485	1.60%	0.129%
29	22.409	3367	3370	3377	rVB	100513	144233	2.44%	0.197%
30	22.780	3430	3433	3440	rBV2	112663	178504	3.02%	0.243%
31	23.321	3517	3525	3537	rVB2	2209542	4505750	76.21%	6.146%
32	23.462	3541	3549	3559	rVB	2230940	4315666	72.99%	5.886%
33	23.974	3631	3636	3645	rVB	164290	323562	5.47%	0.441%
34	24.703	3756	3760	3769	rVB2	157431	346237	5.86%	0.472%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006216.D
Acq On : 03 Jul 2016 01:20
Operator : UM/SJ
Sample : H3797-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHS3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Title : SVOA CALIBRATION


Sum of corrected areas: 73316425

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006216.D
Acq On : 03 Jul 2016 01:20
Operator : UM/SJ
Sample : H3797-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHS3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

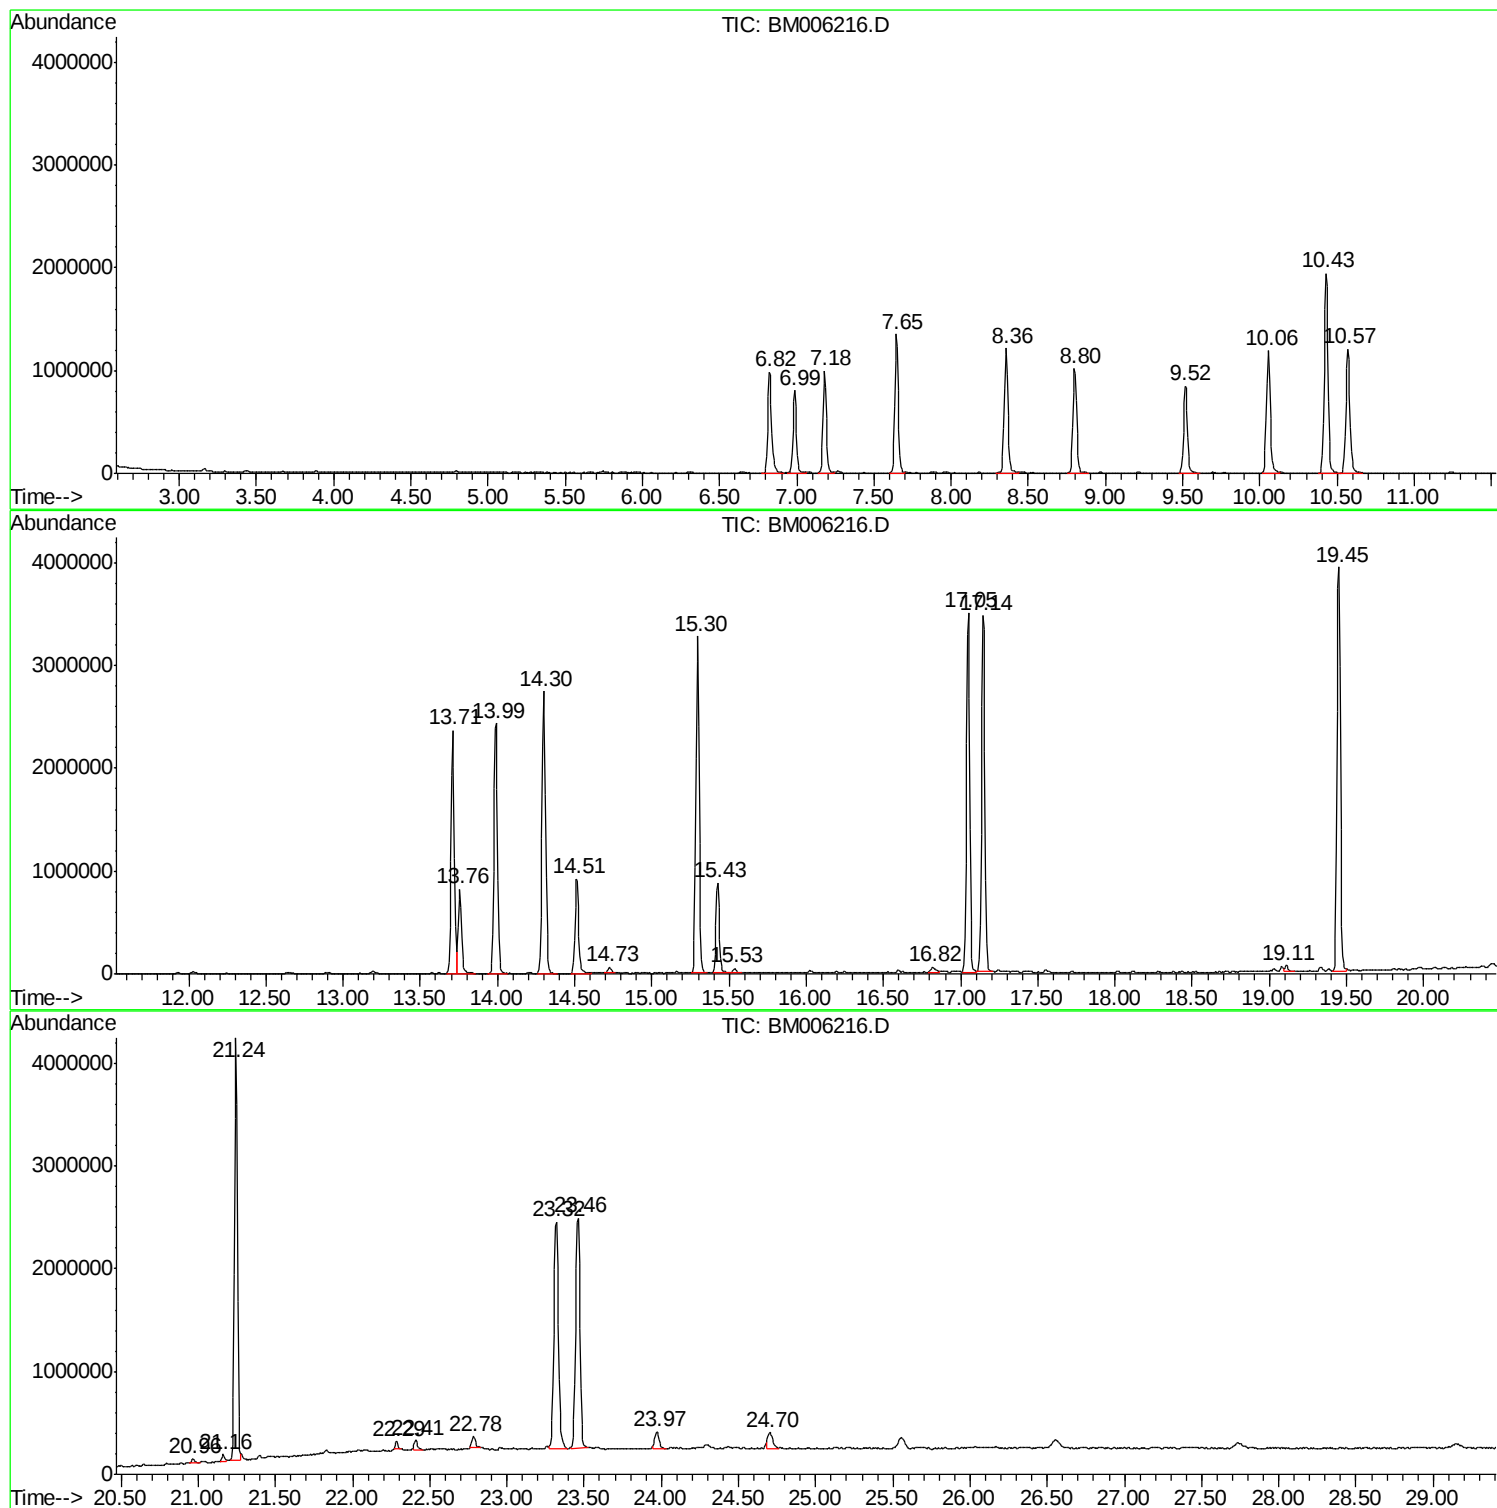

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006216.D
Acq On : 03 Jul 2016 01:20
Operator : UM/SJ
Sample : H3797-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHS3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006216.D
Acq On : 03 Jul 2016 01:20
Operator : UM/SJ
Sample : H3797-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHS3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc