

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
 Data File : BM006217.D
 Acq On : 03 Jul 2016 01:56
 Operator : UM/SJ
 Sample : H3819-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.822	713	720	737	rBV	958169	1646465	34.05%	2.567%
2	6.987	739	748	760	rVV	781768	1220758	25.24%	1.903%
3	7.181	773	781	791	rBV	989602	1600348	33.09%	2.495%
4	7.645	852	860	869	rBV	1173567	1905432	39.40%	2.971%
5	8.357	973	981	987	rBV	1176037	2005452	41.47%	3.127%
6	8.410	987	990	997	rVB	86499	136622	2.83%	0.213%
7	8.798	1049	1056	1065	rBV	968424	1659805	34.32%	2.588%
8	9.516	1171	1178	1194	rVB	841613	1444401	29.87%	2.252%
9	10.051	1262	1269	1284	rBV	1123943	2064368	42.69%	3.219%
10	10.428	1323	1333	1349	rBV	1708348	3008216	62.21%	4.690%
11	10.569	1349	1357	1371	rBV	1164992	2165820	44.79%	3.377%
12	13.710	1884	1891	1896	rBV	2083963	3137170	64.87%	4.892%
13	13.757	1896	1899	1910	rVB	378961	535948	11.08%	0.836%
14	13.986	1927	1938	1948	rBV	2281319	3718344	76.89%	5.798%
15	14.298	1983	1991	2004	rVB2	2531265	4073080	84.23%	6.351%
16	14.516	2021	2028	2045	rBV	806805	1340646	27.72%	2.090%
17	15.298	2154	2161	2170	rBV	2925269	4481945	92.68%	6.988%
18	15.427	2177	2183	2197	rBV	742382	1140312	23.58%	1.778%
19	15.533	2197	2201	2210	rVB2	37691	60875	1.26%	0.095%
20	16.815	2415	2419	2426	rBV5	34275	63506	1.31%	0.099%
21	17.051	2452	2459	2469	rVV	3092821	4680588	96.79%	7.298%
22	17.145	2469	2475	2486	rVB	3041039	4636759	95.88%	7.230%
23	19.451	2860	2867	2874	rBV	3419632	4835810	100.00%	7.540%
24	20.962	3121	3124	3132	rBV6	47965	83643	1.73%	0.130%
25	21.245	3166	3172	3181	rBV	3531593	4476594	92.57%	6.980%
26	22.786	3431	3434	3440	rVB3	78129	112414	2.32%	0.175%
27	23.321	3518	3525	3534	rVB2	1942410	3808353	78.75%	5.938%
28	23.462	3541	3549	3557	rBV	2003520	3892322	80.49%	6.069%
29	23.974	3633	3636	3643	rVB2	117554	198888	4.11%	0.310%


Sum of corrected areas: 64134884

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006217.D
Acq On : 03 Jul 2016 01:56
Operator : UM/SJ
Sample : H3819-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHT8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

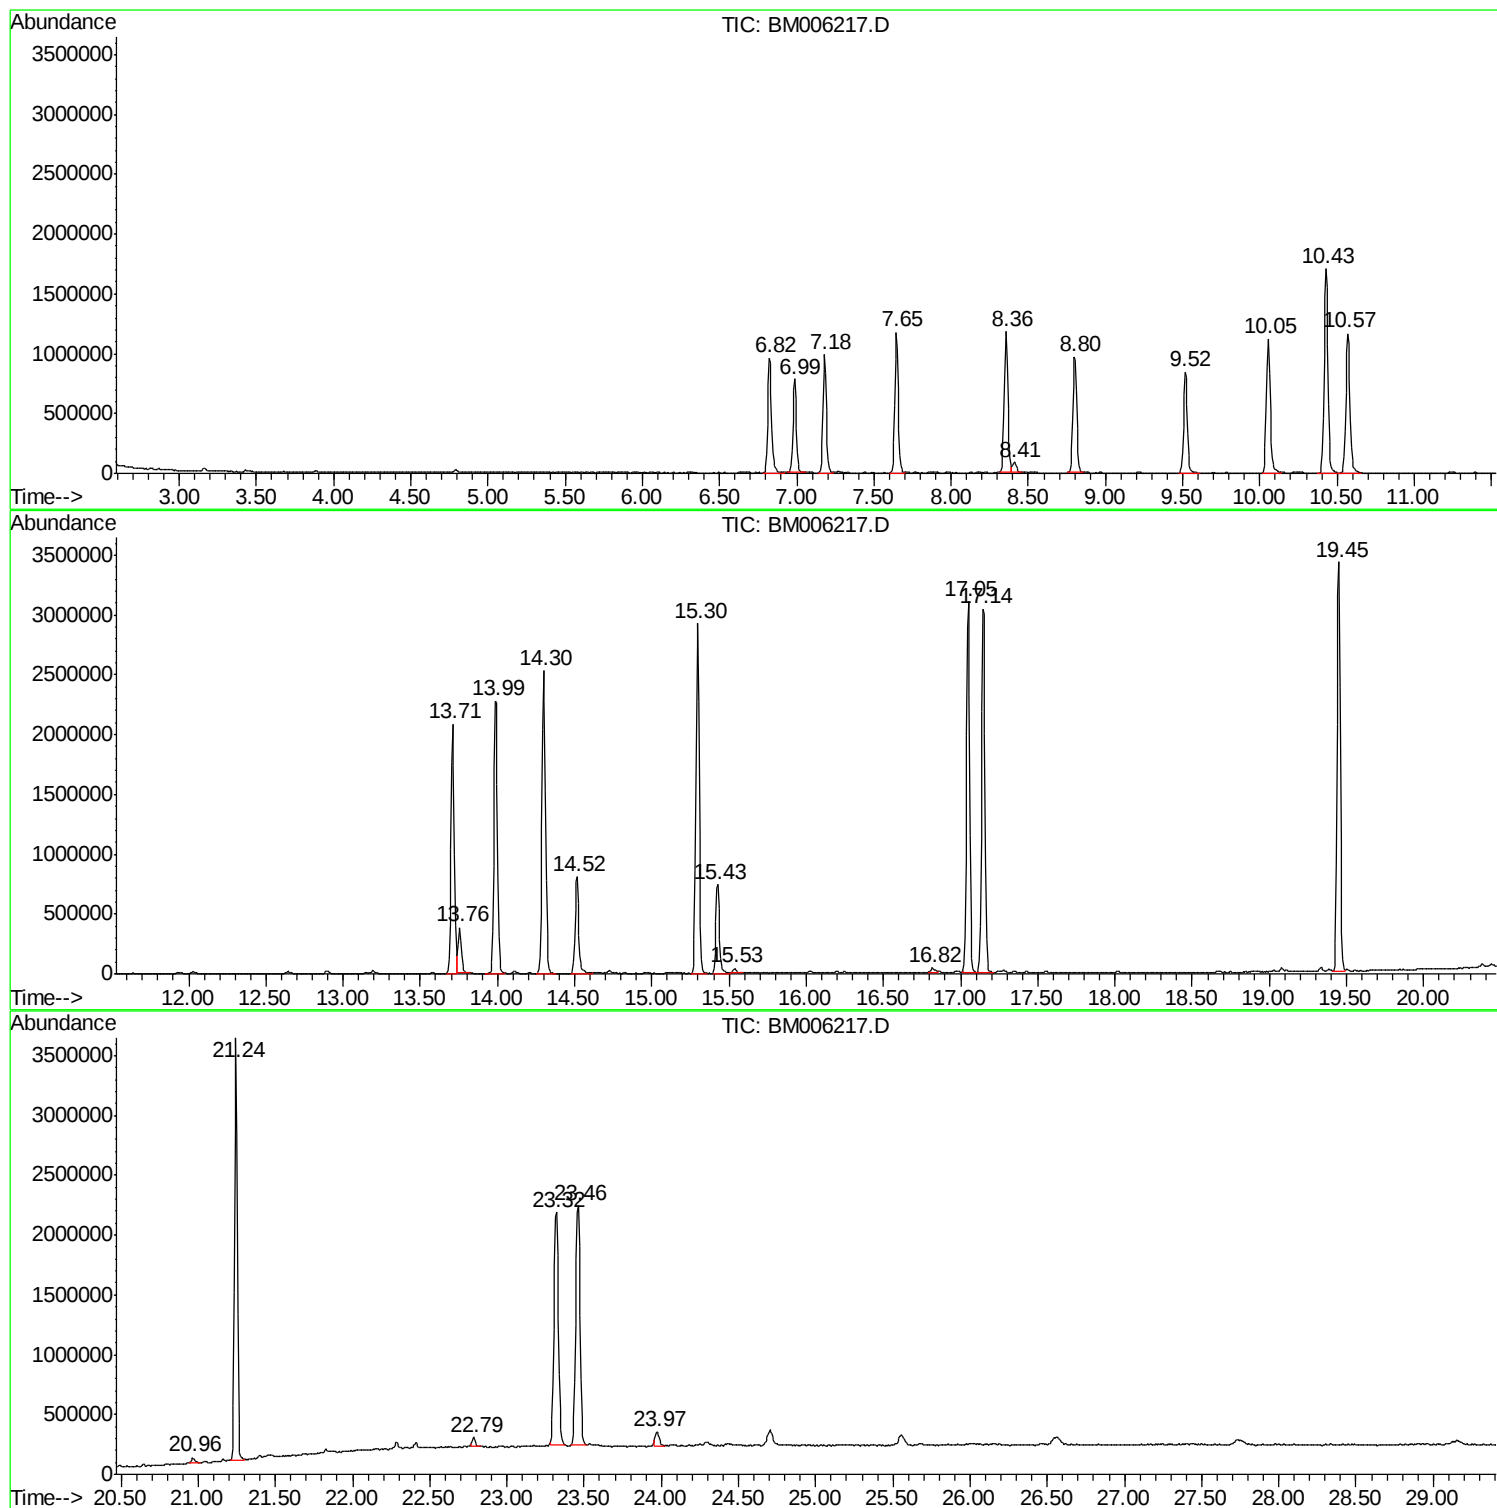

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006217.D
Acq On : 03 Jul 2016 01:56
Operator : UM/SJ
Sample : H3819-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHT8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070216\
Data File : BM006217.D
Acq On : 03 Jul 2016 01:56
Operator : UM/SJ
Sample : H3819-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHT8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc