
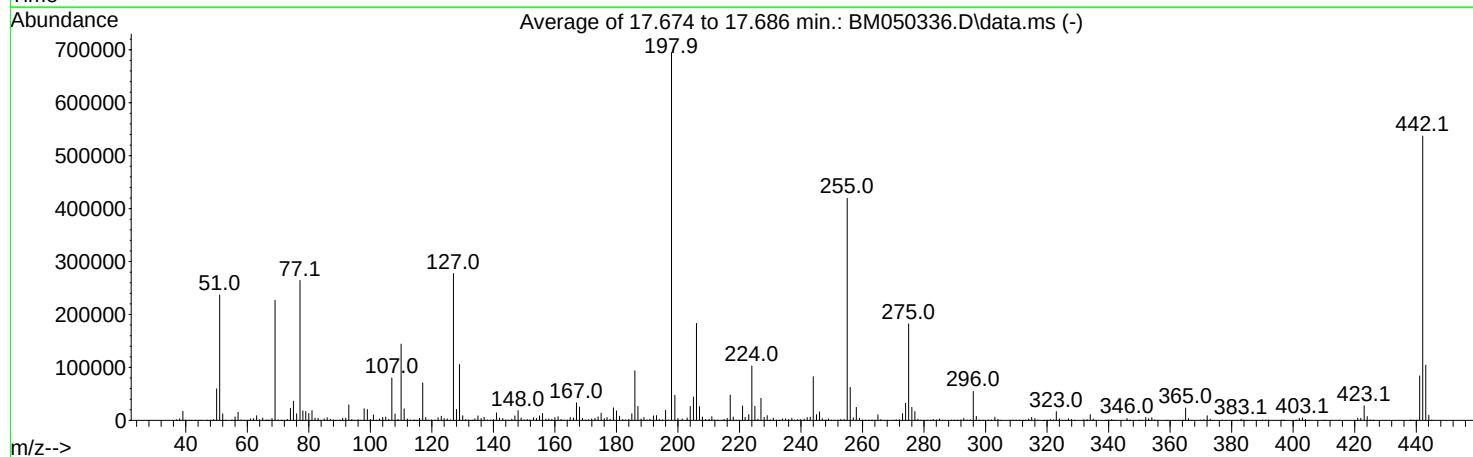


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070225\
Data File : BM050336.D
Acq On : 02 Jul 2025 09:19
Operator : RC/JU
Sample : DFTPP075
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP075

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM070125.MA.M
Title : SVOA CALIBRATION
Last Update : Tue Jul 01 15:14:38 2025

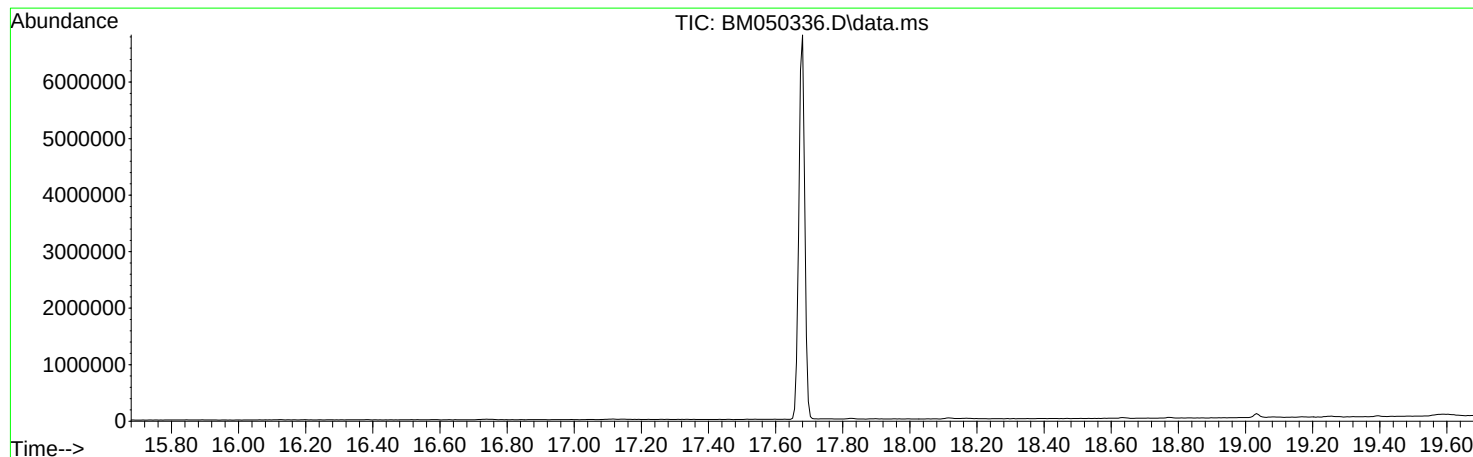

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	236845	PASS
68	69	0.00	2	1.7	3762	PASS
69	198	0.00	100	32.7	227157	PASS
70	69	0.00	2	0.5	1046	PASS
127	198	10	80	39.9	277568	PASS
197	198	0.00	2	0.1	893	PASS
198	198	100	100	100.0	694891	PASS
199	198	5	9	6.8	47453	PASS
275	198	10	60	26.2	182187	PASS
365	198	1	100	3.3	23272	PASS
441	198	0.01	100	12.1	83984	PASS
442	198	50	100	77.3	537216	PASS
443	442	15	24	19.4	104405	PASS