

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070316\
 Data File : BM006226.D
 Acq On : 03 Jul 2016 09:34
 Operator : UM/SJ
 Sample : PB91769BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 04 01:30:42 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 01:30:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	296125	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1461510	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	877813	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	2004881	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	2157249	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1863108	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	22311	3.22	ng/uL	0.00
5) Phenol-d5	6.82	99	949848	34.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	613442	37.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	723841	34.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	775938	34.58	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	391645	33.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	442543	33.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	728185	30.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	1092141	43.94	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	2395498	32.70	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	2923334	32.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	460149	33.14	ng/ul	0.00
57) Fluorene-d10	15.30	176	1973160	31.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	355337	30.25	ng/ul	0.00
70) Anthracene-d10	17.14	188	3006371	31.43	ng/ul	0.00
76) Pyrene-d10	19.45	212	3299717	32.08	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.32	264	2707738	31.28	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.36	70	20903	1.07	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070316\
Data File : BM006226.D
Acq On : 03 Jul 2016 09:34
Operator : UM/SJ
Sample : PB91769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 04 01:30:42 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 01:30:23 2016
Response via : Initial Calibration

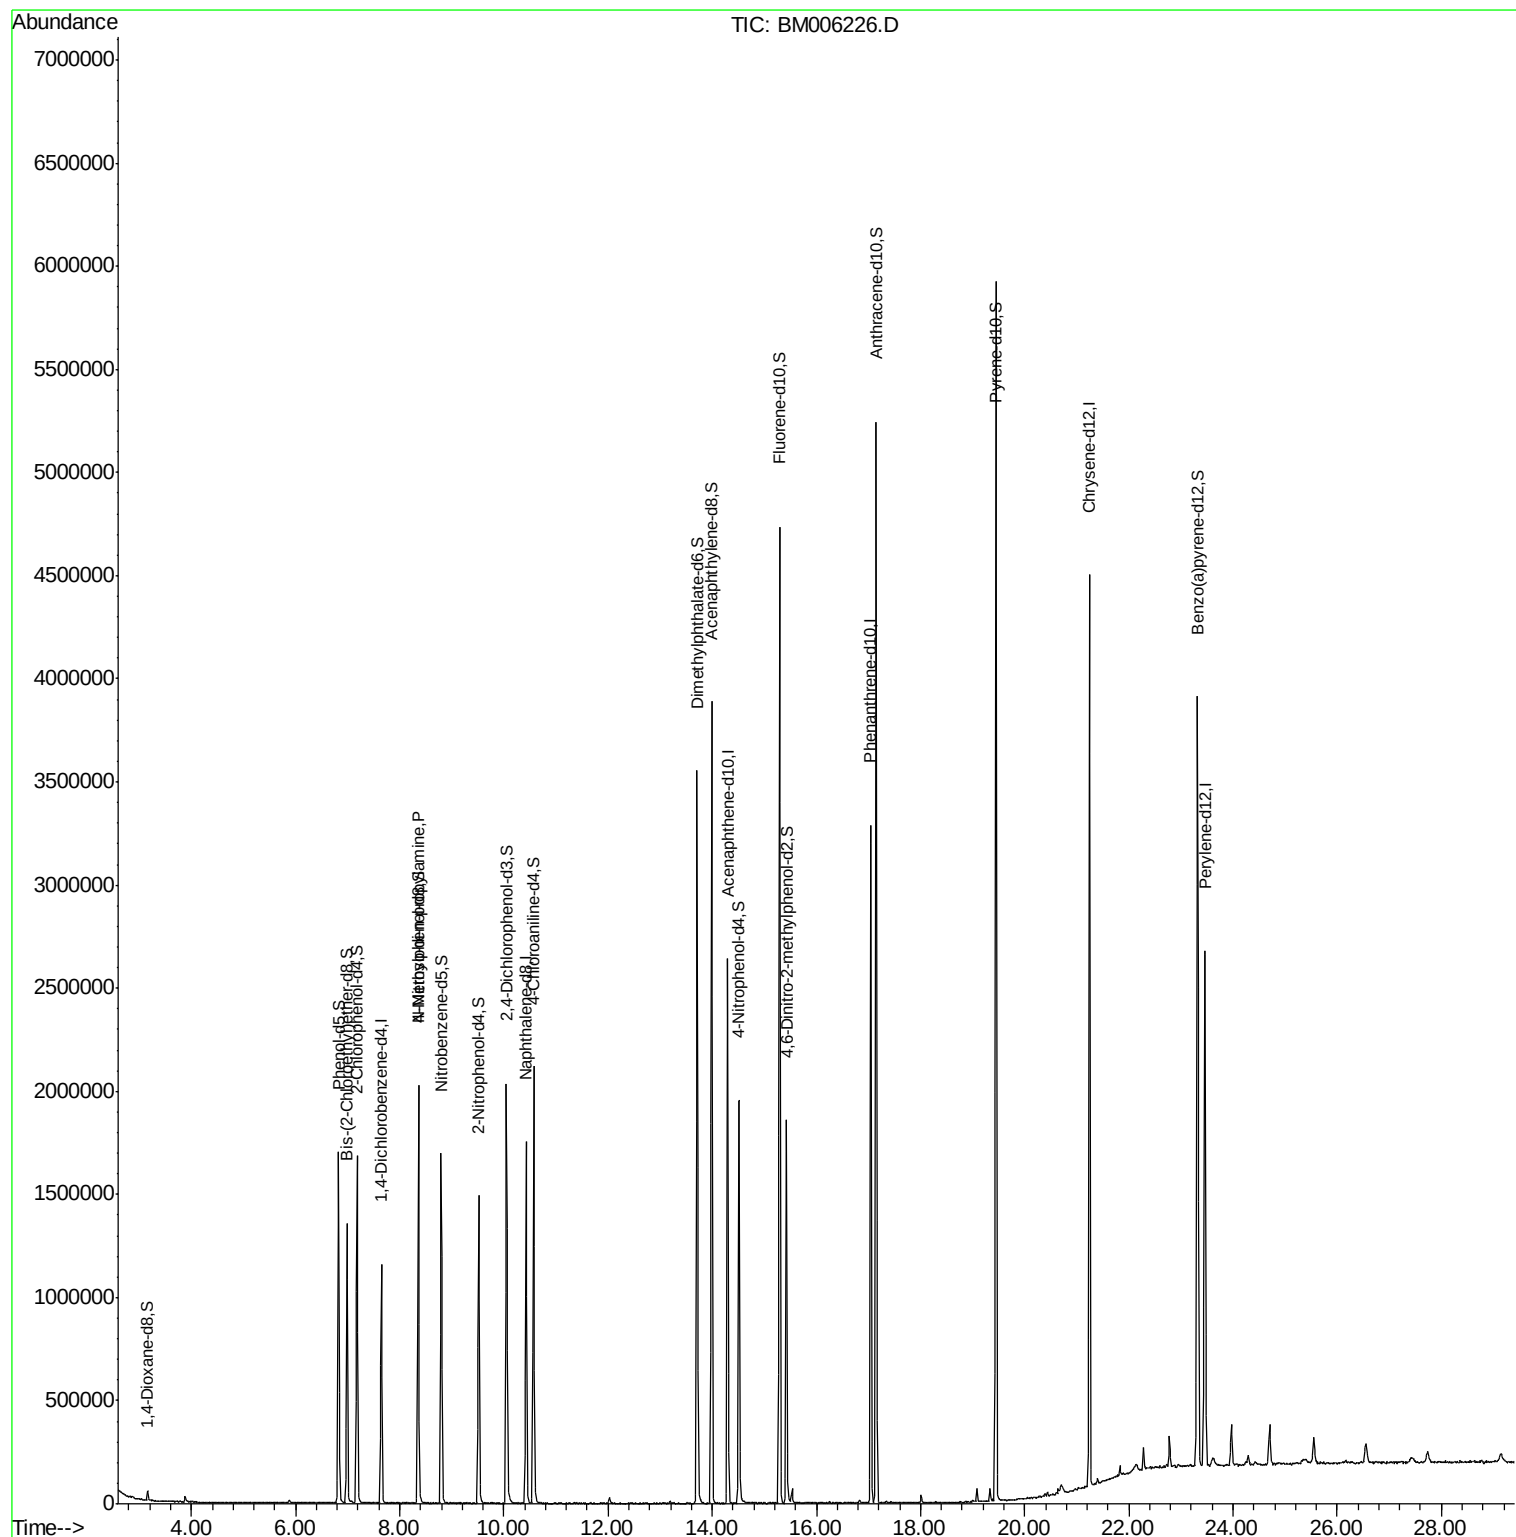

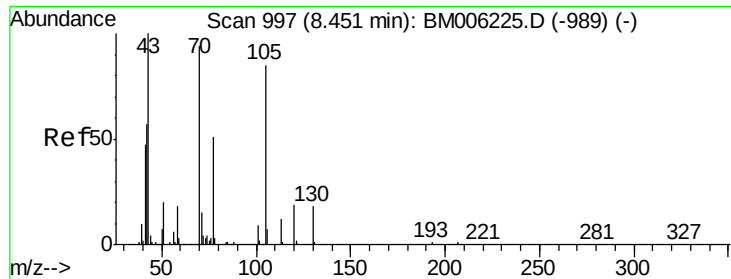

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.07 ng/ul
 RT: 8.36 min Scan# 981
 Delta R.T. -0.09 min
 Lab File: BM006226.D
 Acq: 03 Jul 2016 09:34

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
70	100		
42	378.1	50.6	75.8#
101	0.0	7.9	11.9#
130	0.0	15.8	23.6#

