

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070316\
 Data File : BM006228.D
 Acq On : 03 Jul 2016 10:46
 Operator : UM/SJ
 Sample : PB91677BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 04 01:30:56 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 01:30:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	290725	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1397703	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	807726	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1692778	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1572363	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1549671	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	22812	3.35	ng/uL	0.00
5) Phenol-d5	6.82	99	970827	35.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	634438	39.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	740084	35.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	787031	35.72	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	395441	35.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	448095	35.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	735673	32.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	1093248	45.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	2252699	33.42	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	2835790	33.98	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	410893	32.16	ng/ul	0.00
57) Fluorene-d10	15.29	176	1858888	31.99	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	315462	31.81	ng/ul	0.00
70) Anthracene-d10	17.14	188	2704938	33.49	ng/ul	0.00
76) Pyrene-d10	19.44	212	2687108	35.84	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.32	264	2342049	32.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.35	70	21562	1.12	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070316\
Data File : BM006228.D
Acq On : 03 Jul 2016 10:46
Operator : UM/SJ
Sample : PB91677BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 04 01:30:56 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 01:30:23 2016
Response via : Initial Calibration

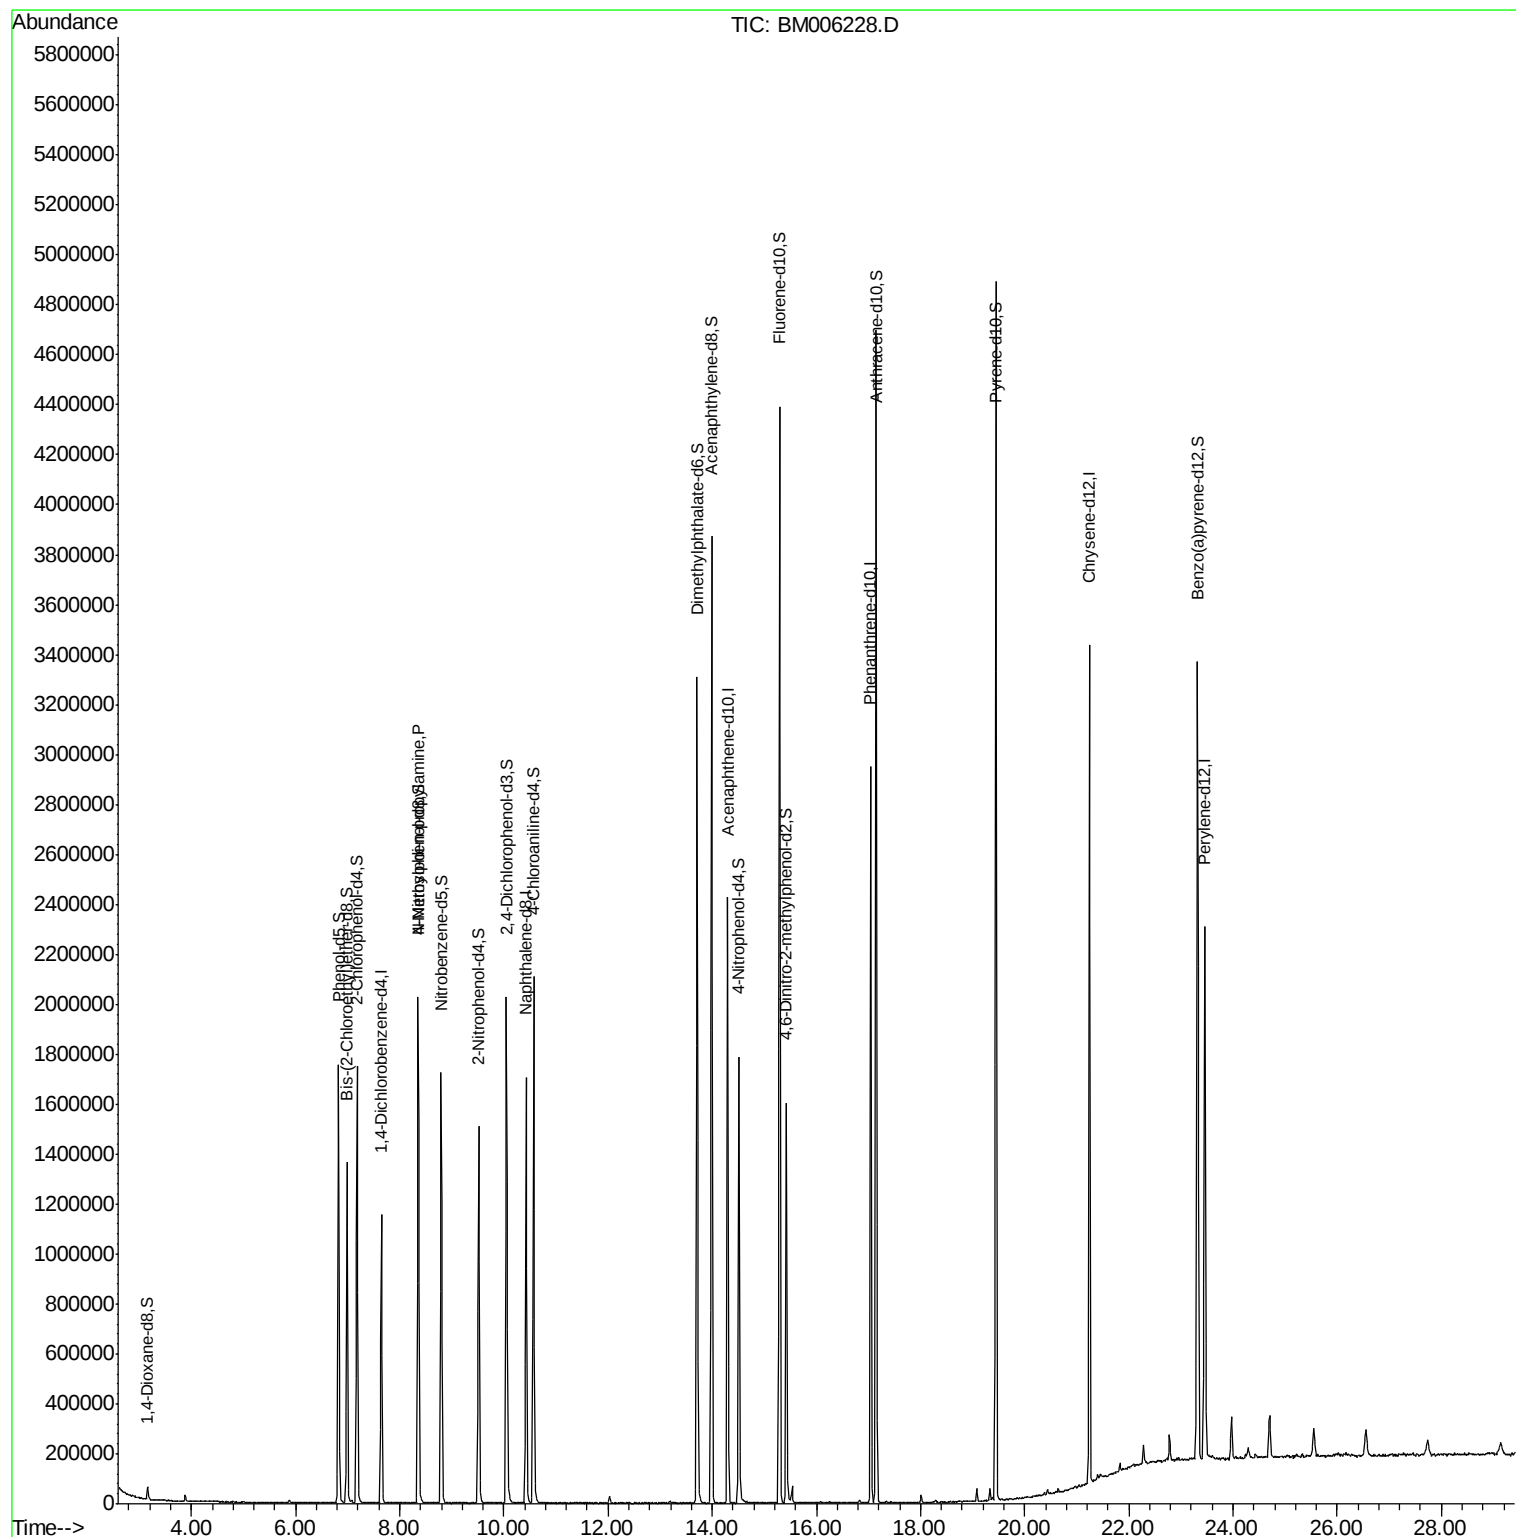

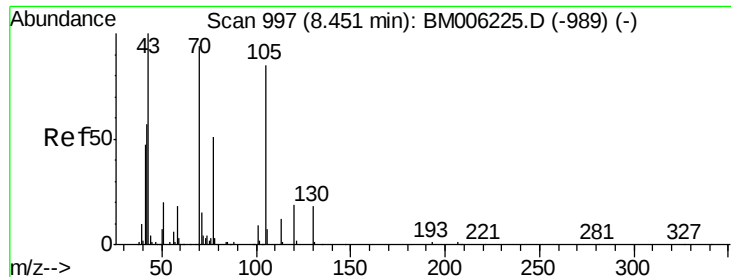

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.12 ng/ul
 RT: 8.35 min Scan# 980
 Delta R.T. -0.10 min
 Lab File: BM006228.D
 Acq: 03 Jul 2016 10:46

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 21562
 Ion Ratio Lower Upper
 70 100
 42 397.2 50.6 75.8#
 101 0.0 7.9 11.9#
 130 0.0 15.8 23.6#

