

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070316\
 Data File : BM006236.D
 Acq On : 03 Jul 2016 15:34
 Operator : UM/SJ
 Sample : H3819-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 04 01:31:54 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 01:30:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	340597	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1580964	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	923887	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	2021286	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1826810	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1611383	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	13063	1.64	ng/uL	0.00
5) Phenol-d5	6.82	99	589131	18.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	389225	20.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	452664	18.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	483972	18.75	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	241964	19.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	267411	18.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	451558	17.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	662500	24.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1530956	19.86	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1859636	19.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	250625	17.15	ng/ul	0.00
57) Fluorene-d10	15.29	176	1282677	19.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	194400	16.41	ng/ul	0.00
70) Anthracene-d10	17.14	188	1899411	19.70	ng/ul	0.00
76) Pyrene-d10	19.44	212	1973585	22.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.32	264	1514676	20.23	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.76	163	230529	2.97	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM070316\
Data File : BM006236.D
Acq On : 03 Jul 2016 15:34
Operator : UM/SJ
Sample : H3819-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 04 01:31:54 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 01:30:23 2016
Response via : Initial Calibration

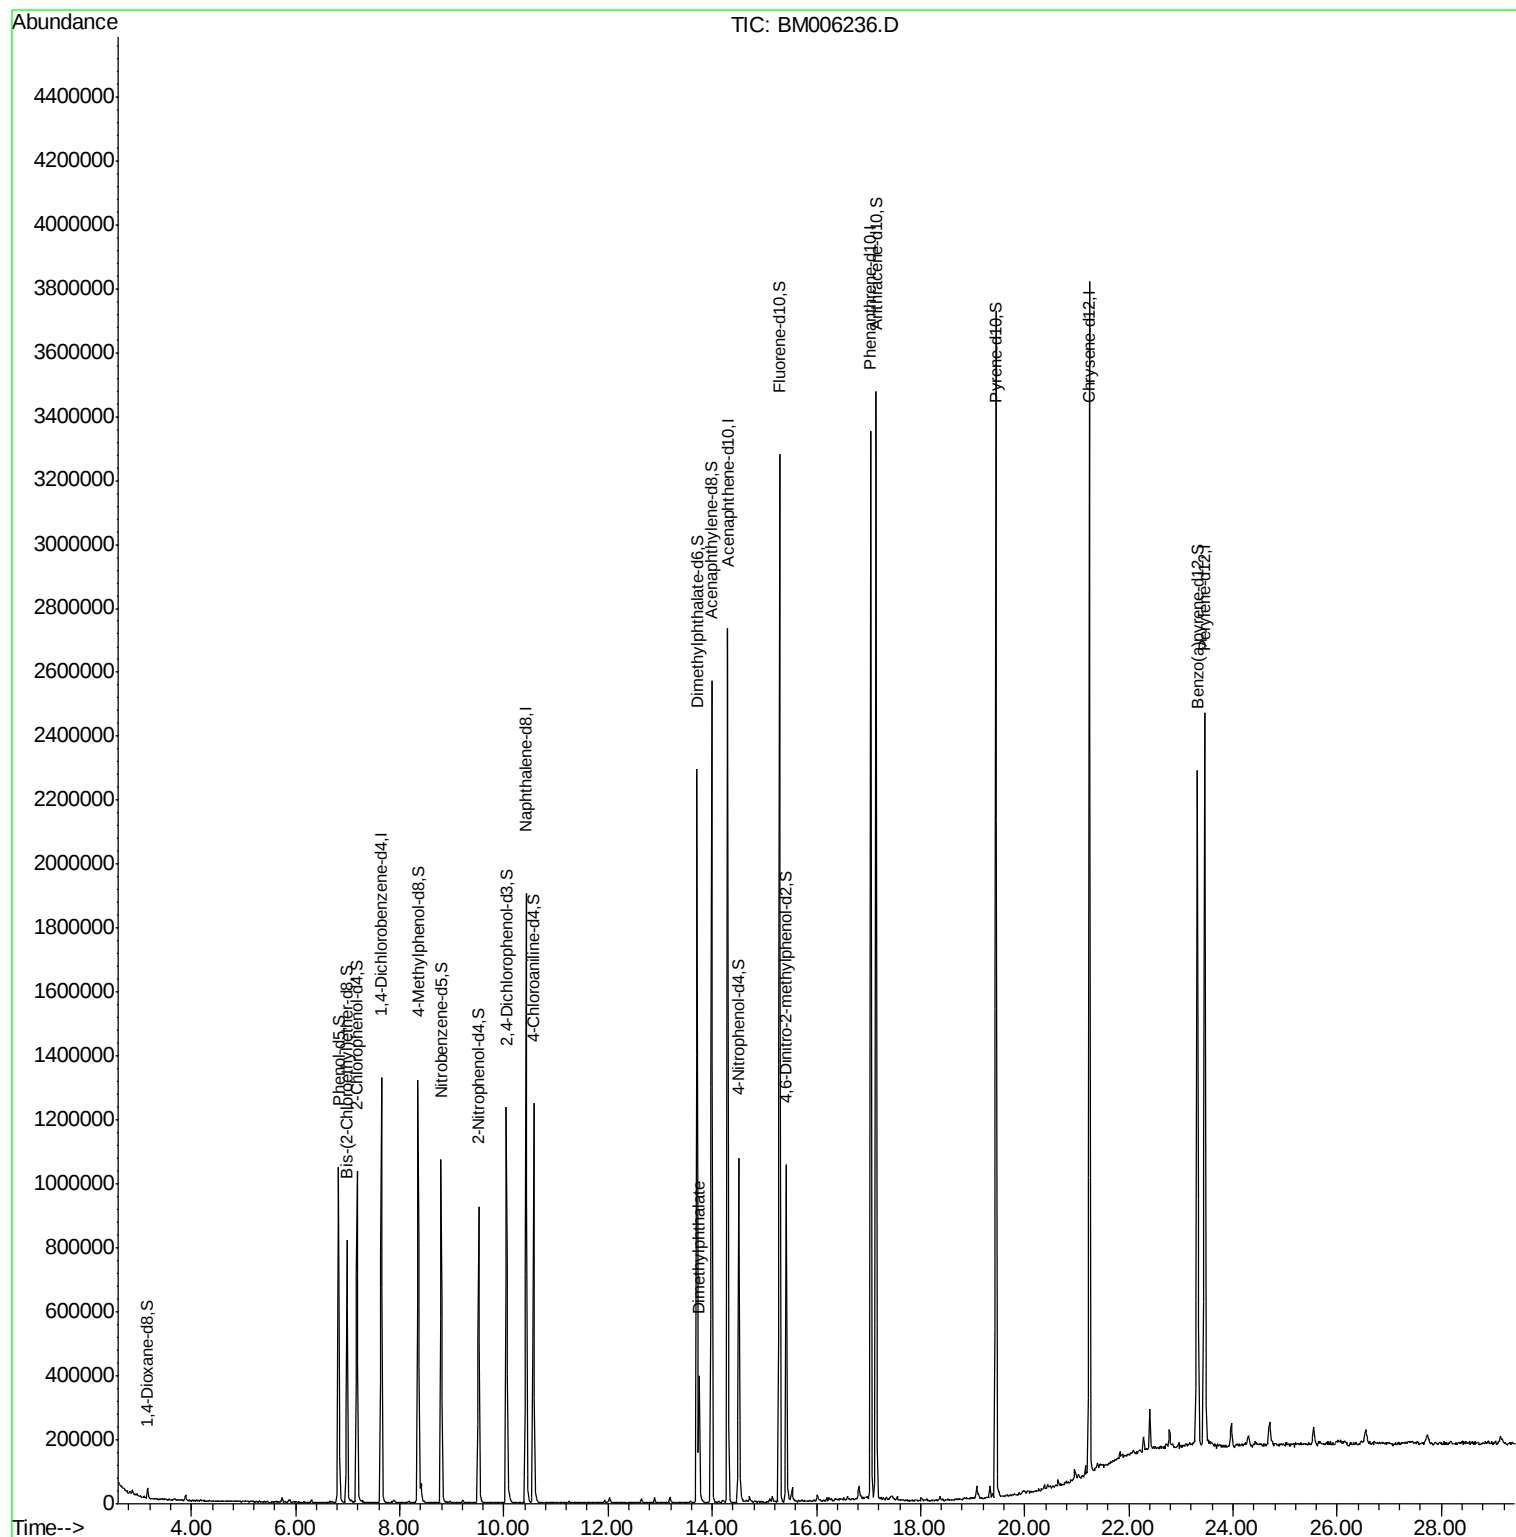

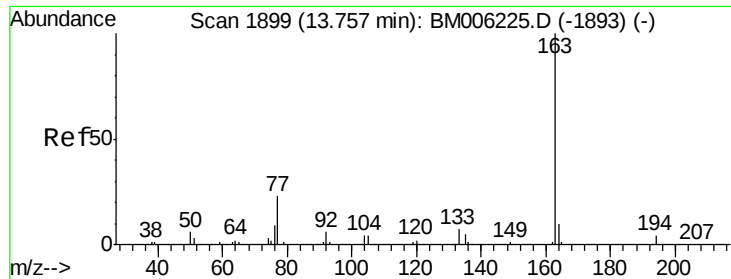

#44

Dimethylphthalate

Concen: 2.97 ng/ul

RT: 13.76 min Scan# 1899

Delta R.T. 0.00 min

Lab File: BM006236.D

Acq: 03 Jul 2016 15:34

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 230529

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.1 7.8 11.8

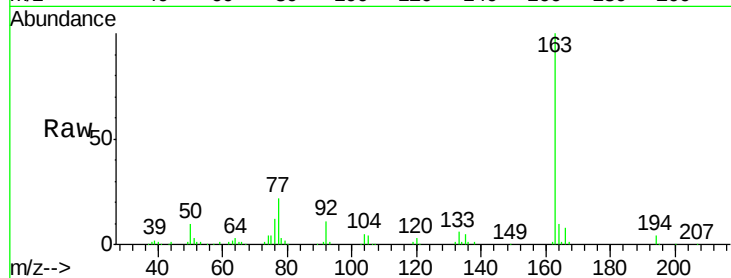

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

