

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006233.D
 Acq On : 03 Jul 2016 13:46
 Operator : UM/SJ
 Sample : H3819-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHX5

Quant Time: Jul 05 04:04:31 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 01:54:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	228652	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1078670	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	659265	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1476696	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1326297	20.00	ng/ul	0.00
83) Perylene-d12	23.45	264	1112518	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	3728	0.70	ng/uL	0.00
5) Phenol-d5	6.82	99	169588	7.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	114100	9.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	132548	8.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	139181	8.03	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	66106	7.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	71847	7.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	123503	7.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	192033	10.47	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	461187	8.38	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	562003	8.25	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	66637	6.39	ng/ul	0.00
57) Fluorene-d10	15.29	176	398145	8.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	41650	4.81	ng/ul	0.00
70) Anthracene-d10	17.14	188	602798	8.56	ng/ul	0.00
76) Pyrene-d10	19.44	212	633090	10.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.31	264	448626	8.68	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.76	163	65914	1.19	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006233.D
Acq On : 03 Jul 2016 13:46
Operator : UM/SJ
Sample : H3819-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX5

Quant Time: Jul 05 04:04:31 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 01:54:46 2016
Response via : Initial Calibration

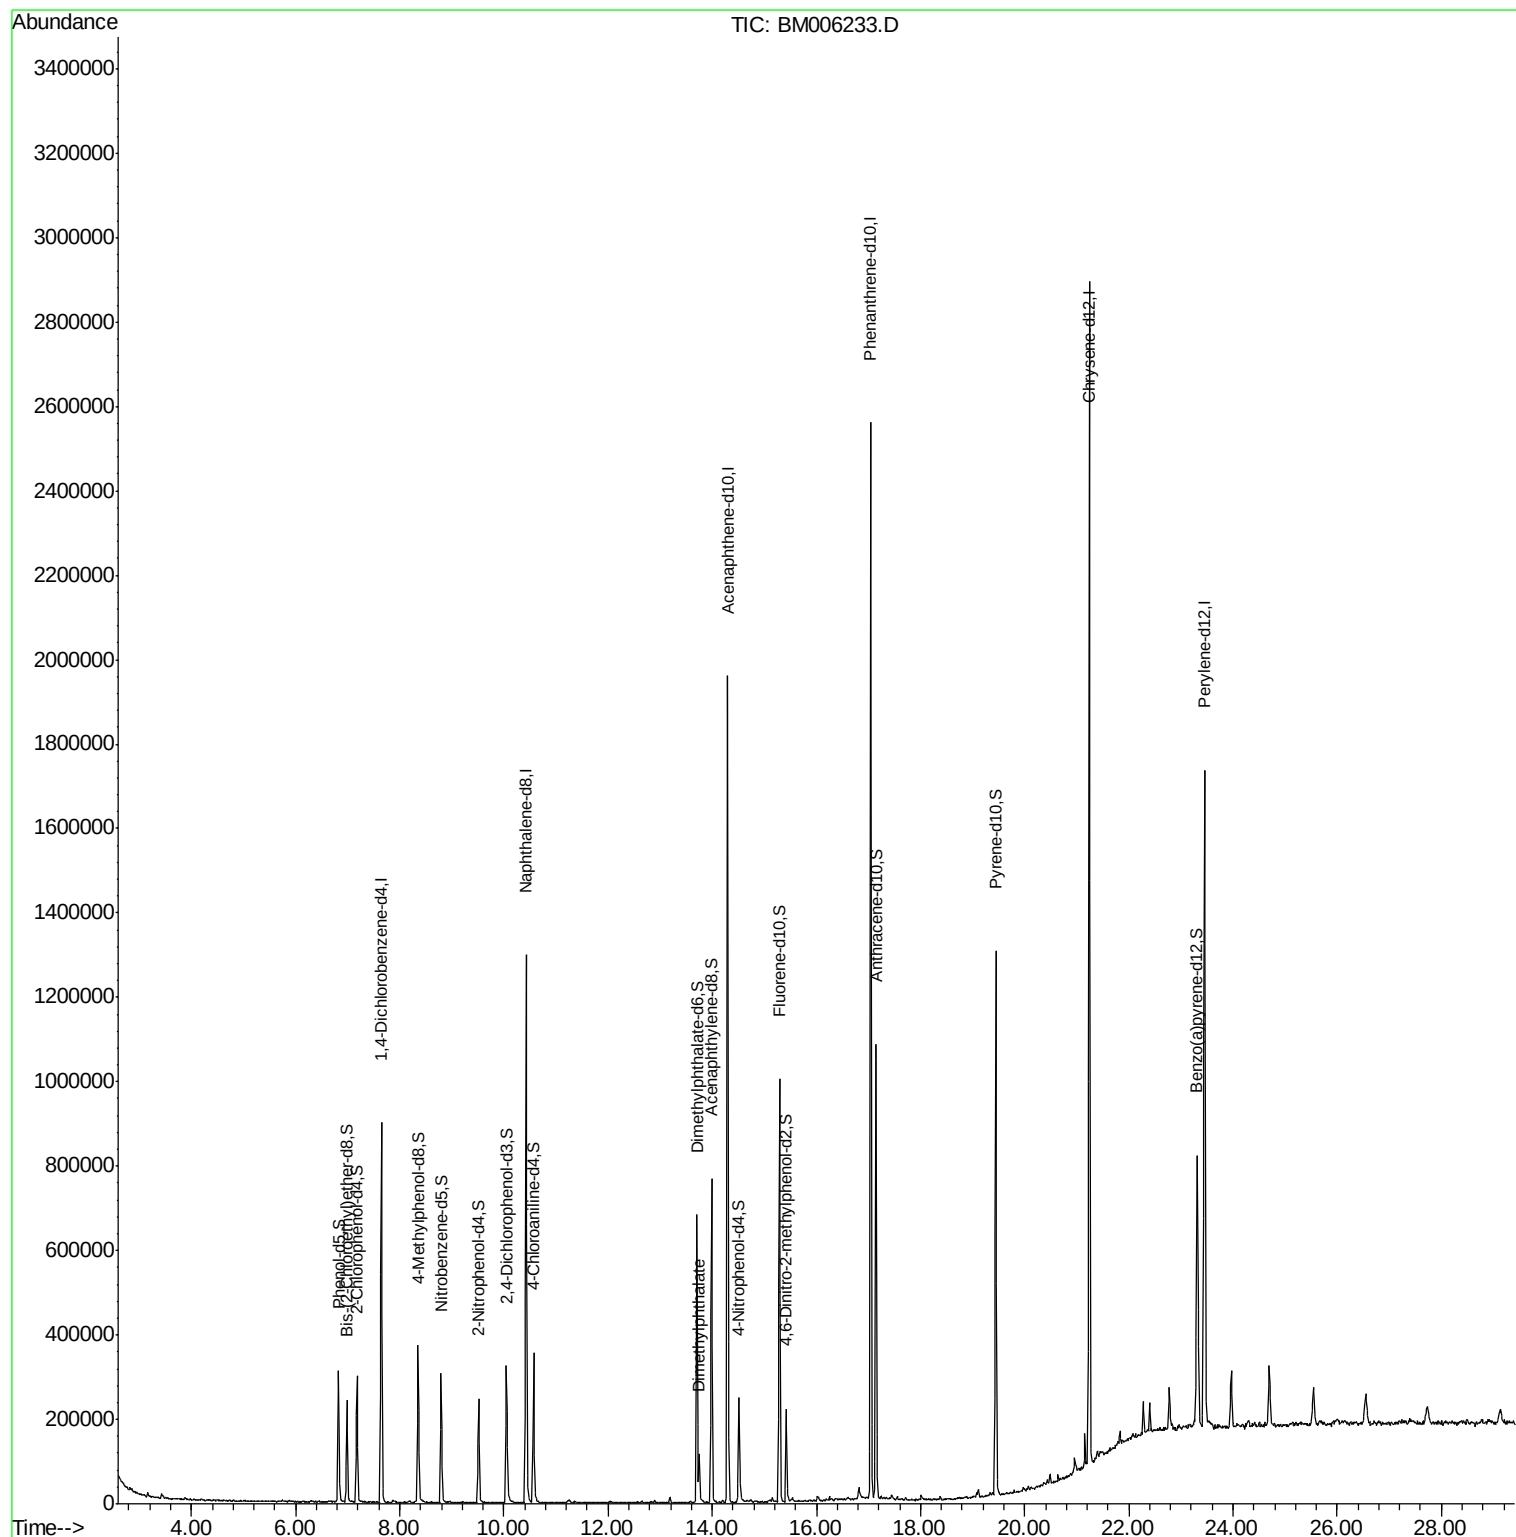

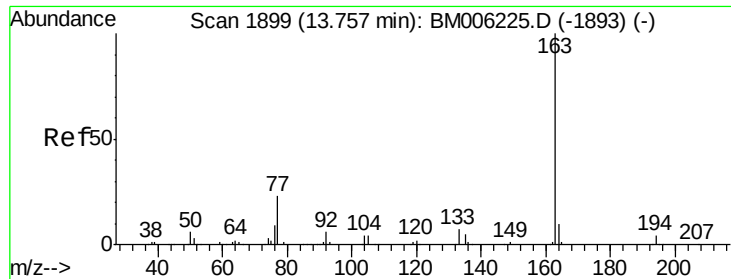

#44

Dimethylphthalate

Concen: 1.19 ng/ul

RT: 13.76 min Scan# 1899

Delta R.T. 0.00 min

Lab File: BM006233.D

Acq: 03 Jul 2016 13:46

Instrument :

BNA_M

ClientSampleId :

BDHX5


Tgt Ion:163 Resp: 65914

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.6 7.8 11.8

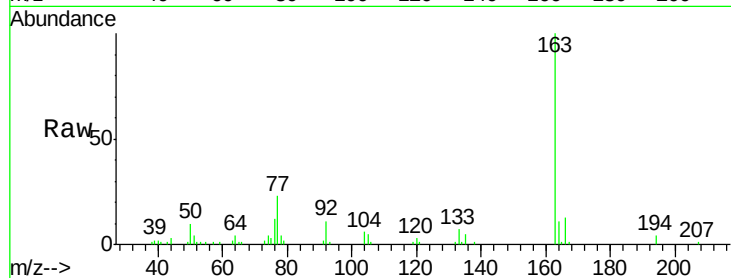

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

