

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006239.D
 Acq On : 03 Jul 2016 17:59
 Operator : UM/SJ
 Sample : H3819-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHY0

Quant Time: Jul 05 04:05:34 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 01:54:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	302982	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1429322	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	855452	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	2046669	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	2383553	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	2348874	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	14431	2.04	ng/uL	0.00
5) Phenol-d5	6.82	99	659285	23.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	430520	25.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	502795	23.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	544517	23.72	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	269674	23.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	300050	23.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	497264	21.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	761376	31.32	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1729565	24.23	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	2115013	23.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	259482	19.18	ng/ul	0.00
57) Fluorene-d10	15.29	176	1464812	23.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	206170	17.19	ng/ul	0.00
70) Anthracene-d10	17.14	188	2326990	23.83	ng/ul	0.00
76) Pyrene-d10	19.44	212	2686456	23.64	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.32	264	2726778	24.99	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.75	163	239461	3.34	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006239.D
Acq On : 03 Jul 2016 17:59
Operator : UM/SJ
Sample : H3819-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHY0

Quant Time: Jul 05 04:05:34 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 01:54:46 2016
Response via : Initial Calibration

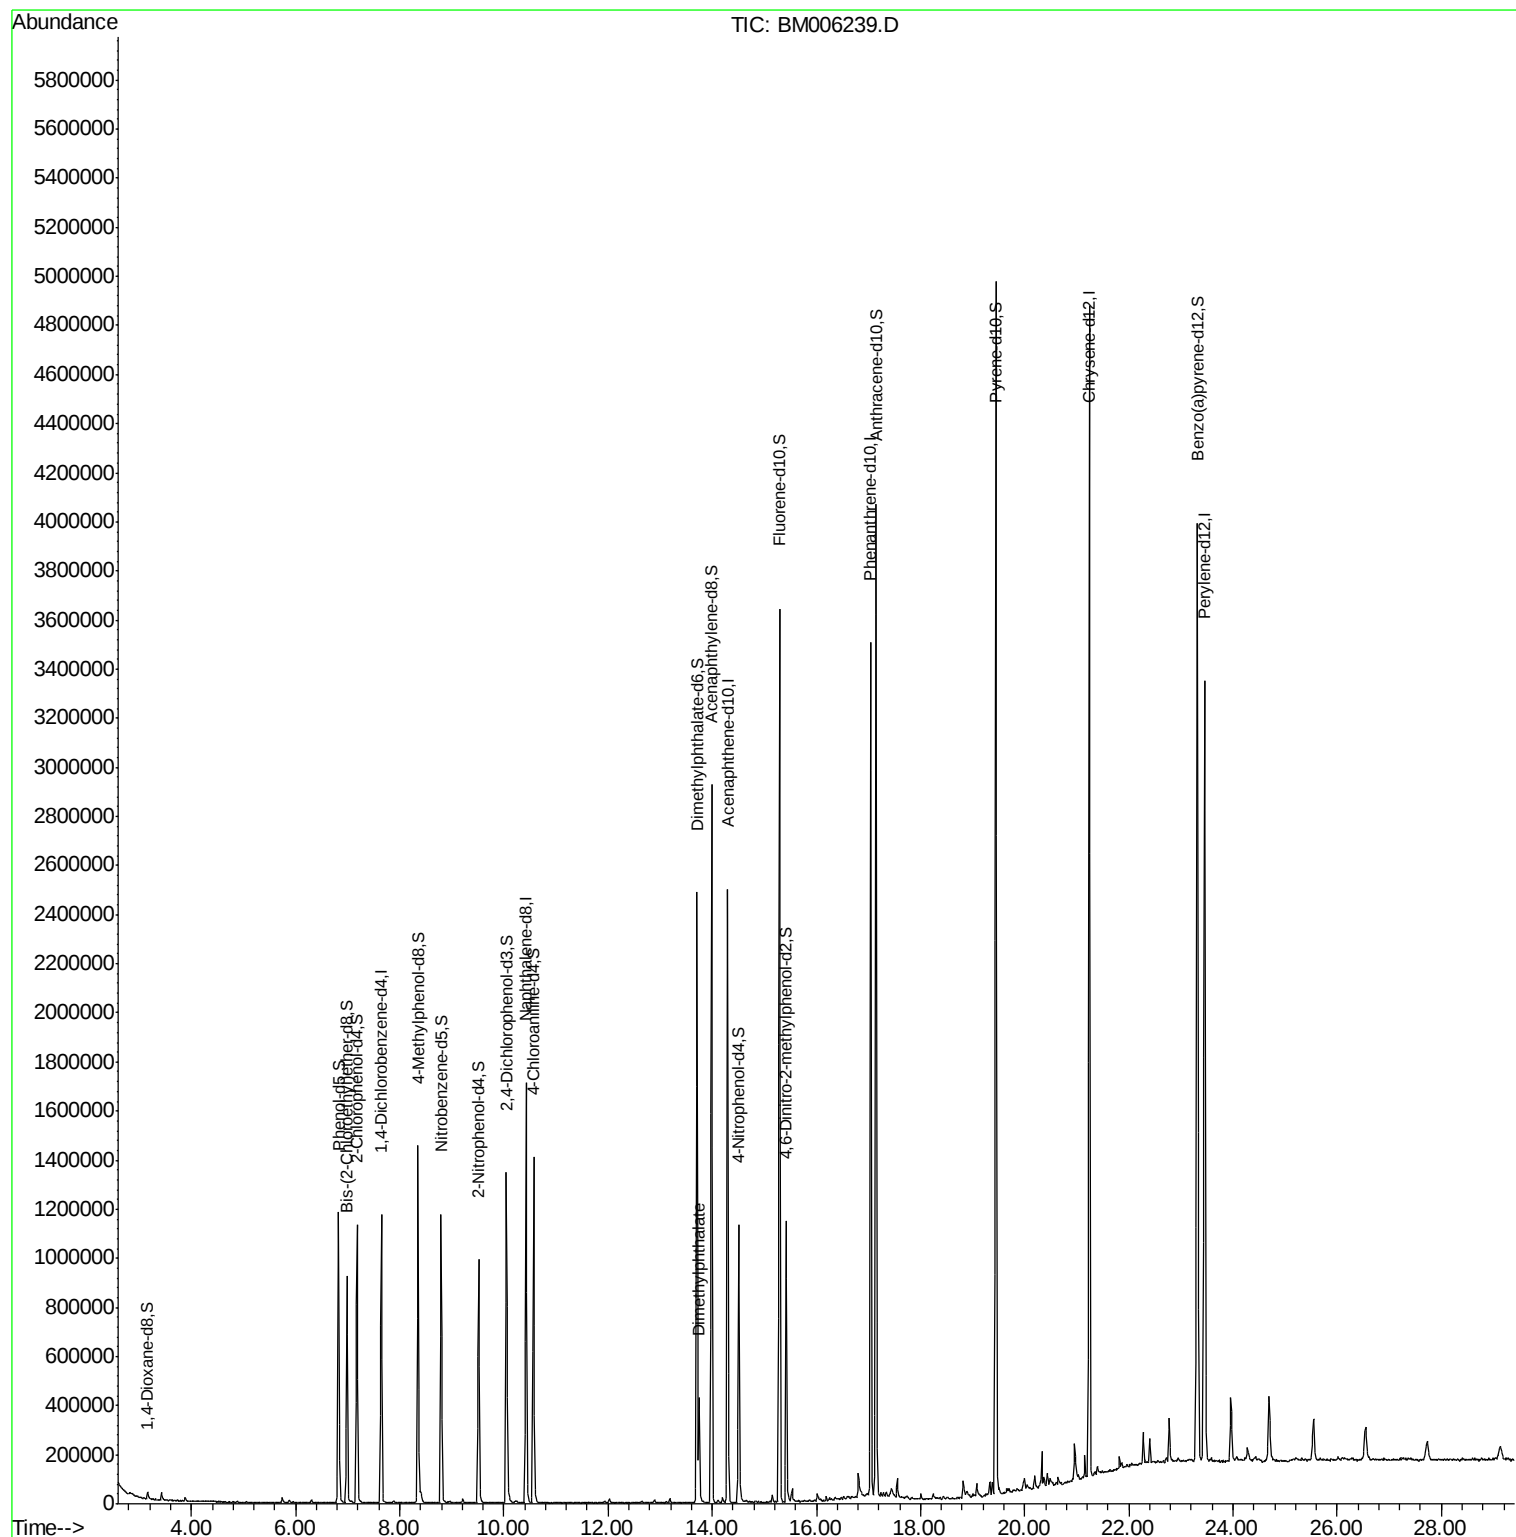

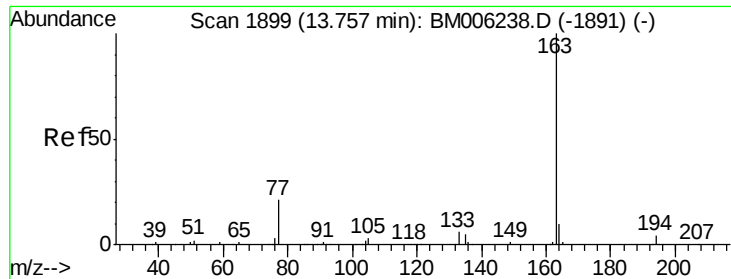

#44

Dimethylphthalate

Concen: 3.34 ng/ul

RT: 13.75 min Scan# 1898

Delta R.T. -0.01 min

Lab File: BM006239.D

Acq: 03 Jul 2016 17:59

Instrument :

BNA_M

ClientSampleId :

BDHY0


Tgt Ion:163 Resp: 239461

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.9 7.8 11.8

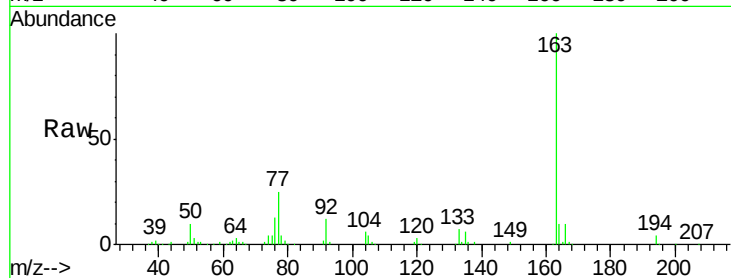

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

