

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006240.D
 Acq On : 03 Jul 2016 18:35
 Operator : UM/SJ
 Sample : H3819-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHY1

Quant Time: Jul 05 04:05:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 04 01:54:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	313668	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1429263	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	787645	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1611866	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1515260	20.00	ng/ul	0.00
83) Perylene-d12	23.45	264	1480271	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	17647	2.41	ng/uL	0.00
5) Phenol-d5	6.82	99	845873	28.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	547854	31.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	645259	28.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	696017	29.28	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	343806	30.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	382579	29.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	636096	27.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	944157	38.84	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	2000482	30.43	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	2505797	30.79	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	371276	29.80	ng/ul	0.00
57) Fluorene-d10	15.29	176	1650102	29.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	277846	29.42	ng/ul	0.00
70) Anthracene-d10	17.14	188	2388038	31.05	ng/ul	0.00
76) Pyrene-d10	19.44	212	2468641	34.16	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.31	264	2285418	33.23	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.75	163	343384	5.20	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006240.D
Acq On : 03 Jul 2016 18:35
Operator : UM/SJ
Sample : H3819-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHY1

Quant Time: Jul 05 04:05:41 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 04 01:54:46 2016
Response via : Initial Calibration

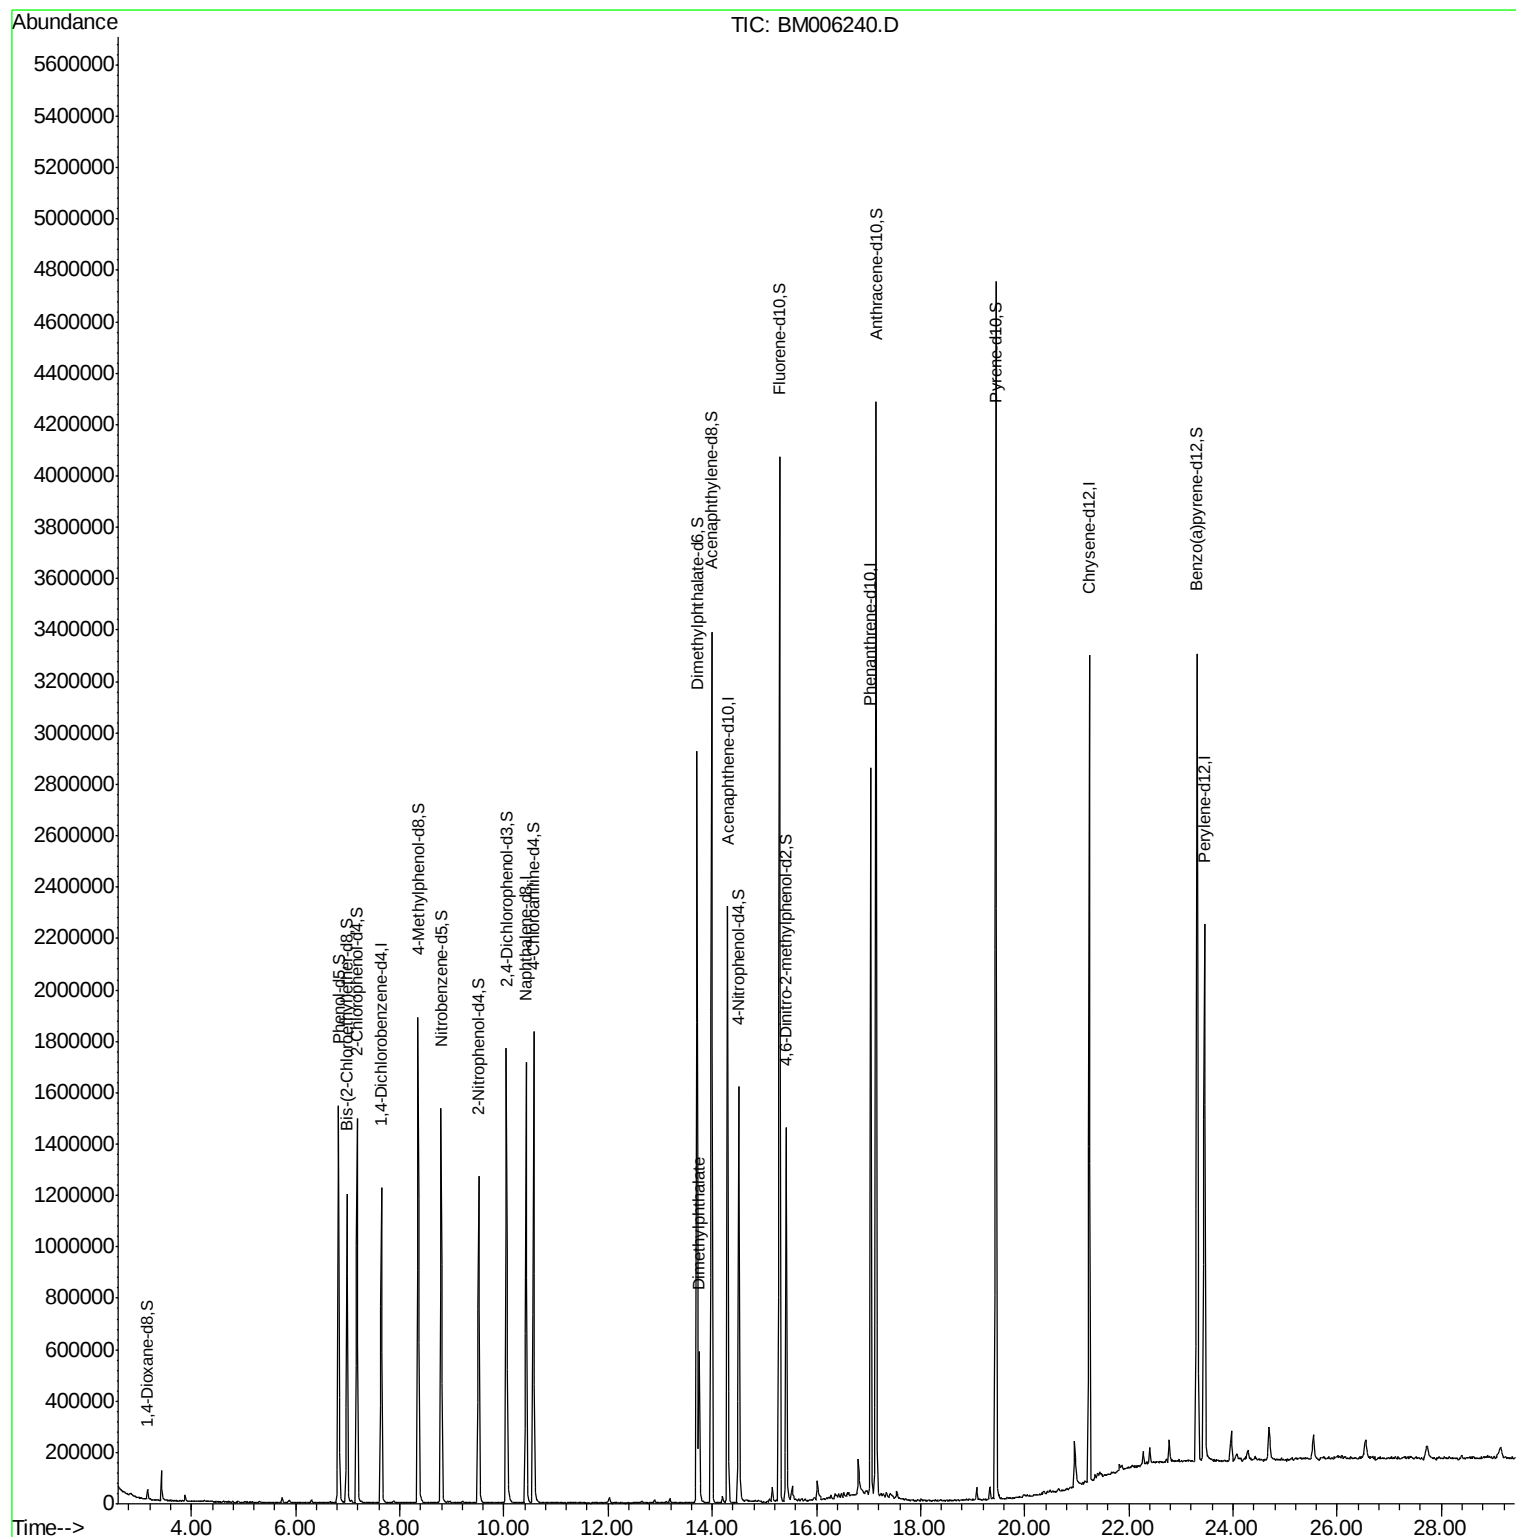

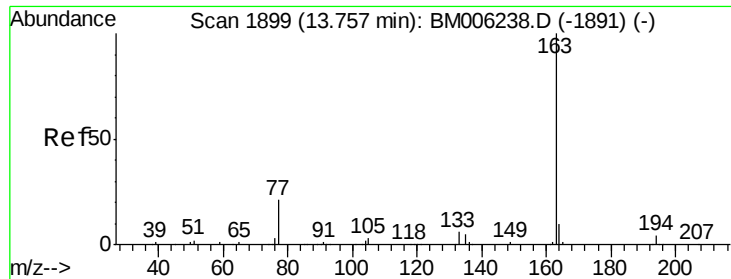

#44

Dimethylphthalate

Concen: 5.20 ng/ul

RT: 13.75 min Scan# 1898

Delta R.T. -0.01 min

Lab File: BM006240.D

Acq: 03 Jul 2016 18:35

Instrument :

BNA_M

ClientSampleId :

BDHY1

Tgt Ion:163 Resp: 343384

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 9.3 7.8 11.8

