

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006230.D
 Acq On : 03 Jul 2016 11:58
 Operator : UM/SJ
 Sample : H3819-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.822	713	720	734	rBV	1740672	2901486	33.24%	3.038%
2	6.987	741	748	760	rBV	1333016	2115067	24.23%	2.215%
3	7.181	773	781	793	rBV	1669643	2743258	31.42%	2.873%
4	7.645	853	860	868	rBV	1006507	1643429	18.82%	1.721%
5	8.357	973	981	987	rBV	2032390	3519267	40.31%	3.685%
6	8.404	987	989	1000	rVB	60693	109444	1.25%	0.115%
7	8.798	1048	1056	1071	rBV	1711365	2923957	33.49%	3.062%
8	9.516	1169	1178	1198	rBV	1474343	2559843	29.32%	2.681%
9	10.051	1261	1269	1284	rBV	1964685	3583825	41.05%	3.753%
10	10.428	1324	1333	1345	rBV	1535996	2683938	30.74%	2.811%
11	10.569	1349	1357	1372	rBV	2069439	3777724	43.27%	3.956%
12	13.710	1884	1891	1896	rBV	3608074	5342783	61.20%	5.595%
13	13.757	1896	1899	1907	rVB	658076	885878	10.15%	0.928%
14	13.986	1928	1938	1952	rBV	3948532	6302639	72.19%	6.600%
15	14.298	1984	1991	2004	rBV2	2253887	3639195	41.69%	3.811%
16	14.510	2019	2027	2046	rBV	1967367	3201989	36.68%	3.353%
17	15.292	2153	2160	2174	rVB	4803567	7473324	85.60%	7.826%
18	15.427	2176	2183	2196	rBV	1828028	2743527	31.43%	2.873%
19	15.533	2196	2201	2211	rVB2	72621	137522	1.58%	0.144%
20	16.021	2279	2284	2291	rBV	71766	121499	1.39%	0.127%
21	16.815	2414	2419	2425	rBV2	122910	207403	2.38%	0.217%
22	17.045	2452	2458	2468	rBV2	2891463	4331111	49.61%	4.536%
23	17.145	2468	2475	2487	rVB2	5164562	7889903	90.38%	8.262%
24	19.080	2799	2804	2808	rBV	69695	93487	1.07%	0.098%
25	19.450	2860	2867	2873	rBV2	5903000	8730176	100.00%	9.142%
26	20.968	3121	3125	3134	rBV2	163487	309238	3.54%	0.324%
27	21.244	3166	3172	3183	rBV	3433970	4589380	52.57%	4.806%
28	22.286	3346	3349	3357	rVB3	63288	92226	1.06%	0.097%
29	22.409	3367	3370	3375	rVB	101837	126953	1.45%	0.133%
30	22.786	3430	3434	3440	rVB2	91070	145950	1.67%	0.153%
31	23.321	3517	3525	3537	rVB2	3428810	6791380	77.79%	7.112%
32	23.462	3541	3549	3557	rBV	1878850	3557323	40.75%	3.725%
33	23.974	3632	3636	3643	rVB	120652	218109	2.50%	0.228%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006230.D
Acq On : 03 Jul 2016 11:58
Operator : UM/SJ
Sample : H3819-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Title : SVOA CALIBRATION


Sum of corrected areas: 95492233

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006230.D
Acq On : 03 Jul 2016 11:58
Operator : UM/SJ
Sample : H3819-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

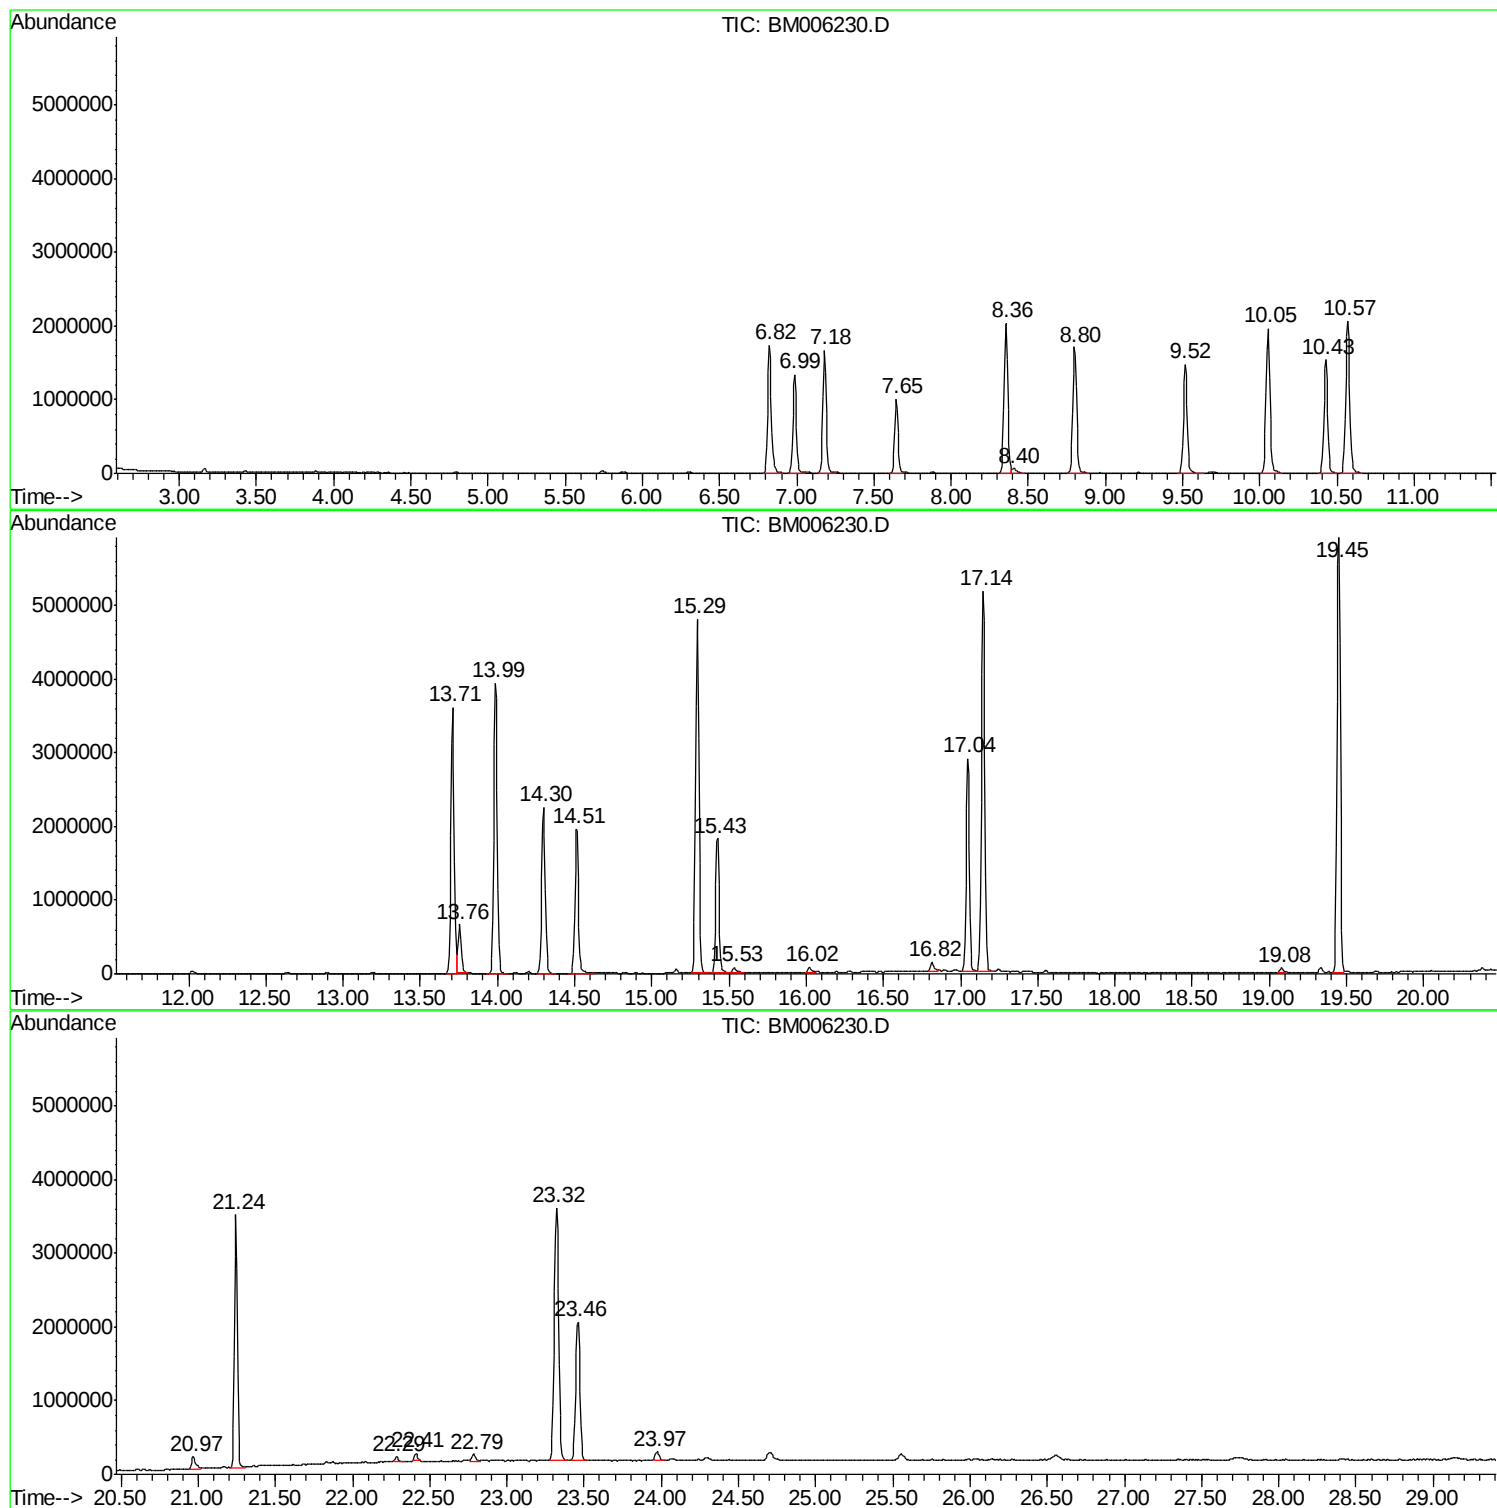

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006230.D
Acq On : 03 Jul 2016 11:58
Operator : UM/SJ
Sample : H3819-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006230.D
Acq On : 03 Jul 2016 11:58
Operator : UM/SJ
Sample : H3819-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc