

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006233.D
 Acq On : 03 Jul 2016 13:46
 Operator : UM/SJ
 Sample : H3819-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHX5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.822	713	720	734	rBV	309961	510873	13.56%	1.576%
2	6.981	741	747	756	rBV	242757	394671	10.48%	1.218%
3	7.181	774	781	791	rBV	299181	502028	13.33%	1.549%
4	7.645	853	860	874	rBV	899635	1475600	39.17%	4.552%
5	8.351	974	980	994	rVB	371792	625816	16.61%	1.931%
6	8.798	1048	1056	1066	rBV	304623	513466	13.63%	1.584%
7	9.516	1172	1178	1190	rBV	247152	428514	11.38%	1.322%
8	10.051	1263	1269	1287	rBV	325360	621939	16.51%	1.919%
9	10.428	1325	1333	1349	rBV	1298359	2305059	61.19%	7.111%
10	10.569	1349	1357	1371	rVV	354952	671557	17.83%	2.072%
11	13.704	1884	1890	1895	rBV	682200	1012997	26.89%	3.125%
12	13.751	1895	1898	1907	rVB	113022	180483	4.79%	0.557%
13	13.986	1931	1938	1950	rBV	767979	1210103	32.12%	3.733%
14	14.298	1983	1991	2001	rBV2	1958110	3163966	83.99%	9.761%
15	14.510	2021	2027	2041	rBV	248101	474083	12.58%	1.463%
16	15.292	2154	2160	2170	rBV	1002937	1536167	40.78%	4.739%
17	15.421	2176	2182	2193	rBV	220882	341317	9.06%	1.053%
18	16.815	2413	2419	2427	rBV3	28316	61667	1.64%	0.190%
19	17.045	2451	2458	2468	rBV	2550635	3766548	99.99%	11.620%
20	17.145	2468	2475	2486	rVB2	1077825	1622187	43.06%	5.005%
21	19.445	2860	2866	2874	rBV	1288866	1786512	47.42%	5.512%
22	20.962	3121	3124	3132	rBV5	30614	58441	1.55%	0.180%
23	21.156	3154	3157	3161	rBV	82494	104442	2.77%	0.322%
24	21.239	3165	3171	3181	rVV	2803492	3767057	100.00%	11.622%
25	22.280	3345	3348	3354	rVB3	72539	92148	2.45%	0.284%
26	22.403	3366	3369	3374	rVB2	66186	85294	2.26%	0.263%
27	22.780	3429	3433	3440	rVB2	92094	141273	3.75%	0.436%
28	23.309	3517	3523	3534	rVB2	637132	1459379	38.74%	4.502%
29	23.450	3540	3547	3556	rBV2	1548766	2964742	78.70%	9.146%
30	23.968	3630	3635	3642	rVB2	131039	247131	6.56%	0.762%
31	24.697	3755	3759	3771	rVB3	143398	288520	7.66%	0.890%


Sum of corrected areas: 32413980

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006233.D
Acq On : 03 Jul 2016 13:46
Operator : UM/SJ
Sample : H3819-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

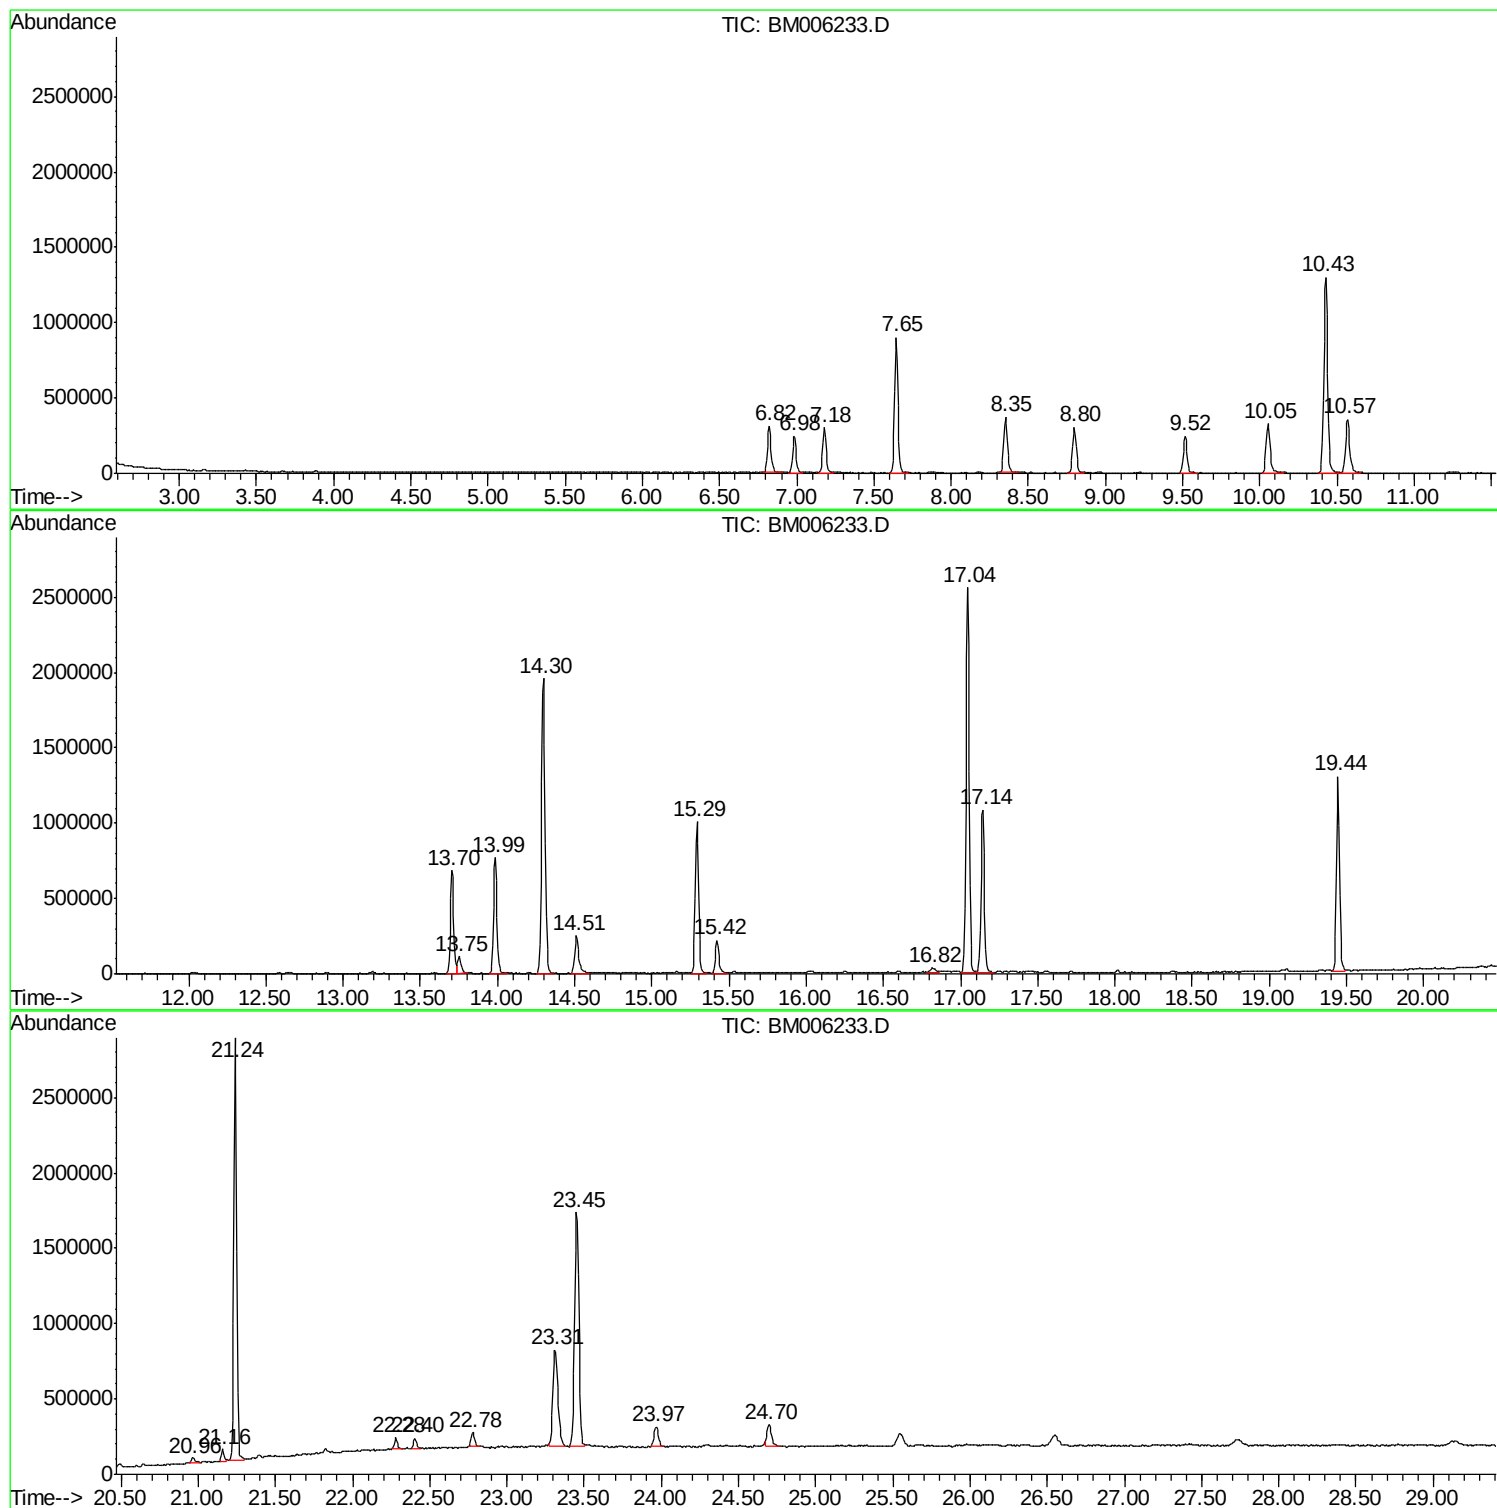

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006233.D
Acq On : 03 Jul 2016 13:46
Operator : UM/SJ
Sample : H3819-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006233.D
Acq On : 03 Jul 2016 13:46
Operator : UM/SJ
Sample : H3819-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc