

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006234.D
 Acq On : 03 Jul 2016 14:22
 Operator : UM/SJ
 Sample : H3819-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.822	711	720	736	rBV	1386423	2350842	33.34%	2.893%
2	6.987	740	748	760	rBV	1080057	1727807	24.50%	2.126%
3	7.181	773	781	792	rBV	1344811	2219621	31.48%	2.732%
4	7.646	852	860	869	rBV	1122667	1823520	25.86%	2.244%
5	8.351	973	980	988	rBV	1675821	2825726	40.08%	3.478%
6	8.798	1048	1056	1071	rBV	1386556	2350468	33.34%	2.893%
7	9.516	1171	1178	1194	rBV	1198049	2033036	28.83%	2.502%
8	10.051	1259	1269	1292	rBV	1631580	2899793	41.13%	3.569%
9	10.428	1325	1333	1347	rBV	1661726	2874496	40.77%	3.538%
10	10.569	1349	1357	1376	rVB	1596429	2961133	42.00%	3.644%
11	13.710	1884	1891	1895	rBV	2921826	4336862	61.51%	5.338%
12	13.751	1895	1898	1909	rVB	515386	788567	11.18%	0.971%
13	13.986	1931	1938	1949	rVB	3281703	5098418	72.31%	6.275%
14	14.298	1983	1991	2002	rBV2	2314670	3758858	53.31%	4.626%
15	14.510	2020	2027	2042	rBV	1512674	2493559	35.36%	3.069%
16	15.292	2153	2160	2168	rBV	4025083	6115754	86.74%	7.527%
17	15.421	2176	2182	2196	rBV	1503529	2146279	30.44%	2.642%
18	15.533	2196	2201	2205	rBV	55150	86230	1.22%	0.106%
19	16.021	2279	2284	2291	rBV	58368	105767	1.50%	0.130%
20	16.816	2414	2419	2429	rBV2	106146	208476	2.96%	0.257%
21	17.045	2452	2458	2468	rBV2	2896923	4387082	62.22%	5.399%
22	17.145	2468	2475	2486	rVB2	4163215	6364039	90.26%	7.832%
23	19.074	2800	2803	2806	rBV	51216	72192	1.02%	0.089%
24	19.109	2806	2809	2814	rVB	99604	128434	1.82%	0.158%
25	19.445	2860	2866	2879	rBV2	4653338	7051023	100.00%	8.678%
26	19.974	2946	2956	2965	rBV3	34647	89556	1.27%	0.110%
27	20.962	3120	3124	3134	rBV2	129446	242751	3.44%	0.299%
28	21.239	3165	3171	3176	rBV	3171965	4336245	61.50%	5.337%
29	22.403	3366	3369	3374	rVB	98189	135387	1.92%	0.167%
30	22.780	3430	3433	3440	rBV3	79839	144074	2.04%	0.177%
31	23.315	3517	3524	3539	rVB2	2704260	5446302	77.24%	6.703%
32	23.456	3541	3548	3557	rVV	1845243	3459639	49.07%	4.258%
33	23.968	3631	3635	3643	rVB2	104960	190312	2.70%	0.234%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006234.D
Acq On : 03 Jul 2016 14:22
Operator : UM/SJ
Sample : H3819-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Title : SVOA CALIBRATION


Sum of corrected areas: 81252248

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006234.D
Acq On : 03 Jul 2016 14:22
Operator : UM/SJ
Sample : H3819-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

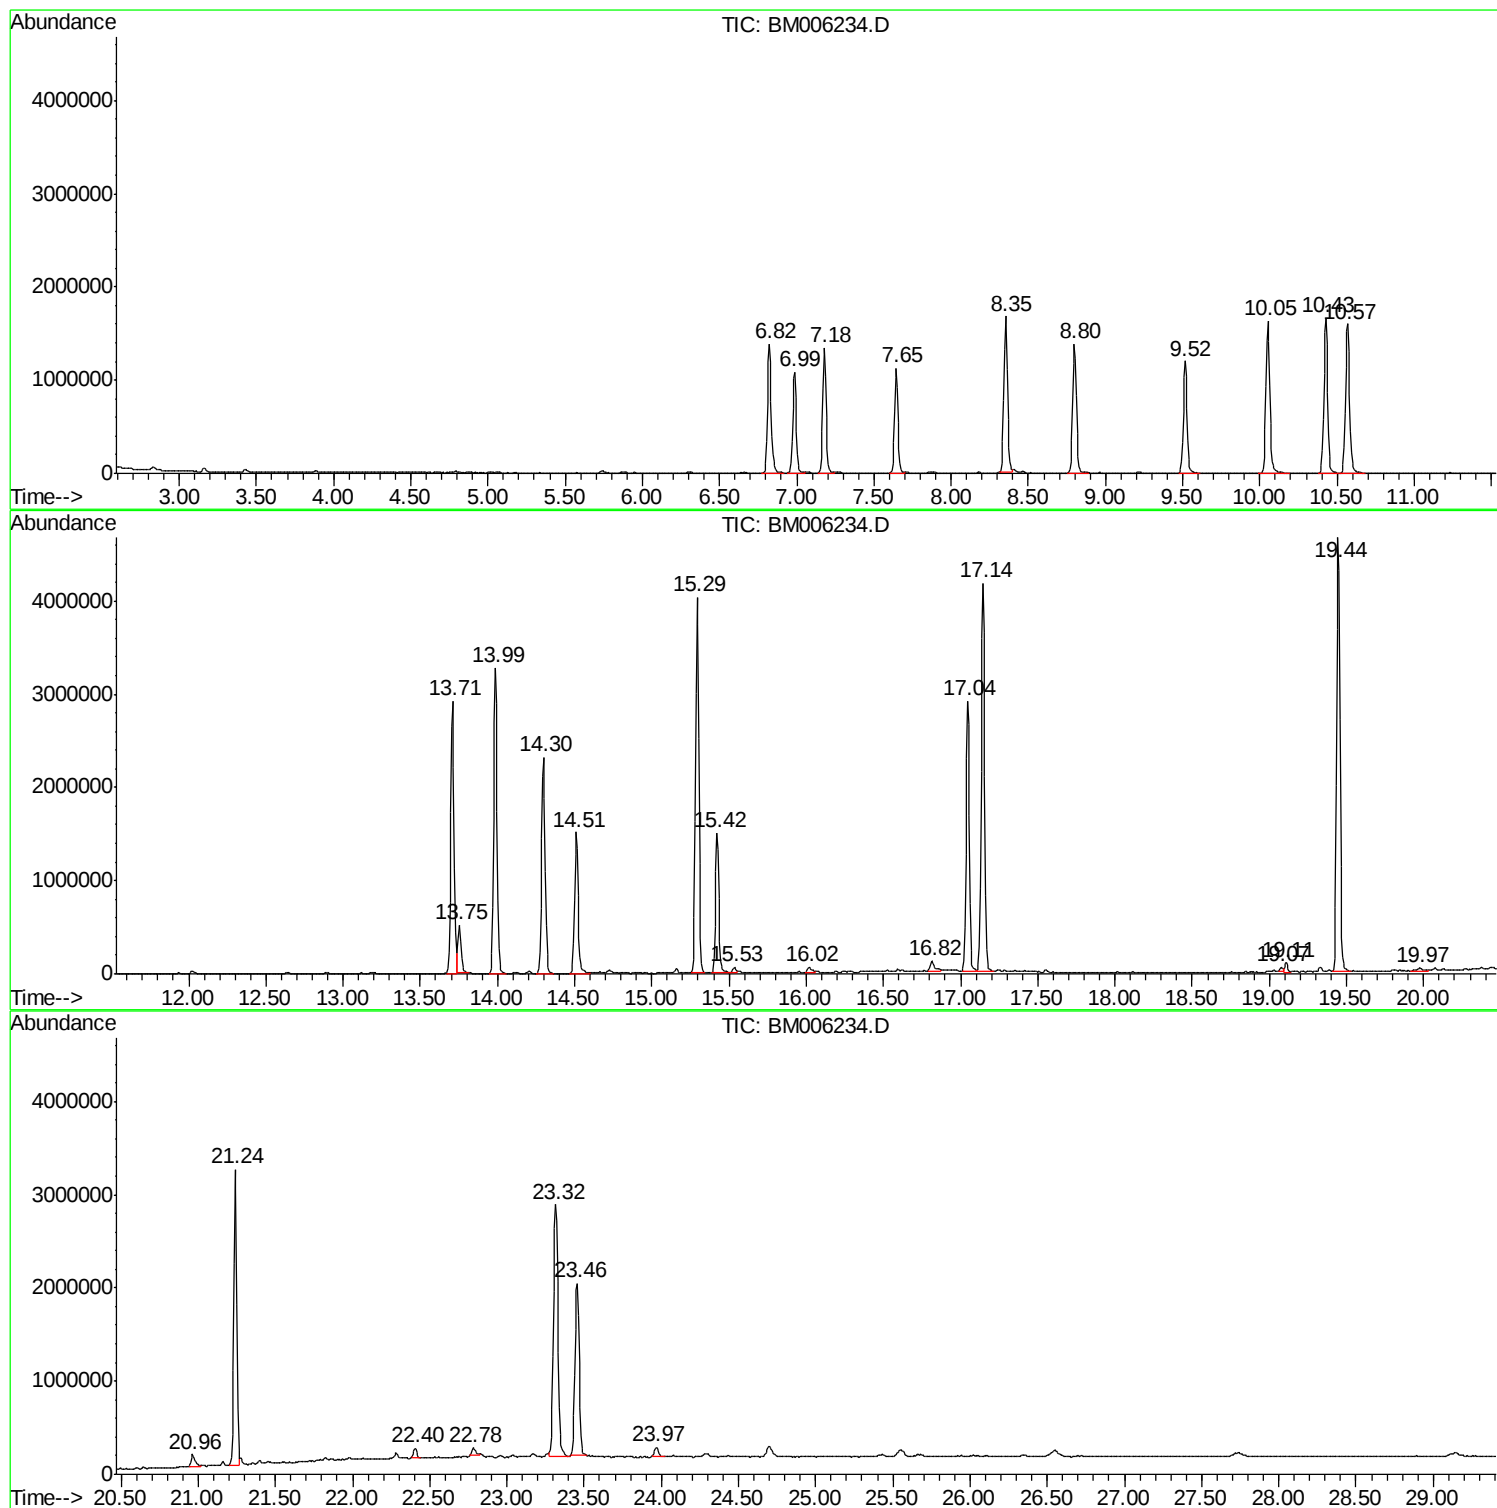

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006234.D
Acq On : 03 Jul 2016 14:22
Operator : UM/SJ
Sample : H3819-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006234.D
Acq On : 03 Jul 2016 14:22
Operator : UM/SJ
Sample : H3819-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc