

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006235.D
 Acq On : 03 Jul 2016 14:58
 Operator : UM/SJ
 Sample : H3819-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.822	710	720	739	rBV	1017703	1751141	31.24%	2.498%
2	6.987	741	748	760	rBV	798478	1288916	22.99%	1.839%
3	7.181	774	781	792	rBV	989033	1631116	29.10%	2.327%
4	7.645	851	860	870	rBV	1161242	1891370	33.74%	2.698%
5	8.351	967	980	996	rBV	1281453	2189972	39.07%	3.124%
6	8.798	1049	1056	1064	rBV	1037250	1738331	31.01%	2.480%
7	9.516	1171	1178	1188	rBV	869732	1506696	26.88%	2.149%
8	10.051	1262	1269	1285	rVB	1211223	2149864	38.35%	3.067%
9	10.428	1324	1333	1345	rBV	1680017	2988949	53.32%	4.264%
10	10.569	1349	1357	1369	rBV	1233143	2276133	40.60%	3.247%
11	13.704	1884	1890	1895	rBV	2257441	3491609	62.29%	4.981%
12	13.751	1895	1898	1913	rVB	405575	658368	11.74%	0.939%
13	13.986	1929	1938	1949	rBV	2640838	4026677	71.83%	5.744%
14	14.298	1982	1991	2000	rBV2	2377004	3908756	69.73%	5.576%
15	14.510	2020	2027	2042	rBV	1208719	1961810	35.00%	2.798%
16	15.292	2153	2160	2171	rBV	3239878	4986605	88.96%	7.113%
17	15.421	2176	2182	2197	rBV	1151293	1687555	30.10%	2.407%
18	15.533	2197	2201	2204	rBV2	43947	70046	1.25%	0.100%
19	16.045	2280	2288	2299	rBV2	80464	222900	3.98%	0.318%
20	16.815	2415	2419	2424	rBV2	88052	149848	2.67%	0.214%
21	17.045	2452	2458	2468	rBV2	2957900	4442917	79.26%	6.338%
22	17.145	2468	2475	2485	rVB	3478246	5245621	93.58%	7.483%
23	18.956	2779	2783	2789	rBV	165692	213838	3.81%	0.305%
24	19.333	2843	2847	2852	rVB	50408	70962	1.27%	0.101%
25	19.445	2859	2866	2875	rBV2	3944819	5605635	100.00%	7.996%
26	20.962	3120	3124	3132	rBV2	165524	291935	5.21%	0.416%
27	21.162	3154	3158	3165	rVB	319339	360659	6.43%	0.514%
28	21.239	3165	3171	3182	rBV	3181653	4288033	76.50%	6.117%
29	22.280	3345	3348	3353	rVB2	67017	79065	1.41%	0.113%
30	22.780	3430	3433	3441	rVB2	95103	137955	2.46%	0.197%
31	23.315	3516	3524	3537	rVB2	2290484	4568203	81.49%	6.516%
32	23.456	3540	3548	3557	rBV	1915635	3687900	65.79%	5.261%
33	23.968	3631	3635	3643	rVB	131885	254418	4.54%	0.363%
34	24.697	3755	3759	3768	rVB	125379	279092	4.98%	0.398%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006235.D
Acq On : 03 Jul 2016 14:58
Operator : UM/SJ
Sample : H3819-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Title : SVOA CALIBRATION


Sum of corrected areas: 70102895

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006235.D
Acq On : 03 Jul 2016 14:58
Operator : UM/SJ
Sample : H3819-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BDHX7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

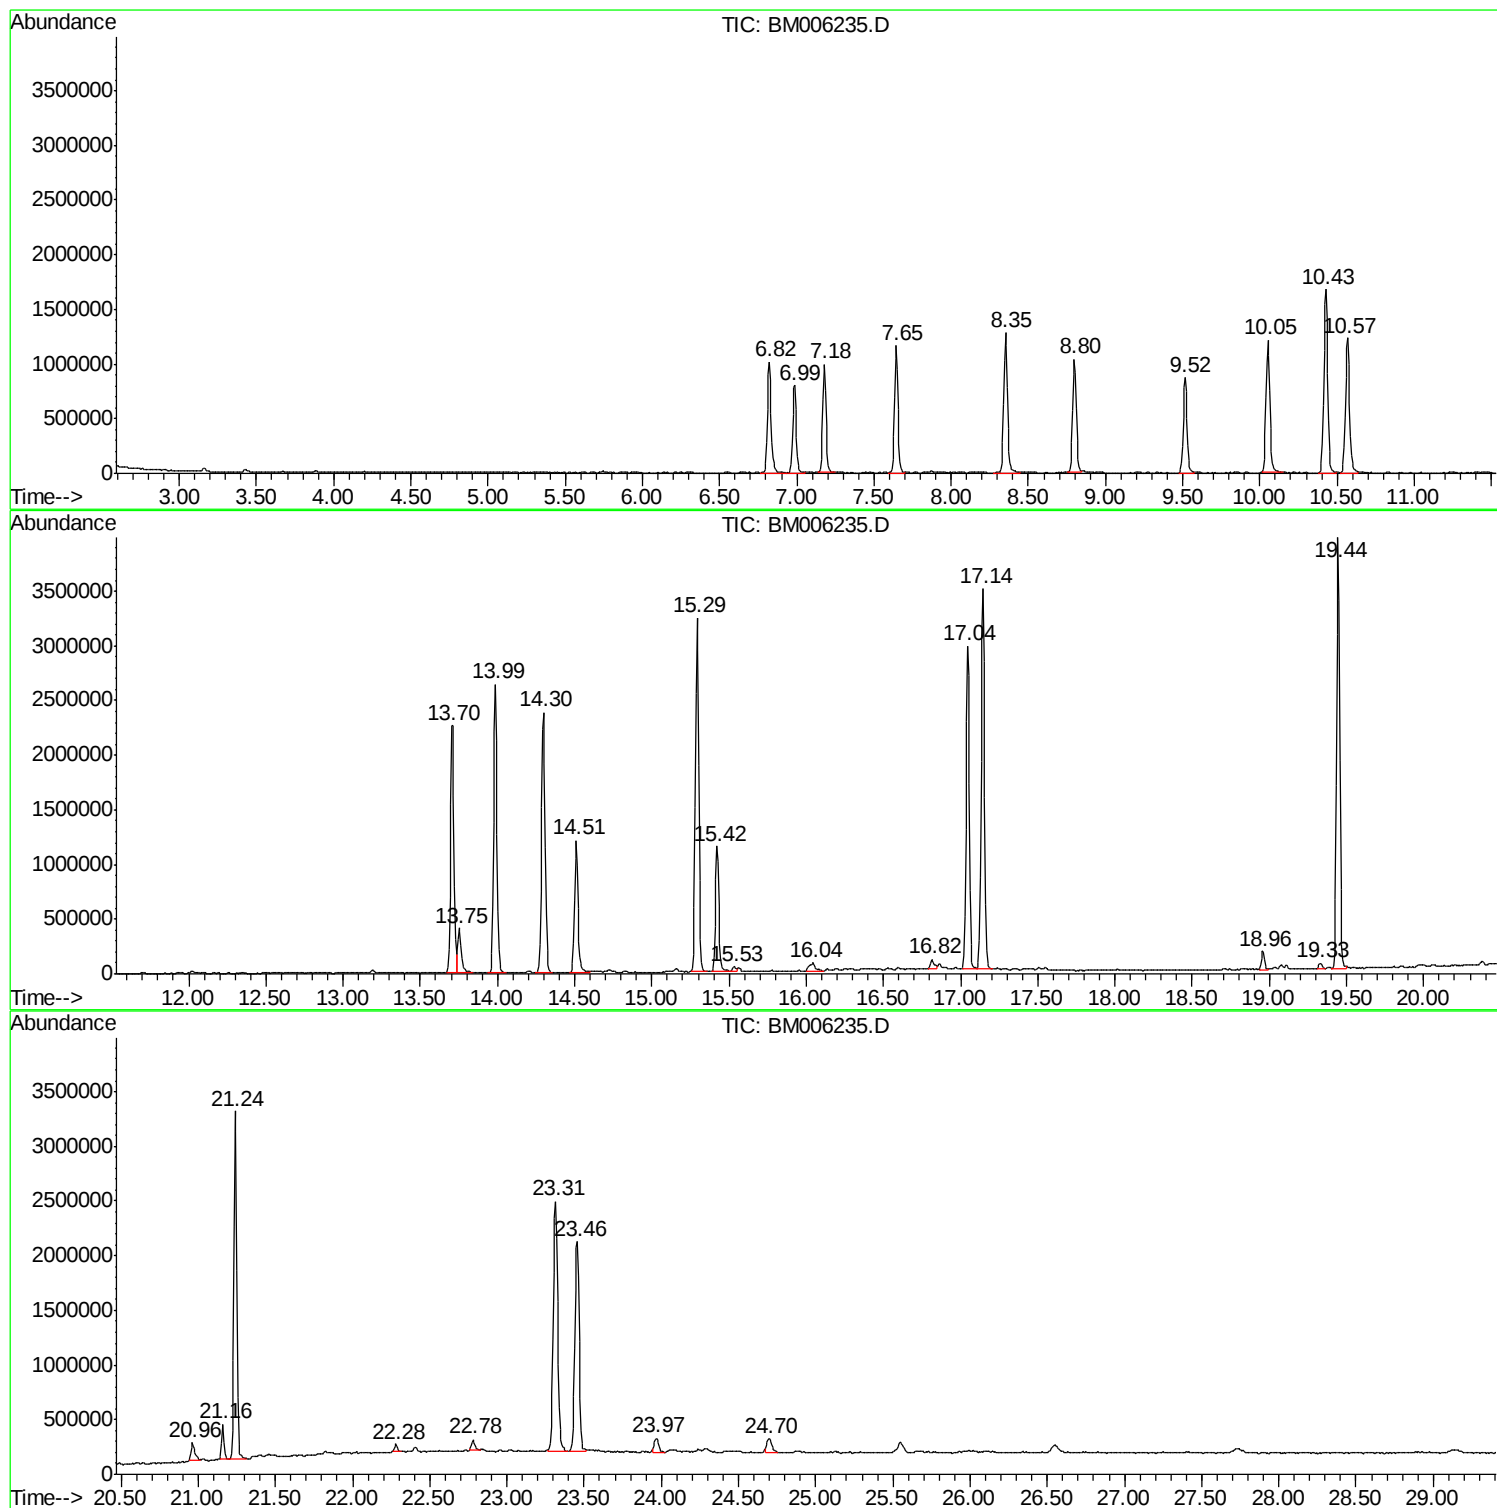

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006235.D
Acq On : 03 Jul 2016 14:58
Operator : UM/SJ
Sample : H3819-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006235.D
Acq On : 03 Jul 2016 14:58
Operator : UM/SJ
Sample : H3819-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHX7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc