

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
 Data File : BM006244.D
 Acq On : 03 Jul 2016 20:59
 Operator : UM/SJ
 Sample : H3797-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDHQ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.828	37	41	46	rBV	47328	75757	1.38%	0.109%
2	3.422	139	142	153	rVB	60446	87295	1.59%	0.126%
3	6.822	713	720	737	rBV	1191905	2053666	37.45%	2.966%
4	6.981	741	747	760	rVV	963665	1549200	28.25%	2.237%
5	7.175	773	780	794	rBV	1199537	2028613	36.99%	2.930%
6	7.645	853	860	874	rVB	1032942	1714308	31.26%	2.476%
7	8.351	970	980	997	rBV	1536583	2587302	47.18%	3.737%
8	8.798	1048	1056	1071	rBV	1272451	2105496	38.39%	3.041%
9	9.516	1170	1178	1194	rVB	1048052	1788186	32.61%	2.583%
10	10.051	1260	1269	1283	rBV	1418394	2556338	46.61%	3.692%
11	10.428	1325	1333	1348	rBV	1448910	2586725	47.17%	3.736%
12	10.563	1349	1356	1374	rVB	1438310	2692294	49.09%	3.888%
13	13.710	1879	1891	1895	rBV	2358661	3605256	65.74%	5.207%
14	13.751	1895	1898	1916	rVB	1151454	1685467	30.73%	2.434%
15	13.986	1931	1938	1951	rVB	2841172	4426250	80.71%	6.393%
16	14.292	1983	1990	2001	rBV2	1975917	3237535	59.04%	4.676%
17	14.510	2020	2027	2041	rBV	740279	1248280	22.76%	1.803%
18	15.292	2153	2160	2168	rBV	3432652	5144056	93.80%	7.429%
19	15.421	2176	2182	2192	rBV	639048	952812	17.37%	1.376%
20	15.527	2197	2200	2206	rBV	43813	59261	1.08%	0.086%
21	16.810	2413	2418	2426	rBV2	54746	107865	1.97%	0.156%
22	17.045	2451	2458	2467	rBV	2434610	3544315	64.63%	5.119%
23	17.145	2468	2475	2487	rVB2	3434017	5162384	94.13%	7.456%
24	17.551	2539	2544	2555	rVB	43675	69079	1.26%	0.100%
25	19.074	2799	2803	2807	rBV	38848	57724	1.05%	0.083%
26	19.445	2859	2866	2874	rBV	3824590	5484049	100.00%	7.921%
27	21.239	3165	3171	3180	rBV	2831169	3624800	66.10%	5.235%
28	22.403	3365	3369	3374	rBV	92980	128146	2.34%	0.185%
29	22.780	3429	3433	3441	rVB2	77021	125156	2.28%	0.181%
30	23.315	3516	3524	3536	rVB2	2519840	4960084	90.45%	7.164%
31	23.450	3540	3547	3555	rBV2	1726707	3313988	60.43%	4.786%
32	23.962	3630	3634	3645	rVB3	104310	211541	3.86%	0.306%
33	24.697	3754	3759	3769	rVB2	112347	265253	4.84%	0.383%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006244.D
Acq On : 03 Jul 2016 20:59
Operator : UM/SJ
Sample : H3797-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHQ1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Title : SVOA CALIBRATION


Sum of corrected areas: 69238481

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006244.D
Acq On : 03 Jul 2016 20:59
Operator : UM/SJ
Sample : H3797-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHQ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

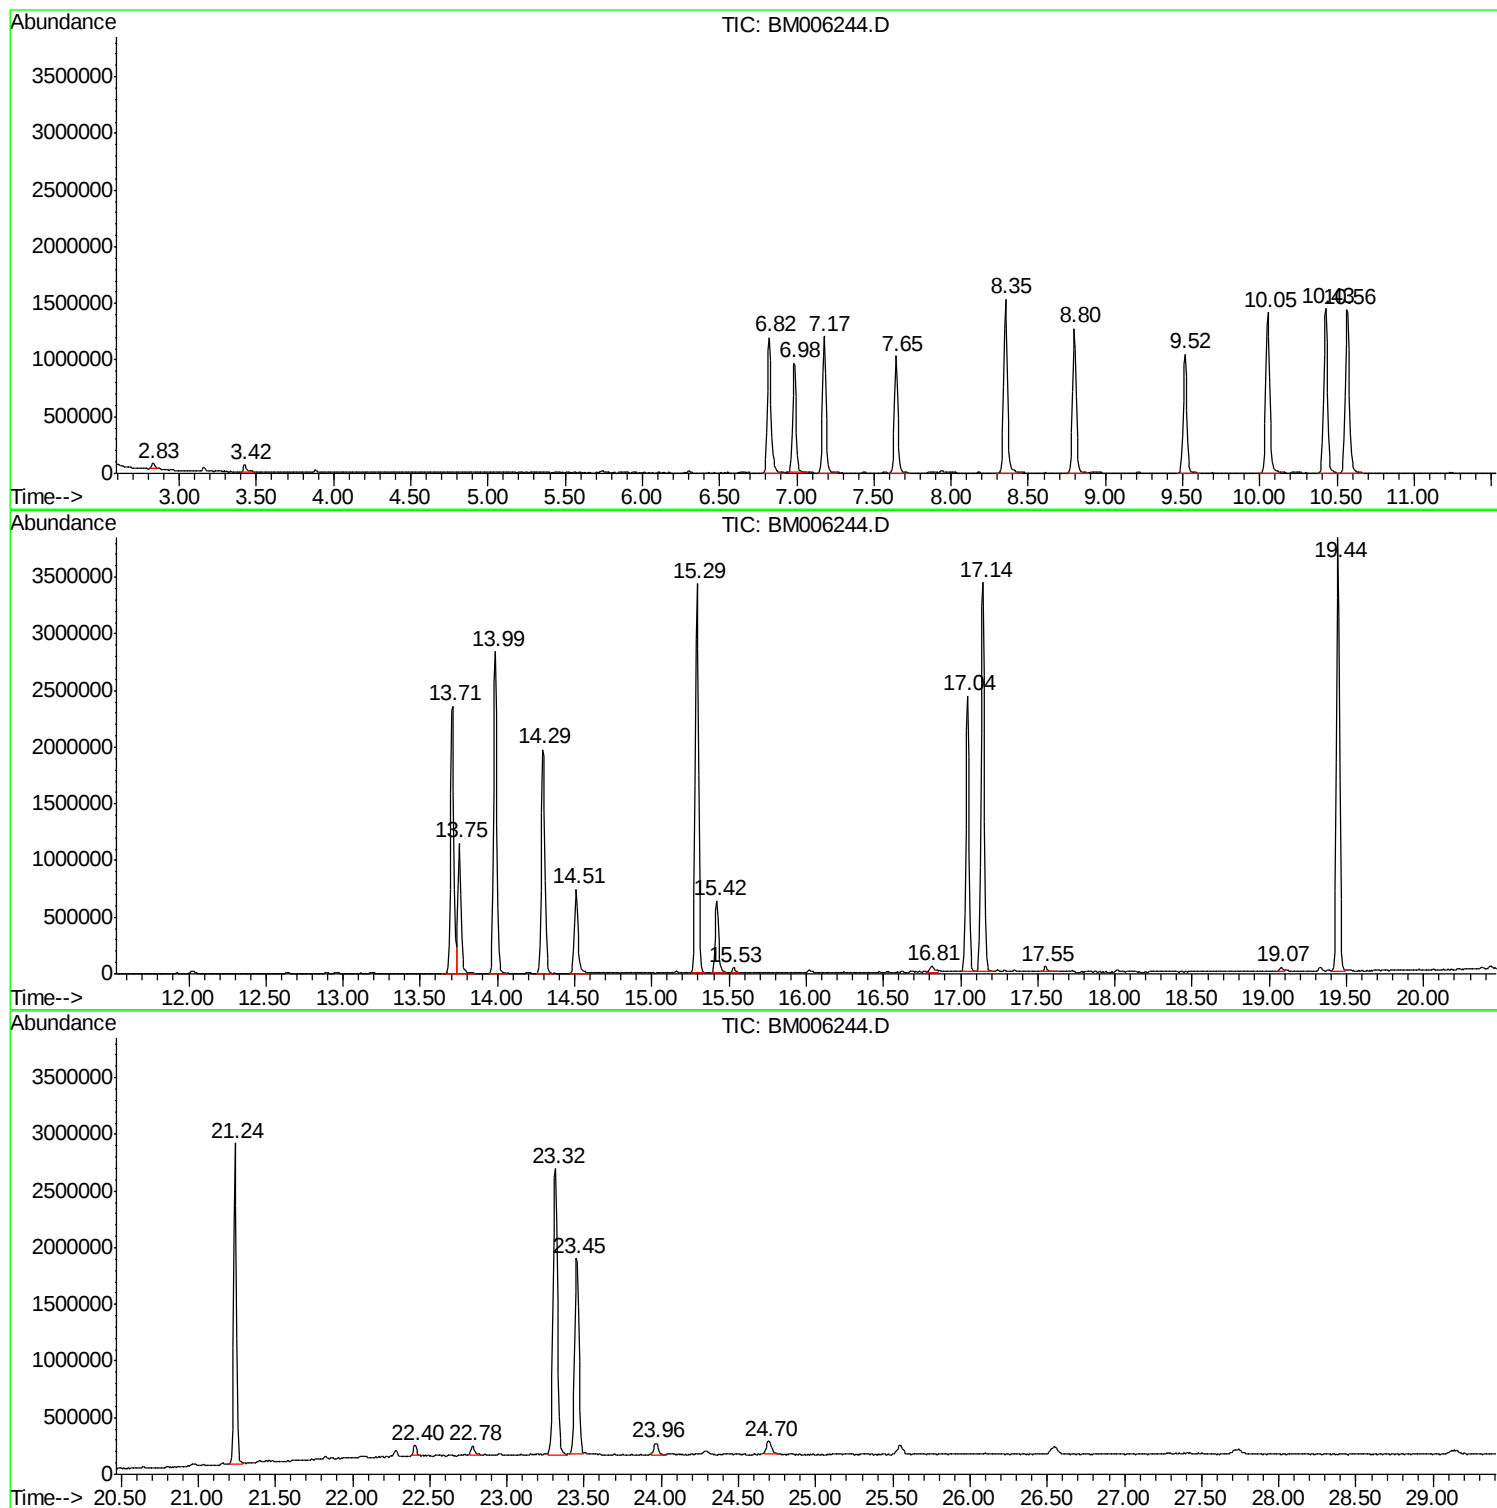

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006244.D
Acq On : 03 Jul 2016 20:59
Operator : UM/SJ
Sample : H3797-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHQ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070316\
Data File : BM006244.D
Acq On : 03 Jul 2016 20:59
Operator : UM/SJ
Sample : H3797-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDHQ1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc