

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
 Data File : BM006267.D
 Acq On : 05 Jul 2016 20:45
 Operator : UM/SJ
 Sample : H3877-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 V001-BF002-01

Quant Time: Jul 06 01:00:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 05 17:51:55 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	203904	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	880906	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	473885	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	974214	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1006144	20.00	ng/ul	0.00
83) Perylene-d12	23.45	264	1021690	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	7053	1.48	ng/uL	0.00
5) Phenol-d5	6.82	99	311810	16.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	204356	18.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	240402	16.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	247383	16.01	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	119713	17.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	124568	15.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	219265	15.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	324141	21.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	680532	17.21	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	870068	17.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	90566	12.08	ng/ul	0.00
57) Fluorene-d10	15.29	176	589416	17.29	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	62503	10.95	ng/ul	0.00
70) Anthracene-d10	17.14	188	862866	18.56	ng/ul	0.00
76) Pyrene-d10	19.44	212	924140	19.26	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.31	264	910799	19.19	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.75	163	140285	3.53	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
Data File : BM006267.D
Acq On : 05 Jul 2016 20:45
Operator : UM/SJ
Sample : H3877-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
V001-BF002-01

Quant Time: Jul 06 01:00:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 05 17:51:55 2016
Response via : Initial Calibration

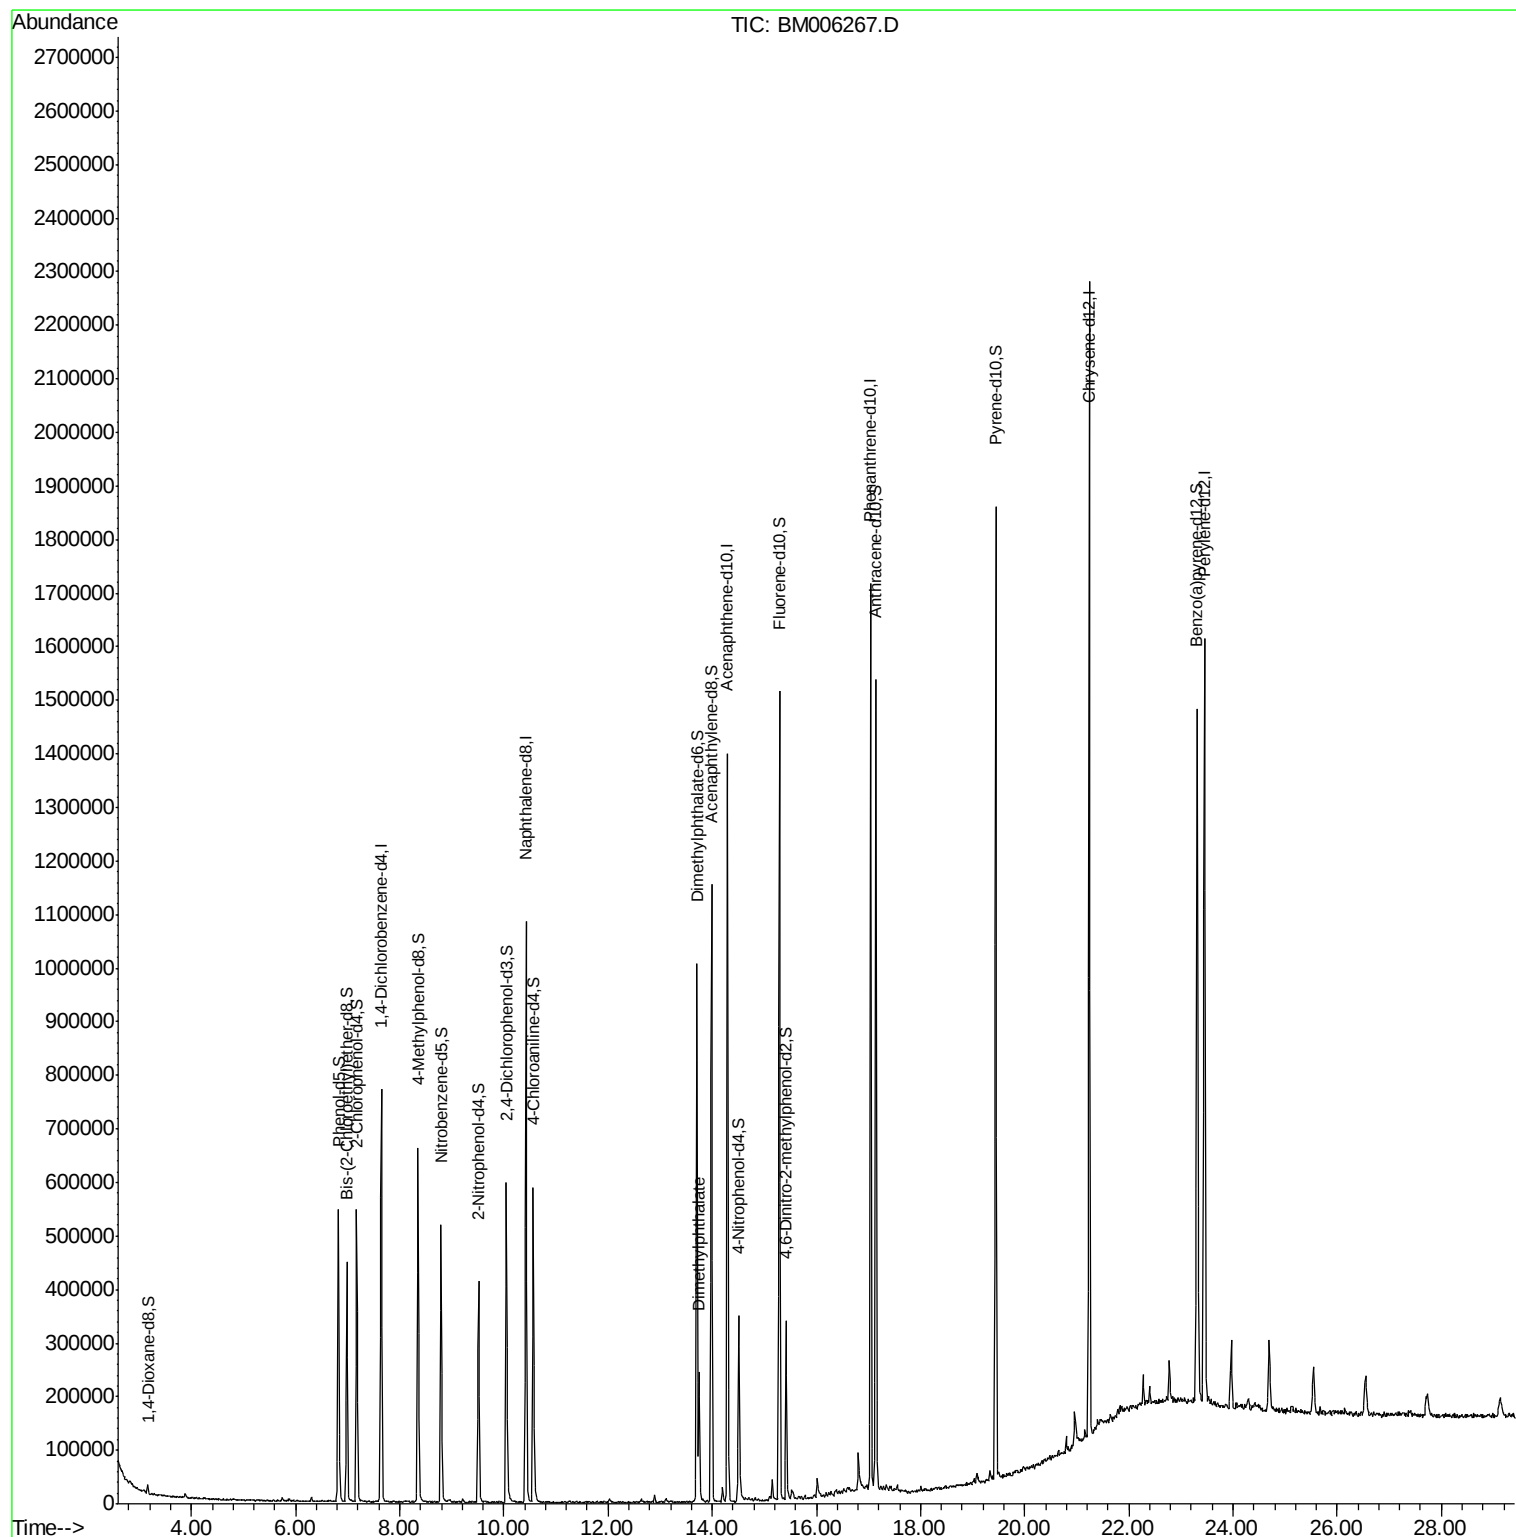

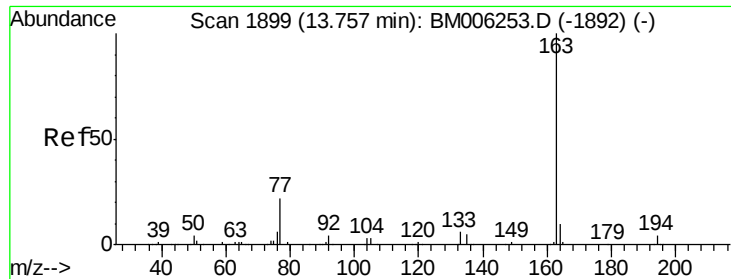

#44

Dimethylphthalate

Concen: 3.53 ng/ul

RT: 13.75 min Scan# 1898

Delta R.T. -0.01 min

Lab File: BM006267.D

Acq: 05 Jul 2016 20:45

Instrument :

BNA_M

ClientSampleId :

V001-BF002-01


Tgt Ion:163 Resp: 140285

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 9.8 7.8 11.8

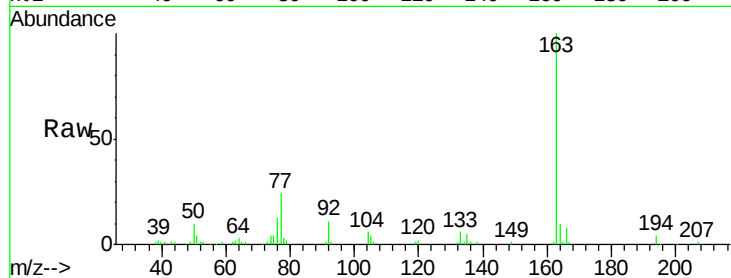

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

