

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
 Data File : BM006271.D
 Acq On : 05 Jul 2016 23:10
 Operator : UM/SJ
 Sample : H3877-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 V001-BF005-02

Quant Time: Jul 06 01:00:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 05 17:51:55 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	221820	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	957972	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.29	164	502814	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1066437	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	1130242	20.00	ng/ul	0.00
83) Perylene-d12	23.46	264	1168992	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.16	96	5228	1.01	ng/uL	0.00
5) Phenol-d5	6.82	99	229562	11.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	147473	12.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	175039	11.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	184499	10.98	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	84584	11.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	89362	10.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	163526	10.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	230797	14.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	504860	12.03	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	643943	12.39	ng/ul	0.00
51) 4-Nitrophenol-d4	14.51	143	71302	8.97	ng/ul	0.00
57) Fluorene-d10	15.29	176	442850	12.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	43572	6.97	ng/ul	0.00
70) Anthracene-d10	17.14	188	666381	13.10	ng/ul	0.00
76) Pyrene-d10	19.44	212	738364	13.70	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.31	264	735123	13.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.75	163	151107	3.58	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
Data File : BM006271.D
Acq On : 05 Jul 2016 23:10
Operator : UM/SJ
Sample : H3877-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
V001-BF005-02

Quant Time: Jul 06 01:00:46 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 05 17:51:55 2016
Response via : Initial Calibration

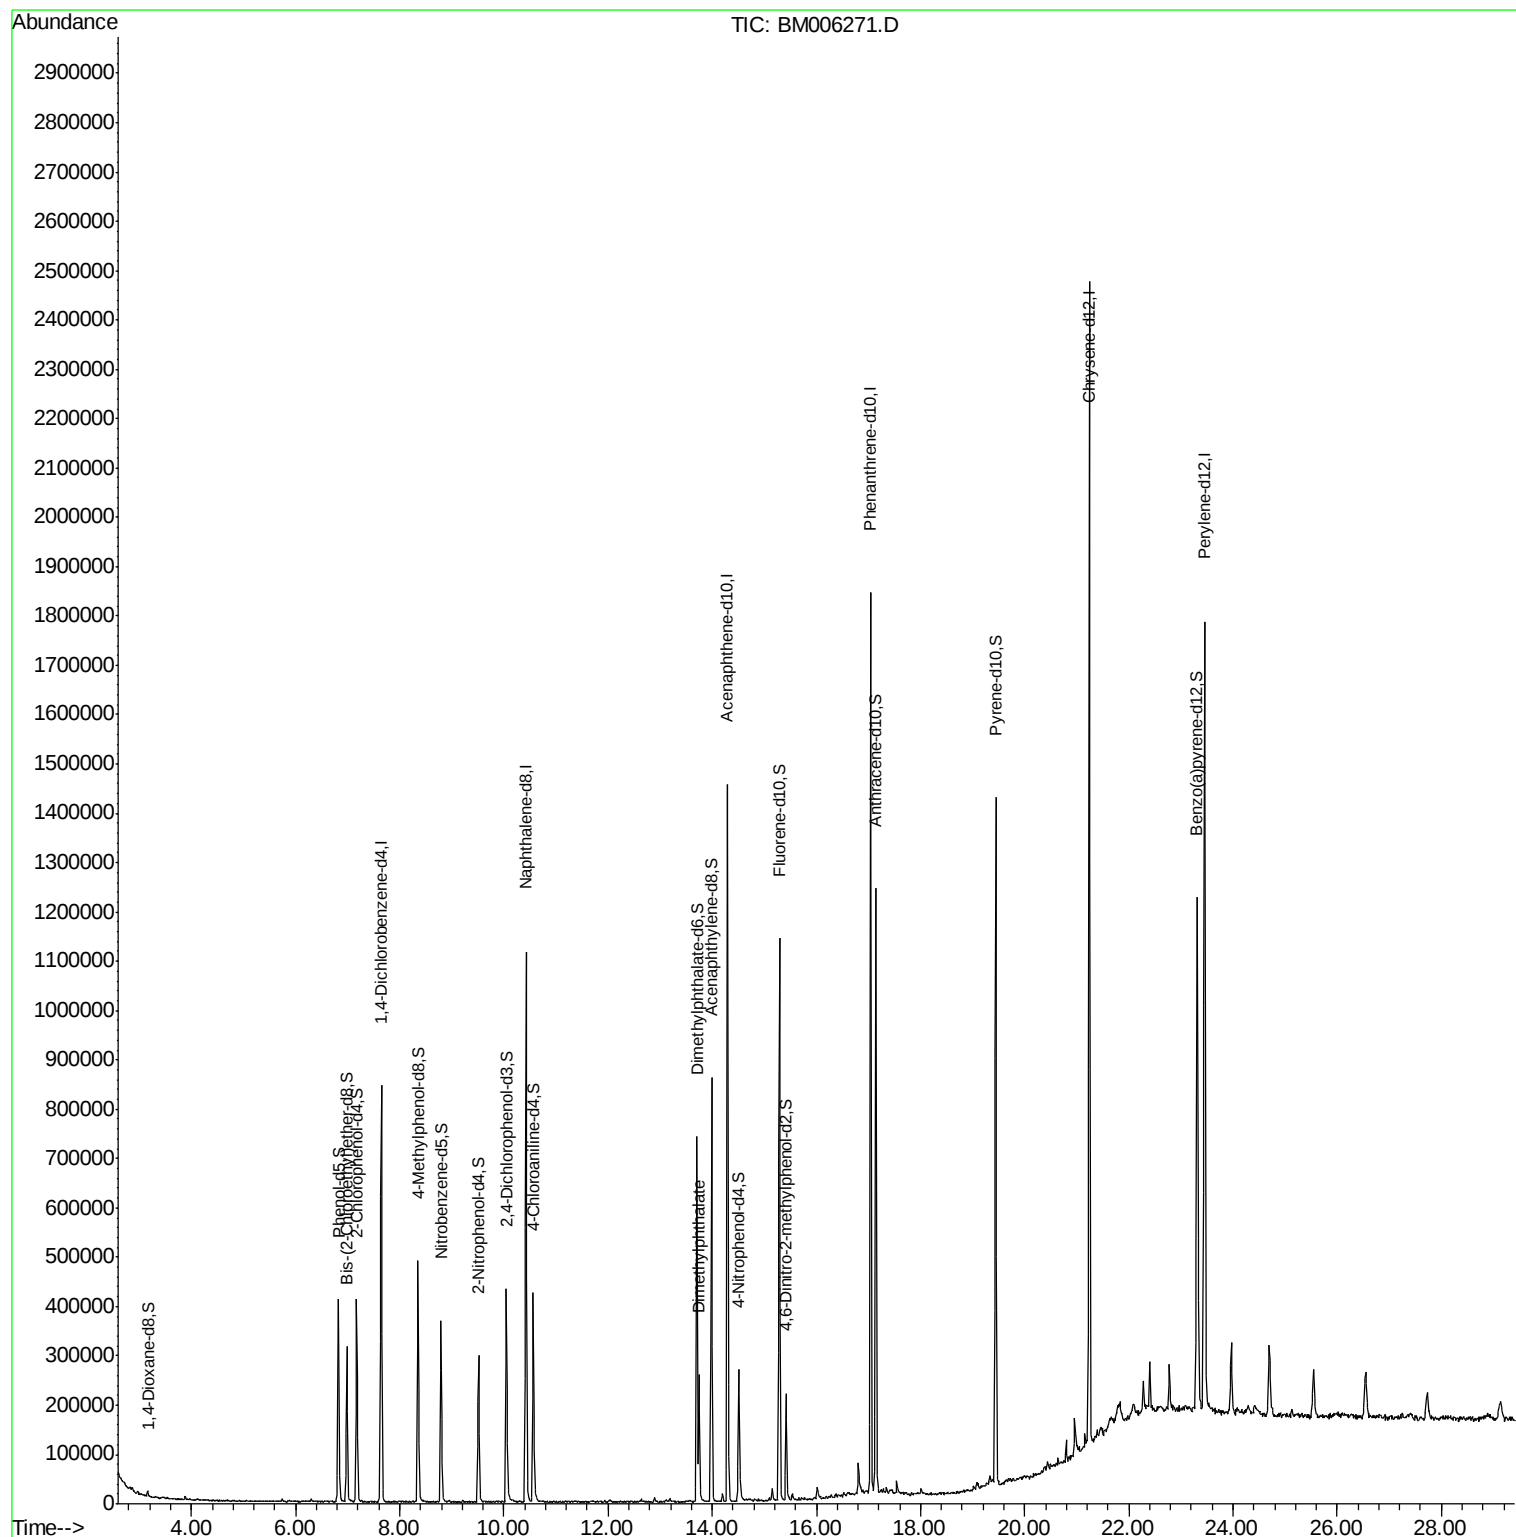

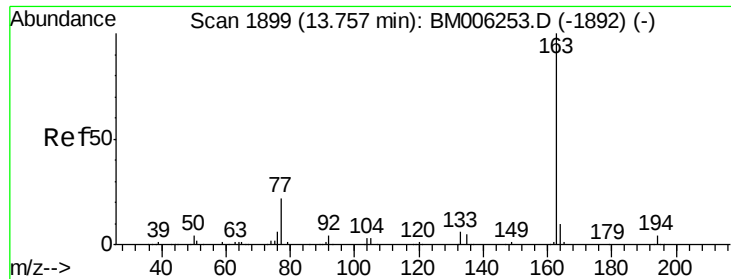

#44

Dimethylphthalate

Concen: 3.58 ng/ul

RT: 13.75 min Scan# 1898

Delta R.T. -0.01 min

Lab File: BM006271.D

Acq: 05 Jul 2016 23:10

Instrument :

BNA_M

ClientSampleId :

V001-BF005-02


Tgt Ion:163 Resp: 151107

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.5 7.8 11.8

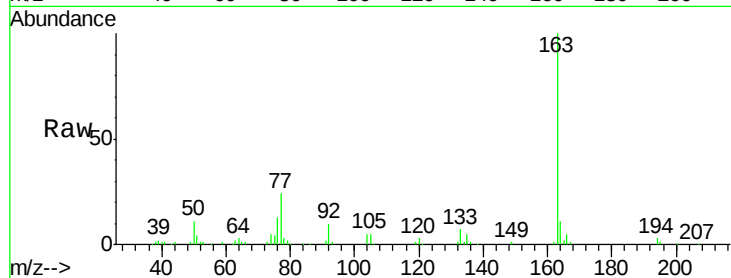

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

