

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
 Data File : BM006254.D
 Acq On : 05 Jul 2016 11:48
 Operator : UM/SJ
 Sample : PB91683BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.822	712	720	738	rBV	1543032	2496191	30.45%	3.007%
2	6.987	741	748	760	rBV	1172584	1895911	23.13%	2.284%
3	7.181	774	781	797	rBV	1471936	2450259	29.89%	2.951%
4	7.646	852	860	873	rBV	857983	1397845	17.05%	1.684%
5	8.351	973	980	1001	rBV	1889301	3192752	38.95%	3.846%
6	8.798	1049	1056	1071	rBV	1560911	2608571	31.82%	3.142%
7	9.516	1170	1178	1194	rBV	1300419	2244994	27.39%	2.704%
8	10.051	1262	1269	1290	rBV	1756536	3191181	38.93%	3.844%
9	10.428	1325	1333	1344	rBV	1228366	2176385	26.55%	2.622%
10	10.569	1348	1357	1373	rBV	1888150	3440940	41.97%	4.145%
11	13.710	1884	1891	1912	rVB	3366849	5055467	61.67%	6.089%
12	13.986	1930	1938	1949	rBV	3728889	5791897	70.65%	6.976%
13	14.298	1983	1991	2001	rBV2	1783661	2929264	35.73%	3.528%
14	14.510	2020	2027	2045	rBV	1737597	2792480	34.06%	3.364%
15	15.292	2153	2160	2173	rVB	4632738	6935026	84.60%	8.353%
16	15.422	2176	2182	2196	rBV	1575929	2296485	28.01%	2.766%
17	15.533	2196	2201	2208	rVB	63697	96091	1.17%	0.116%
18	17.045	2451	2458	2468	rBV	2428255	3471135	42.34%	4.181%
19	17.145	2468	2475	2489	rVV2	4970822	7474109	91.17%	9.003%
20	19.451	2860	2867	2874	rBV2	5479704	8197854	100.00%	9.875%
21	21.245	3167	3172	3180	rBV	2853118	3554872	43.36%	4.282%
22	23.321	3517	3525	3537	rBV2	3161685	6327739	77.19%	7.622%
23	23.462	3541	3549	3558	rVB	1511613	2875185	35.07%	3.463%
24	24.703	3757	3760	3766	rVB	65101	127616	1.56%	0.154%


Sum of corrected areas: 83020249

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
Data File : BM006254.D
Acq On : 05 Jul 2016 11:48
Operator : UM/SJ
Sample : PB91683BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK83

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

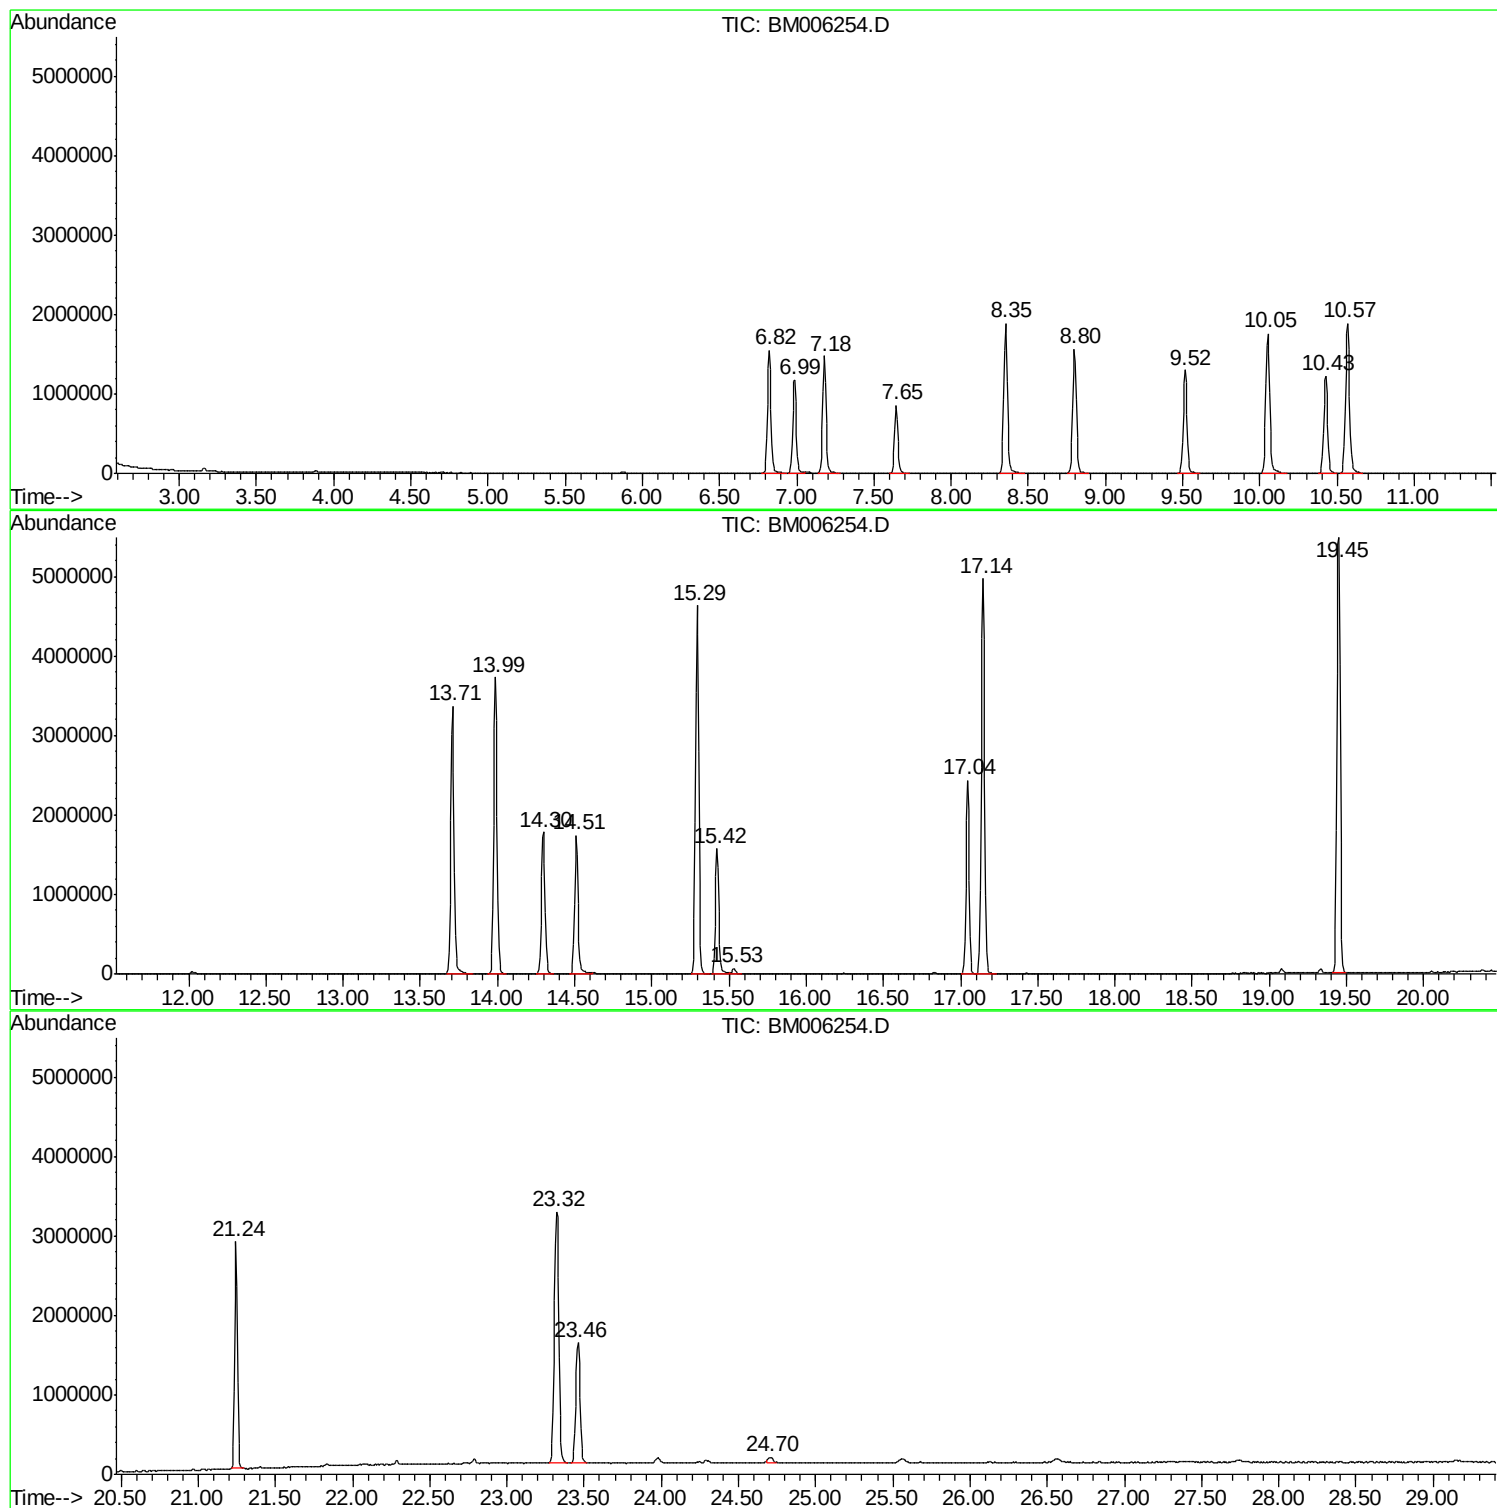

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
Data File : BM006254.D
Acq On : 05 Jul 2016 11:48
Operator : UM/SJ
Sample : PB91683BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK83

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070516\
Data File : BM006254.D
Acq On : 05 Jul 2016 11:48
Operator : UM/SJ
Sample : PB91683BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK83

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM070216.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc