

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070524\
 Data File : BM046411.D
 Acq On : 06 Jul 2024 10:18
 Operator : MA/JU
 Sample : PB161679BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK679

Quant Time: Jul 08 00:47:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 05 16:01:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.535	152	11956	0.400	ng/ul	0.00
4) Naphthalene-d8	10.299	136	34477	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.178	164	19194	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.94
17) Chrysene-d12	21.140	240	18437	0.400	ng/ul	0.00
23) Perylene-d12	23.297	264	18278	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.130	96	42700	3.458	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.899	152	14318	0.281	ng/ul	0.00
18) Fluoranthene-d10	18.970	212	20267	0.314	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.164	88	328	0.023	ng/ul#	42
20) Pyrene	19.337	202	3831	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.162	252	5916	0.096	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070524\
Data File : BM046411.D
Acq On : 06 Jul 2024 10:18
Operator : MA/JU
Sample : PB161679BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK679

Quant Time: Jul 08 00:47:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 05 16:01:25 2024
Response via : Initial Calibration




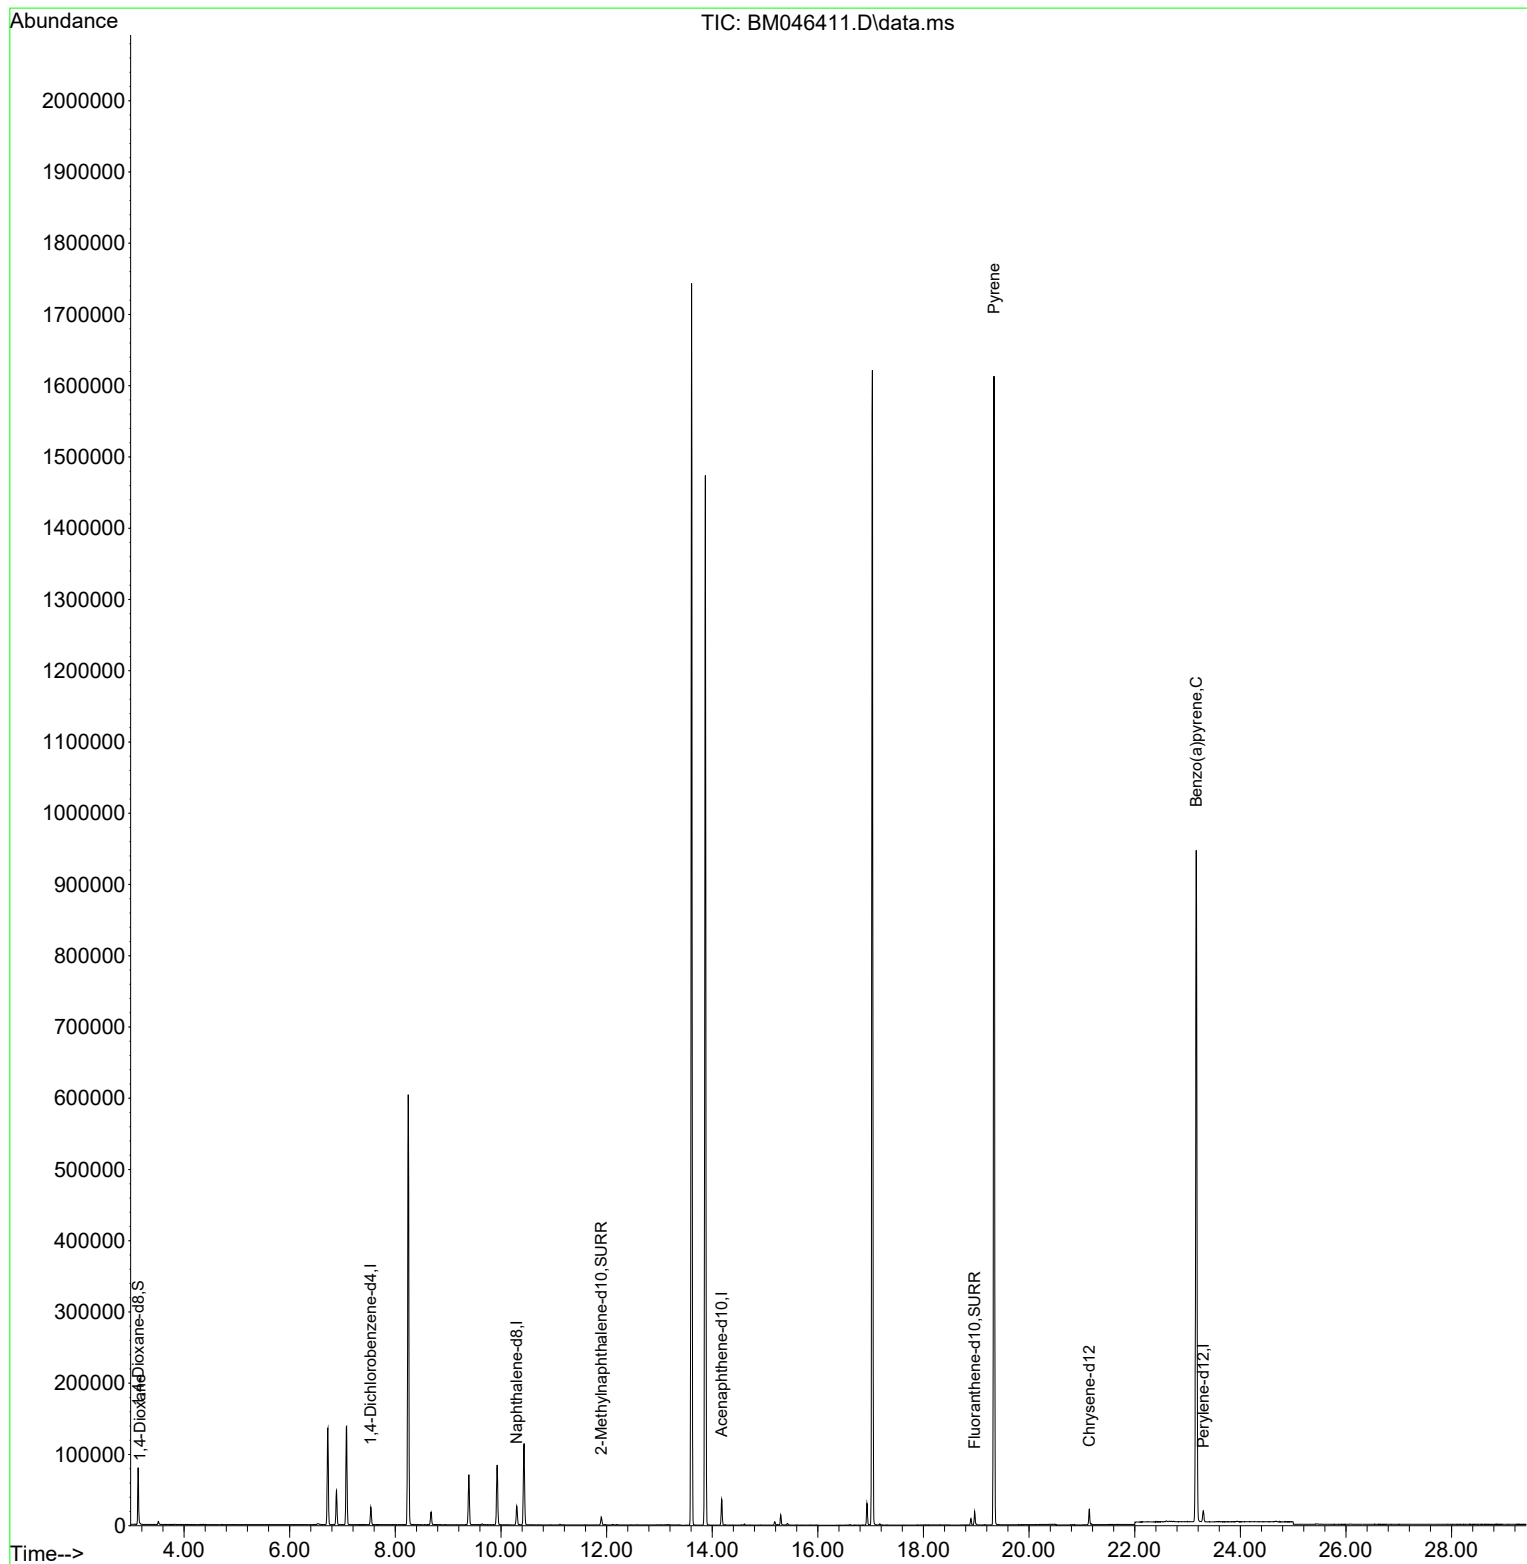


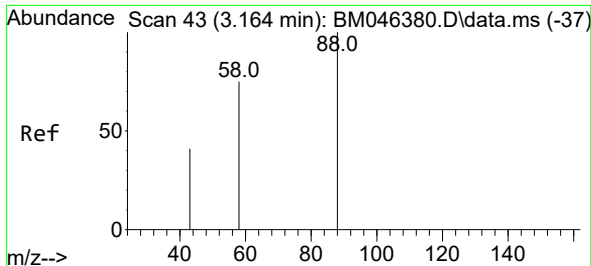

#2
1,4-Dioxane
Concen: 0.023 ng/ul
RT: 3.164 min Scan# 41
Delta R.T. 0.000 min
Lab File: BM046411.D
Acq: 06 Jul 2024 10:18




Instrument :
BNA_M
ClientSampleId :
SBLK679


Tgt Ion: 88 Resp: 328
Ion Ratio Lower Upper
88 100
43 120.3 41.9 62.9#
58 46.6 56.5 84.7#

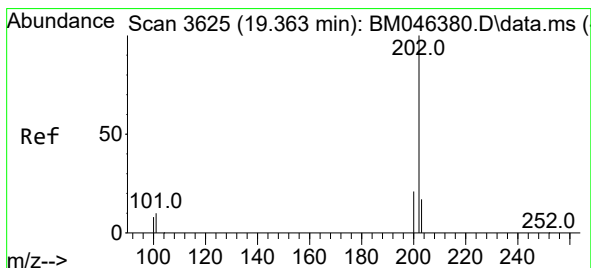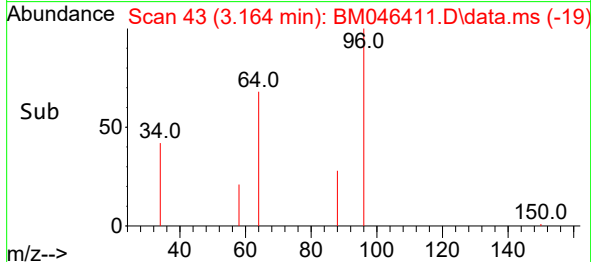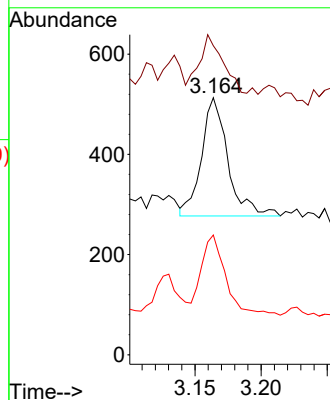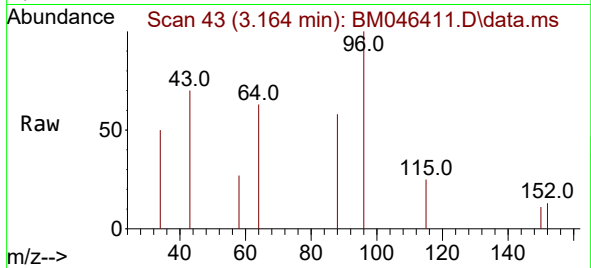

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.337 min Scan# 3619
Delta R.T. -0.026 min
Lab File: BM046411.D
Acq: 06 Jul 2024 10:18


Tgt Ion: 202 Resp: 3831
Ion Ratio Lower Upper
202 100
101 151.0 8.2 12.4#
100 1090.7 6.9 10.3#

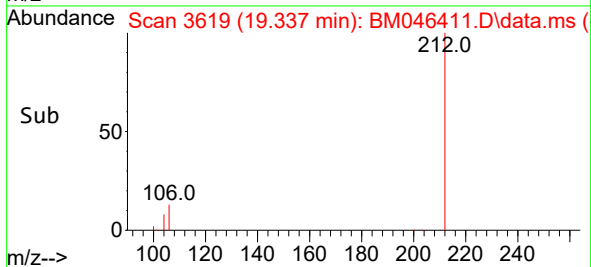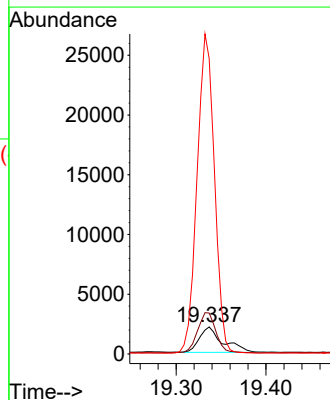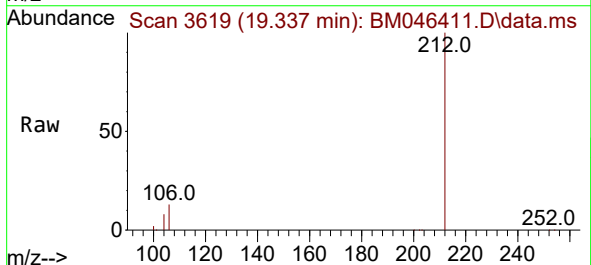

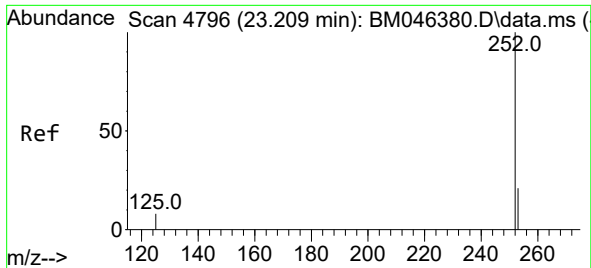

#26
 Benzo(a)pyrene
 Concen: 0.096 ng/ul
 RT: 23.162 min Scan# 41
 Delta R.T. -0.047 min
 Lab File: BM046411.D
 Acq: 06 Jul 2024 10:18

Instrument :
 BNA_M
 ClientSampleId :
 SBLK679

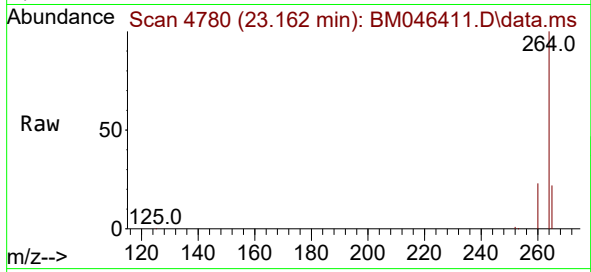

Tgt Ion:252 Resp: 5916
 Ion Ratio Lower Upper
 252 100
 253 44.2 18.9 28.3#
 125 44.4 8.1 12.1#

