

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070524\
 Data File : BM046413.D
 Acq On : 06 Jul 2024 11:31
 Operator : MA/JU
 Sample : P2982-08
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4CF4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/08/2024
 Supervised By :mohammad ahmed 07/08/2024

Quant Time: Jul 08 00:47:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 05 16:01:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.535	152	11459	0.400	ng/ul	0.00
4) Naphthalene-d8	10.298	136	33812	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.178	164	21246	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.934	188	32179	0.400	ng/ul	0.00
17) Chrysene-d12	21.149	240	12287	0.400	ng/ul	# 0.00
23) Perylene-d12	23.305	264	21145	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.130	96	28747	2.429	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.899	152	12986	0.260	ng/ul	0.00
18) Fluoranthene-d10	18.979	212	11854	0.275	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.348	128	150911	1.681	ng/ul	99
7) 2-Methylnaphthalene	11.976	142	127821	2.106	ng/ul	98
8) 1-Methylnaphthalene	12.196	142	142056	2.271	ng/ul	99
10) Acenaphthylene	13.896	152	875695	8.121	ng/ul	100
11) Acenaphthene	14.243	153	198401	2.822	ng/ul	98
12) Fluorene	15.238	166	599673	7.226	ng/ul	99
14) Pentachlorophenol	16.592	266	214	0.023	ng/ul	93
15) Phenanthrene	16.985	178	8777140	91.083	ng/ul	100
16) Anthracene	17.069	178	2068920	22.135	ng/ul	100
19) Fluoranthene	19.016	202	10842801	174.582	ng/ul	98
20) Pyrene	19.378	202	9097849	142.367	ng/ul	97
21) Benzo(a)anthracene	21.131	228	4289355	78.132	ng/ul	93
22) Chrysene	21.184	228	3691436	67.628	ng/ul	97
24) Benzo(b)fluoranthene	22.677	252	4136487m	46.014	ng/ul	
25) Benzo(k)fluoranthene	22.709	252	1446838m	15.944	ng/ul	
26) Benzo(a)pyrene	23.218	252	1865325m	26.252	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.463	276	1478091	15.398	ng/ul#	91
28) Dibenzo(a,h)anthracene	25.473	278	486026	6.545	ng/ul	97
29) Benzo(g,h,i)perylene	26.107	276	216404	2.827	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070524\
Data File : BM046413.D
Acq On : 06 Jul 2024 11:31
Operator : MA/JU
Sample : P2982-08
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4CF4

Quant Time: Jul 08 00:47:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 05 16:01:25 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

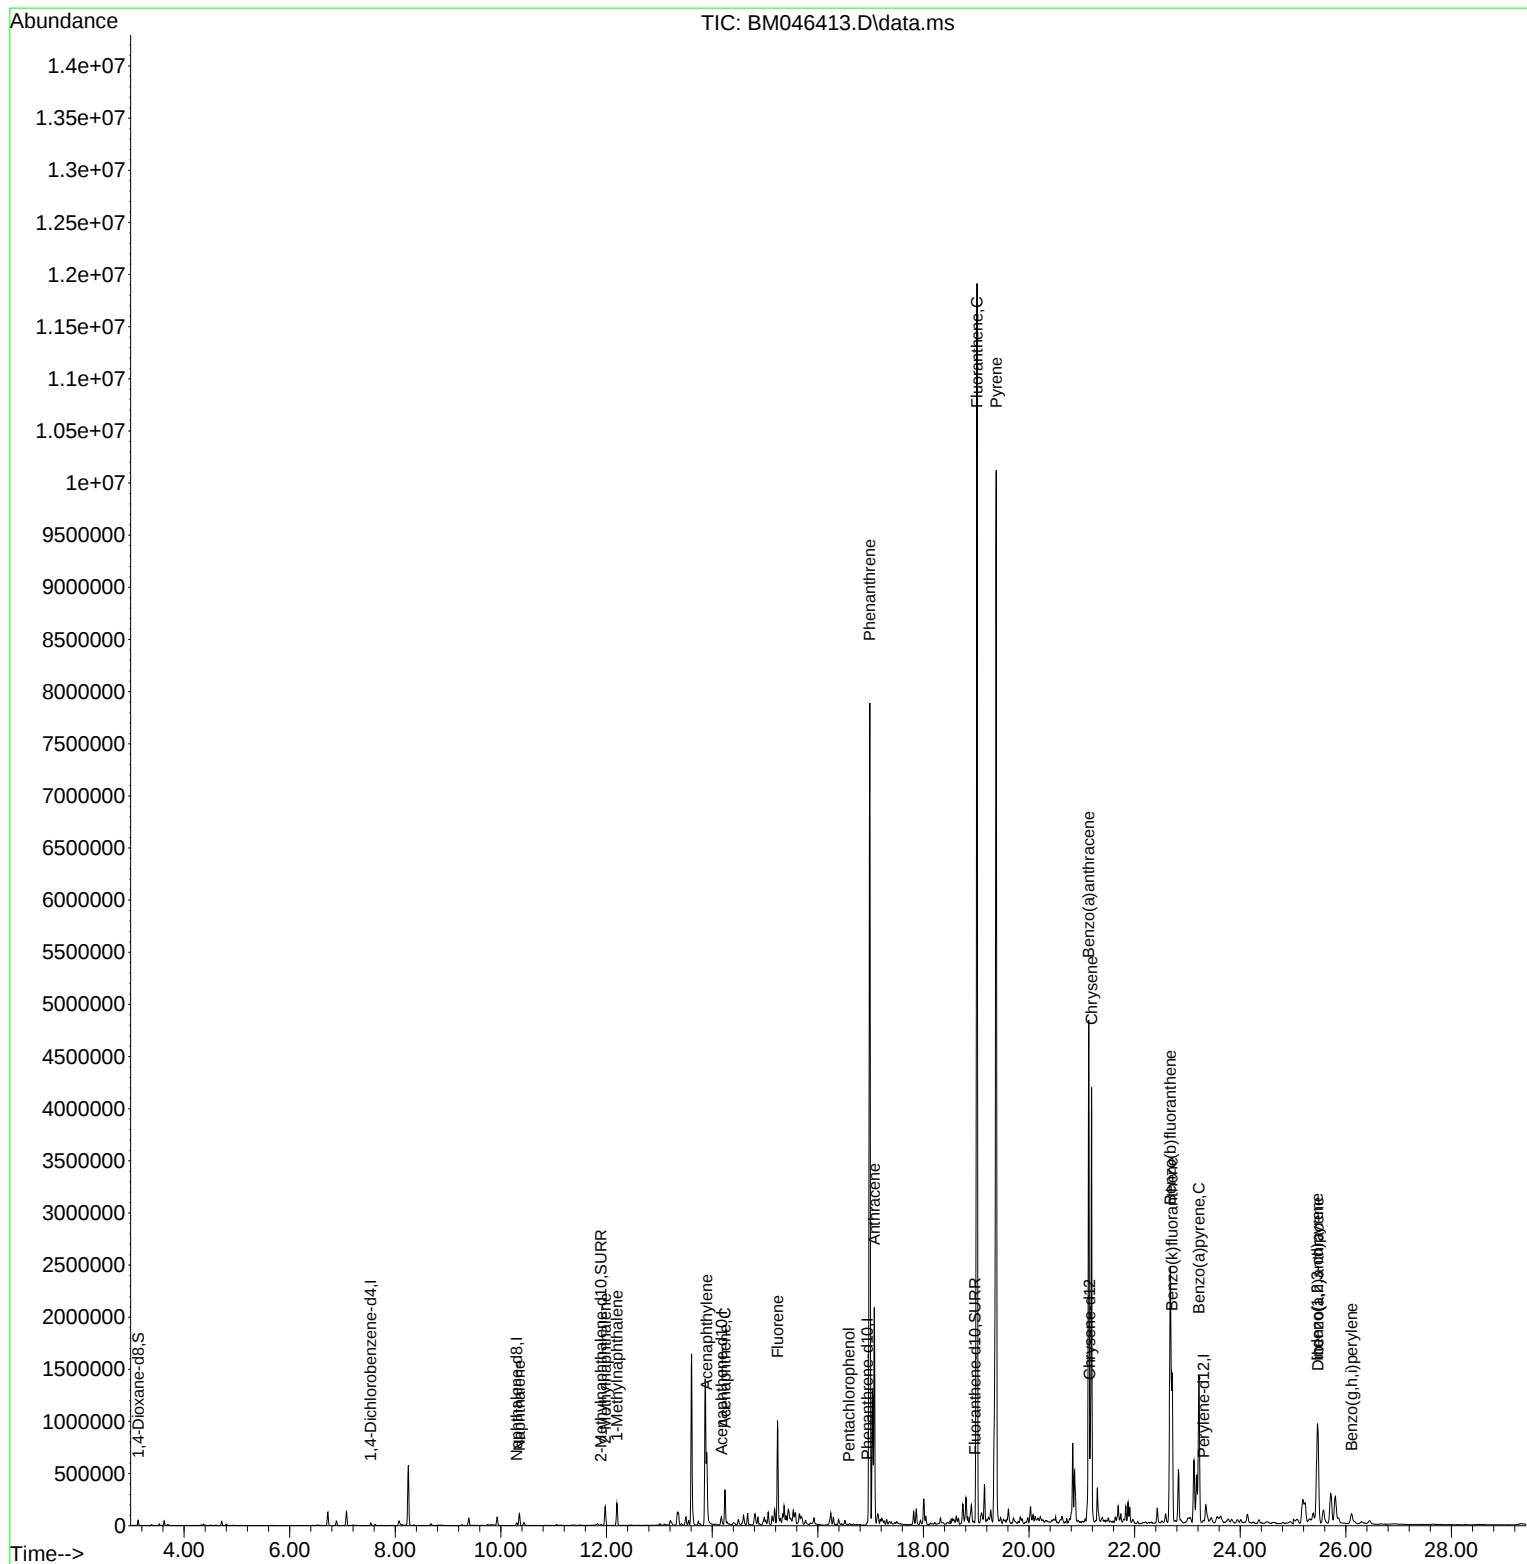

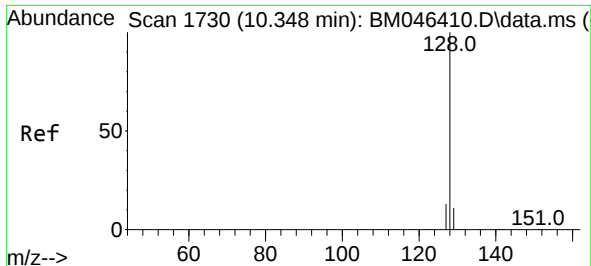

#5
Naphthalene
Concen: 1.681 ng/ul
RT: 10.348 min Scan# 1730
Delta R.T. -0.004 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Instrument :
BNA_M
ClientSampleId :
A4CF4




Tgt Ion:128 Resp: 15091
Ion Ratio Lower Upper
128 100
129 11.0 9.4 14.0
127 13.1 10.8 16.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024




#7
2-Methylnaphthalene
Concen: 2.106 ng/ul
RT: 11.976 min Scan# 2026
Delta R.T. -0.004 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Tgt Ion:142 Resp: 127821
Ion Ratio Lower Upper
142 100
141 88.6 69.8 104.6





#8
1-Methylnaphthalene
Concen: 2.271 ng/ul
RT: 12.196 min Scan# 2066
Delta R.T. -0.004 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Instrument :
BNA_M
ClientSampleId :
A4CF4



Tgt Ion:142 Resp: 142050
Ion Ratio Lower Upper
142 100
141 91.5 72.4 108.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

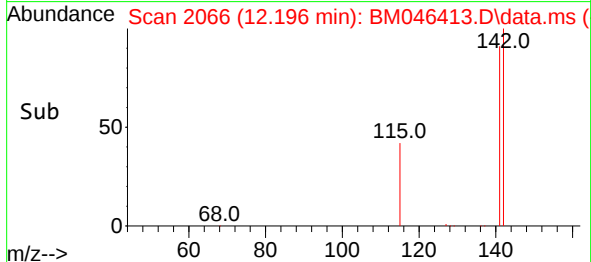

#10
Acenaphthylene
Concen: 8.121 ng/ul
RT: 13.896 min Scan# 2392
Delta R.T. -0.003 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31


Tgt Ion:152 Resp: 875695
Ion Ratio Lower Upper
152 100
151 19.8 15.9 23.9
153 13.8 11.0 16.6

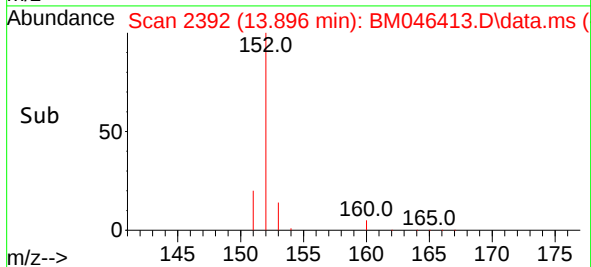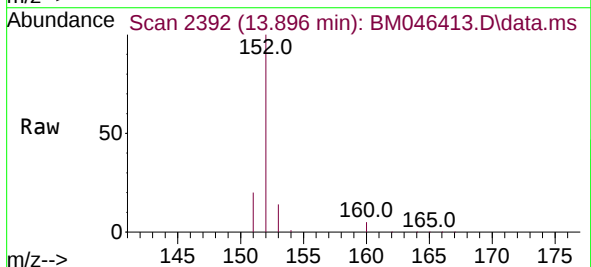



#11
Acenaphthene
Concen: 2.822 ng/ul
RT: 14.243 min Scan# 2467
Delta R.T. -0.003 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Instrument :
BNA_M
ClientSampleId :
A4CF4



Tgt Ion:153 Resp: 19840
Ion Ratio Lower Upper
153 100
152 48.8 40.4 60.6
154 88.7 72.1 108.1




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024



#12
Fluorene
Concen: 7.226 ng/ul
RT: 15.238 min Scan# 2682
Delta R.T. -0.003 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31


Tgt Ion:166 Resp: 599673
Ion Ratio Lower Upper
166 100
165 98.3 78.0 117.0
167 14.5 11.4 17.0

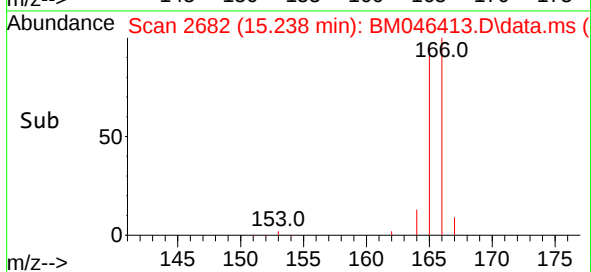

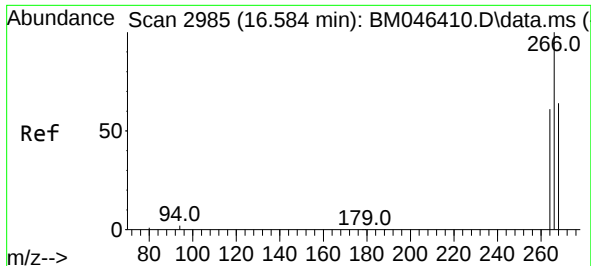

#14
Pentachlorophenol
Concen: 0.023 ng/ul
RT: 16.592 min Scan# 2985
Delta R.T. 0.006 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Instrument :
BNA_M
ClientSampleId :
A4CF4



Tgt Ion:266 Resp: 214
Ion Ratio Lower Upper
266 100
264 63.1 51.0 76.6
268 74.3 50.8 76.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

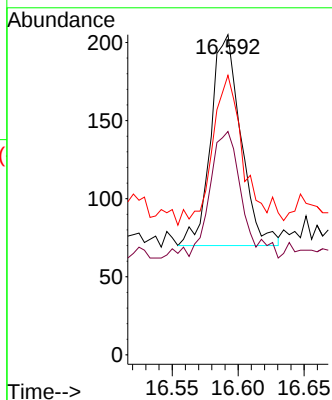

#15
Phenanthrene
Concen: 91.083 ng/ul
RT: 16.985 min Scan# 3080
Delta R.T. 0.010 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31


Tgt Ion:178 Resp: 8777140
Ion Ratio Lower Upper
178 100
179 16.3 12.7 19.1
176 20.0 16.0 24.0

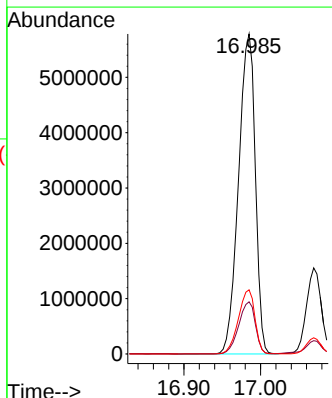

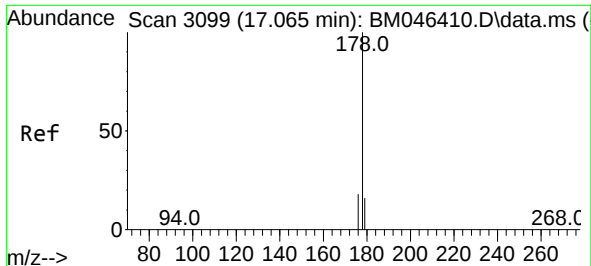

#16
 Anthracene
 Concen: 22.135 ng/ul
 RT: 17.069 min Scan# 3100
 Delta R.T. 0.001 min
 Lab File: BM046413.D
 Acq: 06 Jul 2024 11:31




Instrument :
 BNA_M
 ClientSampleId :
 A4CF4



Tgt Ion:178 Resp: 2068920
 Ion Ratio Lower Upper
 178 100
 179 15.5 12.6 18.8
 176 18.8 14.9 22.3




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 07/08/2024
 Supervised By :mohammad ahmed 07/08/2024

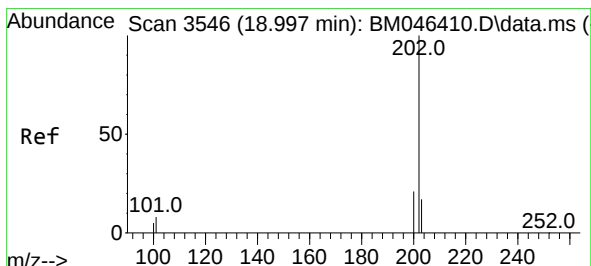

#19
 Fluoranthene
 Concen: 174.582 ng/ul
 RT: 19.016 min Scan# 3550
 Delta R.T. 0.011 min
 Lab File: BM046413.D
 Acq: 06 Jul 2024 11:31


Tgt Ion:202 Resp:10842801
 Ion Ratio Lower Upper
 202 100
 101 8.7 6.3 9.5
 100 6.6 5.0 7.6

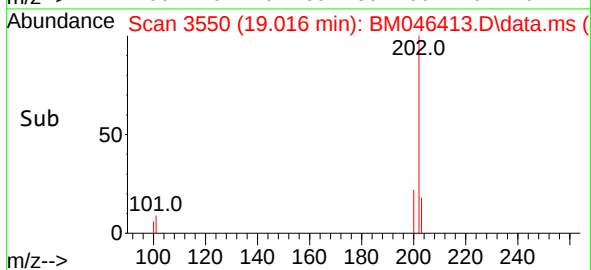



#20
Pyrene
Concen: 142.367 ng/u1
RT: 19.378 min Scan# 30
Delta R.T. 0.015 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Instrument :
BNA_M
ClientSampleId :
A4CF4



Tgt Ion:202 Resp: 9097849
Ion Ratio Lower Upper
202 100
101 9.1 8.2 12.4
100 7.3 6.9 10.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024



#21
Benzo(a)anthracene
Concen: 78.132 ng/u1
RT: 21.131 min Scan# 4085
Delta R.T. 0.005 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31

Tgt Ion:228 Resp: 4289355
Ion Ratio Lower Upper
228 100
229 20.8 15.8 23.6
226 32.5 22.0 33.0

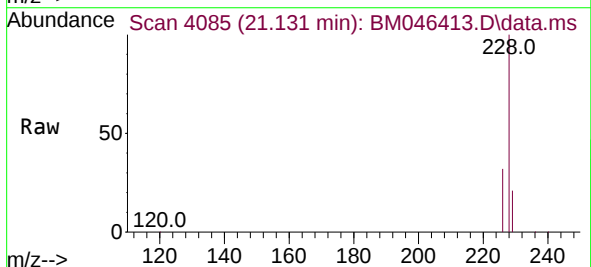



#22

Chrysene

Concen: 67.628 ng/ul

RT: 21.184 min Scan# 41

Delta R.T. 0.005 min

Lab File: BM046413.D


Acq: 06 Jul 2024 11:31

Instrument :

BNA_M

ClientSampleId :

A4CF4

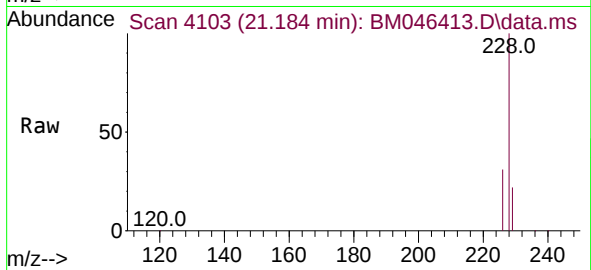

Tgt Ion:228 Resp: 3691430

Ion Ratio Lower Upper

228 100

226 31.4 24.1 36.1




229 22.1 15.8 23.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/08/2024

Supervised By :mohammad ahmed 07/08/2024

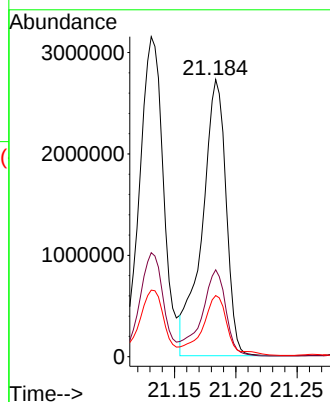

#24

Benzo(b)fluoranthene

Concen: 46.014 ng/ul m

RT: 22.677 min Scan# 4614

Delta R.T. 0.014 min

Lab File: BM046413.D

Acq: 06 Jul 2024 11:31




Tgt Ion:252 Resp: 4136487


Ion Ratio Lower Upper

252 100

253 22.8 0.0 47.0


125 7.5 0.0 18.4

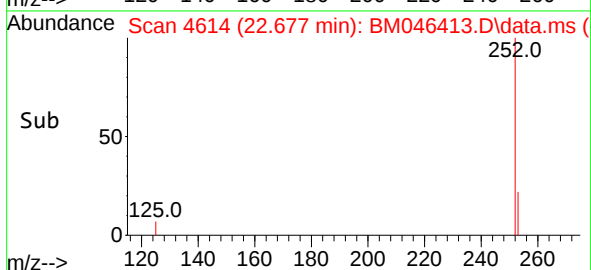



#25
Benzo(k)fluoranthene
Concen: 15.944 ng/ul m
RT: 22.709 min Scan# 4625
Delta R.T. 0.002 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Instrument :
BNA_M
ClientSampleId :
A4CF4



Tgt Ion:252 Resp: 1446838
Ion Ratio Lower Upper
252 100
253 23.5 18.4 27.6
125 7.1 7.5 11.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024



#26
Benzo(a)pyrene
Concen: 26.252 ng/ul m
RT: 23.218 min Scan# 4799
Delta R.T. 0.008 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31


Tgt Ion:252 Resp: 1865325
Ion Ratio Lower Upper
252 100
253 22.8 18.9 28.3
125 7.5 8.1 12.1

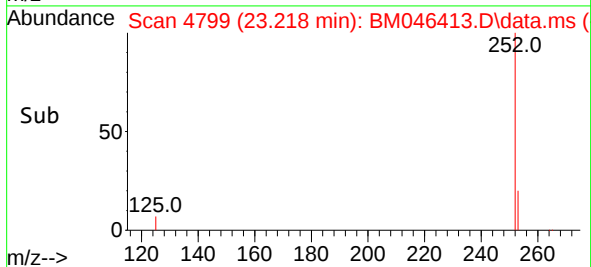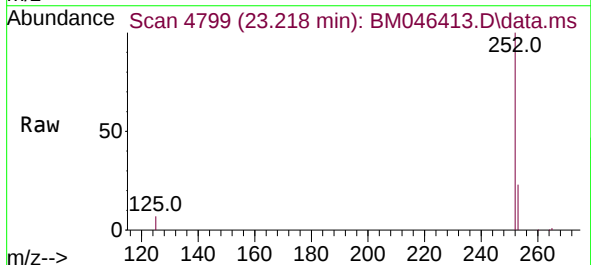



#27
Indeno(1,2,3-cd)pyrene
Concen: 15.398 ng/ul
RT: 25.463 min Scan# 5547
Delta R.T. 0.016 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Instrument :
BNA_M
ClientSampleId :
A4CF4




Tgt Ion:276 Resp: 147809
Ion Ratio Lower Upper
276 100
138 15.4 15.7 23.5
227 0.2 0.1 0.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/08/2024
Supervised By :mohammad ahmed 07/08/2024

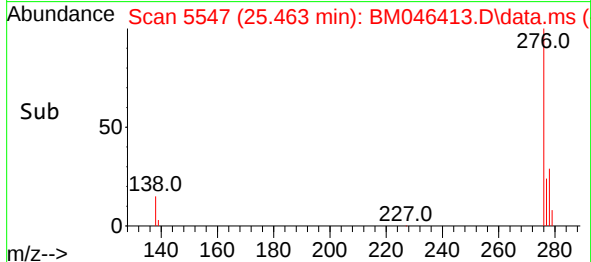


#28
Dibenzo(a,h)anthracene
Concen: 6.545 ng/ul
RT: 25.473 min Scan# 5550
Delta R.T. -0.000 min
Lab File: BM046413.D
Acq: 06 Jul 2024 11:31




Tgt Ion:278 Resp: 486026
Ion Ratio Lower Upper
278 100
139 13.2 12.6 18.8
279 26.9 20.7 31.1

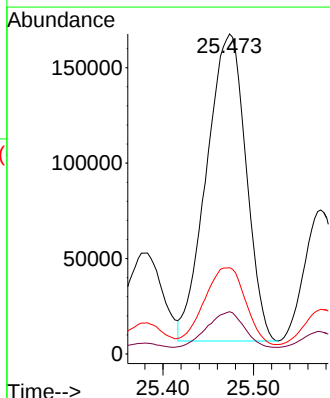



#29
 Benzo(g,h,i)perylene
 Concen: 2.827 ng/ul
 RT: 26.107 min Scan# 51
 Delta R.T. 0.016 min
 Lab File: BM046413.D
 Acq: 06 Jul 2024 11:31

Instrument :
 BNA_M
 ClientSampleId :
 A4CF4



Tgt Ion:276 Resp: 216404
 Ion Ratio Lower Upper
 276 100
 138 17.0 15.4 23.0
 277 26.7 19.7 29.5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/08/2024
 Supervised By :mohammad ahmed 07/08/2024

