


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A4TV3

Quant Time: Jul 07 10:56:10 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

Manual Integration

APPROVED
umangi
7/7/2016 6:04:23 PM

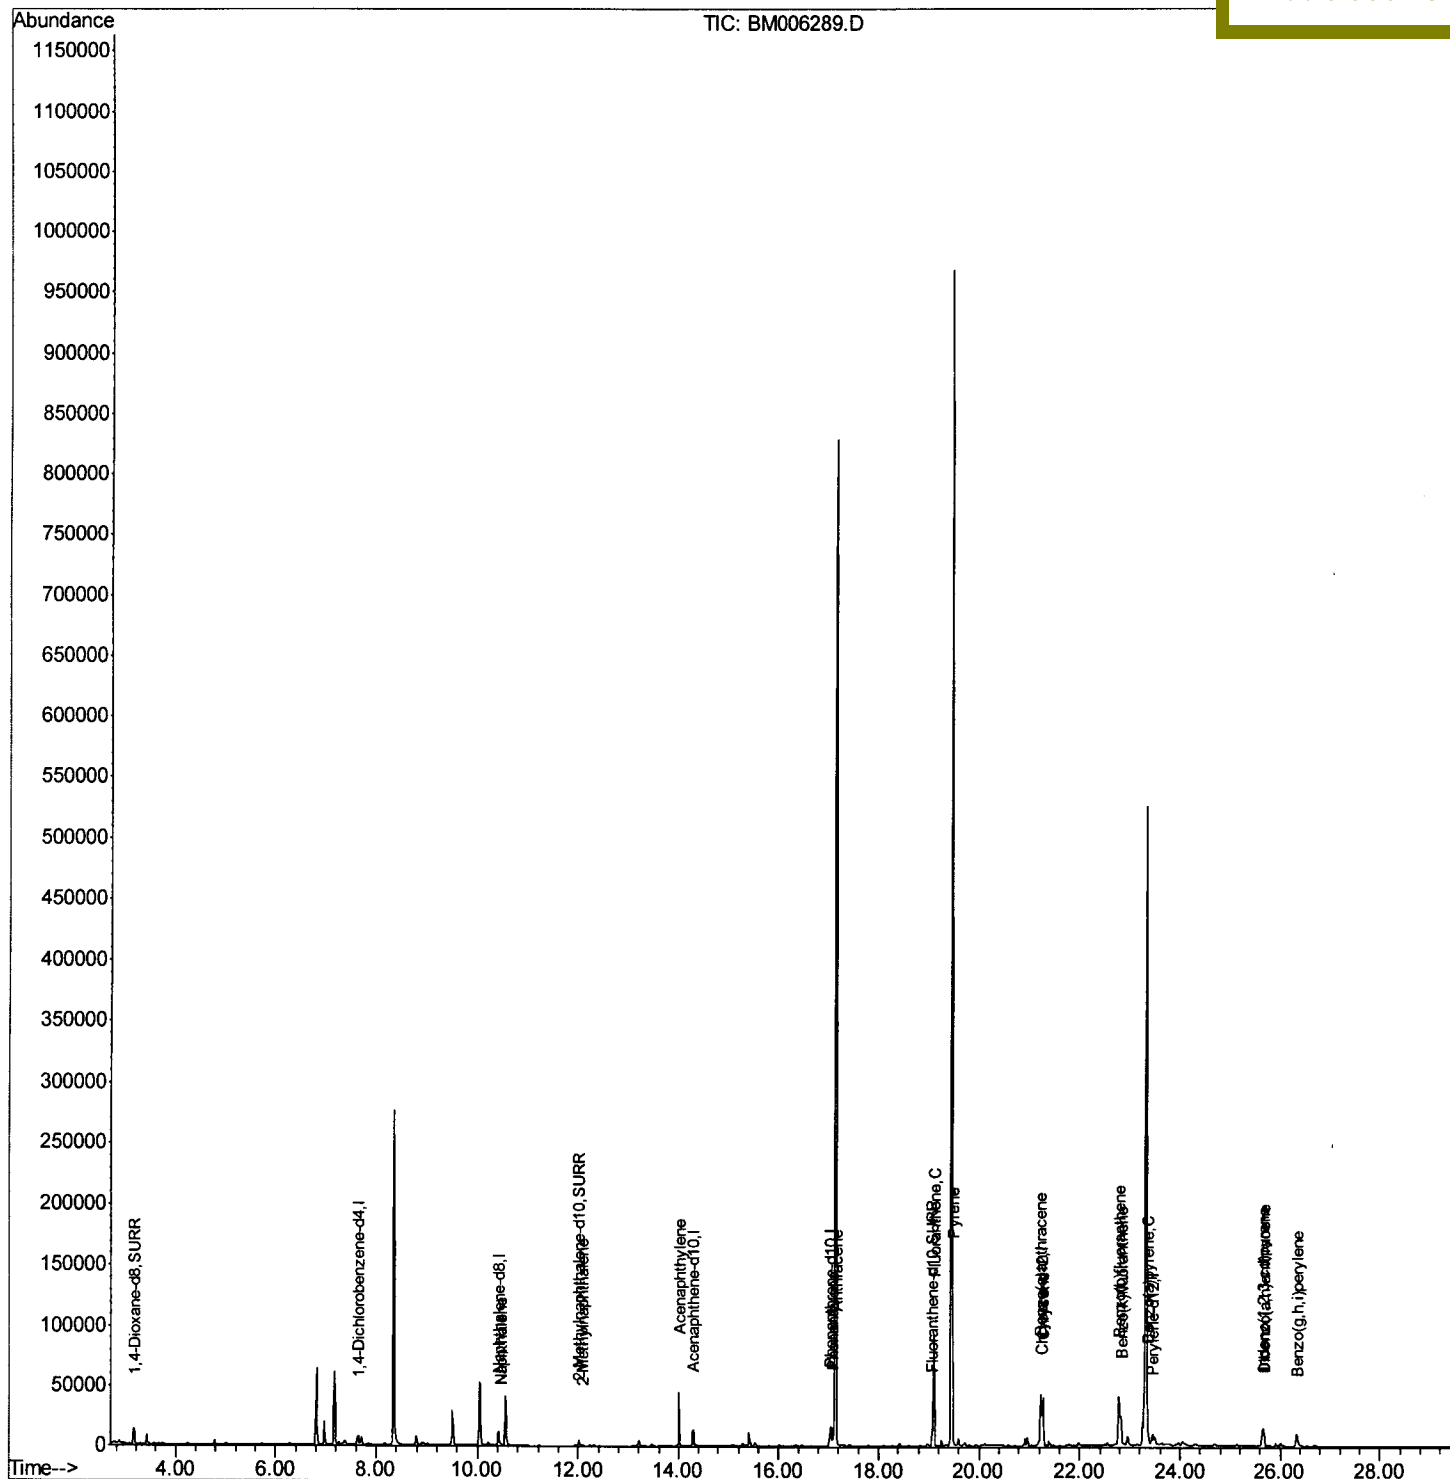

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

APPROVED
 umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:51:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

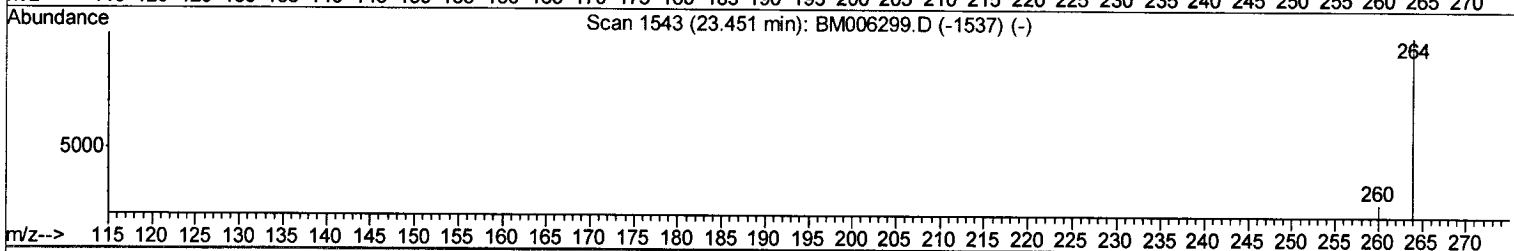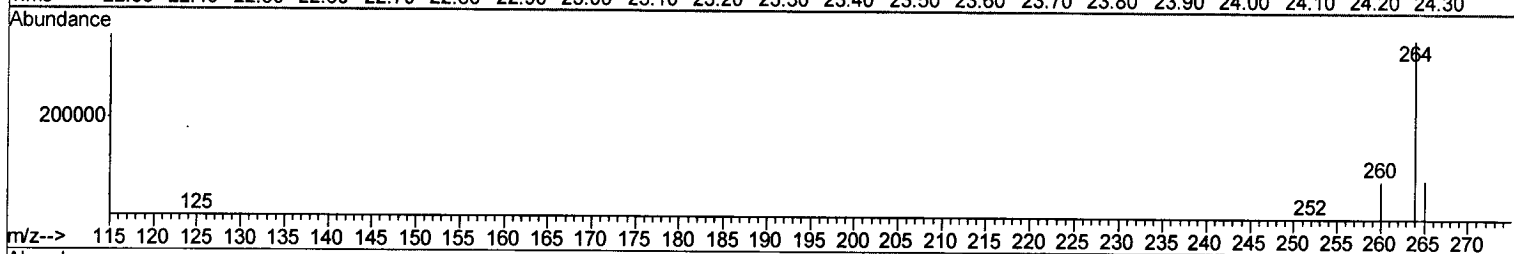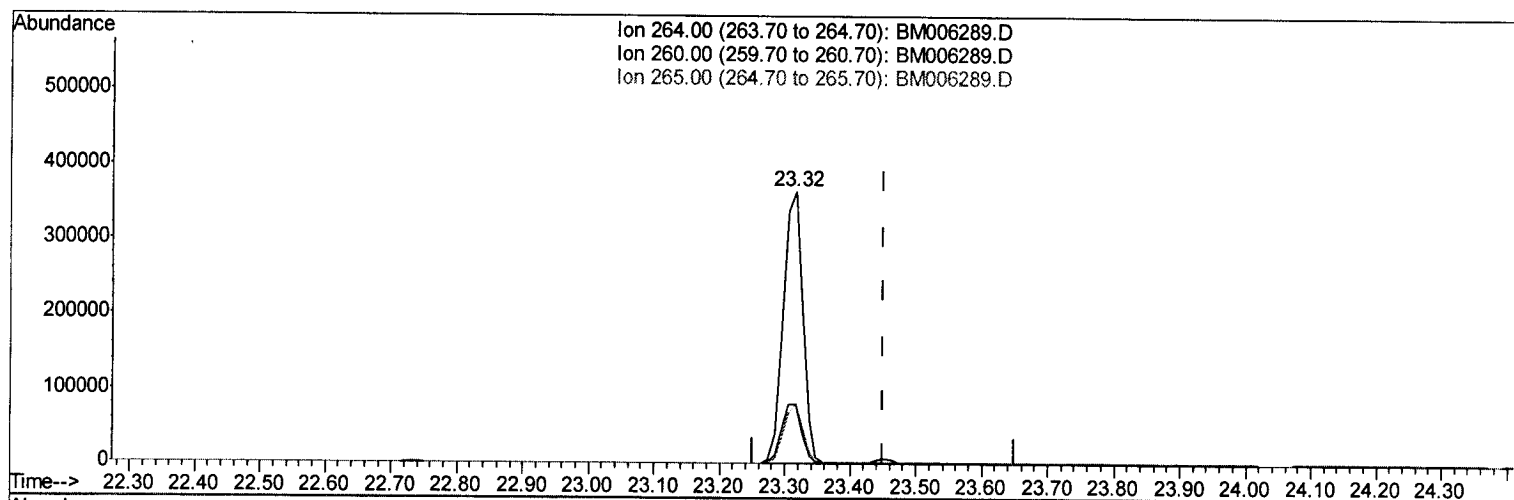

TIC: BM006289.D

(22) Perylene-d12 (I)
 23.316min (-0.135) 0.40ng/ul
 response 739621

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	21.64
265.00	38.20	22.08#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV3

Manual Integration

umangi
7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:51:46 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

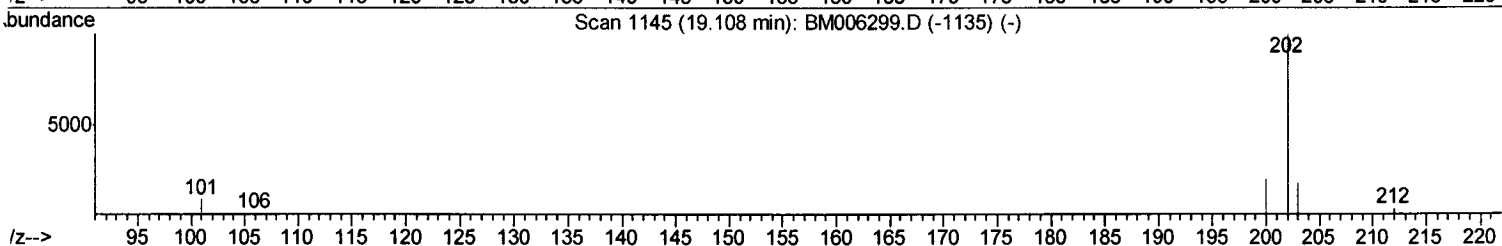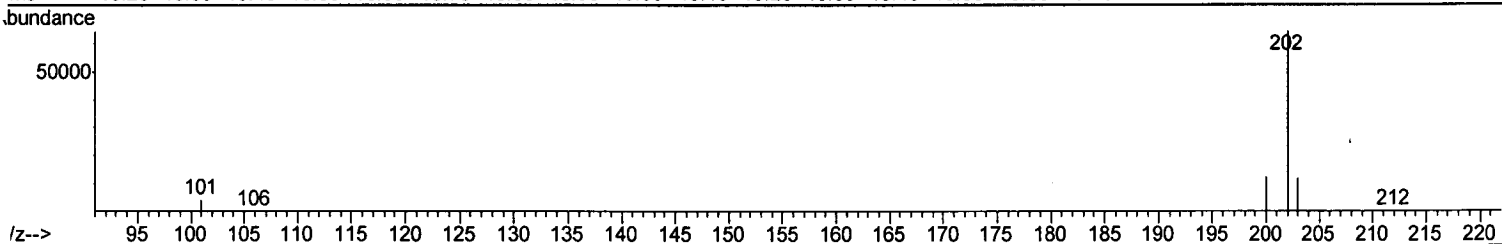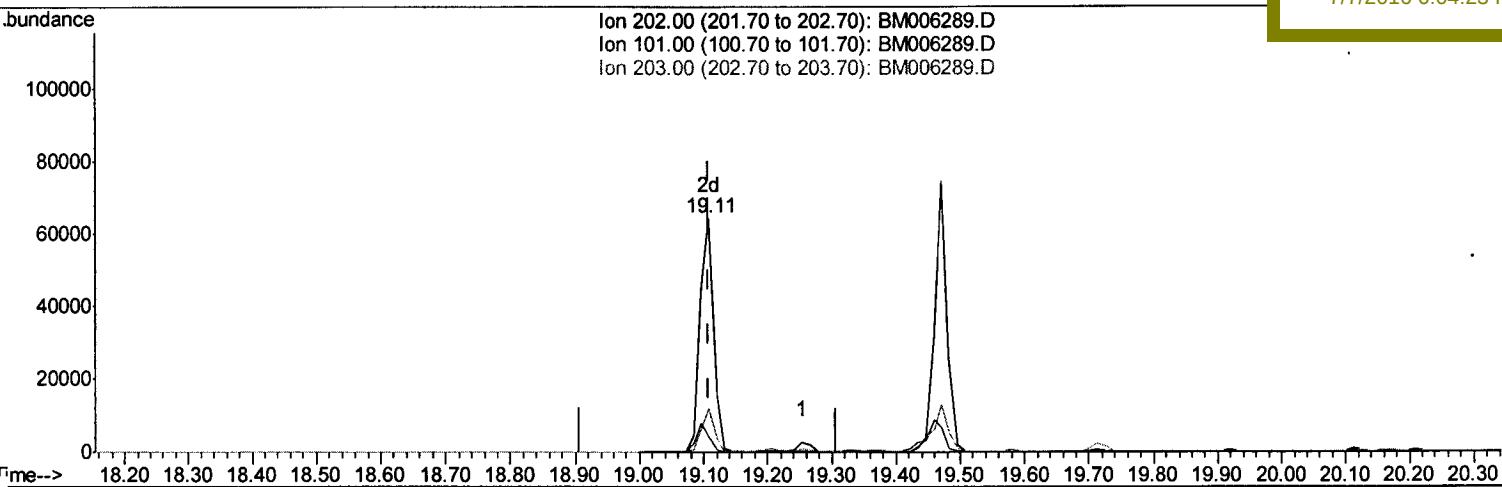

TIC: BM006289.D

(17) Fluoranthene (C)

19.108min (+0.000) 1.49ng/ul m U.M
response 95179 27/11/16

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	6.68
203.00	16.30	18.22
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

Quant Time: Jul 07 10:51:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

umangi
 7/7/2016 6:04:23 PM

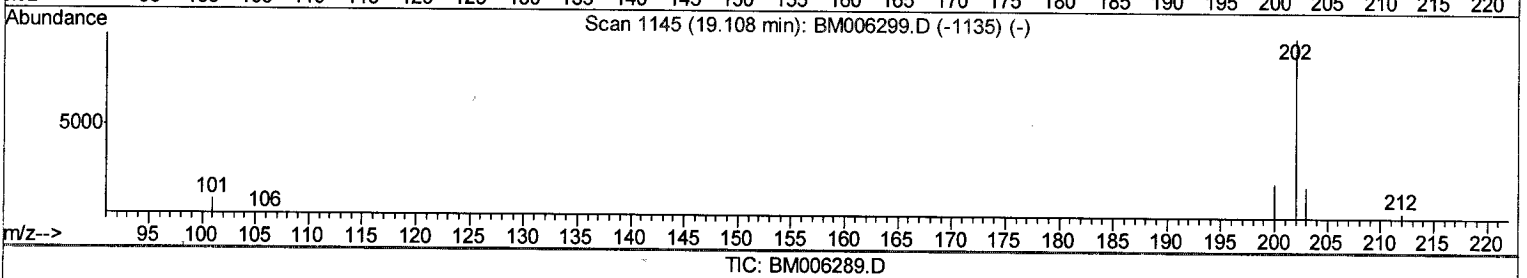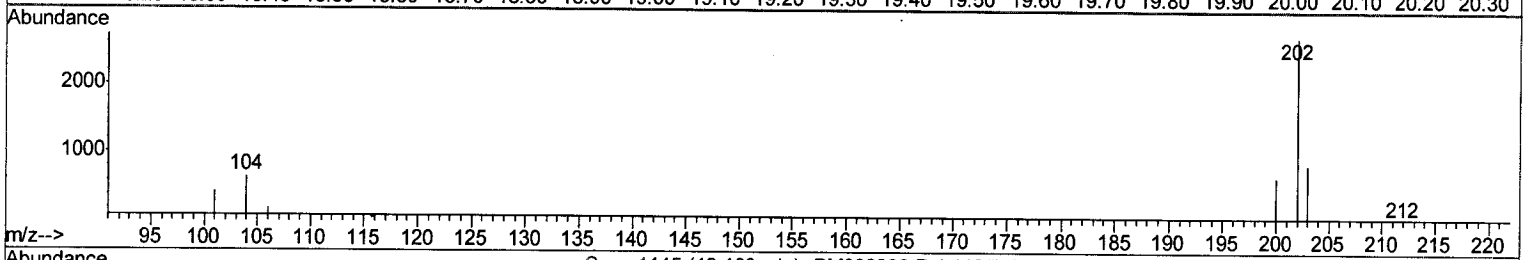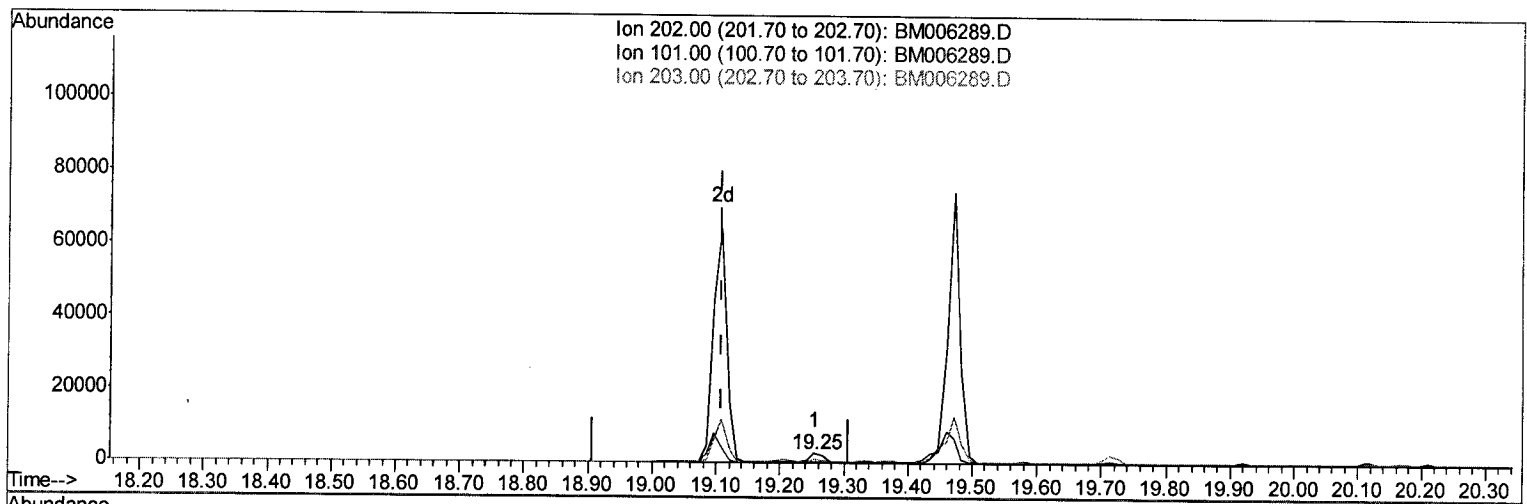

TIC: BM006289.D

(17) Fluoranthene (C)

19.254min (+0.145) 0.06ng/ul

response 3672

Ion	Exp%	Act%
202.00	100	100
101.00	9.60	15.87
203.00	16.30	31.92
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:51:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

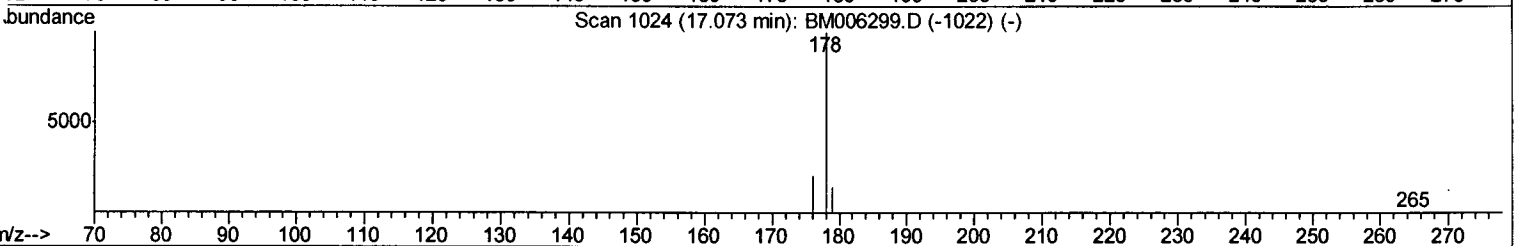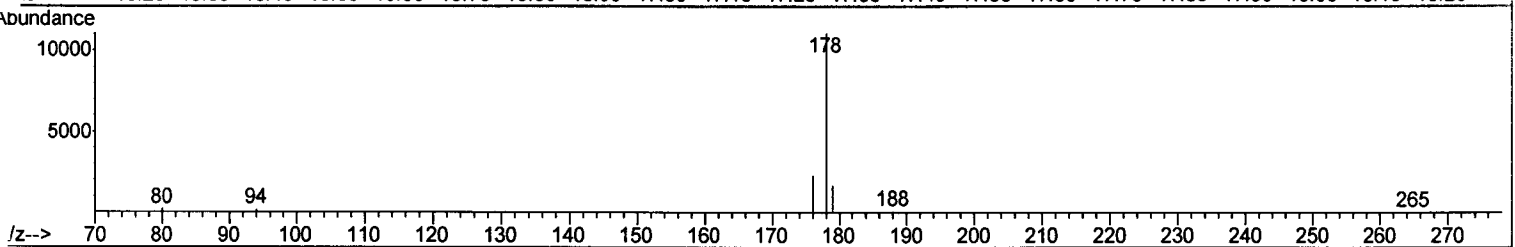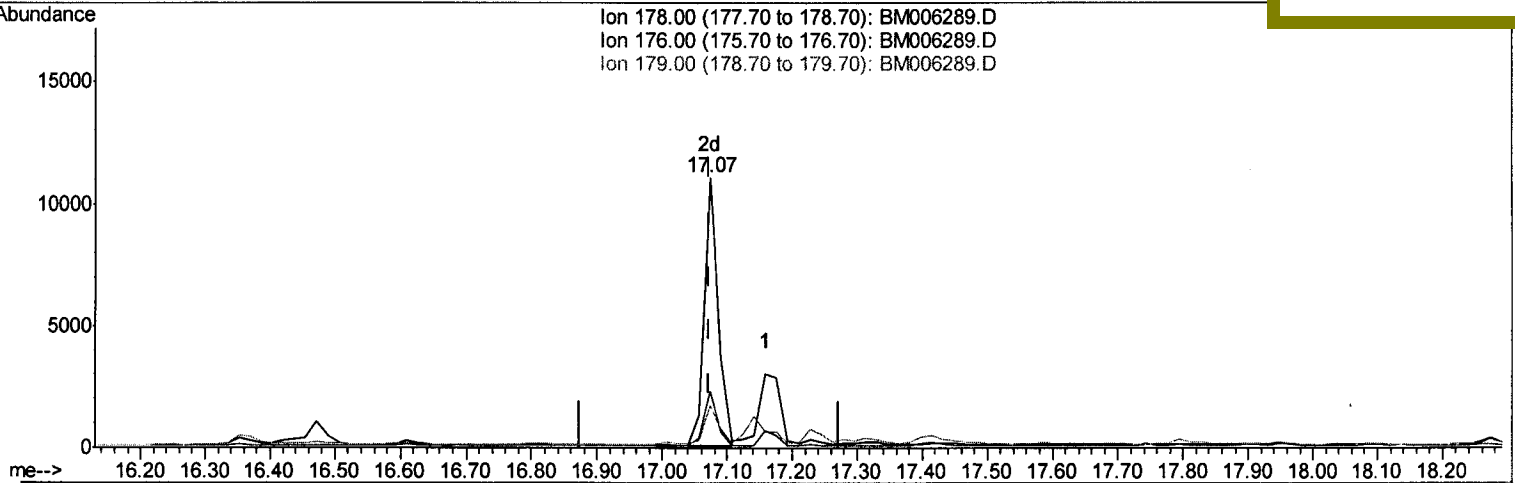

TIC: BM006289.D

(14) Phenanthrene

17.073min (+0.000) 0.29ng/ul m U.M

response 16526

07/11/16

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	20.70#
179.00	17.70	15.68
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

Quant Time: Jul 07 10:51:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

umangi
 7/7/2016 6:04:23 PM

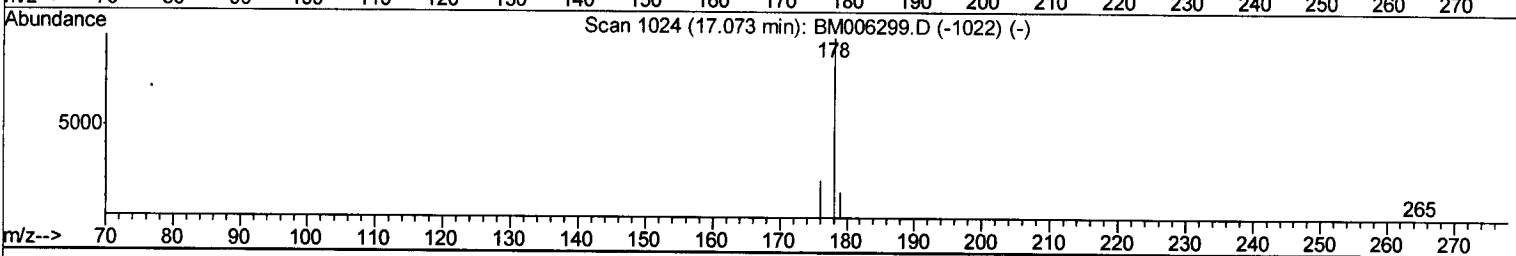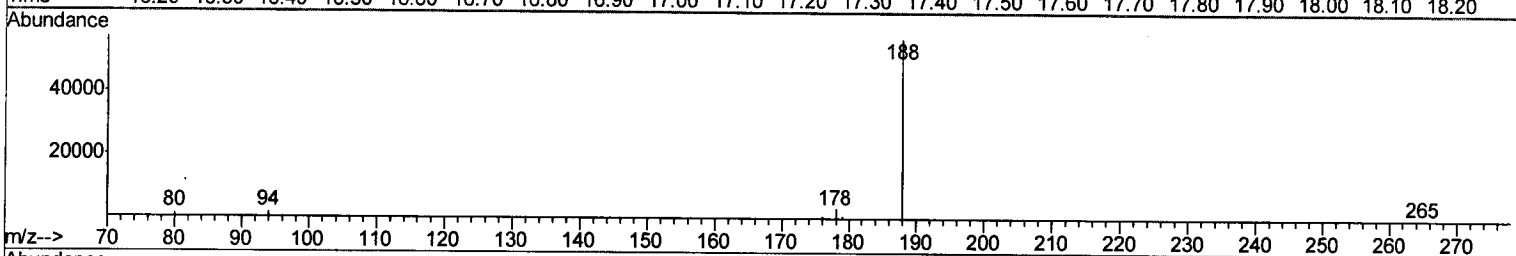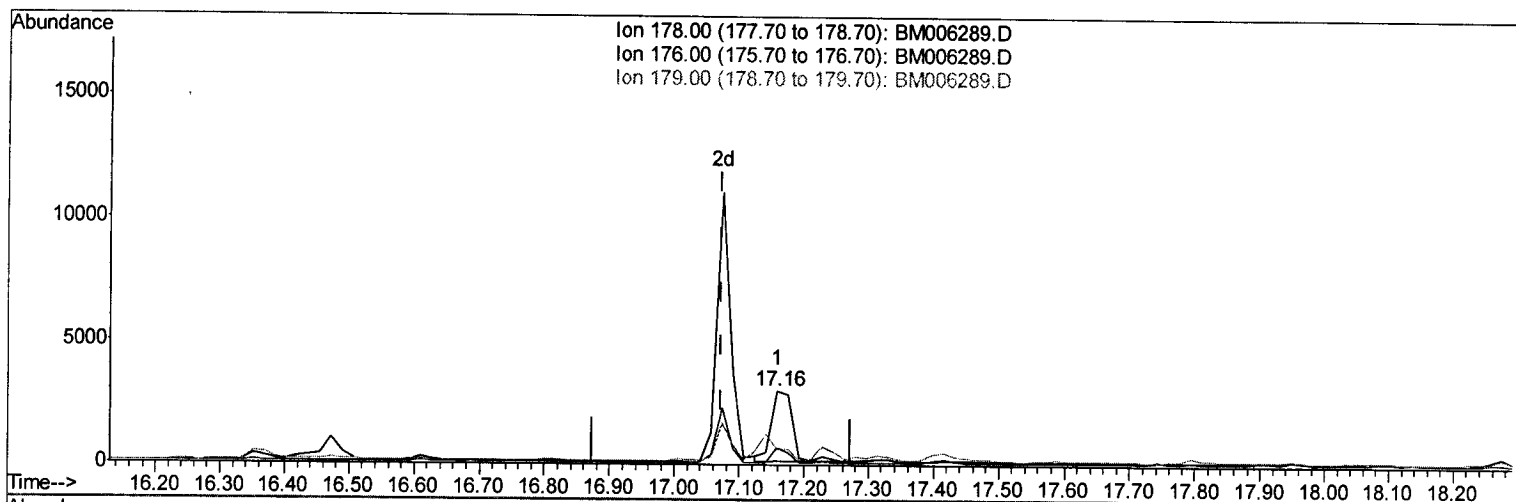

TIC: BM006289.D

(14) Phenanthrene

17.159min (+0.086) 0.12ng/ul

response 6678

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	23.97#
179.00	17.70	21.83#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV3

Quant Time: Jul 07 10:50:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

Manual Integration

umangi
7/7/2016 6:04:23 PM

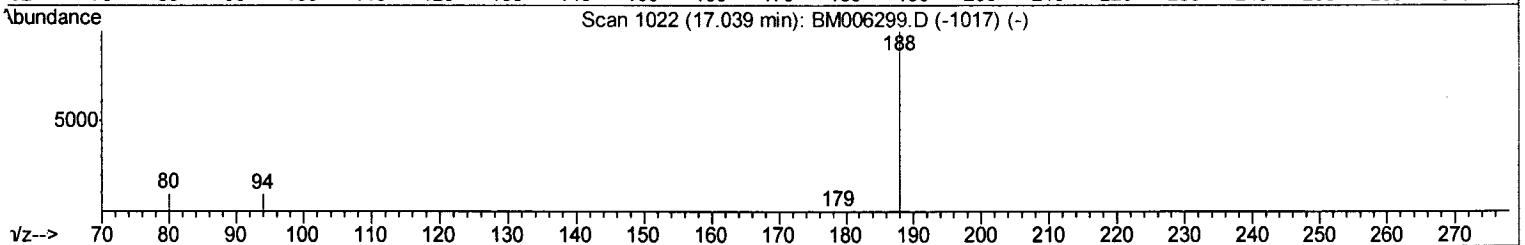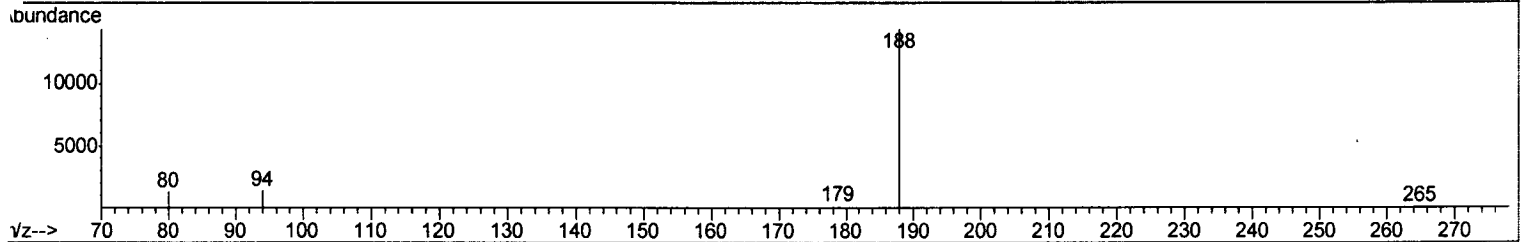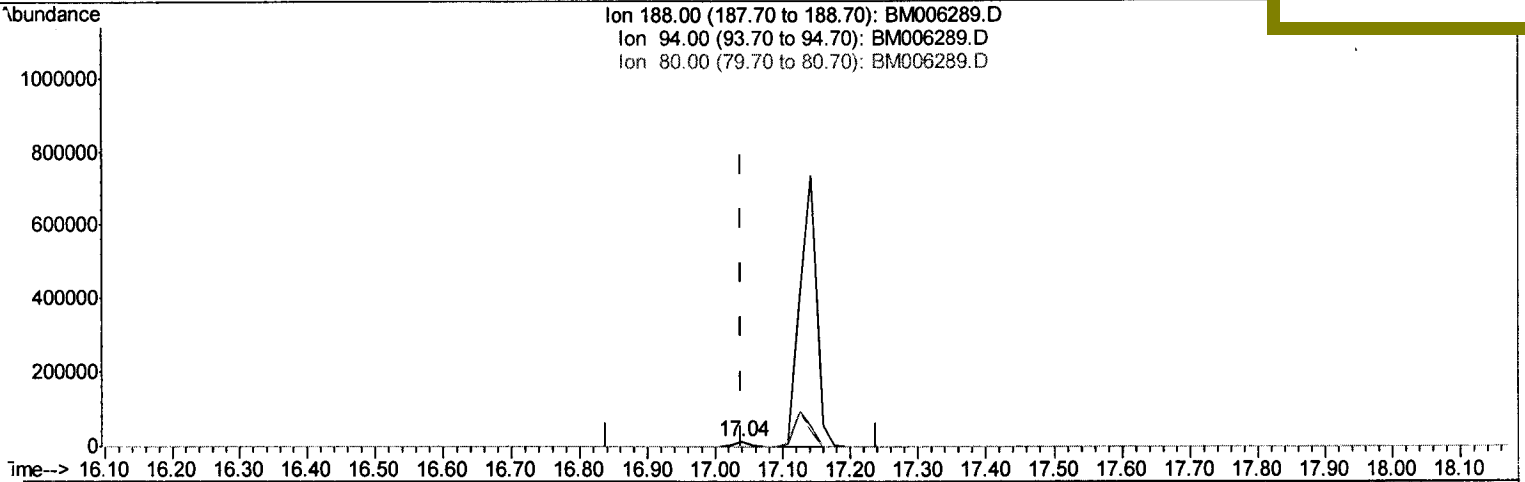

TIC: BM006289.D

(12) Phenanthrene-d10 (I)

17.039min (+0.000) 0.40ng/ul m U.M

response 20883

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	9.63
80.00	11.90	9.09#
0.00	0.00	0.00

07/11/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV3

Manual Integration

APPROVED
umangi
7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:50:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

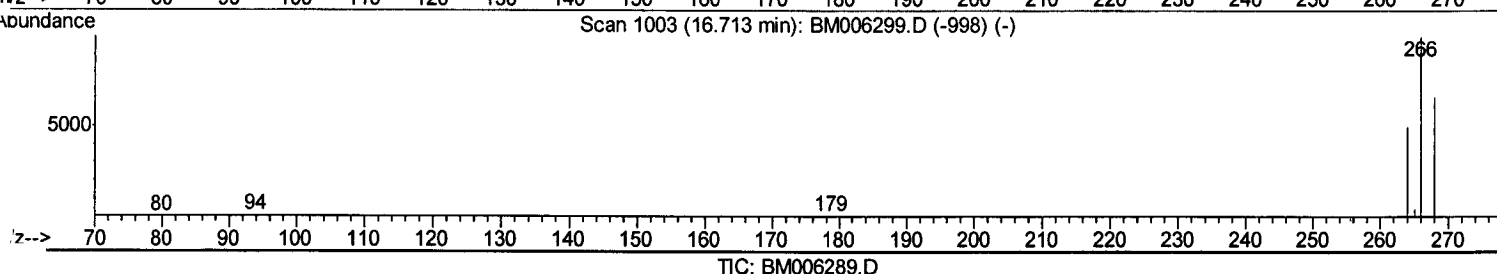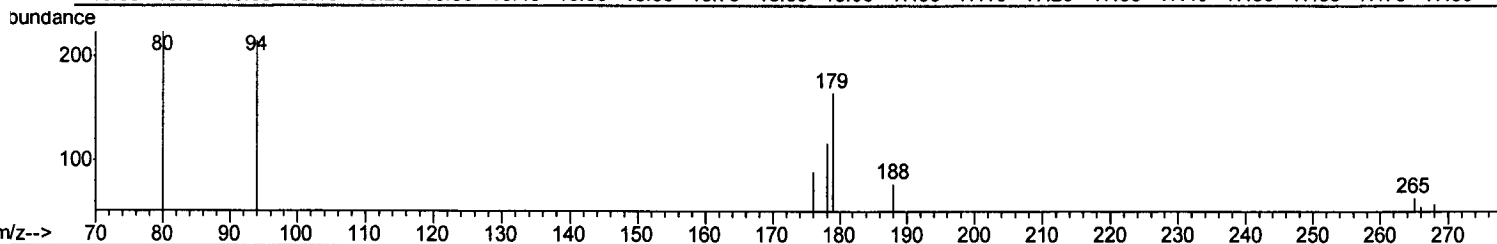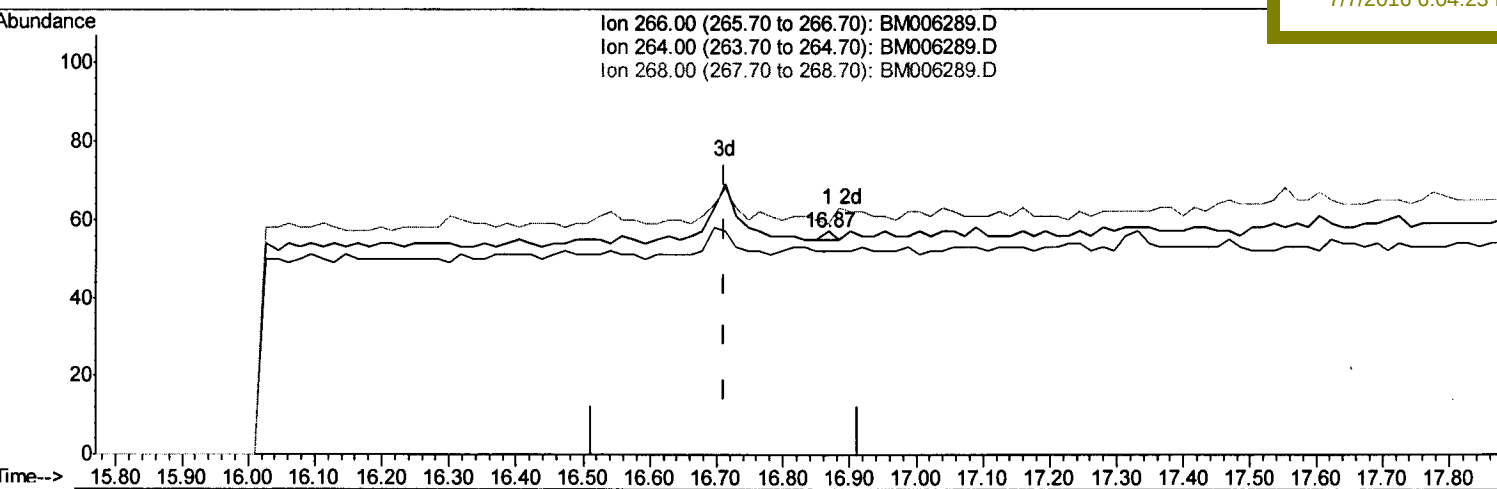

(13) Pentachlorophenol

16.867min (+0.154) 0.00ng/ul

response 2

Ion	Exp%	Act%
266.00	100	100
264.00	64.80	0.00#
268.00	58.50	600.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

APPROVED
 umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:50:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

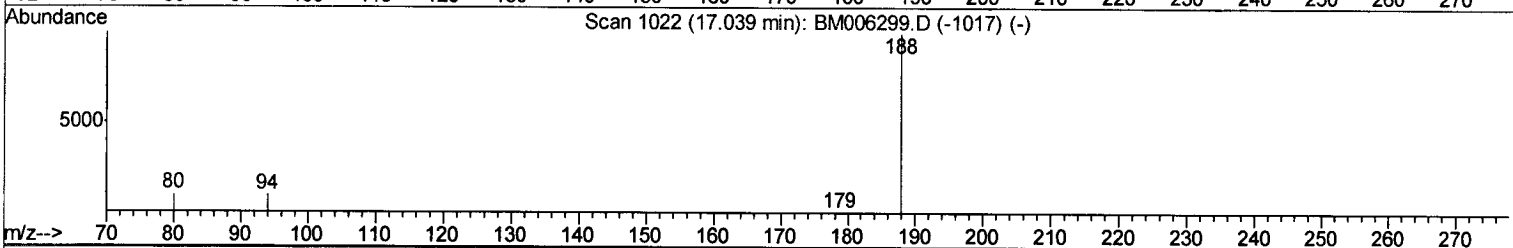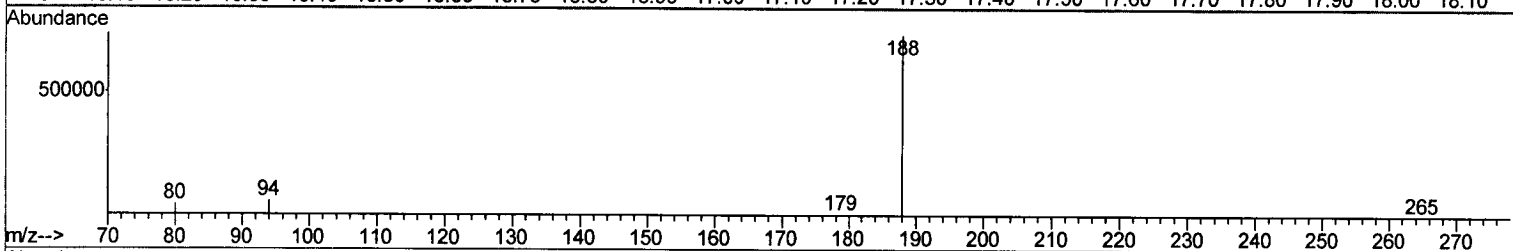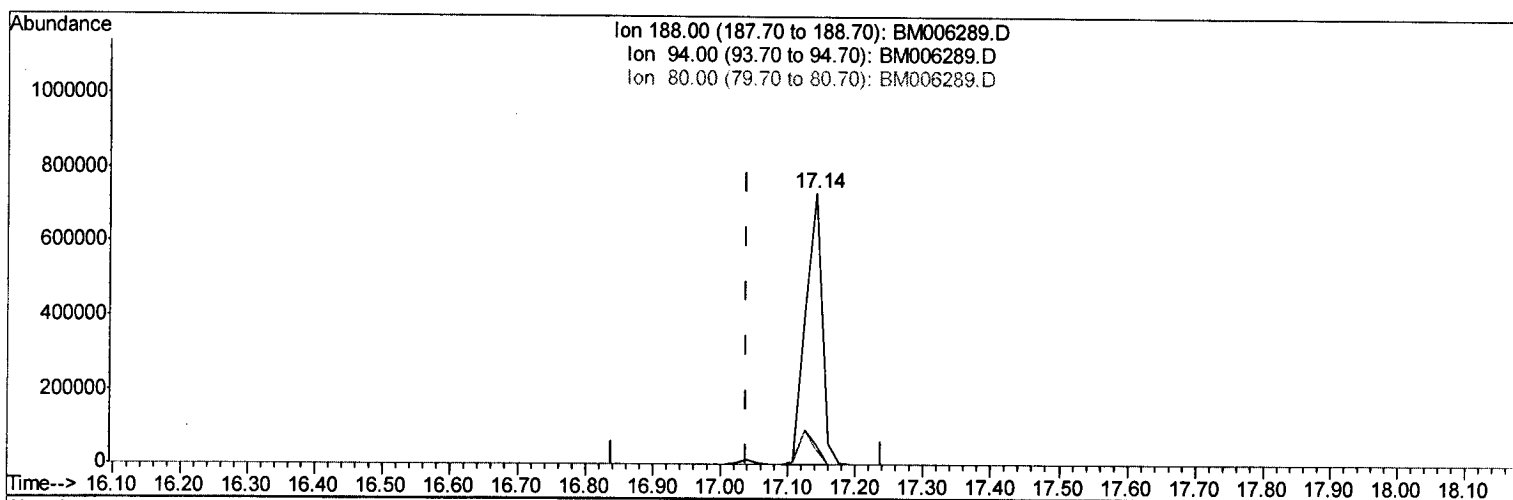

TIC: BM006289.D

(12) Phenanthrene-d10 (I)

17.142min (+0.103) 0.40ng/ul

response 1244791

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.37#
80.00	11.90	5.38#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integrati

umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:51:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

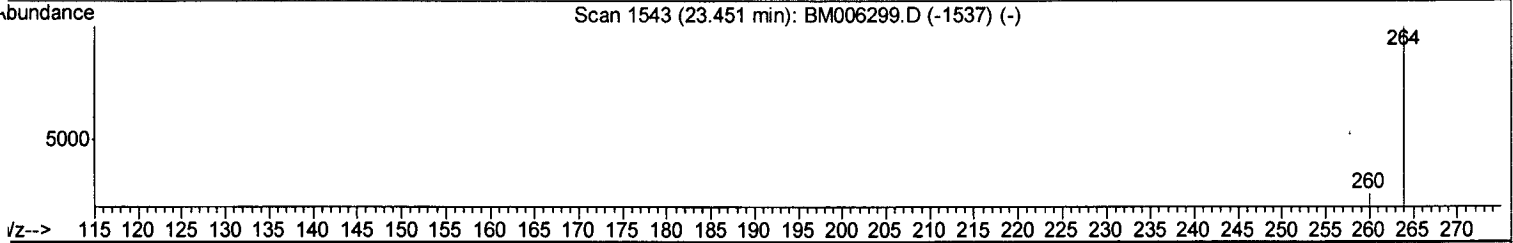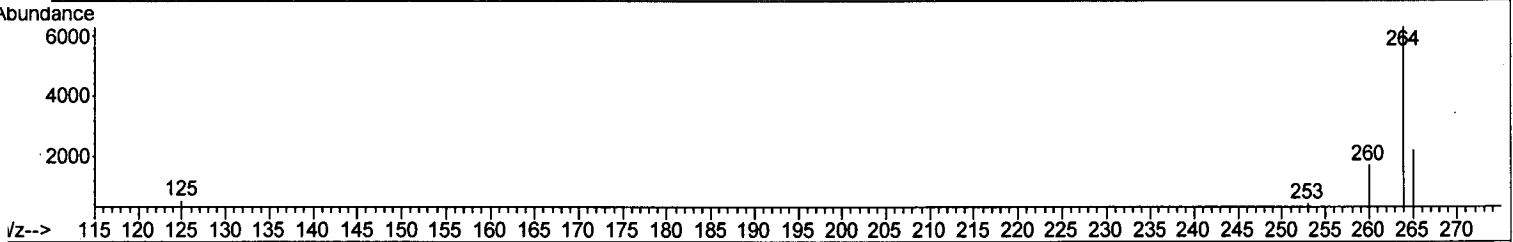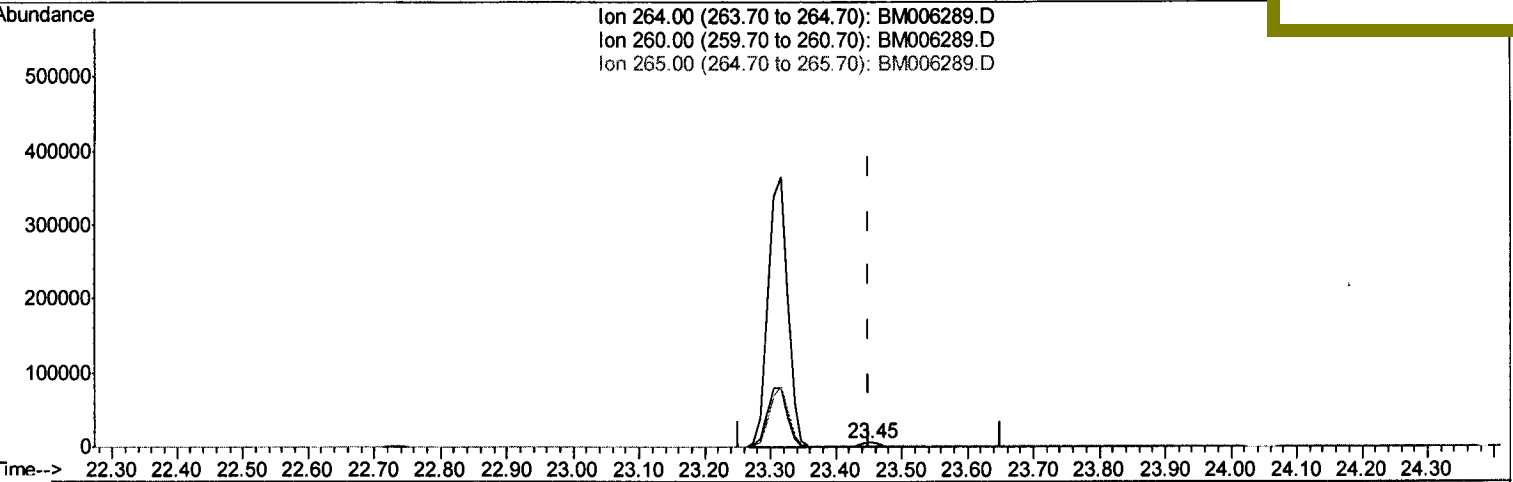

TIC: BM006289.D

(22) Perylene-d12 (I)

23.451min (+0.000) 0.40ng/ul m

response 10954

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.90
265.00	38.20	34.77
0.00	0.00	0.00

U.M
 07/11/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integrati

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

umangi
 7/7/2016 6:04:23 PM

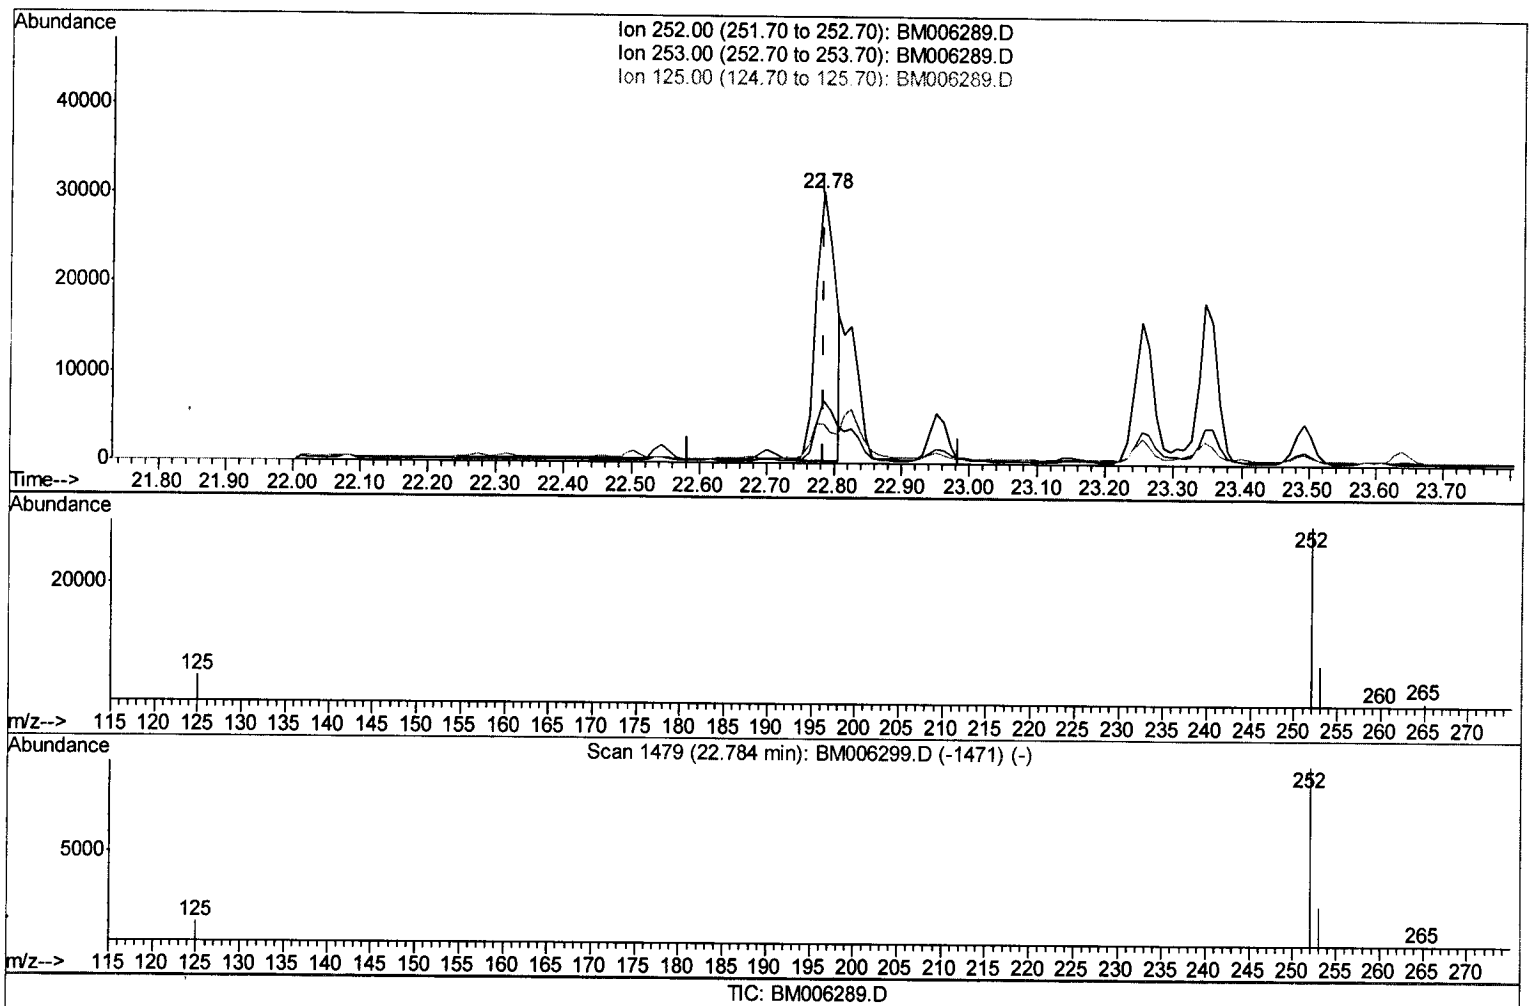

TIC: BM006289.D

(23) Benzo(b)fluoranthene
 22.784min (+0.000) 1.53ng/ui
 response 60143

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	23.24
125.00	14.40	14.62
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

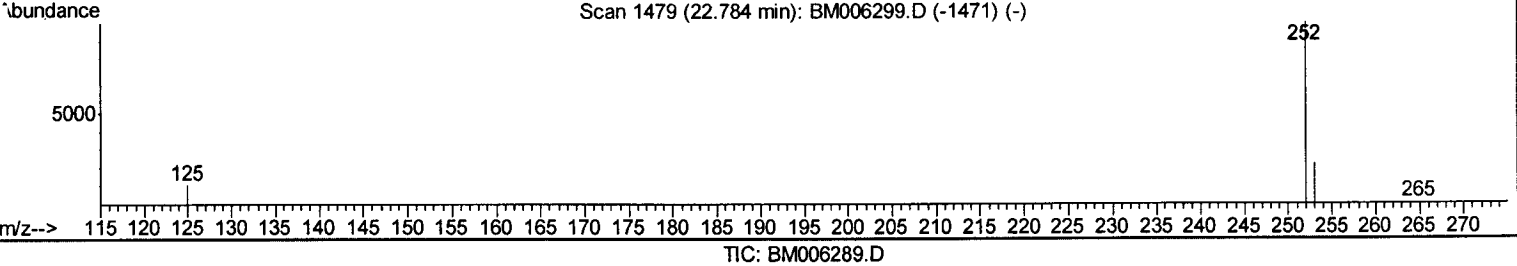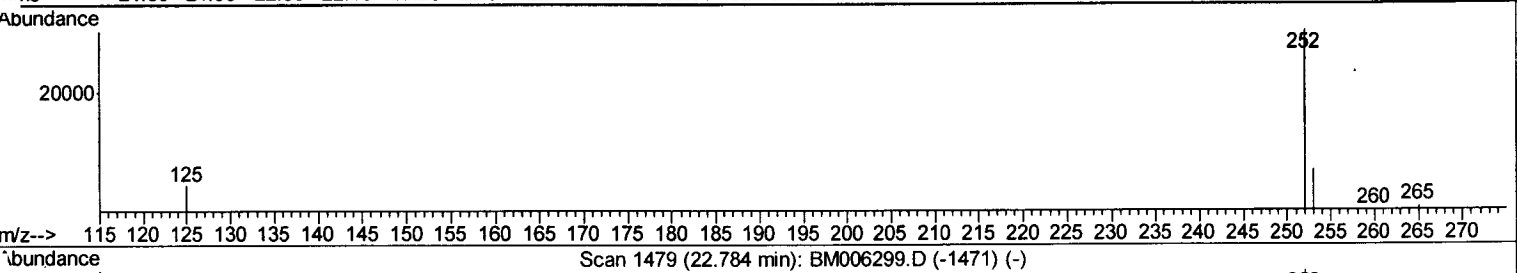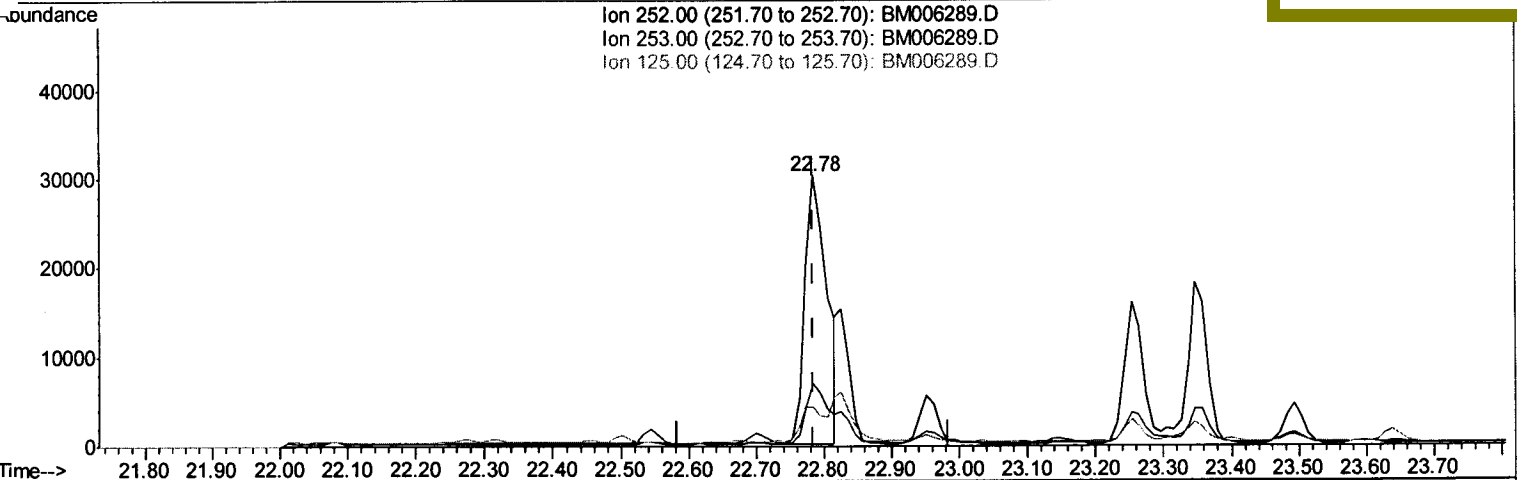

(23) Benzo(b)fluoranthene

22.784min (+0.000) 1.76ng/ul m *U.M*
07/11/16

response 69102

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	23.24
125.00	14.40	14.62
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

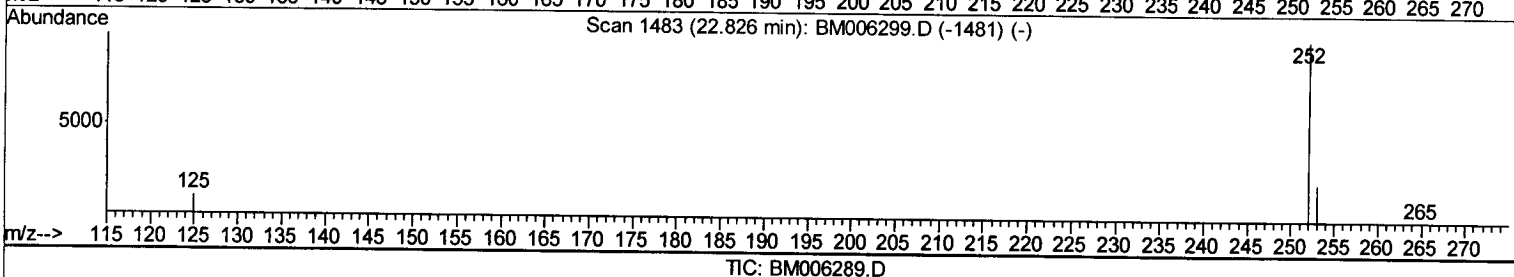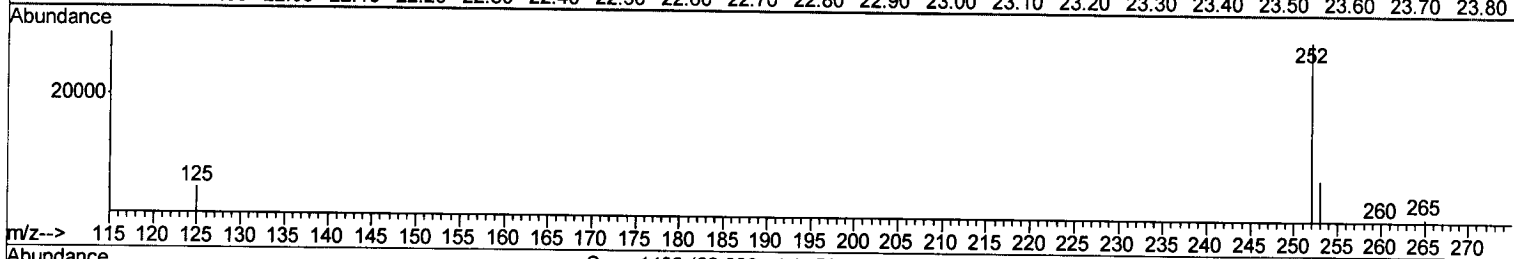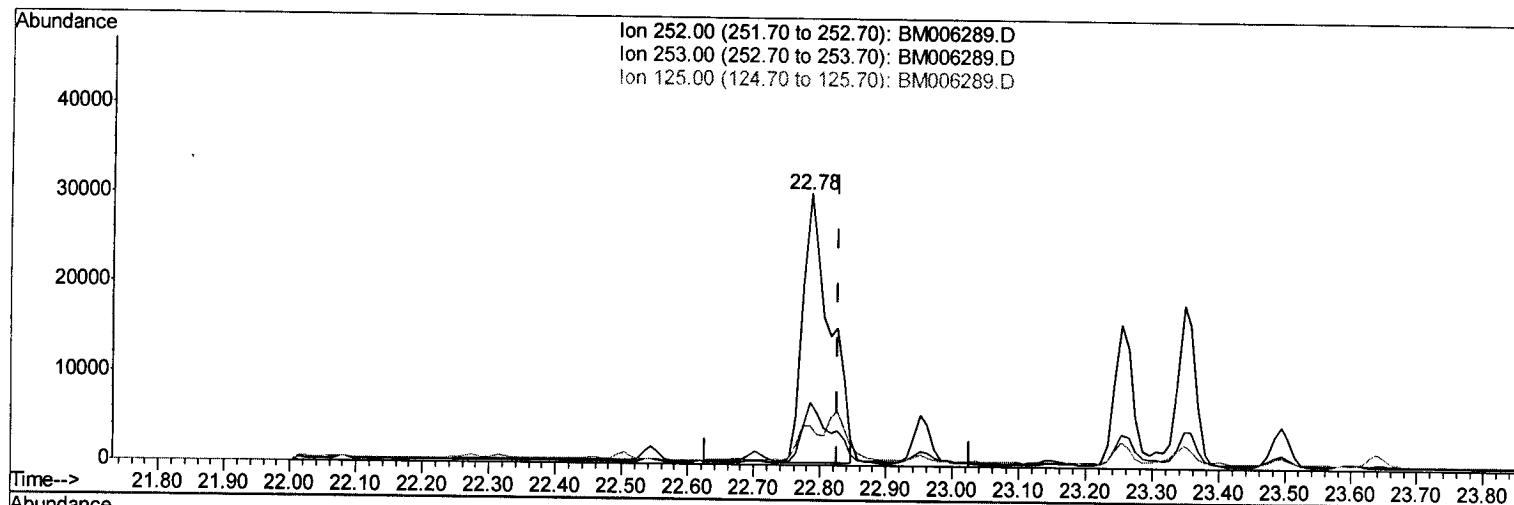

(24) Benzo(k)fluoranthene

22.784min (-0.042) 2.35ng/ul

response 85881

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	23.24
125.00	13.00	14.62
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

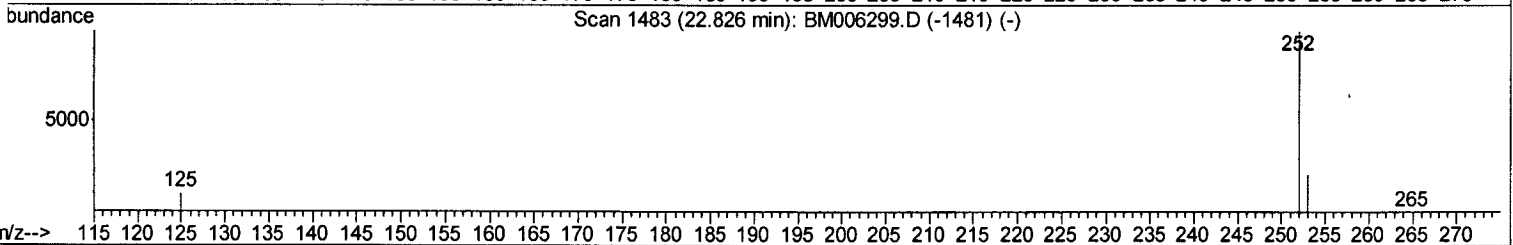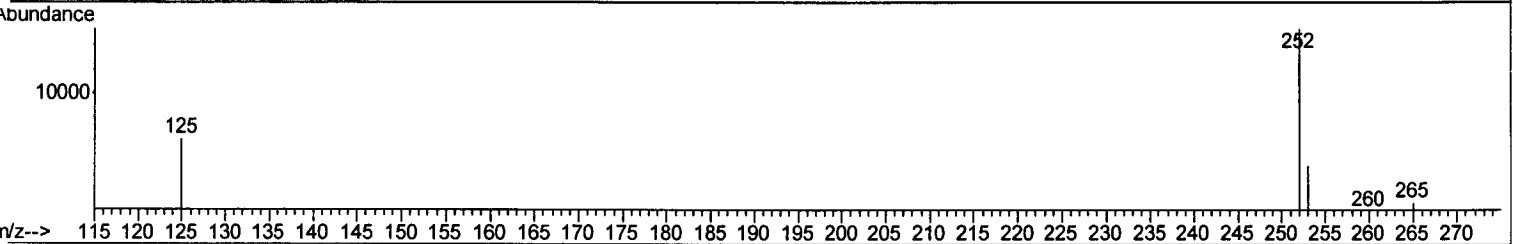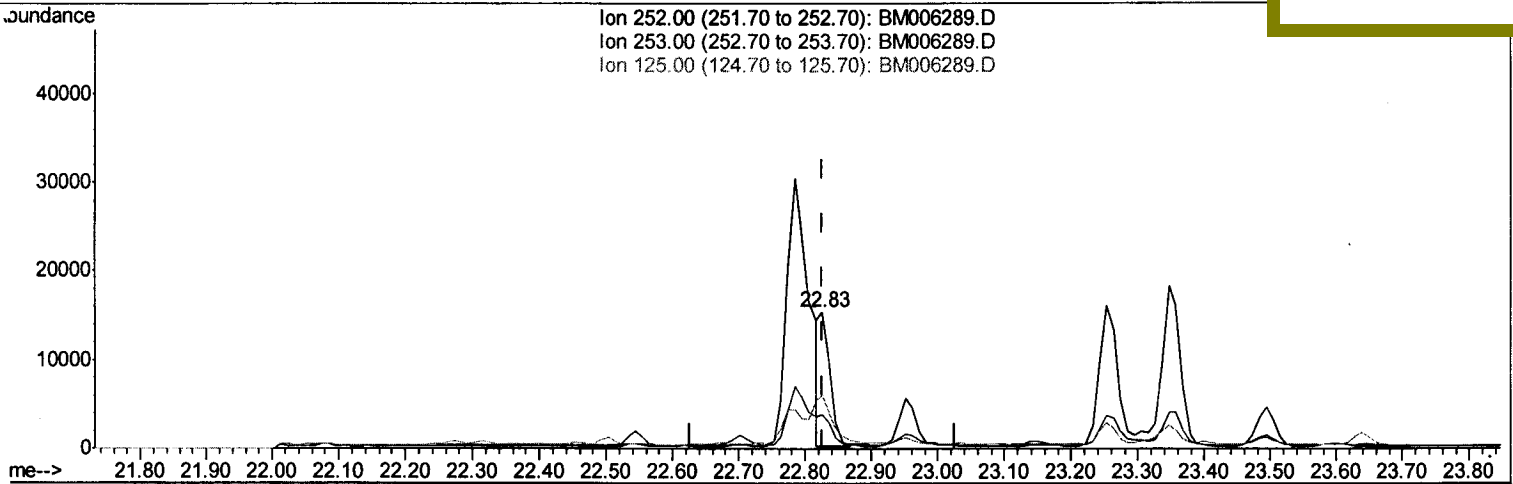

TIC: BM006289.D

(24) Benzo(k)fluoranthene

22.826min (+0.000) 0.48ng/ul m

response 17473

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	25.26
125.00	13.00	39.84#
0.00	0.00	0.00

U.M
 07/11/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc. :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/7/2016 6:04:23 PM

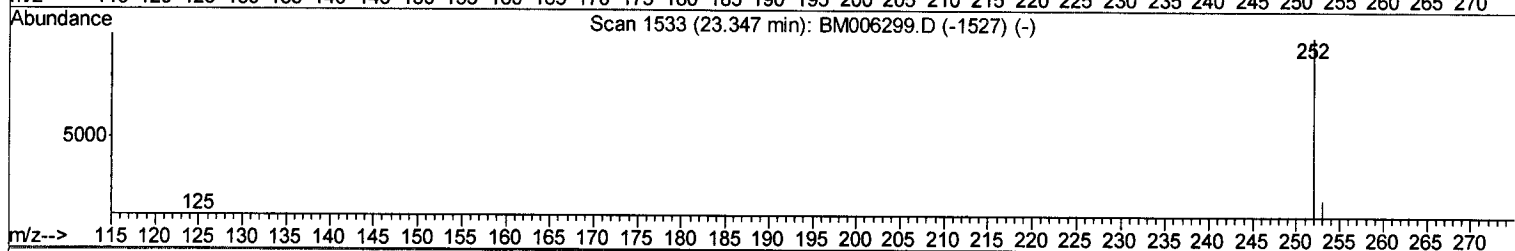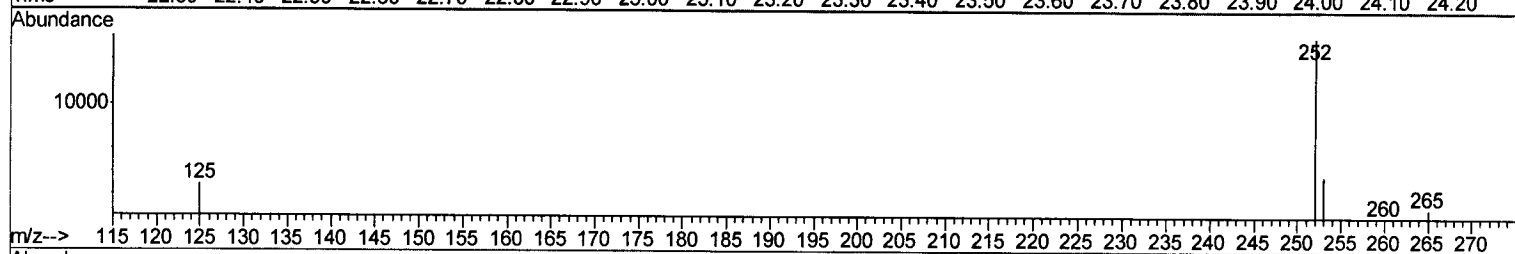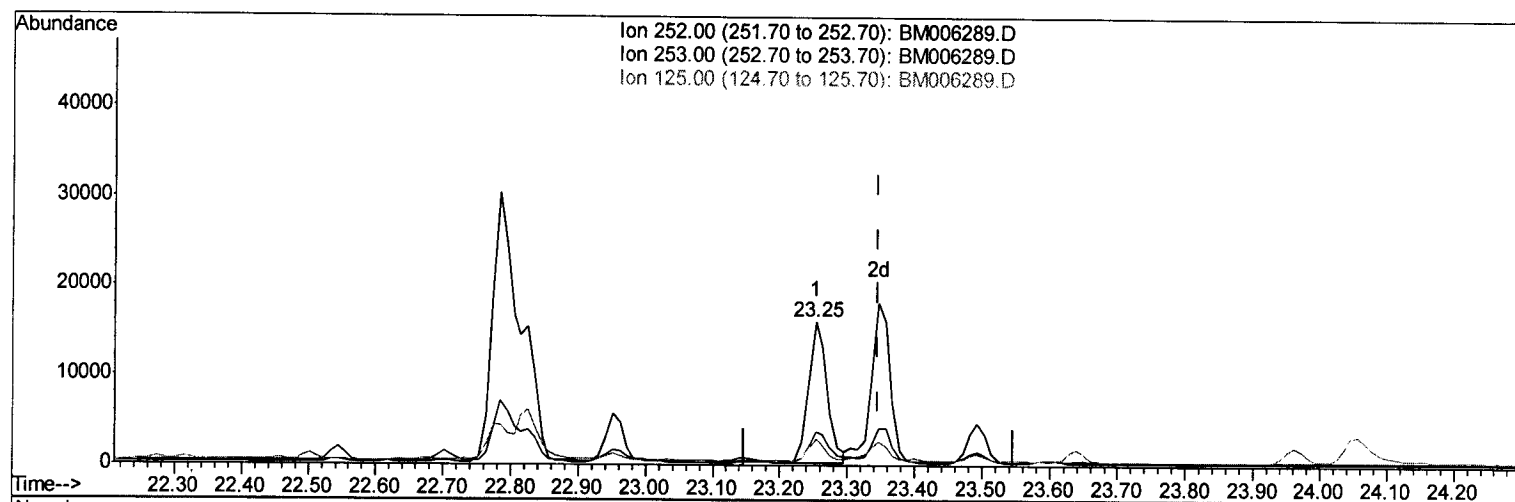

TIC: BM006289.D

(25) Benzo(a)pyrene (C)

23.253min (-0.094) 0.83ng/ul

response 30362

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	23.00
125.00	15.90	17.68
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA M
ClientSampleId :
A4TV3

Quant Time: Jul 07 10:53:28 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

Manual Integration

APPROVED
umangi
7/7/2016 6:04:23 PM

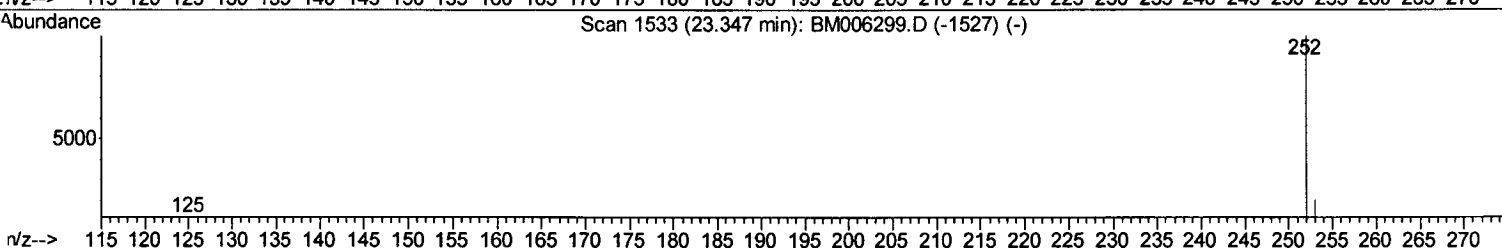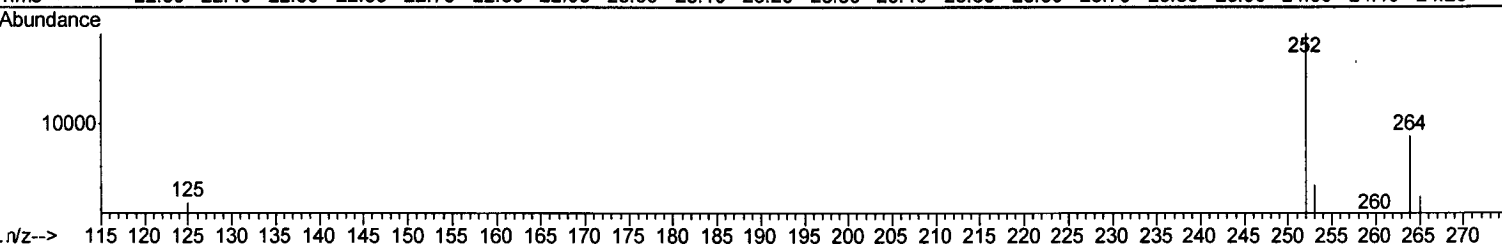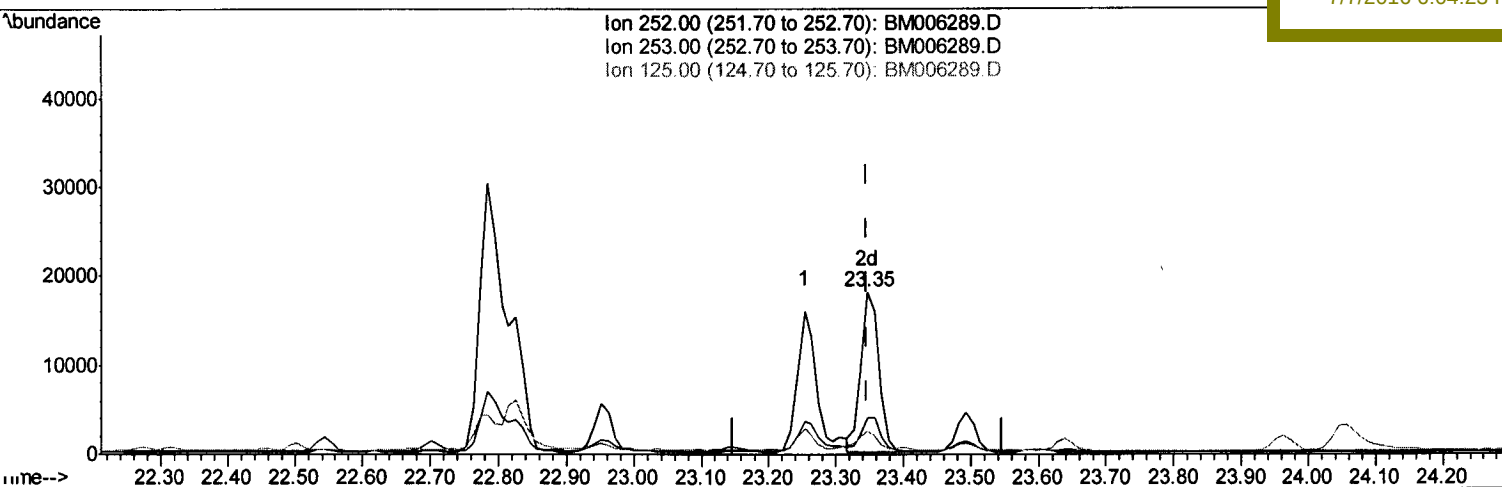

TIC: BM006289.D

(25) Benzo(a)pyrene (C)

23.347min (+0.000) 0.92ng/ul m U.M

response 33625

07/11/16

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	23.01
125.00	15.90	14.47
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/7/2016 6:04:23 PM

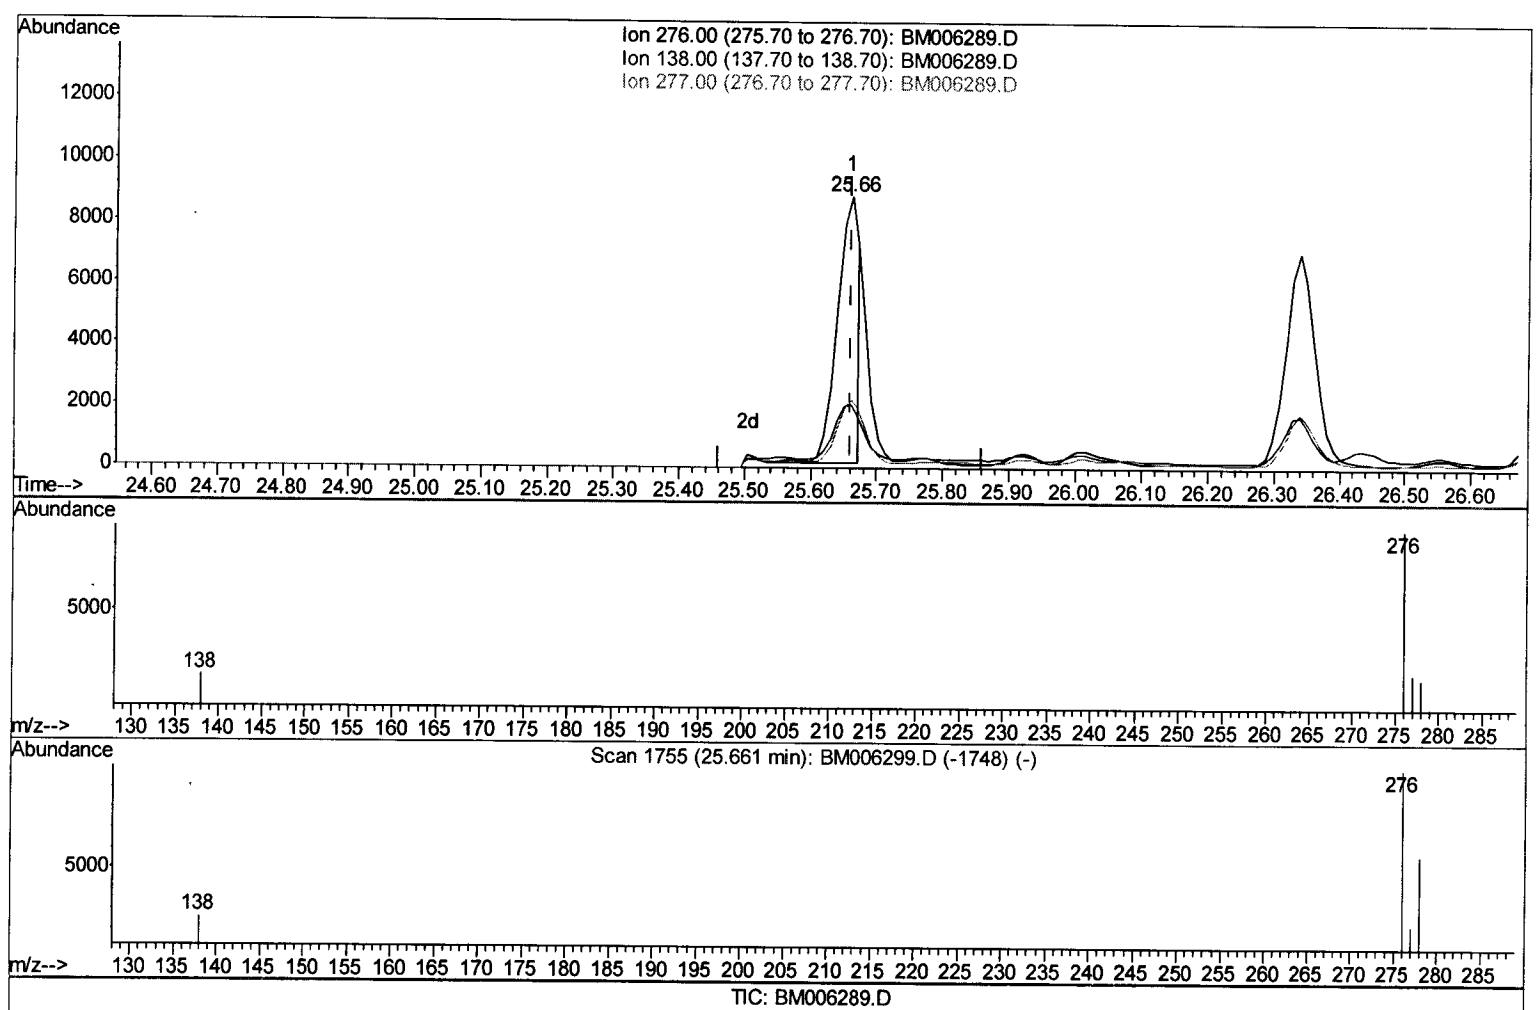

TIC: BM006289.D

(26) Indeno(1,2,3-cd)pyrene

25.661min (+0.000) 0.50ng/ul

response 20107

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	22.18
277.00	24.80	21.97
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

APPROVED
 umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

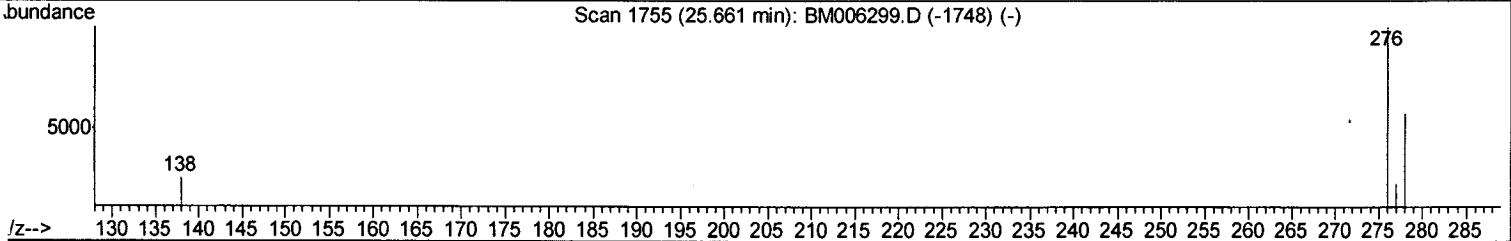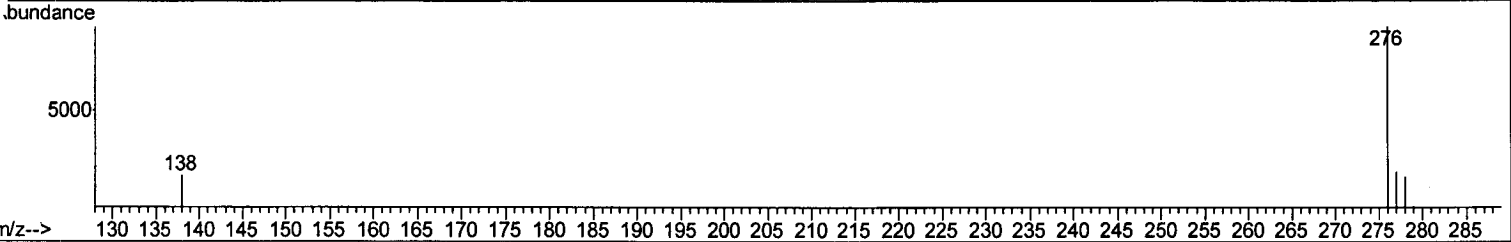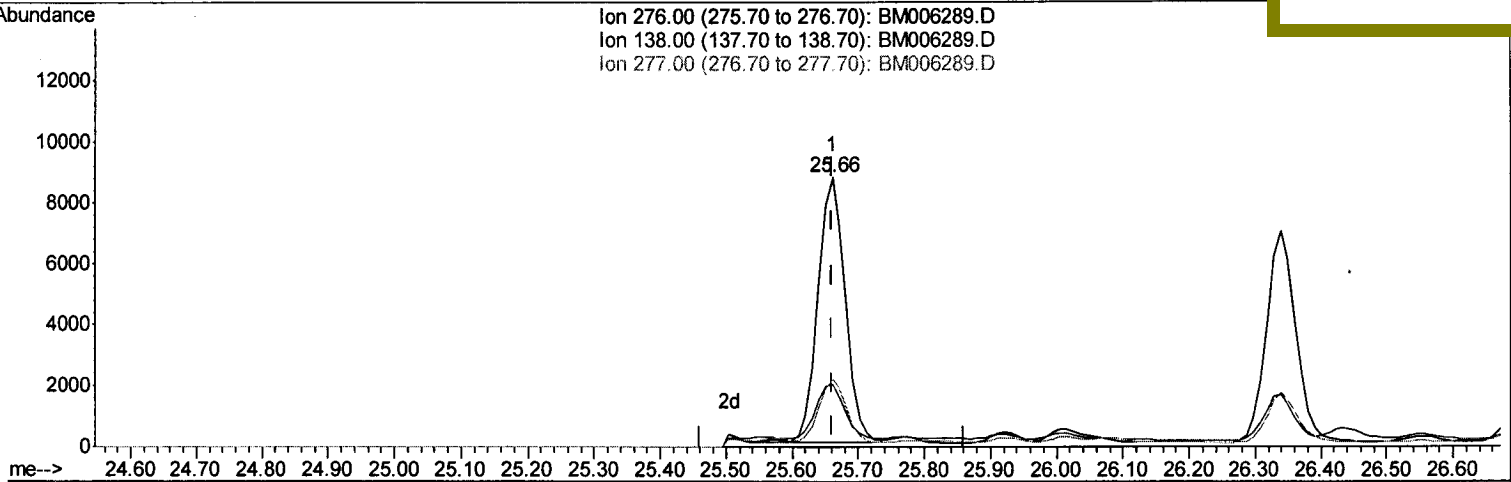

TIC: BM006289.D

(26) Indeno(1,2,3-cd)pyrene

25.661min (+0.000) 0.61ng/ul m

response 24902

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	17.91
277.00	24.80	17.74#
0.00	0.00	0.00

U.M
 07/11/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV3

Manual Integration

APPROVED
 umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

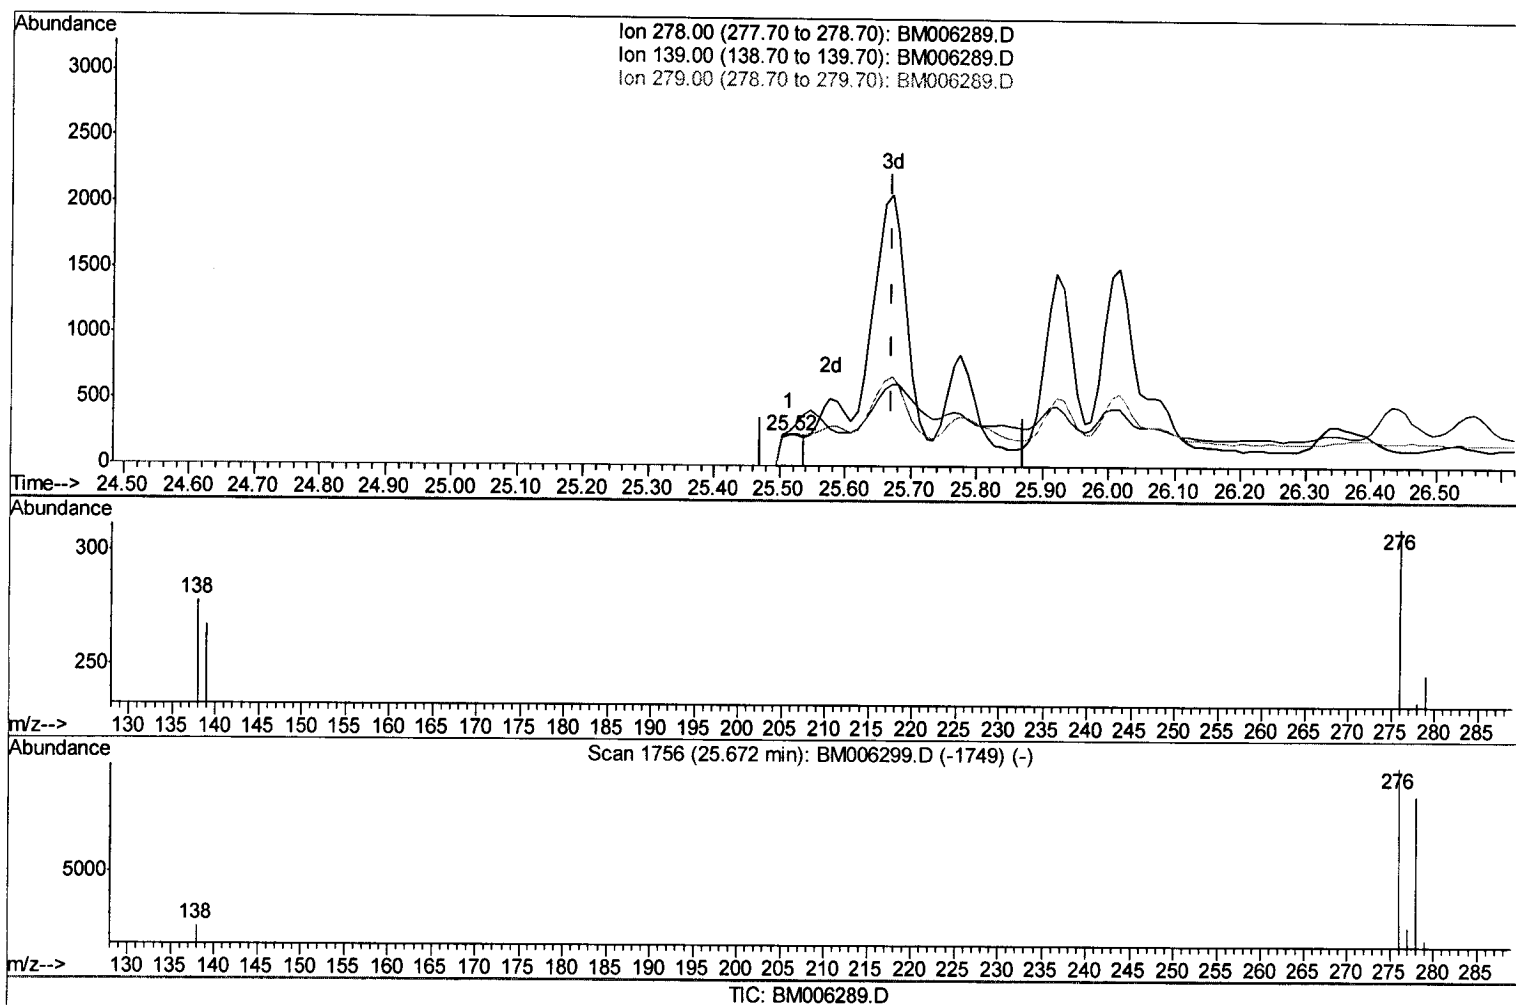

(27) Dibenzo(a,h)anthracene

25.515min (-0.156) 0.02ng/ul

response 567

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	113.62#
279.00	25.20	105.11#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV3

Quant Time: Jul 07 10:53:28 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

Manual Integration

umangi
7/7/2016 6:04:23 PM

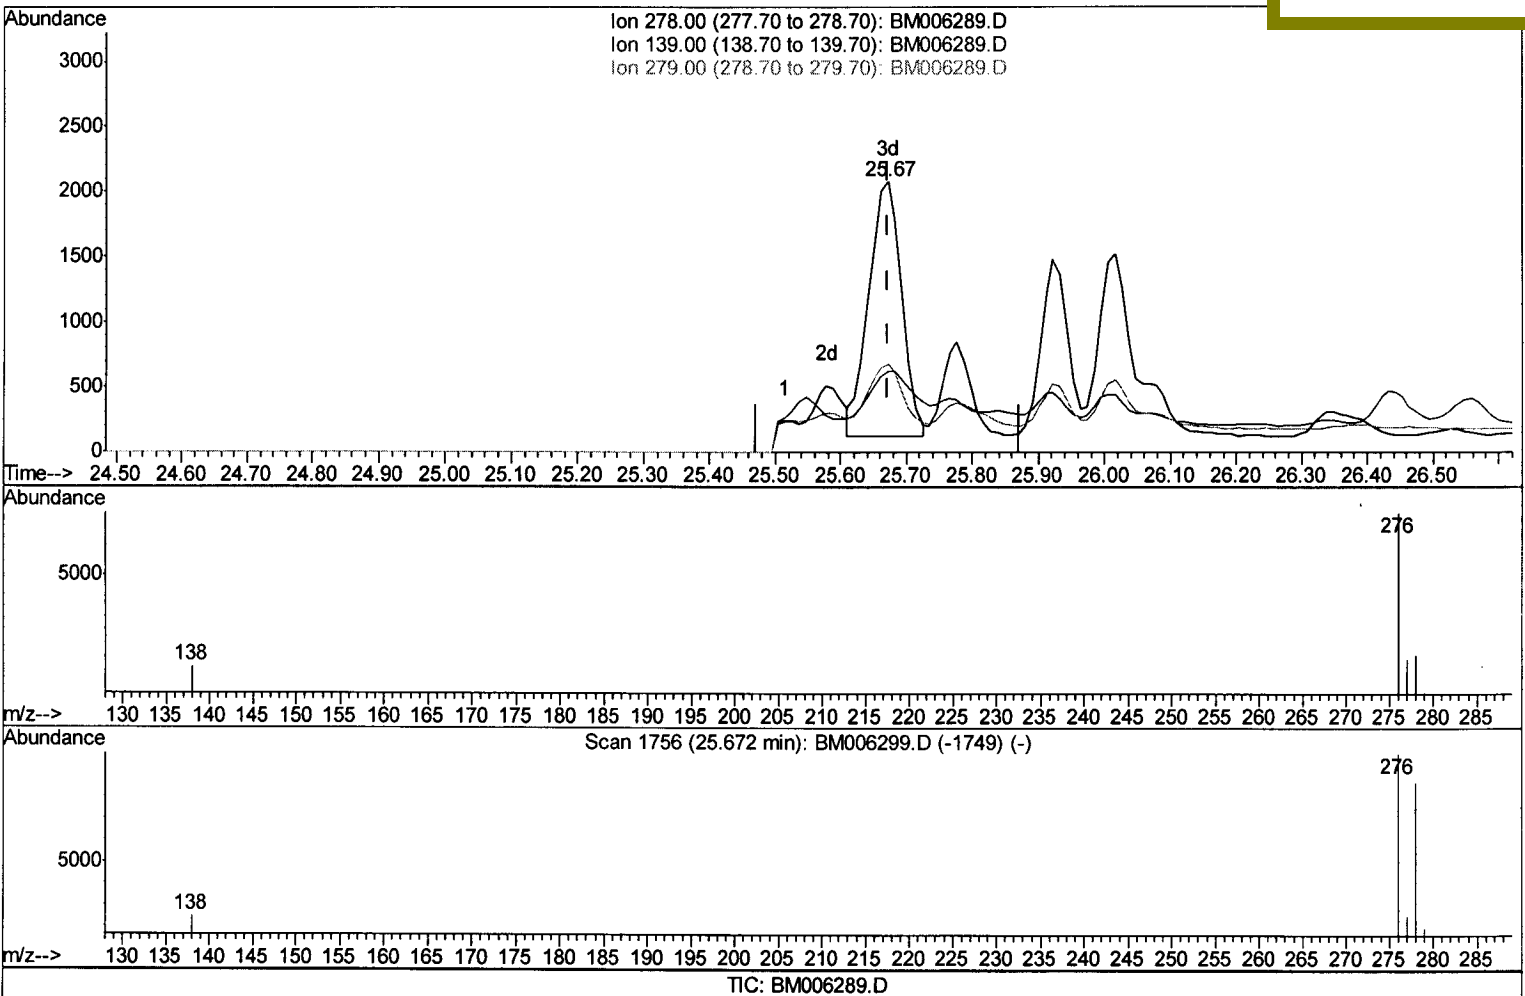

(27) Dibenzo(a,h)anthracene

25.672min (+0.000) 0.21ng/ul m

response 6792

U.M
07/11/16

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	29.97#
279.00	25.20	32.76#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006289.D
 Acq On : 06 Jul 2016 19:02
 Operator : UM/SJ
 Sample : H3811-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4TV3

Manual Integration

APPROVED
 umangi
 7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:53:28 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

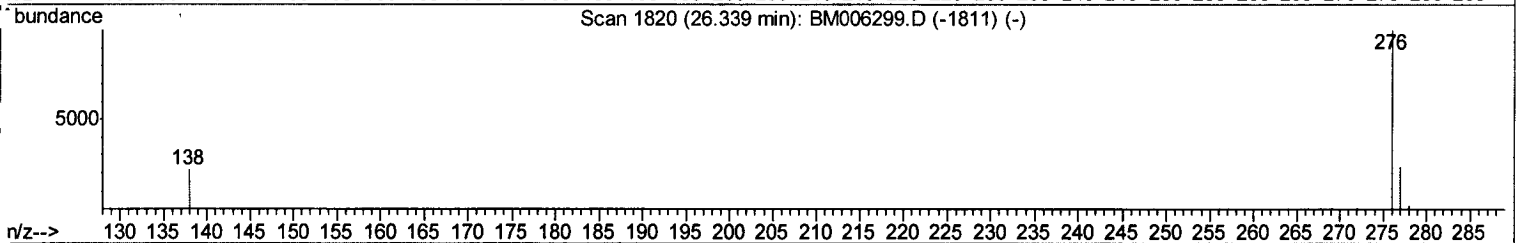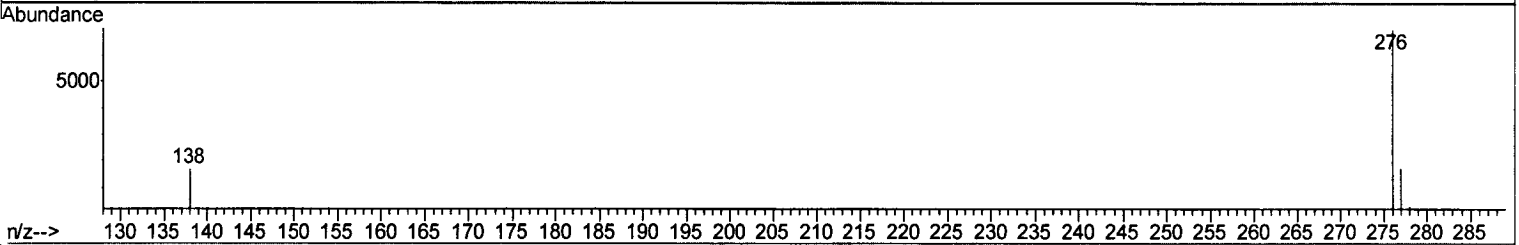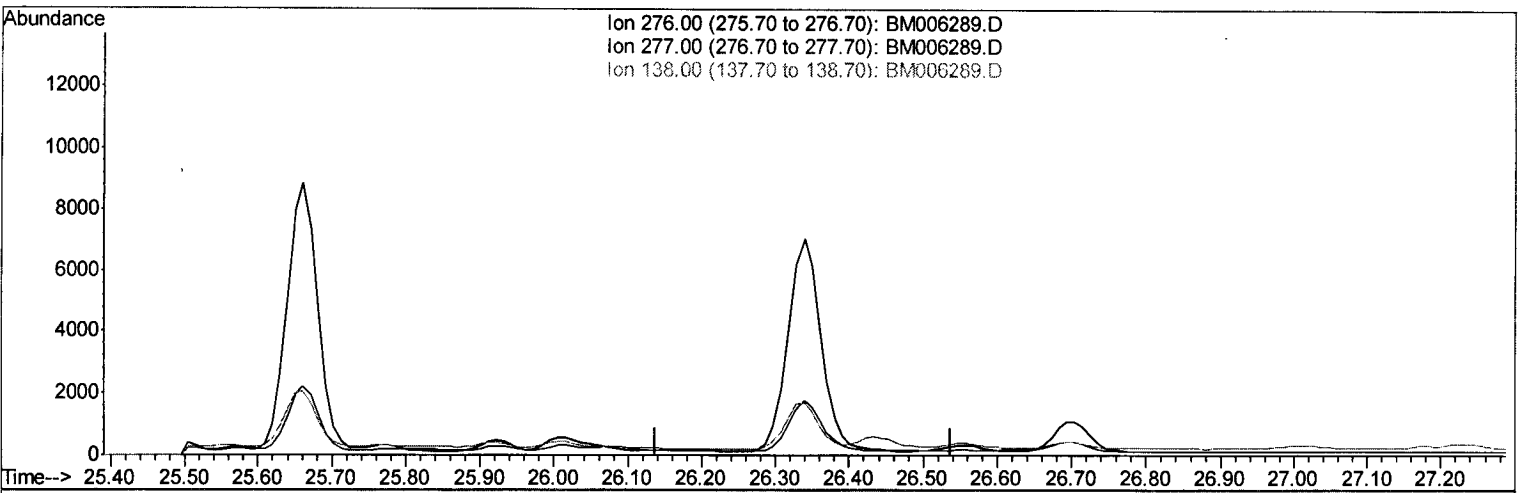

(28) Benzo(g,h,i)perylene

26.339min (-26.339) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	23.60	0.00#
138.00	28.10	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV3

Manual Integration

umangi
7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:53:28 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

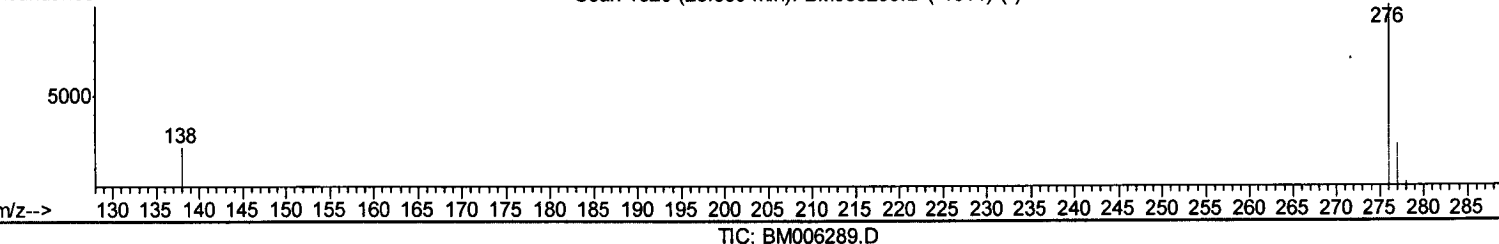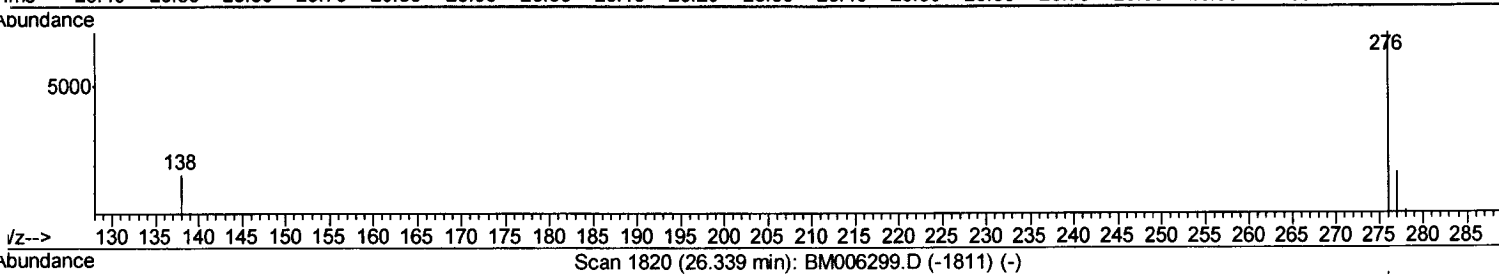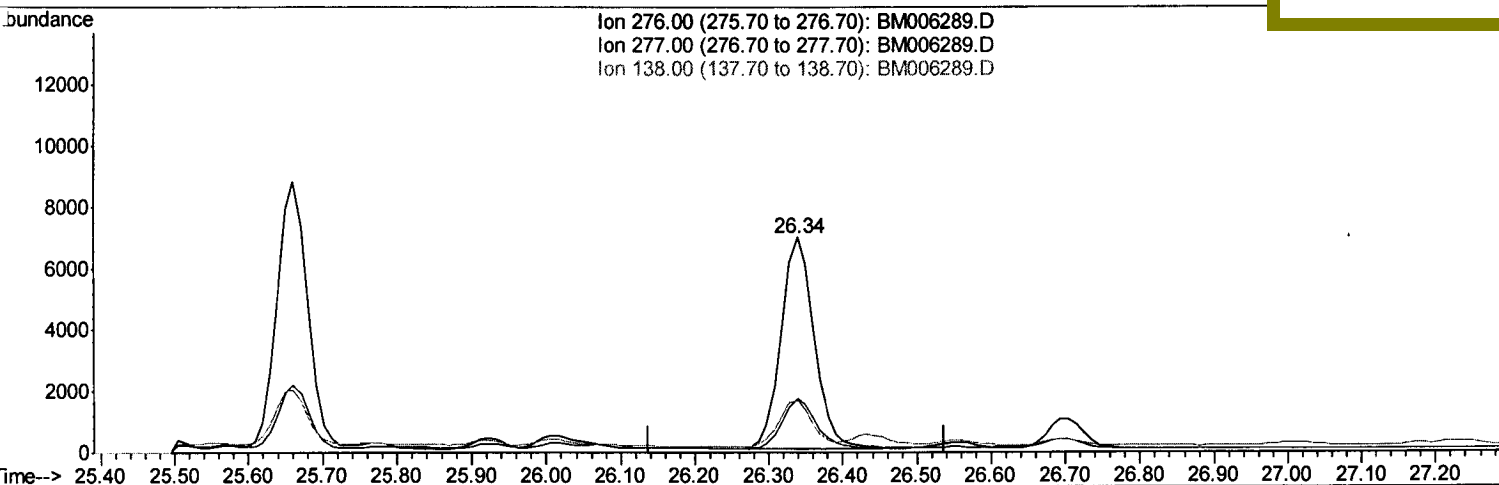

(28) Benzo(g,h,i)perylene

26.339min (+0.000) 0.63ng/ul m

response 21668

U.M
07/11/16

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	25.00
138.00	28.10	24.28
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006289.D
Acq On : 06 Jul 2016 19:02
Operator : UM/SJ
Sample : H3811-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV3

Manual Integration

APPROVED
umangi
7/7/2016 6:04:23 PM

Quant Time: Jul 07 10:56:10 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	4264	0.40	ng/ul	0.00
4) Naphthalene-d8	10.43	136	17021	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	9942	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.04	188	20883m	0.40	ng/ul	0.00
18) Chrysene-d12	21.24	240	14362	0.40	ng/ul	0.00
22) Perylene-d12	23.45	264	10954m	0.40	ng/ul	0.00

u.m
07/11/16

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	9823	5.45	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.02	152	7564	0.38	ng/ul	0.00
16) Fluoranthene-d10	19.07	212	15976	0.36	ng/ul	-0.01

Target Compounds

					Qvalue
5) Naphthalene	10.48	128	1285	0.03 ng/ul#	77
7) 2-Methylnaphthalene	12.09	142	779	0.03 ng/ul	99
9) Acenaphthylene	14.01	152	6477	0.19 ng/ul#	94
14) Phenanthrene	17.07	178	16526m	0.29 ng/ul	
15) Anthracene	17.16	178	6447	0.12 ng/ul#	86
17) Fluoranthene	19.11	202	95179m	1.49 ng/ul	
19) Pyrene	19.47	202	100530	1.67 ng/ul	96
20) Benzo(a)anthracene	21.22	228	38475	0.83 ng/ul#	92
21) Chrysene	21.27	228	44109	0.97 ng/ul	94
23) Benzo(b)fluoranthene	22.78	252	69102m	1.76 ng/ul	
24) Benzo(k)fluoranthene	22.83	252	17473m	0.48 ng/ul	
25) Benzo(a)pyrene	23.35	252	33625m	0.92 ng/ul	
26) Indeno(1,2,3-cd)pyrene	25.66	276	24902m	0.61 ng/ul	
27) Dibenzo(a,h)anthracene	25.67	278	6792m	0.21 ng/ul	
28) Benzo(g,h,i)perylene	26.34	276	21668m	0.63 ng/ul	

u.m
07/11/16

u.m
07/11/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed