

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

Quant Time: Jul 07 11:20:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/7/2016 6:05:03 PM

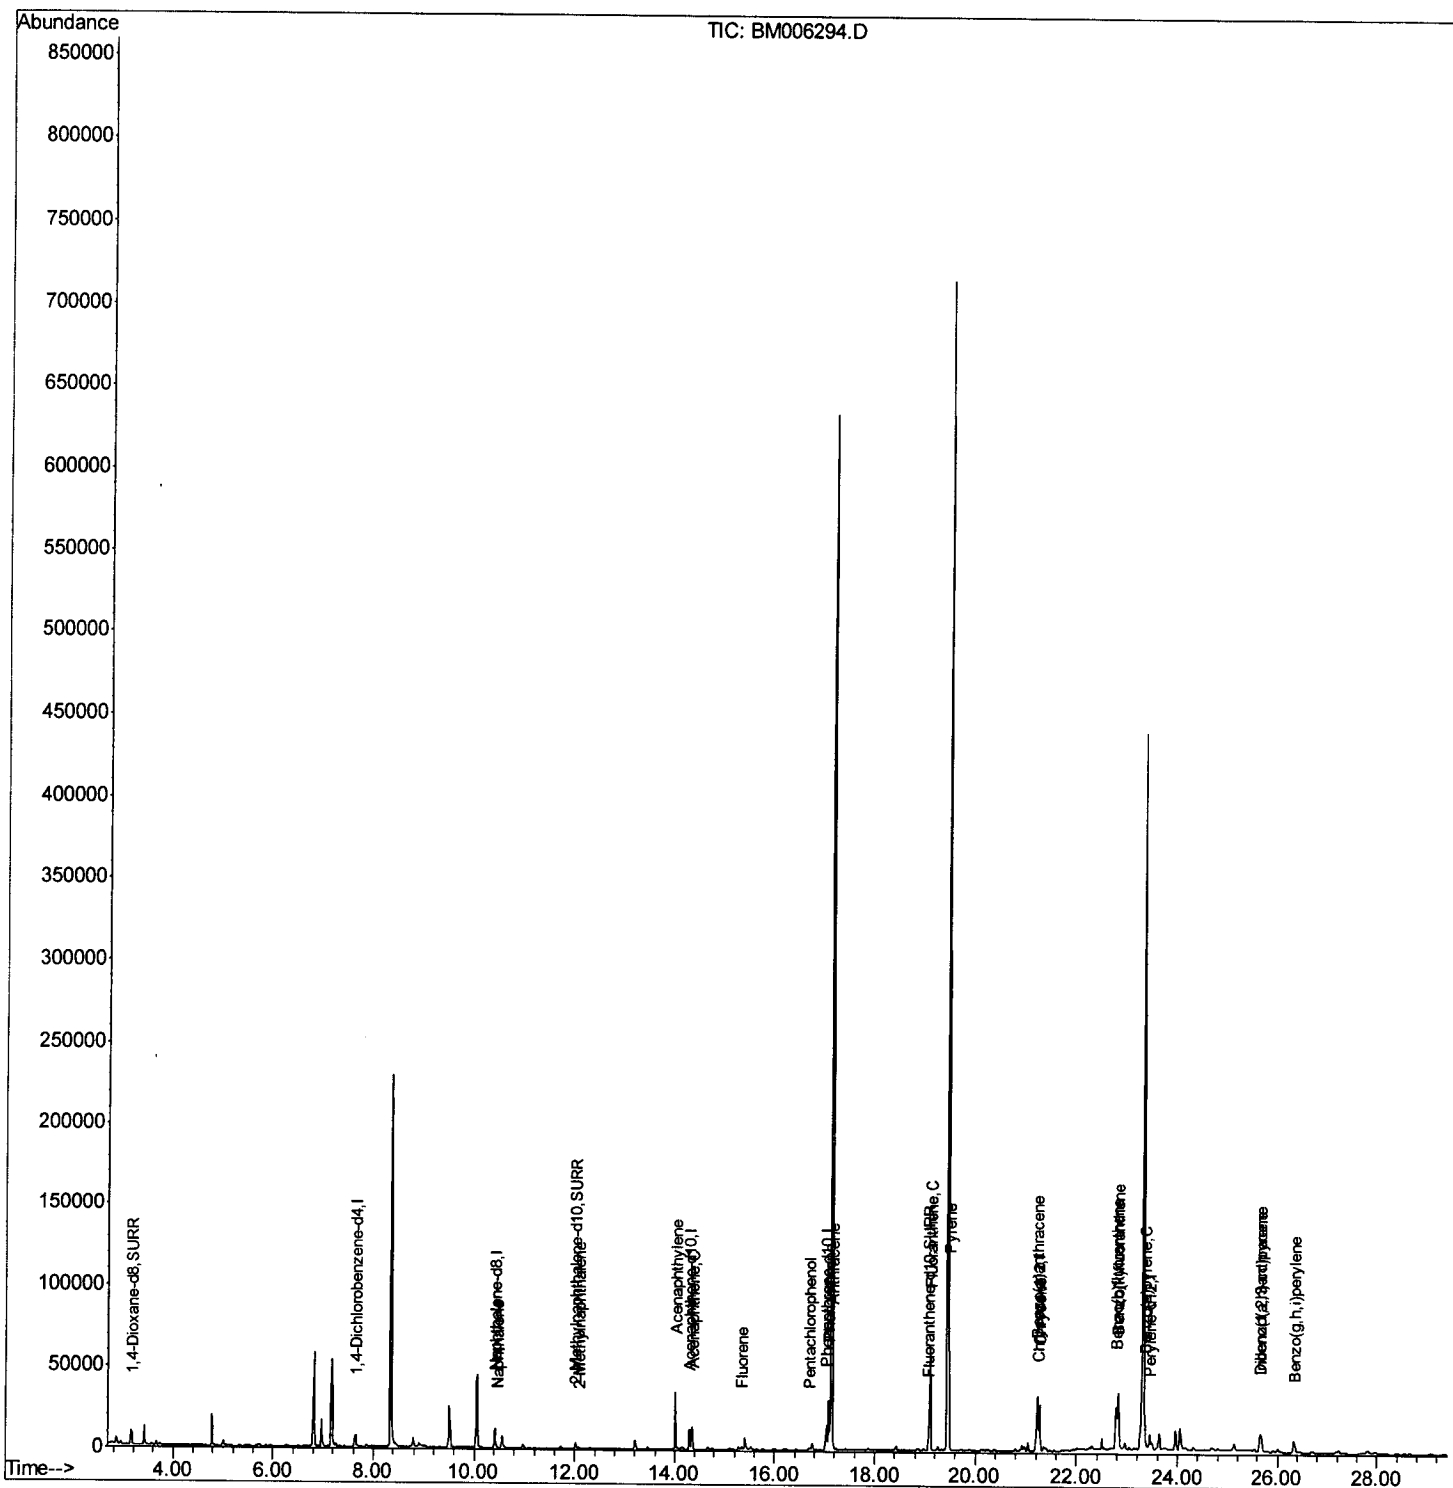

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

Quant Time: Jul 07 11:16:15 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

umangi
 7/7/2016 6:05:03 PM

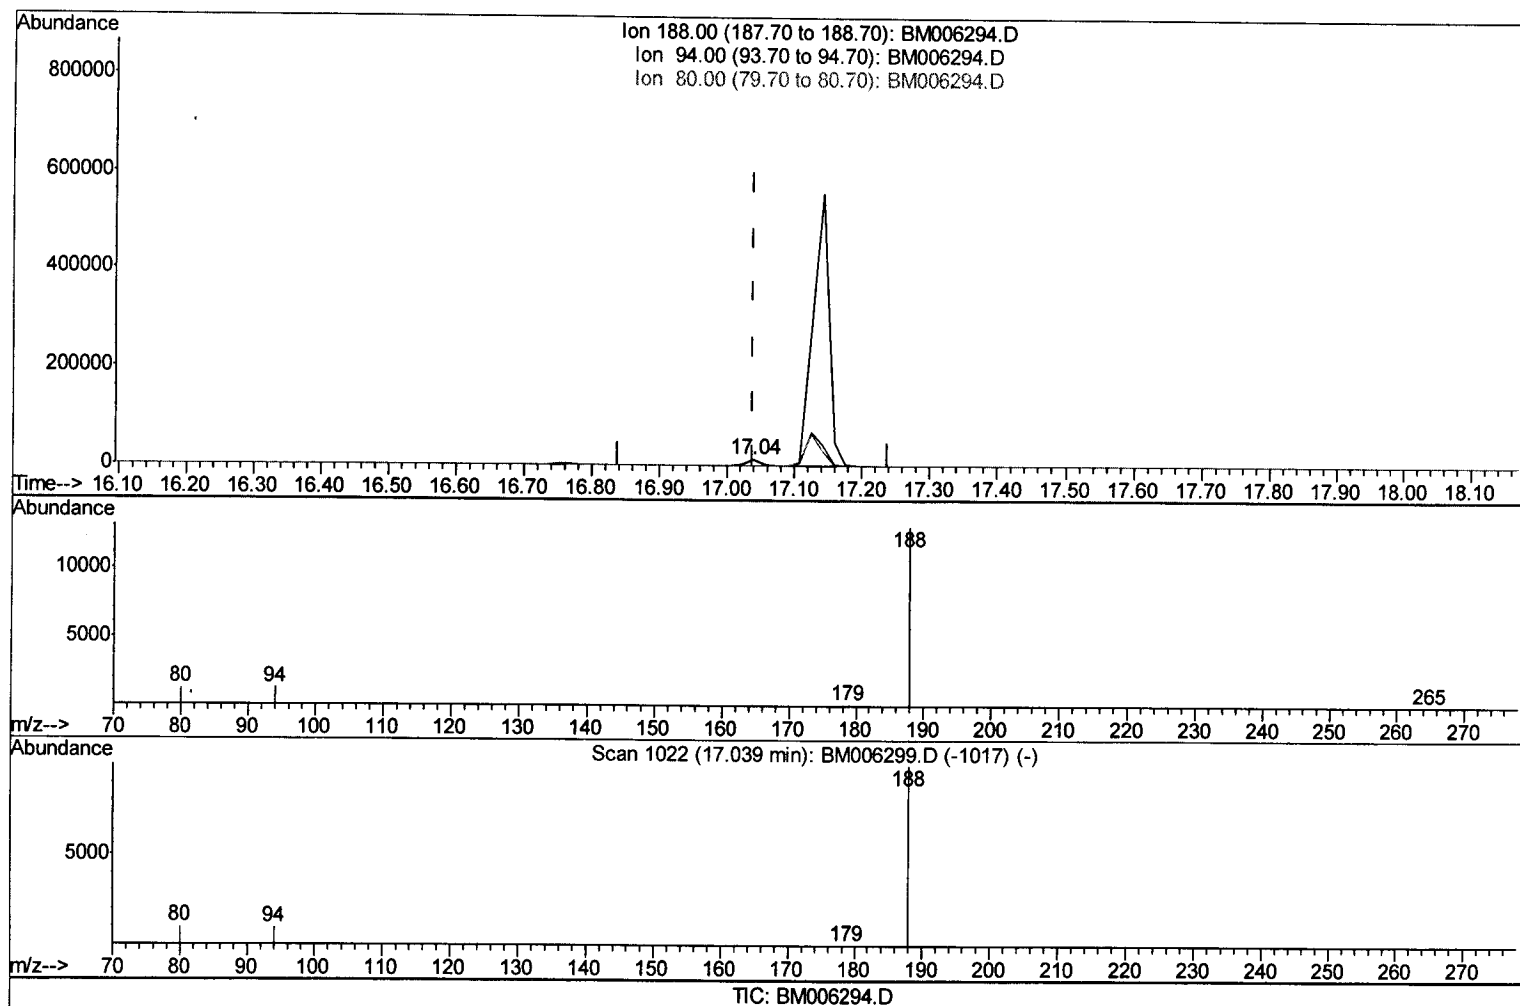

(12) Phenanthrene-d10 (I)

17.039min (+0.000) 0.40ng/ul m U.M
 response 19043 07/11/16

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	9.74
80.00	11.90	9.42#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006294.D
Acq On : 06 Jul 2016 22:03
Operator : UM/SJ
Sample : H3811-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

Manual Integration

APPROVED
umangi
7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:16:15 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

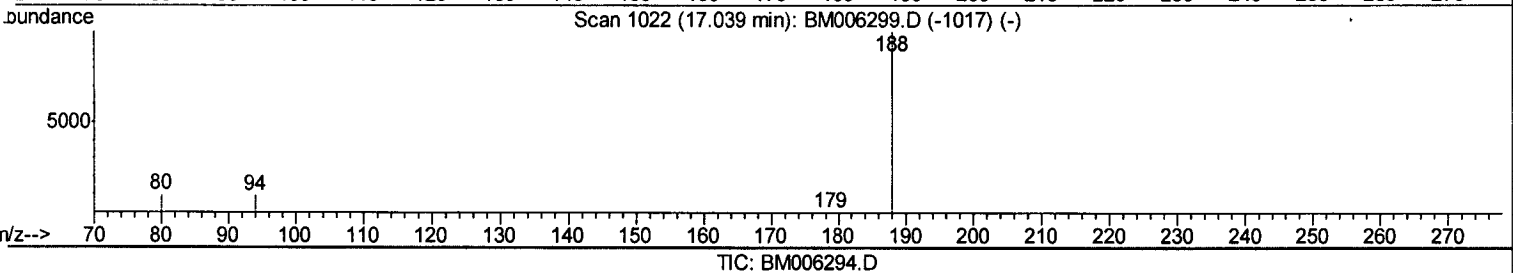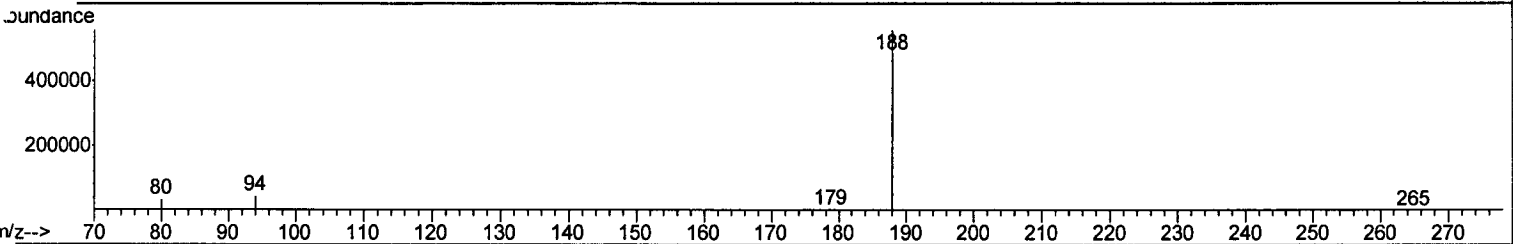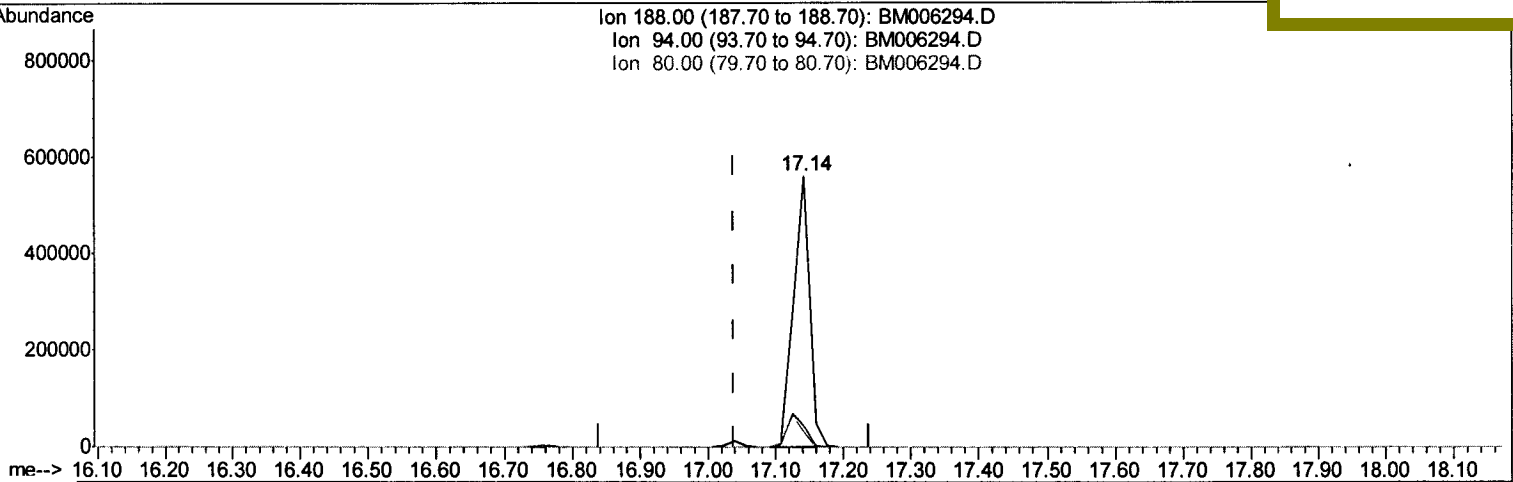

(12) Phenanthrene-d10 (I)

17.142min (+0.103) 0.40ng/ul

response 921740

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.61#
80.00	11.90	5.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

Quant Time: Jul 07 11:16:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/7/2016 6:05:03 PM

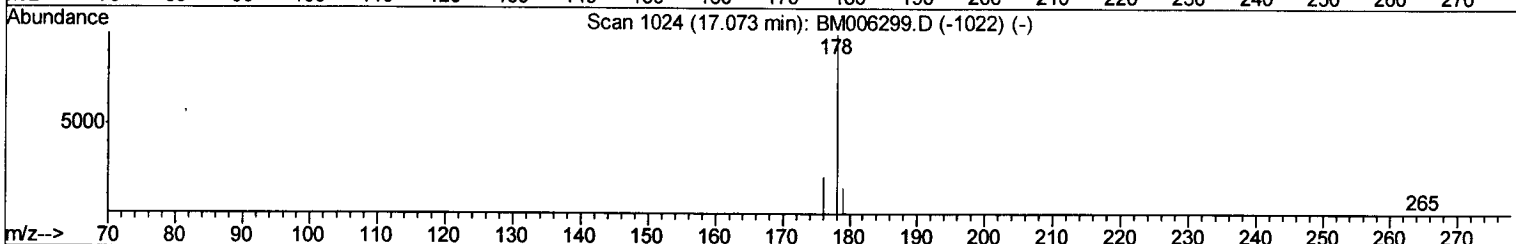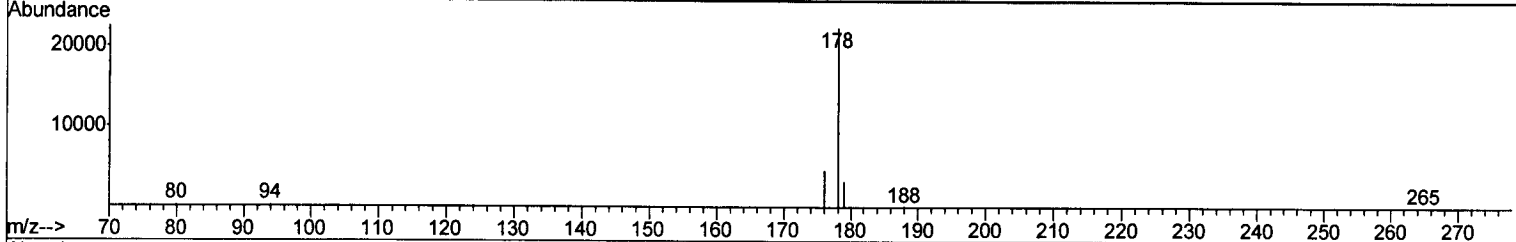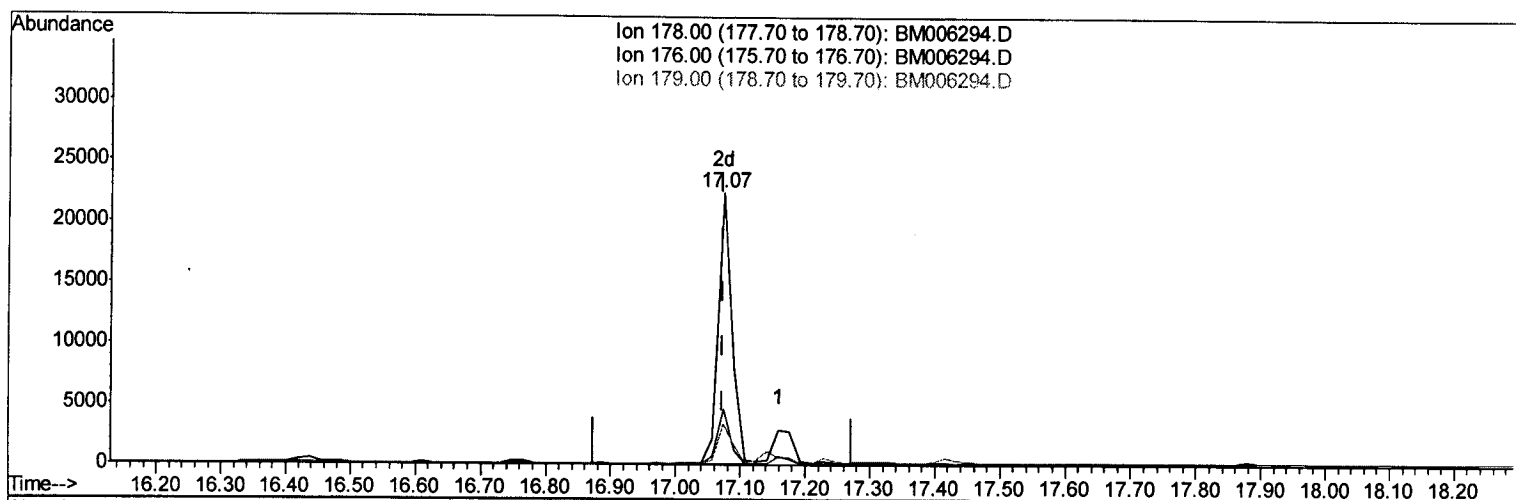

TIC: BM006294.D

(14) Phenanthrene

17.073min (+0.000) 0.64ng/ul m UM
 response 33914
 07/11/16

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	20.51#
179.00	17.70	14.94
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006294.D
Acq On : 06 Jul 2016 22:03
Operator : UM/SJ
Sample : H3811-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

Manual Integration

umangi
7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:16:48 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

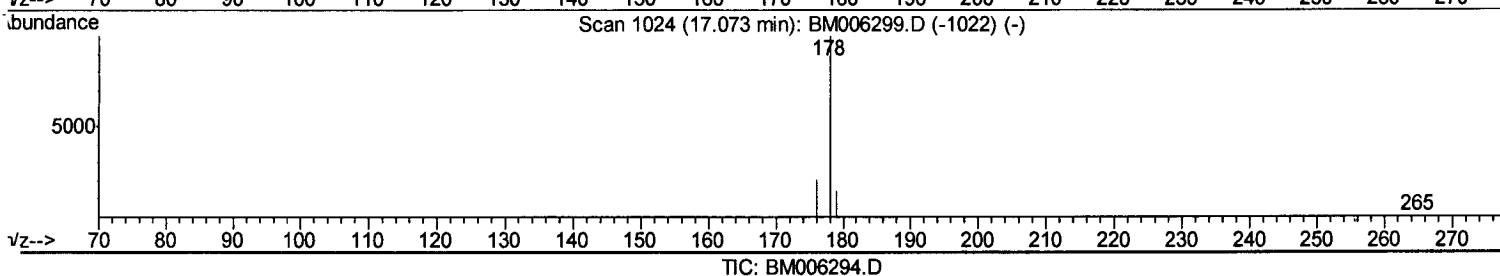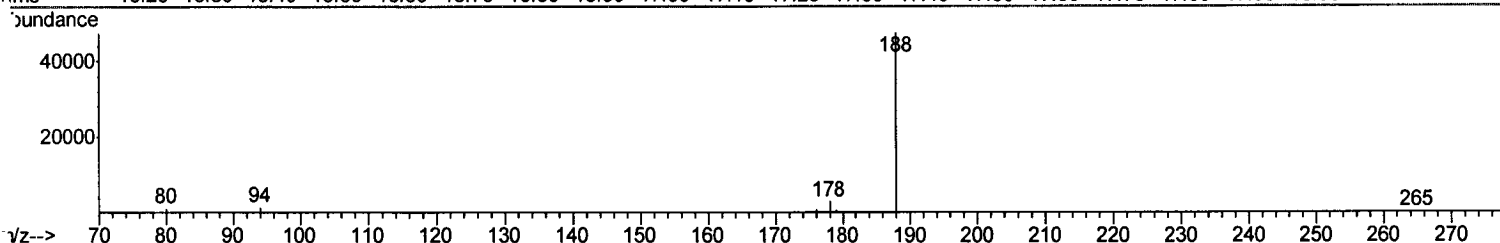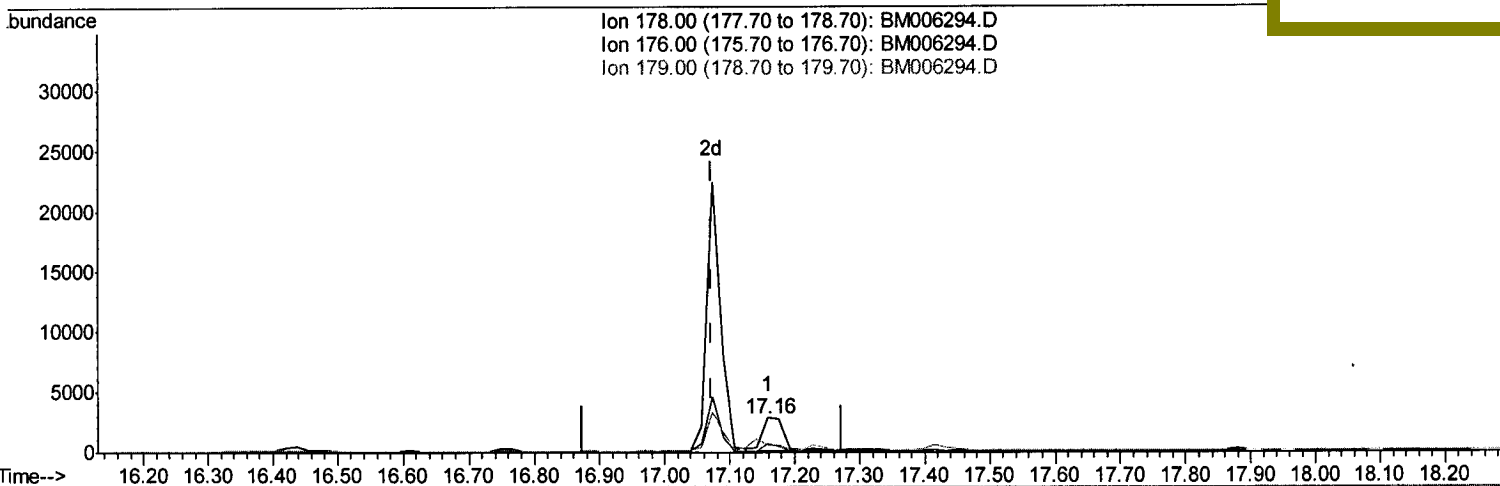

TIC: BM006294.D

(14) Phenanthrene

17.159min (+0.086) 0.12ng/ul

response 6241

Ion	Exp%	Act%
178.00	100	100
176.00	16.20	24.35#
179.00	17.70	22.52#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

umangi
 7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:16:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

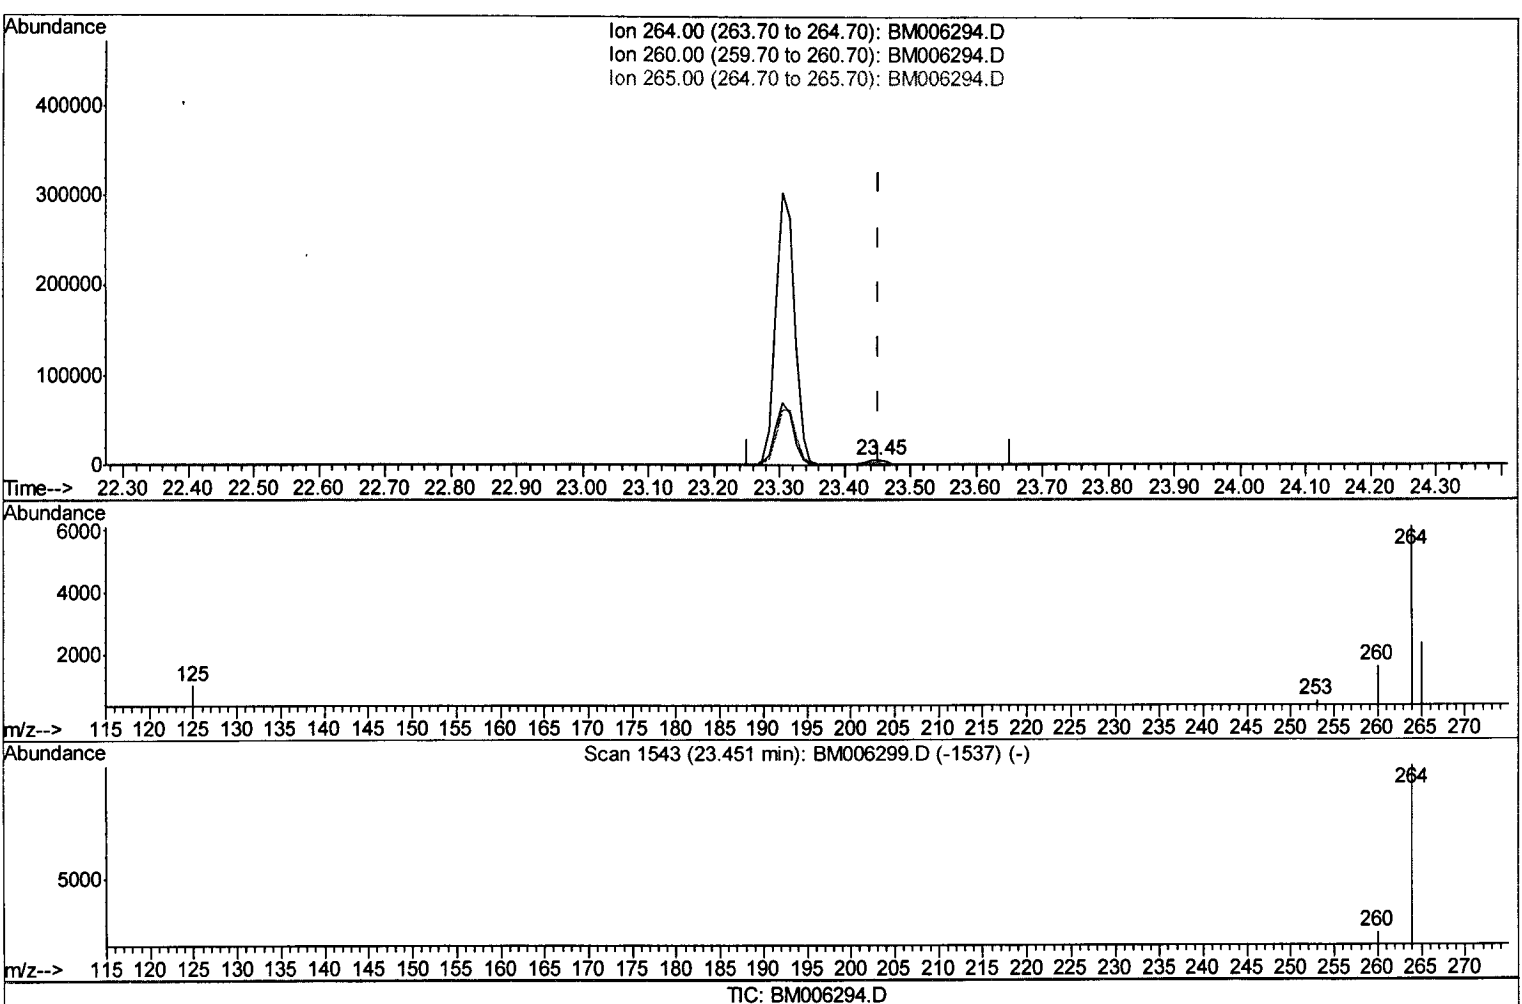

(22) Perylene-d12 (I)

23.451min (+0.000) 0.40ng/ul m

response 11257

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	26.58
265.00	38.20	38.73
0.00	0.00	0.00

U.M
 07/11/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Quant Time: Jul 07 11:16:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

Manual Integration

APPROVED
 umangi
 7/7/2016 6:05:03 PM

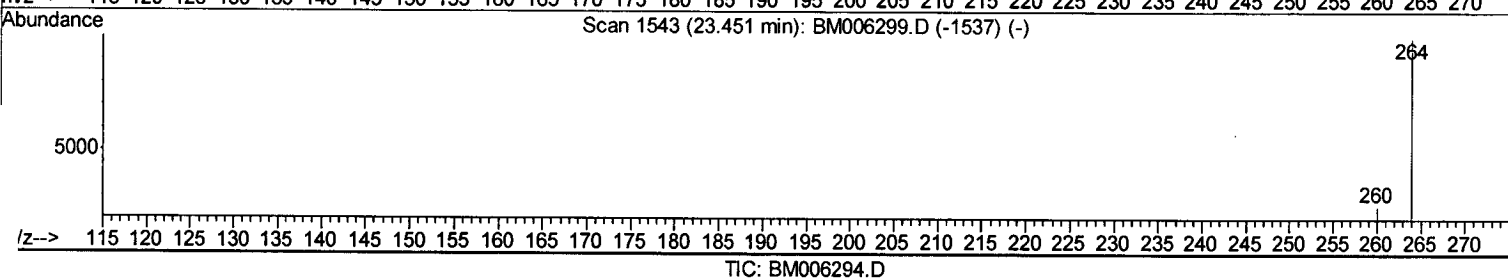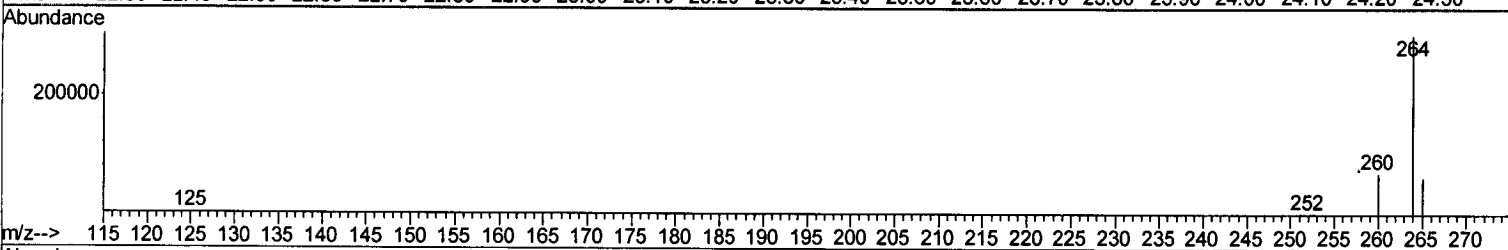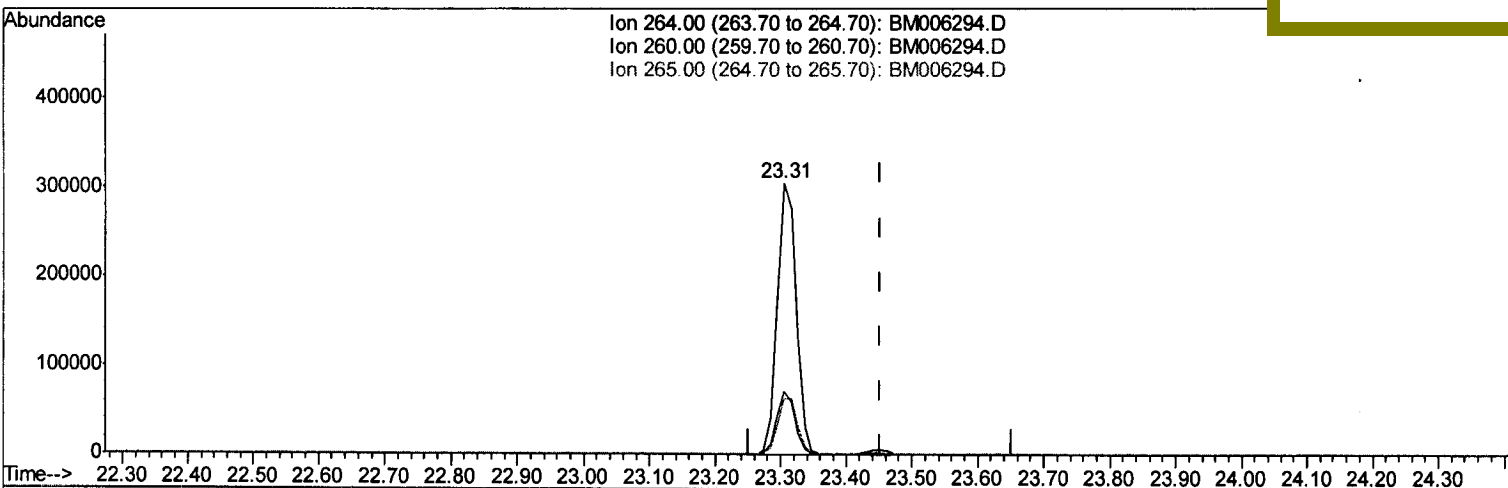

TIC: BM006294.D

(22) Perylene-d12 (I)

23.305min (-0.146) 0.40ng/ul

response 590474

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	23.07
265.00	38.20	20.57#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

umangi
 7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

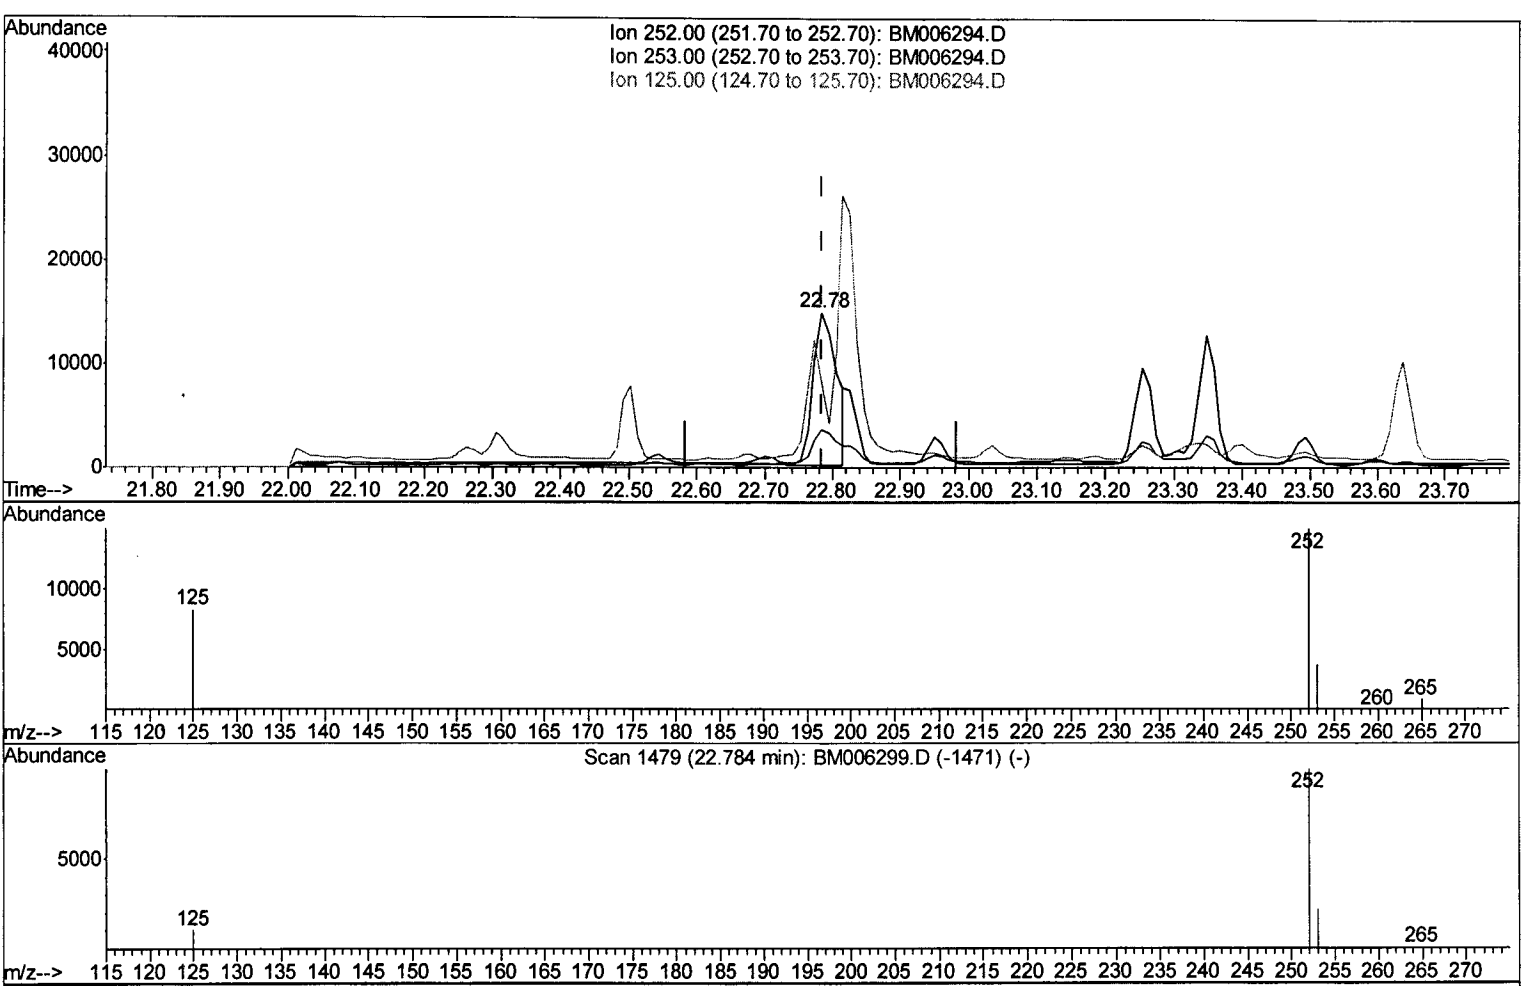

TIC: BM006294.D

(23) Benzo(b)fluoranthene

22.784min (+0.000) 0.89ng/ul m U.M

response 35976

07/11/16

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	25.16
125.00	14.40	55.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

Manual Integration

APPROVED
 umangi
 7/7/2016 6:05:03 PM

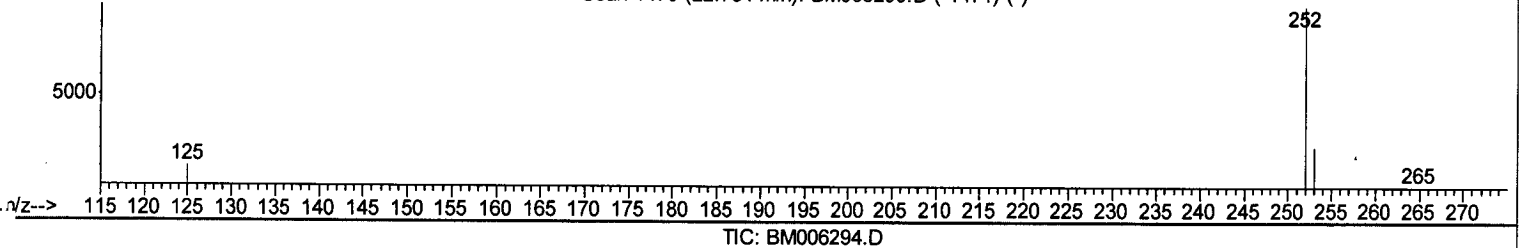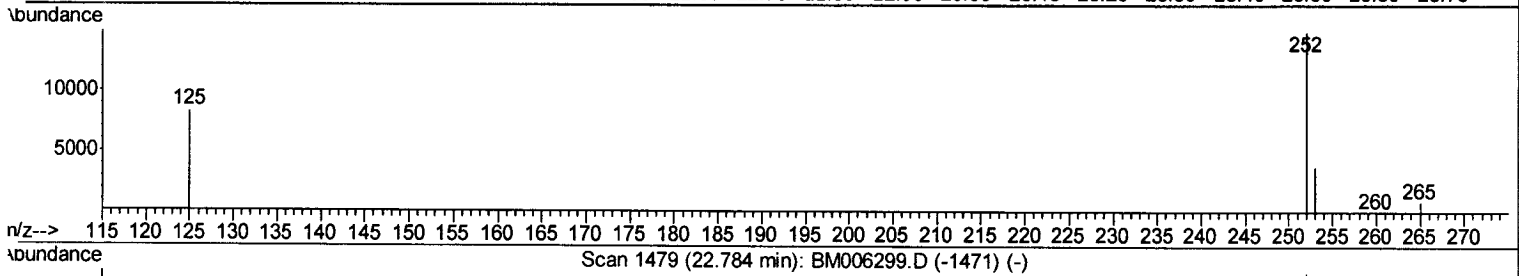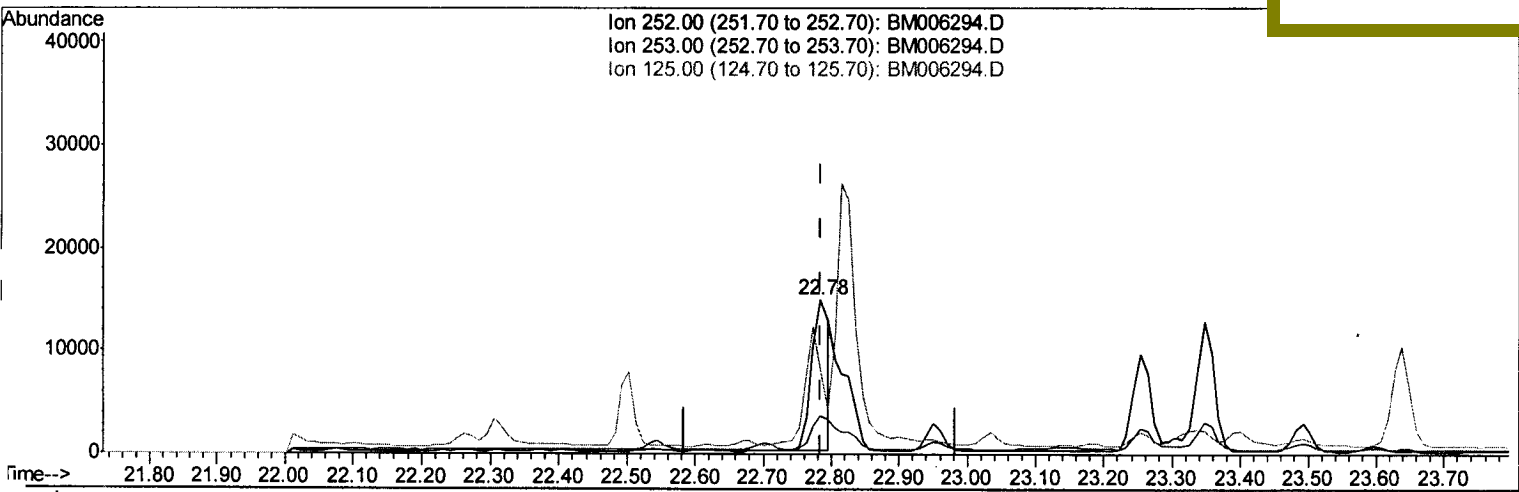

(23) Benzo(b)fluoranthene
 22.784min (+0.000) 0.64ng/ul
 response 25621

Ion	Exp%	Act%
252.00	100	100
253.00	22.70	25.16
125.00	14.40	55.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integration

umangi
 7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

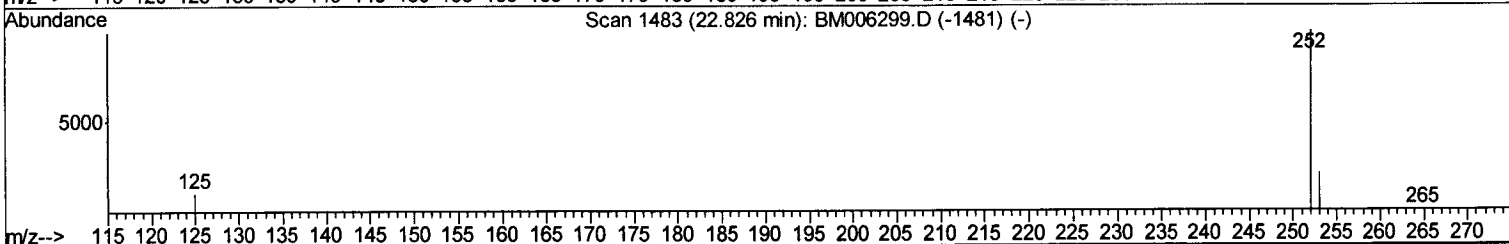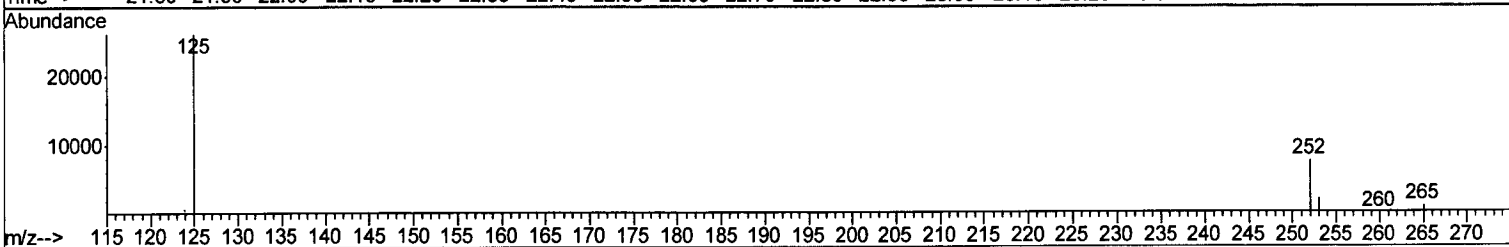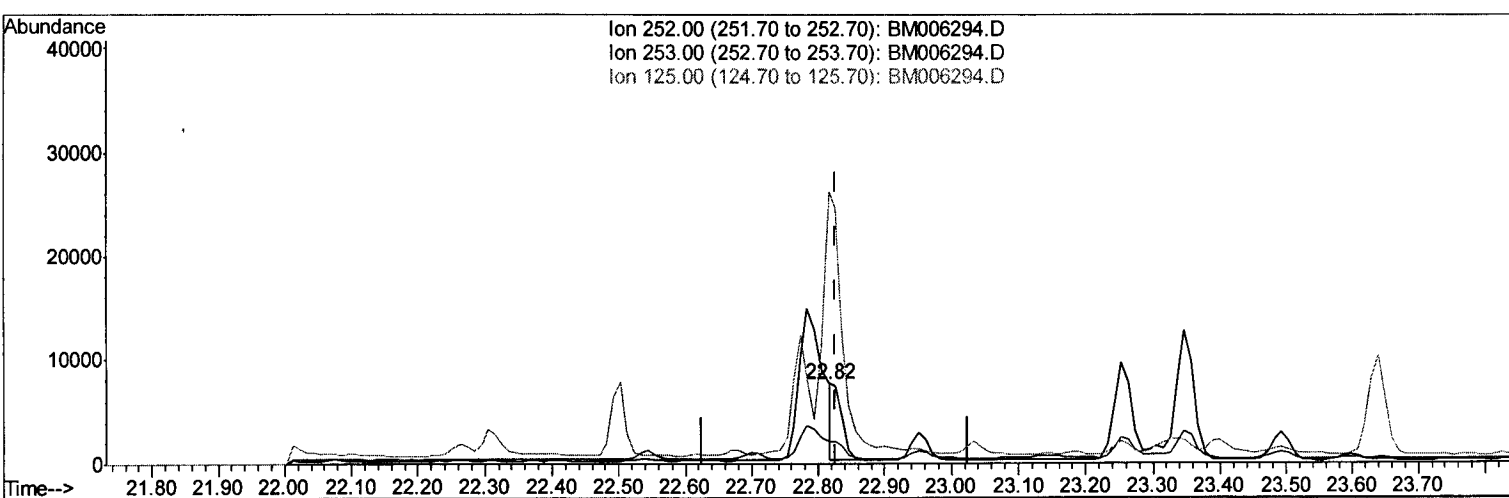

TIC: BM006294.D

(24) Benzo(k)fluoranthene

22.815min (-0.010) 0.21ng/ul m

response 7891

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	28.14
125.00	13.00	340.33#
0.00	0.00	0.00

U.M
 07/11/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 A4TV6MSD

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/7/2016 6:05:03 PM

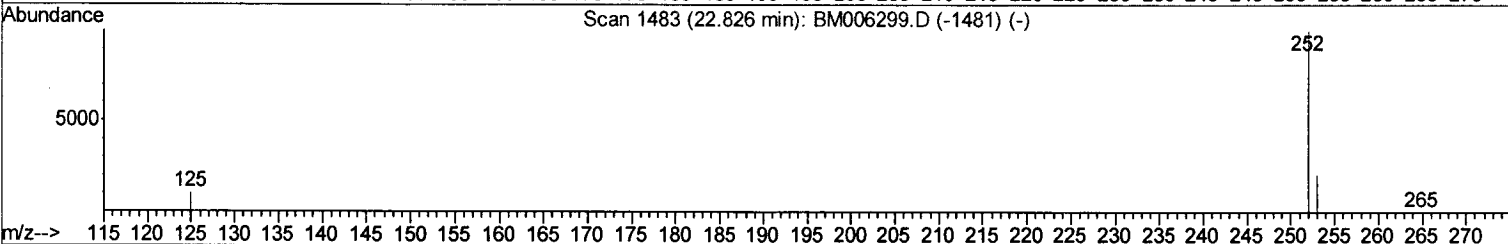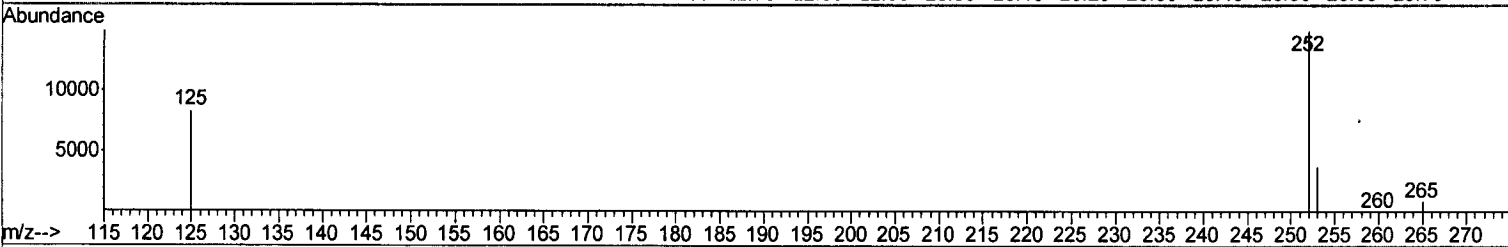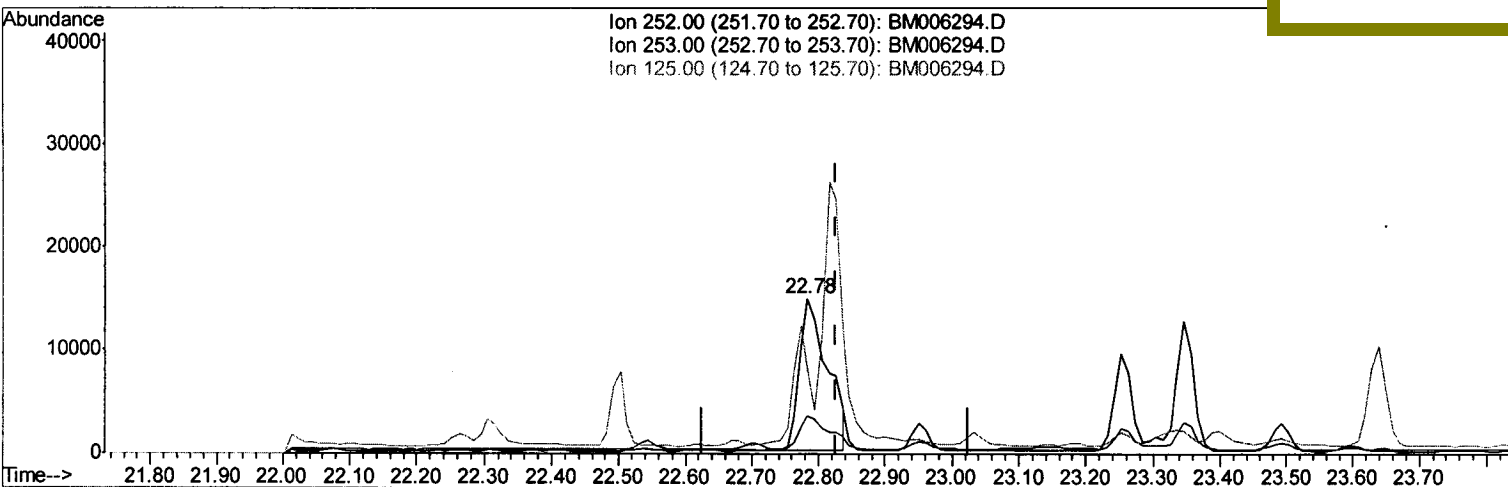

(24) Benzo(k)fluoranthene

22.784min (-0.042) 1.14ng/ul

response 42856

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	25.16
125.00	13.00	55.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA M
 ClientSampleId :
 A4TV6MSD

Manual Integration

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

APPROVED
 umangi
 7/7/2016 6:05:03 PM

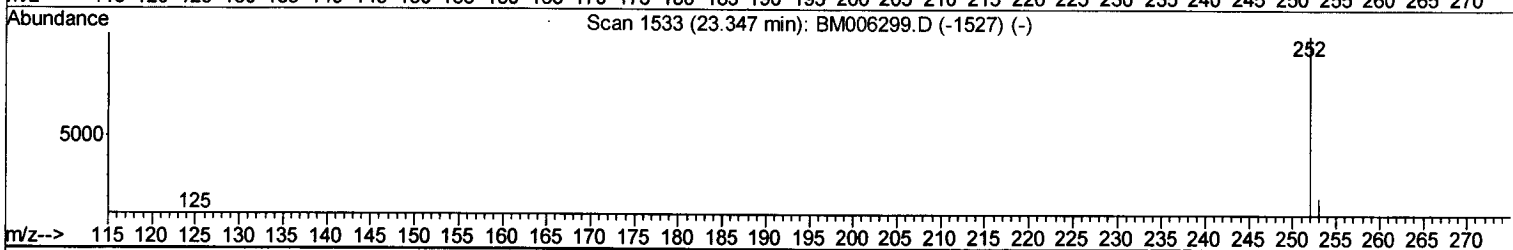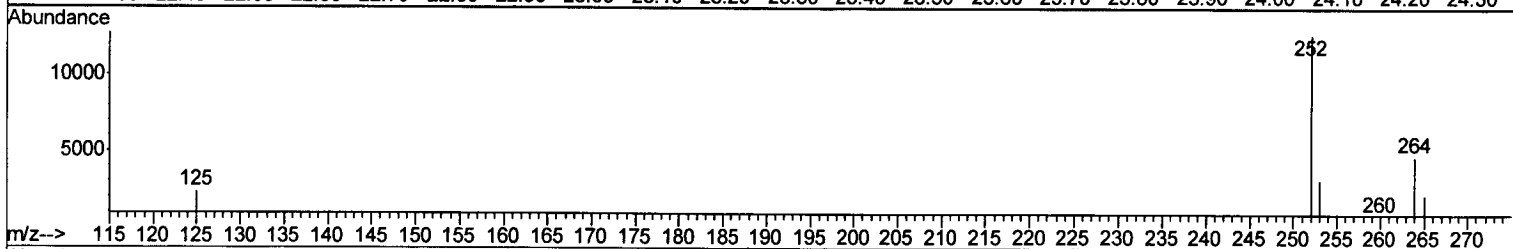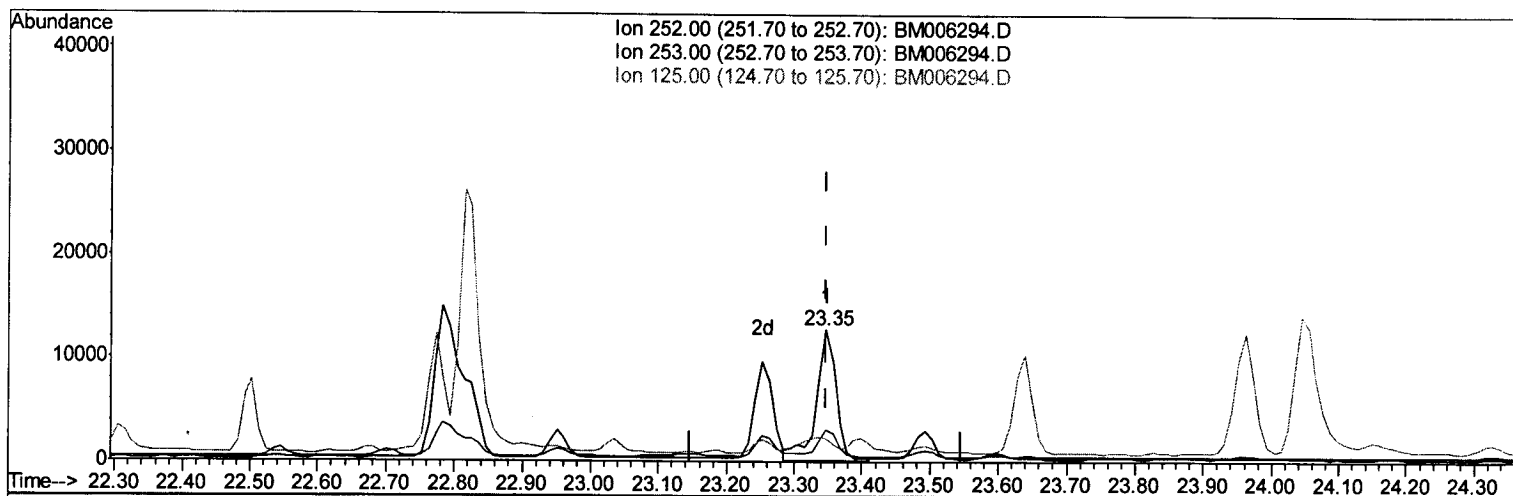

TIC: BM006294.D

(25) Benzo(a)pyrene (C)

23.347min (+0.000) 0.68ng/ul m

response 25361

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	24.71
125.00	15.90	18.28
0.00	0.00	0.00

U.M
 07/11/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4TV6MSD

Manual Integrati

umangi
 7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

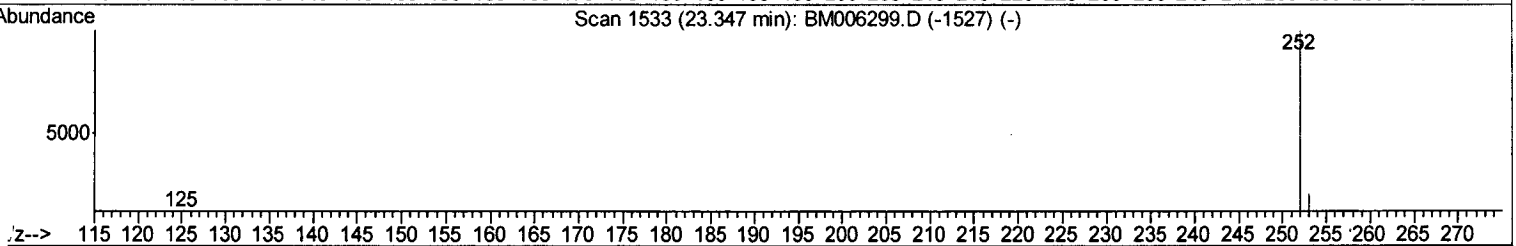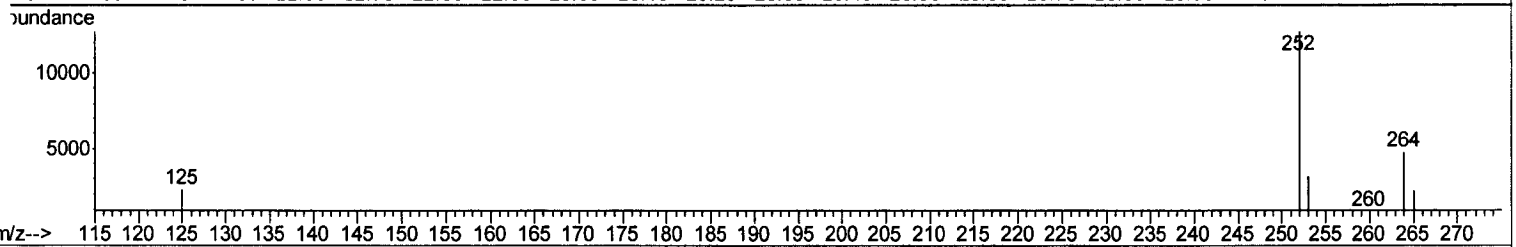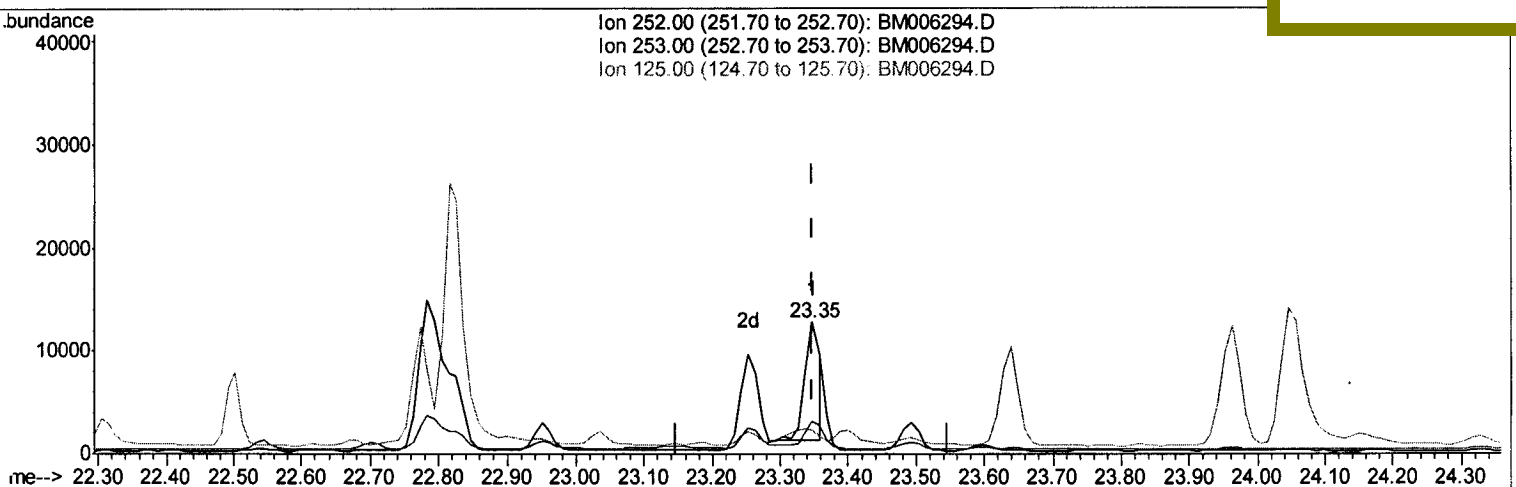

TIC: BM006294.D

(25) Benzo(a)pyrene (C)

23.347min (+0.000) 0.45ng/ul

response 17050

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	24.71
125.00	15.90	18.28
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A4TV6MSD

Manual Integration

umangi
 7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

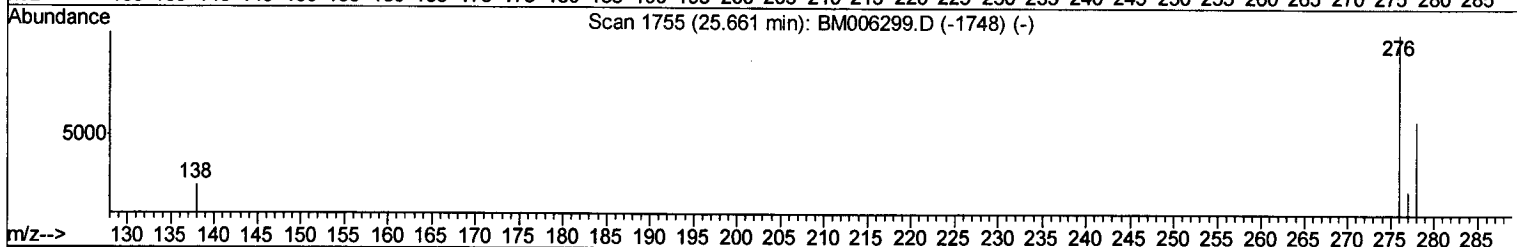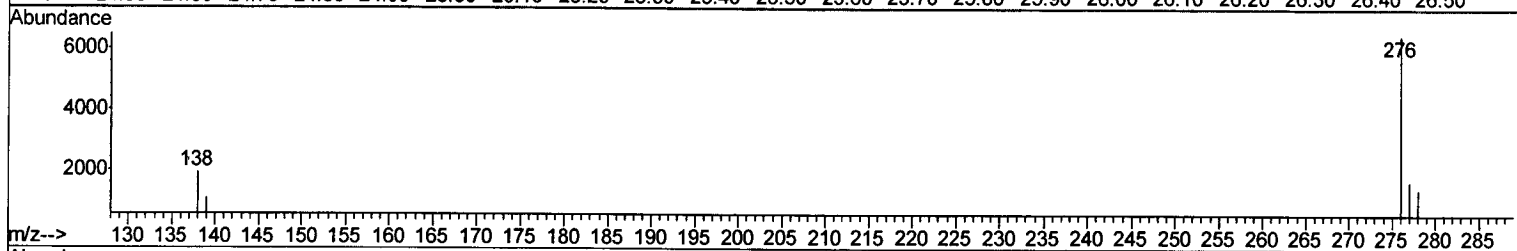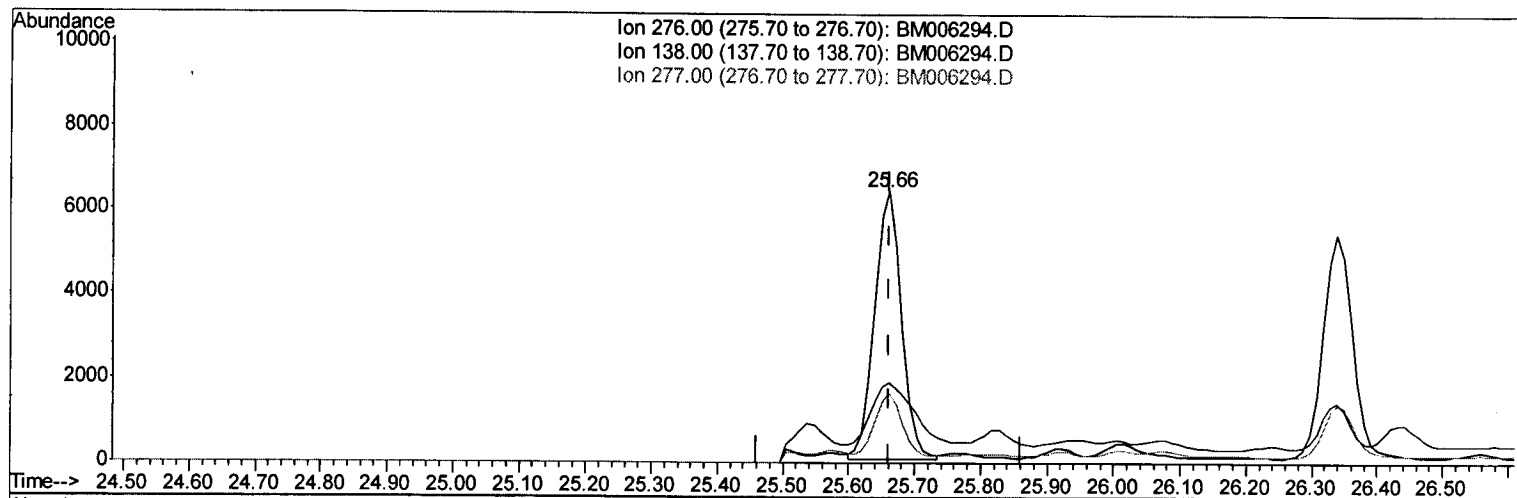

TIC: BM006294.D

(26) Indeno(1,2,3-cd)pyrene

25.661min (+0.000) 0.44ng/ul m

response 18118

U.M
 07/11/16

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	0.00#
277.00	24.80	3.91#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006294.D
Acq On : 06 Jul 2016 22:03
Operator : UM/SJ
Sample : H3811-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

Manual Integration

APPROVED
umangi
7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

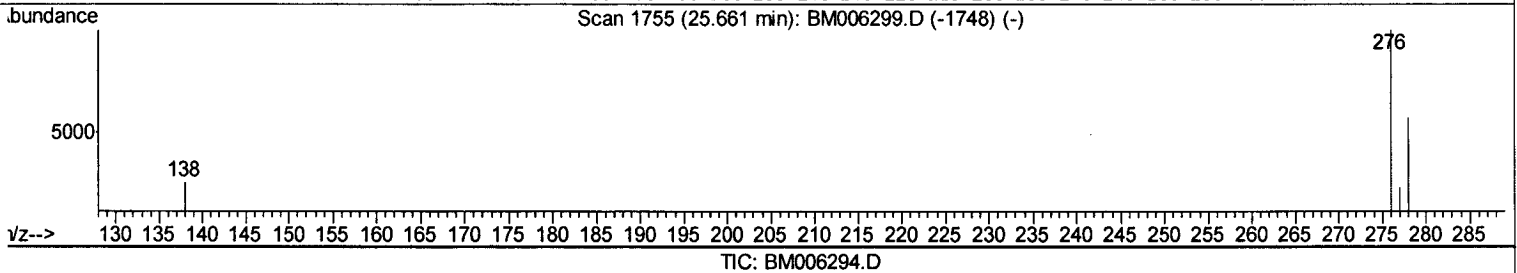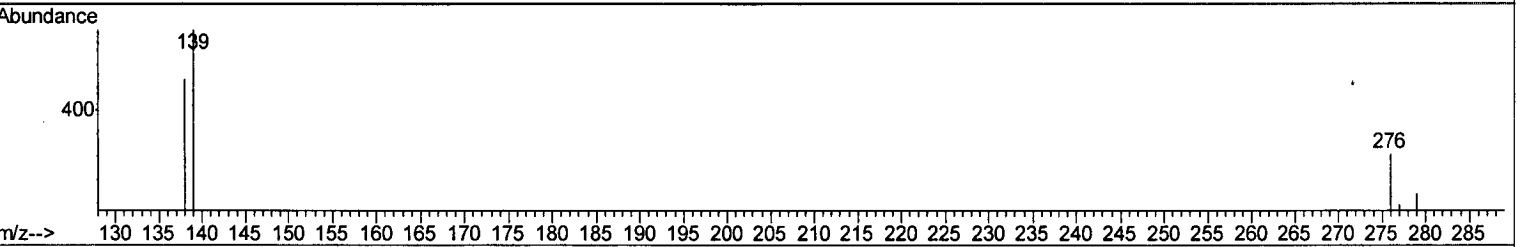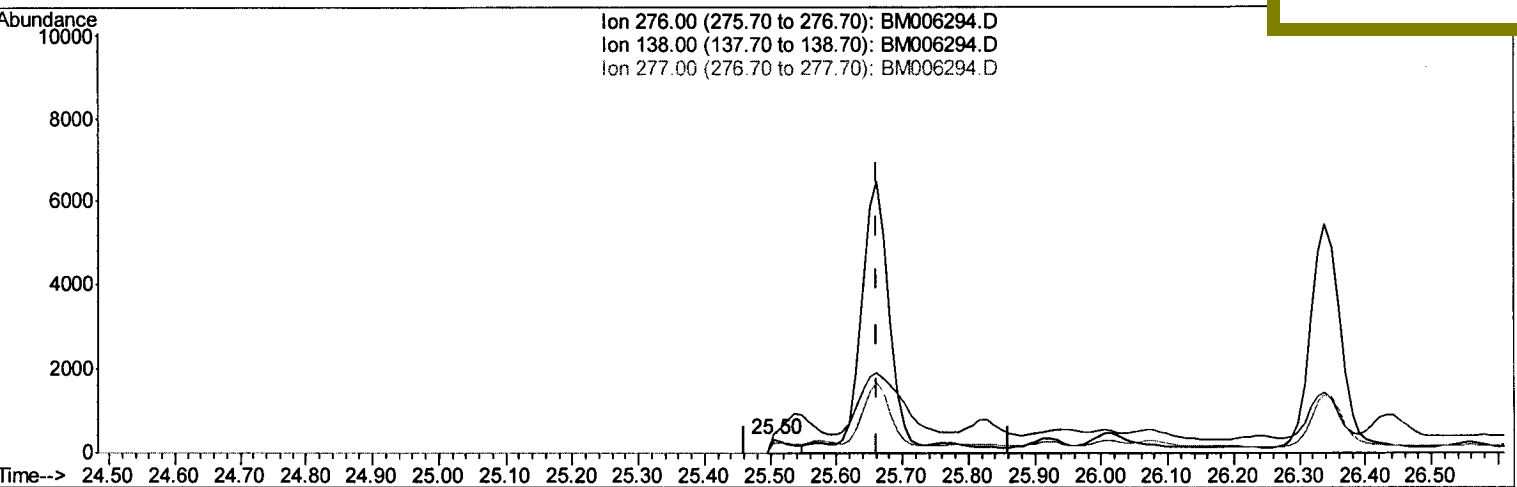

(26) Indeno(1,2,3-cd)pyrene

25.505min (-0.156) 0.02ng/ul

response 726

Ion	Exp%	Act%
276.00	100	100
138.00	20.40	0.00#
277.00	24.80	97.66#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 A4TV6MSD

Manual Integration

umangi
 7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

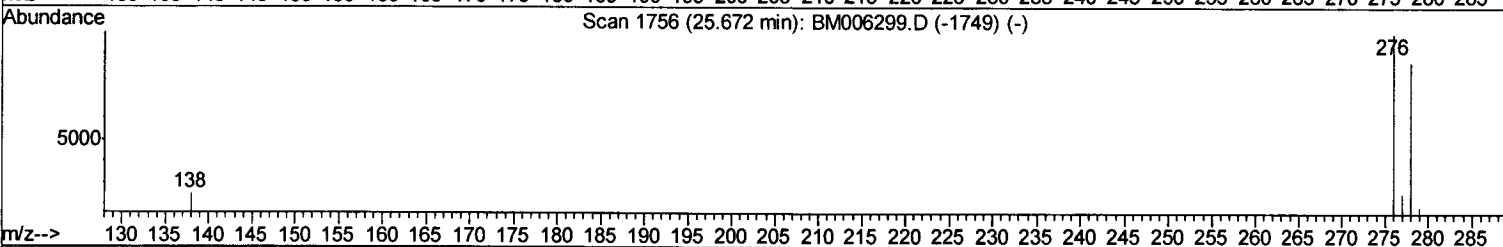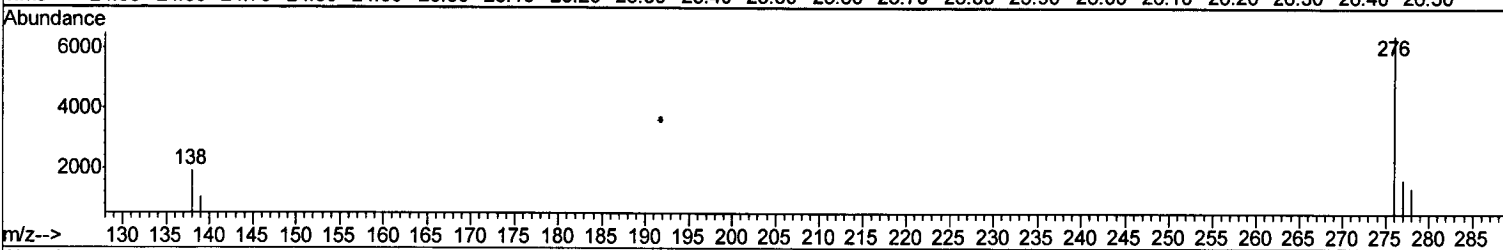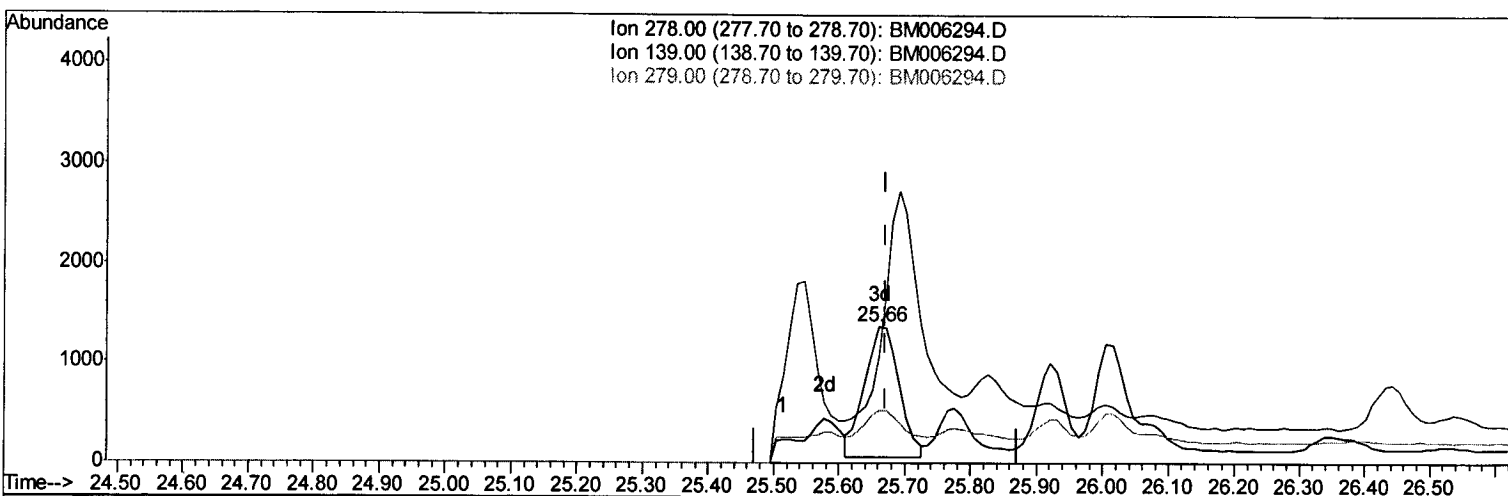

TIC: BM006294.D

(27) Dibenzo(a,h)anthracene

25.661min (-0.010) 0.15ng/ul m

response 4738

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	77.49#
279.00	25.20	38.38#
0.00	0.00	0.00

```




Data Path   : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File   : BM006294.D
Acq On      : 06 Jul 2016   22:03
Operator    : UM/SJ
Sample      : H3811-08MSD
Misc        :
ALS Vial    : 16      Sample Multiplier: 1

```

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

umangi
7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

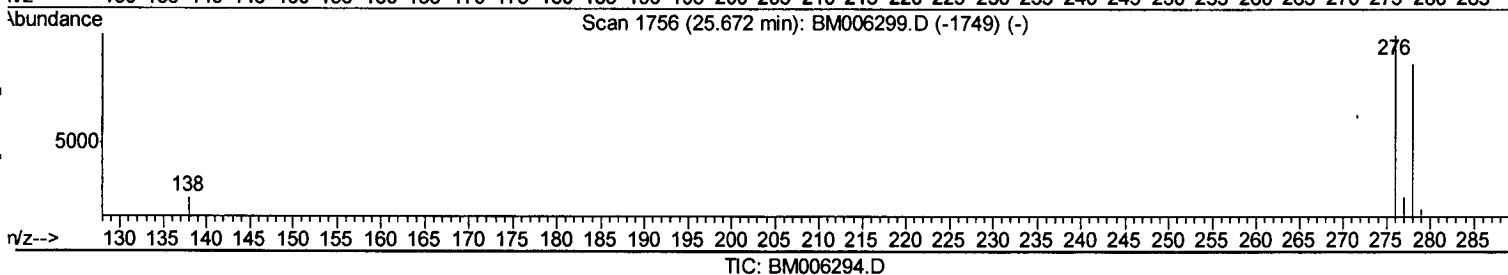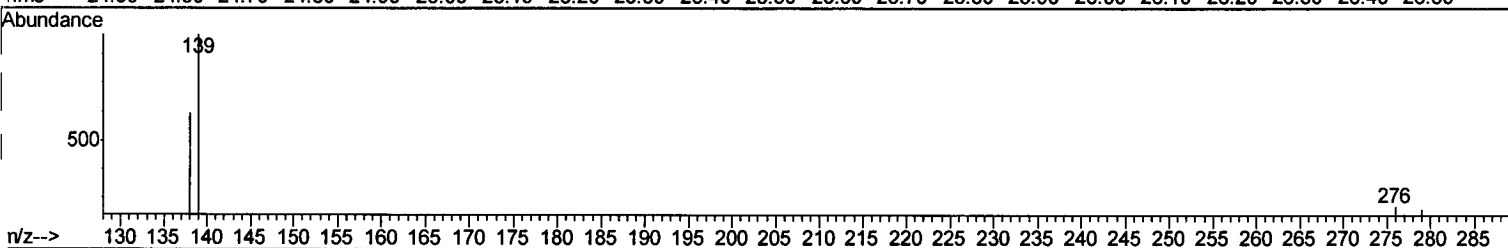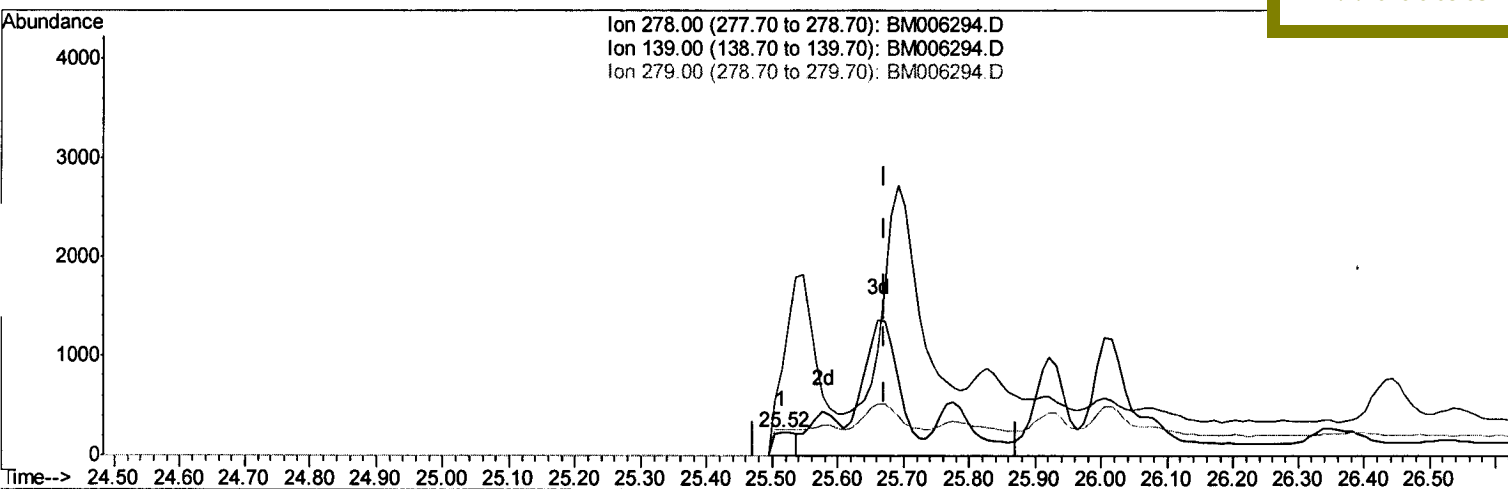

(27) Dibenzo(a,h)anthracene

25.515min (-0.156) 0.02ng/ul

response 575

Ion	Exp%	Act%
278.00	100	100
139.00	20.50	364.02#
279.00	25.20	109.21#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path: Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File: BM006294.D
 Acq On: 06 Jul 2016 22:03
 Operator: UM/SJ
 Sample: H3811-08MSD
 Misc:
 ALS Vial: 16 Sample Multiplier: 1

Instrument:
 BNA_M
 Client Sample ID:
 A4TV6MSD

Manual Integration

Quant Time: Jul 07 11:17:51 2016
 Quant Method: Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title: ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update: Thu Jul 07 05:51:09 2016
 Response via: Initial Calibration

APPROVED
 umangi
 7/7/2016 6:05:03 PM

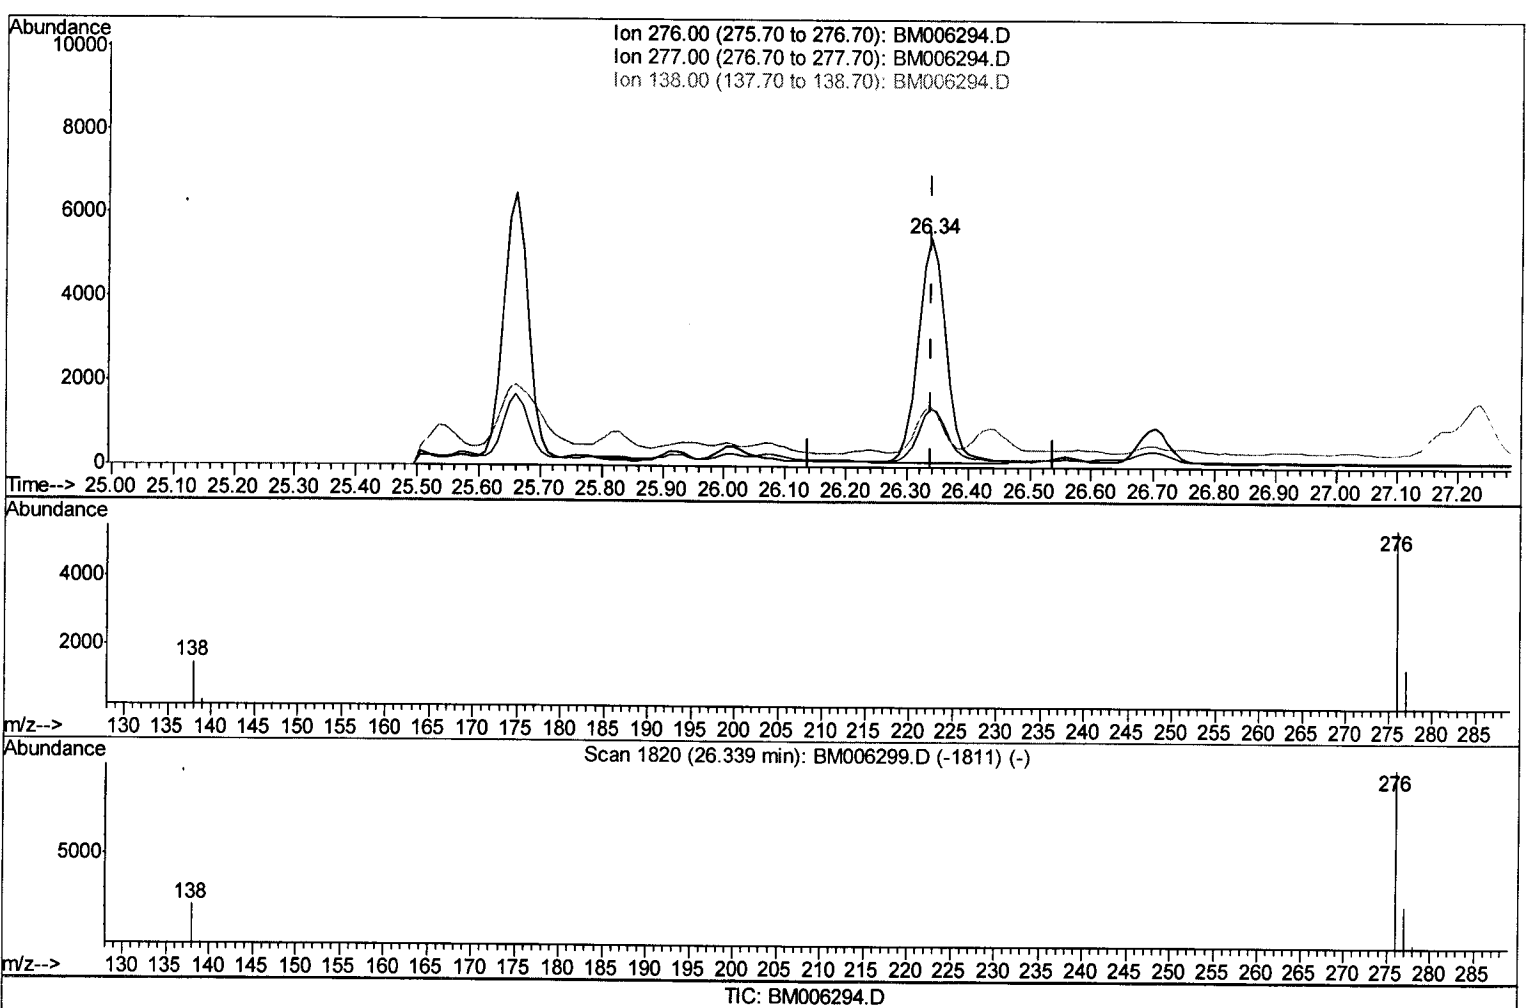

(28) Benzo(g,h,i)perylene

26.339min (+0.000) 0.48ng/ul m U.M

response 16946

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	25.45
138.00	28.10	26.51
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
Data File : BM006294.D
Acq On : 06 Jul 2016 22:03
Operator : UM/SJ
Sample : H3811-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4TV6MSD

Manual Integration

umangi
7/7/2016 6:05:03 PM

Quant Time: Jul 07 11:17:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 07 05:51:09 2016
Response via : Initial Calibration

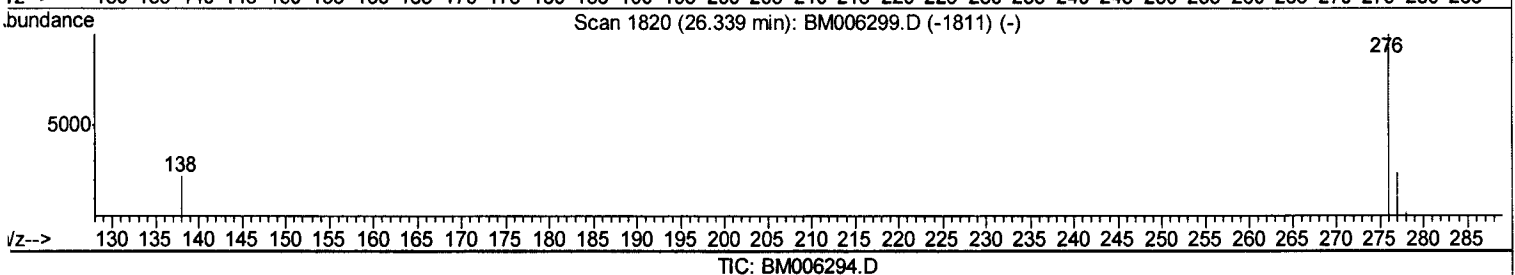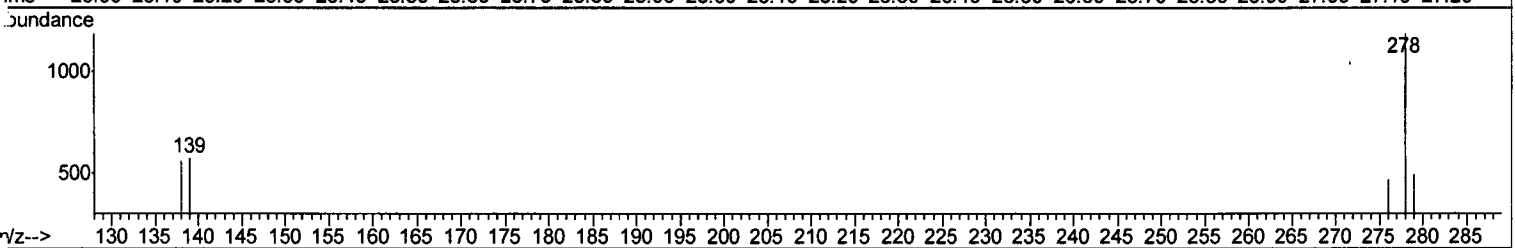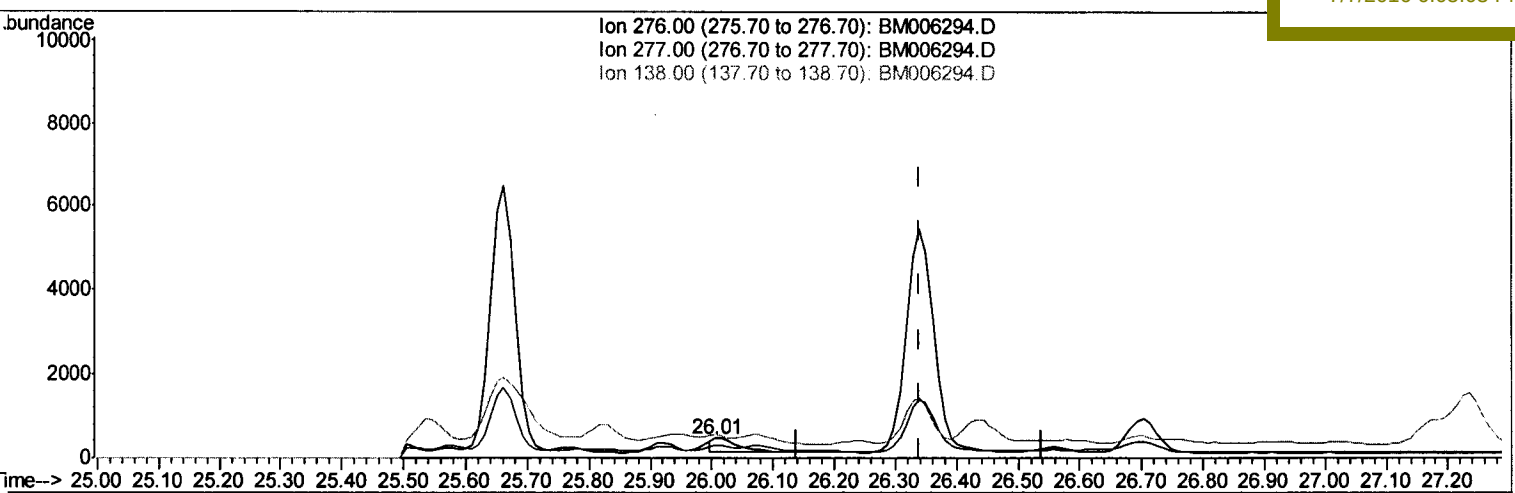

(28) Benzo(g,h,i)perylene

26.005min (-0.334) 0.03ng/ul

response 921

Ion	Exp%	Act%
276.00	100	100
277.00	23.60	63.48#
138.00	28.10	118.90#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM070716\
 Data File : BM006294.D
 Acq On : 06 Jul 2016 22:03
 Operator : UM/SJ
 Sample : H3811-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 A4TV6MSD

Quant Time: Jul 07 11:20:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 07 05:51:09 2016
 Response via : Initial Calibration

Manual Integration

umangi
 7/7/2016 6:05:03 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	4645	0.40	ng/ul	0.00
4) Naphthalene-d8	10.43	136	17845	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	9643	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.04	188	19043m	0.40	ng/ul	0.00
18) Chrysene-d12	21.24	240	12703	0.40	ng/ul	0.00
22) Perylene-d12	23.45	264	11257m	0.40	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	7316	3.73	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.02	152	6438	0.31	ng/ul	0.00
16) Fluoranthene-d10	19.07	212	10894	0.27	ng/ul	-0.01

Target Compounds

						Qvalue
5) Naphthalene	10.48	128	1356	0.03	ng/ul#	78
7) 2-Methylnaphthalene	12.09	142	719	0.03	ng/ul	100
9) Acenaphthylene	14.01	152	2963	0.09	ng/ul#	94
10) Acenaphthene	14.35	153	8762	0.27	ng/ul	88
11) Fluorene	15.34	166	1474	0.04	ng/ul#	79
13) Pentachlorophenol	16.70	266	1420	0.48	ng/ul	94
14) Phenanthrene	17.07	178	33914m	0.64	ng/ul	94
15) Anthracene	17.16	178	6061	0.12	ng/ul#	85
17) Fluoranthene	19.11	202	64096	1.10	ng/ul	94
19) Pyrene	19.47	202	69312	1.30	ng/ul	96
20) Benzo(a)anthracene	21.22	228	22315	0.54	ng/ul#	92
21) Chrysene	21.27	228	26234	0.65	ng/ul	95
23) Benzo(b)fluoranthene	22.78	252	35976m	0.89	ng/ul	
24) Benzo(k)fluoranthene	22.82	252	7891m	0.21	ng/ul	
25) Benzo(a)pyrene	23.35	252	25361m	0.68	ng/ul	
26) Indeno(1,2,3-cd)pyrene	25.66	276	18118m	0.44	ng/ul	
27) Dibenzo(a,h)anthracene	25.66	278	4738m	0.15	ng/ul	
28) Benzo(g,h,i)perylene	26.34	276	16946m	0.48	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed