



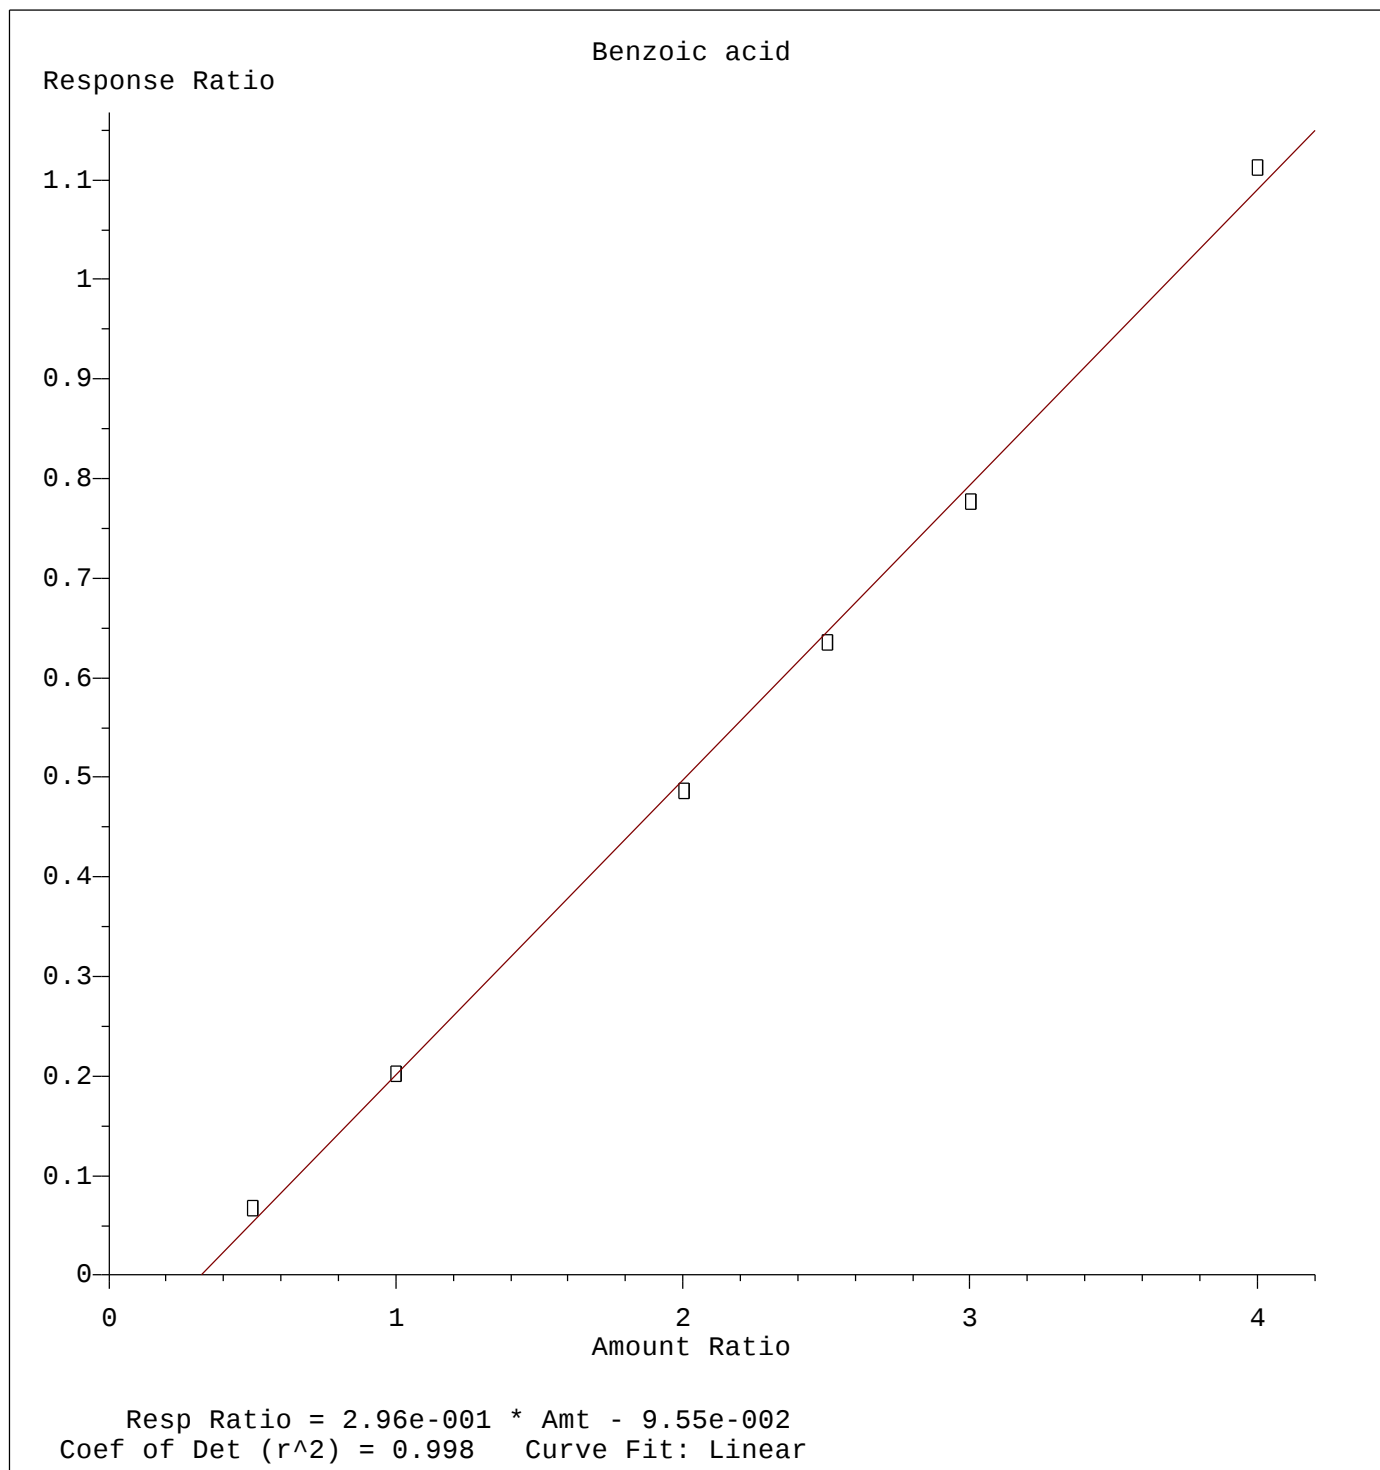

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070720.M
Calibration Table Last Updated: Mon Jul 06 18:41:39 2020

Hexachlorocyclopentadiene

Response Ratio

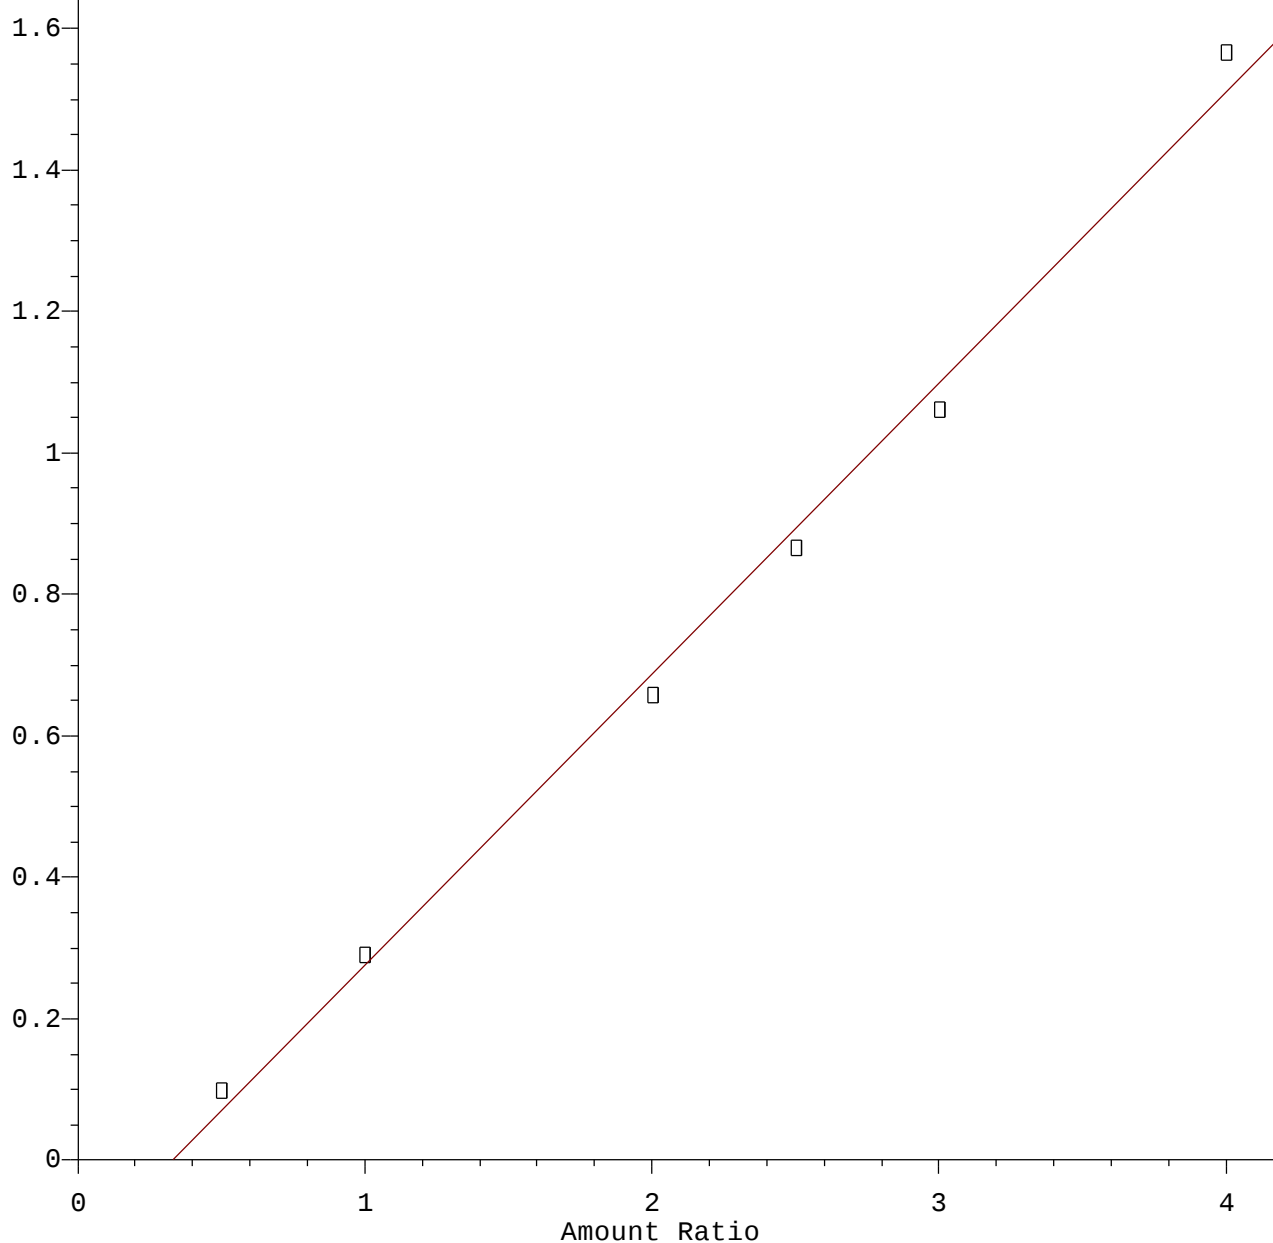


Resp Ratio = $4.12 \times 10^{-1} \times \text{Amt} - 1.36 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070720.M
Calibration Table Last Updated: Mon Jul 06 18:41:39 2020

2,4-Dinitrophenol

Response Ratio

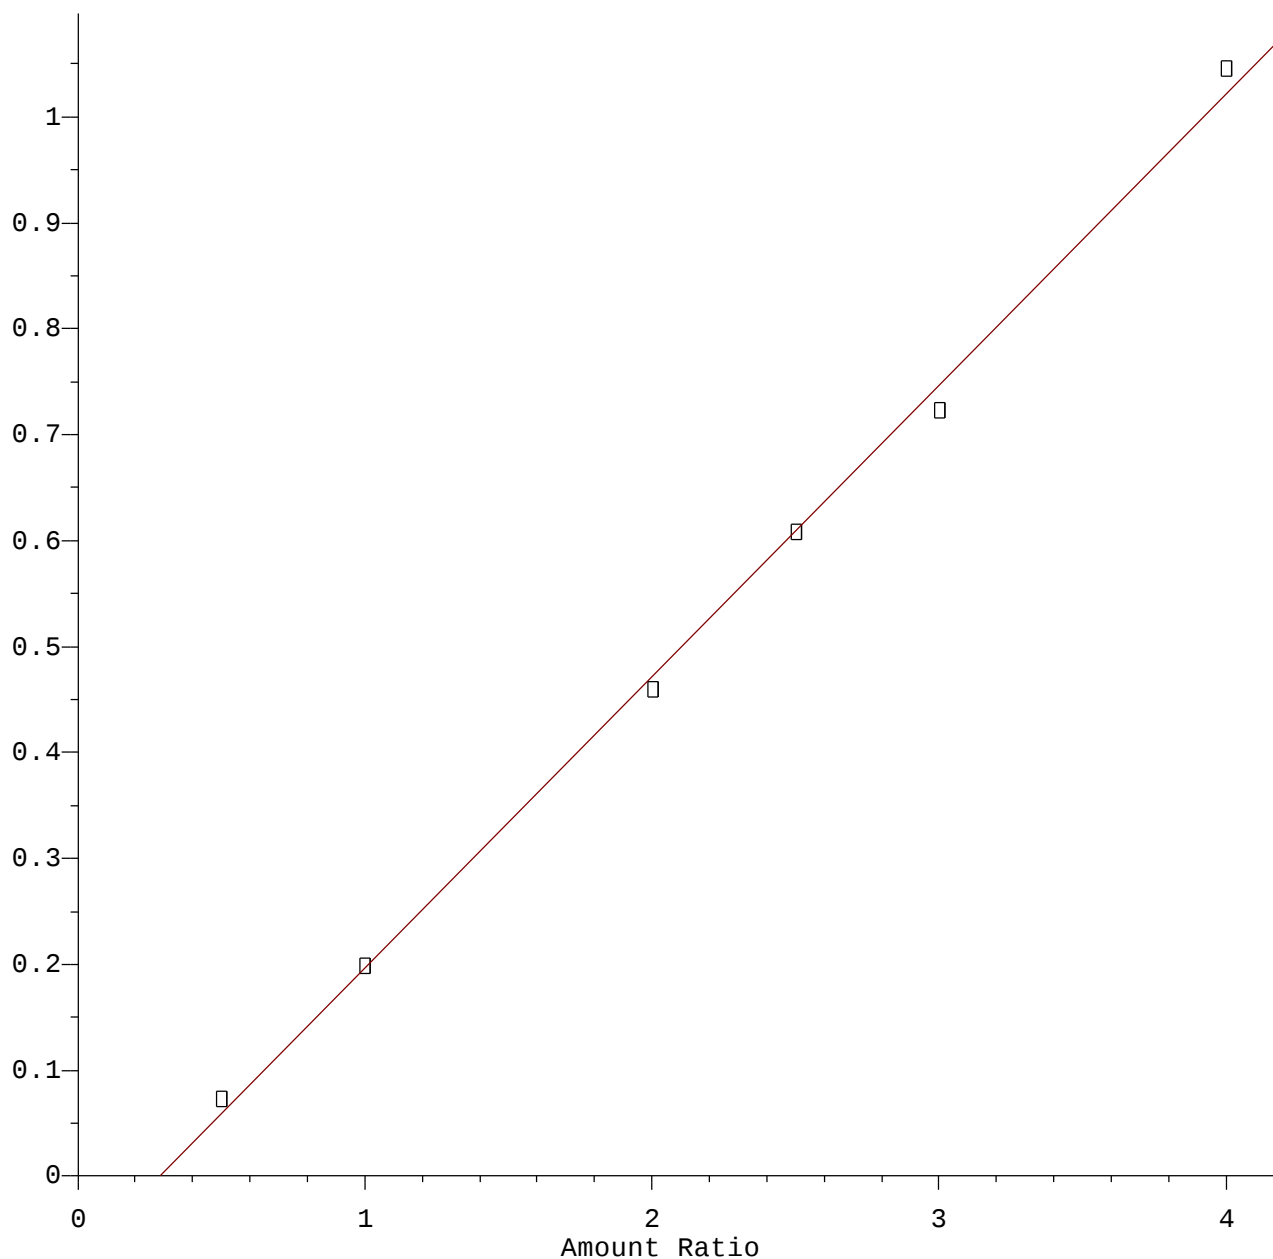


Resp Ratio = $2.75 \times 10^{-1} \times \text{Amt} - 7.88 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070720.M
Calibration Table Last Updated: Mon Jul 06 18:41:39 2020

4-Nitroaniline

Response Ratio

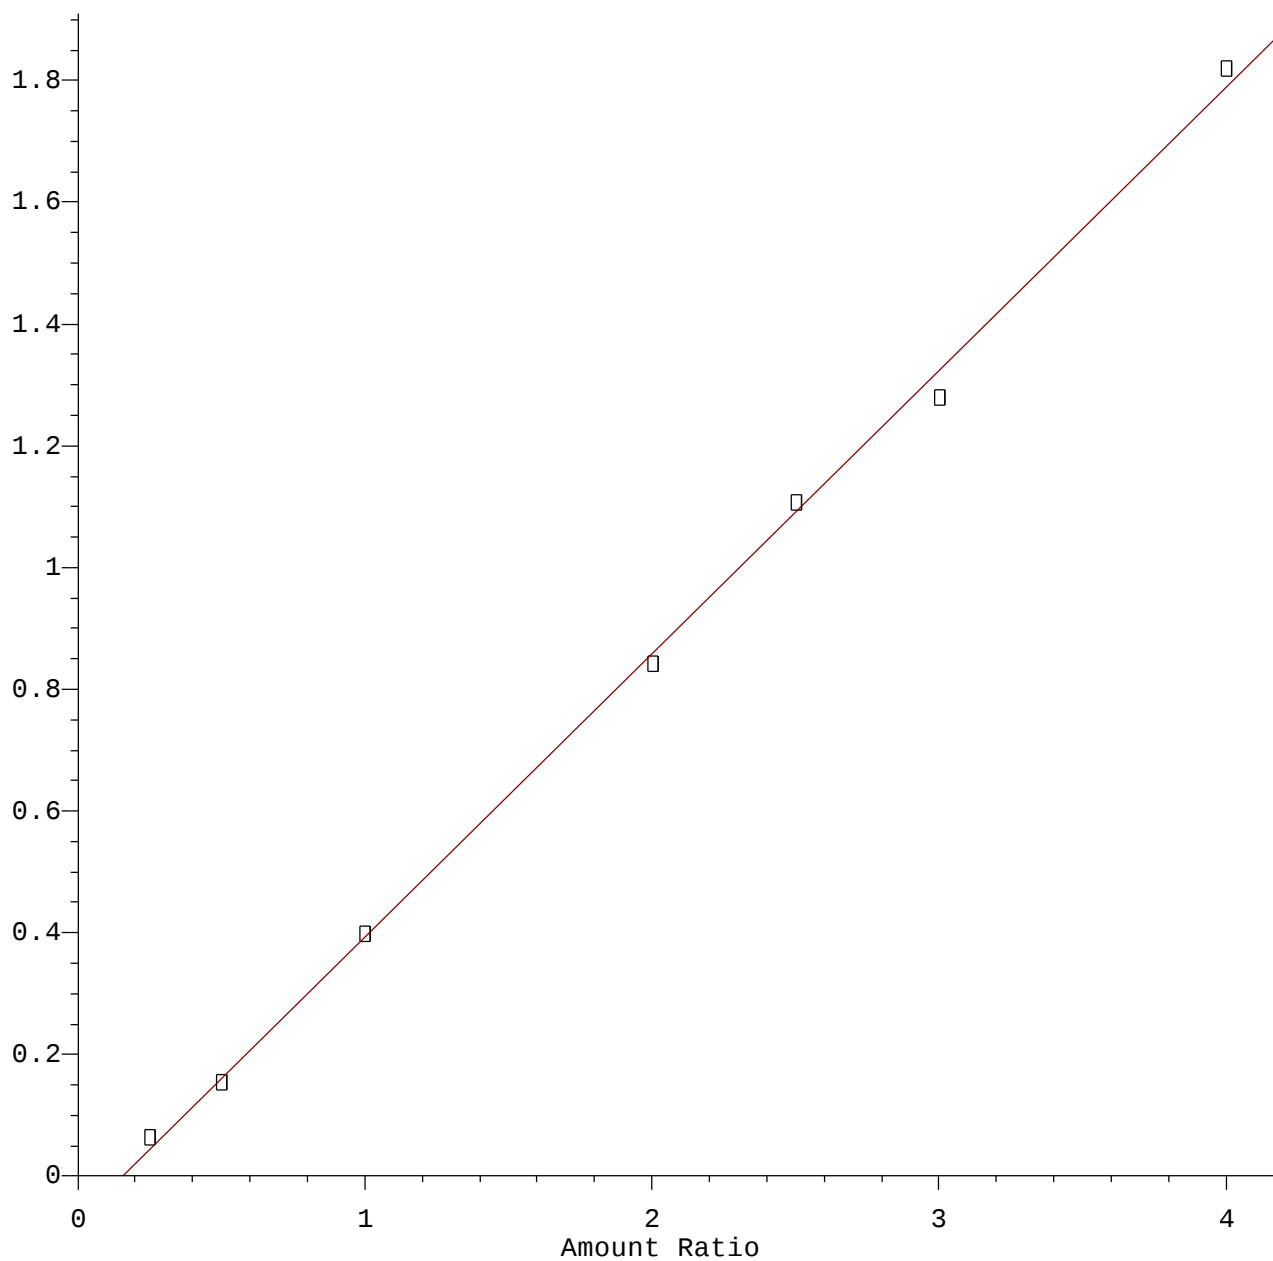

Resp Ratio = $4.65 \times 10^{-1} \times \text{Amt} - 7.16 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070720.M
Calibration Table Last Updated: Mon Jul 06 18:41:39 2020