


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM070720\
Data File : BM026661.D
Acq On : 06 Jul 2020 11:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM070720.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 06 18:41:39 2020

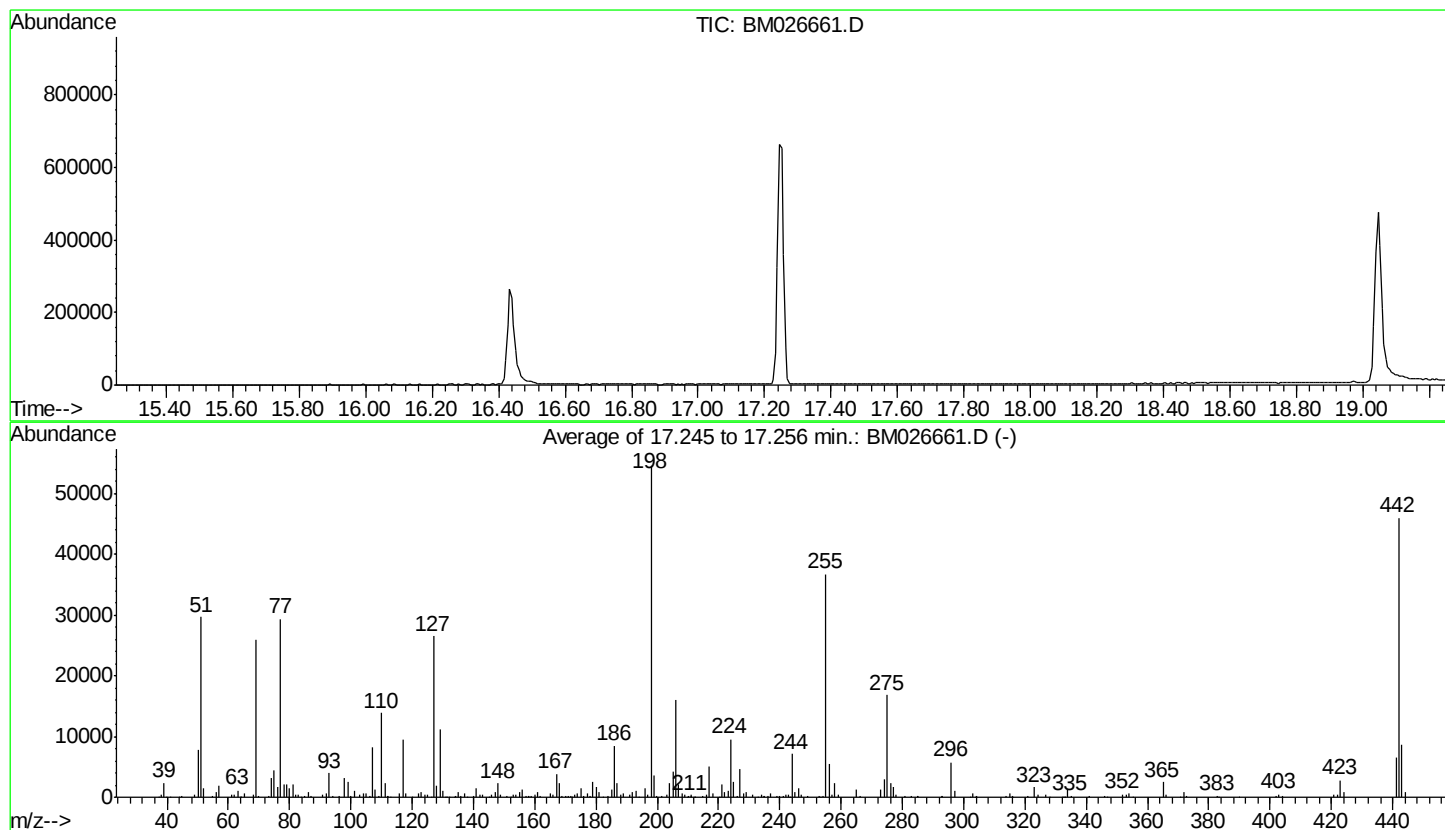

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	29616	PASS
68	69	0.00	2	1.9	502	PASS
69	198	0.00	100	47.5	25947	PASS
70	69	0.00	2	0.6	145	PASS
127	198	10	80	48.6	26519	PASS
197	198	0.00	2	0.7	367	PASS
198	198	100	100	100.0	54584	PASS
199	198	5	9	6.7	3633	PASS
275	198	10	60	30.8	16819	PASS
365	198	1	100	4.5	2466	PASS
441	198	0.01	100	12.0	6572	PASS
442	198	50	100	84.2	45954	PASS
443	442	15	24	19.0	8710	PASS