
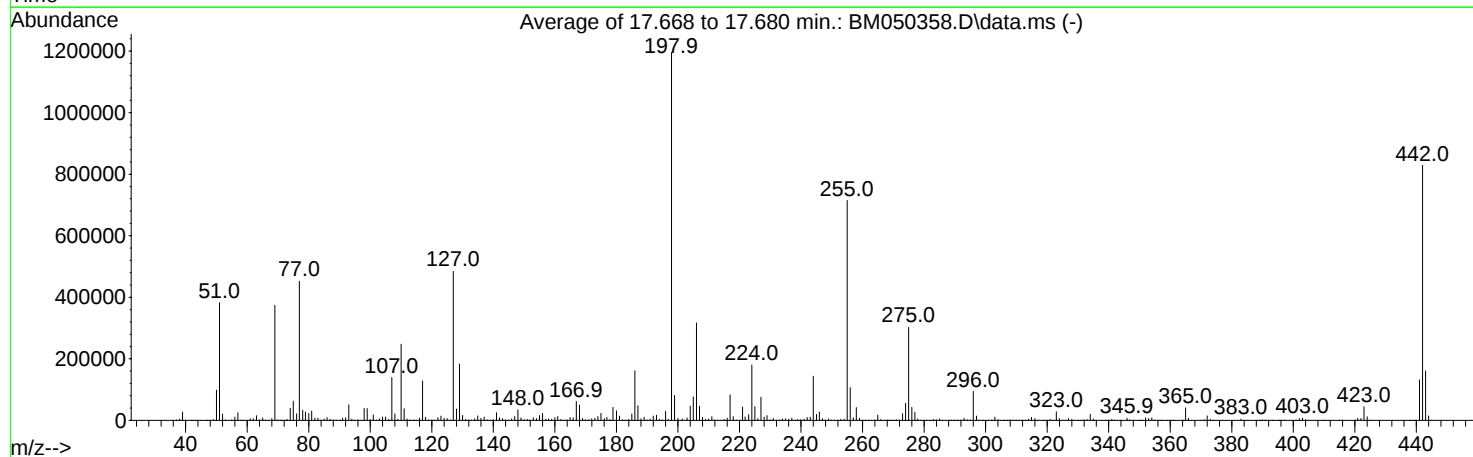


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM070725\
Data File : BM050358.D
Acq On : 07 Jul 2025 10:01
Operator : RC/JU
Sample : DFTPP092
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP092

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM070325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 03 12:56:29 2025

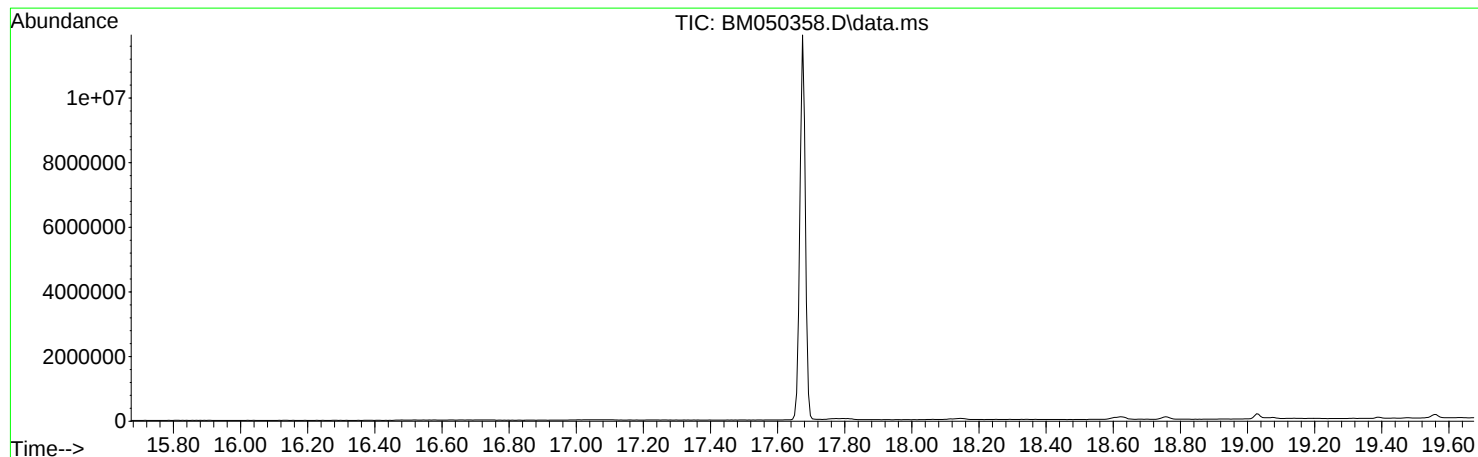

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	382238	PASS
68	69	0.00	2	1.5	5654	PASS
69	198	0.00	100	31.3	374090	PASS
70	69	0.00	2	0.6	2293	PASS
127	198	10	80	40.5	484203	PASS
197	198	0.00	2	0.3	3694	PASS
198	198	100	100	100.0	1195563	PASS
199	198	5	9	6.8	80923	PASS
275	198	10	60	25.3	302165	PASS
365	198	1	100	3.4	40523	PASS
441	198	0.01	100	11.0	131645	PASS
442	198	50	100	69.3	828907	PASS
443	442	15	24	19.4	160616	PASS