


Data Path : Z:\HPCHEM1\BNA_M\Data\BM070815\
 Data File : BM001878.D
 Acq On : 08 Jul 2015 11:46
 Operator : TP/UM
 Sample : DFTPP69
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP69

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041515.M
 Title : SVOA CALIBRATION
 Last Update : Wed Apr 15 18:00:48 2015

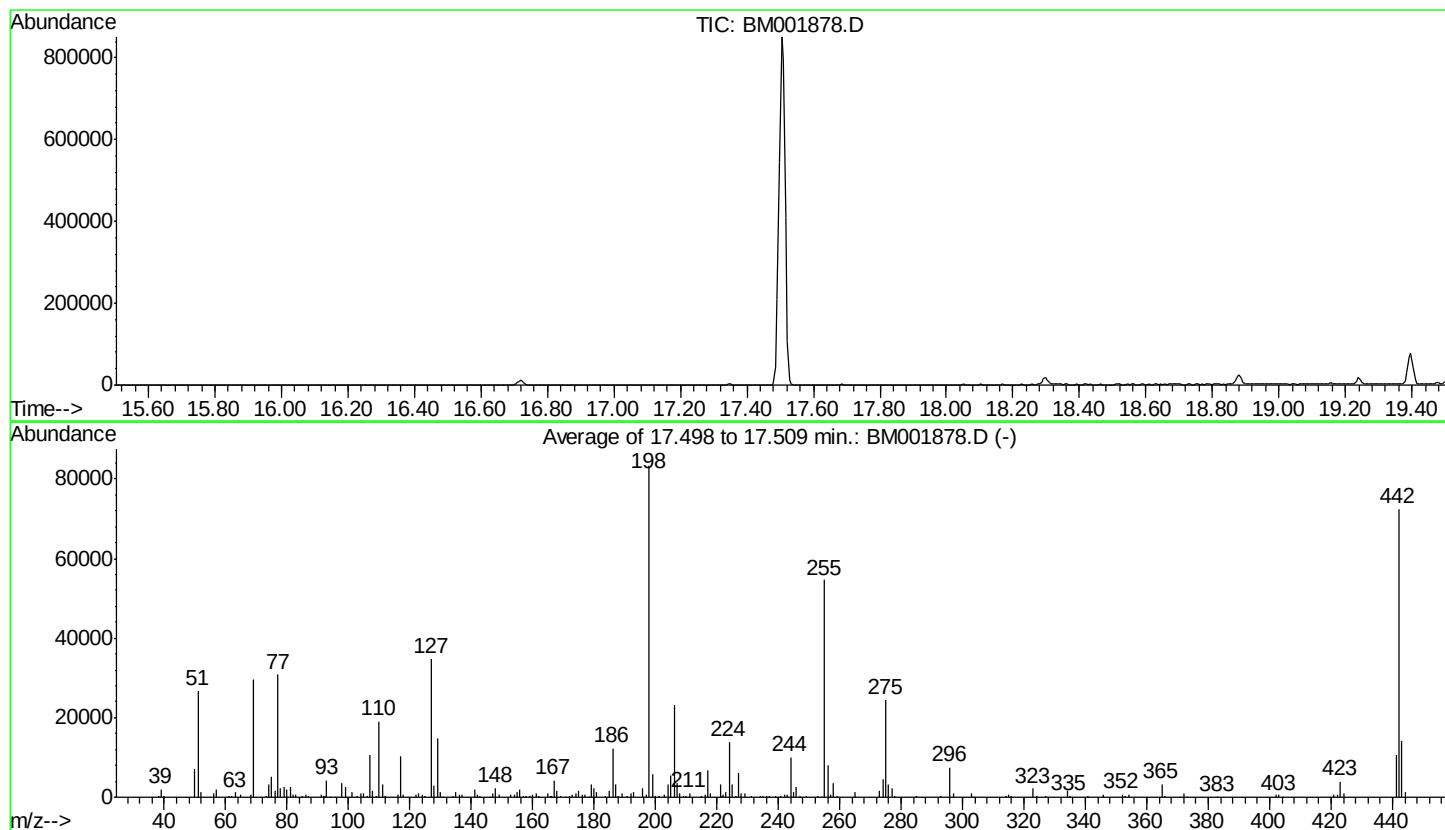

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	26717	PASS
68	69	0.00	2	1.8	538	PASS
69	198	0.00	100	35.7	29741	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	34872	PASS
197	198	0.00	2	0.9	723	PASS
198	198	100	100	100.0	83357	PASS
199	198	5	9	6.8	5670	PASS
275	198	10	60	29.5	24618	PASS
365	198	1	100	3.9	3261	PASS
441	443	0.01	100	75.4	10751	PASS
442	198	50	100	86.9	72410	PASS
443	442	15	24	19.7	14251	PASS

m/z	Abundance
38.00	385.0
39.00	1740.0
40.00	487.0
43.90	793.0
50.10	6498.0
51.10	23848.0
52.00	1325.0
56.00	735.0
57.00	1516.0
61.90	360.0
63.00	1108.0
64.90	512.0
68.00	507.0
69.00	26056.0
73.00	387.0
74.10	2707.0
75.00	4225.0
76.10	1316.0
77.00	26464.0
78.00	1740.0
79.00	1924.0
79.90	1615.0
81.00	2250.0
82.00	574.0
83.00	617.0
85.00	317.0
86.00	610.0
90.90	504.0
91.90	506.0
93.00	3414.0
98.00	3338.0
99.00	2220.0
100.90	1026.0
102.90	384.0
104.10	739.0
105.00	842.0
106.00	393.0
107.00	8837.0
108.00	1118.0
108.90	321.0
110.00	15483.0
111.00	2888.0
115.90	446.0
117.00	9022.0
117.90	490.0
121.90	589.0
122.90	1025.0
124.00	428.0
124.90	319.0
127.00	28304.0
128.00	2270.0
129.00	12104.0
130.00	1162.0
130.90	331.0
134.00	393.0
135.00	926.0
136.00	364.0
137.10	486.0
141.00	1761.0
141.90	598.0
142.90	342.0
147.00	842.0
147.90	2080.0
149.00	319.0
152.90	563.0
154.00	452.0
155.00	1092.0
156.00	1476.0
157.00	377.0
158.00	340.0
160.00	502.0
161.00	858.0
164.90	513.0
165.90	473.0
167.00	3315.0
168.10	1352.0
173.00	469.0
174.00	778.0
175.00	1228.0
176.00	348.0
176.90	532.0
178.90	2451.0
180.00	1638.0
181.00	982.0
185.00	1136.0
186.00	9502.0
187.10	2663.0
187.90	313.0
188.90	803.0
192.00	793.0
193.00	744.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

196.00	1753.0
197.10	516.0
198.00	63872.0
198.90	4082.0
203.10	438.0
204.00	2410.0
205.00	3930.0
206.00	17832.0
207.00	2925.0
208.00	657.0
211.10	830.0
216.00	322.0
217.00	5015.0
217.90	505.0
221.00	2218.0
222.00	655.0
222.90	1179.0
224.00	10740.0
225.00	2557.0
227.00	4848.0
228.00	626.0
228.90	800.0
231.00	422.0
234.00	352.0
241.80	360.0
243.00	611.0
244.00	7660.0
245.00	1117.0
245.90	1546.0
247.00	309.0
255.00	38584.0
256.00	6178.0
257.00	455.0
258.00	2391.0
265.00	1160.0
273.00	1374.0
274.00	2954.0
275.00	16816.0
276.00	2286.0
277.10	1501.0
296.00	5608.0
297.00	832.0
303.00	636.0
315.00	501.0
315.90	354.0
323.00	1349.0
327.00	399.0
334.00	928.0
345.90	307.0
352.00	520.0
354.10	553.0
364.90	1877.0
372.10	677.0
402.00	387.0
421.10	367.0
422.00	421.0
423.10	2387.0
424.00	488.0
441.10	5843.0
442.10	42176.0
443.10	8944.0
444.00	1329.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

m/z	Abundance
38.00	494.0
39.00	2558.0
40.00	363.0
44.00	811.0
50.10	8342.0
51.10	31400.0
52.10	1743.0
56.00	949.0
57.00	2133.0
60.90	476.0
62.00	498.0
63.10	1486.0
65.00	634.0
68.00	549.0
69.00	34904.0
73.00	475.0
74.00	3741.0
75.00	5970.0
76.10	1780.0
77.10	36944.0
78.00	2539.0
79.00	3428.0
80.00	2090.0
81.00	2810.0
81.90	859.0
82.90	790.0
85.00	469.0
86.00	855.0
86.90	475.0
91.00	714.0
92.20	695.0
93.00	4922.0
94.00	410.0
95.90	370.0
98.00	3906.0
99.00	2743.0
101.00	1578.0
103.00	584.0
104.00	1405.0
105.00	1214.0
105.90	345.0
107.00	12277.0
108.00	2076.0
109.00	533.0
110.00	22528.0
111.00	3687.0
112.00	558.0
116.00	670.0
117.00	11848.0
118.00	920.0
121.90	874.0
122.90	1200.0
123.90	601.0
124.90	510.0
127.00	41560.0
128.00	3195.0
129.00	17616.0
129.90	1609.0
134.00	509.0
134.90	1308.0
135.90	668.0
137.00	657.0
141.00	2508.0
141.80	663.0
142.90	555.0
146.00	452.0
146.90	1191.0
148.00	2790.0
148.90	522.0
153.00	904.0
153.90	643.0
155.00	1242.0
155.90	2442.0
157.10	321.0
157.80	416.0
159.00	454.0
159.90	792.0
161.00	1246.0
162.00	377.0
165.00	1017.0
166.10	857.0
167.00	4891.0
168.00	2097.0
169.10	383.0
170.90	355.0
172.00	668.0
173.00	583.0
173.90	1057.0
175.00	2114.0
176.00	498.0
176.90	834.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

179.00	3982.0
180.00	2775.0
181.00	1175.0
183.80	405.0
185.00	1854.0
186.00	14954.0
187.00	3960.0
188.00	370.0
188.90	1081.0
191.00	523.0
192.00	1284.0
193.00	1491.0
195.90	2921.0
197.00	820.0
198.00	96496.0
199.00	6652.0
199.80	513.0
201.30	404.0
203.00	823.0
204.00	3577.0
205.00	7115.0
206.00	27784.0
207.00	4003.0
207.90	1098.0
209.00	345.0
210.10	460.0
210.90	1081.0
214.90	361.0
216.00	760.0
217.00	7801.0
217.90	988.0
221.00	3732.0
221.70	1209.0
223.00	1677.0
224.00	16069.0
225.10	3488.0
226.00	429.0
227.00	6966.0
227.90	1006.0
228.90	1322.0
231.00	335.0
233.90	587.0
235.00	622.0
236.00	321.0
237.00	431.0
238.90	321.0
240.90	398.0
241.90	922.0
243.00	976.0
244.00	11143.0
245.00	1316.0
246.00	3025.0
246.90	577.0
248.90	359.0
252.90	331.0
255.00	62624.0
256.00	9231.0
257.10	522.0
258.00	3924.0
259.00	614.0
265.00	1699.0
272.90	1666.0
274.00	5282.0
275.00	29264.0
276.00	3785.0
277.00	2982.0
278.00	360.0
285.00	363.0
292.90	656.0
296.00	8551.0
297.00	1251.0
303.00	1073.0
314.00	431.0
315.00	906.0
315.90	474.0
323.00	2474.0
324.00	572.0
326.90	534.0
334.00	1914.0
335.00	543.0
341.00	416.0
346.00	603.0
352.00	669.0
353.00	668.0
354.10	604.0
365.00	3656.0
366.00	521.0
371.00	320.0
372.10	1399.0
401.90	488.0
403.00	768.0
421.00	541.0
422.00	635.0
423.10	4318.0
424.10	1116.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

441.10	11636.0
442.10	80744.0
443.10	15435.0
444.10	1539.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

m/z	Abundance
39.00	1874.0
40.00	408.0
44.00	801.0
50.00	6692.0
51.00	24904.0
52.00	1255.0
56.00	873.0
57.00	1740.0
61.00	400.0
62.00	346.0
63.00	954.0
65.10	481.0
68.10	558.0
69.00	28264.0
73.00	308.0
74.00	3192.0
75.00	4917.0
76.00	1455.0
77.00	29200.0
78.00	2060.0
79.00	2411.0
80.00	2052.0
81.00	2490.0
81.90	646.0
83.00	544.0
85.00	477.0
86.00	682.0
86.80	342.0
91.00	612.0
91.90	617.0
93.00	4478.0
98.00	3433.0
99.00	2395.0
101.00	1373.0
103.00	447.0
103.90	1110.0
105.00	888.0
106.00	319.0
107.00	10830.0
108.00	1800.0
109.10	366.0
110.00	19048.0
111.00	2686.0
111.90	383.0
115.90	605.0
117.00	10221.0
117.90	580.0
121.90	857.0
122.90	1145.0
123.80	487.0
124.90	485.0
127.00	34752.0
128.00	2833.0
129.00	15146.0
130.00	1418.0
134.10	583.0
135.00	1271.0
136.00	615.0
137.00	617.0
141.00	2024.0
142.00	547.0
143.00	419.0
147.00	1310.0
147.90	2138.0
149.00	785.0
153.10	656.0
154.10	471.0
154.90	1289.0
156.00	1924.0
157.90	530.0
159.10	400.0
160.00	725.0
161.00	901.0
161.80	317.0
165.00	1213.0
165.90	583.0
167.00	4683.0
167.90	1875.0
169.00	447.0
171.90	477.0
173.00	647.0
174.10	960.0
175.10	1474.0
176.00	669.0
176.90	975.0
178.10	323.0
179.00	3705.0
180.00	2332.0
180.90	1312.0
183.90	400.0
185.00	2054.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

186.00	12573.0
187.00	3450.0
187.90	534.0
188.90	818.0
190.80	432.0
191.90	921.0
193.00	1331.0
196.00	2445.0
197.10	833.0
197.90	89704.0
198.90	6278.0
199.90	576.0
201.30	434.0
202.90	992.0
204.00	3440.0
205.00	5822.0
206.00	23768.0
207.00	3768.0
208.00	1018.0
208.90	415.0
210.10	528.0
211.00	1135.0
214.90	335.0
216.10	490.0
216.90	7505.0
218.00	960.0
221.00	3390.0
221.90	1063.0
223.10	1293.0
224.00	14800.0
225.00	3672.0
226.00	537.0
227.00	6881.0
228.00	1143.0
229.00	1263.0
231.00	535.0
234.00	495.0
235.00	653.0
236.10	378.0
237.00	587.0
239.00	304.0
241.00	397.0
242.00	694.0
243.00	742.0
244.00	11478.0
245.00	1525.0
246.00	2708.0
247.00	436.0
249.00	482.0
253.00	310.0
254.10	458.0
255.00	62616.0
256.00	8760.0
257.10	615.0
258.00	3997.0
258.90	759.0
265.00	1442.0
273.00	1508.0
274.00	5251.0
275.00	27776.0
276.00	3695.0
277.00	2537.0
277.90	439.0
285.00	452.0
293.00	669.0
296.00	8479.0
297.00	1153.0
303.00	845.0
303.90	416.0
314.00	646.0
315.00	1011.0
316.00	397.0
323.10	2838.0
324.10	430.0
326.90	401.0
334.10	1831.0
334.90	503.0
341.00	367.0
345.90	682.0
352.00	1023.0
352.90	361.0
354.00	826.0
365.00	4252.0
366.00	628.0
372.10	1308.0
372.90	353.0
383.00	368.0
401.90	615.0
402.90	749.0
404.10	313.0
421.00	618.0
422.00	588.0
423.00	5011.0
423.90	996.0
441.10	14774.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

442.10	94312.0
443.10	18376.0
444.00	1498.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69

m/z	Abundance
44.00	963.0

Instrument :
BNA_M
ClientSampleId :
DFTPP69