

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070816\
 Data File : BM006313.D
 Acq On : 07 Jul 2016 11:12
 Operator : UM/SJ
 Sample : PB91937BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK37

Quant Time: Jul 08 01:32:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 01:14:08 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	3470	0.40	ng/ul	0.00
4) Naphthalene-d8	10.43	136	13288	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	7291	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.14	188	1108216	0.40	ng/ul	0.10
18) Chrysene-d12	21.24	240	13774	0.40	ng/ul	0.00
22) Perylene-d12	23.32	264	945548	0.40	ng/ul	-0.14
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.17	96	10743	7.32	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.03	152	6696	0.43	ng/ul	0.01
16) Fluoranthene-d10	19.08	212	13387	0.01	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Fluorene	15.29	166	2126	0.08	ng/ul#	22
19) Pyrene	19.44	202	1910	0.03	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070816\
Data File : BM006313.D
Acq On : 07 Jul 2016 11:12
Operator : UM/SJ
Sample : PB91937BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK37

Quant Time: Jul 08 01:32:19 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 01:14:08 2016
Response via : Initial Calibration

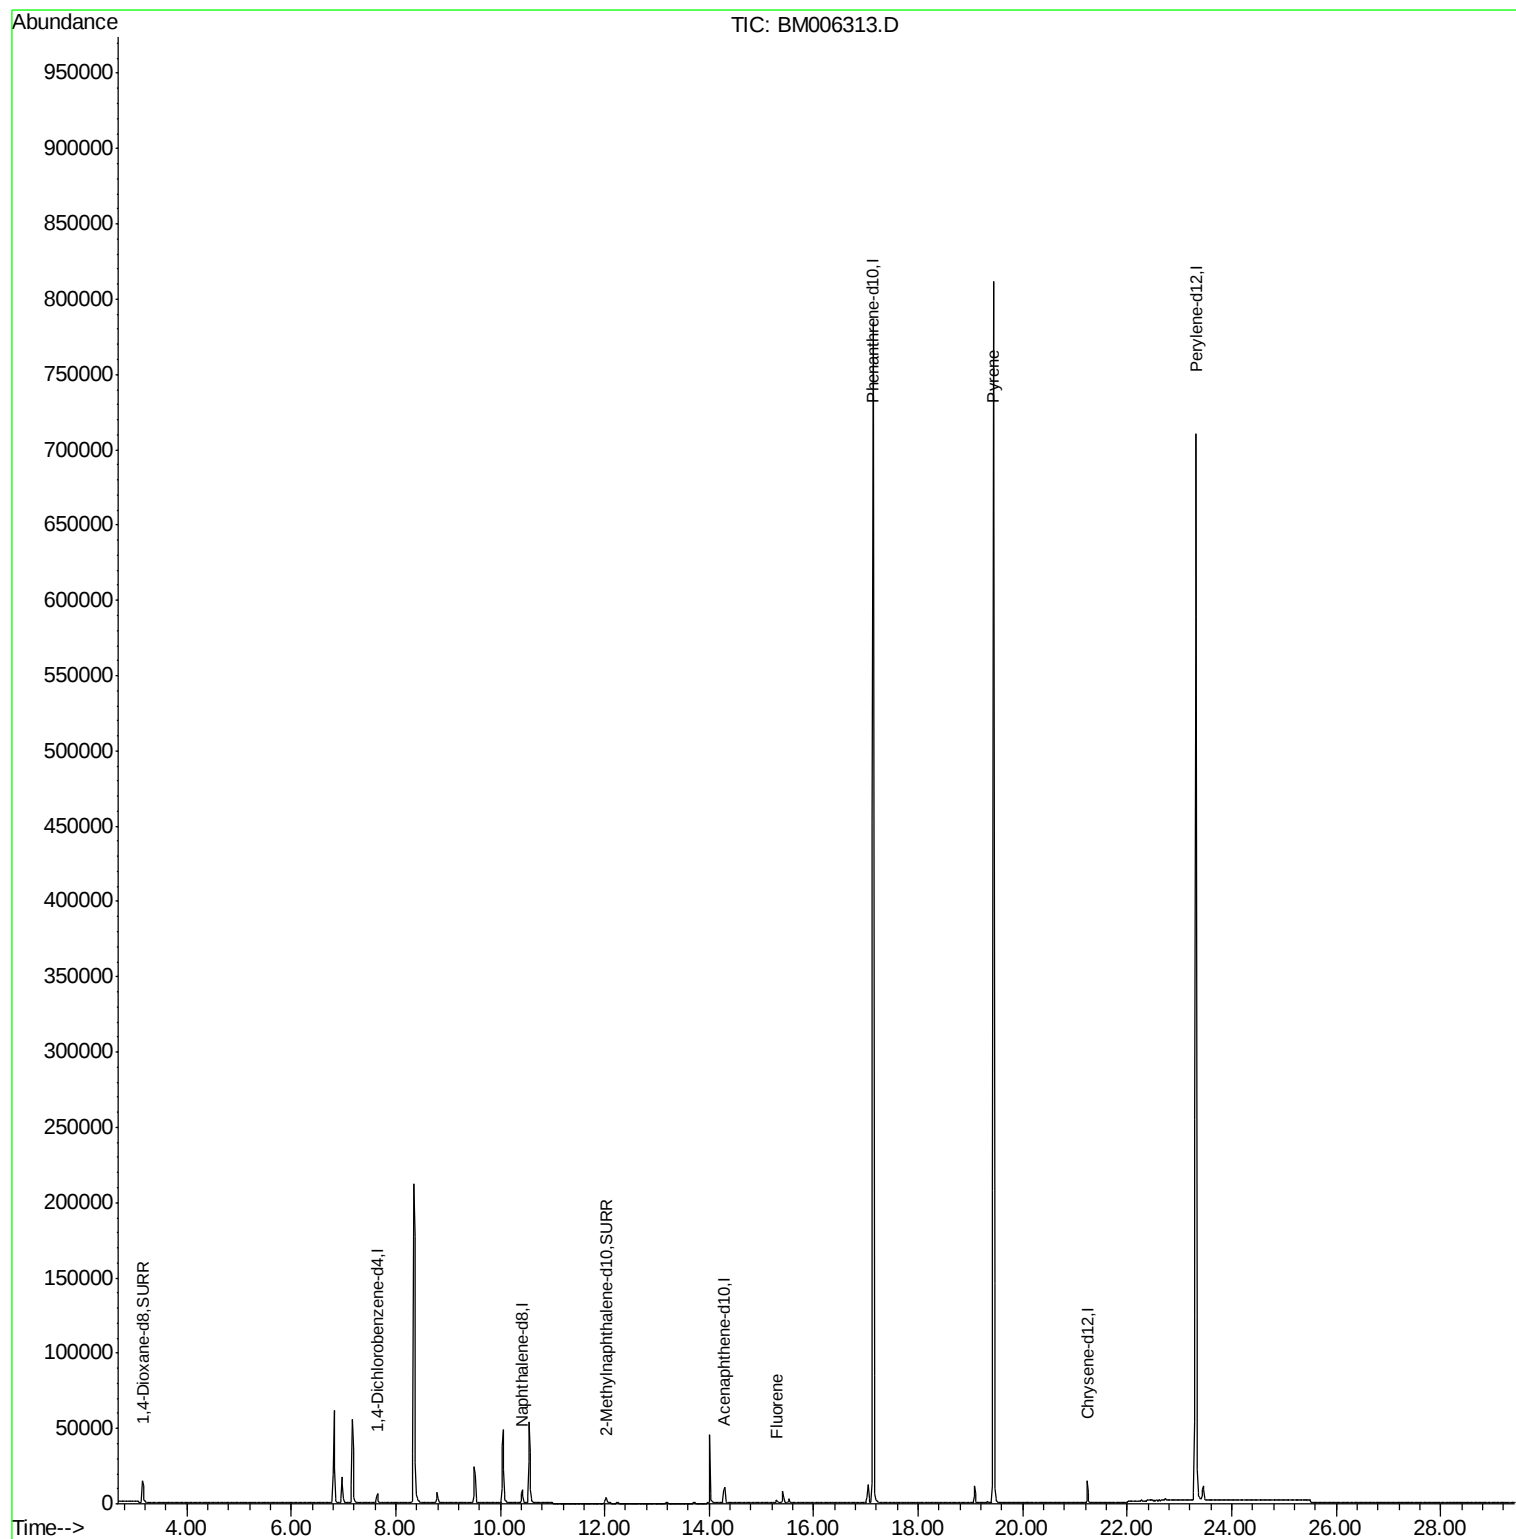

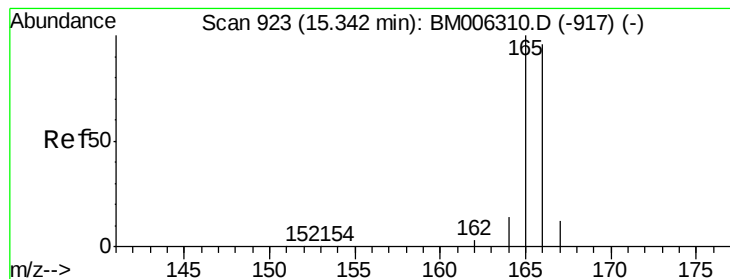

#11

Fluorene

Concen: 0.08 ng/ul

RT: 15.29 min Scan# 920

Delta R.T. -0.05 min

Lab File: BM006313.D

Acq: 07 Jul 2016 11:12

Instrument :

BNA_M

ClientSampleId :

SBLK37


Tgt Ion:166 Resp: 2126

Ion Ratio Lower Upper




166 100

165 8.5 69.6 104.4#

167 29.8 11.9 17.9#

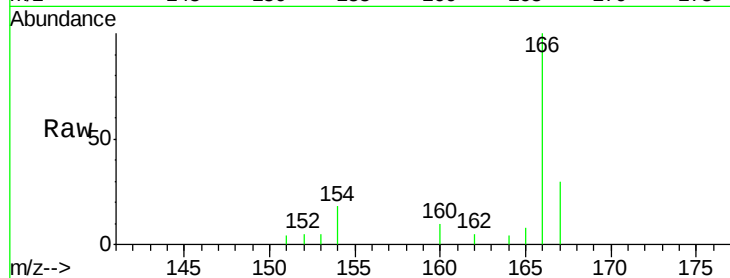

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

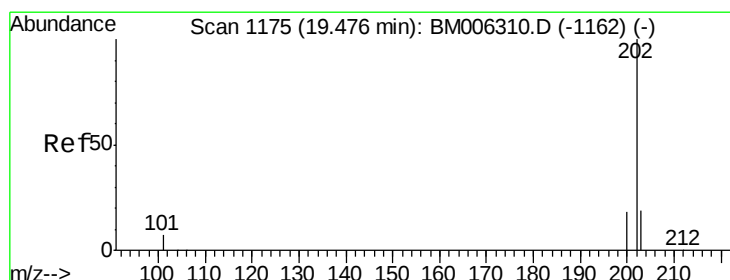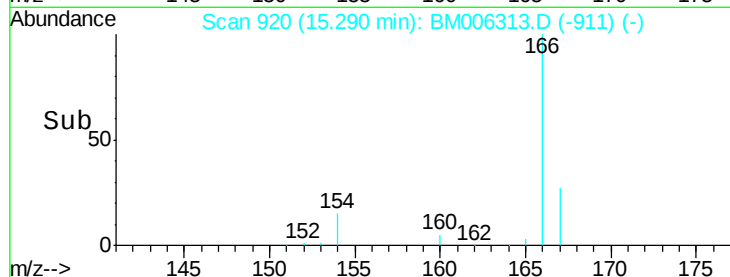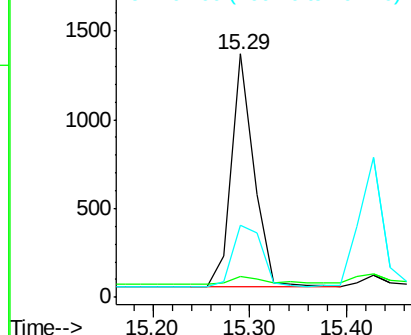

#19

Pyrene

Concen: 0.03 ng/ul

RT: 19.44 min Scan# 1172

Delta R.T. -0.04 min

Lab File: BM006313.D

Acq: 07 Jul 2016 11:12


Tgt Ion:202 Resp: 1910

Ion Ratio Lower Upper

202 100

200 8.7 17.8 26.8#

203 132.8 12.8 19.2#

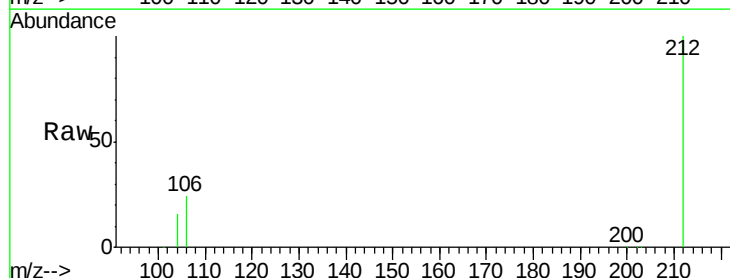

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

