

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070816\
 Data File : BM006314.D
 Acq On : 07 Jul 2016 11:49
 Operator : UM/SJ
 Sample : PB91683BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK82

Quant Time: Jul 08 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 01:14:08 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	3887	0.40	ng/ul	-0.01
4) Naphthalene-d8	10.43	136	16040	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.30	164	9442	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.14	188	1366300	0.40	ng/ul	0.10
18) Chrysene-d12	21.25	240	12704	0.40	ng/ul	0.00
22) Perylene-d12	23.32	264	896819	0.40	ng/ul	-0.13
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.16	96	9786	5.96	ng/uL	-0.01
6) 2-Methylnaphthalene-d10	12.02	152	7464	0.40	ng/ul	0.00
16) Fluoranthene-d10	19.08	212	15559	0.01	ng/ul	0.00
Target Compounds						
					Qvalue	
11) Fluorene	15.29	166	2580	0.07	ng/ul#	20
19) Pyrene	19.44	202	2149	0.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM070816\
Data File : BM006314.D
Acq On : 07 Jul 2016 11:49
Operator : UM/SJ
Sample : PB91683BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK82

Quant Time: Jul 08 01:32:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM070716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 01:14:08 2016
Response via : Initial Calibration

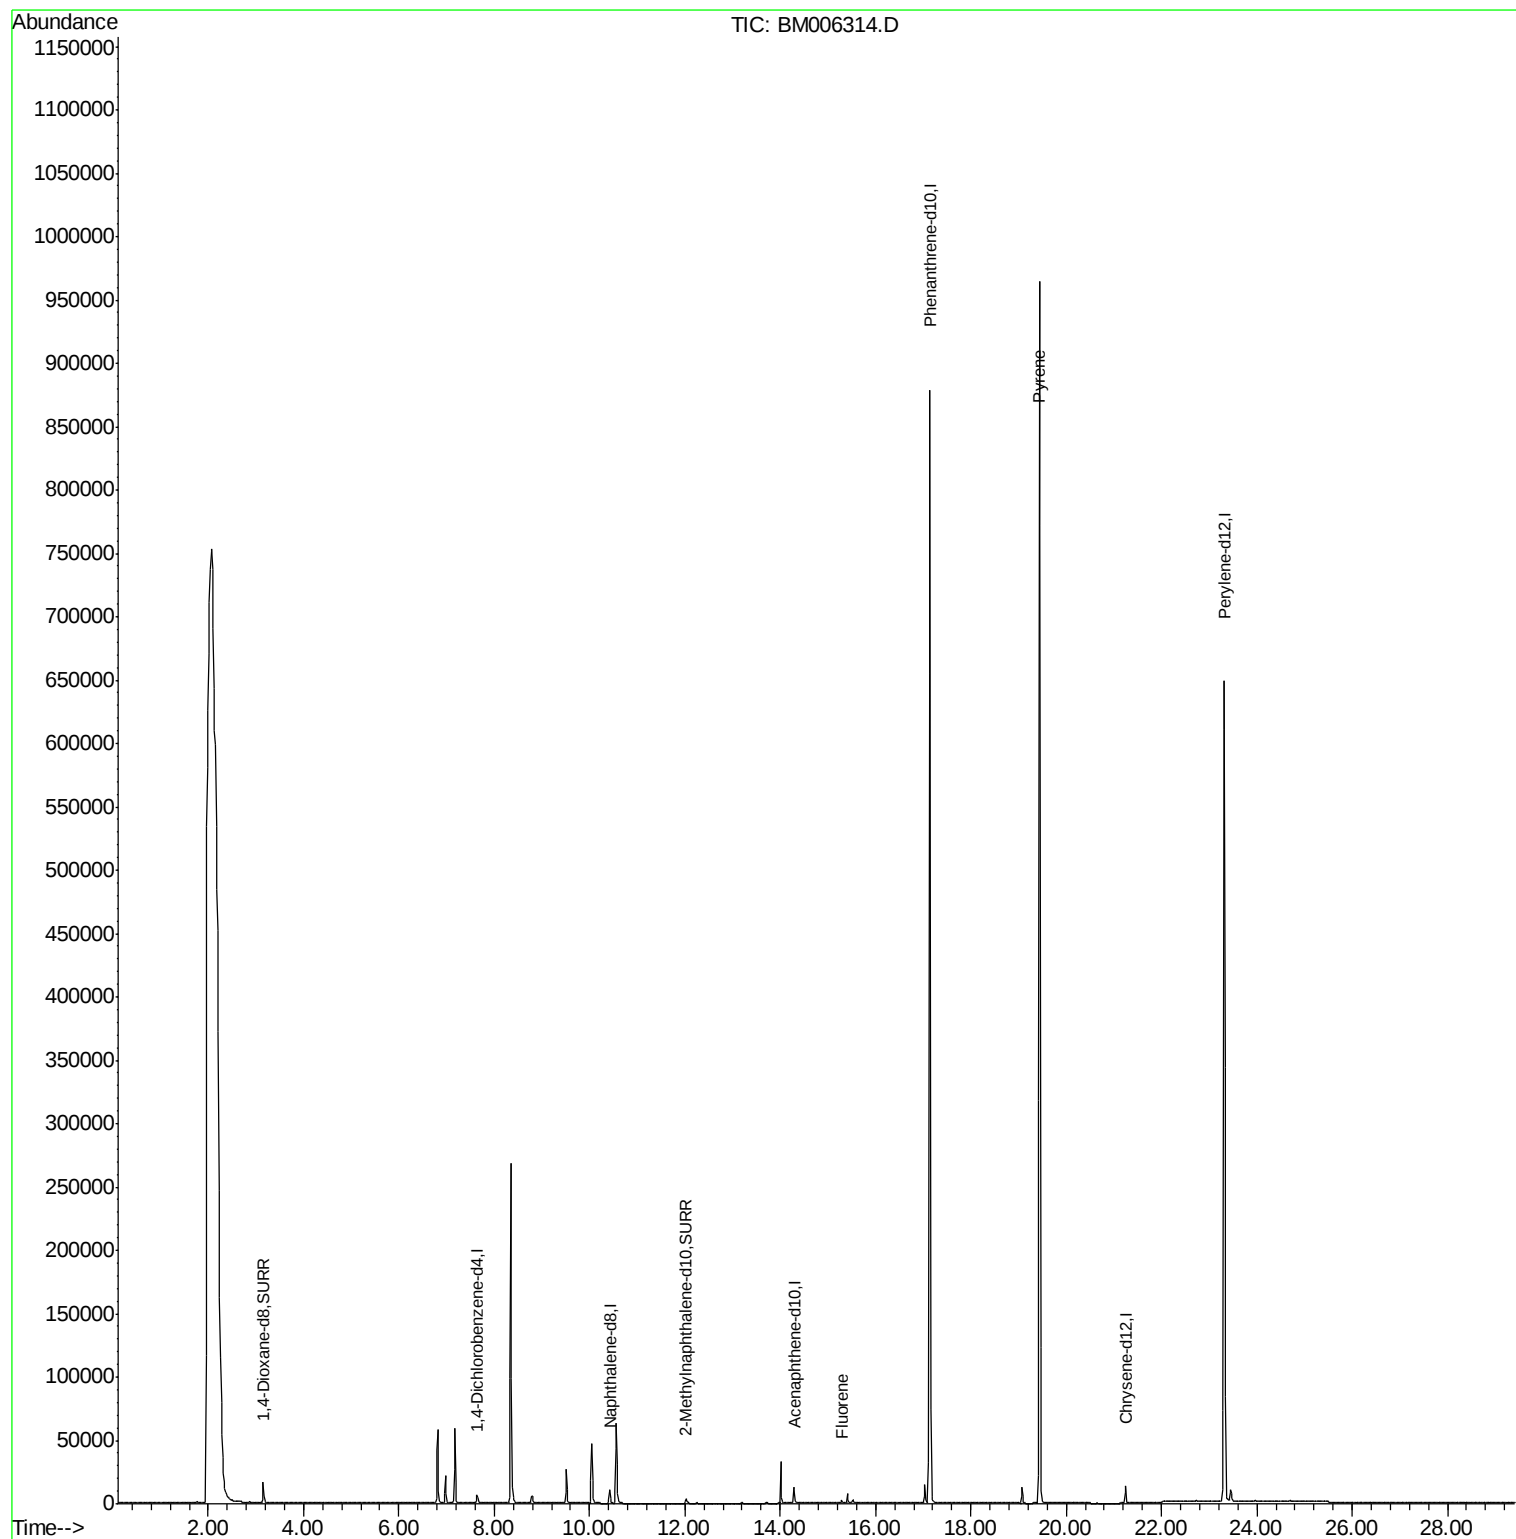

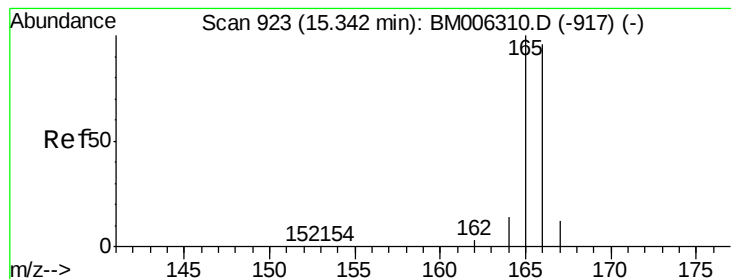

#11

Fluorene

Concen: 0.07 ng/ul

RT: 15.29 min Scan# 1087

Delta R.T. -0.05 min

Lab File: BM006314.D

Acq: 07 Jul 2016 11:49

Instrument :

BNA_M

ClientSampleId :

SBLK82





Tgt Ion:166 Resp: 2580

Ion Ratio Lower Upper

166 100

165 7.2 69.6 104.4#

167 31.3 11.9 17.9#

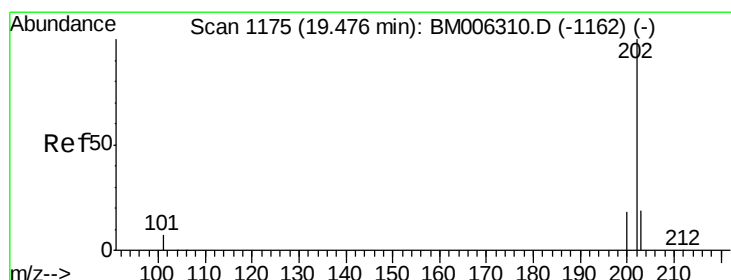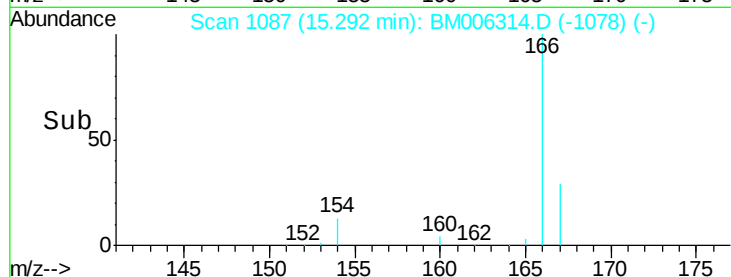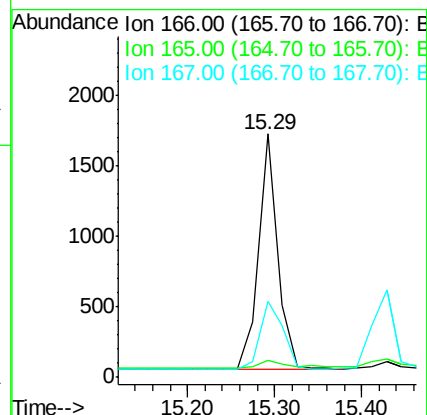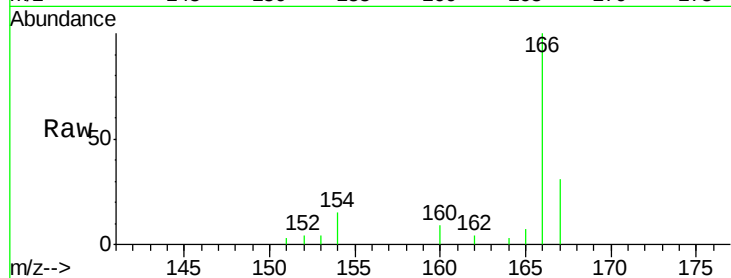

#19

Pyrene

Concen: 0.04 ng/ul

RT: 19.44 min Scan# 1339

Delta R.T. -0.04 min

Lab File: BM006314.D

Acq: 07 Jul 2016 11:49

Tgt Ion:202 Resp: 2149

Ion Ratio Lower Upper

202 100

200 6.9 17.8 26.8#

203 145.9 12.8 19.2#

